

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072519\
 Data File : P0058366.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Jul 2019 19:09
 Operator : SM/AJ
 Sample : K2646-11
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 COMP-2

Manual Integrations
 APPROVED

Ankita
 7/25/2019 2:00:10 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 25 01:22:18 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0071719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 17 11:13:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.191	3.533	996276	747445	29.400	23.304m
2) SA Decachlor...	9.693	8.428	1143206	754971	22.346	22.026

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072519\
Data File : P0058366.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Jul 2019 19:09
Operator : SM/AJ
Sample : K2646-11
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
COMP-2


Manual Integrations
APPROVED

Ankita
7/25/2019 2:00:10 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 25 01:22:18 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0071719.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 17 11:13:08 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

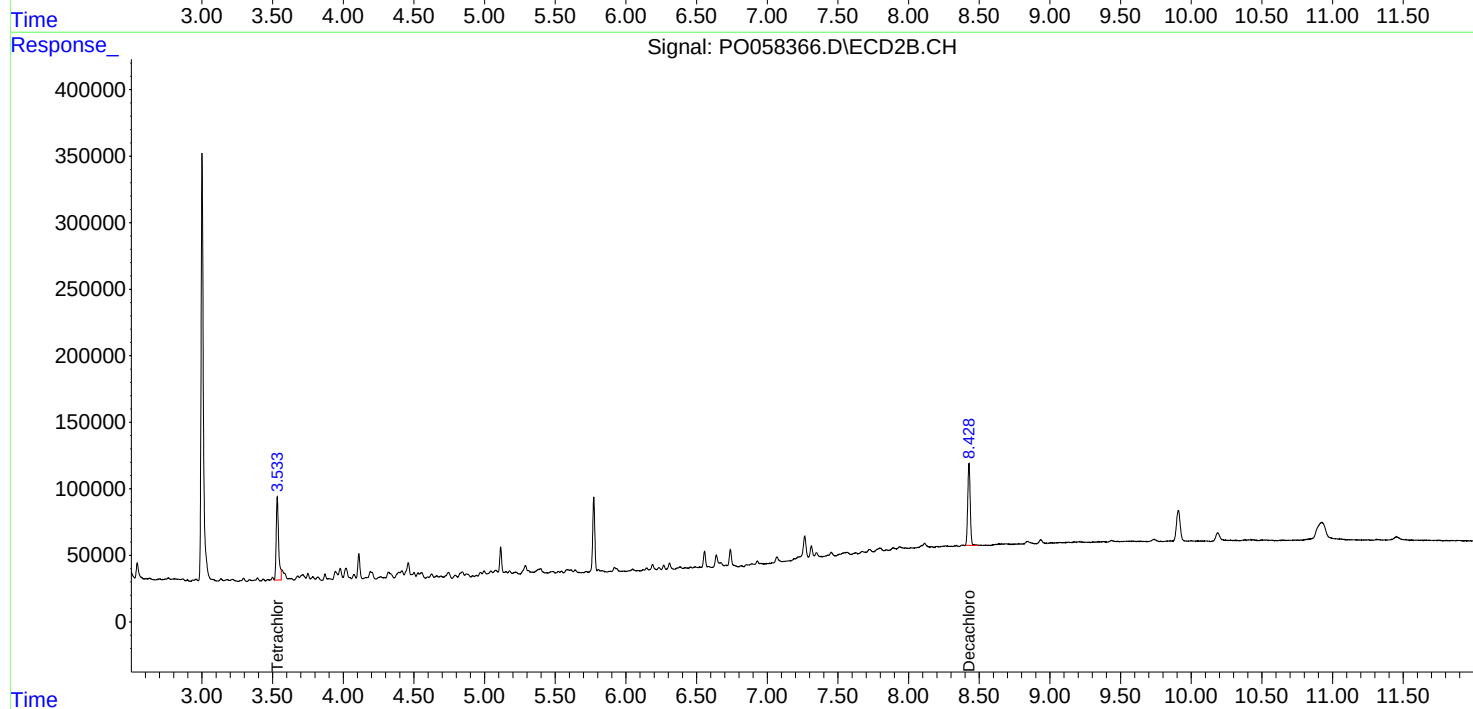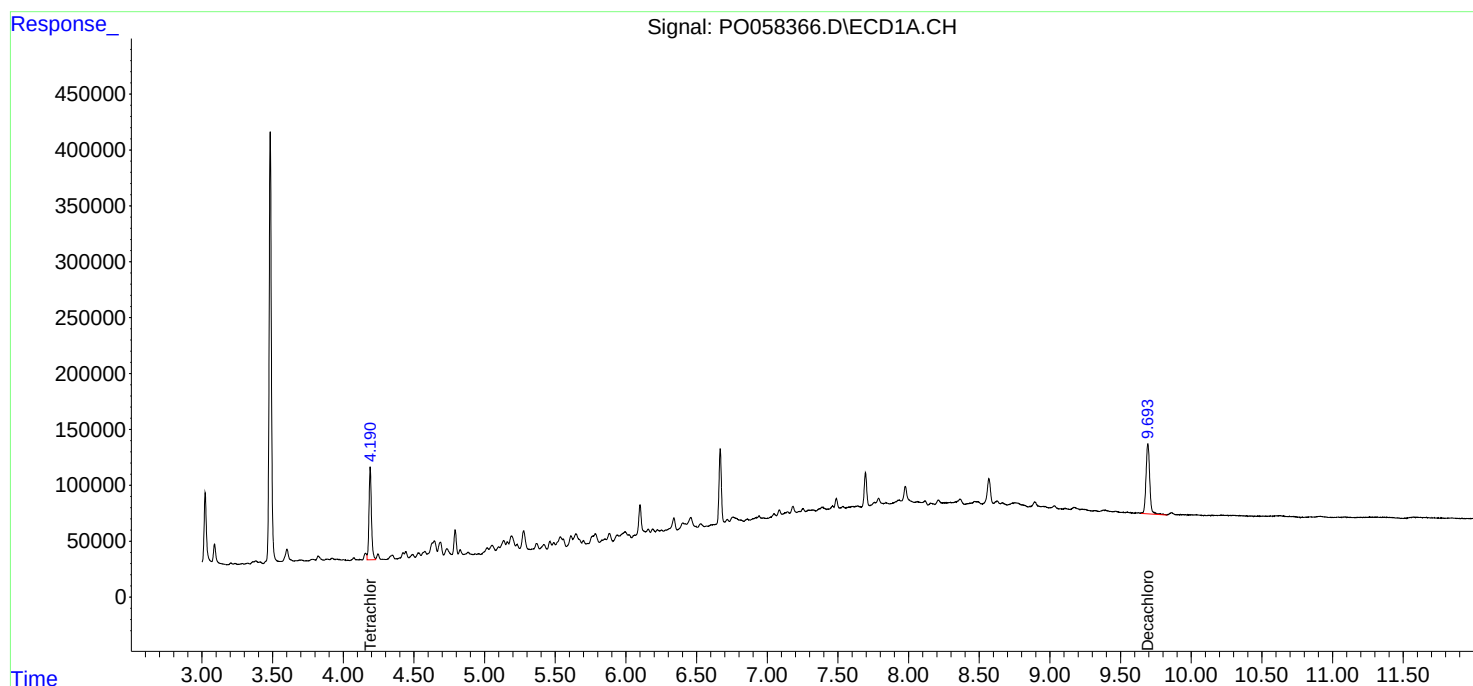

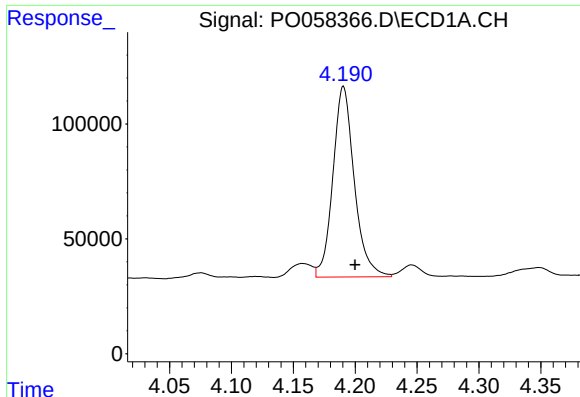


#1 Tetrachloro-m-xylene

R.T.: 4.191 min
Delta R.T.: -0.009 min
Response: 996276
Conc: 29.40 ng/ml

Instrument :
ECD_O
ClientSampleId :
COMP-2


Manual Integrations
APPROVED

Ankita
7/25/2019 2:00:10 PM

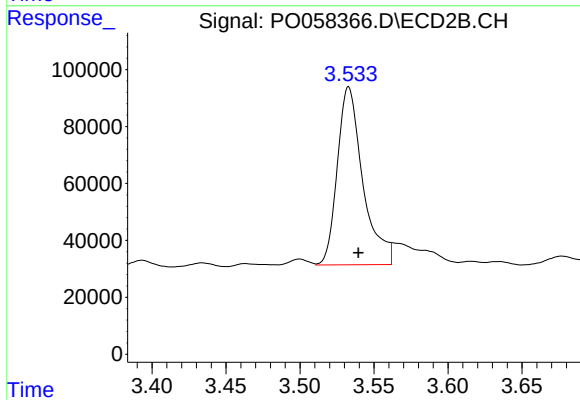


#1 Tetrachloro-m-xylene

R.T.: 3.533 min
Delta R.T.: -0.007 min
Response: 747445
Conc: 23.30 ng/ml m

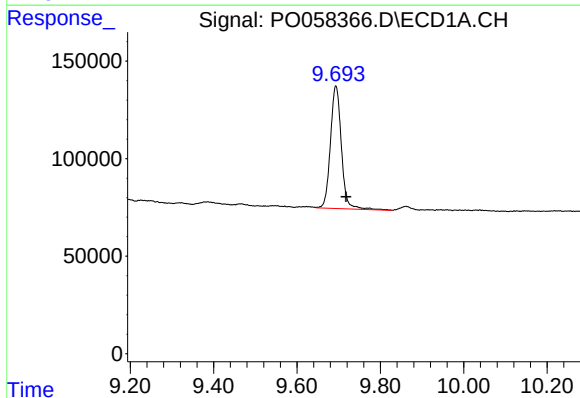

#2 Decachlorobiphenyl

R.T.: 9.693 min
Delta R.T.: -0.025 min
Response: 1143206
Conc: 22.35 ng/ml

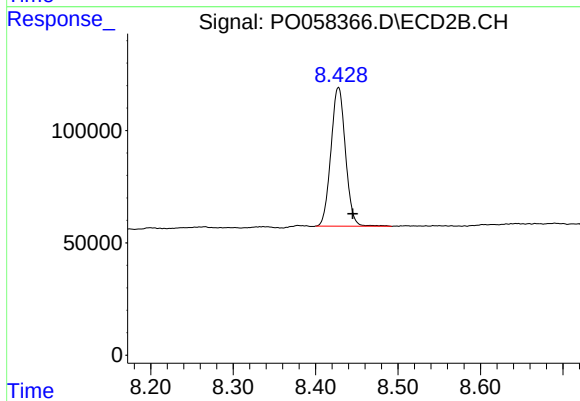

#2 Decachlorobiphenyl

R.T.: 8.428 min
Delta R.T.: -0.017 min
Response: 754971
Conc: 22.03 ng/ml