

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072519\
 Data File : P0058369.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Jul 2019 20:00
 Operator : SM/AJ
 Sample : K3887-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AOC-7(1)

Manual Integrations
 APPROVED

Ankita
 7/25/2019 2:00:16 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 25 07:11:01 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0071719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 17 11:13:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.188	3.530	618126	506978	18.241	15.807m
2) SA Decachlor...	9.690	8.425	406802	308756	7.952	9.008m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072519\
Data File : P0058369.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Jul 2019 20:00
Operator : SM/AJ
Sample : K3887-01
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
AOC-7(1)


Manual Integrations
APPROVED

Ankita
7/25/2019 2:00:16 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 25 07:11:01 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0071719.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 17 11:13:08 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

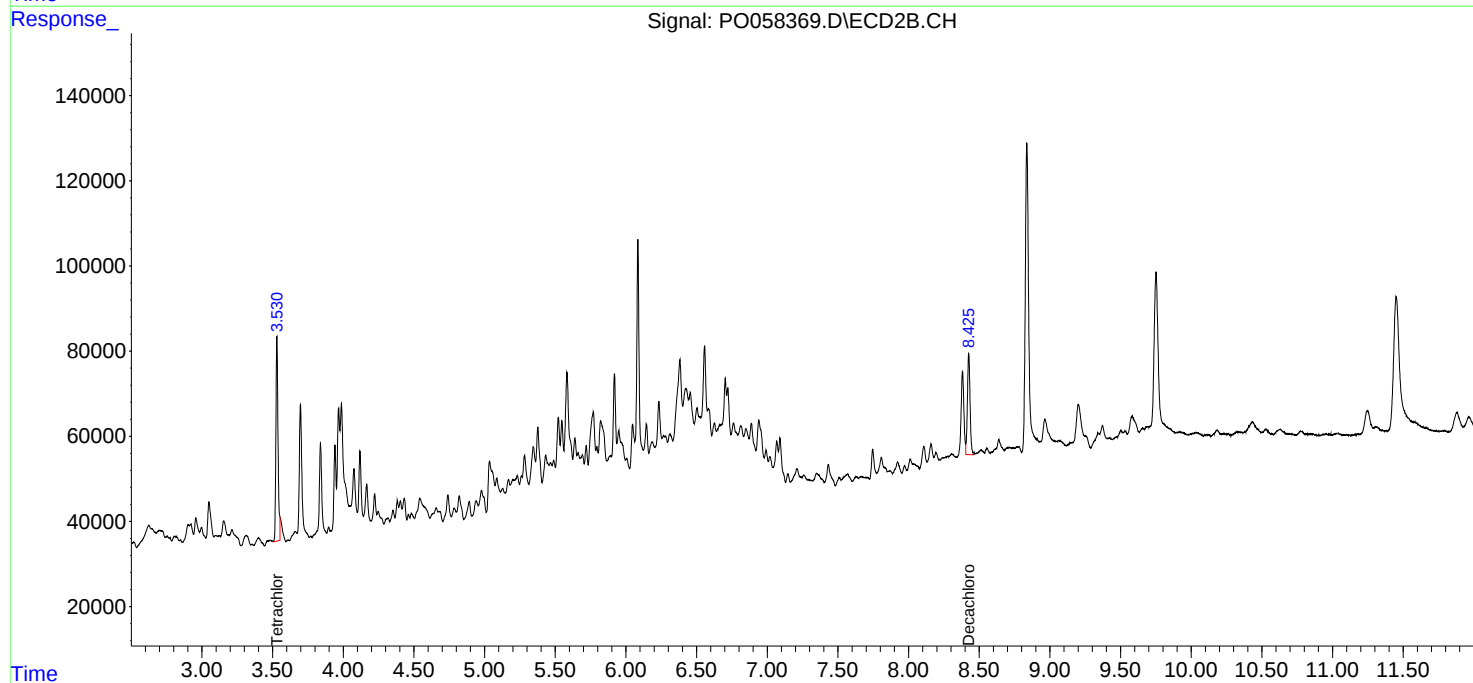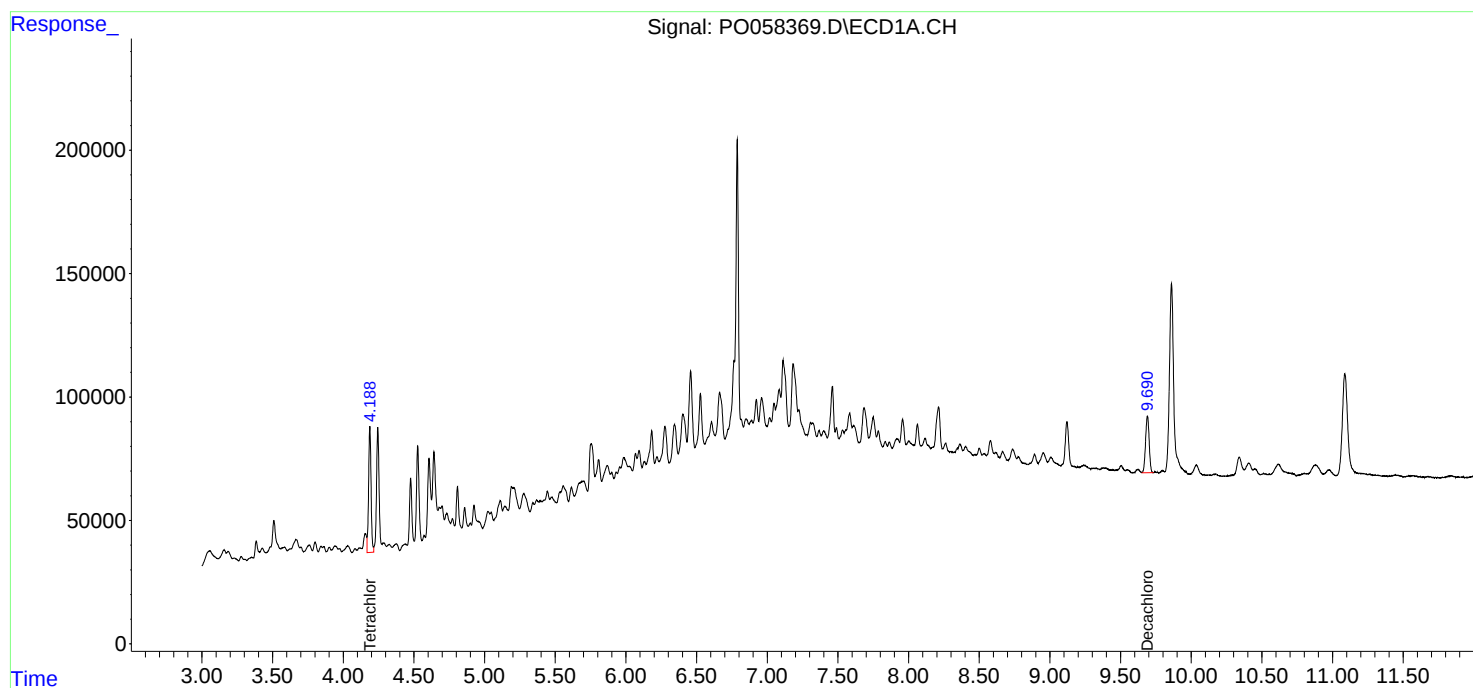

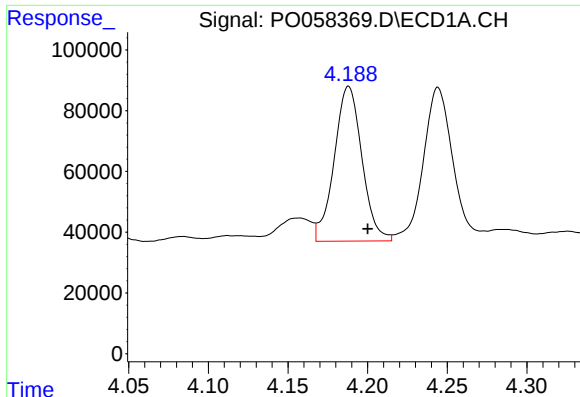


#1 Tetrachloro-m-xylene

R.T.: 4.188 min
Delta R.T.: -0.012 min
Response: 618126
Conc: 18.24 ng/ml

Instrument :
ECD_O
ClientSampleId :
AOC-7(1)


Manual Integrations
APPROVED

Ankita
7/25/2019 2:00:16 PM

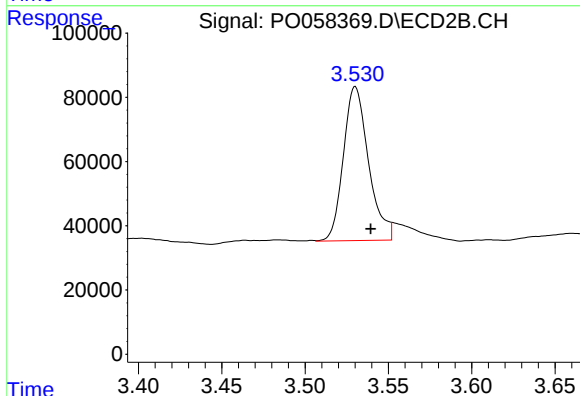


#1 Tetrachloro-m-xylene

R.T.: 3.530 min
Delta R.T.: -0.010 min
Response: 506978
Conc: 15.81 ng/ml m

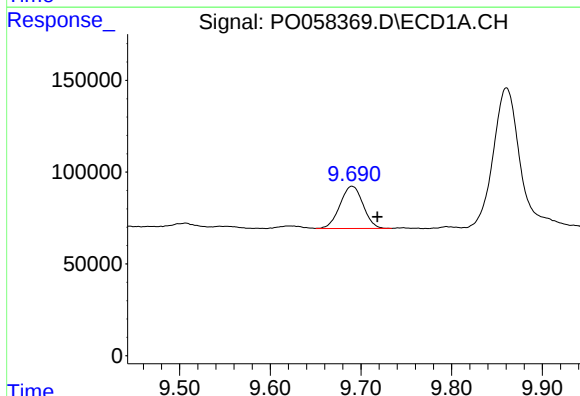

#2 Decachlorobiphenyl

R.T.: 9.690 min
Delta R.T.: -0.028 min
Response: 406802
Conc: 7.95 ng/ml

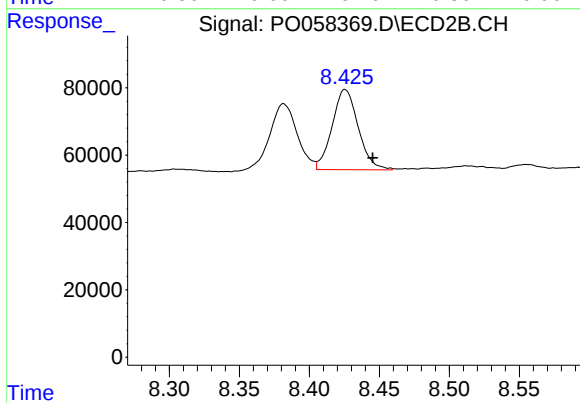

#2 Decachlorobiphenyl

R.T.: 8.425 min
Delta R.T.: -0.020 min
Response: 308756
Conc: 9.01 ng/ml m