

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072519\
 Data File : P0058374.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Jul 2019 21:26
 Operator : SM/AJ
 Sample : K3989-02
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 K580-B8-02

Manual Integrations
 APPROVED

Ankita
 7/25/2019 2:48:12 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 25 01:27:05 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0071719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 17 11:13:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.187	3.529	840501	716886	24.803	22.351
2) SA Decachlor...	9.687	8.424	797465	574744	15.588	16.768m
Target Compounds						
26) L6 AR-1254-1	6.182	5.375	315809	276325	160.702m	135.623
27) L6 AR-1254-2	6.396	5.520	846952	585346	259.083m	323.017
28) L6 AR-1254-3	6.762	5.918	1369978	1252844	388.339m	427.820
29) L6 AR-1254-4	7.045	6.144	1078481	706070	364.497m	382.148m
30) L6 AR-1254-5	7.460	6.555	2212826	1679364	753.881m	617.756m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072519\
Data File : P0058374.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Jul 2019 21:26
Operator : SM/AJ
Sample : K3989-02
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
K580-B8-02


Manual Integrations
APPROVED

Ankita
7/25/2019 2:48:12 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 25 01:27:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0071719.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 17 11:13:08 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

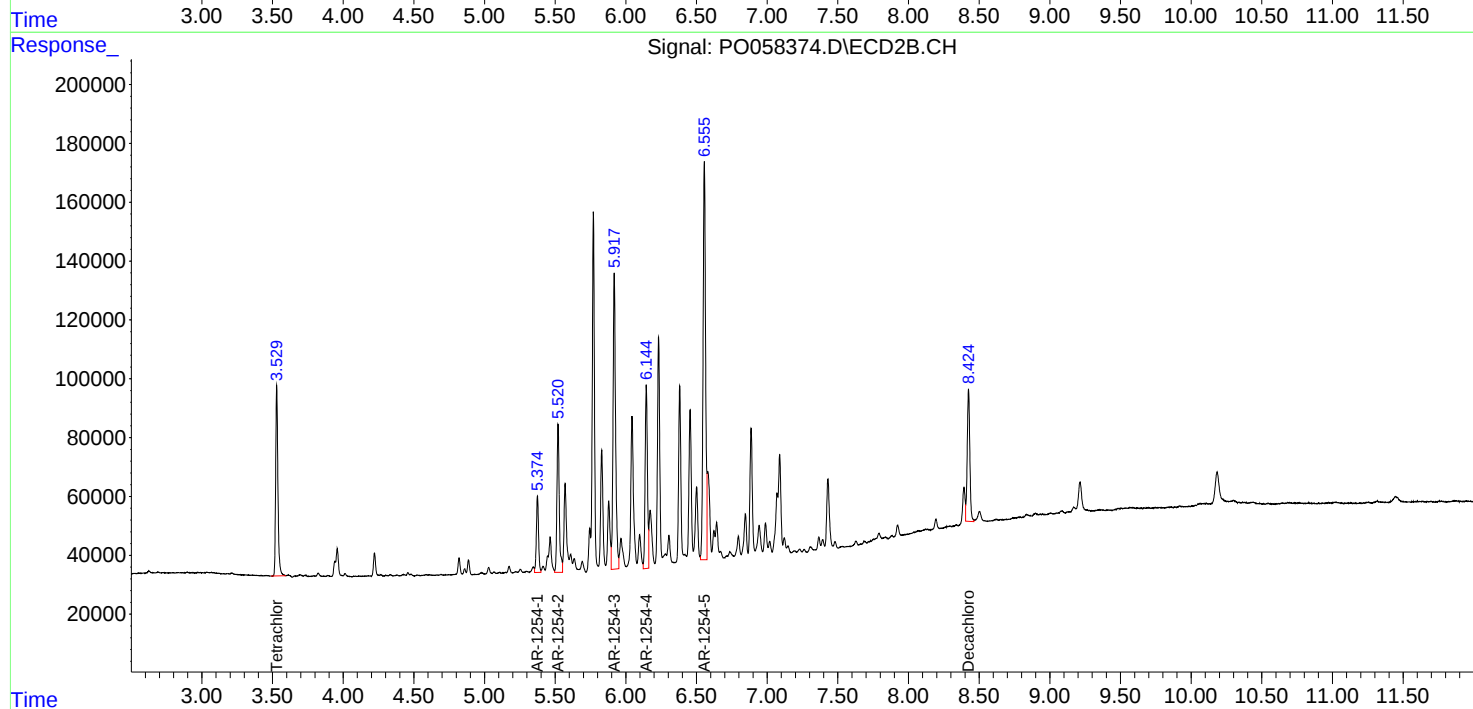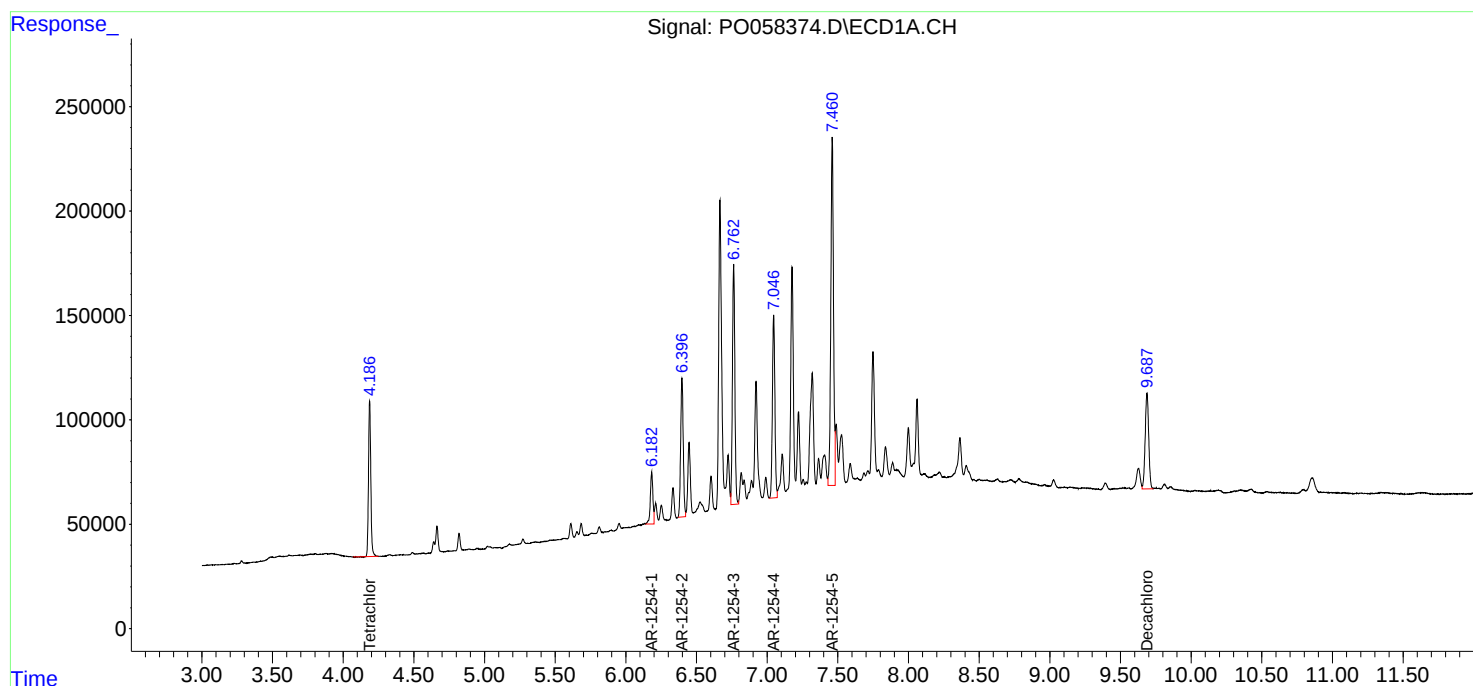

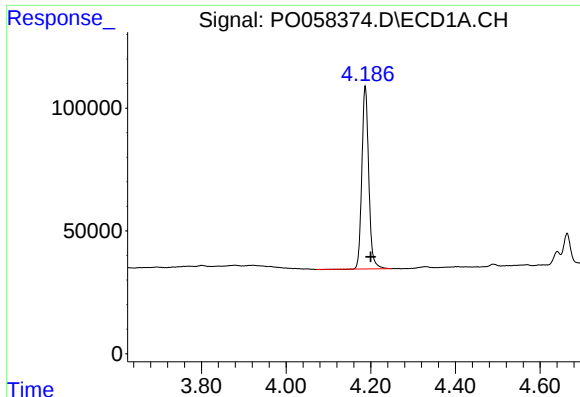


#1 Tetrachloro-m-xylene

R.T.: 4.187 min
Delta R.T.: -0.013 min
Response: 840501
Conc: 24.80 ng/ml

Instrument :
ECD_O
ClientSampleId :
K580-B8-02


Manual Integrations
APPROVED

Ankita
7/25/2019 2:48:12 PM

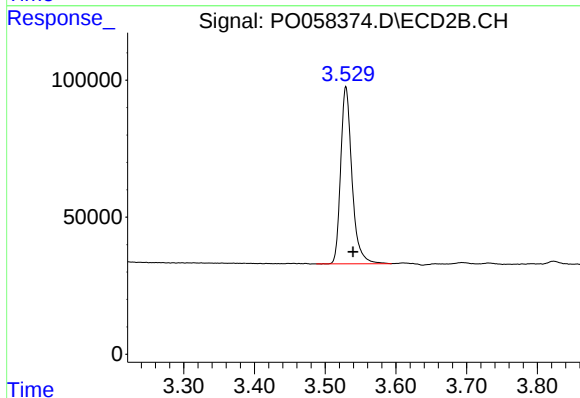


#1 Tetrachloro-m-xylene

R.T.: 3.529 min
Delta R.T.: -0.010 min
Response: 716886
Conc: 22.35 ng/ml

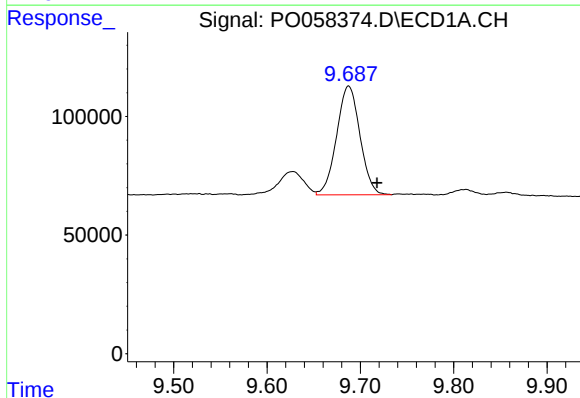


#2 Decachlorobiphenyl

R.T.: 9.687 min
Delta R.T.: -0.031 min
Response: 797465
Conc: 15.59 ng/ml

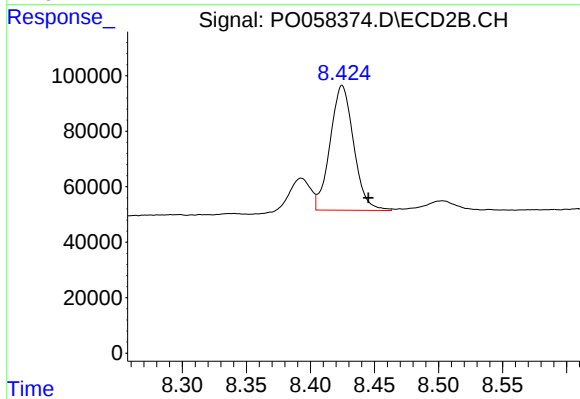

#2 Decachlorobiphenyl

R.T.: 8.424 min
Delta R.T.: -0.021 min
Response: 574744
Conc: 16.77 ng/ml m

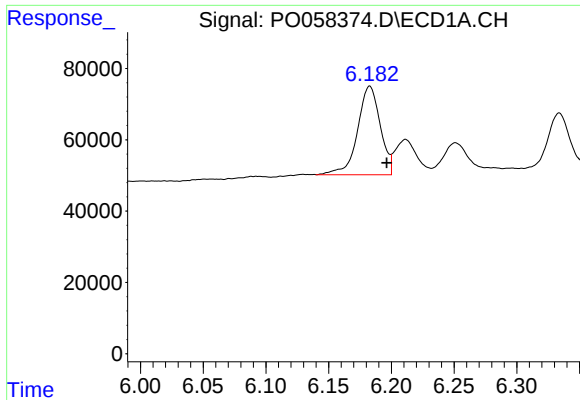


#26 AR-1254-1

R.T.: 6.182 min
Delta R.T.: -0.014 min
Response: 315809
Conc: 160.70 ng/ml m

Instrument :
ECD_O
ClientSampleId :
K580-B8-02


Manual Integrations
APPROVED

Ankita
7/25/2019 2:48:12 PM

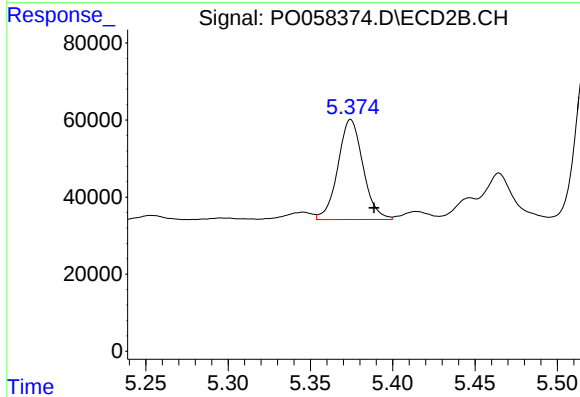


#26 AR-1254-1

R.T.: 5.375 min
Delta R.T.: -0.014 min
Response: 276325
Conc: 135.62 ng/ml

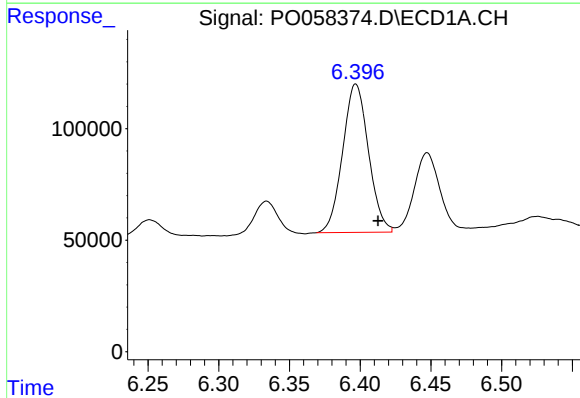


#27 AR-1254-2

R.T.: 6.396 min
Delta R.T.: -0.016 min
Response: 846952
Conc: 259.08 ng/ml m

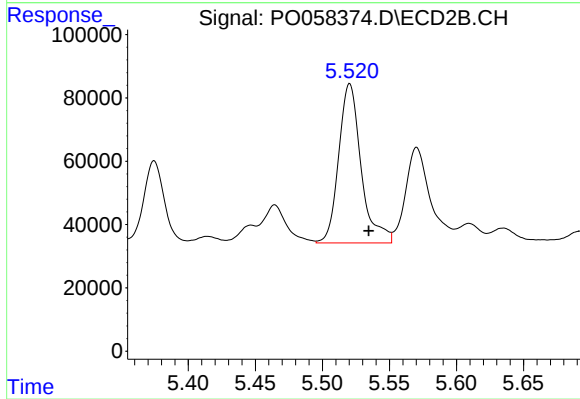

#27 AR-1254-2

R.T.: 5.520 min
Delta R.T.: -0.014 min
Response: 585346
Conc: 323.02 ng/ml

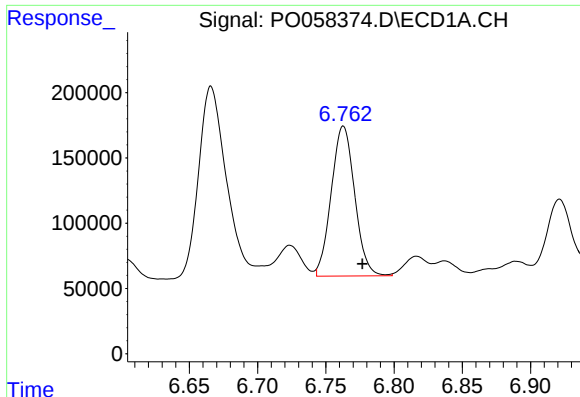


#28 AR-1254-3

R.T.: 6.762 min
Delta R.T.: -0.014 min
Response: 1369978
Conc: 388.34 ng/ml m

Instrument :
ECD_O
ClientSampleId :
K580-B8-02


Manual Integrations
APPROVED

Ankita
7/25/2019 2:48:12 PM

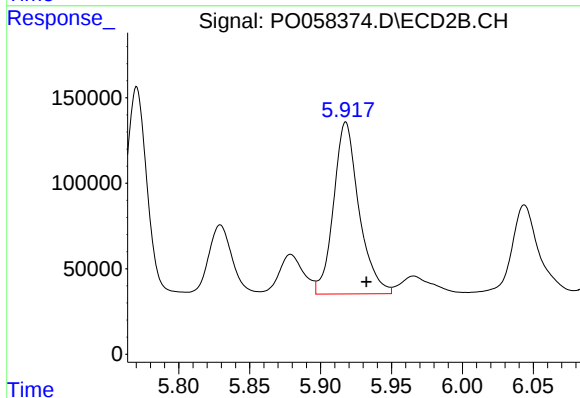


#28 AR-1254-3

R.T.: 5.918 min
Delta R.T.: -0.014 min
Response: 1252844
Conc: 427.82 ng/ml

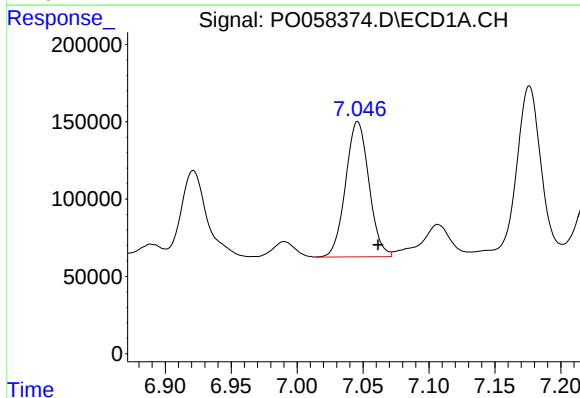


#29 AR-1254-4

R.T.: 7.045 min
Delta R.T.: -0.016 min
Response: 1078481
Conc: 364.50 ng/ml m

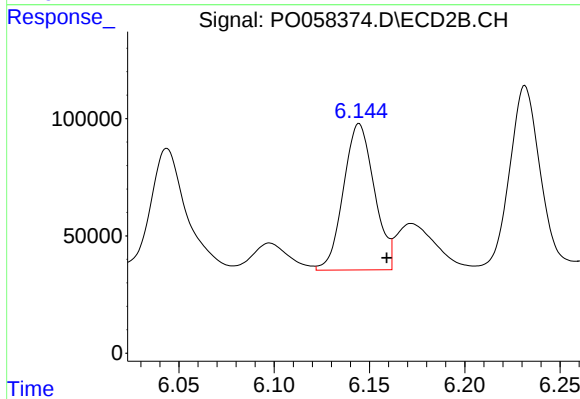

#29 AR-1254-4

R.T.: 6.144 min
Delta R.T.: -0.015 min
Response: 706070
Conc: 382.15 ng/ml m

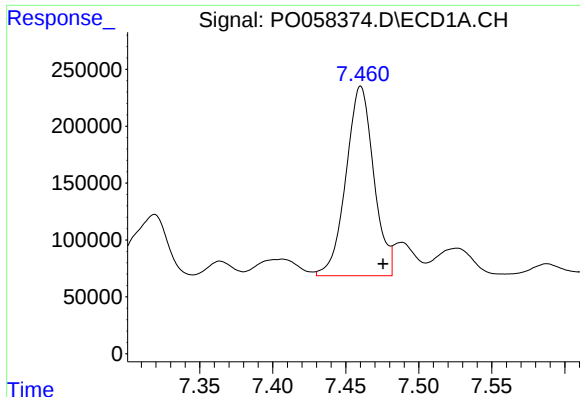


#30 AR-1254-5

R.T.: 7.460 min
Delta R.T.: -0.016 min
Response: 2212826
Conc: 753.88 ng/ml m

Instrument :
ECD_O
ClientSampleId :
K580-B8-02

Manual Integrations
APPROVED

Ankita
7/25/2019 2:48:12 PM

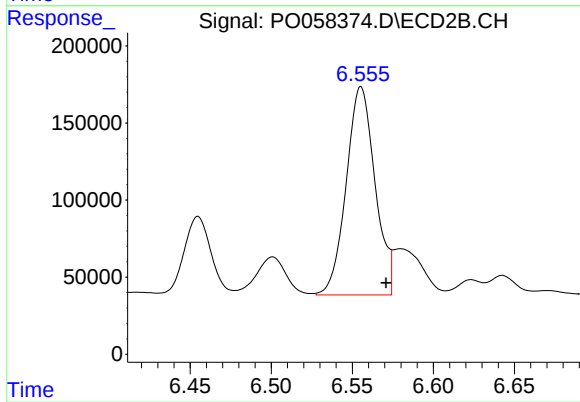

#30 AR-1254-5

R.T.: 6.555 min
Delta R.T.: -0.016 min
Response: 1679364
Conc: 617.76 ng/ml m