

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072619\
 Data File : P0058393.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Jul 2019 10:21
 Operator : SM/AJ
 Sample : K2646-07RE
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 COMP-1RE

Manual Integrations
 APPROVED

Ankita
 7/27/2019 9:39:32 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 25 12:13:55 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0071719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 17 11:13:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.185	3.530	684716	734446	20.206m	22.899
2) SA Decachlor...	9.683	8.420	317861	191232	6.213	5.579

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072619\
Data File : P0058393.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Jul 2019 10:21
Operator : SM/AJ
Sample : K2646-07RE
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
COMP-IRE


Manual Integrations
APPROVED

Ankita
7/27/2019 9:39:32 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 25 12:13:55 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0071719.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 17 11:13:08 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

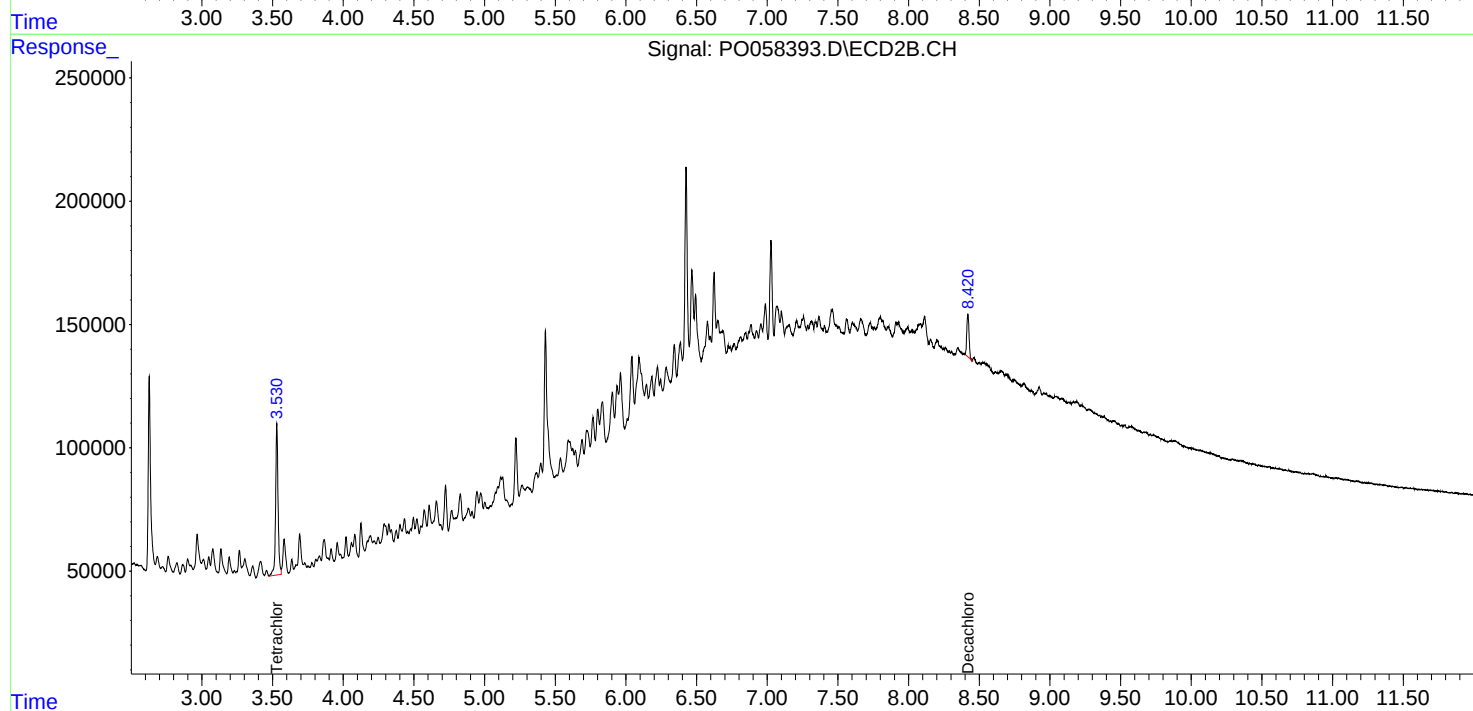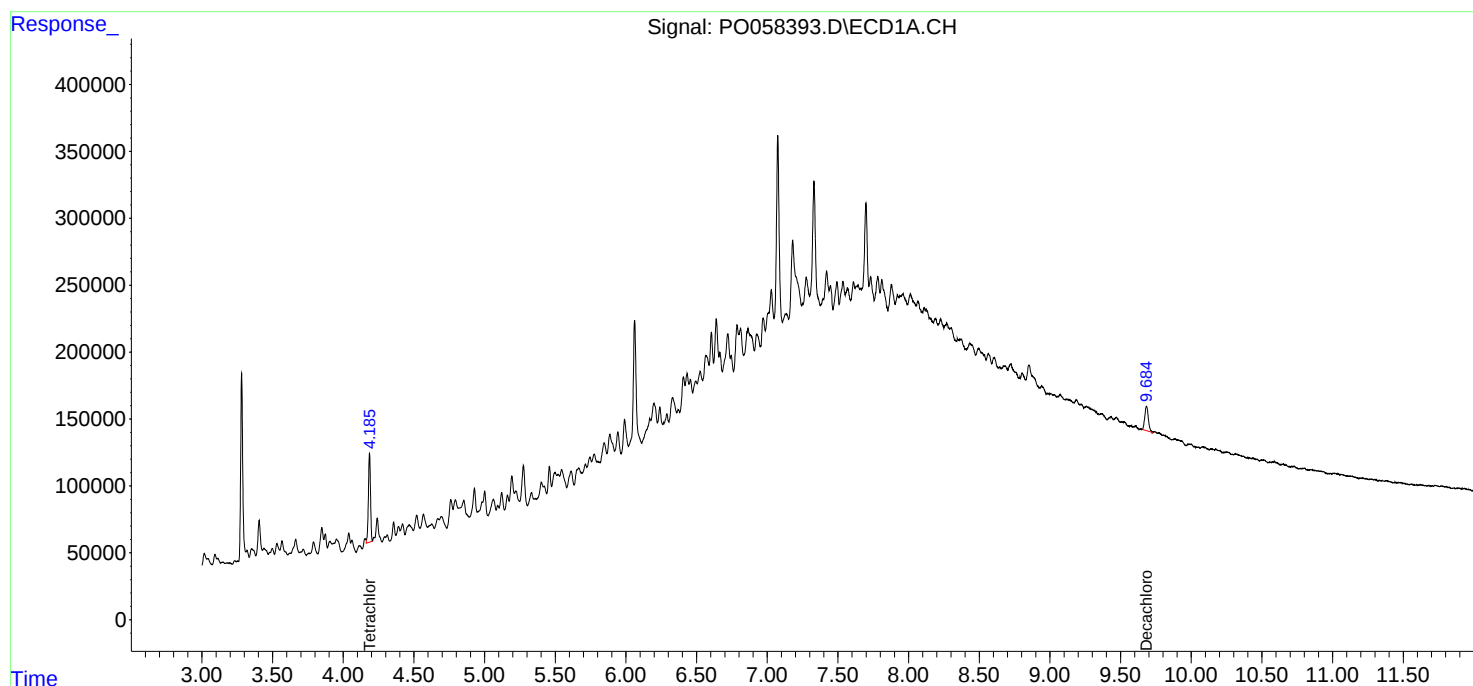

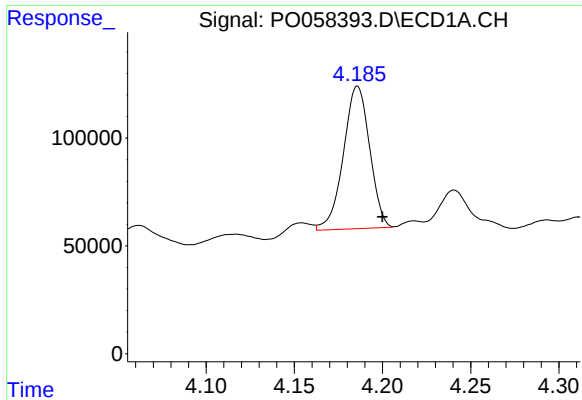


#1 Tetrachloro-m-xylene

R.T.: 4.185 min
Delta R.T.: -0.015 min
Response: 684716
Conc: 20.21 ng/ml m

Instrument :
ECD_O
ClientSampleId :
COMP-1RE


Manual Integrations
APPROVED

Ankita
7/27/2019 9:39:32 AM

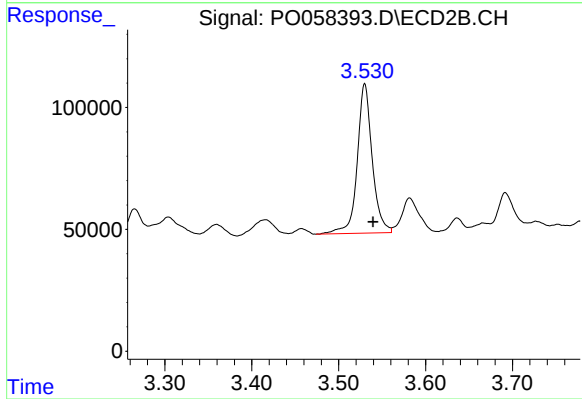


#1 Tetrachloro-m-xylene

R.T.: 3.530 min
Delta R.T.: -0.009 min
Response: 734446
Conc: 22.90 ng/ml

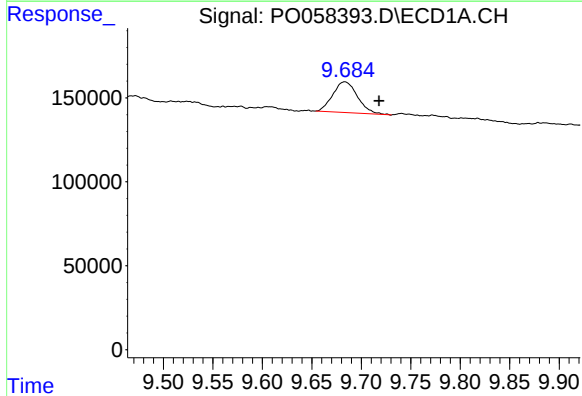

#2 Decachlorobiphenyl

R.T.: 9.683 min
Delta R.T.: -0.035 min
Response: 317861
Conc: 6.21 ng/ml

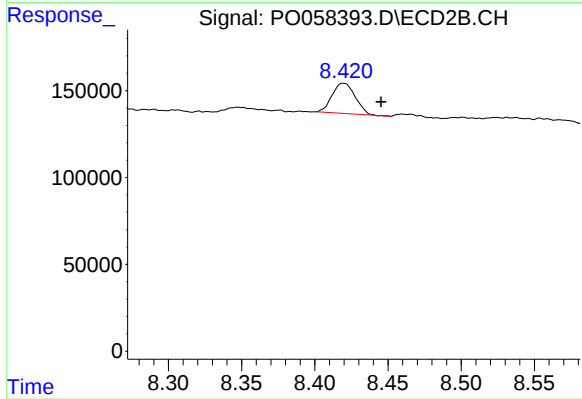

#2 Decachlorobiphenyl

R.T.: 8.420 min
Delta R.T.: -0.025 min
Response: 191232
Conc: 5.58 ng/ml