

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072619\
 Data File : P0058400.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Jul 2019 13:52
 Operator : SM/AJ
 Sample : K3929-06
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 30321

Manual Integrations
 APPROVED

Ankita
 7/27/2019 9:42:04 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 25 14:28:10 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0071719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 17 11:13:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.185	3.527	407550	354929	12.027m	11.066
2) SA Decachlor...	9.683	8.420	366357	259538	7.161	7.572m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072619\
Data File : P0058400.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Jul 2019 13:52
Operator : SM/AJ
Sample : K3929-06
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
30321


Manual Integrations
APPROVED

Ankita
7/27/2019 9:42:04 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 25 14:28:10 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0071719.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 17 11:13:08 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

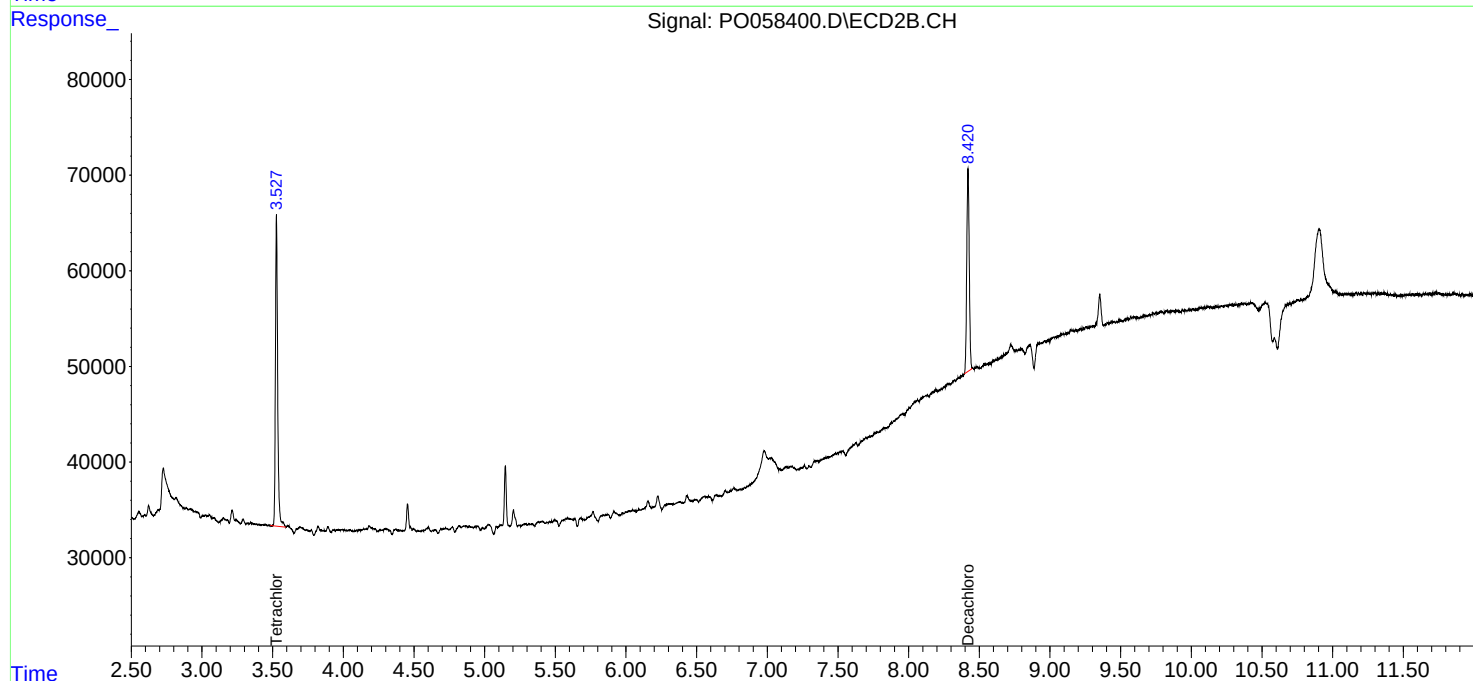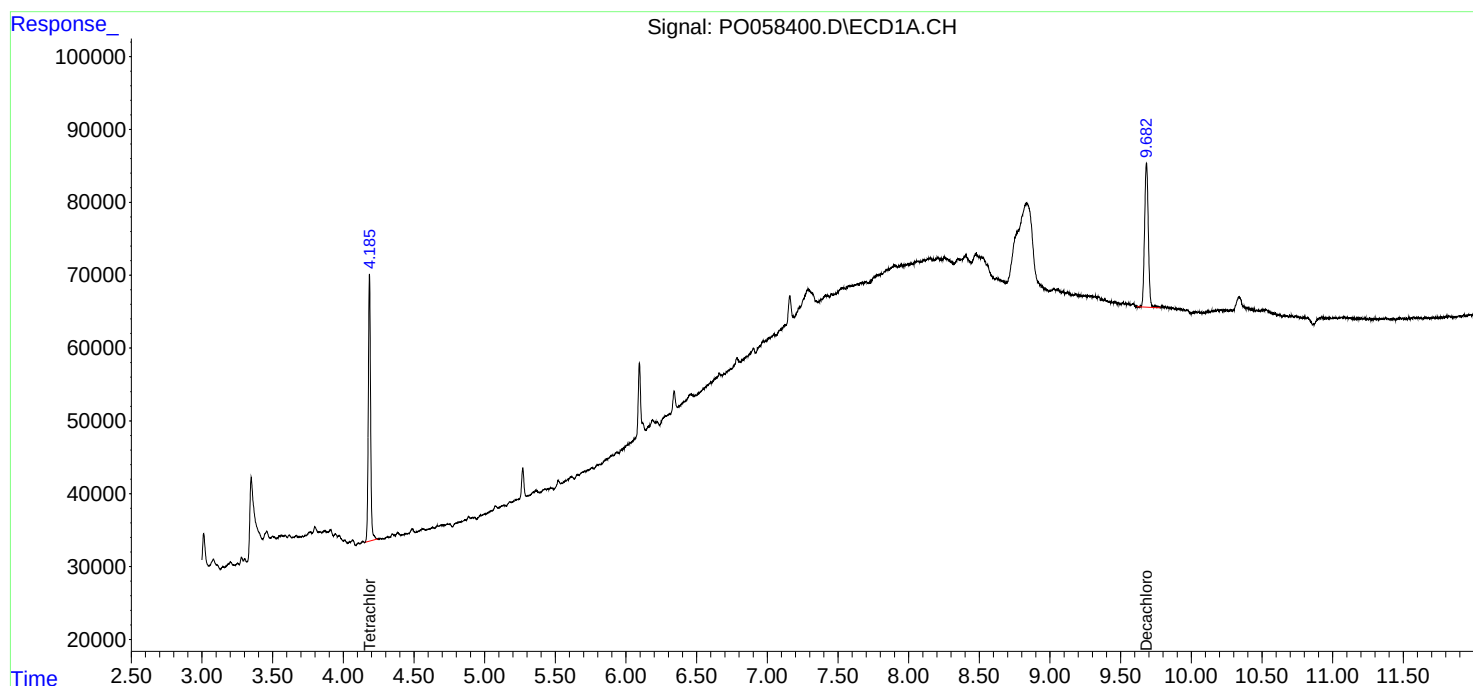

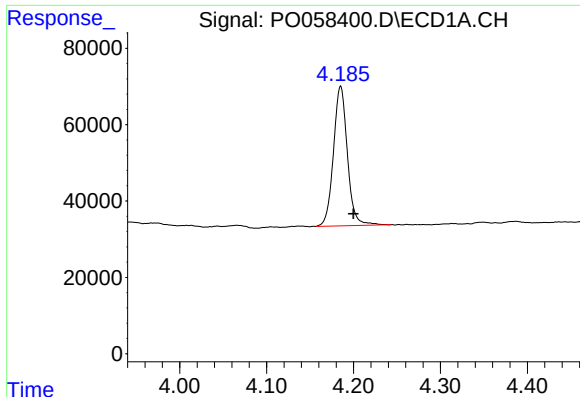


#1 Tetrachloro-m-xylene

R.T.: 4.185 min
Delta R.T.: -0.015 min
Response: 407550
Conc: 12.03 ng/ml m

Instrument :
ECD_O
ClientSampleId :
30321


Manual Integrations
APPROVED

Ankita
7/27/2019 9:42:04 AM

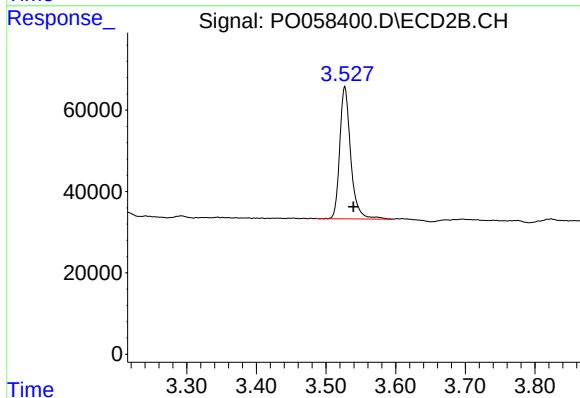


#1 Tetrachloro-m-xylene

R.T.: 3.527 min
Delta R.T.: -0.012 min
Response: 354929
Conc: 11.07 ng/ml

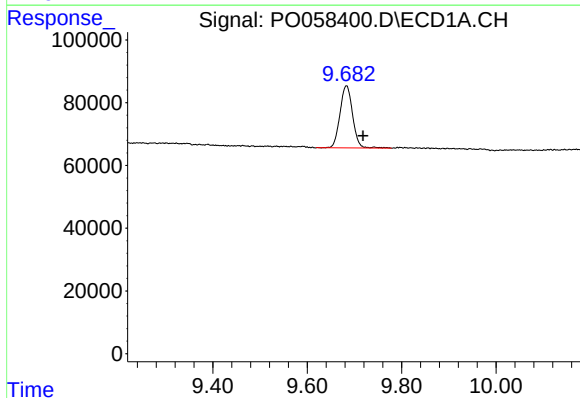

#2 Decachlorobiphenyl

R.T.: 9.683 min
Delta R.T.: -0.035 min
Response: 366357
Conc: 7.16 ng/ml

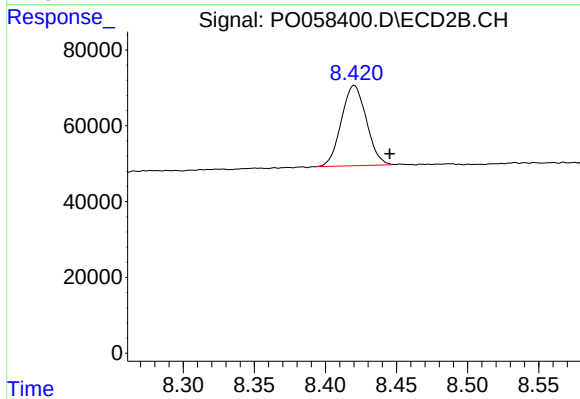

#2 Decachlorobiphenyl

R.T.: 8.420 min
Delta R.T.: -0.025 min
Response: 259538
Conc: 7.57 ng/ml m