

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072619\
 Data File : P0058410.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Jul 2019 18:22
 Operator : SM/AJ
 Sample : K4005-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S13-03-S

Manual Integrations
 APPROVED

Ankita
 7/27/2019 9:42:43 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 26 01:39:11 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0071719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 17 11:13:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.183	3.527	932339	786979	27.513	24.537
2) SA Decachlor...	9.681	8.419	827529	598326	16.176	17.456m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072619\
Data File : P0058410.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Jul 2019 18:22
Operator : SM/AJ
Sample : K4005-02
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
S13-03-S


Manual Integrations
APPROVED

Ankita
7/27/2019 9:42:43 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 26 01:39:11 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0071719.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 17 11:13:08 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

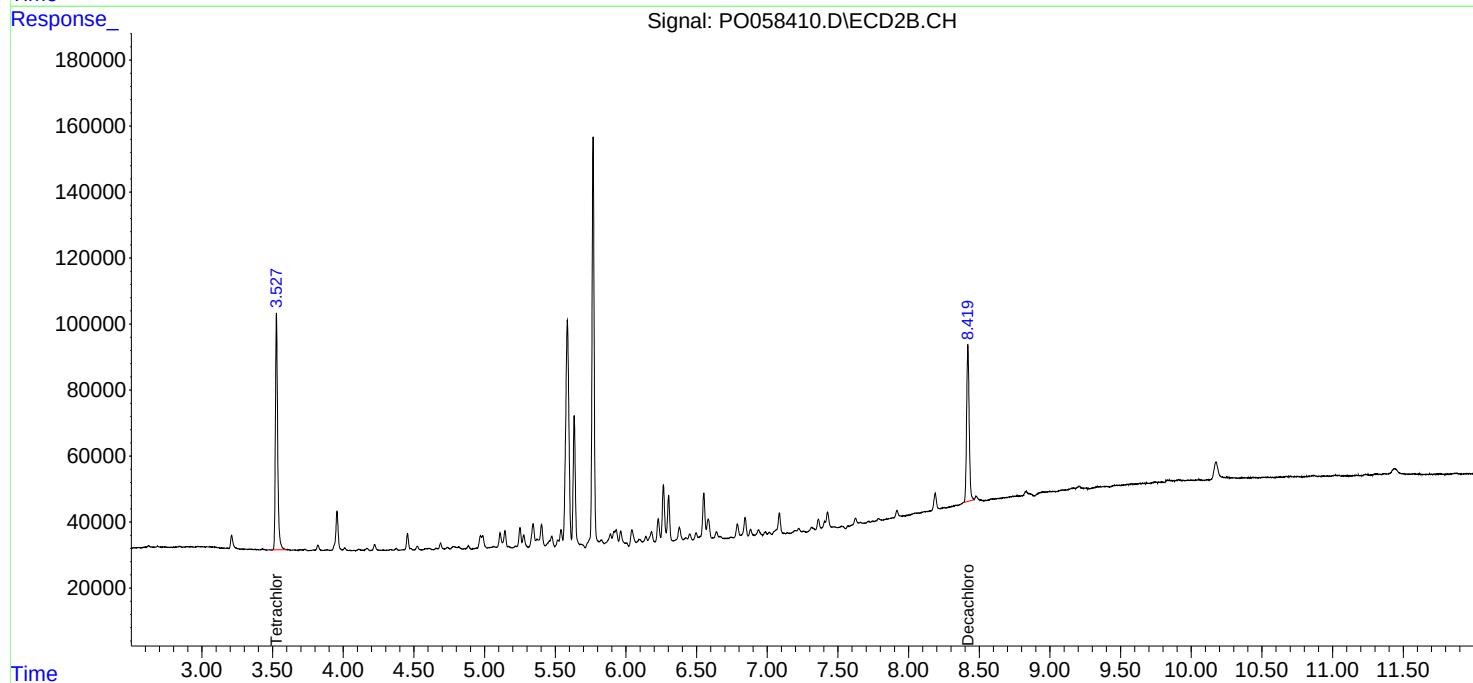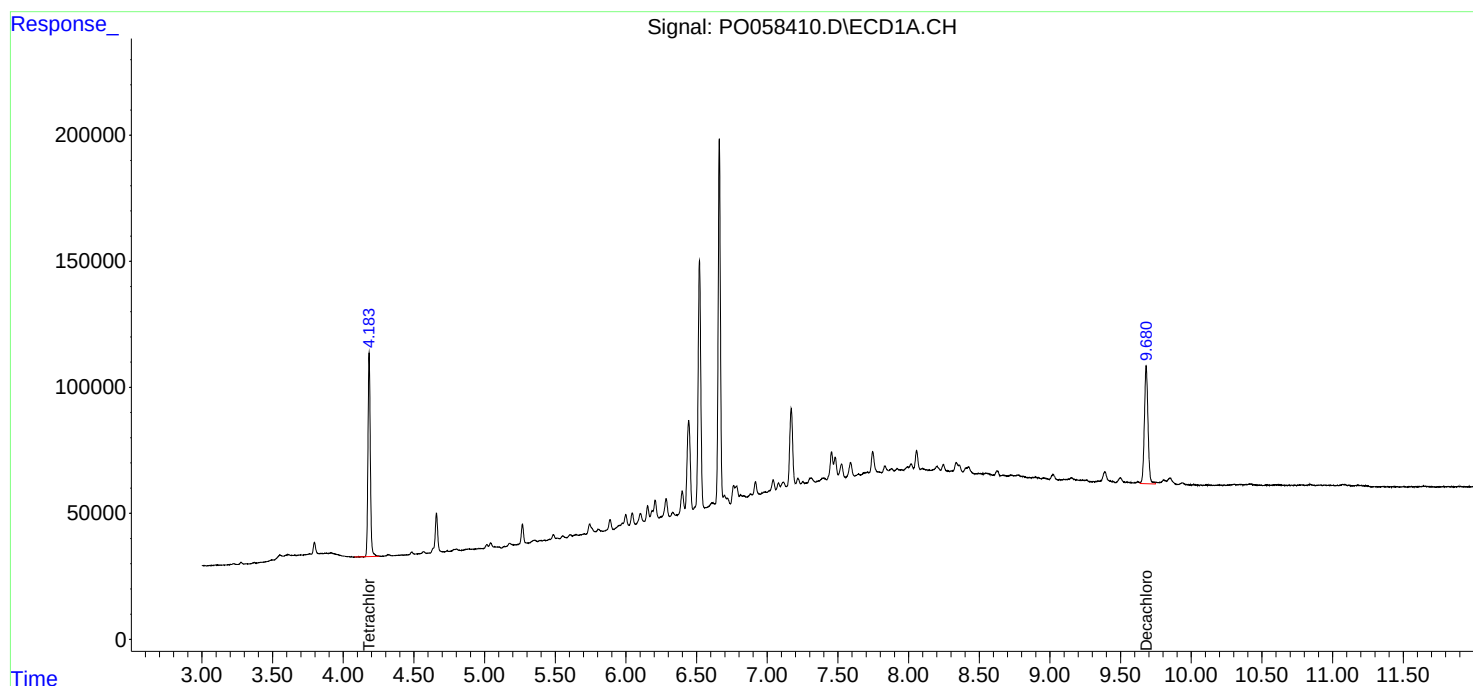

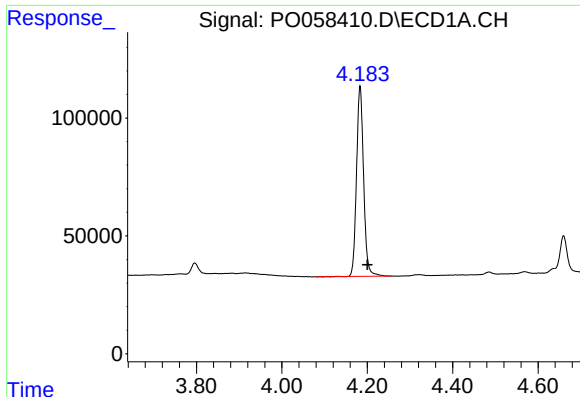


#1 Tetrachloro-m-xylene

R.T.: 4.183 min
Delta R.T.: -0.017 min
Response: 932339
Conc: 27.51 ng/ml

Instrument :
ECD_O
ClientSampleId :
S13-03-S


Manual Integrations
APPROVED

Ankita
7/27/2019 9:42:43 AM

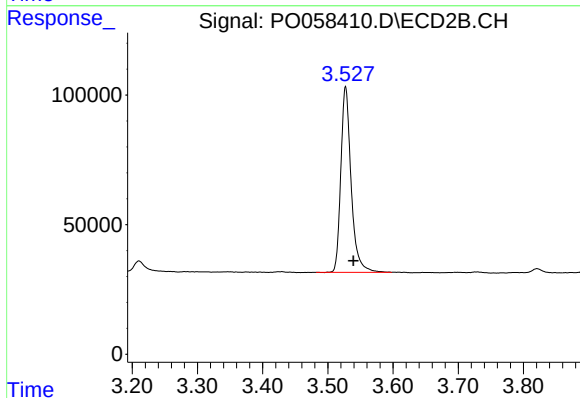


#1 Tetrachloro-m-xylene

R.T.: 3.527 min
Delta R.T.: -0.012 min
Response: 786979
Conc: 24.54 ng/ml

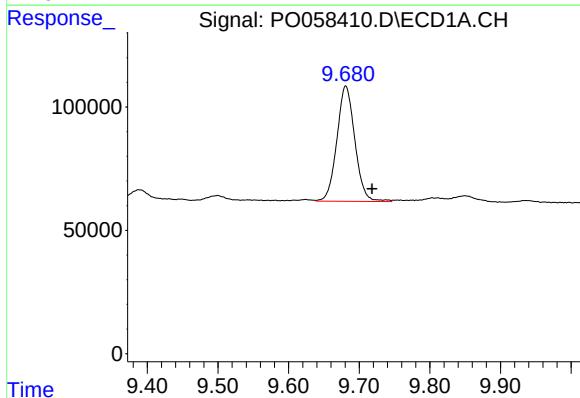

#2 Decachlorobiphenyl

R.T.: 9.681 min
Delta R.T.: -0.037 min
Response: 827529
Conc: 16.18 ng/ml

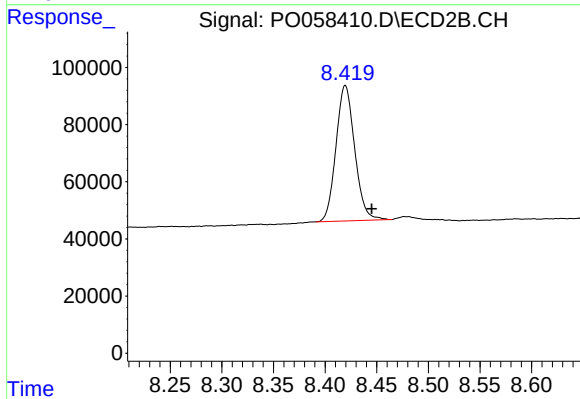

#2 Decachlorobiphenyl

R.T.: 8.419 min
Delta R.T.: -0.026 min
Response: 598326
Conc: 17.46 ng/ml m