

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072619\
 Data File : P0058414.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Jul 2019 19:30
 Operator : SM/AJ
 Sample : K4005-06
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S14-01-S

Manual Integrations
 APPROVED

Ankita
 7/27/2019 9:42:50 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 26 01:40:29 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0071719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 17 11:13:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.184	3.527	1064363	843133	31.409	26.287
2) SA Decachlor...	9.682	8.420	892694	620854	17.449	18.114m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072619\
Data File : P0058414.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Jul 2019 19:30
Operator : SM/AJ
Sample : K4005-06
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
S14-01-S


Manual Integrations
APPROVED

Ankita
7/27/2019 9:42:50 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 26 01:40:29 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0071719.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 17 11:13:08 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

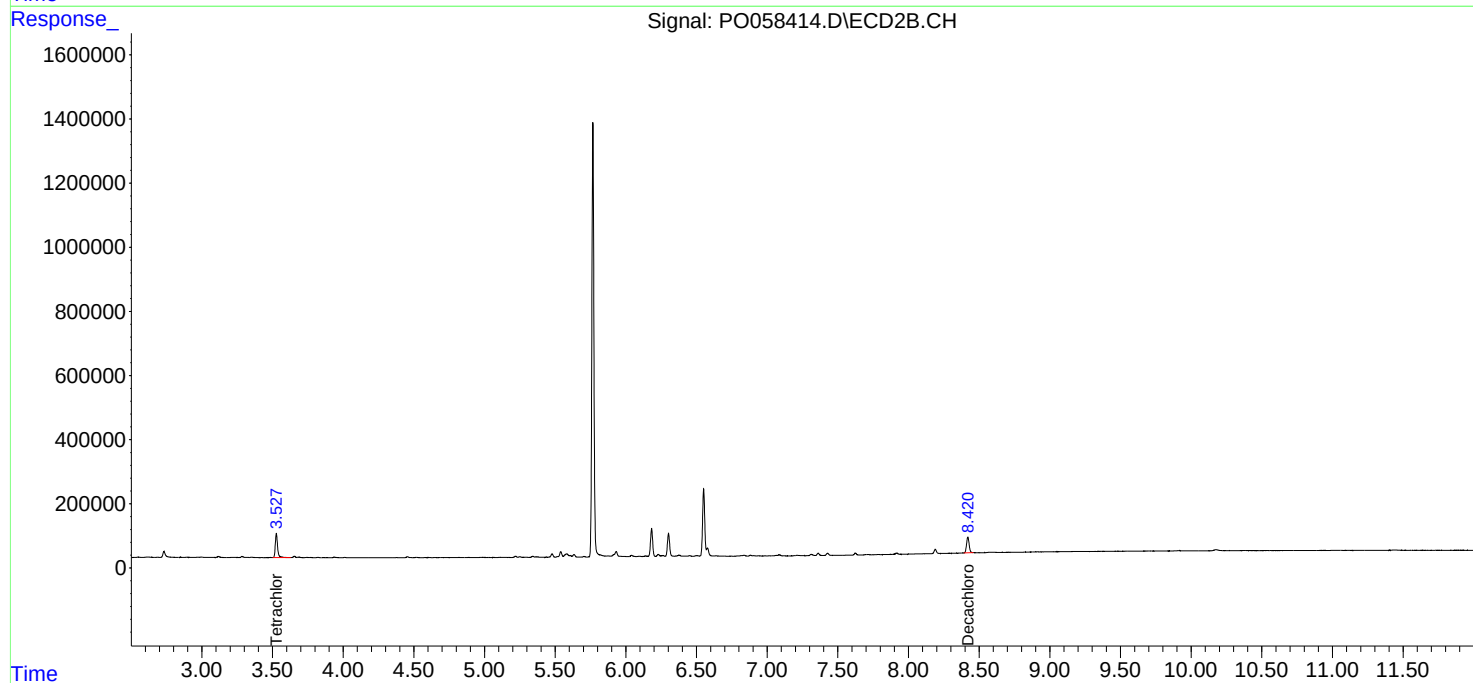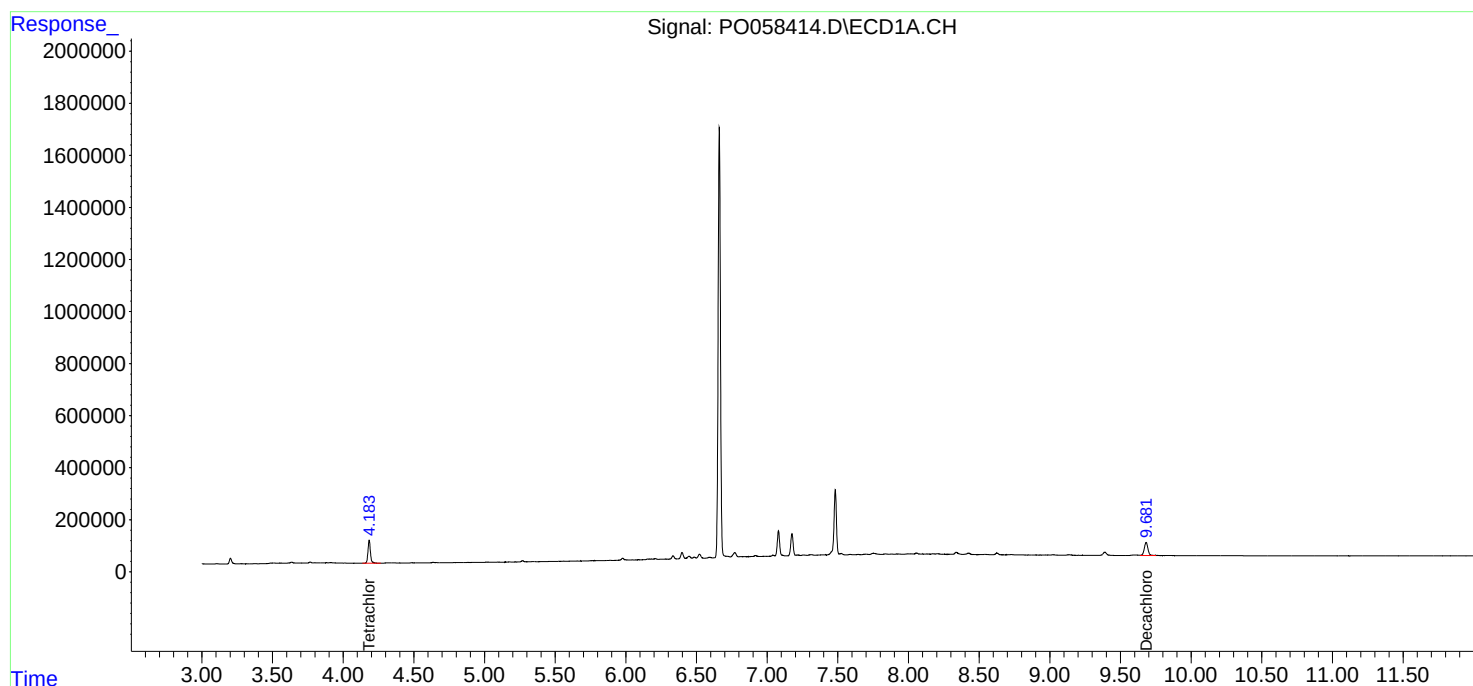

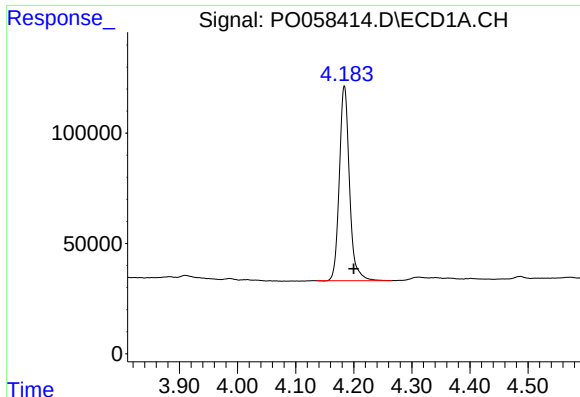


#1 Tetrachloro-m-xylene

R.T.: 4.184 min
Delta R.T.: -0.016 min
Response: 1064363
Conc: 31.41 ng/ml

Instrument :
ECD_O
ClientSampleId :
S14-01-S


Manual Integrations
APPROVED

Ankita
7/27/2019 9:42:50 AM

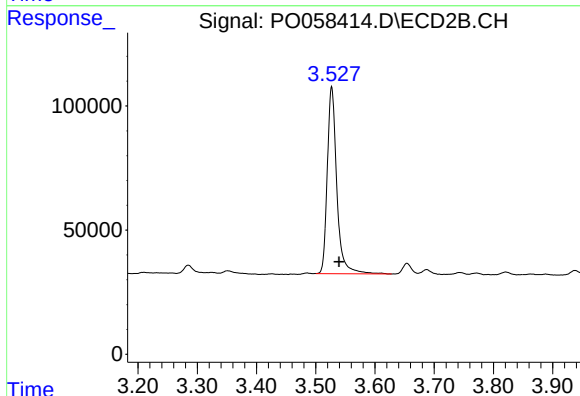


#1 Tetrachloro-m-xylene

R.T.: 3.527 min
Delta R.T.: -0.012 min
Response: 843133
Conc: 26.29 ng/ml

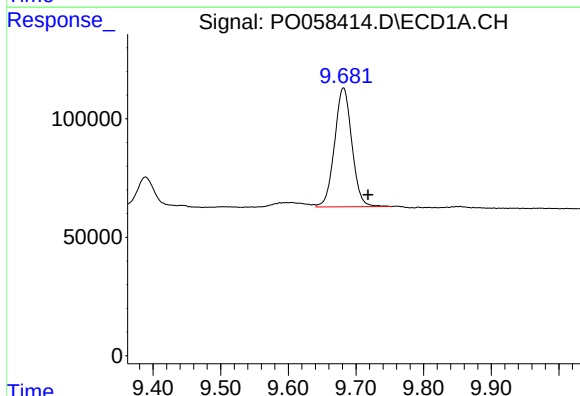

#2 Decachlorobiphenyl

R.T.: 9.682 min
Delta R.T.: -0.036 min
Response: 892694
Conc: 17.45 ng/ml

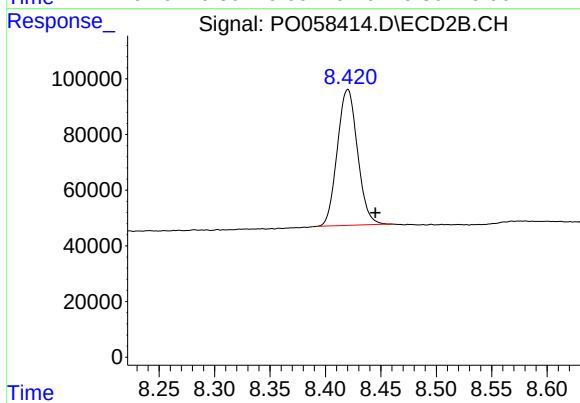

#2 Decachlorobiphenyl

R.T.: 8.420 min
Delta R.T.: -0.025 min
Response: 620854
Conc: 18.11 ng/ml m