

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072619\
 Data File : P0058416.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Jul 2019 20:04
 Operator : SM/AJ
 Sample : K4005-08
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 S14-02-S

Manual Integrations
 APPROVED

Ankita
 7/27/2019 9:42:54 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 26 01:41:02 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0071719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 17 11:13:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.185	3.528	896524	748707	26.456	23.343
2) SA Decachlor...	9.681	8.420	886745	651585	17.333	19.010m
Target Compounds						
41) L9 AR-1268-1	8.338	7.362	153128	104375	14.892	13.369m
42) L9 AR-1268-2	8.427	7.429	98512	79996	10.756m	11.227
43) L9 AR-1268-3	8.626	7.626	151557	111787	18.977	18.558
44) L9 AR-1268-4	9.024	7.918	29777	19648	10.049	9.393m
45) L9 AR-1268-5	9.388	8.189	350928	272581	16.110	16.346m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072619\
Data File : P0058416.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Jul 2019 20:04
Operator : SM/AJ
Sample : K4005-08
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
S14-02-S


Manual Integrations
APPROVED

Ankita
7/27/2019 9:42:54 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 26 01:41:02 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0071719.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 17 11:13:08 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

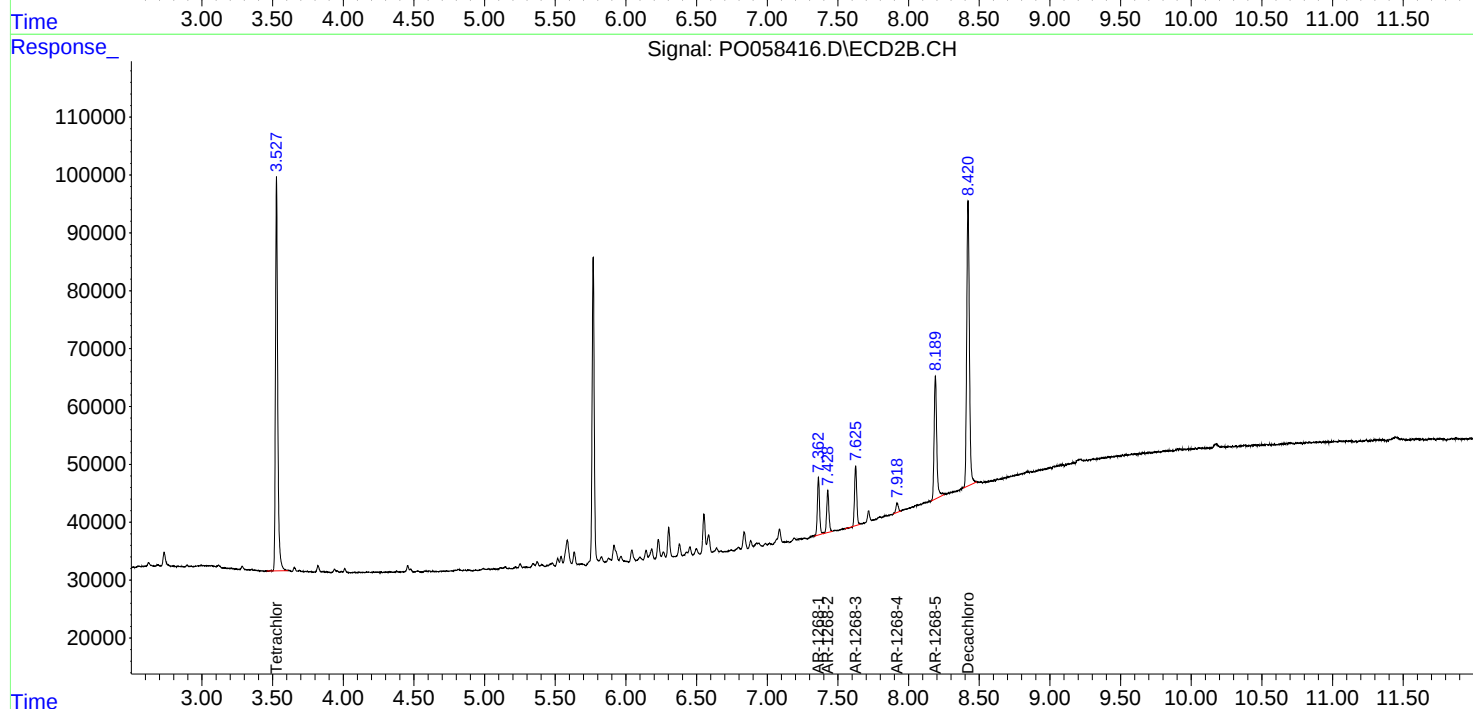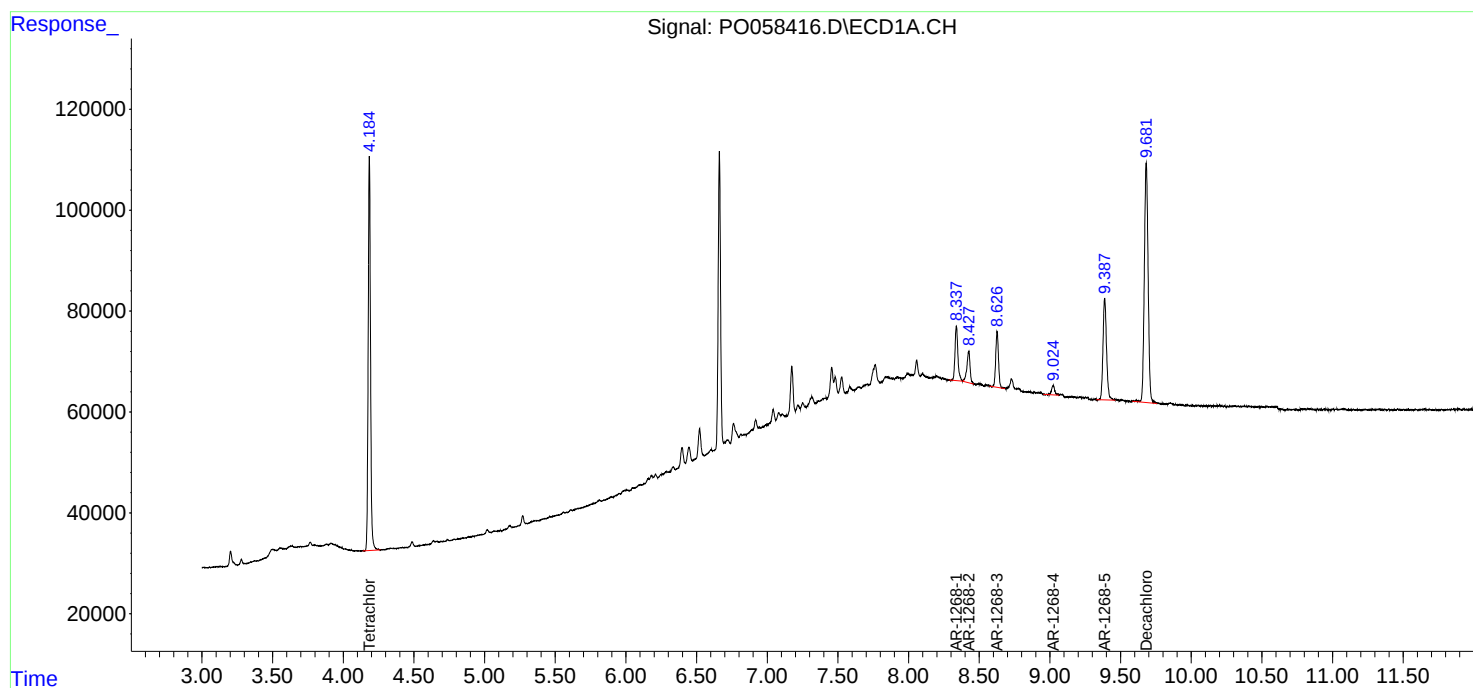

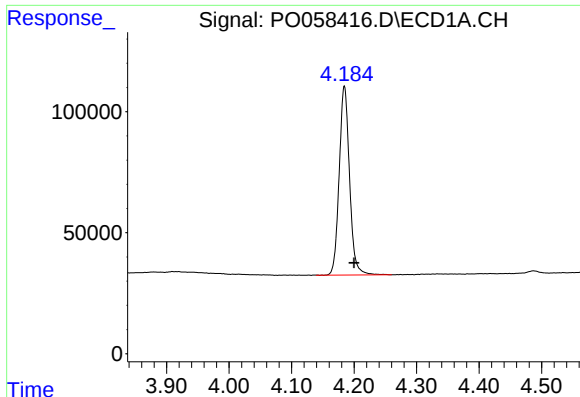


#1 Tetrachloro-m-xylene

R.T.: 4.185 min
Delta R.T.: -0.015 min
Response: 896524
Conc: 26.46 ng/ml

Instrument :
ECD_O
ClientSampleId :
S14-02-S


Manual Integrations
APPROVED

Ankita
7/27/2019 9:42:54 AM

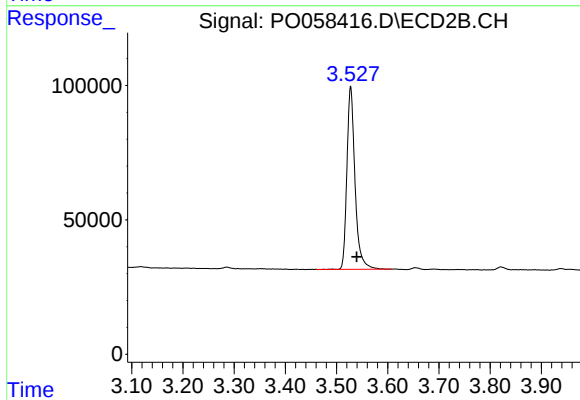


#1 Tetrachloro-m-xylene

R.T.: 3.528 min
Delta R.T.: -0.012 min
Response: 748707
Conc: 23.34 ng/ml

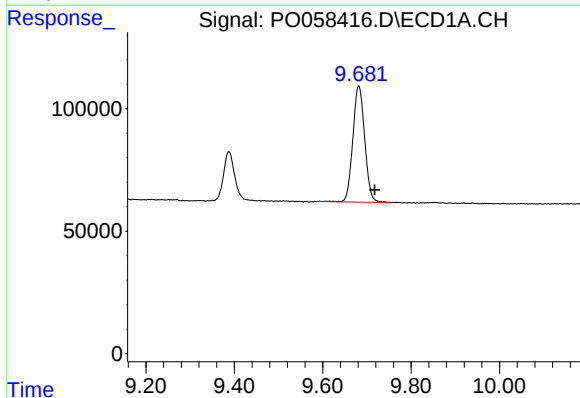


#2 Decachlorobiphenyl

R.T.: 9.681 min
Delta R.T.: -0.037 min
Response: 886745
Conc: 17.33 ng/ml

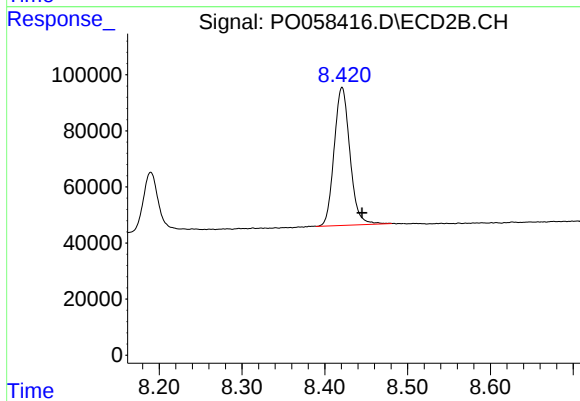

#2 Decachlorobiphenyl

R.T.: 8.420 min
Delta R.T.: -0.025 min
Response: 651585
Conc: 19.01 ng/ml m

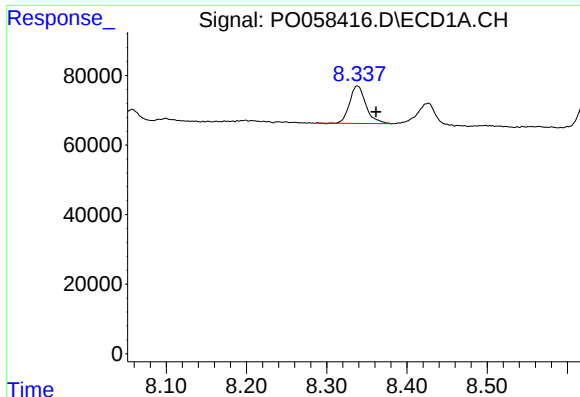


#41 AR-1268-1

R.T.: 8.338 min
Delta R.T.: -0.023 min
Response: 153128
Conc: 14.89 ng/ml

Instrument :
ECD_O
ClientSampleId :
S14-02-S


Manual Integrations
APPROVED

Ankita
7/27/2019 9:42:54 AM

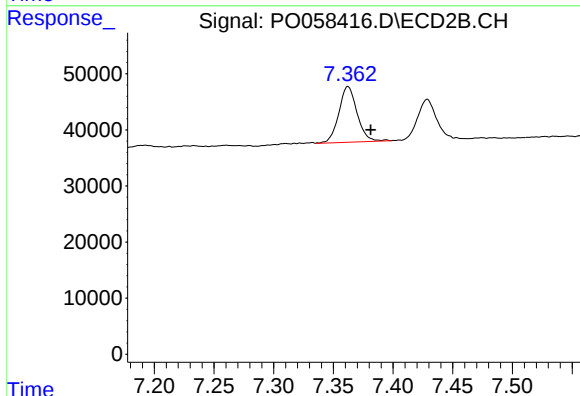


#41 AR-1268-1

R.T.: 7.362 min
Delta R.T.: -0.020 min
Response: 104375
Conc: 13.37 ng/ml m

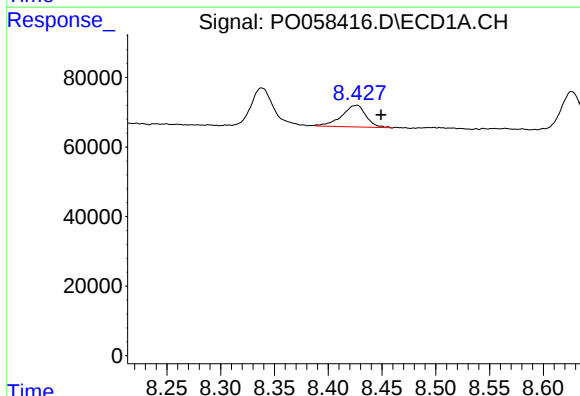


#42 AR-1268-2

R.T.: 8.427 min
Delta R.T.: -0.023 min
Response: 98512
Conc: 10.76 ng/ml m

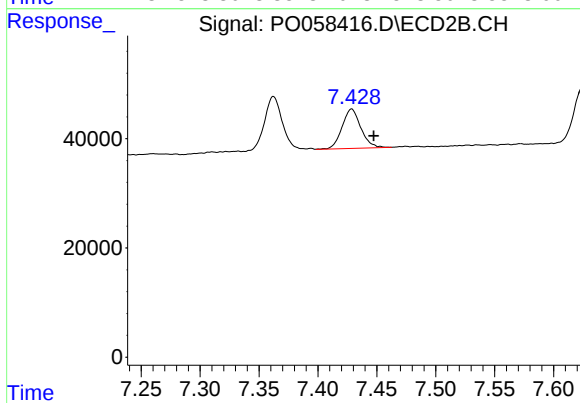

#42 AR-1268-2

R.T.: 7.429 min
Delta R.T.: -0.019 min
Response: 79996
Conc: 11.23 ng/ml

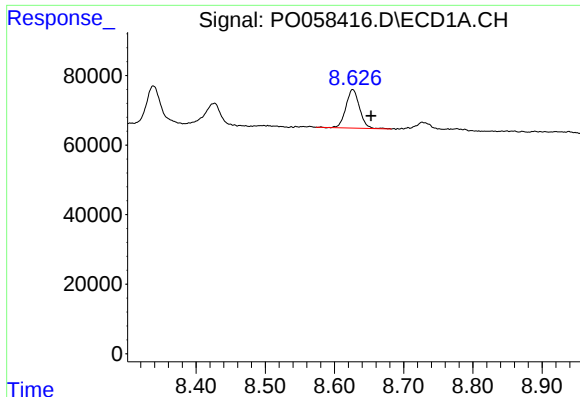


#43 AR-1268-3

R.T.: 8.626 min
Delta R.T.: -0.027 min
Response: 151557
Conc: 18.98 ng/ml

Instrument :
ECD_O
ClientSampleId :
S14-02-S


Manual Integrations
APPROVED

Ankita
7/27/2019 9:42:54 AM

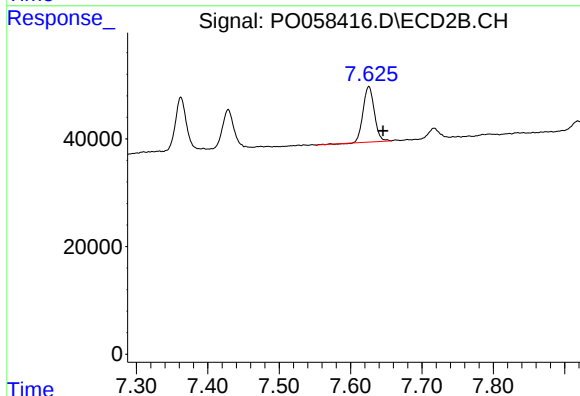


#43 AR-1268-3

R.T.: 7.626 min
Delta R.T.: -0.020 min
Response: 111787
Conc: 18.56 ng/ml

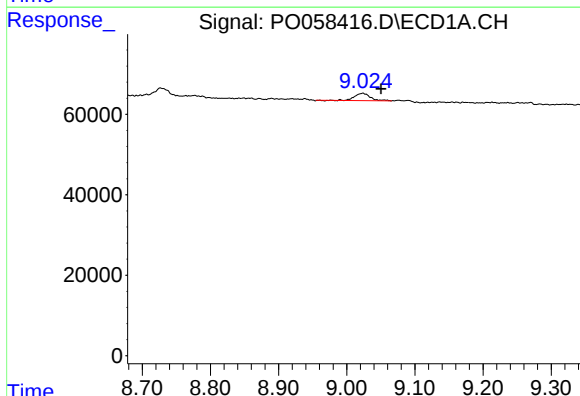


#44 AR-1268-4

R.T.: 9.024 min
Delta R.T.: -0.027 min
Response: 29777
Conc: 10.05 ng/ml

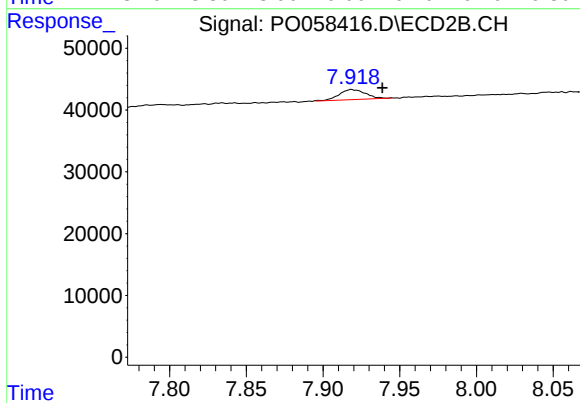

#44 AR-1268-4

R.T.: 7.918 min
Delta R.T.: -0.021 min
Response: 19648
Conc: 9.39 ng/ml m

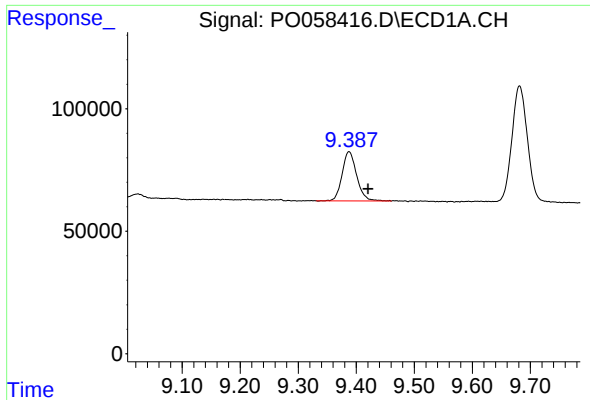


#45 AR-1268-5

R.T.: 9.388 min
Delta R.T.: -0.032 min
Response: 350928
Conc: 16.11 ng/ml

Instrument :
ECD_O
ClientSampleId :
S14-02-S

Manual Integrations
APPROVED

Ankita
7/27/2019 9:42:54 AM

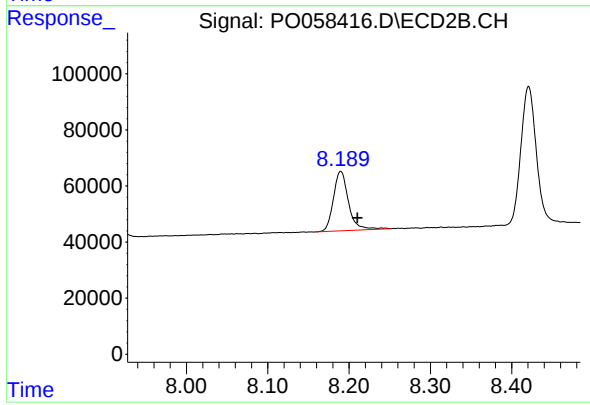

#45 AR-1268-5

R.T.: 8.189 min
Delta R.T.: -0.021 min
Response: 272581
Conc: 16.35 ng/ml m