

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072719\
 Data File : P0058450.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 26 Jul 2019 13:17
 Operator : SM/AJ
 Sample : K3849-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S12-03-S

Manual Integrations
 APPROVED

Ankita
 7/27/2019 9:47:40 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 26 14:15:36 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0071719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 17 11:13:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.185	3.530	911424	767857	26.896m	23.940
2) SA Decachlor...	9.685	8.424	1199502	763506	23.446m	22.275

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072719\
Data File : P0058450.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Jul 2019 13:17
Operator : SM/AJ
Sample : K3849-01
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
S12-03-S


Manual Integrations
APPROVED

Ankita
7/27/2019 9:47:40 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 26 14:15:36 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0071719.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 17 11:13:08 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

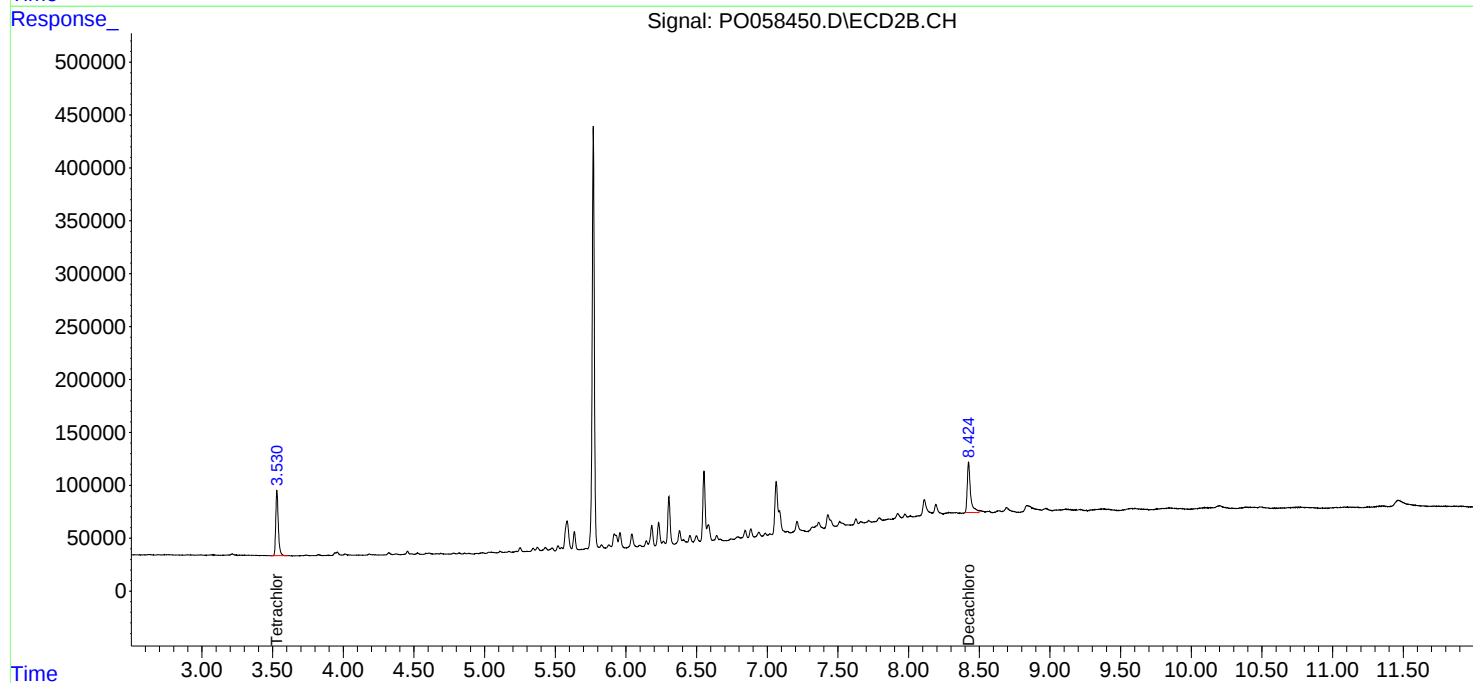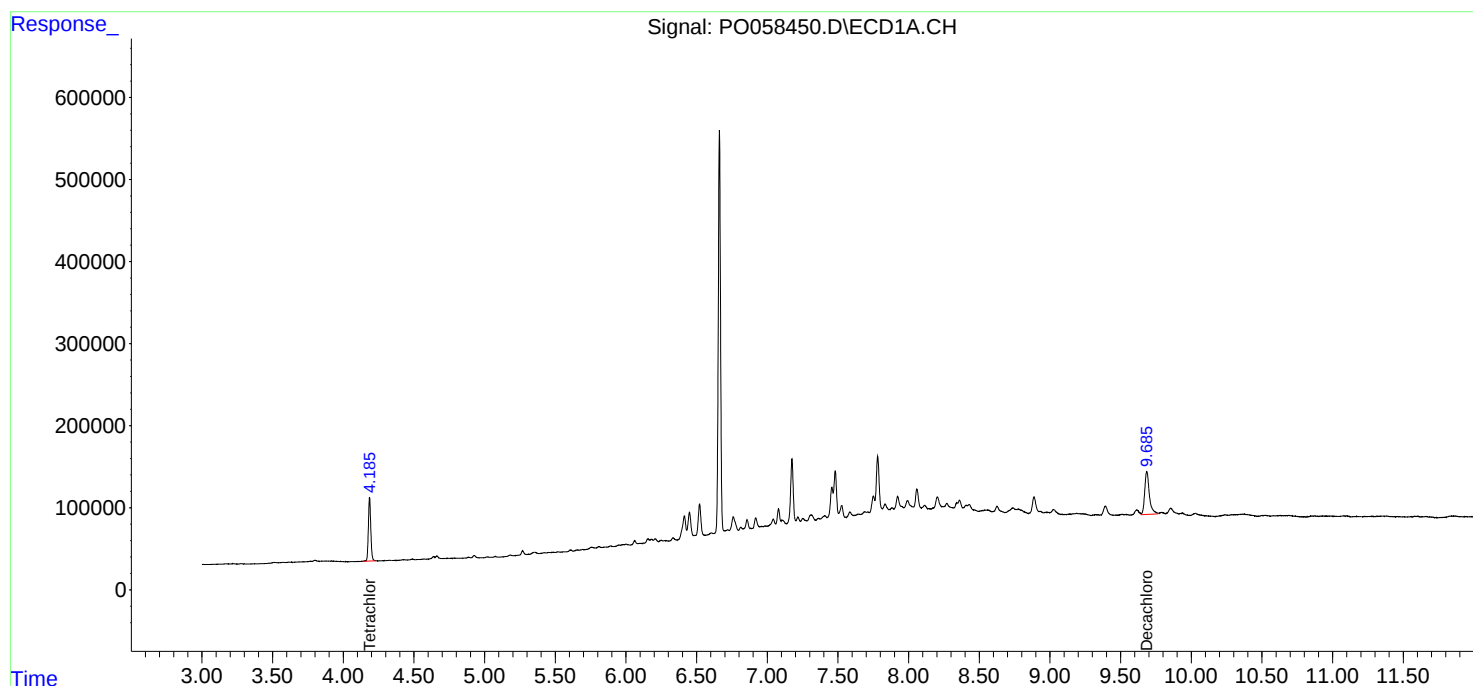

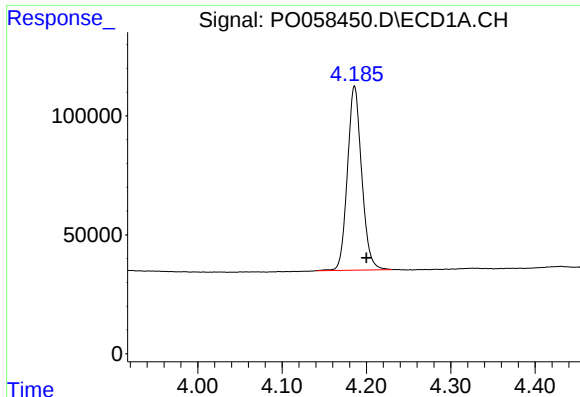


#1 Tetrachloro-m-xylene

R.T.: 4.185 min
Delta R.T.: -0.015 min
Response: 911424
Conc: 26.90 ng/ml m

Instrument :
ECD_O
ClientSampleId :
S12-03-S


Manual Integrations
APPROVED

Ankita
7/27/2019 9:47:40 AM

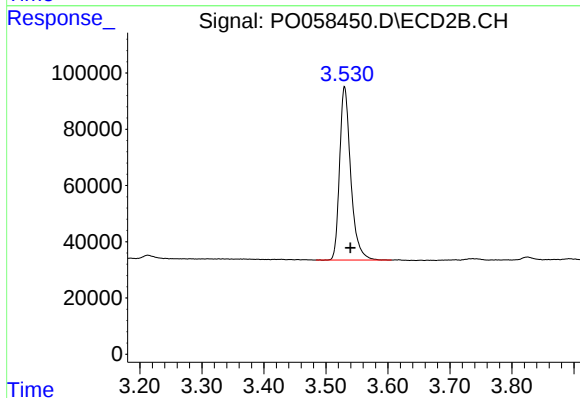


#1 Tetrachloro-m-xylene

R.T.: 3.530 min
Delta R.T.: -0.009 min
Response: 767857
Conc: 23.94 ng/ml

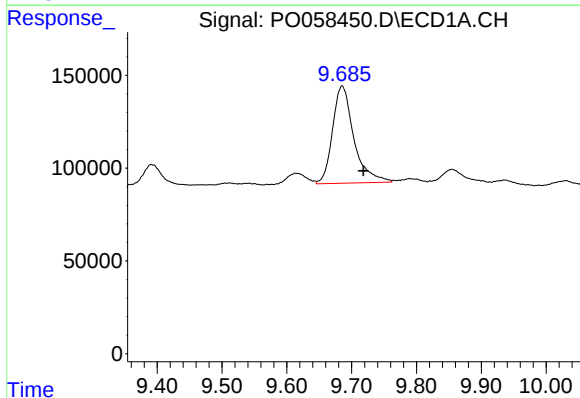

#2 Decachlorobiphenyl

R.T.: 9.685 min
Delta R.T.: -0.033 min
Response: 1199502
Conc: 23.45 ng/ml m

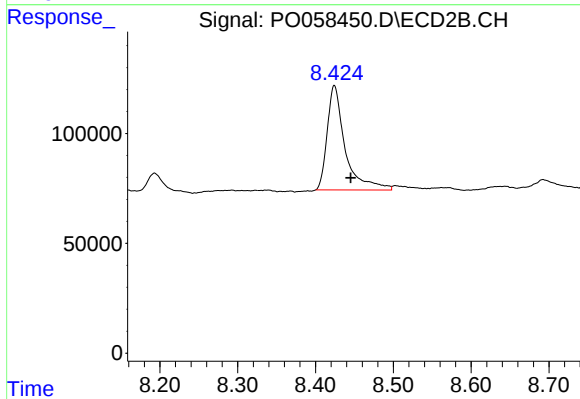

#2 Decachlorobiphenyl

R.T.: 8.424 min
Delta R.T.: -0.021 min
Response: 763506
Conc: 22.28 ng/ml