

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072719\
 Data File : P0058452.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 26 Jul 2019 14:28
 Operator : SM/AJ
 Sample : K4005-04RE
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S13-04-SRE

Manual Integrations
 APPROVED

Ankita
 7/27/2019 9:47:47 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 26 15:09:13 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0071719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 17 11:13:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.184	3.527	689120	654641	20.336m	20.411
2) SA Decachlor...	9.681	8.419	269698	194692	5.272m	5.680m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072719\
Data File : P0058452.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Jul 2019 14:28
Operator : SM/AJ
Sample : K4005-04RE
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
S13-04-SRE


Manual Integrations
APPROVED

Ankita
7/27/2019 9:47:47 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 26 15:09:13 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0071719.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 17 11:13:08 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

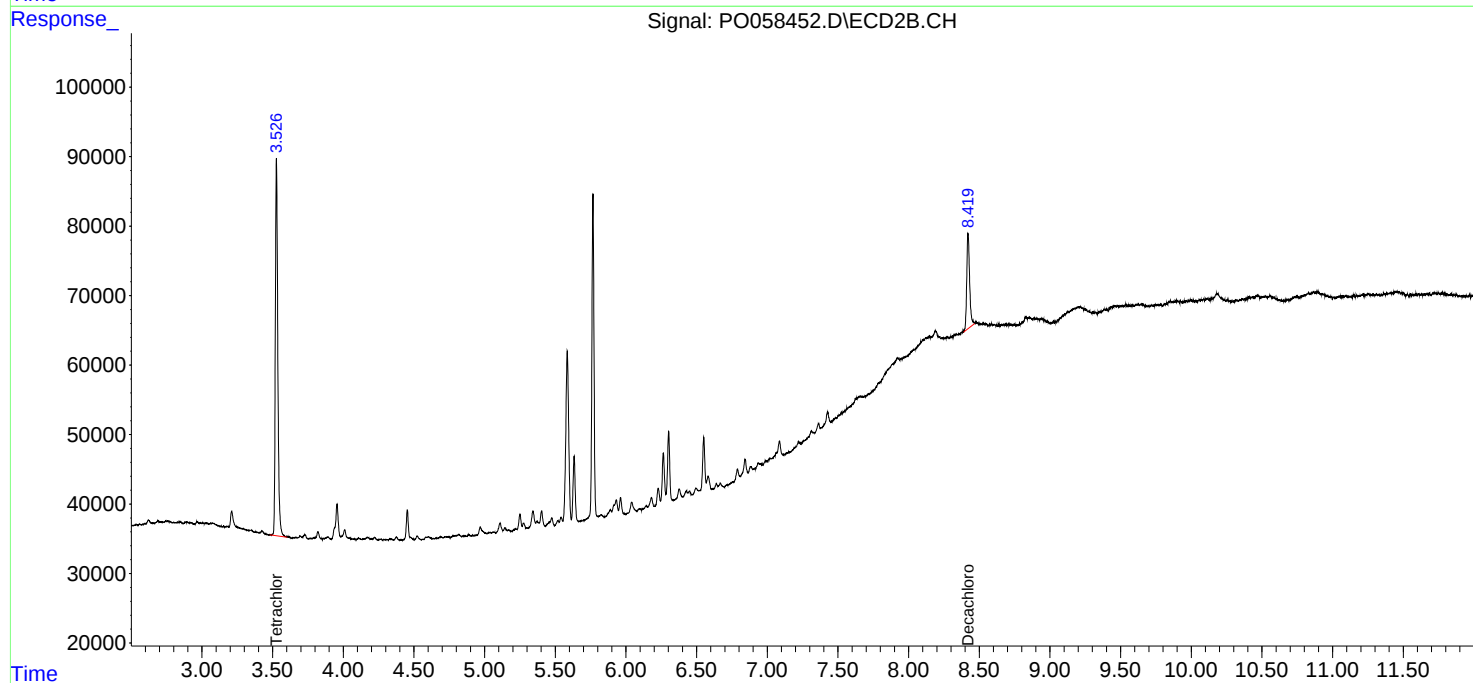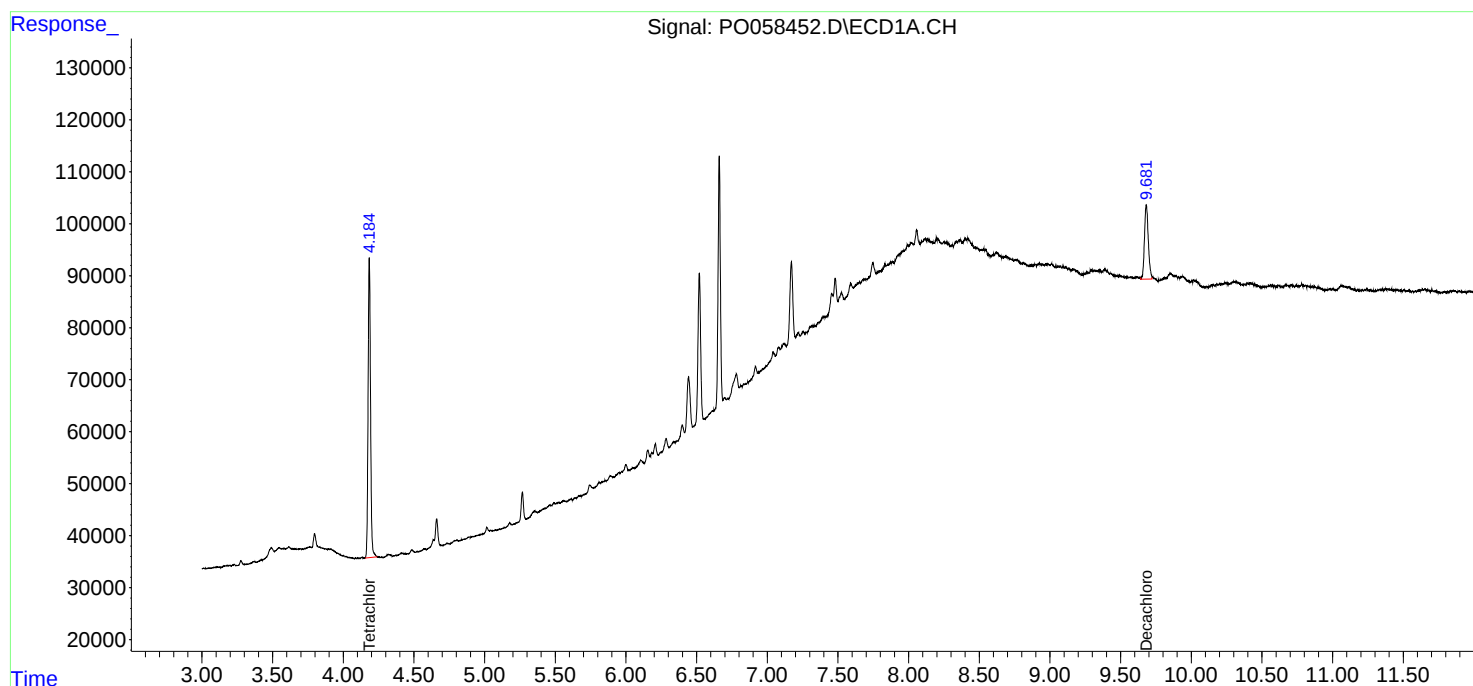

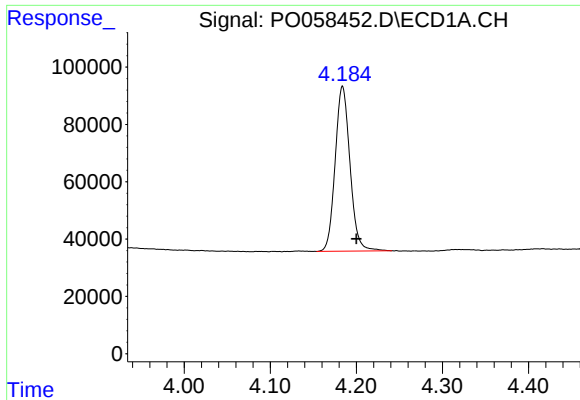


#1 Tetrachloro-m-xylene

R.T.: 4.184 min
Delta R.T.: -0.016 min
Response: 689120
Conc: 20.34 ng/ml m

Instrument :
ECD_O
ClientSampleId :
S13-04-SRE


Manual Integrations
APPROVED

Ankita
7/27/2019 9:47:47 AM

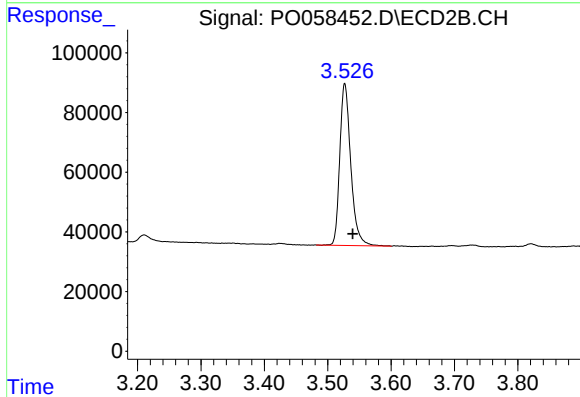


#1 Tetrachloro-m-xylene

R.T.: 3.527 min
Delta R.T.: -0.012 min
Response: 654641
Conc: 20.41 ng/ml

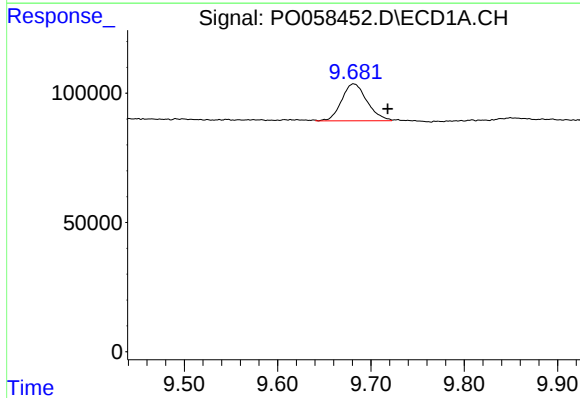

#2 Decachlorobiphenyl

R.T.: 9.681 min
Delta R.T.: -0.037 min
Response: 269698
Conc: 5.27 ng/ml m

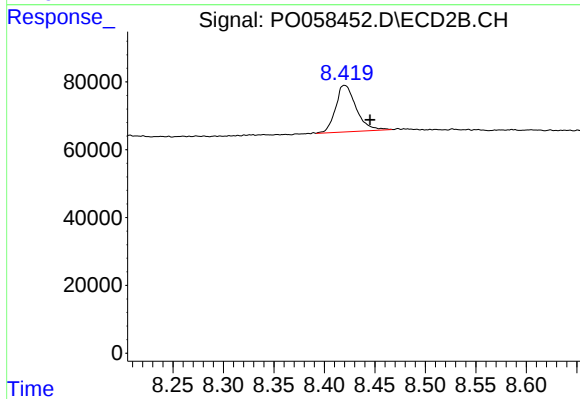

#2 Decachlorobiphenyl

R.T.: 8.419 min
Delta R.T.: -0.026 min
Response: 194692
Conc: 5.68 ng/ml m