

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0073019\
 Data File : P0058568.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 Jul 2019 17:13
 Operator : SM/AJ
 Sample : K4024-05
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-6-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 30 01:22:38 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072819.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jul 27 06:49:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.174	3.522	898451	818278	21.289	20.482
2) SA Decachlor...	9.663	8.412	936112	698416	17.286	17.694
Target Compounds						
27) L6 AR-1254-2	0.000	5.570	0	93024	N.D.	40.632 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0073019\
Data File : P0058568.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Jul 2019 17:13
Operator : SM/AJ
Sample : K4024-05
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP-6-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 30 01:22:38 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072819.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jul 27 06:49:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

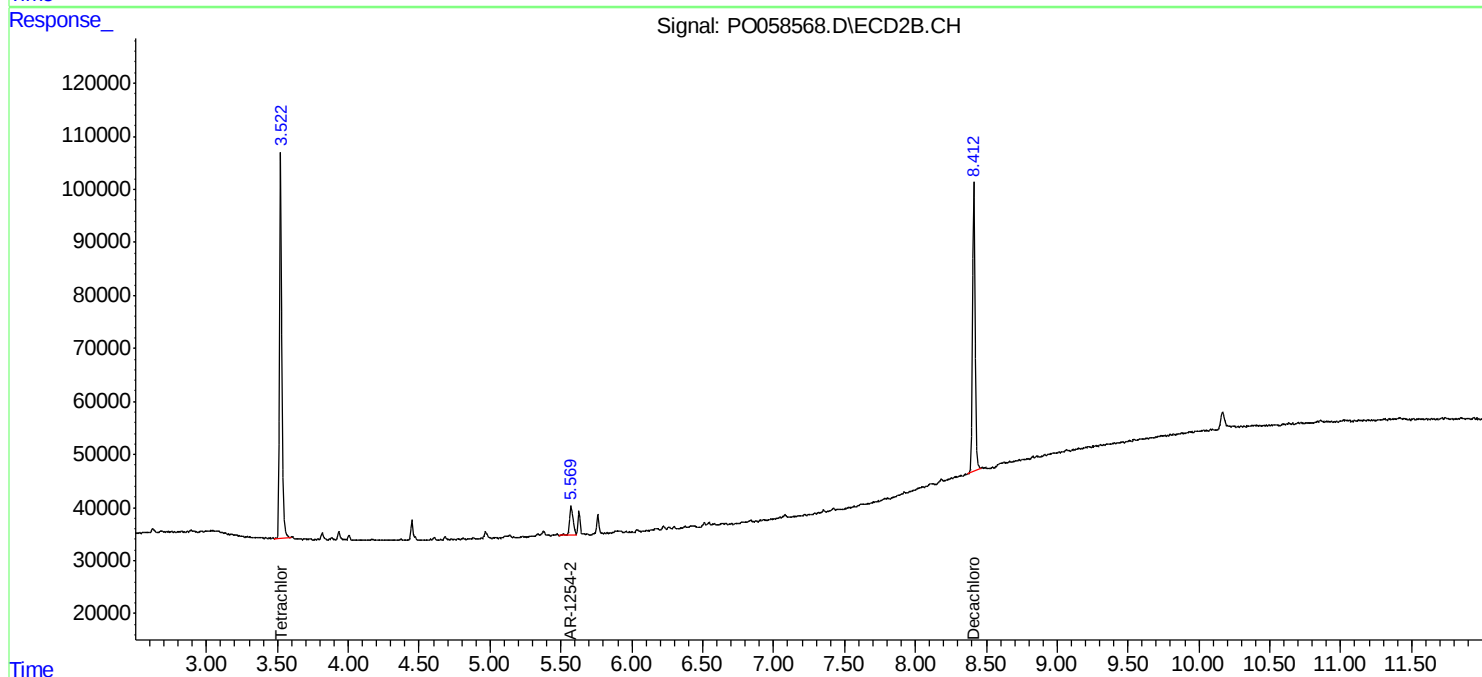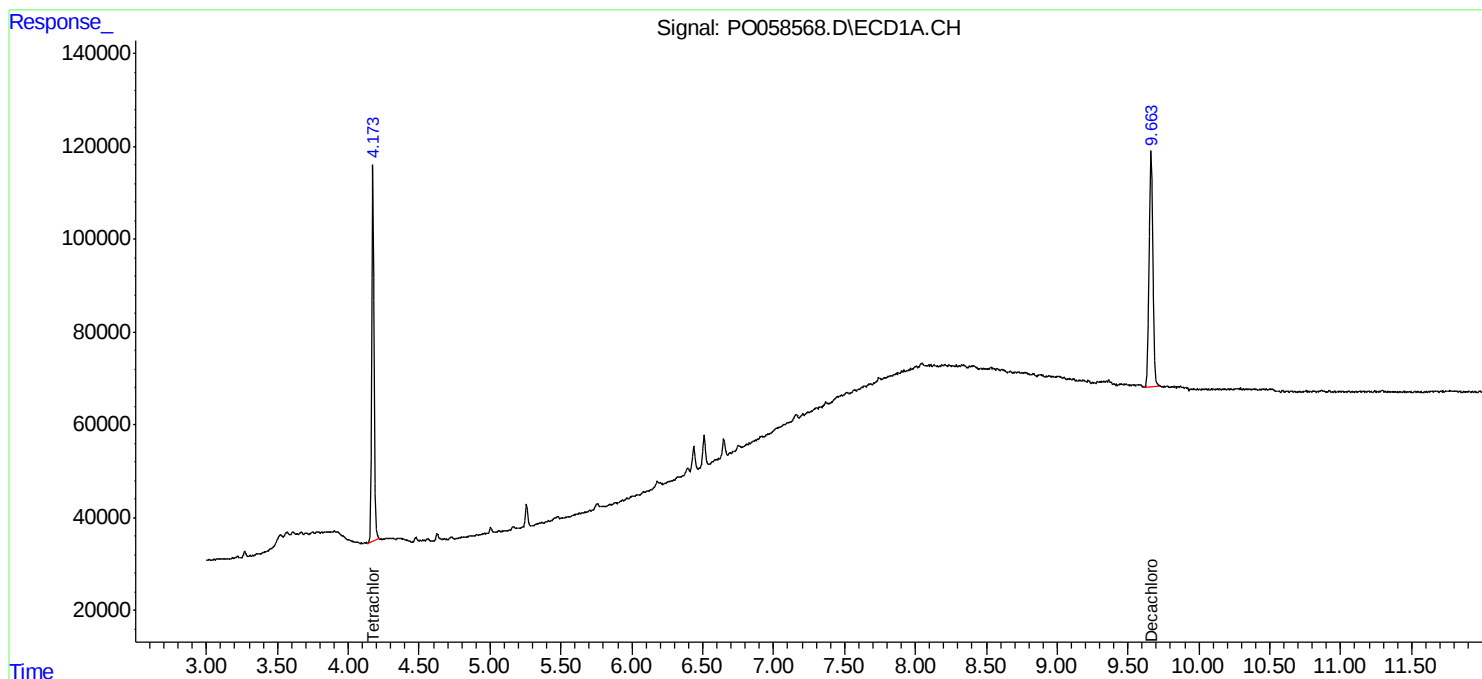


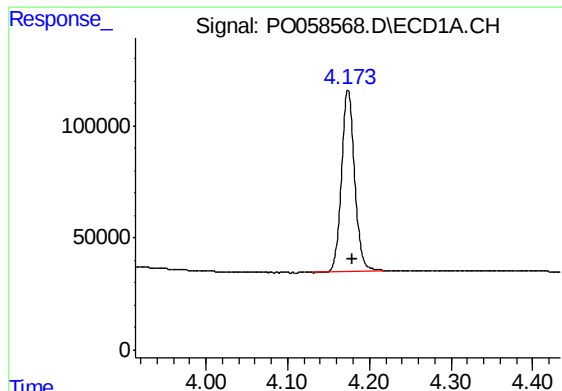

#1 Tetrachloro-m-xylene


R.T.: 4.174 min
Delta R.T.: -0.005 min
Response: 898451
Conc: 21.29 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-6-A

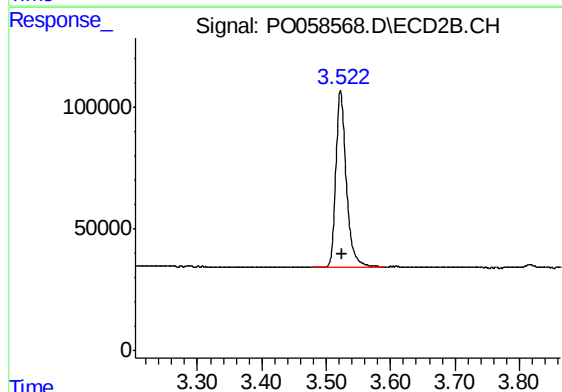


#1 Tetrachloro-m-xylene

R.T.: 3.522 min
Delta R.T.: -0.002 min
Response: 818278
Conc: 20.48 ng/ml

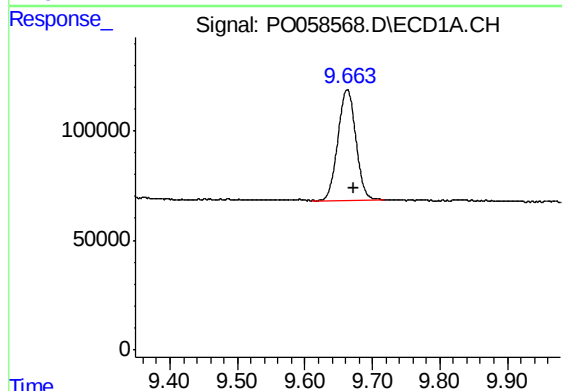


#2 Decachlorobiphenyl

R.T.: 9.663 min
Delta R.T.: -0.010 min
Response: 936112
Conc: 17.29 ng/ml

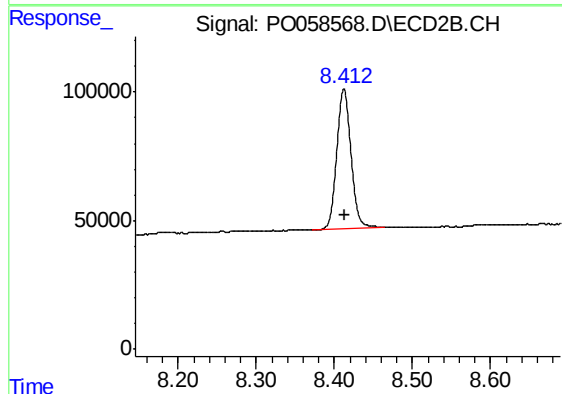

#2 Decachlorobiphenyl


R.T.: 8.412 min
Delta R.T.: -0.002 min
Response: 698416
Conc: 17.69 ng/ml

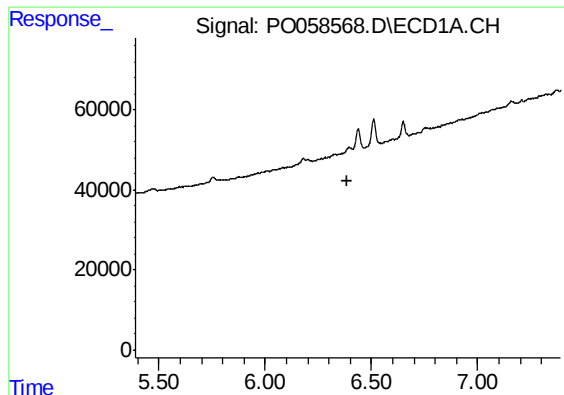

#27 AR-1254-2

R.T.: 0.000 min
Exp R.T. : 6.389 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
TP-6-A

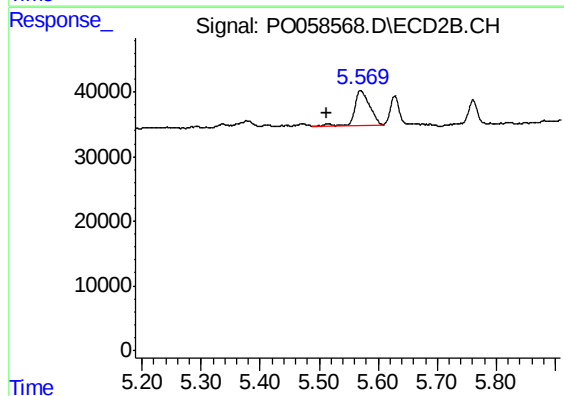

#27 AR-1254-2

R.T.: 5.570 min
Delta R.T.: 0.056 min
Response: 93024
Conc: 40.63 ng/ml