

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0073019\
 Data File : P0058557.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 Jul 2019 14:01
 Operator : SM/AJ
 Sample : K4021-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-10

Manual Integrations
 APPROVED

Ankita
 7/30/2019 2:16:15 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 30 01:18:19 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072819.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jul 27 06:49:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.175	3.523	783491	723770	18.565	18.117
2) SA Decachlor...	9.664	8.413	1038765	760963	19.181	19.278
Target Compounds						
31) L7 AR-1260-1	6.906	6.035	247818	202968	86.073	85.279
32) L7 AR-1260-2	7.162	6.222	513927	299803	123.538	98.968
33) L7 AR-1260-3	7.515	6.372	399769	197888	107.350	73.296 #
34) L7 AR-1260-4	7.740	6.836	370082	213144	108.599	94.331
35) L7 AR-1260-5	8.045	7.079	696926	603710	94.758m	112.102

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO073019\
Data File : PO058557.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Jul 2019 14:01
Operator : SM/AJ
Sample : K4021-01
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
TP-10


Manual Integrations
APPROVED

Ankita
7/30/2019 2:16:15 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 30 01:18:19 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO072819.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jul 27 06:49:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

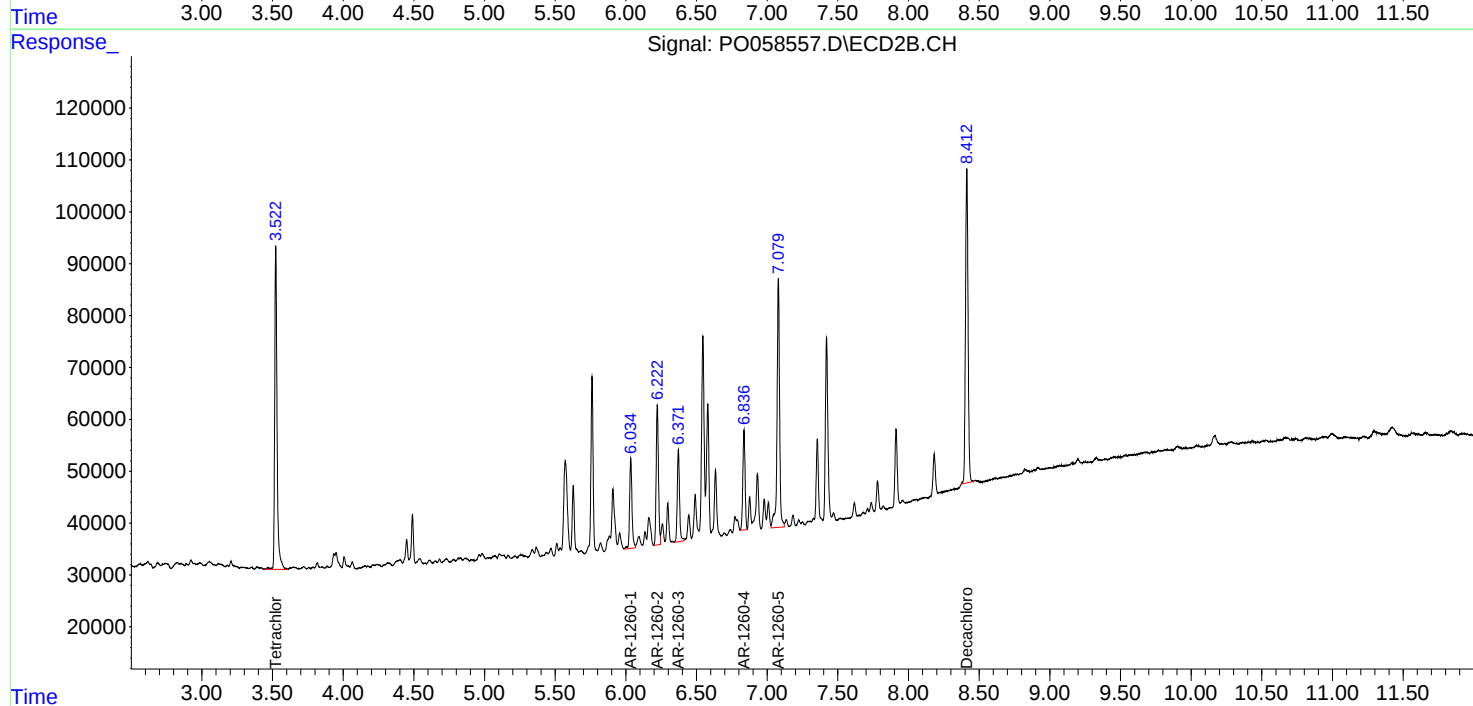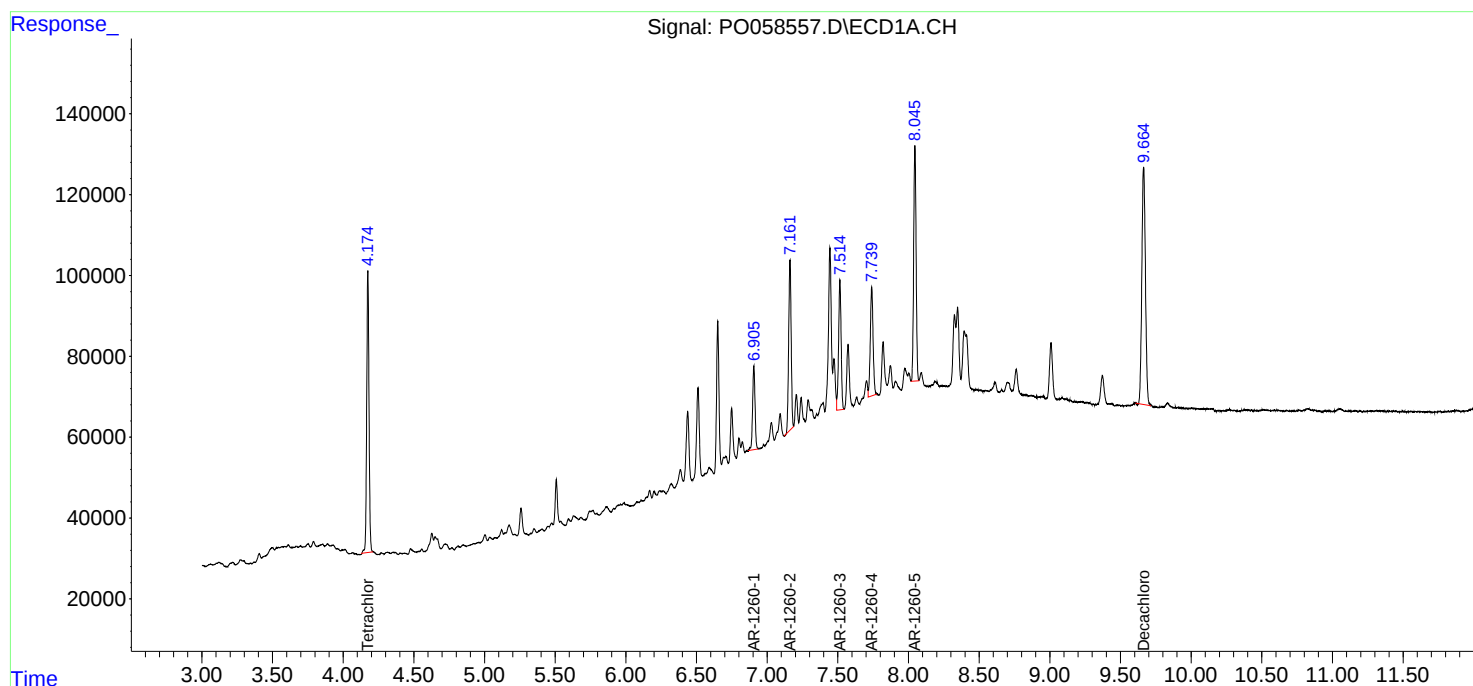

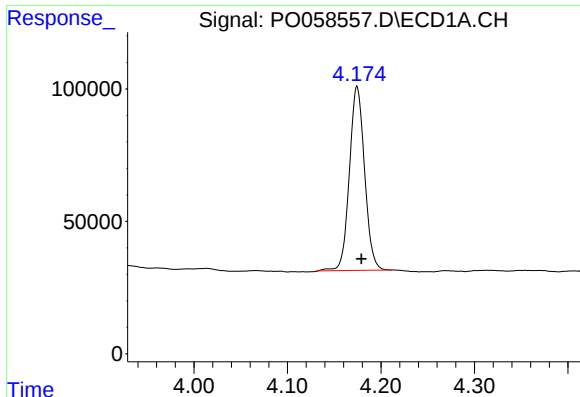


#1 Tetrachloro-m-xylene

R.T.: 4.175 min
Delta R.T.: -0.005 min
Response: 783491
Conc: 18.56 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-10


Manual Integrations
APPROVED

Ankita
7/30/2019 2:16:15 PM

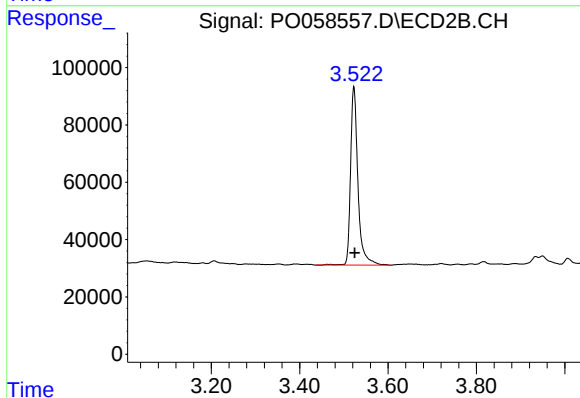


#1 Tetrachloro-m-xylene

R.T.: 3.523 min
Delta R.T.: -0.002 min
Response: 723770
Conc: 18.12 ng/ml

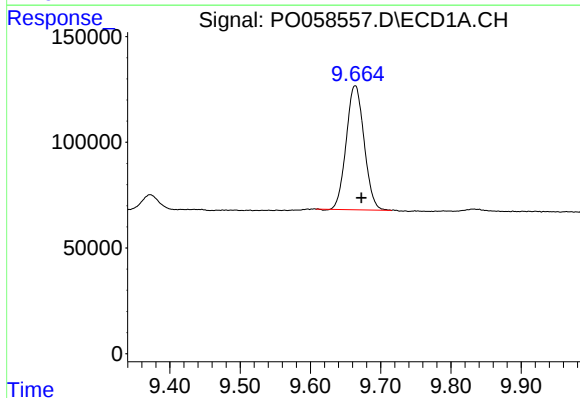


#2 Decachlorobiphenyl

R.T.: 9.664 min
Delta R.T.: -0.009 min
Response: 1038765
Conc: 19.18 ng/ml

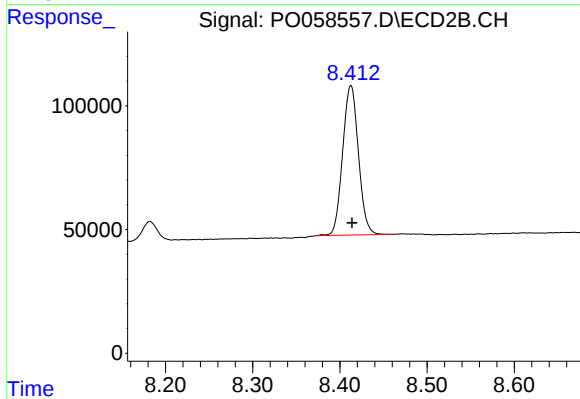

#2 Decachlorobiphenyl

R.T.: 8.413 min
Delta R.T.: -0.001 min
Response: 760963
Conc: 19.28 ng/ml

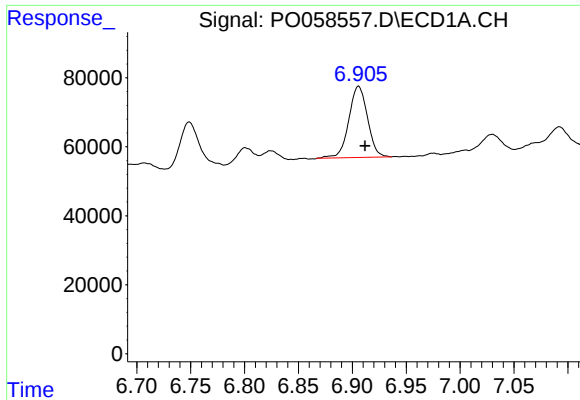


#31 AR-1260-1

R.T.: 6.906 min
Delta R.T.: -0.006 min
Response: 247818
Conc: 86.07 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-10


Manual Integrations
APPROVED

Ankita
7/30/2019 2:16:15 PM

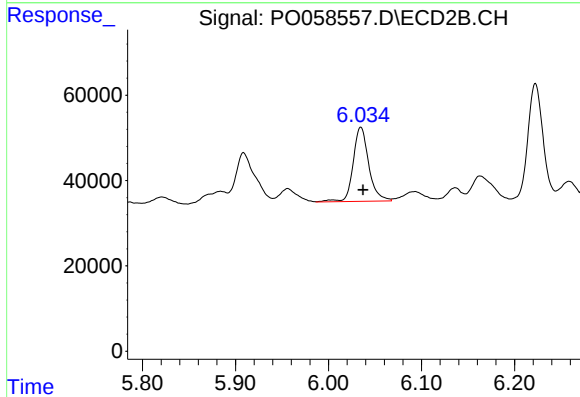


#31 AR-1260-1

R.T.: 6.035 min
Delta R.T.: -0.002 min
Response: 202968
Conc: 85.28 ng/ml

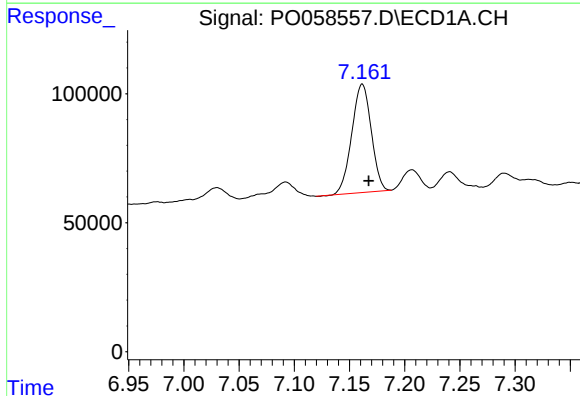


#32 AR-1260-2

R.T.: 7.162 min
Delta R.T.: -0.006 min
Response: 513927
Conc: 123.54 ng/ml

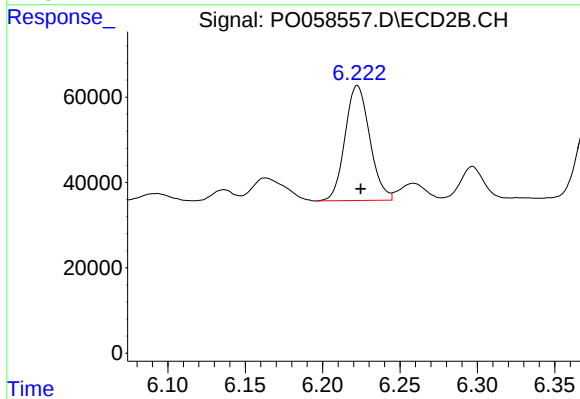

#32 AR-1260-2

R.T.: 6.222 min
Delta R.T.: -0.002 min
Response: 299803
Conc: 98.97 ng/ml

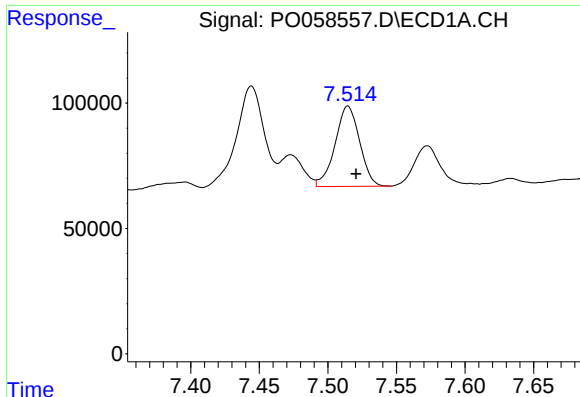


#33 AR-1260-3

R.T.: 7.515 min
Delta R.T.: -0.006 min
Response: 399769
Conc: 107.35 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-10


Manual Integrations
APPROVED

Ankita
7/30/2019 2:16:15 PM

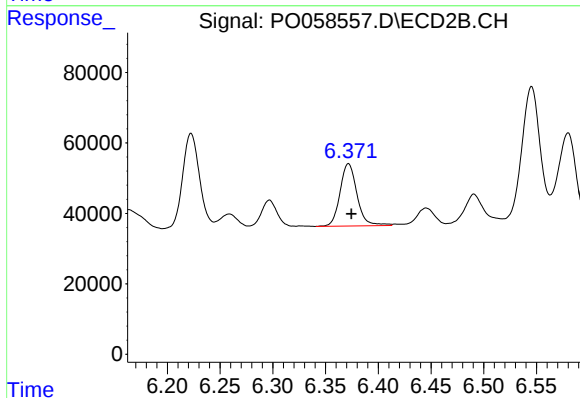


#33 AR-1260-3

R.T.: 6.372 min
Delta R.T.: -0.003 min
Response: 197888
Conc: 73.30 ng/ml

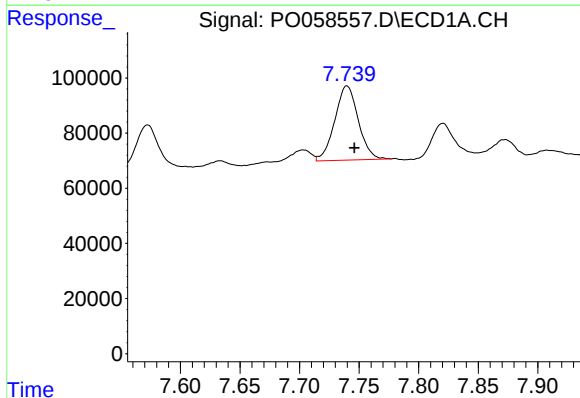


#34 AR-1260-4

R.T.: 7.740 min
Delta R.T.: -0.006 min
Response: 370082
Conc: 108.60 ng/ml

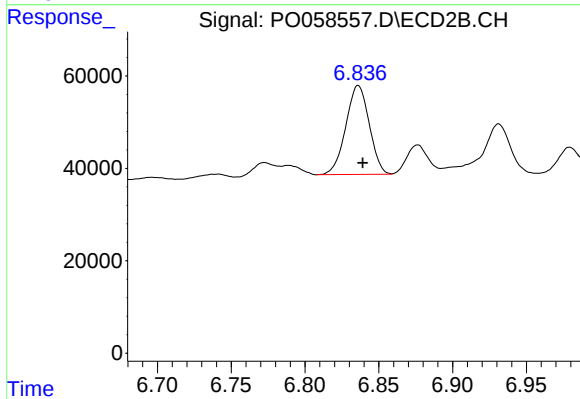

#34 AR-1260-4

R.T.: 6.836 min
Delta R.T.: -0.003 min
Response: 213144
Conc: 94.33 ng/ml

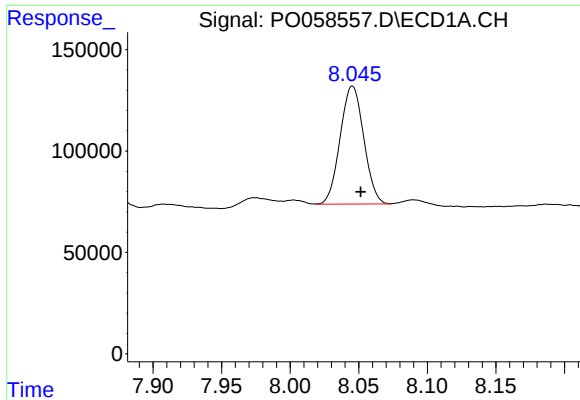


#35 AR-1260-5

R.T.: 8.045 min
Delta R.T.: -0.006 min
Response: 696926
Conc: 94.76 ng/ml m

Instrument :
ECD_O
ClientSampleId :
TP-10

Manual Integrations
APPROVED

Ankita
7/30/2019 2:16:15 PM

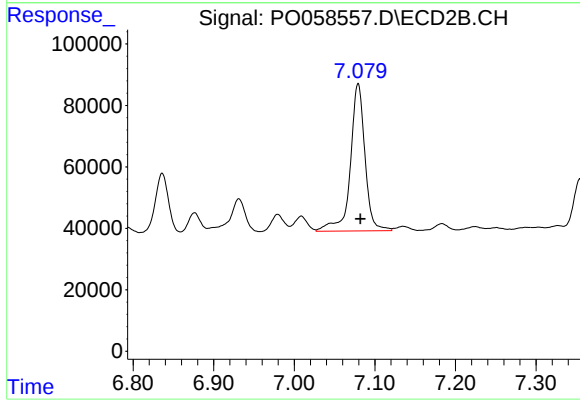

#35 AR-1260-5

R.T.: 7.079 min
Delta R.T.: -0.003 min
Response: 603710
Conc: 112.10 ng/ml