

Data Path : Z:\bestpcbsrv\HPCHEM1\ECD 0\Data\P0073118\
Data File : P0047441.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 31 Jul 2018 14:12
Operator : SM/SJ
Sample : J4188-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
HA-BASELINEWATER-N48971

Manual Integrations
APPROVED

Sohil
8/1/2018 4:44:15 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 31 15:43:24 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072718.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 27 02:33:29 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	nq/ml	nq/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.408	3.653	2809482	3553545	13.915	14.462m
2) SA Decachlor...	10.104	8.647	1819165	1851436	11.154	11.778

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0073118\
Data File : P0047441.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 31 Jul 2018 14:12
Operator : SM/SJ
Sample : J4188-01
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
HA-BASELINEWATER-N48971


Manual Integrations
APPROVED

Sohil
8/1/2018 4:44:15 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 31 15:43:24 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072718.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 27 02:33:29 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

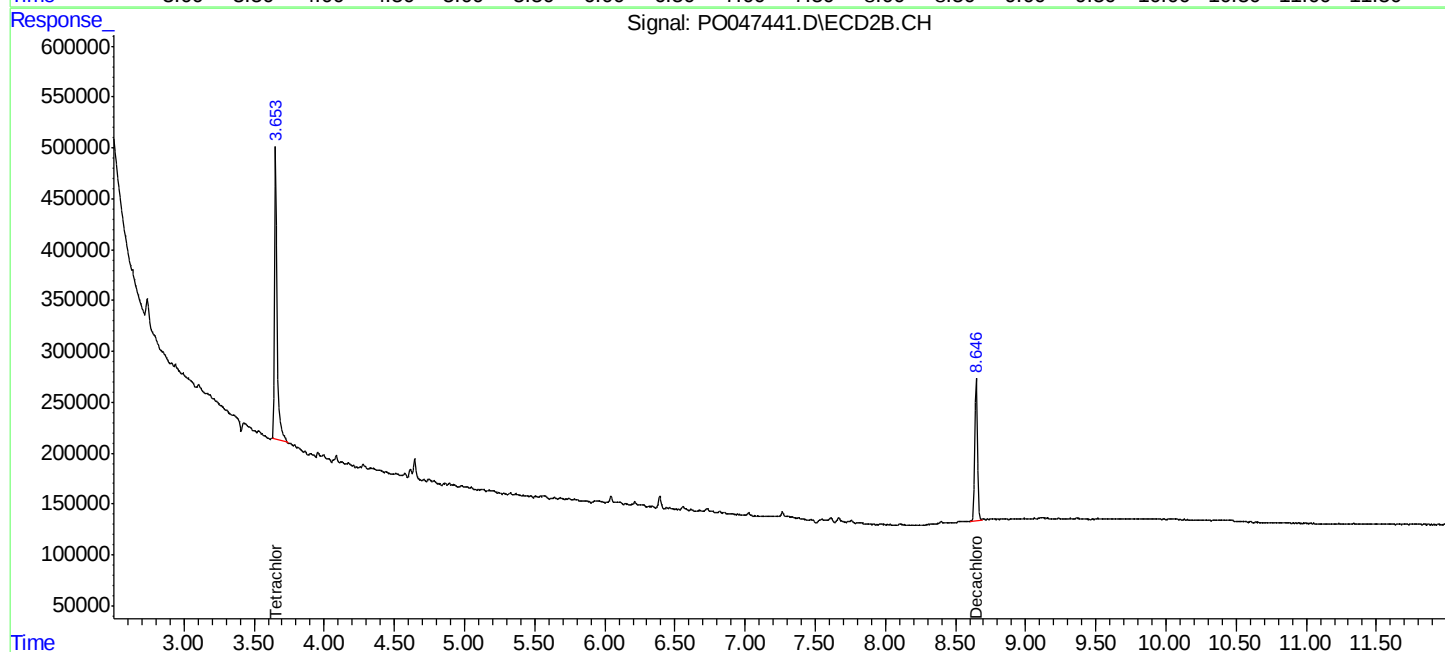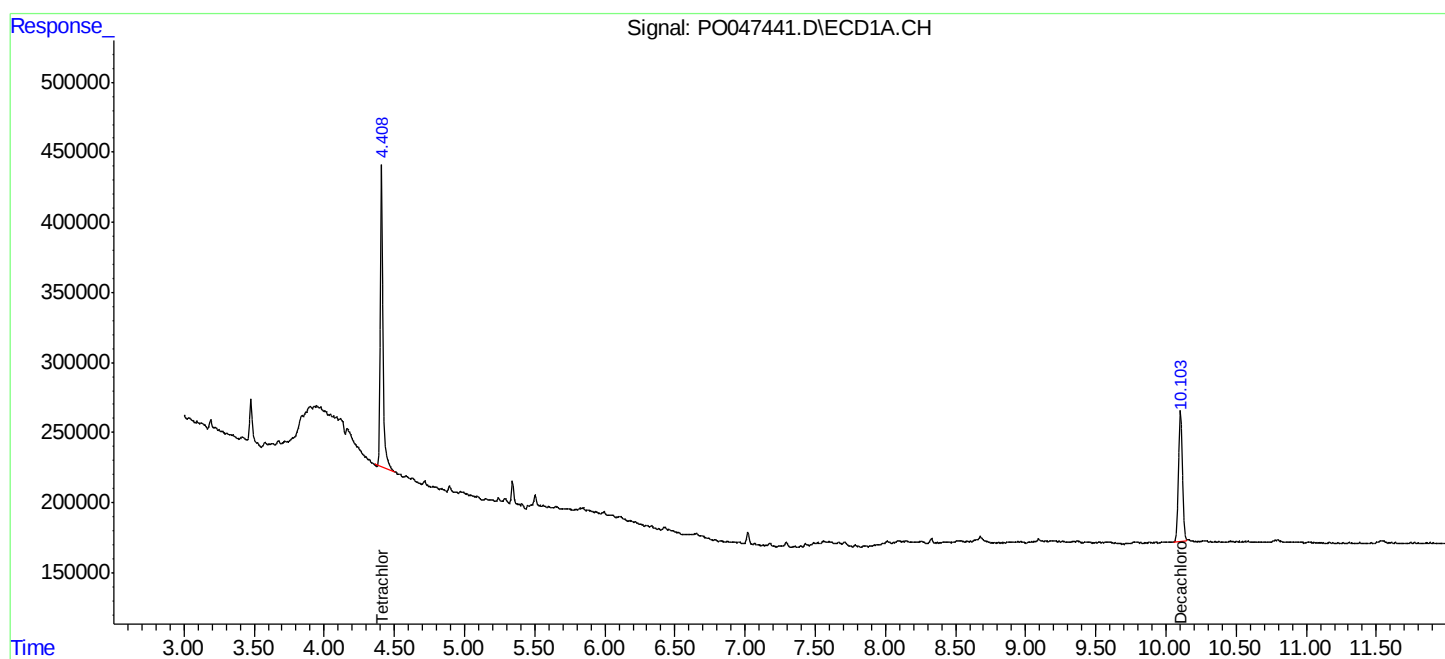

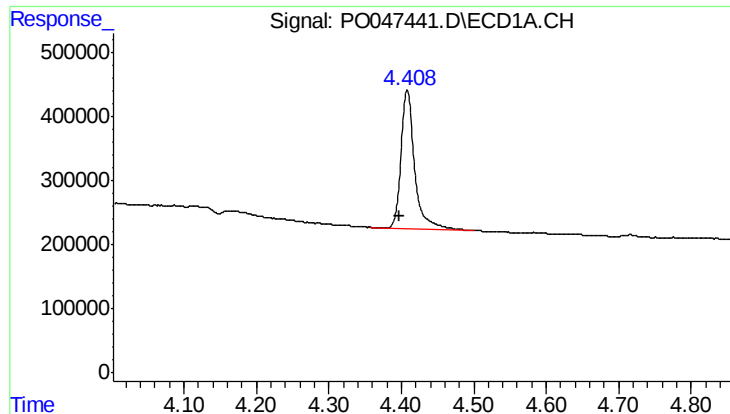


#1 Tetrachloro-m-xylene

R.T.: 4.408 min
Delta R.T.: 0.011 min
Response: 2809482
Conc: 13.92 ng/ml

Instrument :
ECD_O
ClientSampleId :
HA-BASELINEWATER-N48971


Manual Integrations
APPROVED

Sohil
8/1/2018 4:44:15 PM

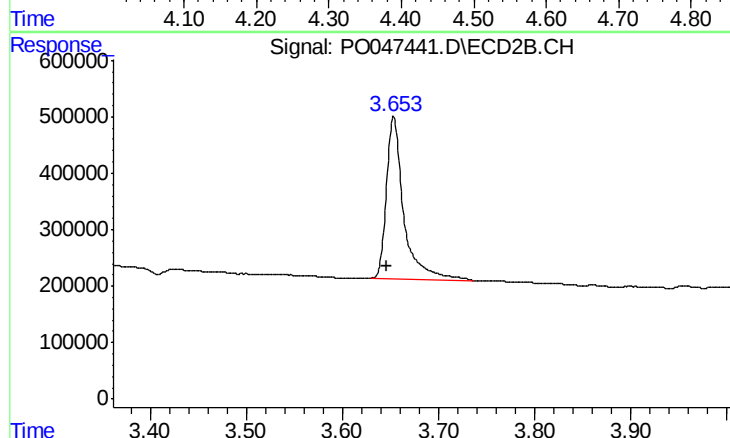


#1 Tetrachloro-m-xylene

R.T.: 3.653 min
Delta R.T.: 0.007 min
Response: 3553545
Conc: 14.46 ng/ml m

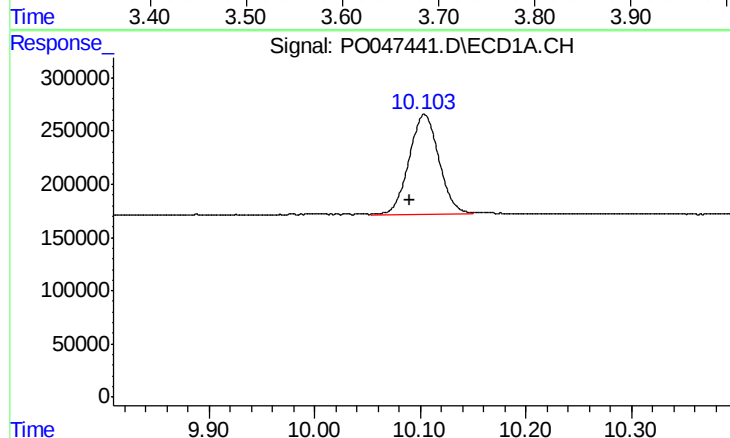

#2 Decachlorobiphenyl

R.T.: 10.104 min
Delta R.T.: 0.014 min
Response: 1819165
Conc: 11.15 ng/ml

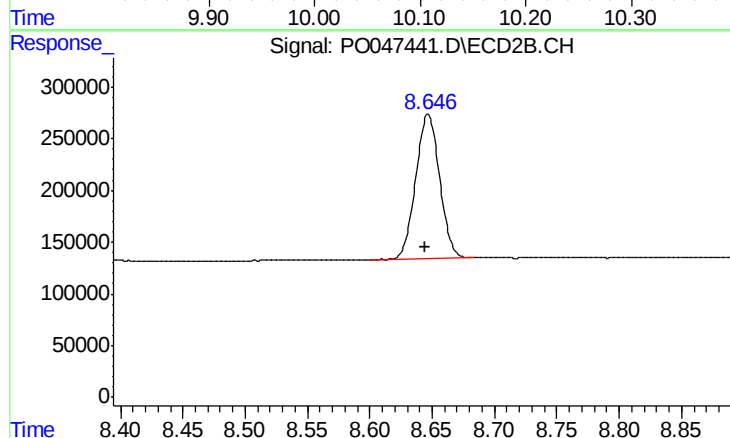

#2 Decachlorobiphenyl

R.T.: 8.647 min
Delta R.T.: 0.002 min
Response: 1851436
Conc: 11.78 ng/ml