

Data Path : Z:\bestpcbsrv\HPCHEM1\ECD 0\Data\P0073118\
Data File : P0047475.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 31 Jul 2018 23:21
Operator : SM/SJ
Sample : J3825-15
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
CL-01-073018-C

Manual Integrations
APPROVED

Sohil
8/1/2018 4:45:36 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 01 07:01:47 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072718.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 27 02:33:29 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	nq/ml	nq/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.407	3.652	3529539	4111044	17.482m	16.731
2)	SA Decachlor...	10.102	8.645	1927762	1715501	11.819	10.913

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0073118\
Data File : P0047475.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 31 Jul 2018 23:21
Operator : SM/SJ
Sample : J3825-15
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
CL-01-073018-C


Manual Integrations
APPROVED

Sohil
8/1/2018 4:45:36 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 01 07:01:47 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072718.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 27 02:33:29 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

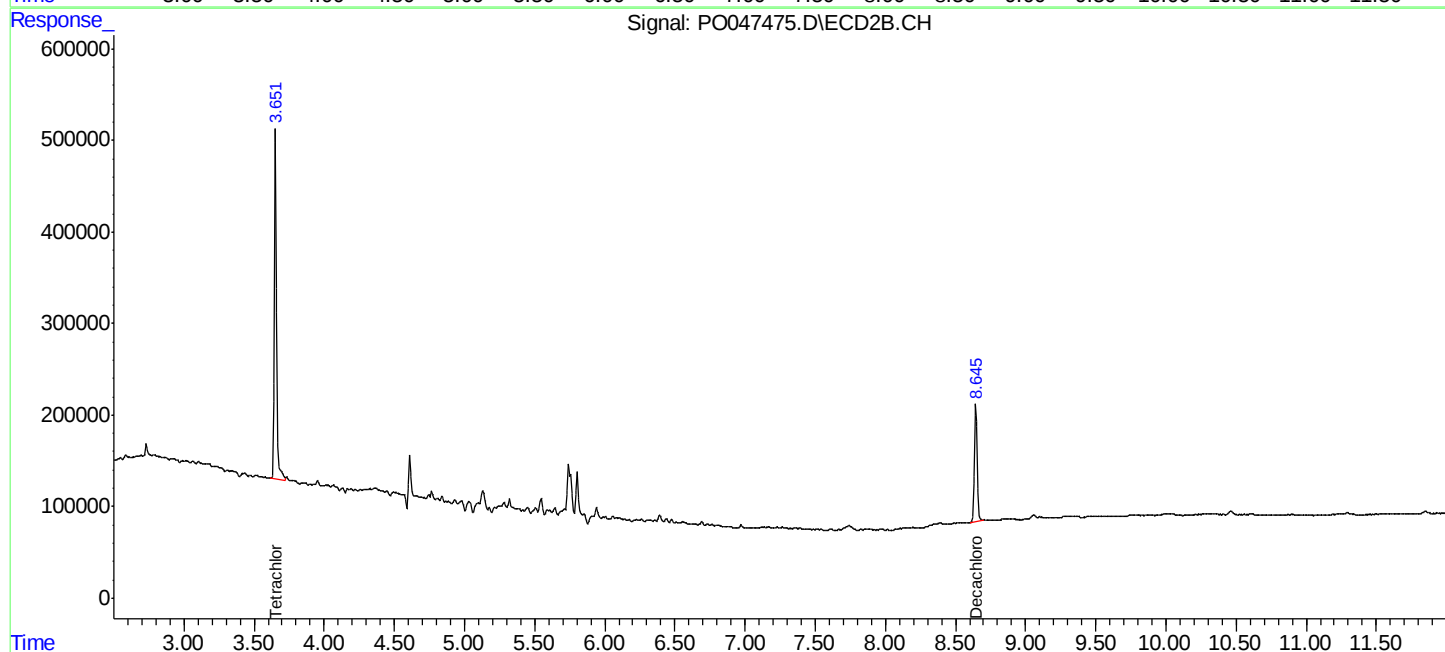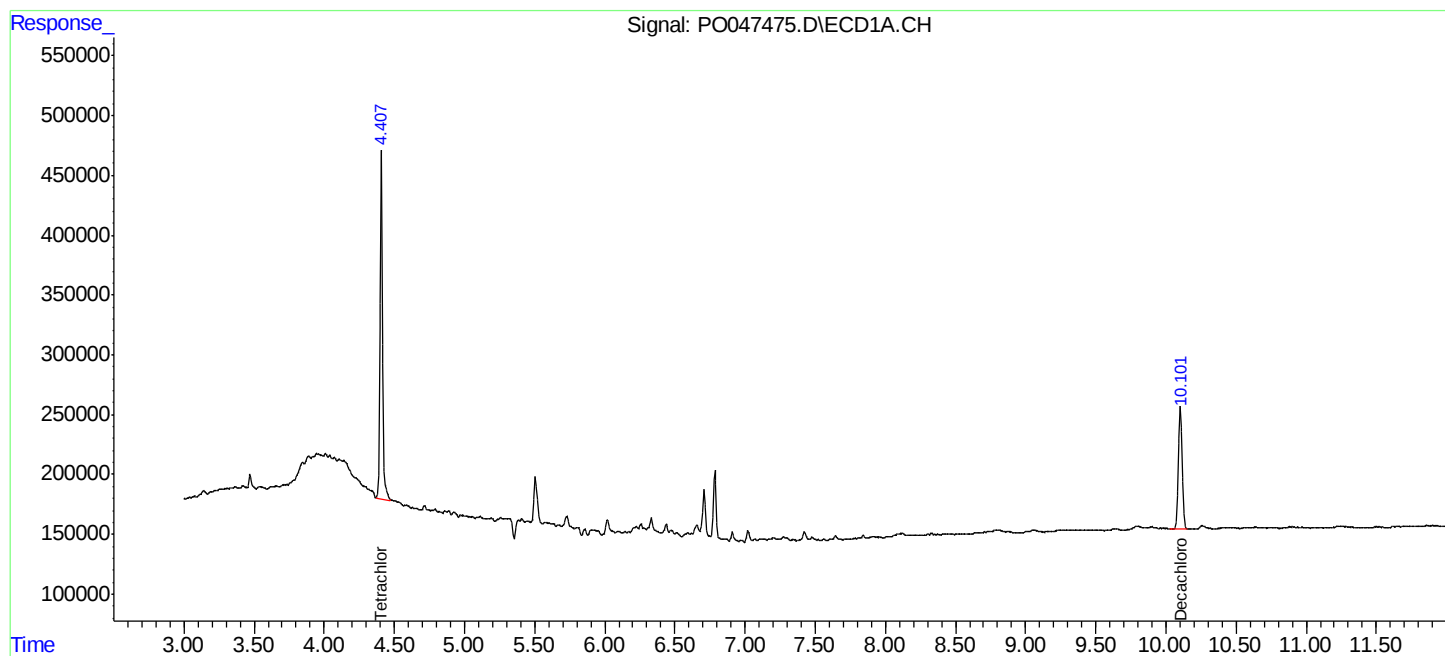

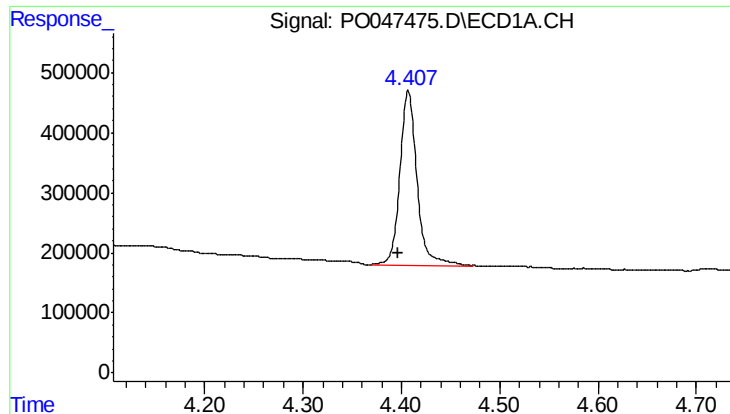


#1 Tetrachloro-m-xylene

R.T.: 4.407 min
Delta R.T.: 0.009 min
Response: 3529539
Conc: 17.48 ng/ml

Instrument :
ECD_O
ClientSampleId :
CL-01-073018-C


Manual Integrations
APPROVED

Sohil
8/1/2018 4:45:36 PM

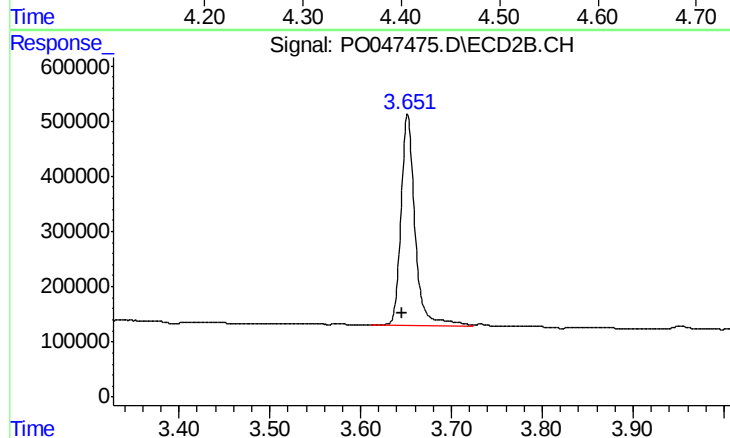


#1 Tetrachloro-m-xylene

R.T.: 3.652 min
Delta R.T.: 0.007 min
Response: 4111044
Conc: 16.73 ng/ml

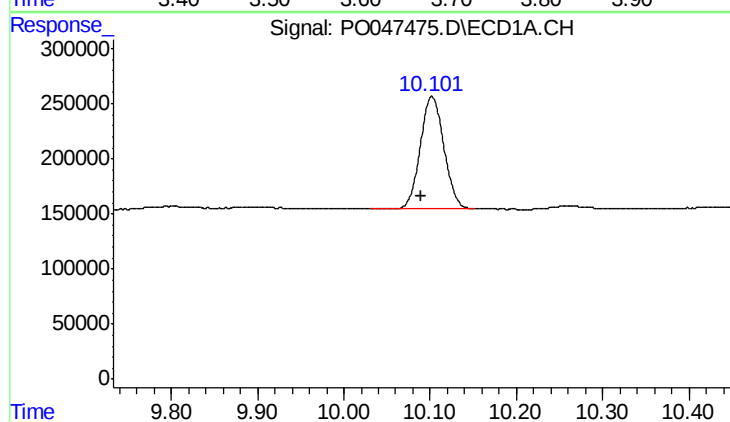

#2 Decachlorobiphenyl

R.T.: 10.102 min
Delta R.T.: 0.012 min
Response: 1927762
Conc: 11.82 ng/ml

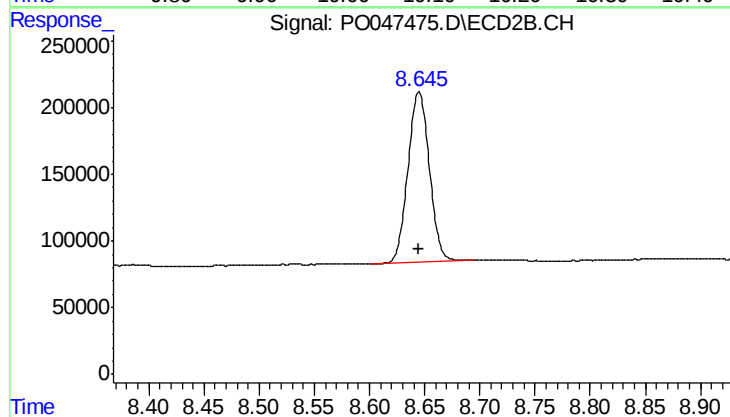

#2 Decachlorobiphenyl

R.T.: 8.645 min
Delta R.T.: 0.000 min
Response: 1715501
Conc: 10.91 ng/ml