

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0080218\
 Data File : P0047571.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Aug 2018 17:43
 Operator : SM/SJ
 Sample : J4257-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 FK-BPM-03-001-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 03 01:12:02 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072718.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jul 27 02:33:29 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.398	3.645	3570115	4426070	17.683	18.013
2) SA Decachlor...	10.088	8.632	2190640	2072467	13.431	13.184
Target Compounds						
3) L1 AR-1016-1	5.293	4.501	9464	94331	1.981	16.500 #
4) L1 AR-1016-2	5.688	4.918	26764	13026	4.546	2.481 #
5) L1 AR-1016-3	5.750	4.966	22576	33732	4.552	7.682 #
6) L1 AR-1016-4	6.059	4.996	18969	16895	4.078	3.258
7) L1 AR-1016-5	6.182	5.195	14261	592448	2.736	101.005 #
9) L2 AR-1221-2	4.703	3.944	39155	69564	23.945	38.347 #
10) L2 AR-1221-3	4.703	3.989	39155	18692	7.584	3.234 #
11) L3 AR-1232-1	0.000	4.323	0	91372	N.D.	38.853 #
12) L3 AR-1232-2	5.558	4.732	135829	137786	46.162	45.089
13) L3 AR-1232-3	5.558	4.732	135829	137786	31.616	29.838
14) L3 AR-1232-4	5.688	0.000	26764	0	9.670	N.D. #
15) L3 AR-1232-5	5.750	4.966	22576	33732	10.109	18.848 #
16) L4 AR-1242-1	5.558	4.732	135829	137786	18.480	17.206
17) L4 AR-1242-2	5.688	4.918	26764	13026	5.783	3.162 #
18) L4 AR-1242-3	5.750	4.996	22576	16895	5.876	4.029 #
19) L4 AR-1242-4	6.059	5.195	18969	592448	4.934	125.459 #
20) L4 AR-1242-5	6.182	5.356	14261	452835	3.331	116.960 #
21) L5 AR-1248-1	6.059	5.195	18969	592448	3.034	79.414 #
22) L5 AR-1248-2	6.182	5.356	14261	452835	2.618	84.643 #
23) L5 AR-1248-3	6.453	5.523	95709	55964	13.600	5.624 #
24) L5 AR-1248-4	6.486	5.551	19218	141749	2.863	20.226 #
25) L5 AR-1248-5	6.634	6.094	54760	1073462	7.737	225.244 #
26) L6 AR-1254-1	6.634	5.523	54760	55964	4.478	4.548
27) L6 AR-1254-2	6.902	5.672	86181	30008	11.556	2.883 #
28) L6 AR-1254-3	7.010	6.094	2632902	1073462	201.888	61.852 #
29) L6 AR-1254-4	7.290	6.306	29173	111444	2.993	10.285 #
30) L6 AR-1254-5	7.560	6.600	37245	200296	5.041	26.190 #
31) L7 AR-1260-1	7.159	6.205	36810	164050	3.926	14.846 #
32) L7 AR-1260-2	7.412	6.378	120788	3503432	10.832	261.293 #
33) L7 AR-1260-3	7.723	6.716	46871	138553	3.643	9.530 #
34) L7 AR-1260-4	8.311	7.251	186482	70613	10.484	3.209 #
35) L7 AR-1260-5	8.682	7.595	618099	61309	54.127	3.930 #
36) L8 AR-1262-1	7.159	6.378	36810	3503432	4.443	308.998 #
37) L8 AR-1262-2	7.412	6.600	120788	200296	12.463	17.750 #
38) L8 AR-1262-3	7.828	6.772	167703	31279	13.665	2.073 #
39) L8 AR-1262-4	7.994	7.009	47785	27497	4.058	2.088 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0080218\
Data File : P0047571.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Aug 2018 17:43
Operator : SM/SJ
Sample : J4257-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-001-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 03 01:12:02 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072718.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 27 02:33:29 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
40)	L8 AR-1262-5	8.311	7.251	186482	70613	8.679	2.734 #
41)	L9 AR-1268-1	8.581	7.543	33739	106031	1.454	4.078 #
42)	L9 AR-1268-2	8.682	7.595	618099	61309	28.847	2.461 #
43)	L9 AR-1268-3	8.931	7.813	122498	57149	6.785	2.896 #
44)	L9 AR-1268-4	9.358	8.046	177571	166569	22.269	19.857
45)	L9 AR-1268-5	9.785	8.373	224736	244229	4.125	4.473



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO080218\
Data File : PO047571.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Aug 2018 17:43
Operator : SM/SJ
Sample : J4257-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-001-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 03 01:12:02 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO072718.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 27 02:33:29 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

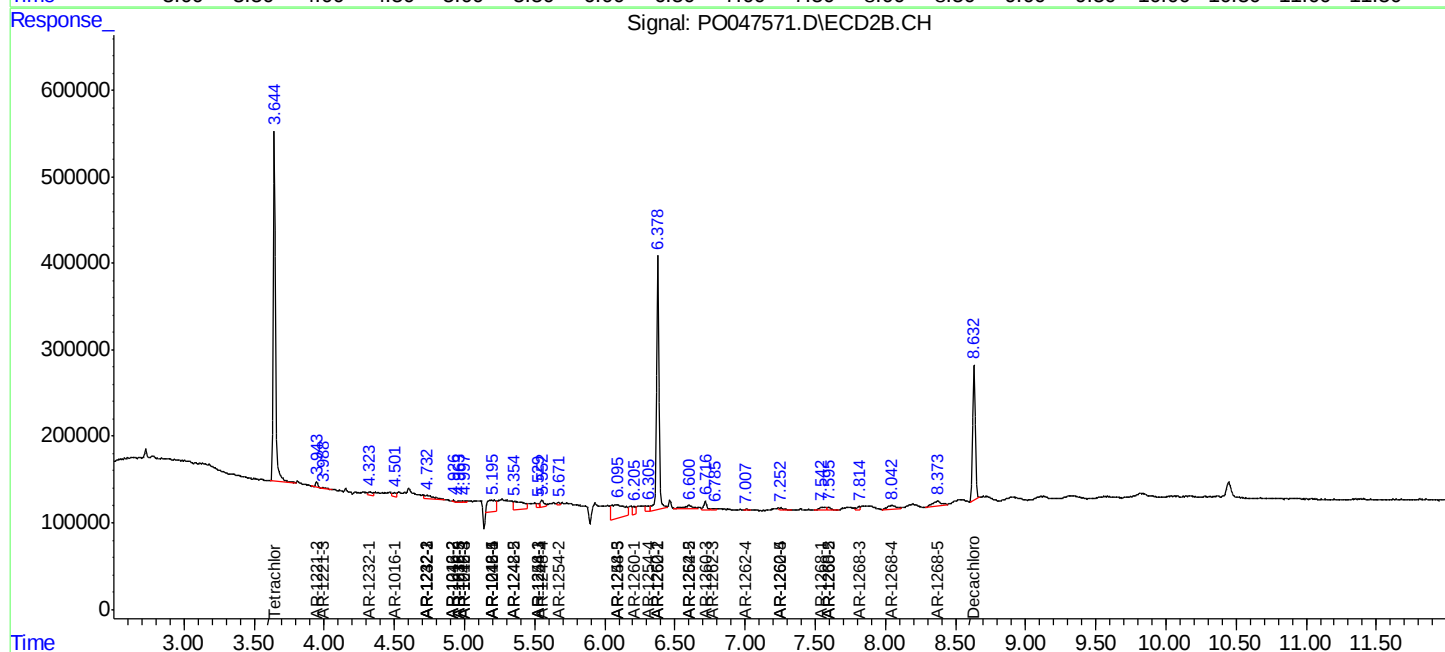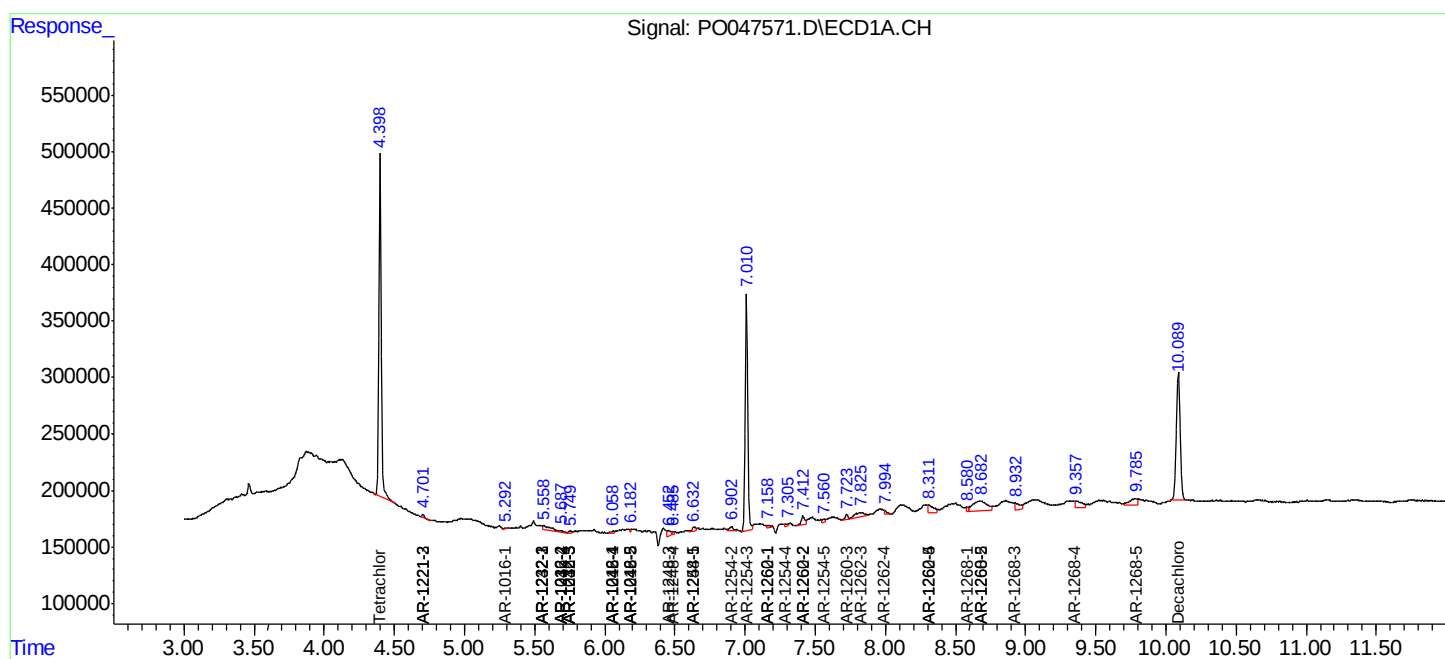


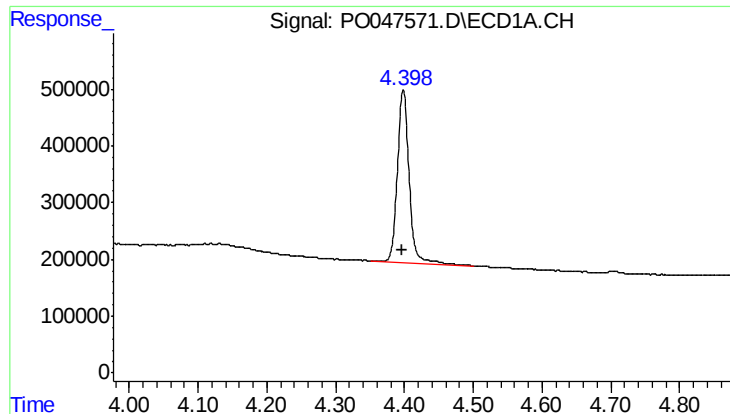

#1 Tetrachloro-m-xylene


R.T.: 4.398 min
Delta R.T.: 0.000 min
Response: 3570115
Conc: 17.68 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-001-A

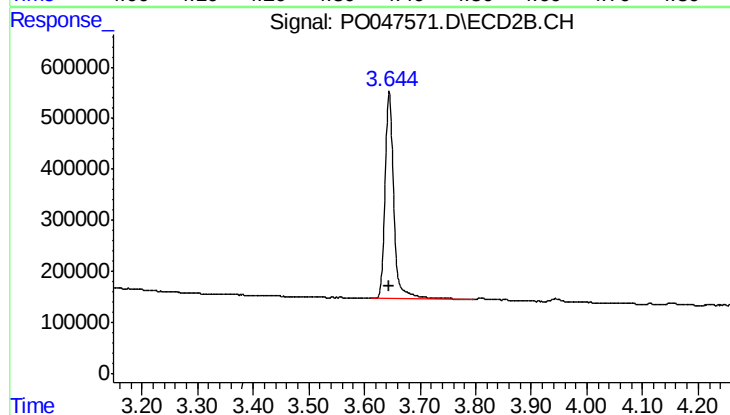


#1 Tetrachloro-m-xylene

R.T.: 3.645 min
Delta R.T.: 0.000 min
Response: 4426070
Conc: 18.01 ng/ml

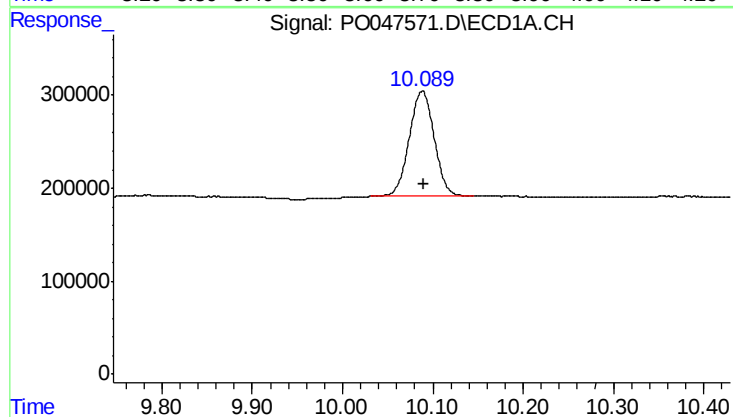


#2 Decachlorobiphenyl

R.T.: 10.088 min
Delta R.T.: -0.001 min
Response: 2190640
Conc: 13.43 ng/ml

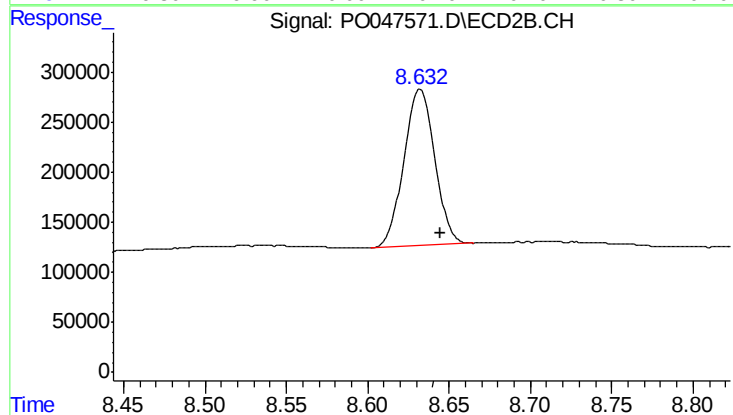

#2 Decachlorobiphenyl


R.T.: 8.632 min
Delta R.T.: -0.012 min
Response: 2072467
Conc: 13.18 ng/ml

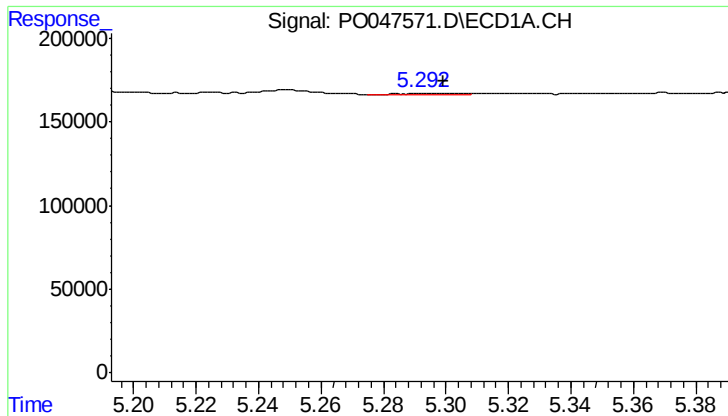

#3 AR-1016-1


R.T.: 5.293 min
Delta R.T.: -0.007 min
Response: 9464
Conc: 1.98 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-001-A

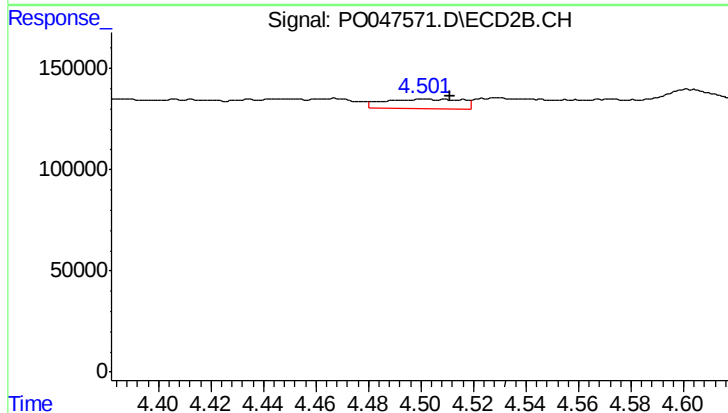


#3 AR-1016-1

R.T.: 4.501 min
Delta R.T.: -0.010 min
Response: 94331
Conc: 16.50 ng/ml

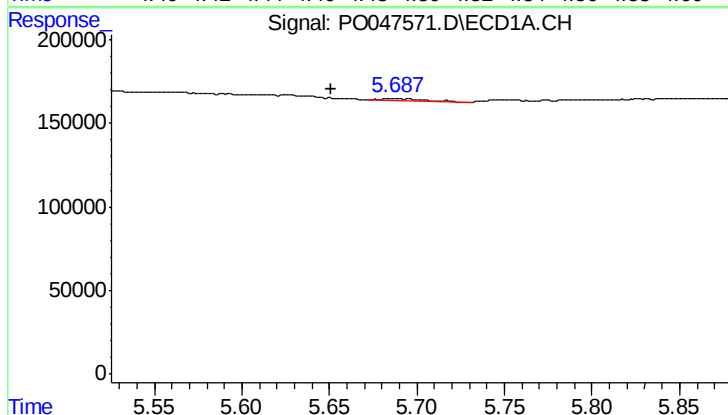


#4 AR-1016-2

R.T.: 5.688 min
Delta R.T.: 0.037 min
Response: 26764
Conc: 4.55 ng/ml

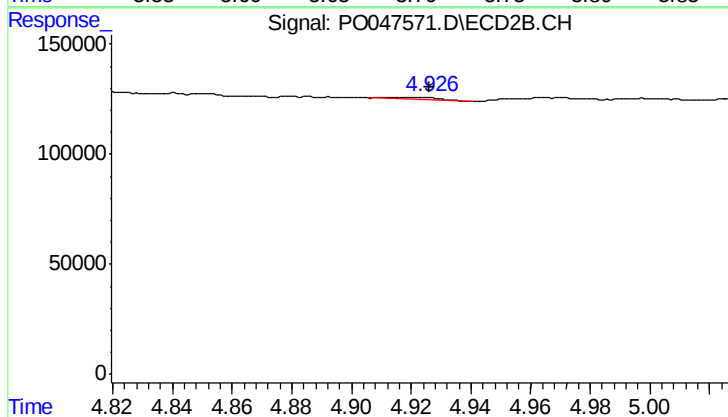

#4 AR-1016-2


R.T.: 4.918 min
Delta R.T.: -0.008 min
Response: 13026
Conc: 2.48 ng/ml

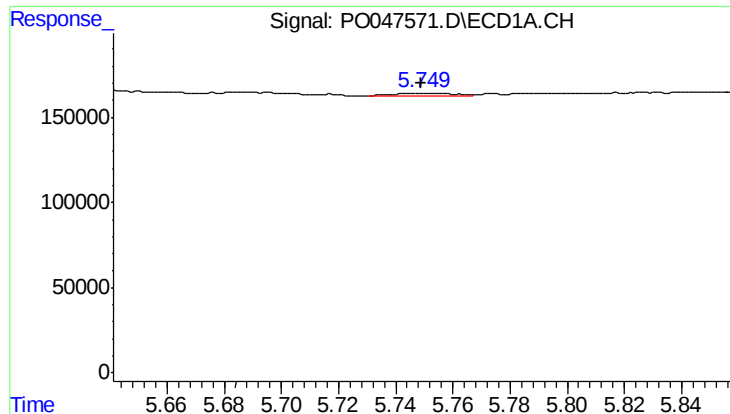

#5 AR-1016-3


R.T.: 5.750 min
Delta R.T.: 0.000 min
Response: 22576
Conc: 4.55 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-001-A

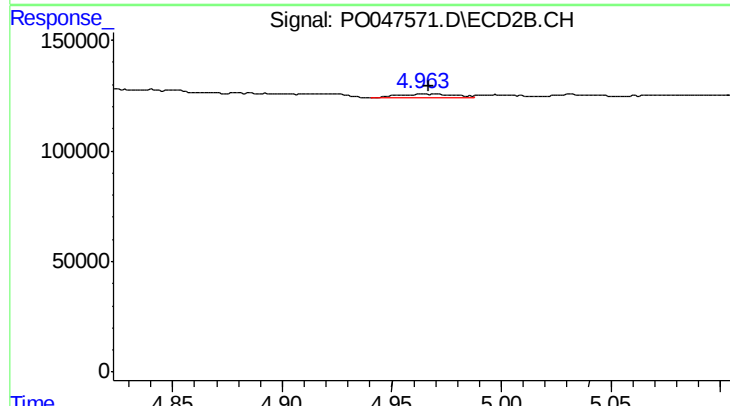


#5 AR-1016-3

R.T.: 4.966 min
Delta R.T.: -0.001 min
Response: 33732
Conc: 7.68 ng/ml

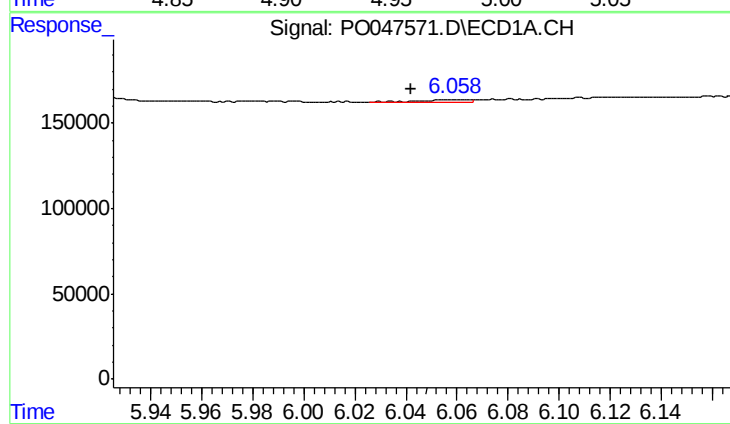


#6 AR-1016-4

R.T.: 6.059 min
Delta R.T.: 0.017 min
Response: 18969
Conc: 4.08 ng/ml

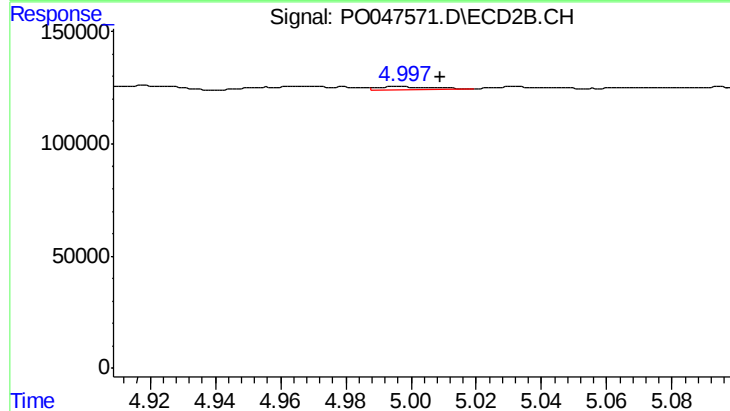

#6 AR-1016-4


R.T.: 4.996 min
Delta R.T.: -0.013 min
Response: 16895
Conc: 3.26 ng/ml

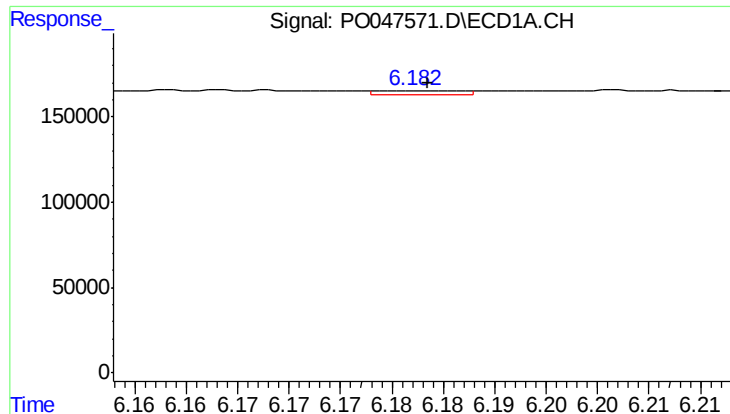

#7 AR-1016-5


R.T.: 6.182 min
Delta R.T.: -0.001 min
Response: 14261
Conc: 2.74 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-001-A

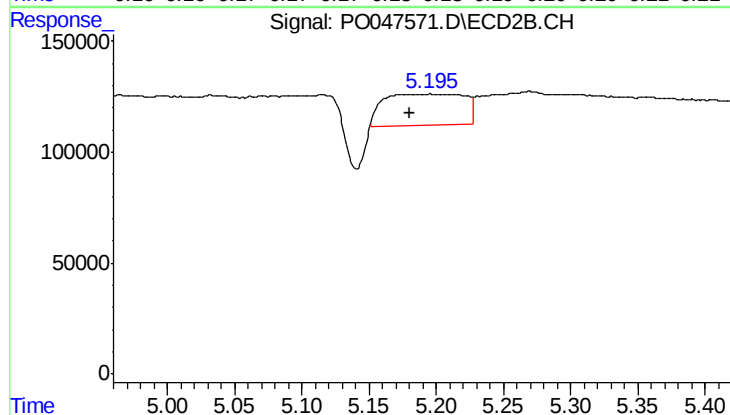


#7 AR-1016-5

R.T.: 5.195 min
Delta R.T.: 0.015 min
Response: 592448
Conc: 101.00 ng/ml

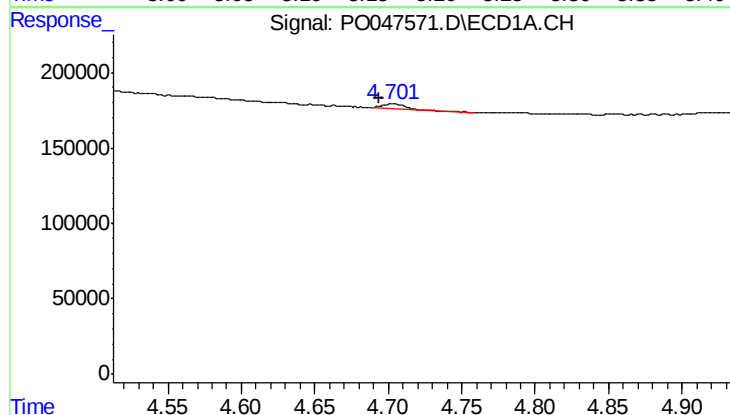


#9 AR-1221-2

R.T.: 4.703 min
Delta R.T.: 0.009 min
Response: 39155
Conc: 23.95 ng/ml

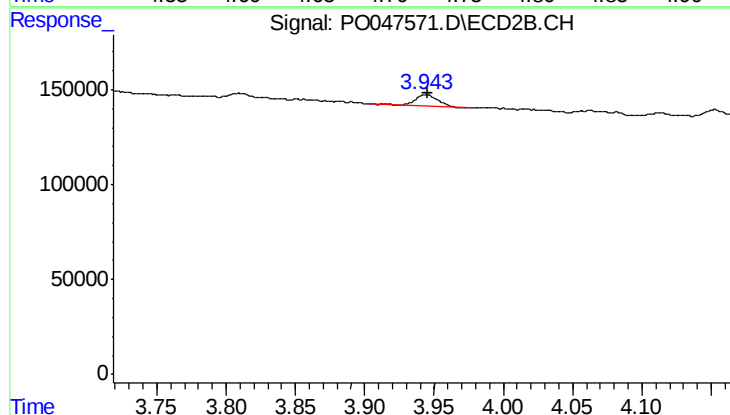

#9 AR-1221-2


R.T.: 3.944 min
Delta R.T.: -0.002 min
Response: 69564
Conc: 38.35 ng/ml

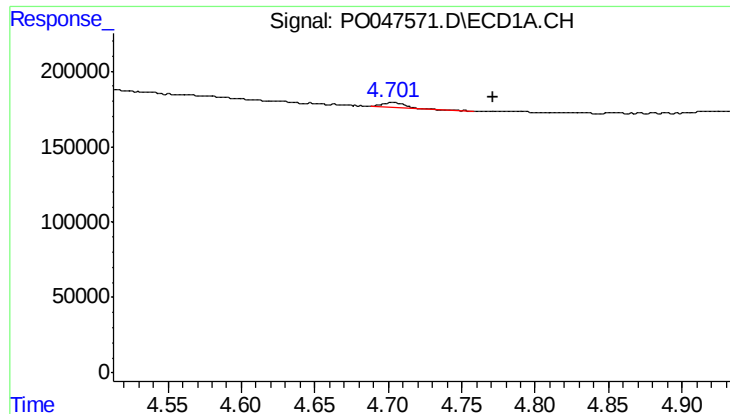

#10 AR-1221-3


R.T.: 4.703 min
Delta R.T.: -0.069 min
Response: 39155
Conc: 7.58 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-001-A

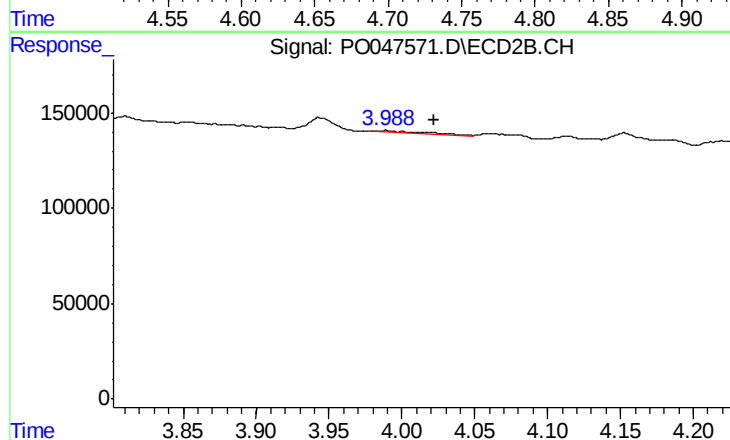


#10 AR-1221-3

R.T.: 3.989 min
Delta R.T.: -0.034 min
Response: 18692
Conc: 3.23 ng/ml

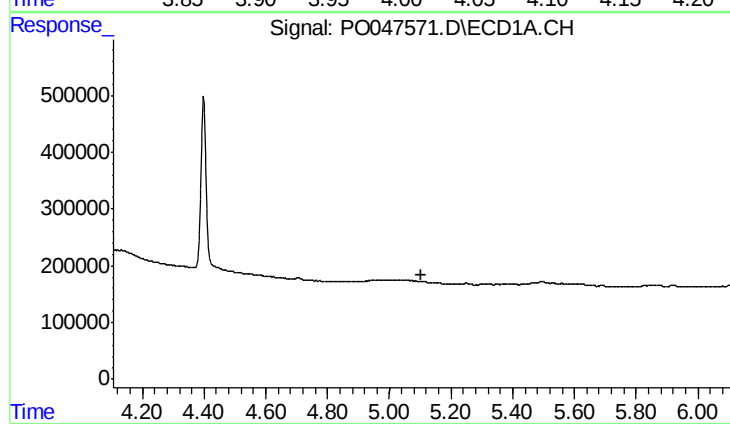


#11 AR-1232-1

R.T.: 0.000 min
Exp R.T.: 5.105 min
Response: 0
Conc: N.D.

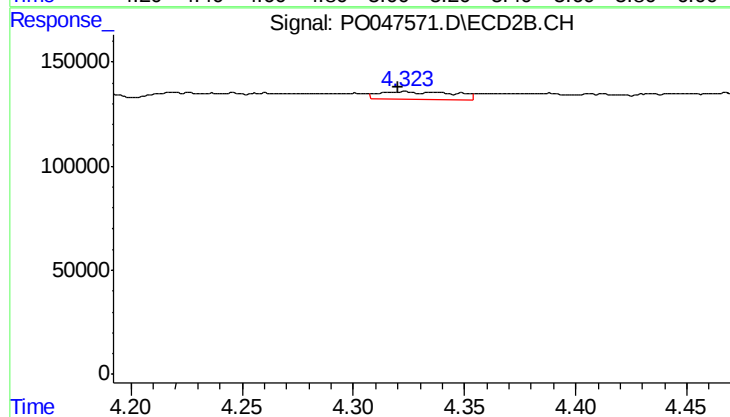

#11 AR-1232-1


R.T.: 4.323 min
Delta R.T.: 0.003 min
Response: 91372
Conc: 38.85 ng/ml

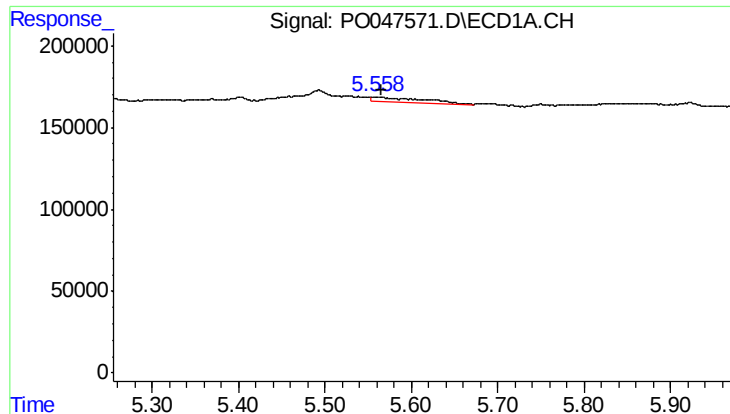

#12 AR-1232-2


R.T.: 5.558 min
Delta R.T.: -0.008 min
Response: 135829
Conc: 46.16 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-001-A

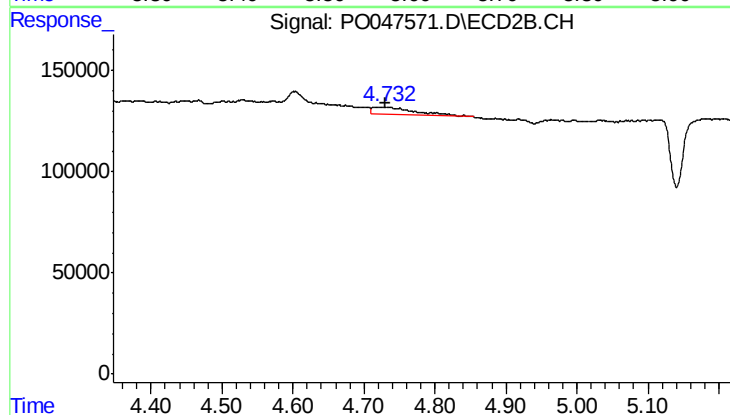


#12 AR-1232-2

R.T.: 4.732 min
Delta R.T.: 0.002 min
Response: 137786
Conc: 45.09 ng/ml

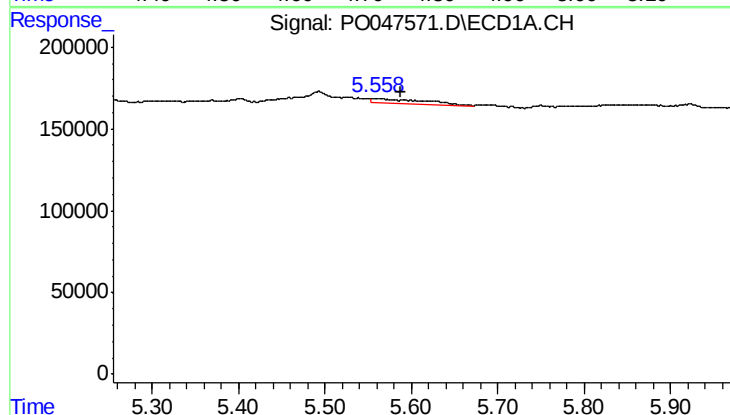


#13 AR-1232-3

R.T.: 5.558 min
Delta R.T.: -0.030 min
Response: 135829
Conc: 31.62 ng/ml

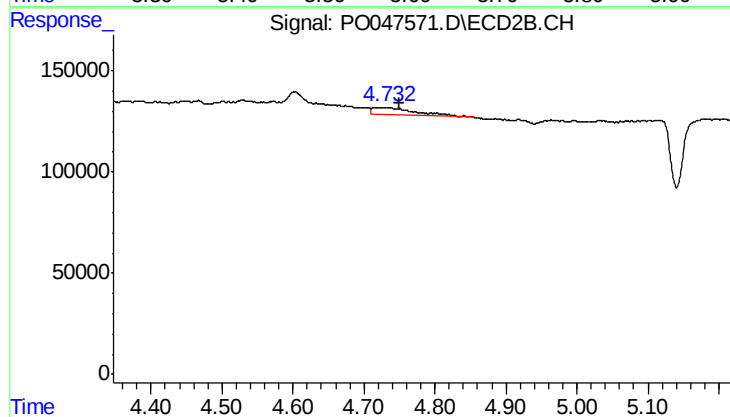

#13 AR-1232-3


R.T.: 4.732 min
Delta R.T.: -0.018 min
Response: 137786
Conc: 29.84 ng/ml

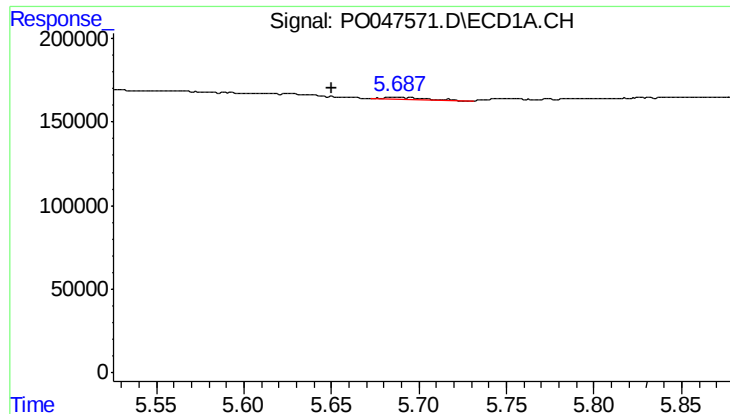

#14 AR-1232-4


R.T.: 5.688 min
Delta R.T.: 0.038 min
Response: 26764
Conc: 9.67 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-001-A

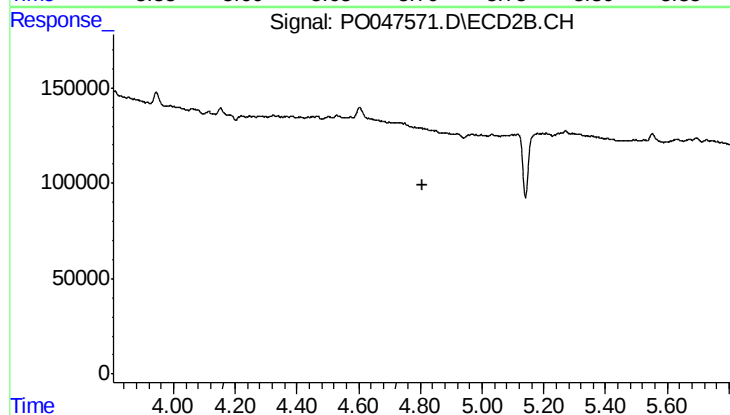


#14 AR-1232-4

R.T.: 0.000 min
Exp R.T.: 4.805 min
Response: 0
Conc: N.D.

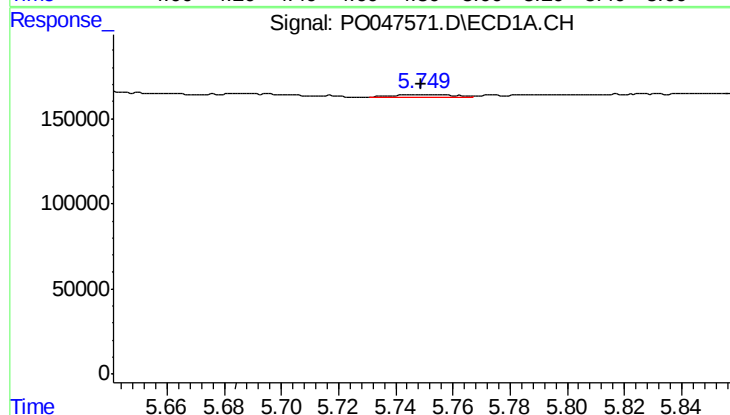


#15 AR-1232-5

R.T.: 5.750 min
Delta R.T.: 0.001 min
Response: 22576
Conc: 10.11 ng/ml

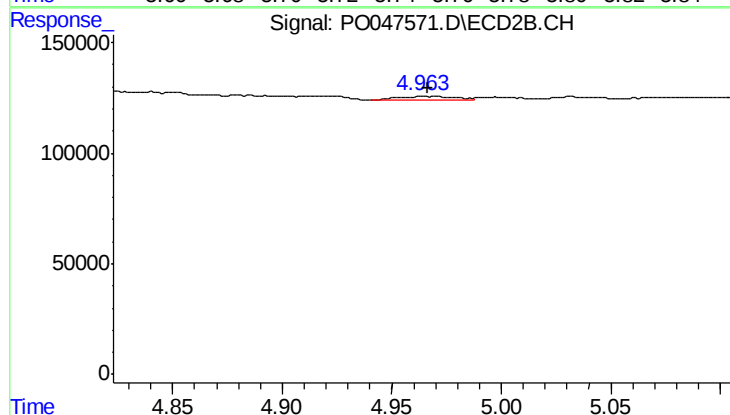

#15 AR-1232-5


R.T.: 4.966 min
Delta R.T.: 0.000 min
Response: 33732
Conc: 18.85 ng/ml

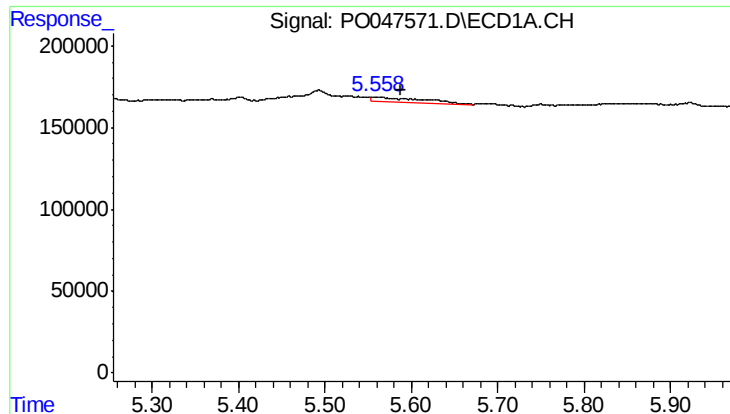

#16 AR-1242-1


R.T.: 5.558 min
Delta R.T.: -0.030 min
Response: 135829
Conc: 18.48 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-001-A

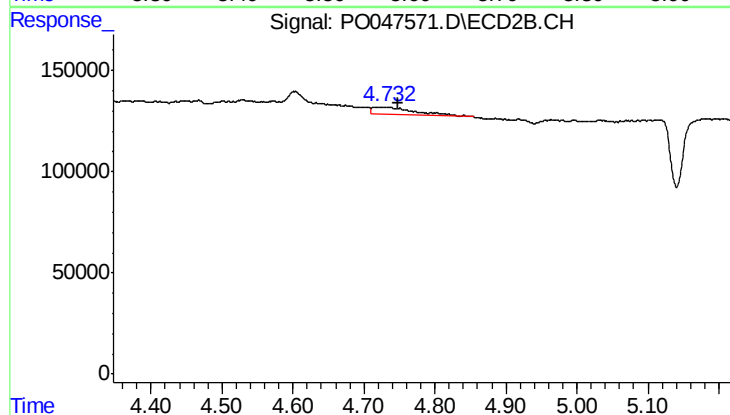


#16 AR-1242-1

R.T.: 4.732 min
Delta R.T.: -0.017 min
Response: 137786
Conc: 17.21 ng/ml

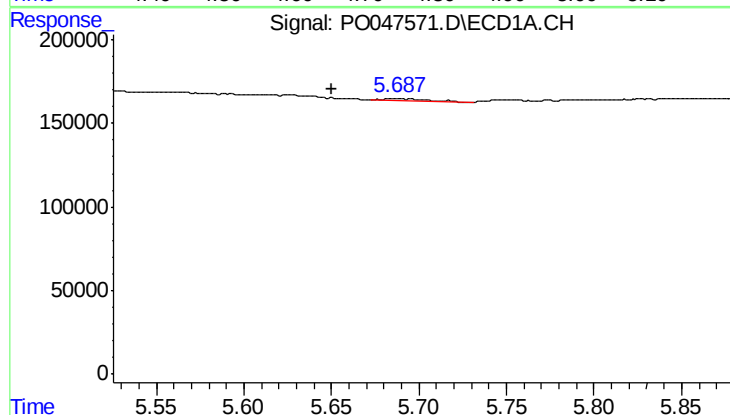


#17 AR-1242-2

R.T.: 5.688 min
Delta R.T.: 0.037 min
Response: 26764
Conc: 5.78 ng/ml

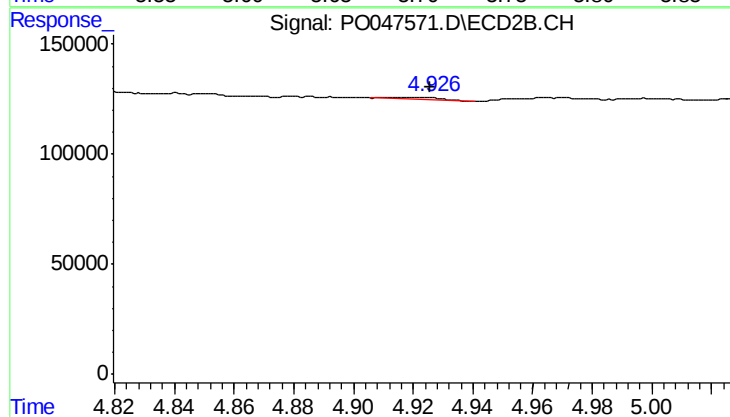

#17 AR-1242-2


R.T.: 4.918 min
Delta R.T.: -0.007 min
Response: 13026
Conc: 3.16 ng/ml

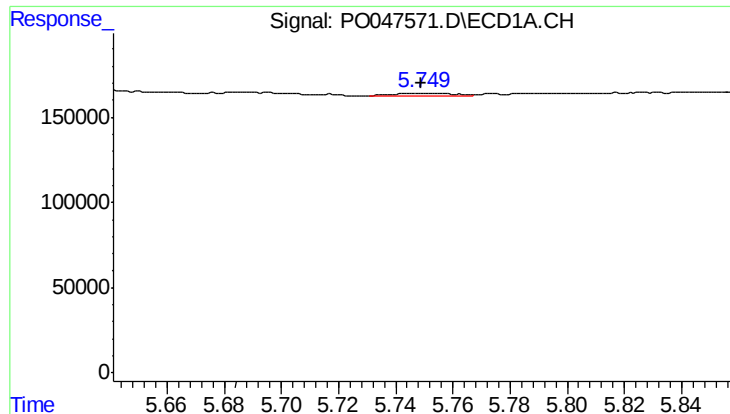

#18 AR-1242-3


R.T.: 5.750 min
Delta R.T.: 0.000 min
Response: 22576
Conc: 5.88 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-001-A

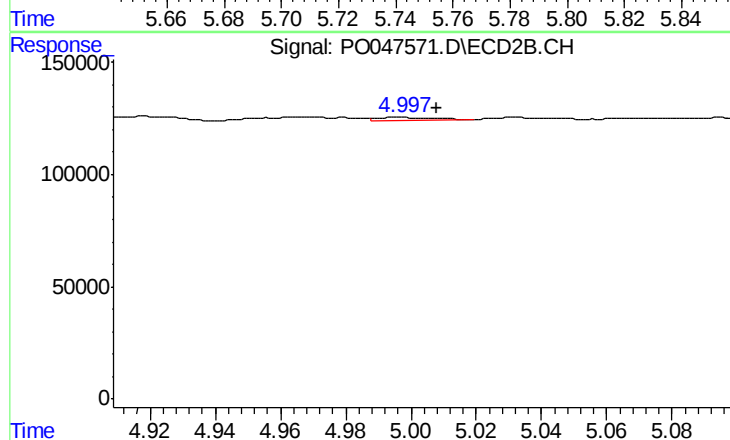


#18 AR-1242-3

R.T.: 4.996 min
Delta R.T.: -0.012 min
Response: 16895
Conc: 4.03 ng/ml

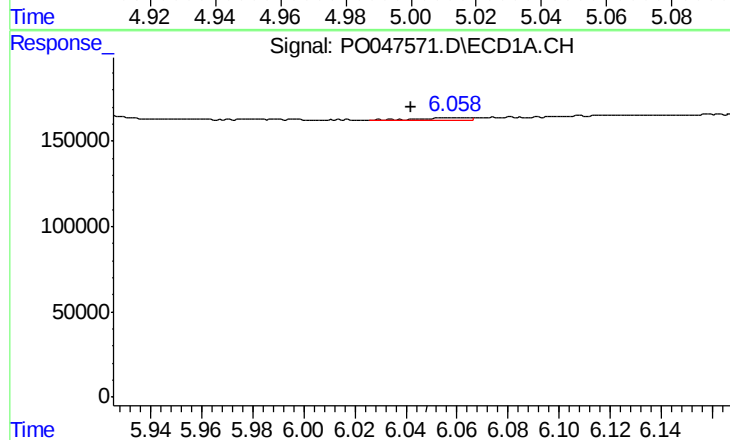


#19 AR-1242-4

R.T.: 6.059 min
Delta R.T.: 0.017 min
Response: 18969
Conc: 4.93 ng/ml

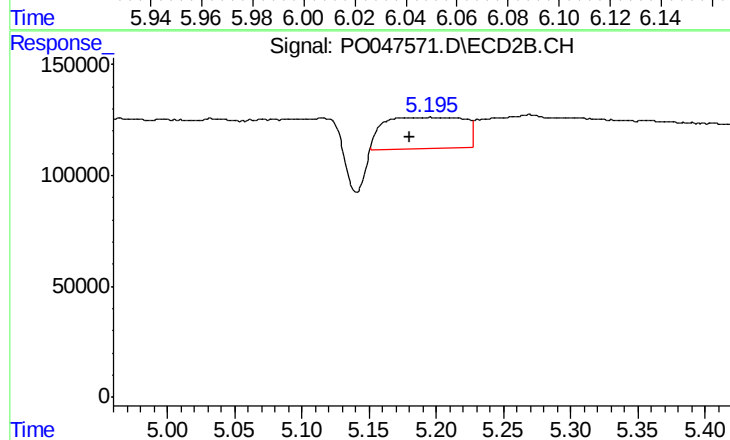

#19 AR-1242-4


R.T.: 5.195 min
Delta R.T.: 0.015 min
Response: 592448
Conc: 125.46 ng/ml

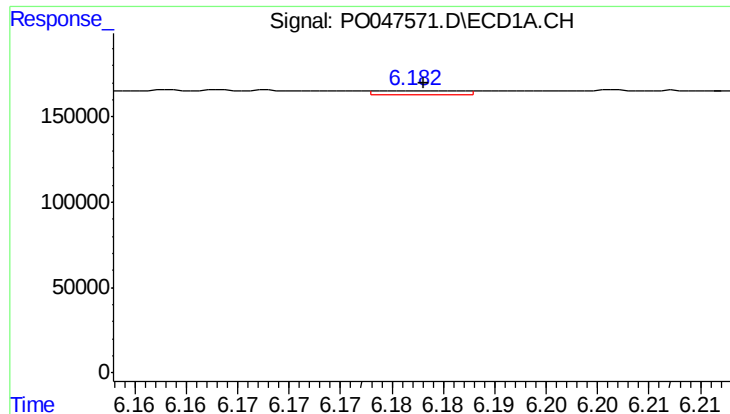

#20 AR-1242-5


R.T.: 6.182 min
Delta R.T.: -0.001 min
Response: 14261
Conc: 3.33 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-001-A

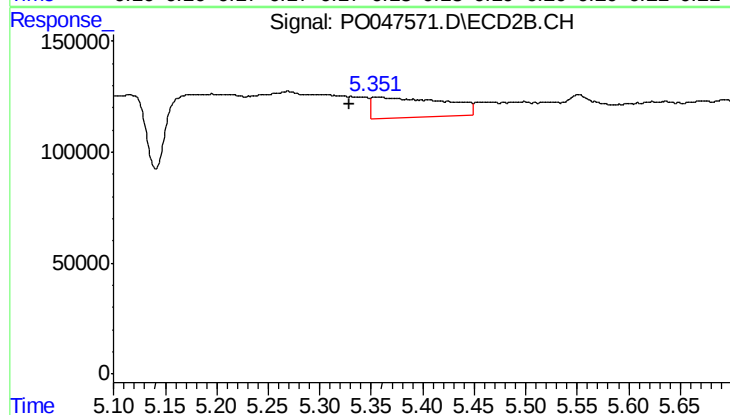


#20 AR-1242-5

R.T.: 5.356 min
Delta R.T.: 0.027 min
Response: 452835
Conc: 116.96 ng/ml

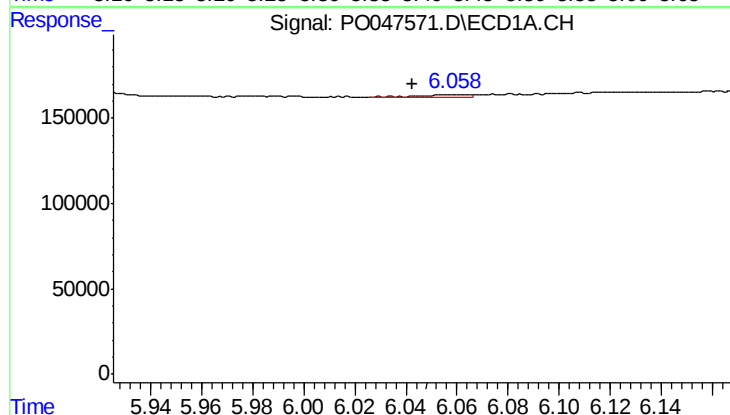


#21 AR-1248-1

R.T.: 6.059 min
Delta R.T.: 0.017 min
Response: 18969
Conc: 3.03 ng/ml

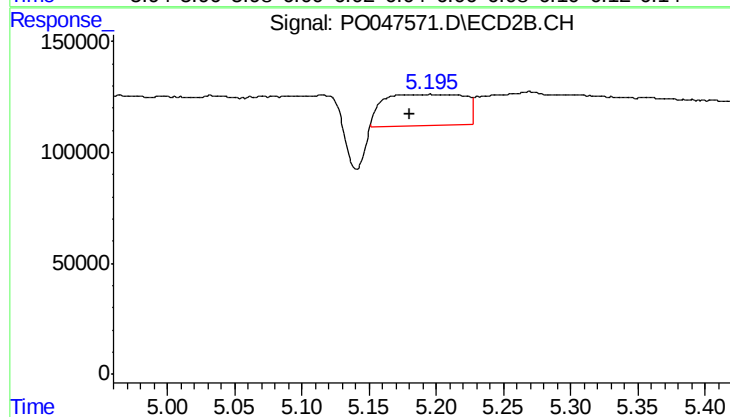

#21 AR-1248-1


R.T.: 5.195 min
Delta R.T.: 0.014 min
Response: 592448
Conc: 79.41 ng/ml

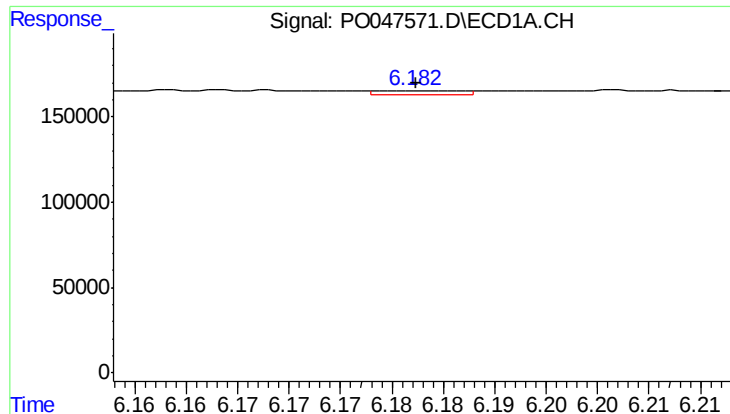

#22 AR-1248-2


R.T.: 6.182 min
Delta R.T.: 0.000 min
Response: 14261
Conc: 2.62 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-001-A

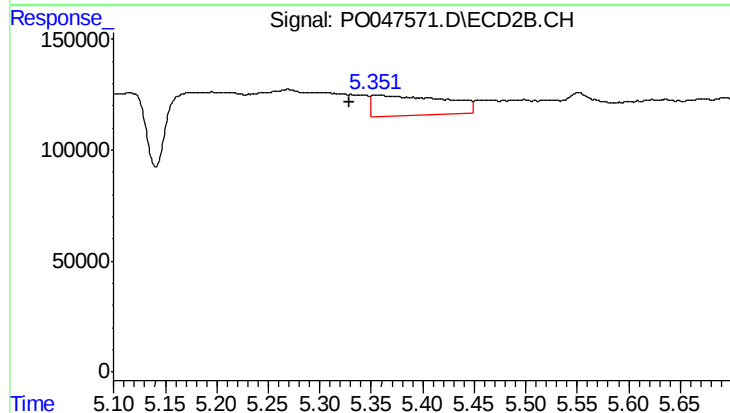


#22 AR-1248-2

R.T.: 5.356 min
Delta R.T.: 0.027 min
Response: 452835
Conc: 84.64 ng/ml

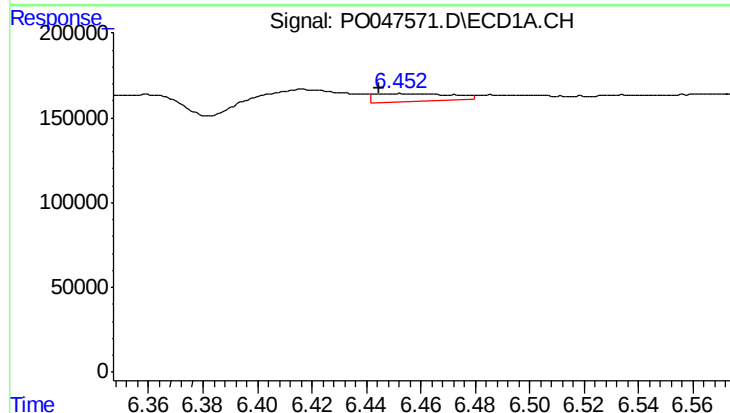


#23 AR-1248-3

R.T.: 6.453 min
Delta R.T.: 0.008 min
Response: 95709
Conc: 13.60 ng/ml

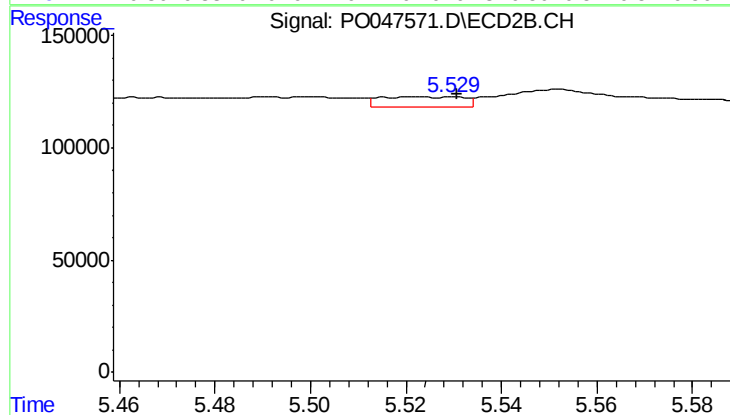

#23 AR-1248-3


R.T.: 5.523 min
Delta R.T.: -0.008 min
Response: 55964
Conc: 5.62 ng/ml

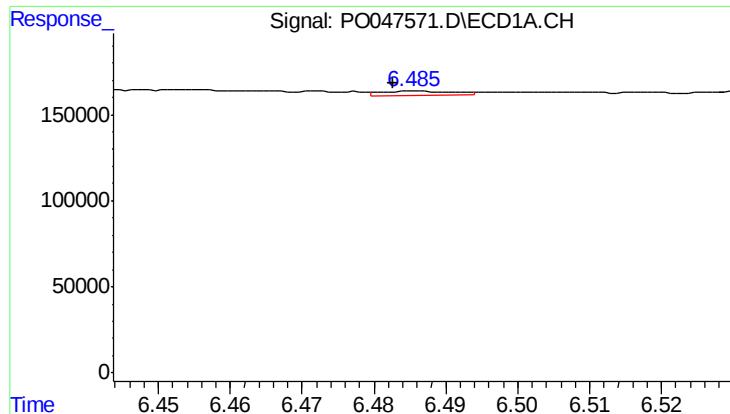

#24 AR-1248-4


R.T.: 6.486 min
Delta R.T.: 0.003 min
Response: 19218
Conc: 2.86 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-001-A

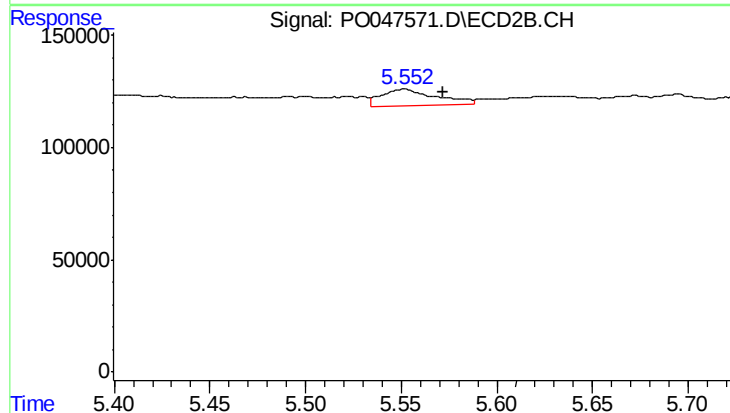


#24 AR-1248-4

R.T.: 5.551 min
Delta R.T.: -0.021 min
Response: 141749
Conc: 20.23 ng/ml

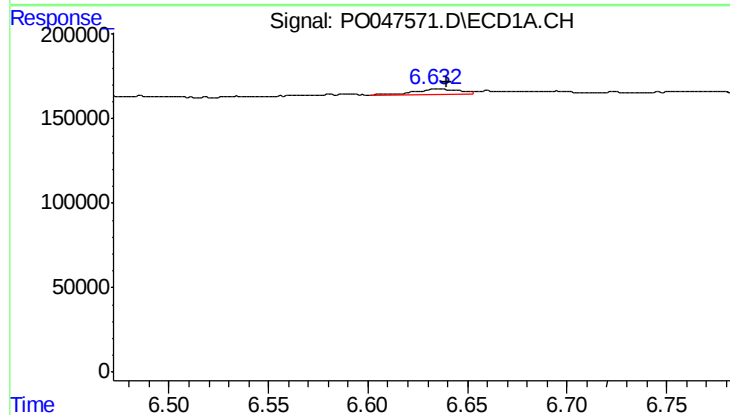


#25 AR-1248-5

R.T.: 6.634 min
Delta R.T.: -0.005 min
Response: 54760
Conc: 7.74 ng/ml

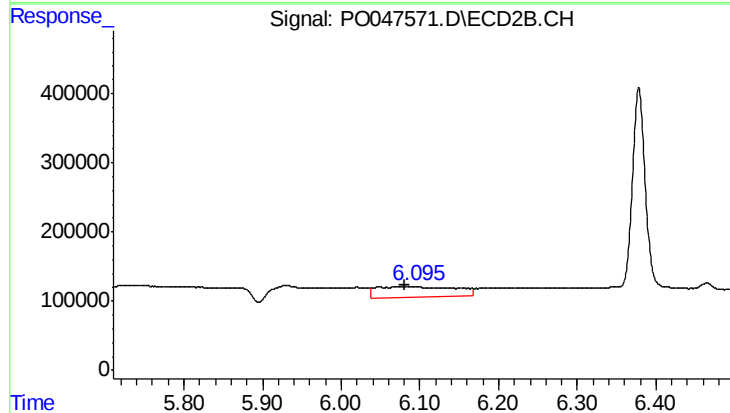

#25 AR-1248-5


R.T.: 6.094 min
Delta R.T.: 0.013 min
Response: 1073462
Conc: 225.24 ng/ml

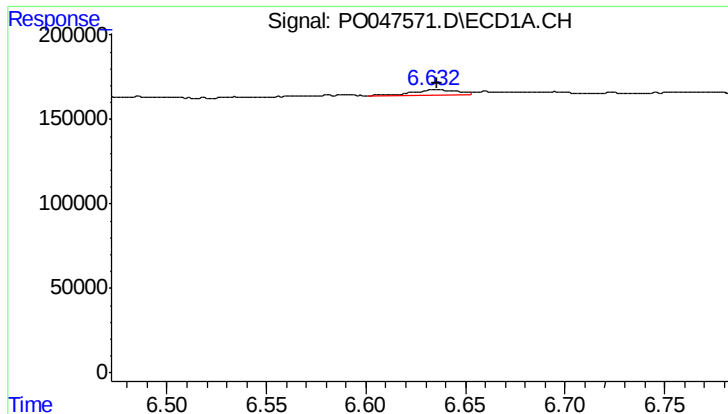

#26 AR-1254-1


R.T.: 6.634 min
Delta R.T.: -0.001 min
Response: 54760
Conc: 4.48 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-001-A

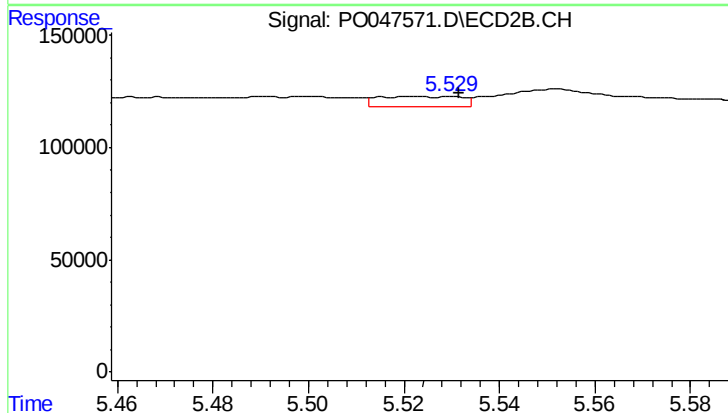


#26 AR-1254-1

R.T.: 5.523 min
Delta R.T.: -0.009 min
Response: 55964
Conc: 4.55 ng/ml

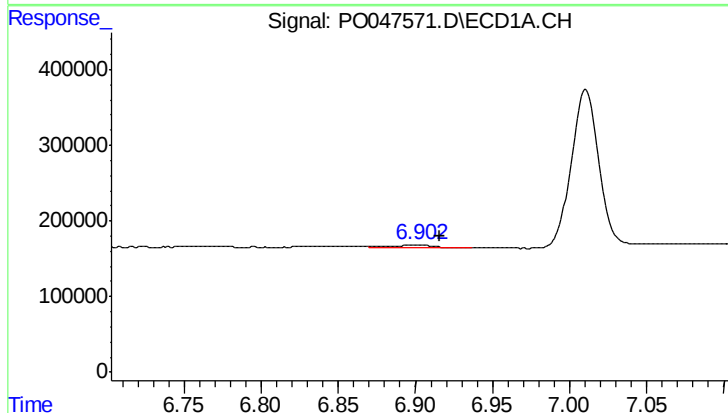


#27 AR-1254-2

R.T.: 6.902 min
Delta R.T.: -0.014 min
Response: 86181
Conc: 11.56 ng/ml

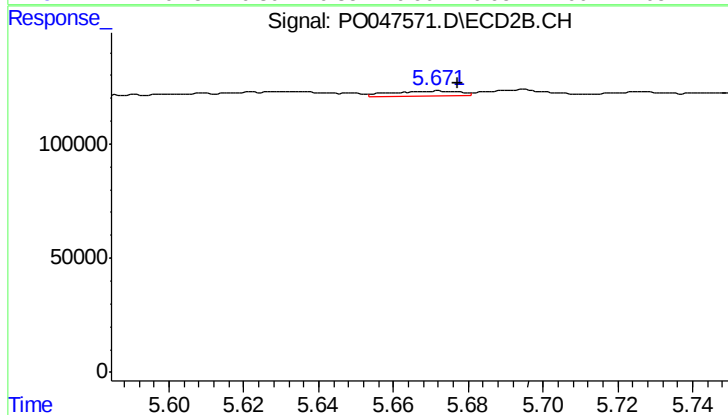

#27 AR-1254-2


R.T.: 5.672 min
Delta R.T.: -0.005 min
Response: 30008
Conc: 2.88 ng/ml

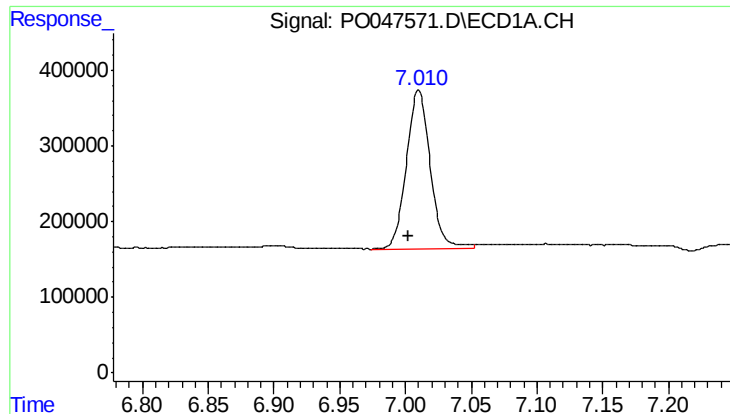

#28 AR-1254-3


R.T.: 7.010 min
Delta R.T.: 0.008 min
Response: 2632902
Conc: 201.89 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-001-A

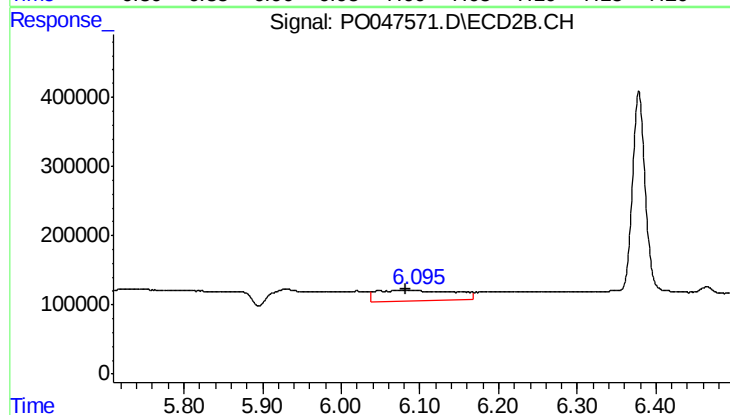


#28 AR-1254-3

R.T.: 6.094 min
Delta R.T.: 0.012 min
Response: 1073462
Conc: 61.85 ng/ml

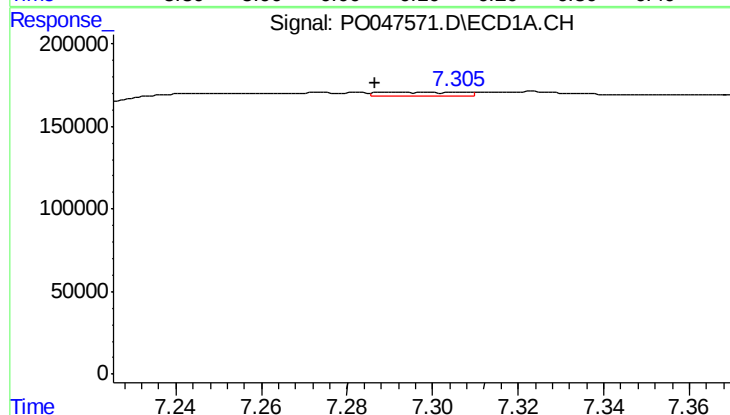


#29 AR-1254-4

R.T.: 7.290 min
Delta R.T.: 0.004 min
Response: 29173
Conc: 2.99 ng/ml

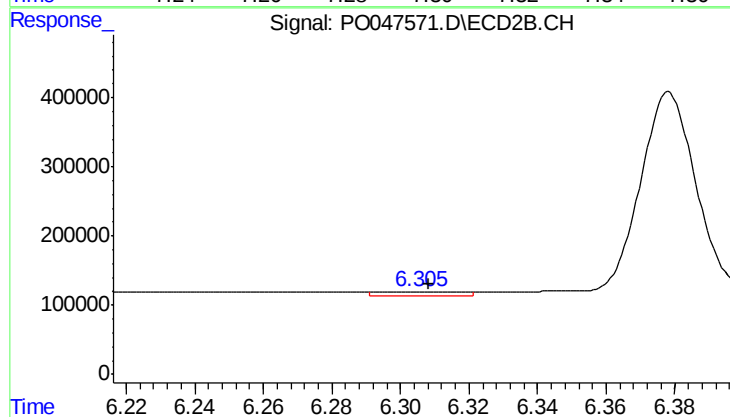

#29 AR-1254-4


R.T.: 6.306 min
Delta R.T.: -0.002 min
Response: 111444
Conc: 10.29 ng/ml

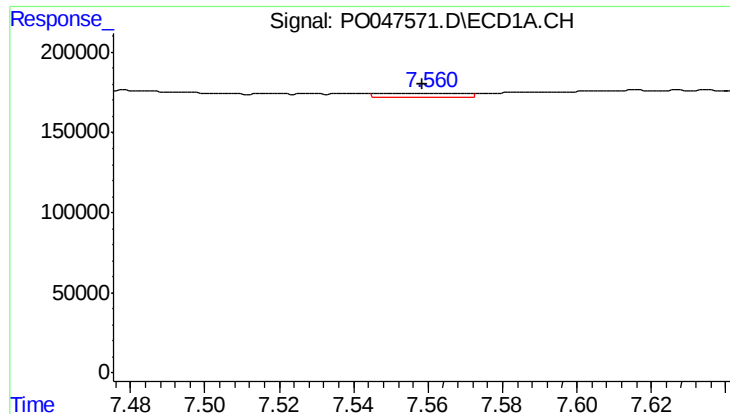

#30 AR-1254-5


R.T.: 7.560 min
Delta R.T.: 0.002 min
Response: 37245
Conc: 5.04 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-001-A

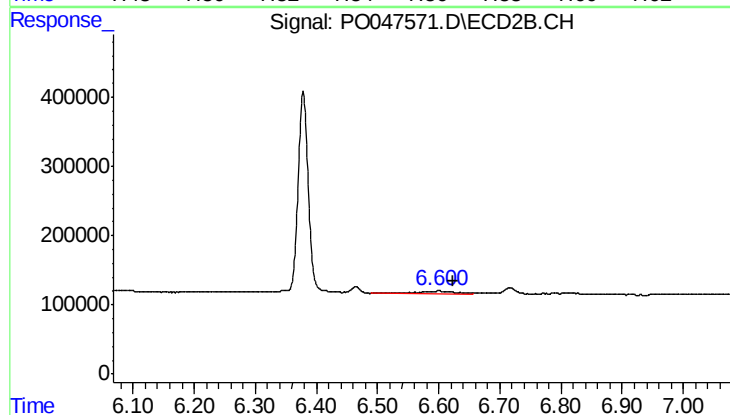


#30 AR-1254-5

R.T.: 6.600 min
Delta R.T.: -0.023 min
Response: 200296
Conc: 26.19 ng/ml

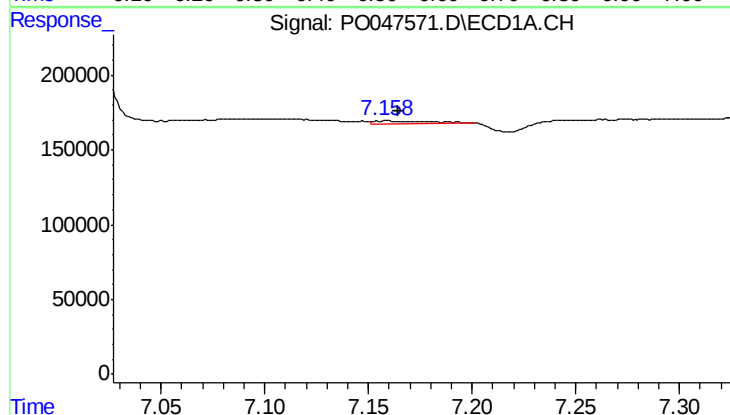


#31 AR-1260-1

R.T.: 7.159 min
Delta R.T.: -0.006 min
Response: 36810
Conc: 3.93 ng/ml

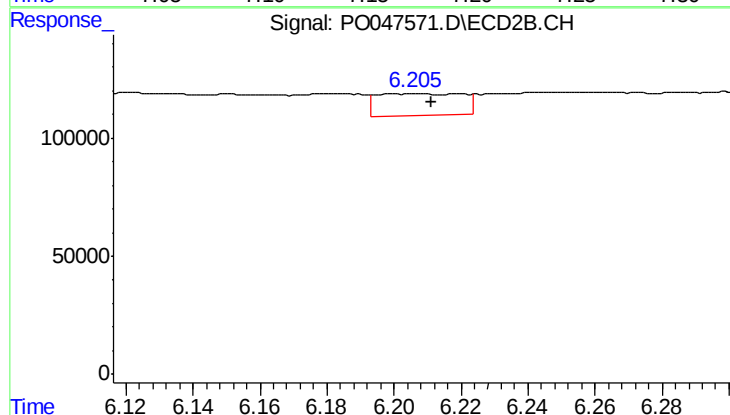

#31 AR-1260-1


R.T.: 6.205 min
Delta R.T.: -0.006 min
Response: 164050
Conc: 14.85 ng/ml

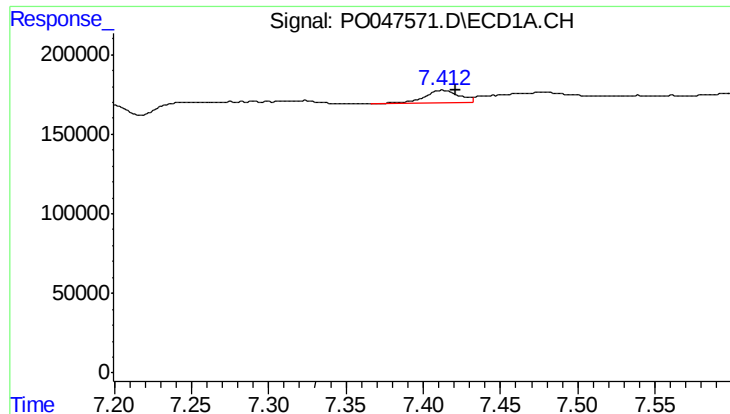

#32 AR-1260-2


R.T.: 7.412 min
Delta R.T.: -0.009 min
Response: 120788
Conc: 10.83 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-001-A

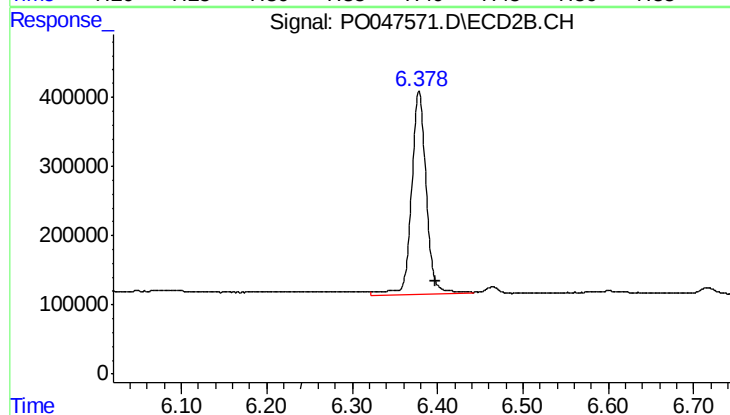


#32 AR-1260-2

R.T.: 6.378 min
Delta R.T.: -0.019 min
Response: 3503432
Conc: 261.29 ng/ml

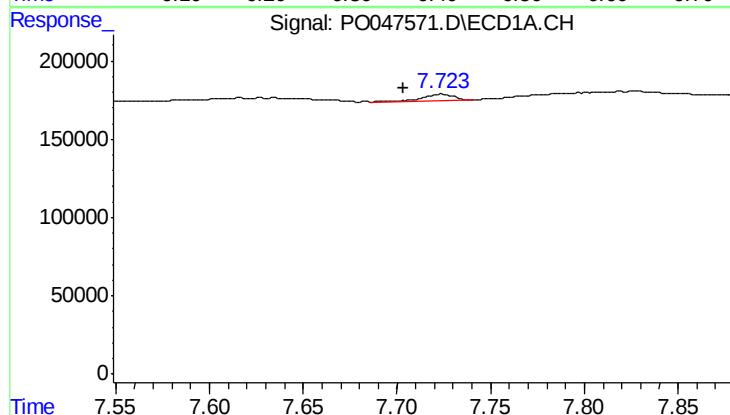


#33 AR-1260-3

R.T.: 7.723 min
Delta R.T.: 0.020 min
Response: 46871
Conc: 3.64 ng/ml

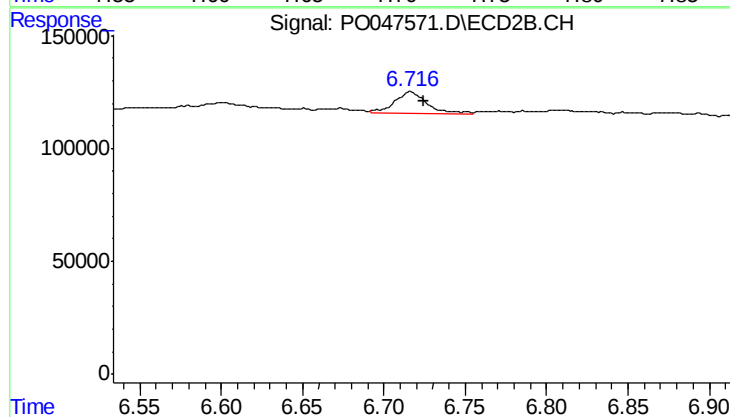

#33 AR-1260-3


R.T.: 6.716 min
Delta R.T.: -0.008 min
Response: 138553
Conc: 9.53 ng/ml

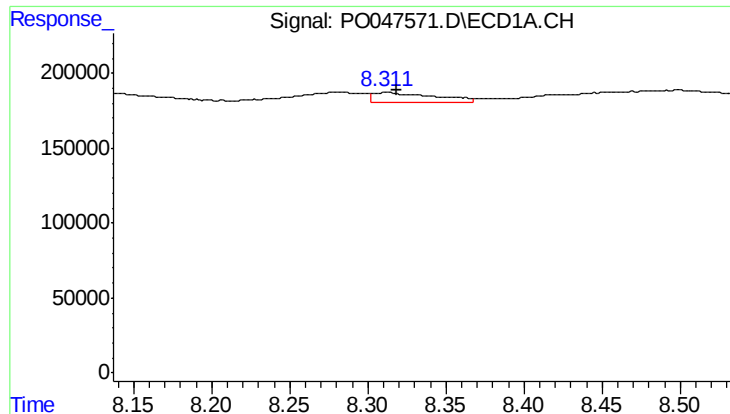

#34 AR-1260-4


R.T.: 8.311 min
Delta R.T.: -0.007 min
Response: 186482
Conc: 10.48 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-001-A

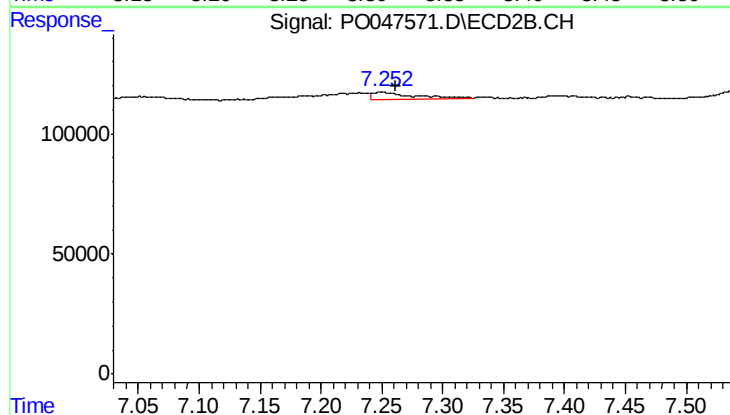


#34 AR-1260-4

R.T.: 7.251 min
Delta R.T.: -0.011 min
Response: 70613
Conc: 3.21 ng/ml

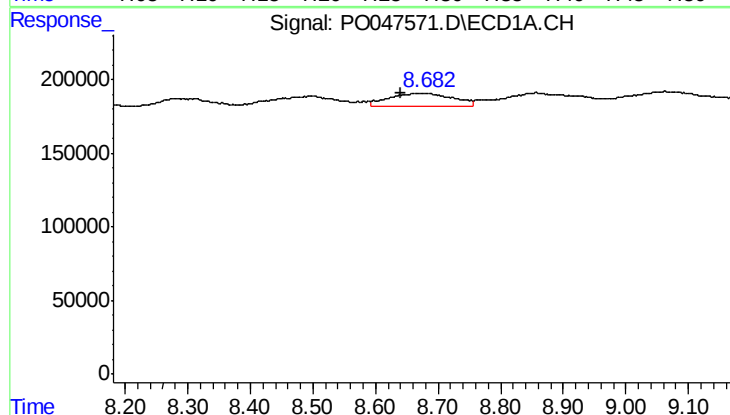


#35 AR-1260-5

R.T.: 8.682 min
Delta R.T.: 0.042 min
Response: 618099
Conc: 54.13 ng/ml

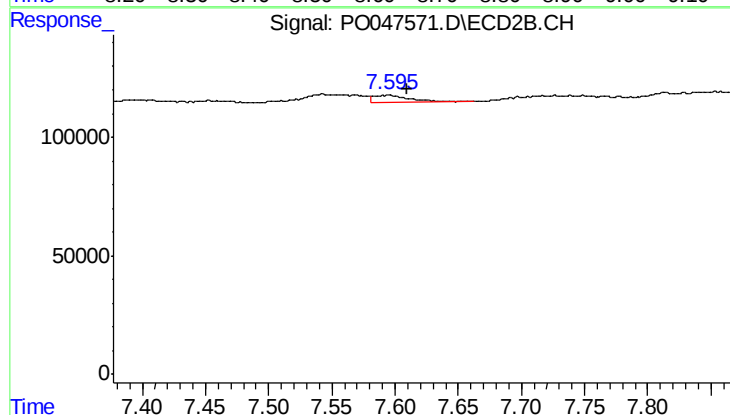

#35 AR-1260-5


R.T.: 7.595 min
Delta R.T.: -0.015 min
Response: 61309
Conc: 3.93 ng/ml

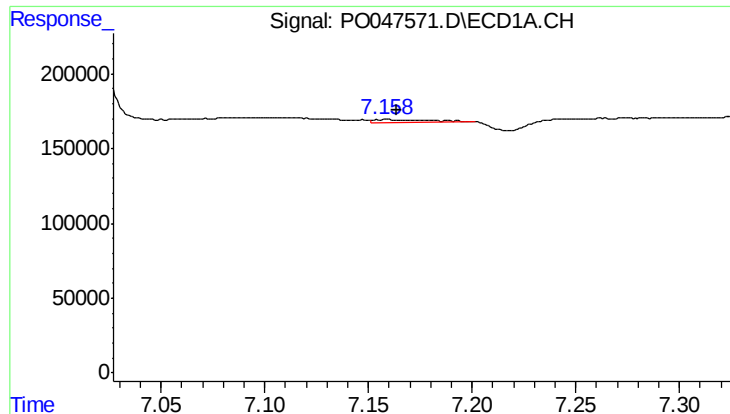

#36 AR-1262-1


R.T.: 7.159 min
Delta R.T.: -0.005 min
Response: 36810
Conc: 4.44 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-001-A

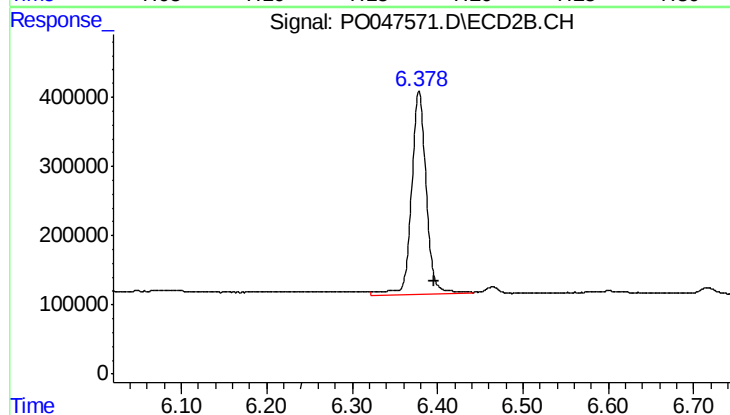


#36 AR-1262-1

R.T.: 6.378 min
Delta R.T.: -0.018 min
Response: 3503432
Conc: 309.00 ng/ml

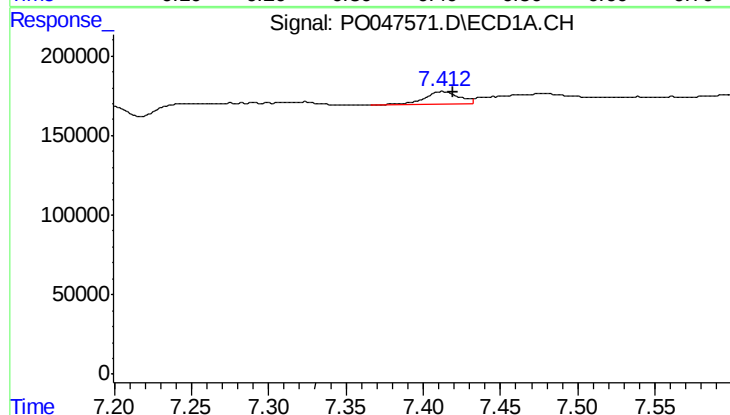


#37 AR-1262-2

R.T.: 7.412 min
Delta R.T.: -0.008 min
Response: 120788
Conc: 12.46 ng/ml

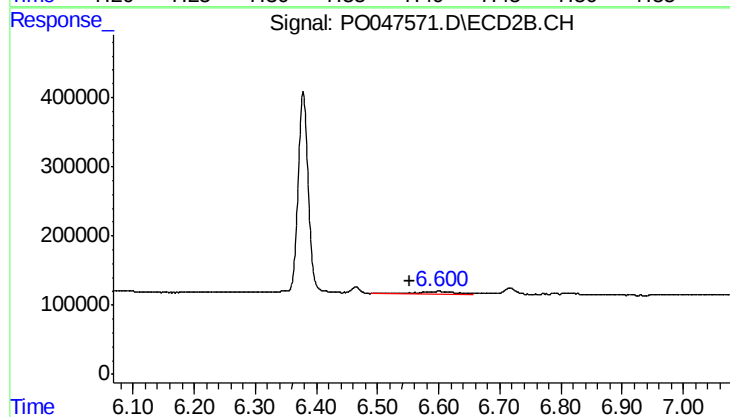

#37 AR-1262-2


R.T.: 6.600 min
Delta R.T.: 0.047 min
Response: 200296
Conc: 17.75 ng/ml

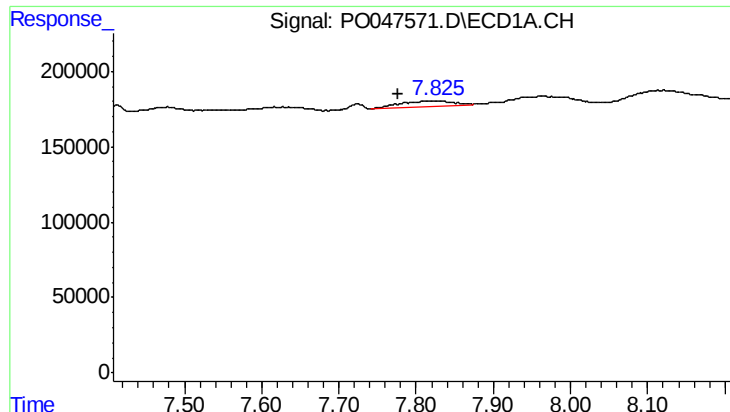

#38 AR-1262-3


R.T.: 7.828 min
Delta R.T.: 0.051 min
Response: 167703
Conc: 13.67 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-001-A

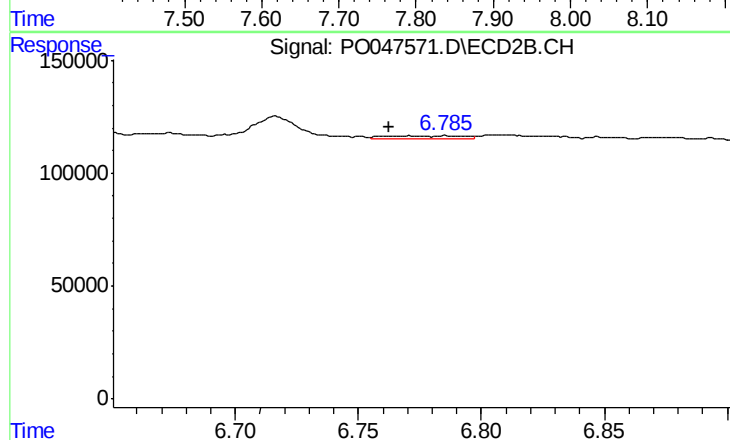


#38 AR-1262-3

R.T.: 6.772 min
Delta R.T.: 0.009 min
Response: 31279
Conc: 2.07 ng/ml

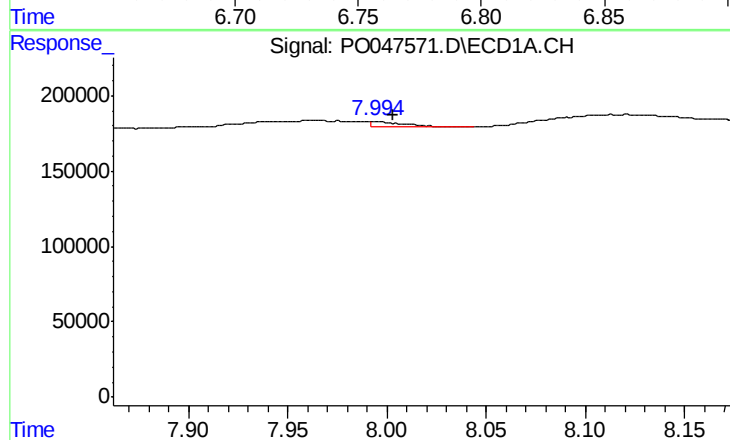


#39 AR-1262-4

R.T.: 7.994 min
Delta R.T.: -0.009 min
Response: 47785
Conc: 4.06 ng/ml

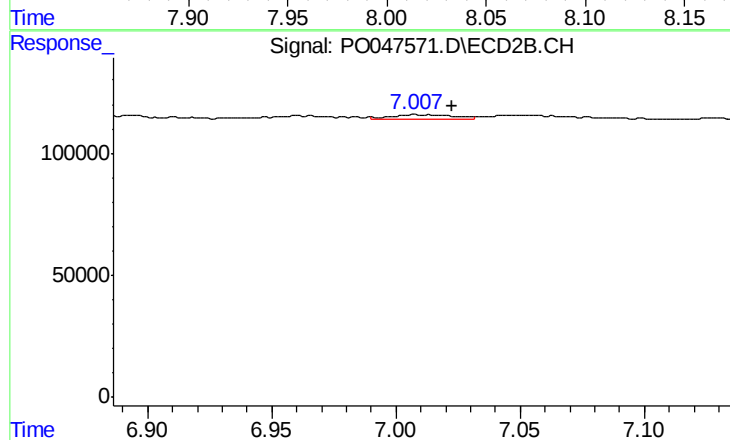

#39 AR-1262-4


R.T.: 7.009 min
Delta R.T.: -0.013 min
Response: 27497
Conc: 2.09 ng/ml

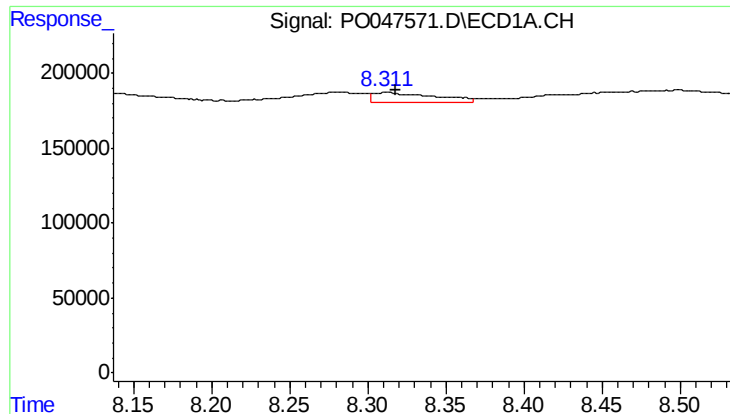

#40 AR-1262-5


R.T.: 8.311 min
Delta R.T.: -0.007 min
Response: 186482
Conc: 8.68 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-001-A

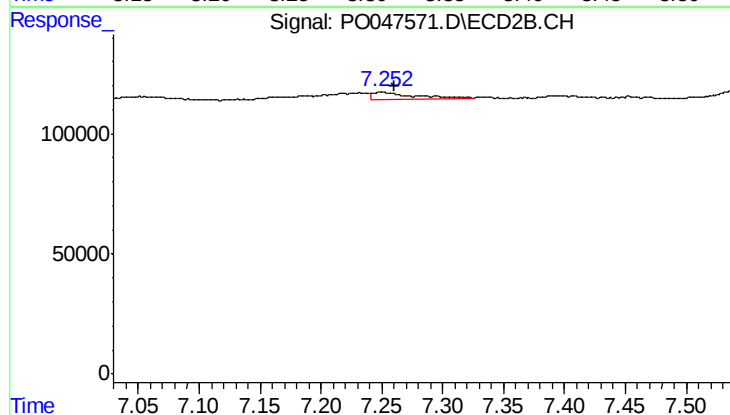


#40 AR-1262-5

R.T.: 7.251 min
Delta R.T.: -0.010 min
Response: 70613
Conc: 2.73 ng/ml

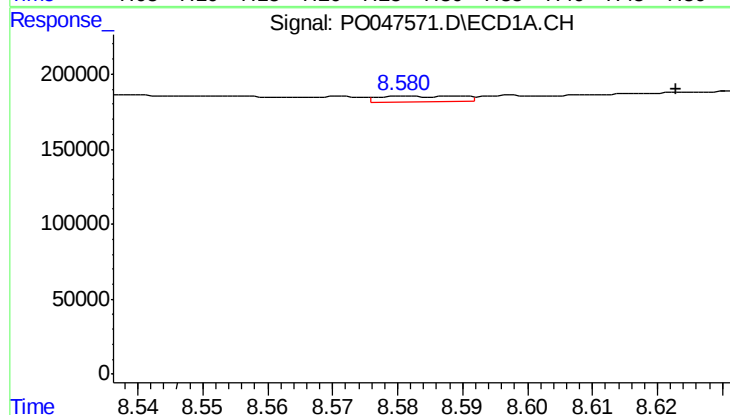


#41 AR-1268-1

R.T.: 8.581 min
Delta R.T.: -0.042 min
Response: 33739
Conc: 1.45 ng/ml

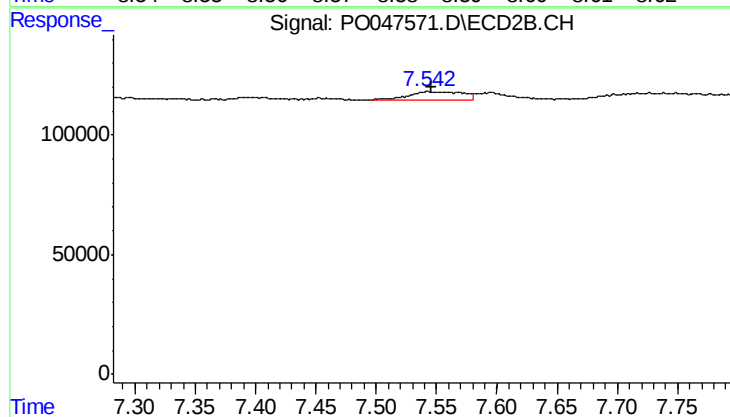

#41 AR-1268-1


R.T.: 7.543 min
Delta R.T.: -0.002 min
Response: 106031
Conc: 4.08 ng/ml

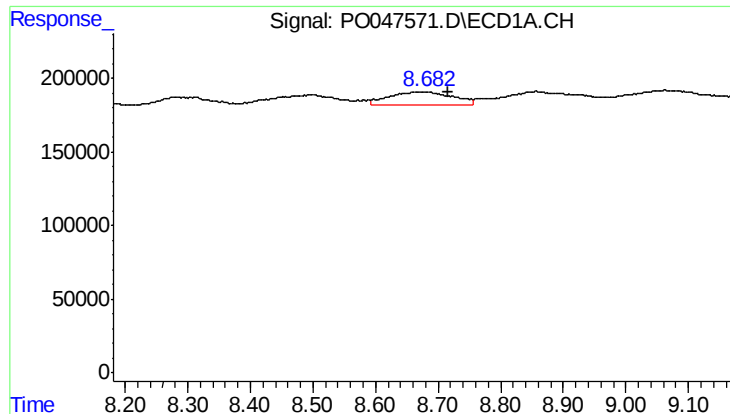

#42 AR-1268-2


R.T.: 8.682 min
Delta R.T.: -0.034 min
Response: 618099
Conc: 28.85 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-001-A

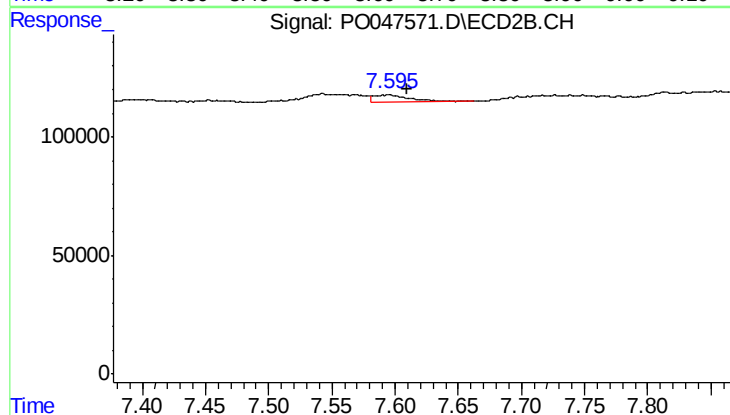


#42 AR-1268-2

R.T.: 7.595 min
Delta R.T.: -0.015 min
Response: 61309
Conc: 2.46 ng/ml

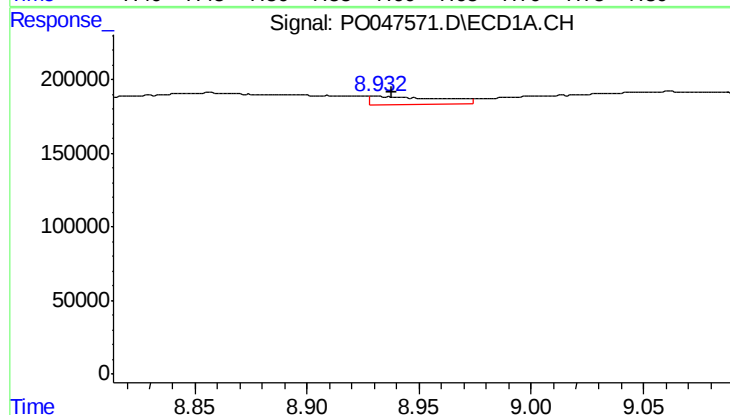


#43 AR-1268-3

R.T.: 8.931 min
Delta R.T.: -0.007 min
Response: 122498
Conc: 6.79 ng/ml

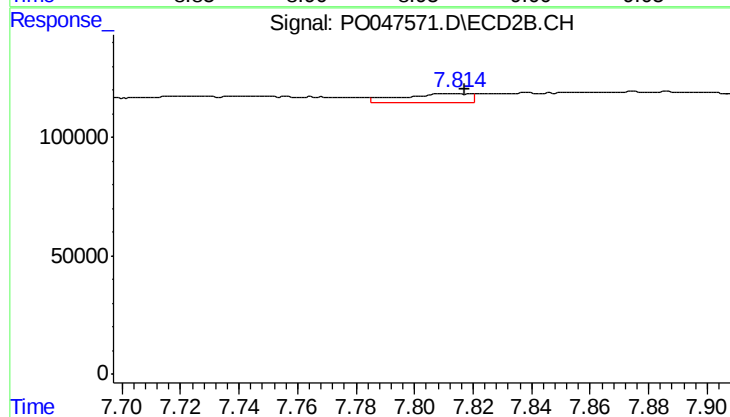

#43 AR-1268-3


R.T.: 7.813 min
Delta R.T.: -0.004 min
Response: 57149
Conc: 2.90 ng/ml

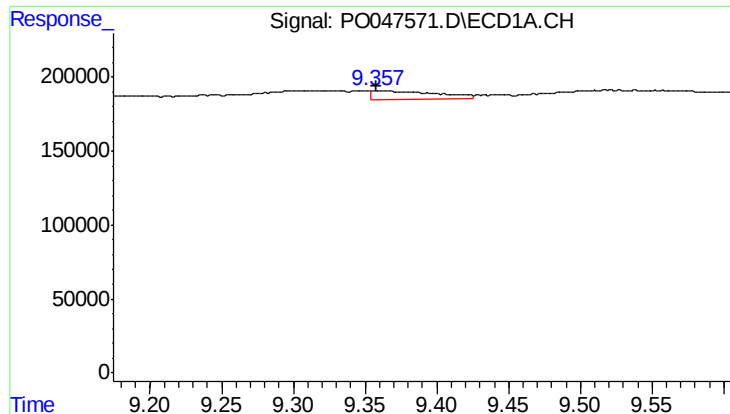

#44 AR-1268-4


R.T.: 9.358 min
Delta R.T.: 0.000 min
Response: 177571
Conc: 22.27 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-001-A

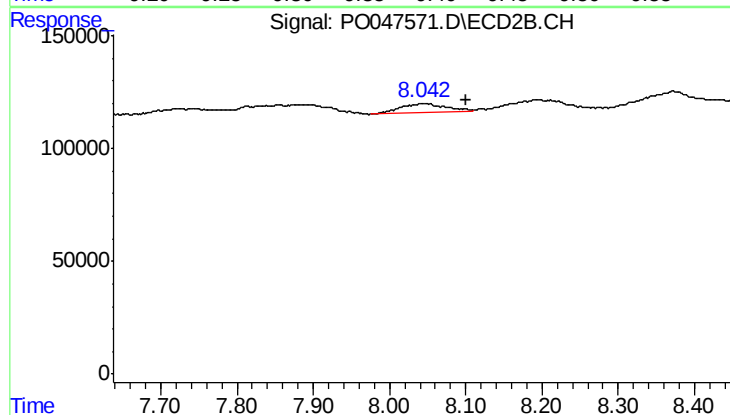


#44 AR-1268-4

R.T.: 8.046 min
Delta R.T.: -0.055 min
Response: 166569
Conc: 19.86 ng/ml

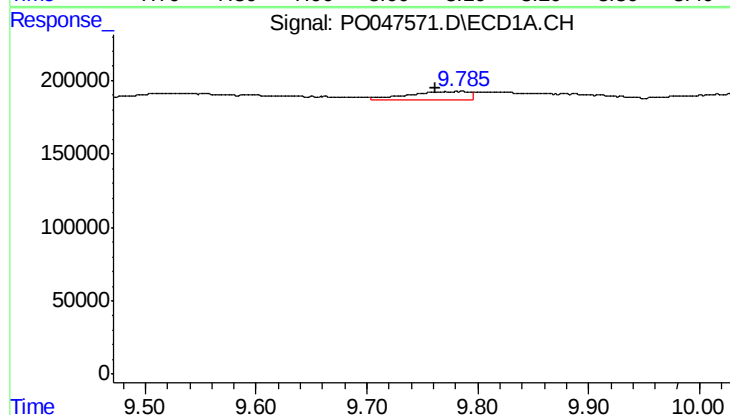

#45 AR-1268-5

R.T.: 9.785 min
Delta R.T.: 0.023 min
Response: 224736
Conc: 4.12 ng/ml

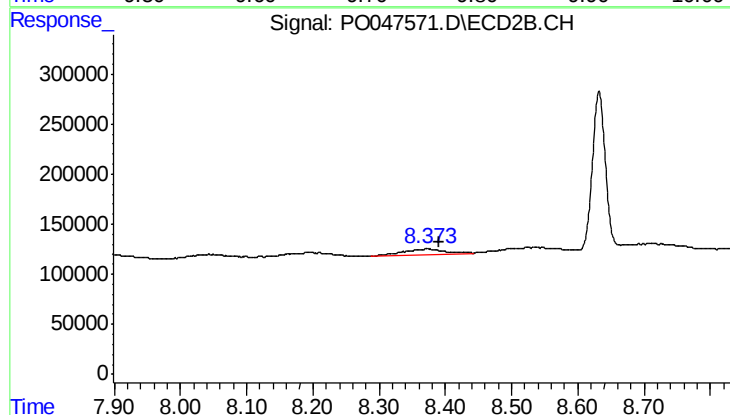

#45 AR-1268-5

R.T.: 8.373 min
Delta R.T.: -0.017 min
Response: 244229
Conc: 4.47 ng/ml