

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0080218\
Data File : P0047567.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Aug 2018 16:39
Operator : SM/SJ
Sample : J4076-03RE
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
SD-LT15-01-A-18RE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 03 02:28:16 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072718.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 27 02:33:29 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.398	3.644	2009731	2411946	9.954	9.816
2) SA Decachlor...	10.086	8.632	756157	807699	4.636	5.138

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080218\
Data File : P0047567.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Aug 2018 16:39
Operator : SM/SJ
Sample : J4076-03RE
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
SD-LT15-01-A-18RE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 03 02:28:16 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072718.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 27 02:33:29 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

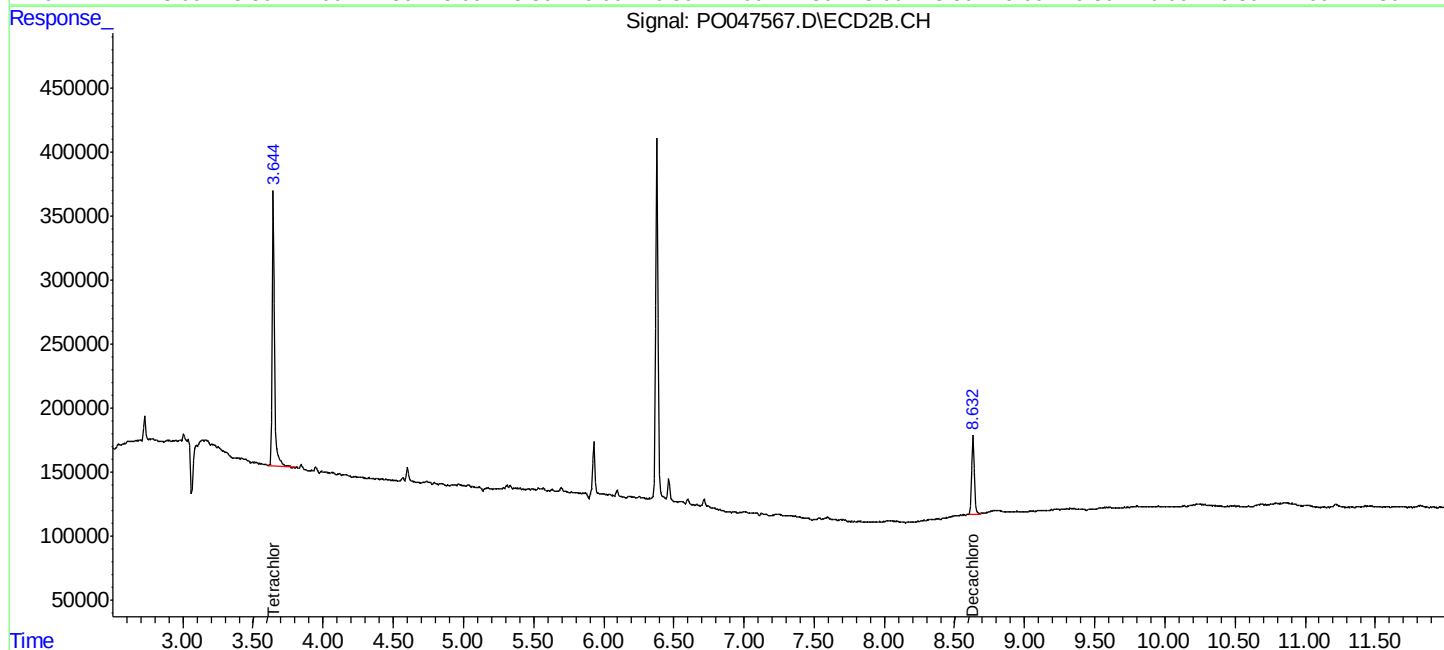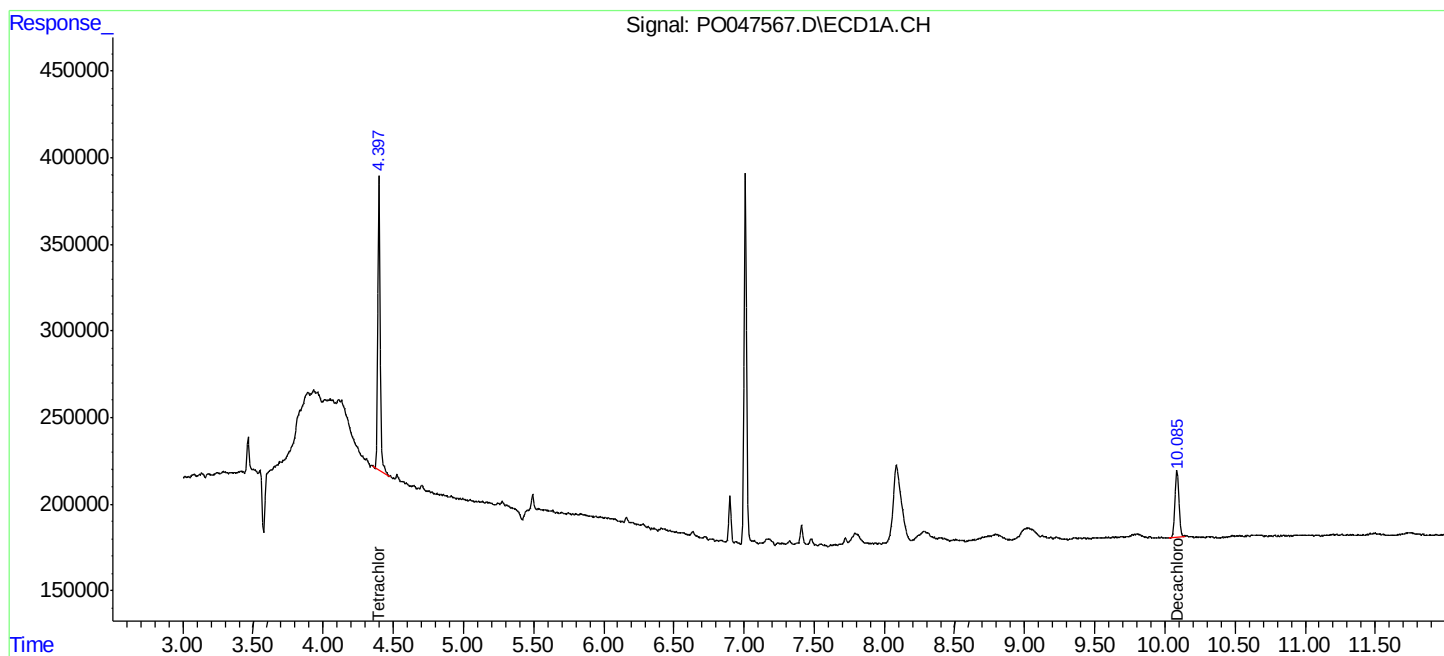


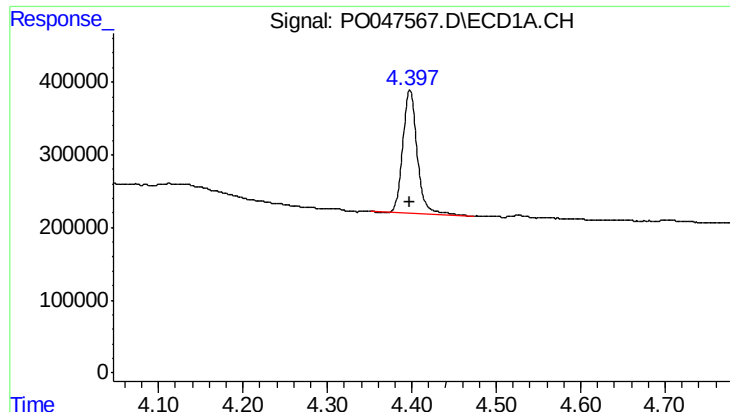

#1 Tetrachloro-m-xylene


R.T.: 4.398 min
Delta R.T.: 0.000 min
Response: 2009731
Conc: 9.95 ng/ml

Instrument :
ECD_O
ClientSampleId :
SD-LT15-01-A-18RE

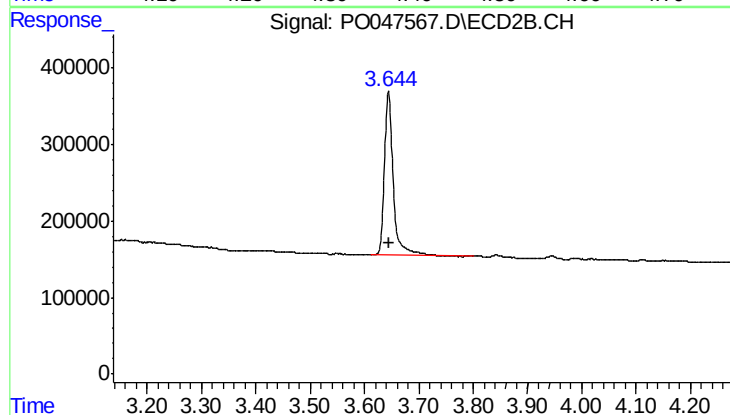


#1 Tetrachloro-m-xylene

R.T.: 3.644 min
Delta R.T.: -0.001 min
Response: 2411946
Conc: 9.82 ng/ml

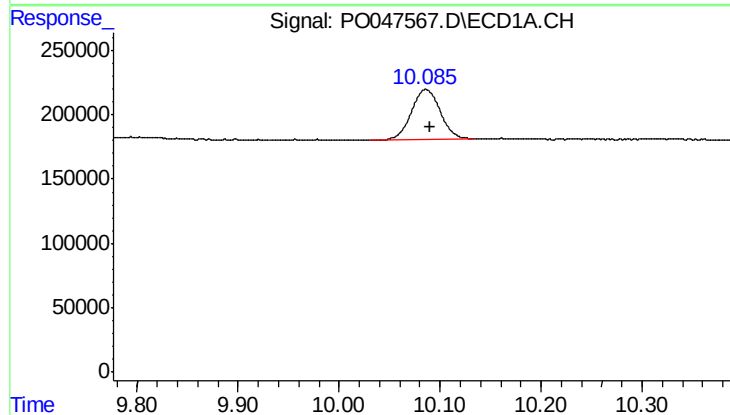

#2 Decachlorobiphenyl

R.T.: 10.086 min
Delta R.T.: -0.004 min
Response: 756157
Conc: 4.64 ng/ml

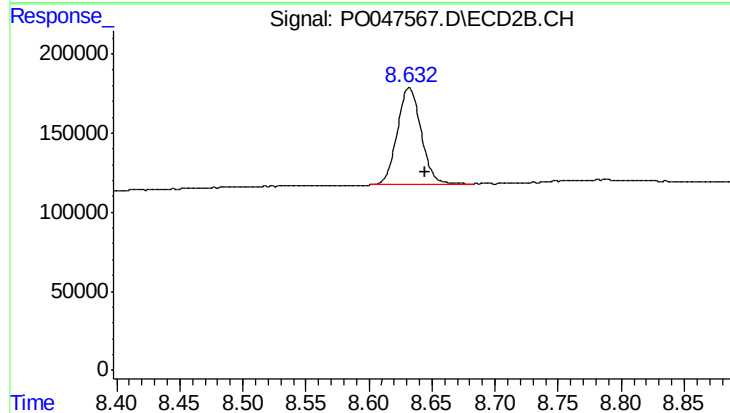

#2 Decachlorobiphenyl

R.T.: 8.632 min
Delta R.T.: -0.012 min
Response: 807699
Conc: 5.14 ng/ml