

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080919\
 Data File : P0059099.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 Aug 2019 17:36
 Operator : SM/SJ
 Sample : K4232-02
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CORE-SAMPLE-BARREL-2-080719

Manual Integrations
 APPROVED

Ankita
 8/12/2019 1:17:44 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 10 01:51:43 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072819.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jul 27 06:49:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.150	3.513	795756	720757	18.856m	18.041
2) SA Decachlor...	9.653	8.393	954573	750644	17.627	19.017m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO080919\
Data File : PO059099.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Aug 2019 17:36
Operator : SM/SJ
Sample : K4232-02
Misc :
ALS Vial : 27 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
CORE-SAMPLE-BARREL-2-080719


Manual Integrations
APPROVED

Ankita
8/12/2019 1:17:44 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 10 01:51:43 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO072819.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jul 27 06:49:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

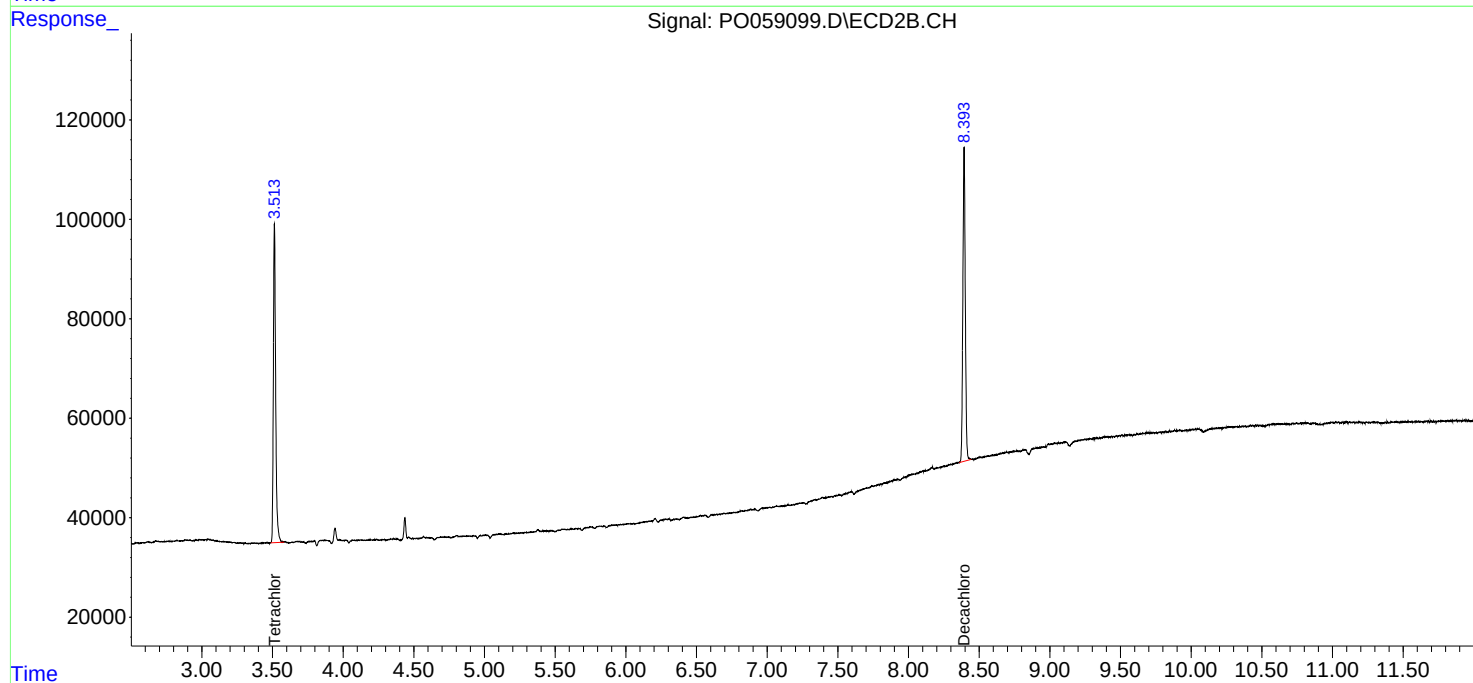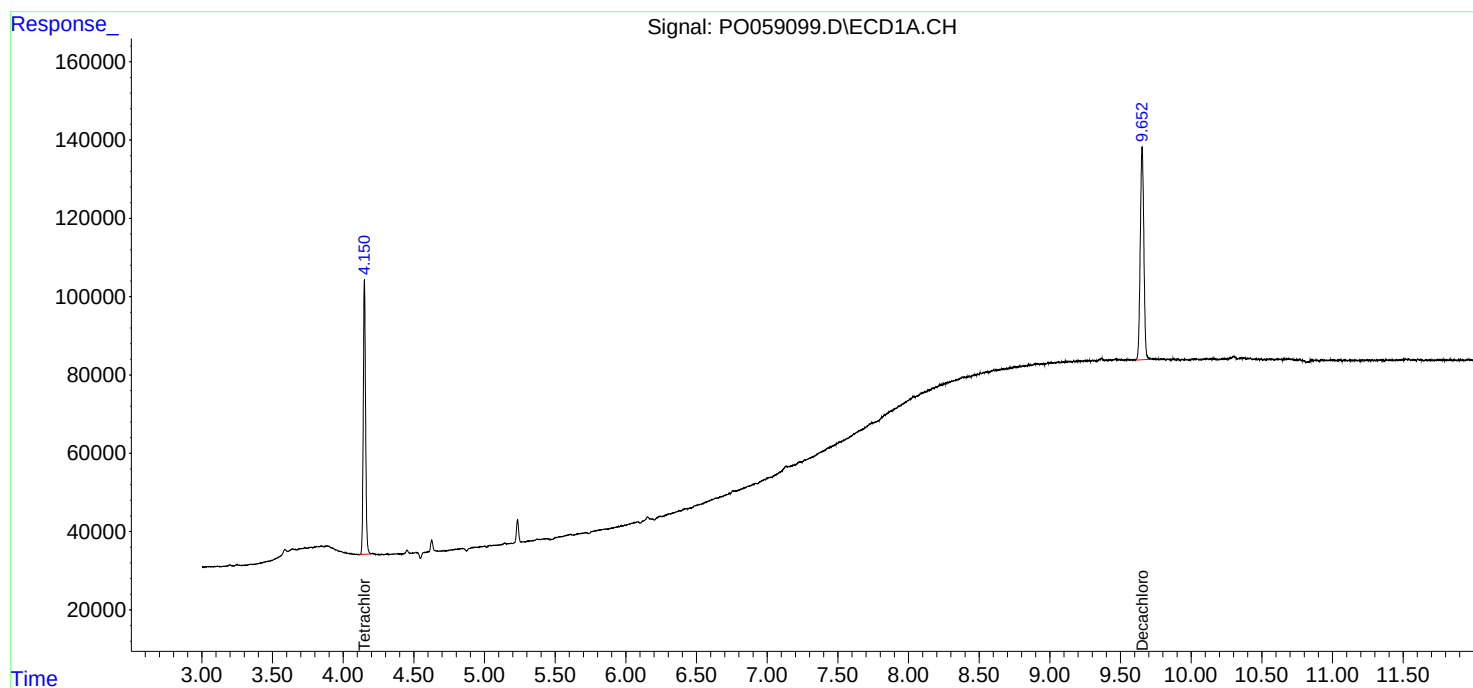

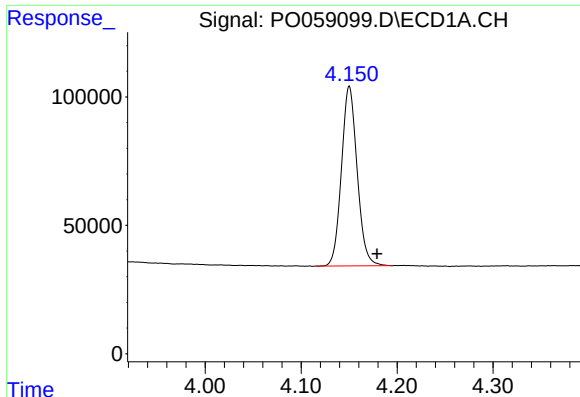


#1 Tetrachloro-m-xylene

R.T.: 4.150 min
Delta R.T.: -0.029 min
Response: 795756
Conc: 18.86 ng/ml m

Instrument :
ECD_O
ClientSampleId :
CORE-SAMPLE-BARREL-2-080719


Manual Integrations
APPROVED

Ankita
8/12/2019 1:17:44 PM

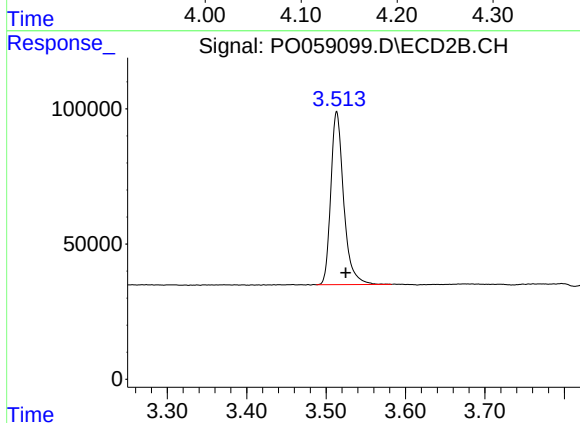


#1 Tetrachloro-m-xylene

R.T.: 3.513 min
Delta R.T.: -0.011 min
Response: 720757
Conc: 18.04 ng/ml

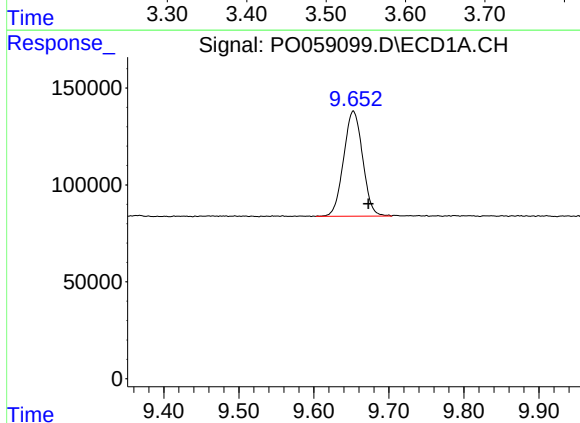

#2 Decachlorobiphenyl

R.T.: 9.653 min
Delta R.T.: -0.020 min
Response: 954573
Conc: 17.63 ng/ml

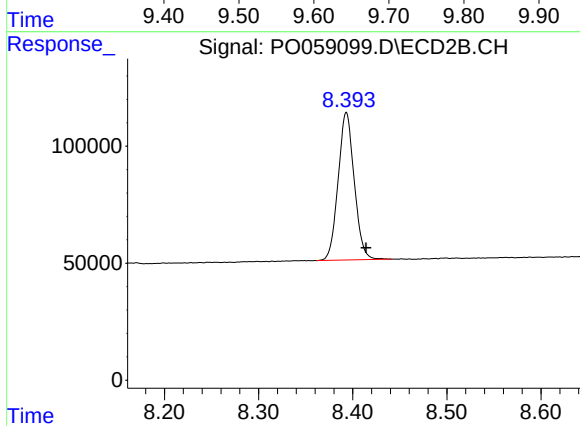

#2 Decachlorobiphenyl

R.T.: 8.393 min
Delta R.T.: -0.021 min
Response: 750644
Conc: 19.02 ng/ml m