

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080919\
 Data File : P0059103.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 Aug 2019 18:42
 Operator : SM/SJ
 Sample : K4233-01
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 DW-SCREEN-2

Manual Integrations
 APPROVED

Ankita
 8/12/2019 1:18:12 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 10 01:54:15 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072819.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jul 27 06:49:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.149	3.514	903159	829704	21.400m	20.768
2) SA Decachlor...	9.651	8.392	1128598	870133	20.840	22.044m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080919\
Data File : P0059103.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Aug 2019 18:42
Operator : SM/SJ
Sample : K4233-01
Misc :
ALS Vial : 31 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
DW-SCREEN-2


Manual Integrations
APPROVED

Ankita
8/12/2019 1:18:12 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 10 01:54:15 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072819.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jul 27 06:49:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

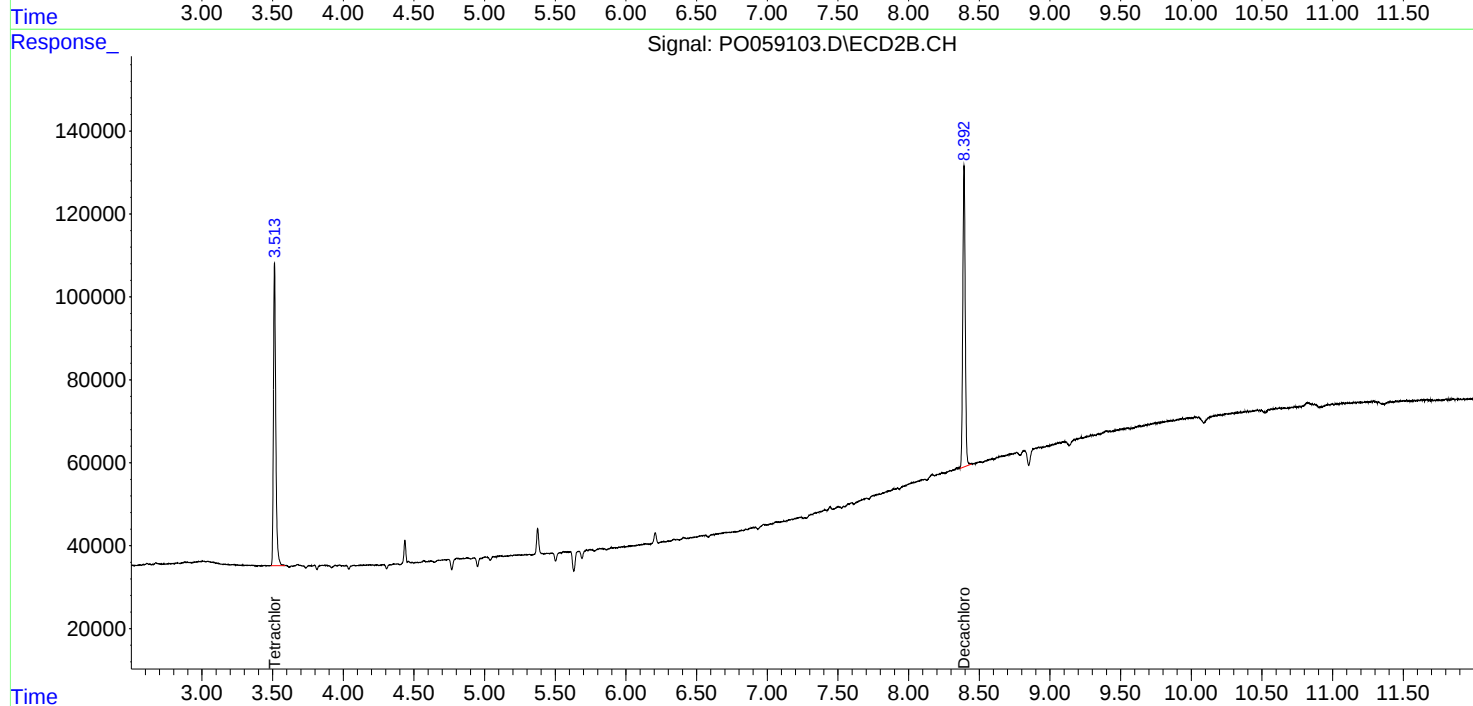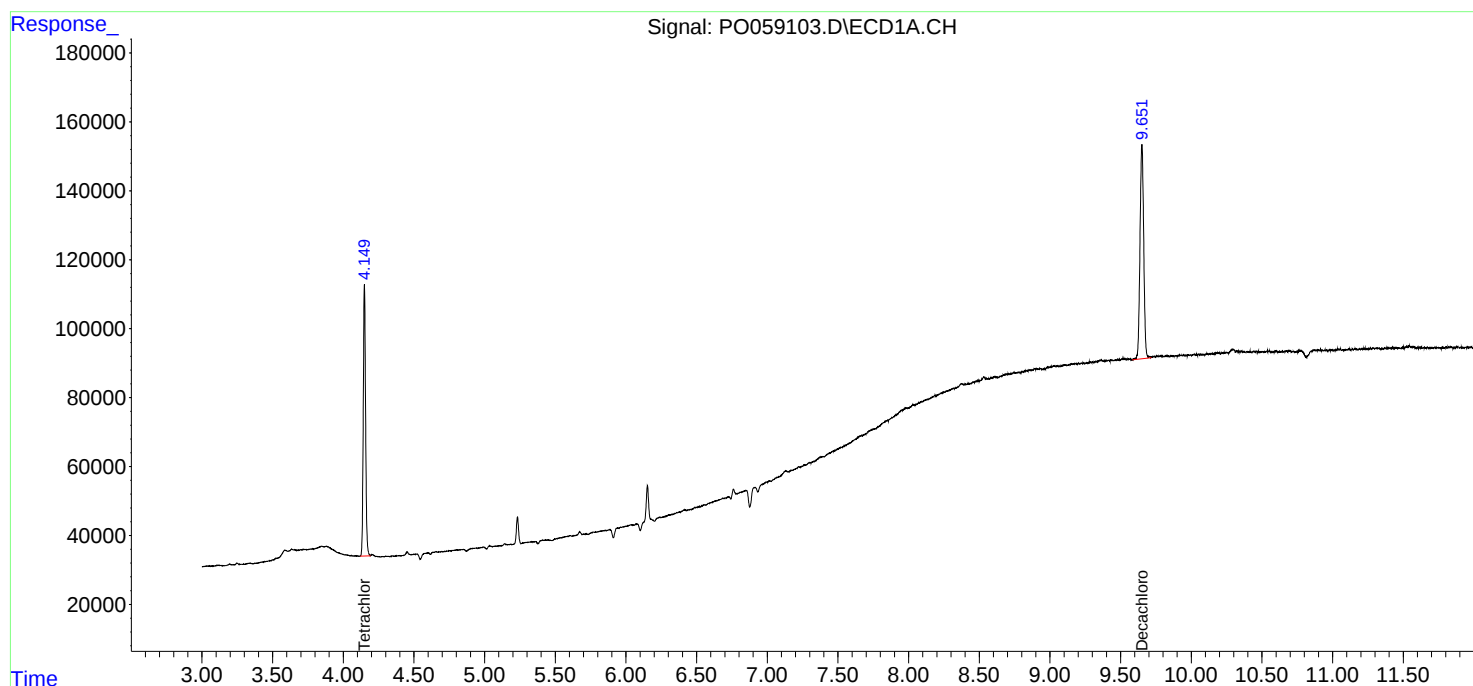

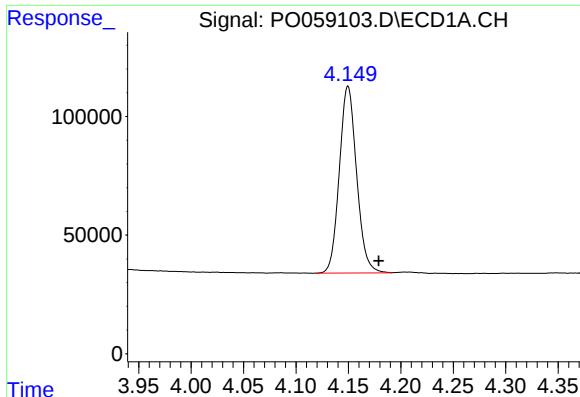


#1 Tetrachloro-m-xylene

R.T.: 4.149 min
Delta R.T.: -0.030 min
Response: 903159
Conc: 21.40 ng/ml m

Instrument :
ECD_O
ClientSampleId :
DW-SCREEN-2


Manual Integrations
APPROVED

Ankita
8/12/2019 1:18:12 PM

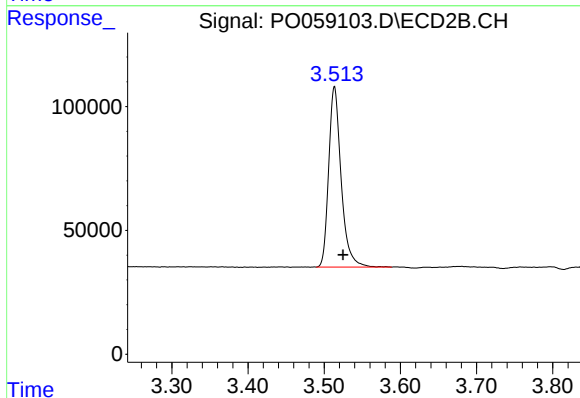


#1 Tetrachloro-m-xylene

R.T.: 3.514 min
Delta R.T.: -0.011 min
Response: 829704
Conc: 20.77 ng/ml

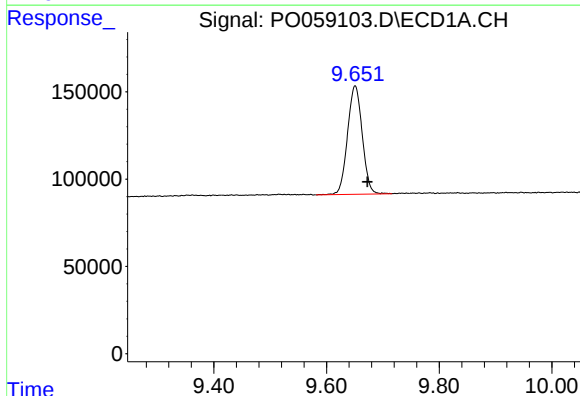

#2 Decachlorobiphenyl

R.T.: 9.651 min
Delta R.T.: -0.022 min
Response: 1128598
Conc: 20.84 ng/ml

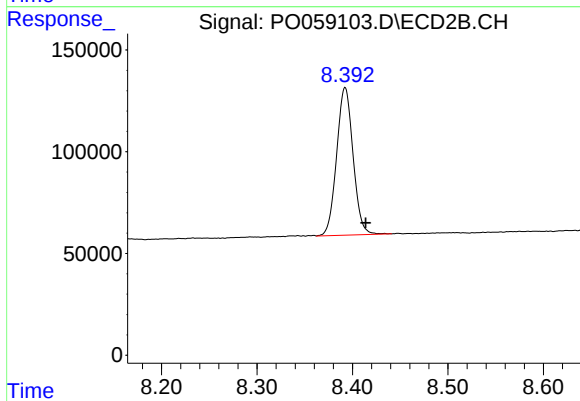

#2 Decachlorobiphenyl

R.T.: 8.392 min
Delta R.T.: -0.022 min
Response: 870133
Conc: 22.04 ng/ml m