

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080919\
 Data File : P0059121.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 Aug 2019 23:49
 Operator : SM/SJ
 Sample : K4235-06
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 HPPER-4-080719-74

Manual Integrations
 APPROVED

Ankita
 8/12/2019 1:18:50 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 10 02:05:43 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072819.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jul 27 06:49:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.149	3.513	745225	670778	17.658m	16.790
2) SA Decachlor...	9.647	8.390	955652	728908	17.646	18.466m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0080919\
Data File : P0059121.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Aug 2019 23:49
Operator : SM/SJ
Sample : K4235-06
Misc :
ALS Vial : 47 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
HPPER-4-080719-74


Manual Integrations
APPROVED

Ankita
8/12/2019 1:18:50 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 10 02:05:43 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072819.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jul 27 06:49:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

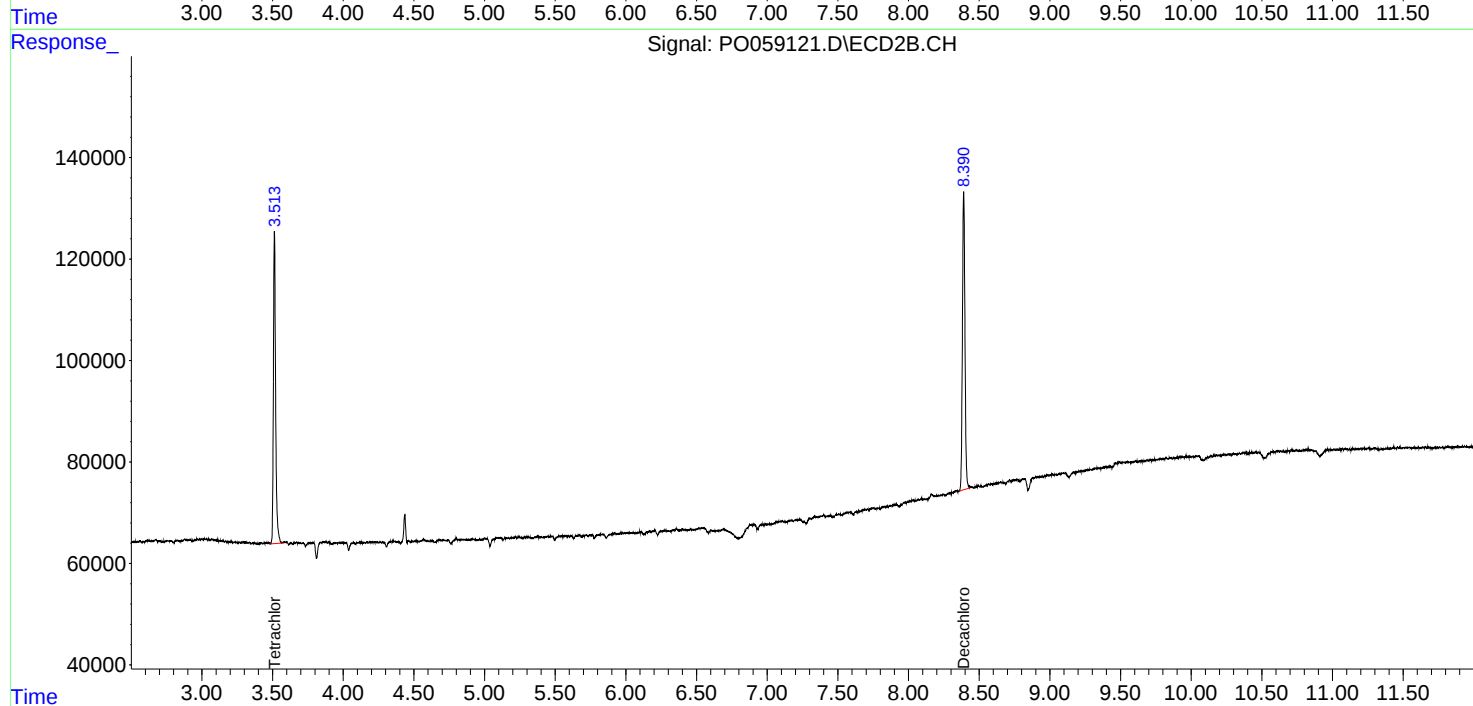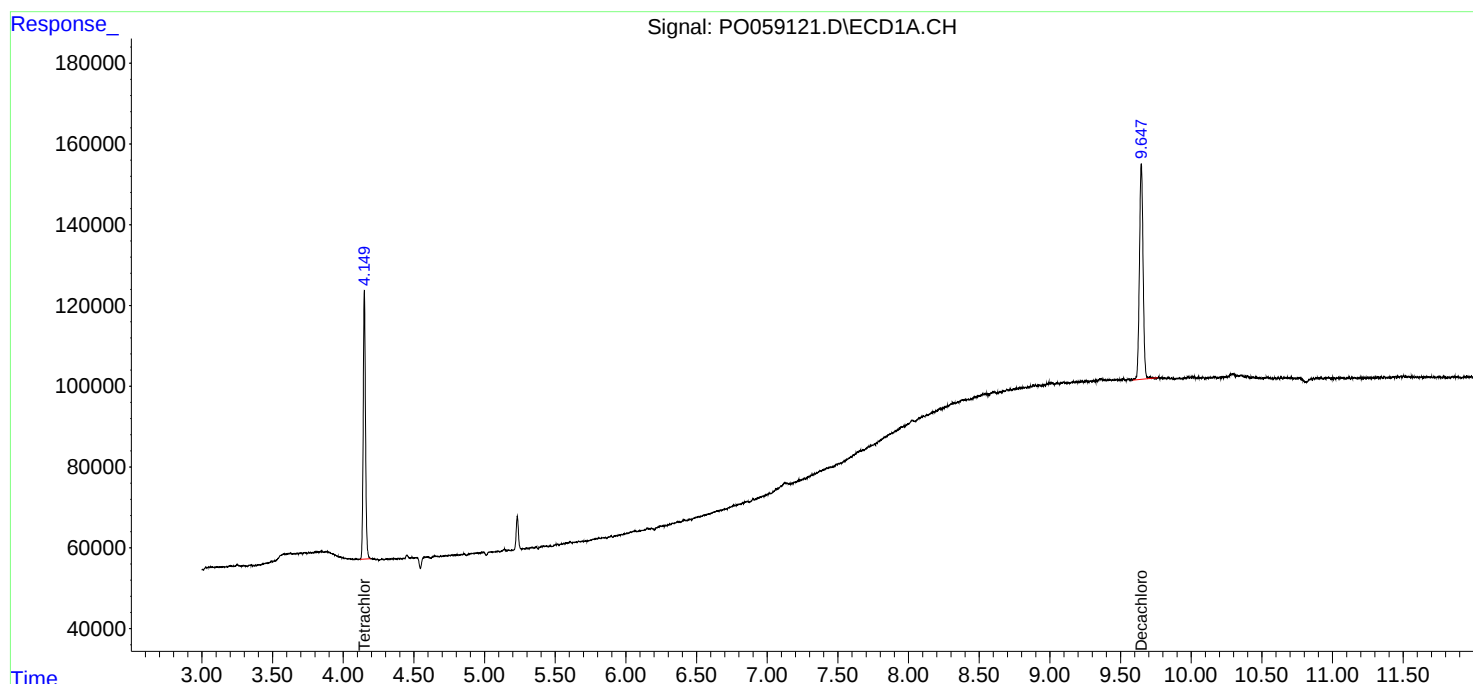

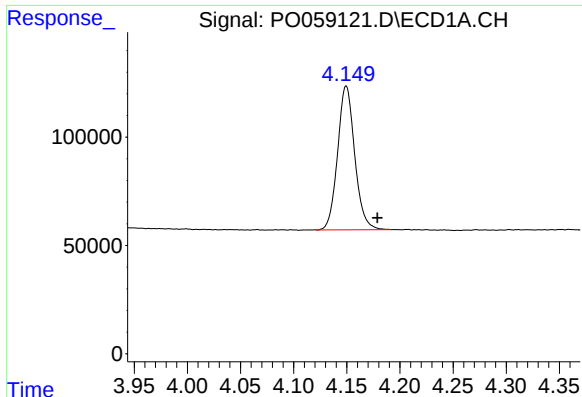


#1 Tetrachloro-m-xylene

R.T.: 4.149 min
Delta R.T.: -0.030 min
Response: 745225
Conc: 17.66 ng/ml m

Instrument :
ECD_O
ClientSampleId :
HPPER-4-080719-74


Manual Integrations
APPROVED

Ankita
8/12/2019 1:18:50 PM

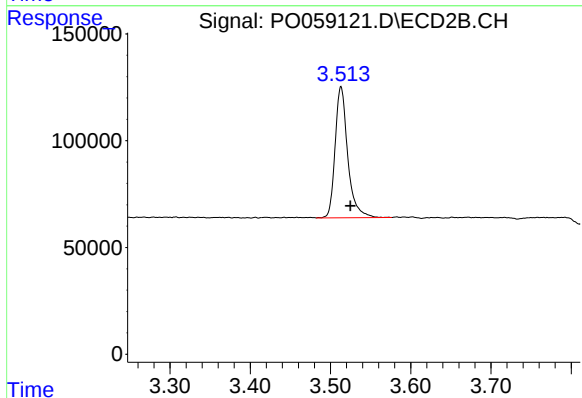


#1 Tetrachloro-m-xylene

R.T.: 3.513 min
Delta R.T.: -0.012 min
Response: 670778
Conc: 16.79 ng/ml

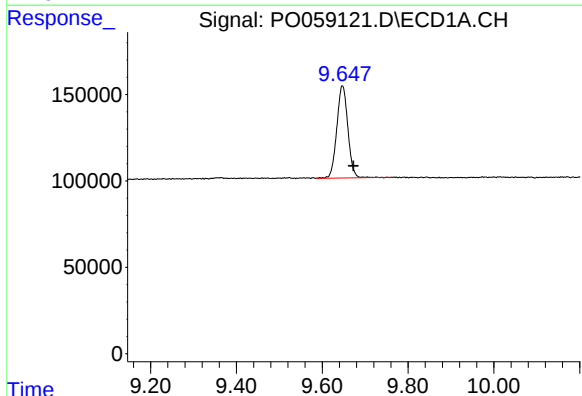

#2 Decachlorobiphenyl

R.T.: 9.647 min
Delta R.T.: -0.026 min
Response: 955652
Conc: 17.65 ng/ml

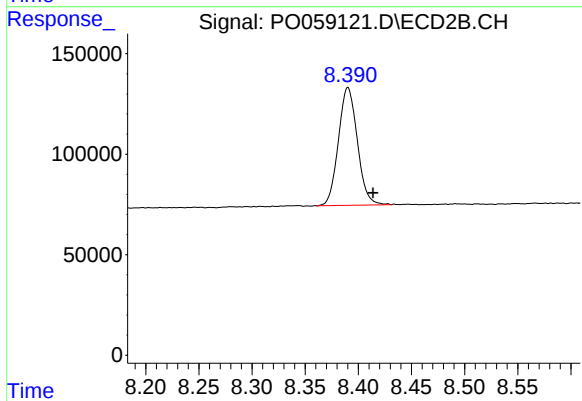

#2 Decachlorobiphenyl

R.T.: 8.390 min
Delta R.T.: -0.024 min
Response: 728908
Conc: 18.47 ng/ml m