

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081019\
 Data File : P0059148.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Aug 2019 10:53
 Operator : SM/SJ
 Sample : K4274-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SAMPLE-CORE-SPLITTER-080819

Manual Integrations
 APPROVED

Ankita
 8/12/2019 1:23:52 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 12 00:56:57 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072819.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jul 27 06:49:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.154	3.515	1096138	904807	25.973	22.648
2) SA Decachlor...	9.651	8.392	1185797	876965	21.896	22.217m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081019\
Data File : PO059148.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Aug 2019 10:53
Operator : SM/SJ
Sample : K4274-01
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SAMPLE-CORE-SPLITTER-080819


Manual Integrations
APPROVED

Ankita
8/12/2019 1:23:52 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 12 00:56:57 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO072819.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jul 27 06:49:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

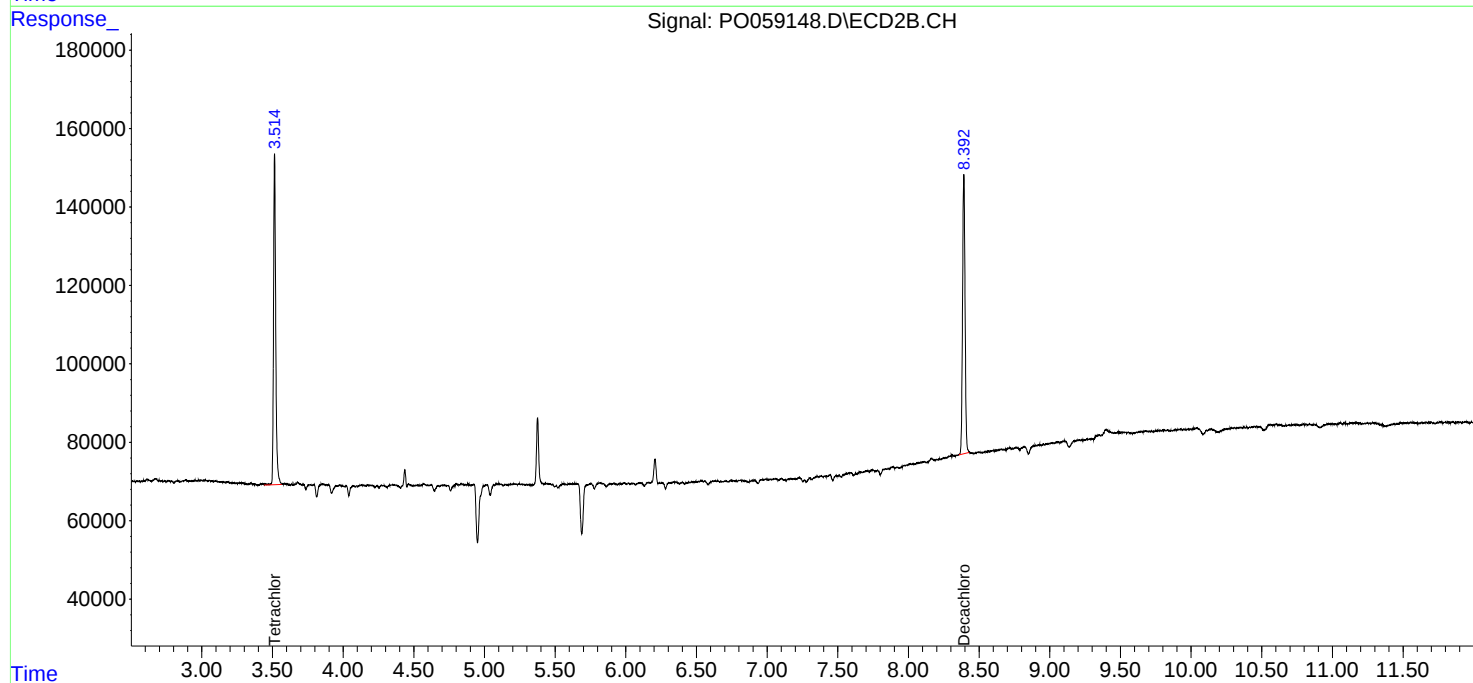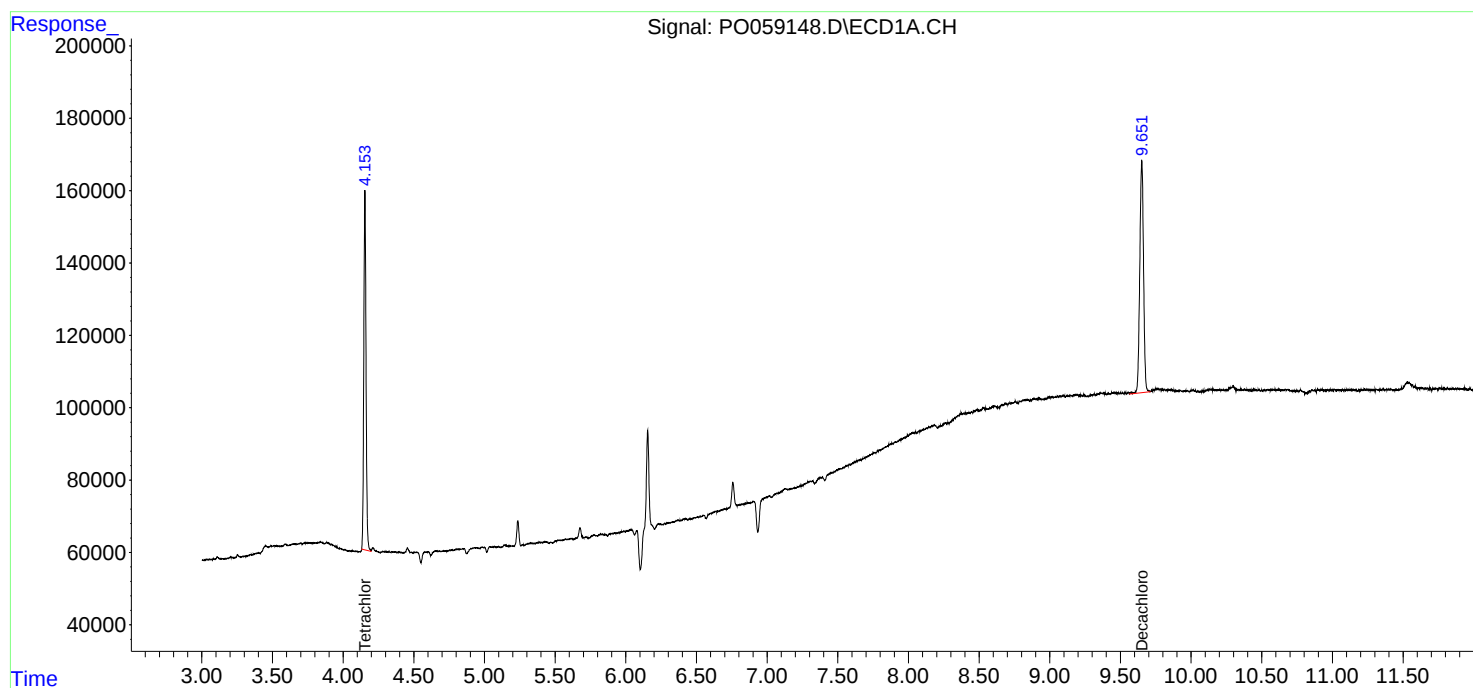

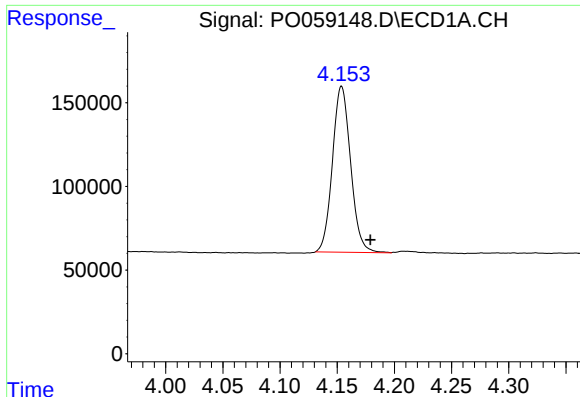


#1 Tetrachloro-m-xylene

R.T.: 4.154 min
Delta R.T.: -0.025 min
Response: 1096138
Conc: 25.97 ng/ml

Instrument :
ECD_O
ClientSampleId :
SAMPLE-CORE-SPLITTER-080819


Manual Integrations
APPROVED

Ankita
8/12/2019 1:23:52 PM

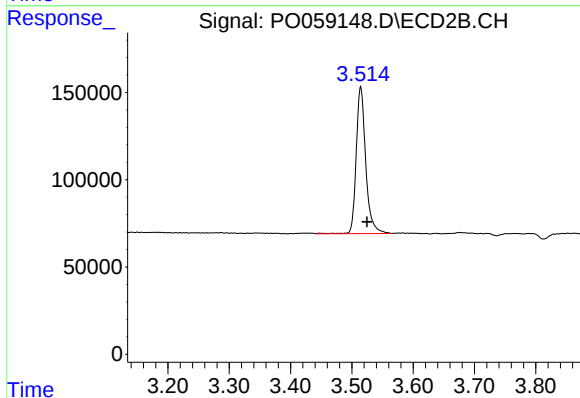


#1 Tetrachloro-m-xylene

R.T.: 3.515 min
Delta R.T.: -0.010 min
Response: 904807
Conc: 22.65 ng/ml

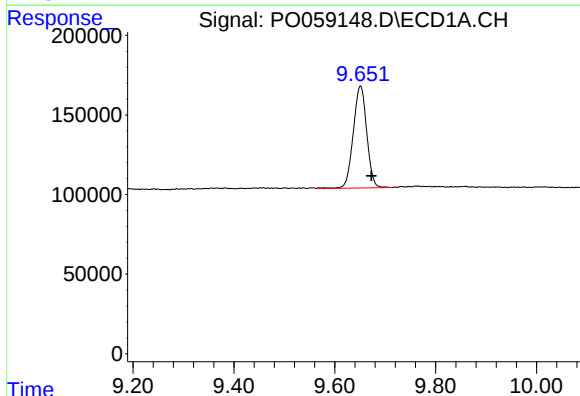

#2 Decachlorobiphenyl

R.T.: 9.651 min
Delta R.T.: -0.022 min
Response: 1185797
Conc: 21.90 ng/ml

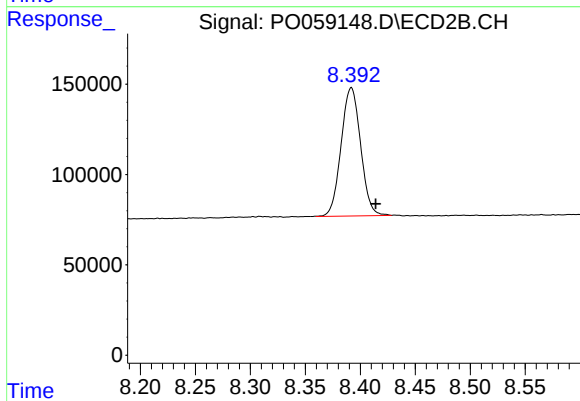

#2 Decachlorobiphenyl

R.T.: 8.392 min
Delta R.T.: -0.023 min
Response: 876965
Conc: 22.22 ng/ml m