

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081919\
 Data File : P0059463.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Aug 2019 18:19
 Operator : SM/AJ
 Sample : K3591-09
 Misc : AR1660 MDL 25PPB
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-MDL-WATER-03-QT3-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 20 01:05:32 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 17 03:09:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.152	3.506	485033	448835	13.853	12.469
2)	SA Decachlor...	9.643	8.380	730844	526640	13.738	13.061
Target Compounds							
3)	L1 AR-1016-1	5.306	4.560	41288	26954	25.743	19.938
4)	L1 AR-1016-2	5.326	4.578	54431	34328	22.751	17.138
5)	L1 AR-1016-3	5.387	4.746	36821	22485	24.720	20.784
6)	L1 AR-1016-4	5.485	4.790	32918	47445	27.211	52.542 #
7)	L1 AR-1016-5	5.774	5.000	35698	18777	27.799	16.301 #
8)	L2 AR-1221-1	0.000	3.666	0	8411	N.D.	20.955 #
9)	L2 AR-1221-2	4.452	3.799	10956	11215	33.732	36.816
10)	L2 AR-1221-3	4.524	3.870	18689	12450	17.767	12.724 #
11)	L3 AR-1232-1	4.524	3.870	18689	12450	14.994	10.920 #
12)	L3 AR-1232-2	5.041	4.578	32528	34328	46.047	26.954 #
13)	L3 AR-1232-3	5.326	4.746	54431	22485	35.544	33.022
14)	L3 AR-1232-4	5.485	4.831	32918	45421	42.101	74.454 #
15)	L3 AR-1232-5	5.572	5.000	39664	18777	65.982	27.584 #
16)	L4 AR-1242-1	5.306	4.560	41288	26954	32.523	26.203
17)	L4 AR-1242-2	5.326	4.578	54431	34328	29.332	22.539
18)	L4 AR-1242-3	5.387	4.746	36821	22485	31.502	26.912
19)	L4 AR-1242-4	5.485	4.831	32918	45421	34.010	54.437 #
20)	L4 AR-1242-5	6.214	5.342	26730	21347	21.271	19.083
21)	L5 AR-1248-1	5.306	4.560	41288	26954	41.183	32.553
22)	L5 AR-1248-2	5.572	4.790	39664	47445	27.337	41.144 #
23)	L5 AR-1248-3	5.774	4.831	35698	45421	21.478	38.241 #
24)	L5 AR-1248-4	6.150	5.000	221624	18777	108.421	12.922 #
25)	L5 AR-1248-5	6.214	5.366	26730	114482	13.479	79.985 #
26)	L6 AR-1254-1	6.150	5.342	221624	21347	106.222	9.000 #
27)	L6 AR-1254-2	6.360	5.483	56597	42910	16.964	20.450
28)	L6 AR-1254-3	6.724	5.898	49860	105475	14.051	31.368 #
29)	L6 AR-1254-4	7.008	6.114	102317	96994	34.736	47.043 #
30)	L6 AR-1254-5	7.422	6.520	208848	145823	67.536	46.964 #
31)	L7 AR-1260-1	6.886	6.010	96519	156002	35.803	68.455 #
32)	L7 AR-1260-2	7.139	6.198	145962	163093	39.338	55.665 #
33)	L7 AR-1260-3	7.492	6.347	120637	110827	36.821	41.835
34)	L7 AR-1260-4	7.717	6.810	201662	97794	65.660	43.223 #
35)	L7 AR-1260-5	8.024	7.052	493482	277091	69.692	50.350 #
36)	L8 AR-1262-1	7.492	6.554	120637	98983	24.859	26.554
37)	L8 AR-1262-2	8.024	7.052	493482	277091	63.957	47.132 #
38)	L8 AR-1262-3	8.309	7.327	279475	135263	54.774	53.233
39)	L8 AR-1262-4	8.374	7.391	173440	361647	44.994	81.840 #
40)	L8 AR-1262-5	8.985	7.884	301560	52200	117.496	28.911 #
41)	L9 AR-1268-1	8.309	7.327	279475	135263	29.698	18.995 #
42)	L9 AR-1268-2	8.374	7.391	173440	361647	22.003	56.087 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081919\
 Data File : P0059463.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Aug 2019 18:19
 Operator : SM/AJ
 Sample : K3591-09
 Misc : AR1660 MDL 25PPB
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-MDL-WATER-03-QT3-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 20 01:05:32 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 17 03:09:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
43) L9	AR-1268-3	8.596	7.591	49707	19822	7.052	3.623 #
44) L9	AR-1268-4	8.985	7.884	301560	52200	108.473	25.572 #
45) L9	AR-1268-5	9.353	8.150	176798	34067	9.587	2.345 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081919\
Data File : PO059463.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Aug 2019 18:19
Operator : SM/AJ
Sample : K3591-09
Misc : AR1660 MDL 25PPB
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 20 01:05:32 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Aug 17 03:09:44 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

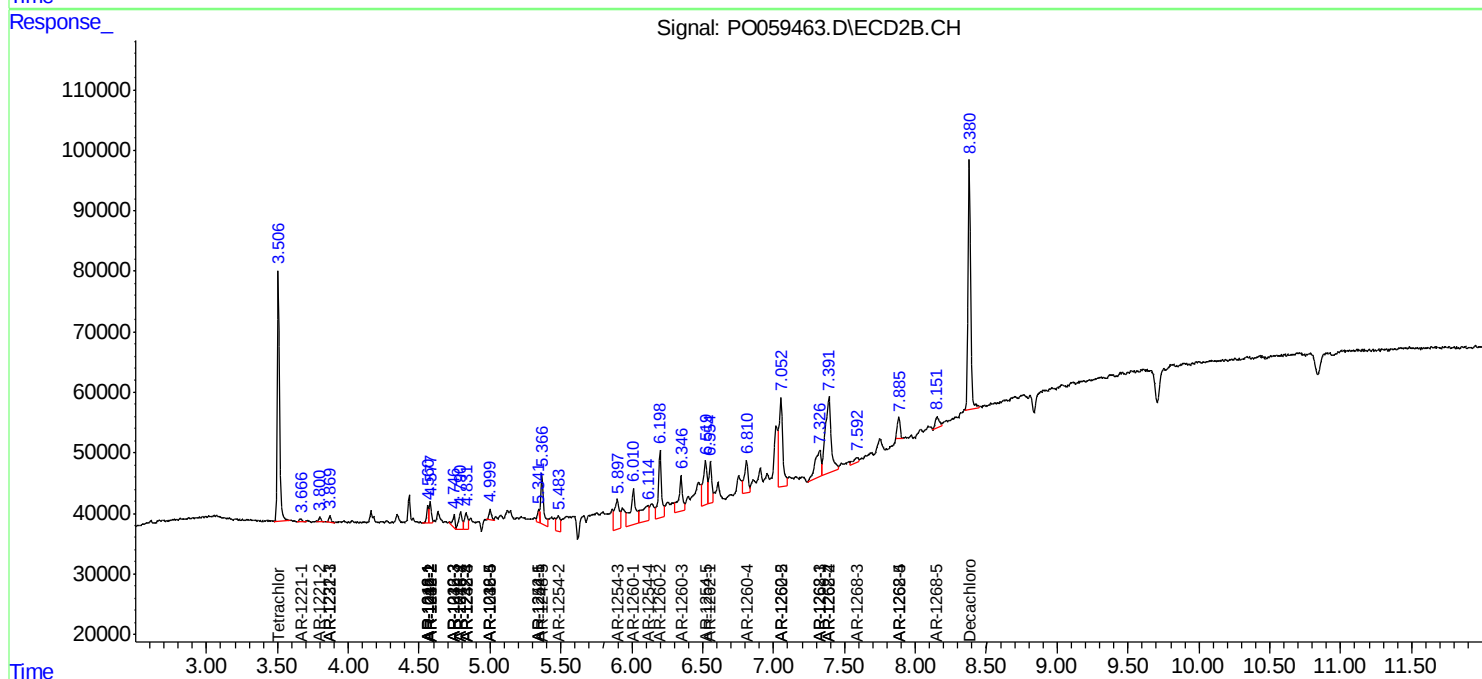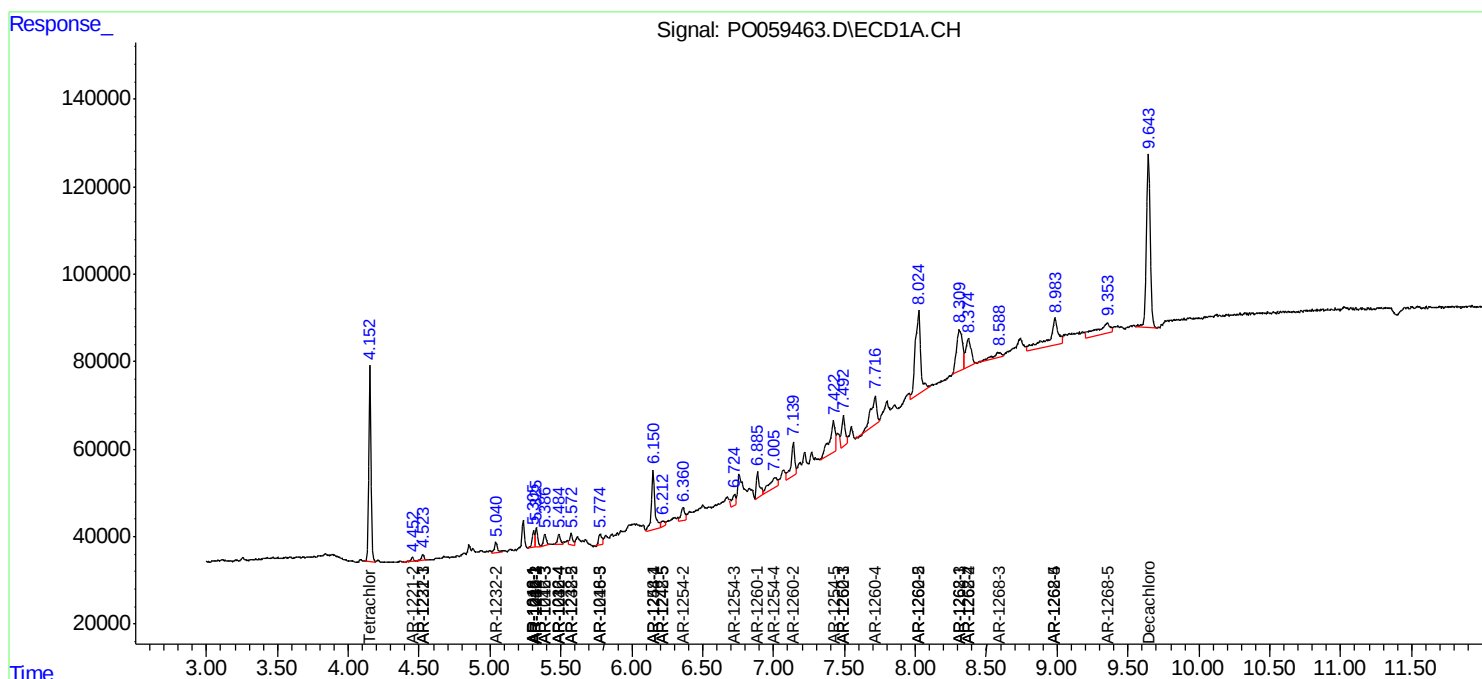


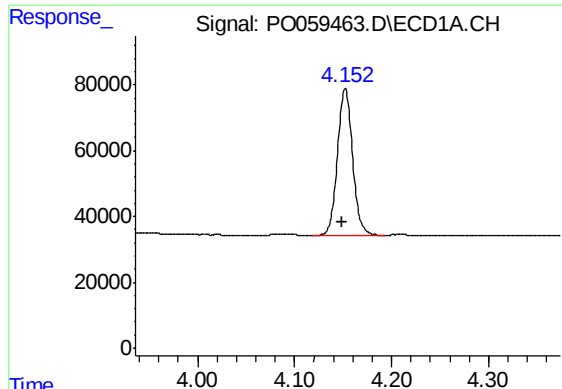

#1 Tetrachloro-m-xylene


R.T.: 4.152 min
Delta R.T.: 0.003 min
Response: 485033
Conc: 13.85 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019




#1 Tetrachloro-m-xylene

R.T.: 3.506 min
Delta R.T.: -0.004 min
Response: 448835
Conc: 12.47 ng/ml




#2 Decachlorobiphenyl

R.T.: 9.643 min
Delta R.T.: 0.002 min
Response: 730844
Conc: 13.74 ng/ml

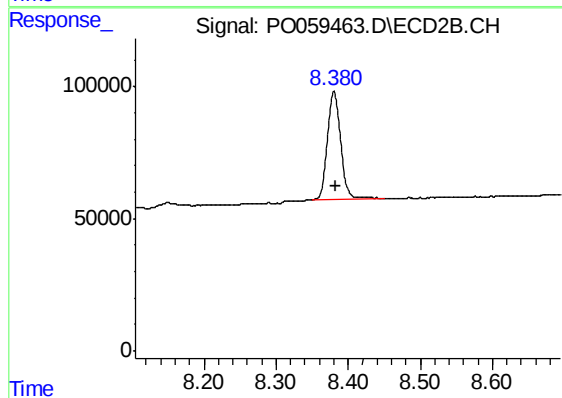

#2 Decachlorobiphenyl


R.T.: 8.380 min
Delta R.T.: -0.003 min
Response: 526640
Conc: 13.06 ng/ml

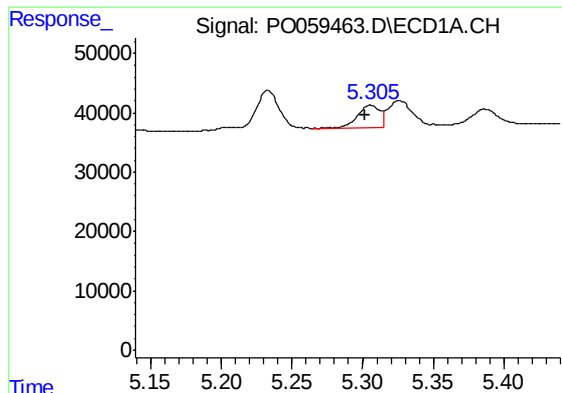

#3 AR-1016-1


R.T.: 5.306 min
Delta R.T.: 0.004 min
Response: 41288
Conc: 25.74 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

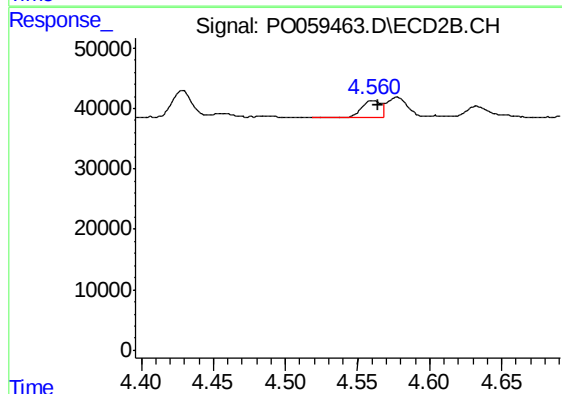


#3 AR-1016-1

R.T.: 4.560 min
Delta R.T.: -0.004 min
Response: 26954
Conc: 19.94 ng/ml




#4 AR-1016-2

R.T.: 5.326 min
Delta R.T.: 0.003 min
Response: 54431
Conc: 22.75 ng/ml

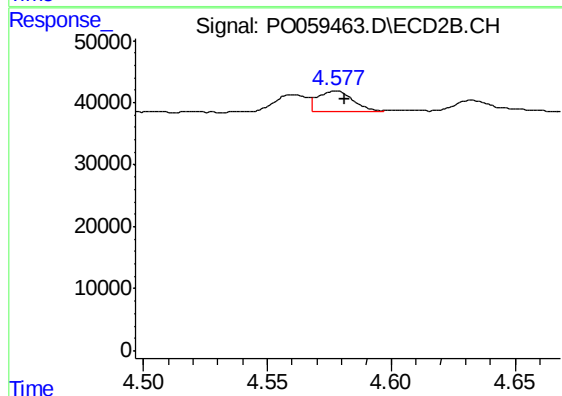

#4 AR-1016-2


R.T.: 4.578 min
Delta R.T.: -0.004 min
Response: 34328
Conc: 17.14 ng/ml

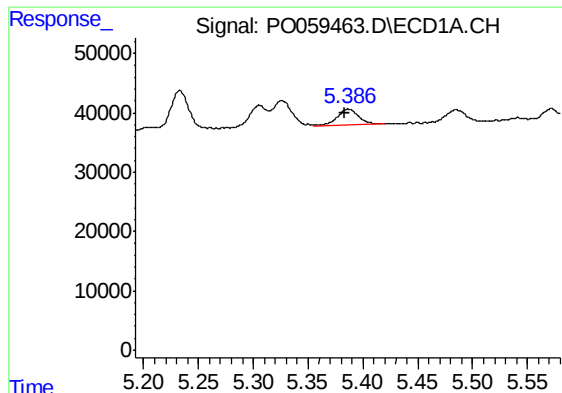

#5 AR-1016-3


R.T.: 5.387 min
Delta R.T.: 0.003 min
Response: 36821
Conc: 24.72 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

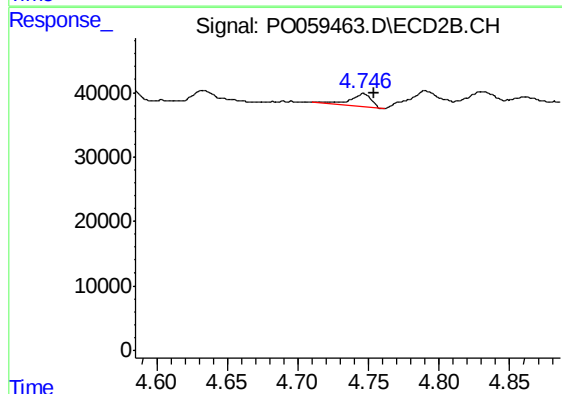


#5 AR-1016-3

R.T.: 4.746 min
Delta R.T.: -0.008 min
Response: 22485
Conc: 20.78 ng/ml

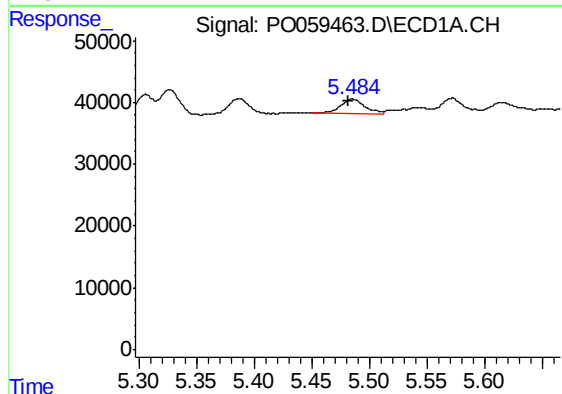


#6 AR-1016-4

R.T.: 5.485 min
Delta R.T.: 0.004 min
Response: 32918
Conc: 27.21 ng/ml

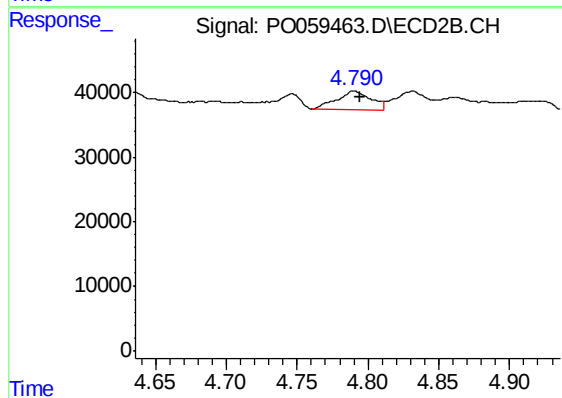

#6 AR-1016-4


R.T.: 4.790 min
Delta R.T.: -0.004 min
Response: 47445
Conc: 52.54 ng/ml

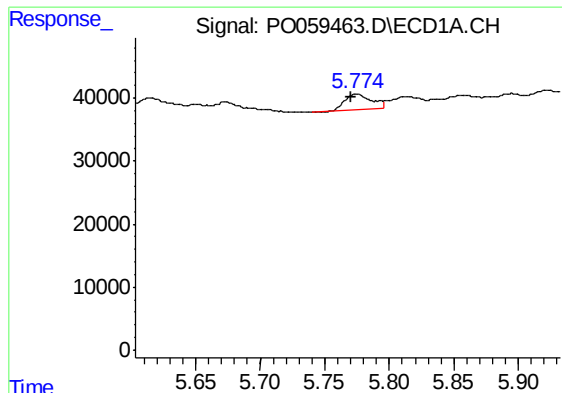

#7 AR-1016-5


R.T.: 5.774 min
Delta R.T.: 0.005 min
Response: 35698
Conc: 27.80 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

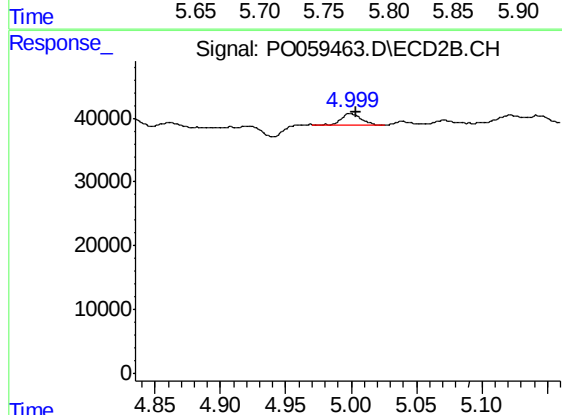


#7 AR-1016-5

R.T.: 5.000 min
Delta R.T.: -0.004 min
Response: 18777
Conc: 16.30 ng/ml

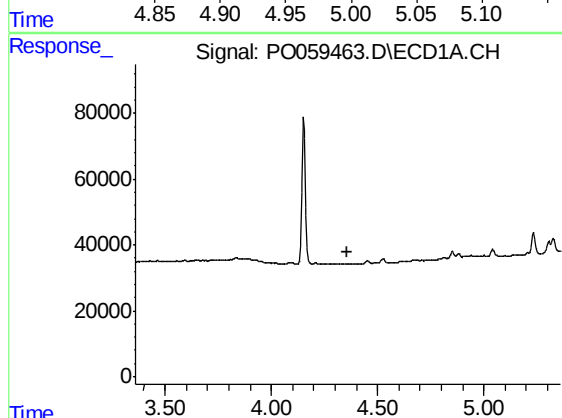


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.360 min
Response: 0
Conc: N.D.

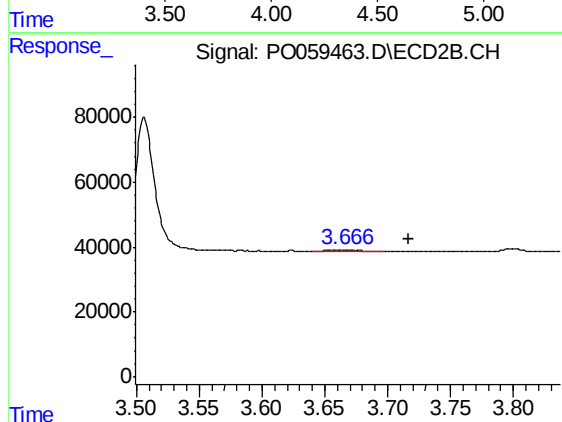

#8 AR-1221-1


R.T.: 3.666 min
Delta R.T.: -0.050 min
Response: 8411
Conc: 20.96 ng/ml

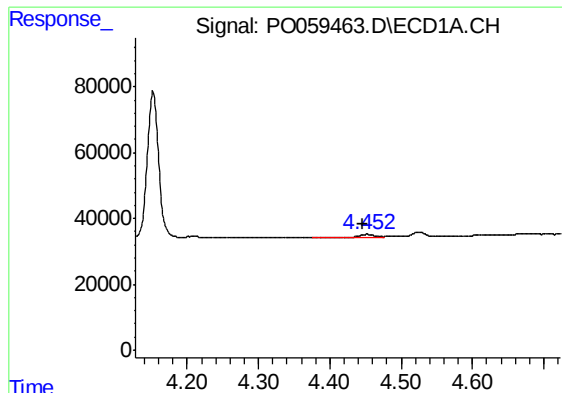

#9 AR-1221-2


R.T.: 4.452 min
Delta R.T.: 0.006 min
Response: 10956
Conc: 33.73 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

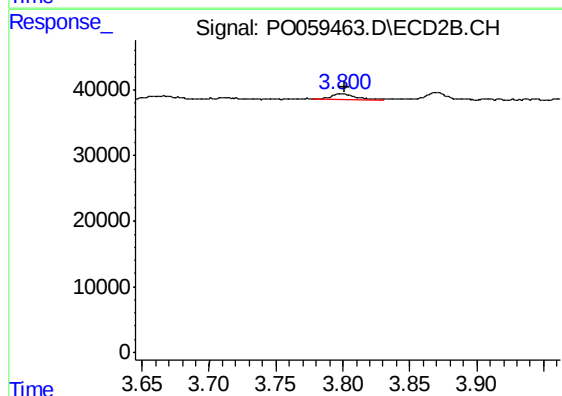


#9 AR-1221-2

R.T.: 3.799 min
Delta R.T.: -0.002 min
Response: 11215
Conc: 36.82 ng/ml

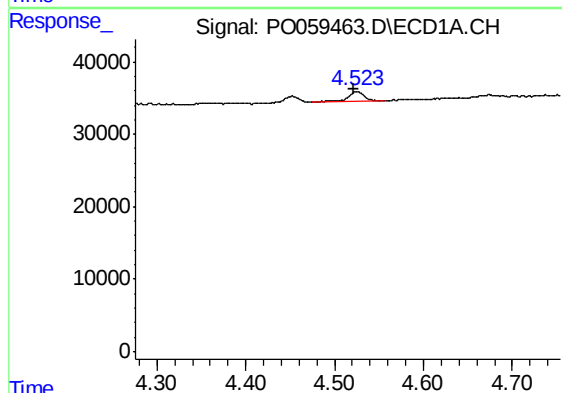


#10 AR-1221-3

R.T.: 4.524 min
Delta R.T.: 0.003 min
Response: 18689
Conc: 17.77 ng/ml

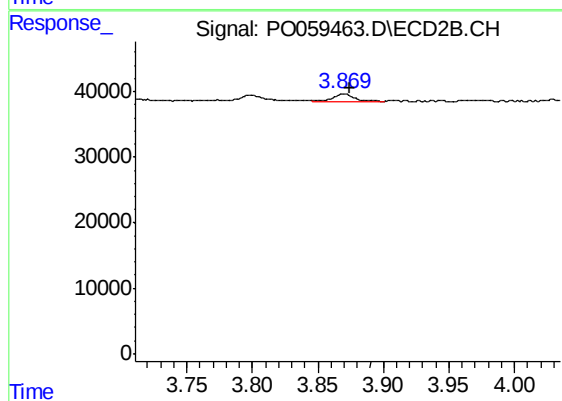

#10 AR-1221-3


R.T.: 3.870 min
Delta R.T.: -0.004 min
Response: 12450
Conc: 12.72 ng/ml

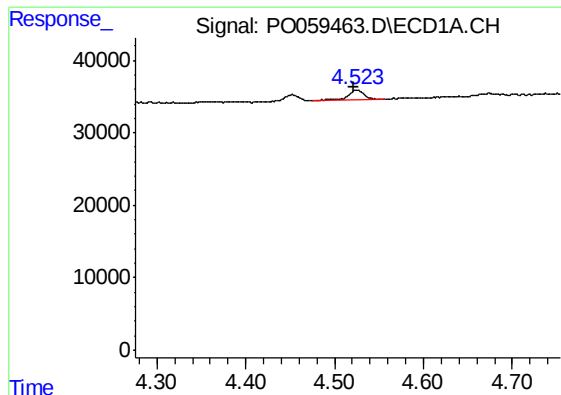

#11 AR-1232-1


R.T.: 4.524 min
Delta R.T.: 0.003 min
Response: 18689
Conc: 14.99 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

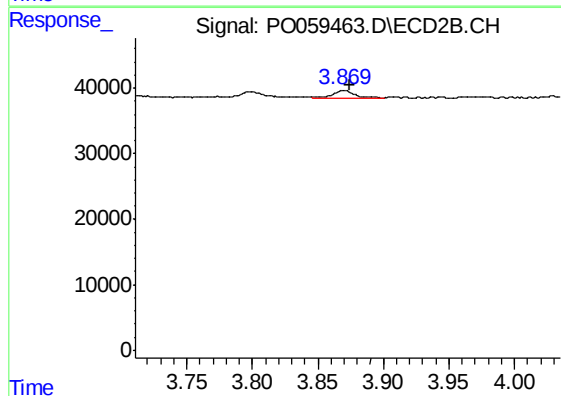


#11 AR-1232-1

R.T.: 3.870 min
Delta R.T.: -0.004 min
Response: 12450
Conc: 10.92 ng/ml

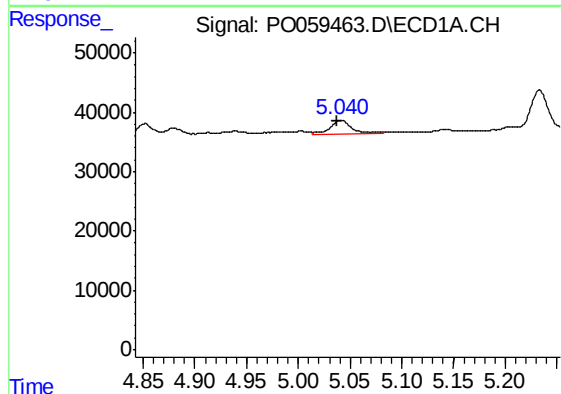


#12 AR-1232-2

R.T.: 5.041 min
Delta R.T.: 0.003 min
Response: 32528
Conc: 46.05 ng/ml

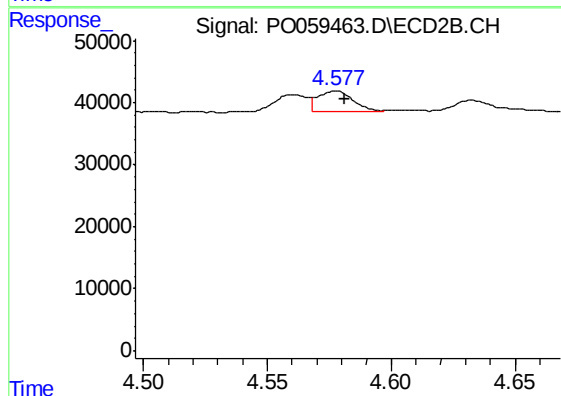

#12 AR-1232-2


R.T.: 4.578 min
Delta R.T.: -0.003 min
Response: 34328
Conc: 26.95 ng/ml



#13 AR-1232-3


R.T.: 5.326 min
Delta R.T.: 0.004 min
Response: 54431
Conc: 35.54 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019




#13 AR-1232-3

R.T.: 4.746 min
Delta R.T.: -0.007 min
Response: 22485
Conc: 33.02 ng/ml




#14 AR-1232-4

R.T.: 5.485 min
Delta R.T.: 0.004 min
Response: 32918
Conc: 42.10 ng/ml

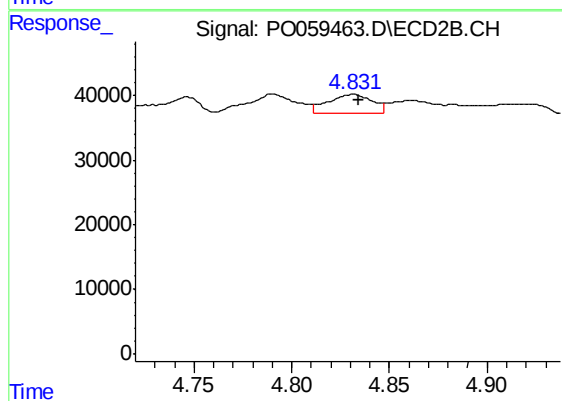

#14 AR-1232-4


R.T.: 4.831 min
Delta R.T.: -0.003 min
Response: 45421
Conc: 74.45 ng/ml

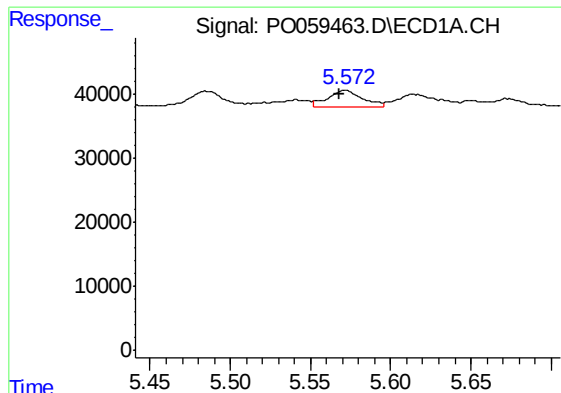

#15 AR-1232-5


R.T.: 5.572 min
Delta R.T.: 0.004 min
Response: 39664
Conc: 65.98 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

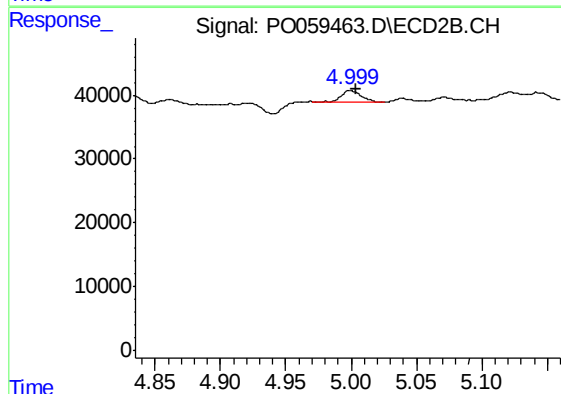


#15 AR-1232-5

R.T.: 5.000 min
Delta R.T.: -0.004 min
Response: 18777
Conc: 27.58 ng/ml

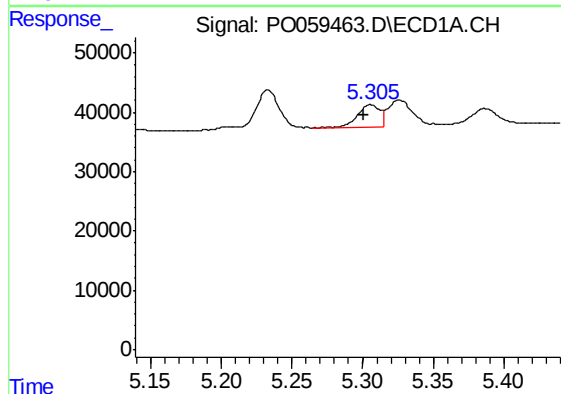


#16 AR-1242-1

R.T.: 5.306 min
Delta R.T.: 0.004 min
Response: 41288
Conc: 32.52 ng/ml

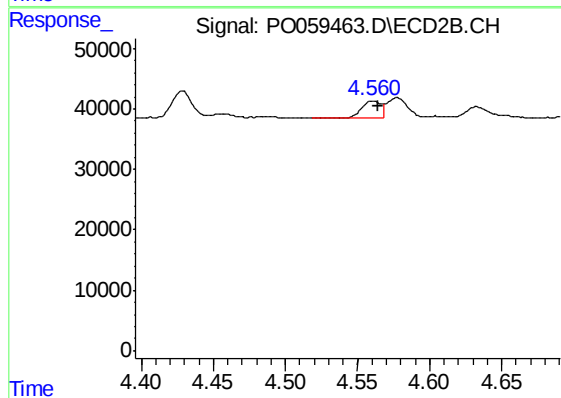

#16 AR-1242-1


R.T.: 4.560 min
Delta R.T.: -0.004 min
Response: 26954
Conc: 26.20 ng/ml

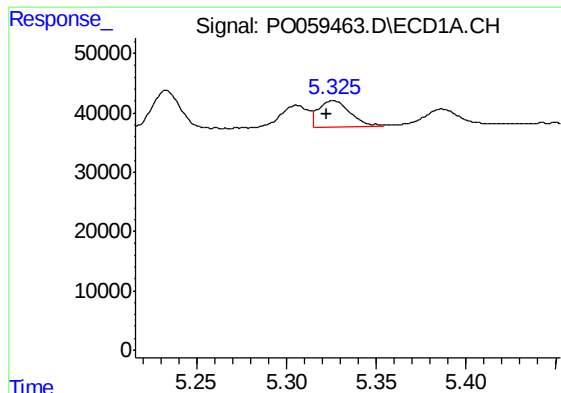

#17 AR-1242-2


R.T.: 5.326 min
Delta R.T.: 0.003 min
Response: 54431
Conc: 29.33 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

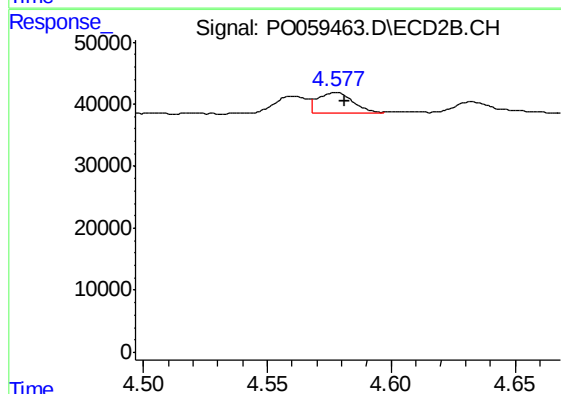


#17 AR-1242-2

R.T.: 4.578 min
Delta R.T.: -0.004 min
Response: 34328
Conc: 22.54 ng/ml

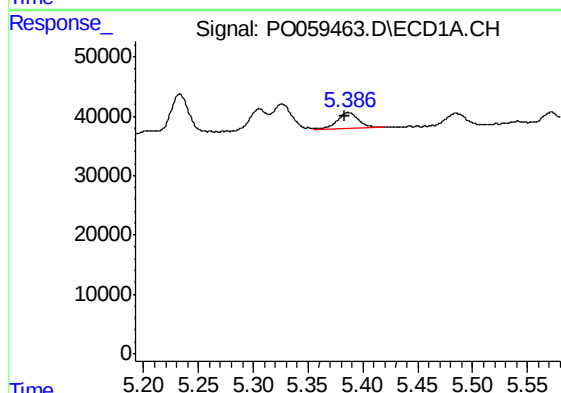


#18 AR-1242-3

R.T.: 5.387 min
Delta R.T.: 0.003 min
Response: 36821
Conc: 31.50 ng/ml

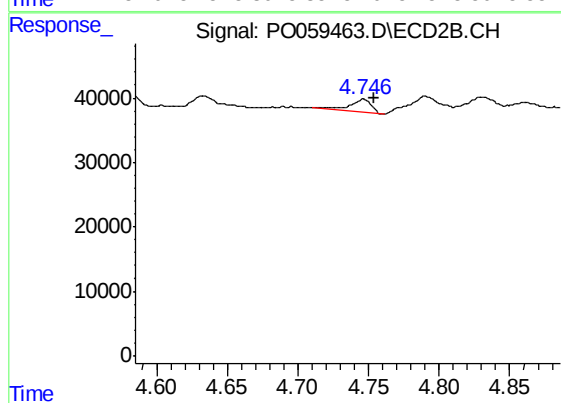

#18 AR-1242-3


R.T.: 4.746 min
Delta R.T.: -0.007 min
Response: 22485
Conc: 26.91 ng/ml



#19 AR-1242-4


R.T.: 5.485 min
Delta R.T.: 0.004 min
Response: 32918
Conc: 34.01 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019




#19 AR-1242-4

R.T.: 4.831 min
Delta R.T.: -0.003 min
Response: 45421
Conc: 54.44 ng/ml

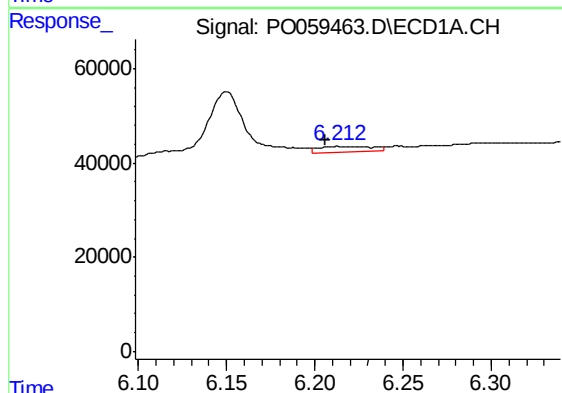


#20 AR-1242-5

R.T.: 6.214 min
Delta R.T.: 0.008 min
Response: 26730
Conc: 21.27 ng/ml

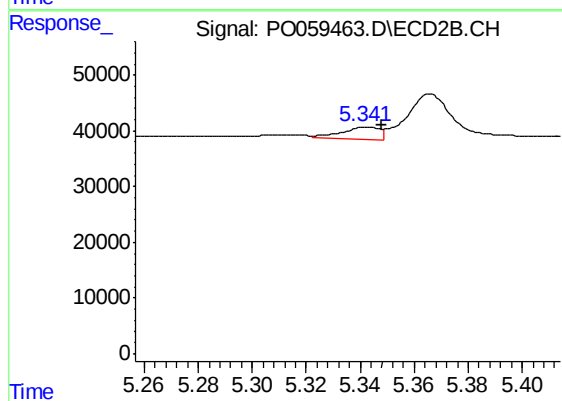

#20 AR-1242-5


R.T.: 5.342 min
Delta R.T.: -0.006 min
Response: 21347
Conc: 19.08 ng/ml

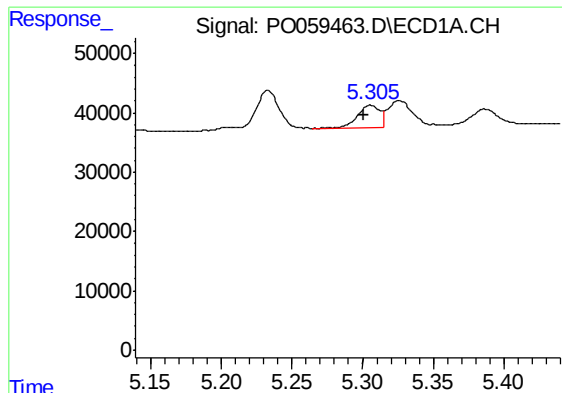

#21 AR-1248-1


R.T.: 5.306 min
Delta R.T.: 0.005 min
Response: 41288
Conc: 41.18 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

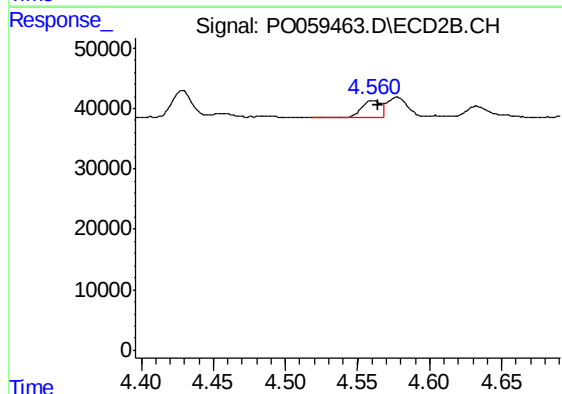


#21 AR-1248-1

R.T.: 4.560 min
Delta R.T.: -0.004 min
Response: 26954
Conc: 32.55 ng/ml

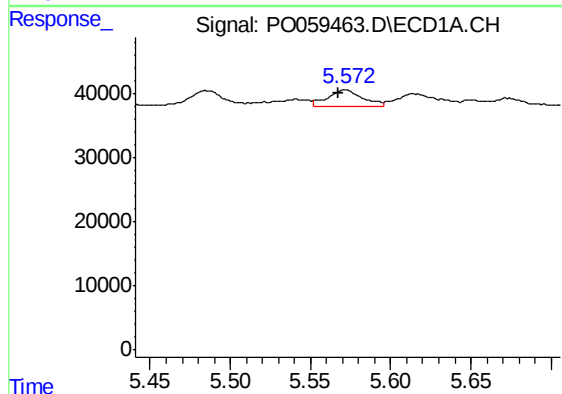


#22 AR-1248-2

R.T.: 5.572 min
Delta R.T.: 0.005 min
Response: 39664
Conc: 27.34 ng/ml

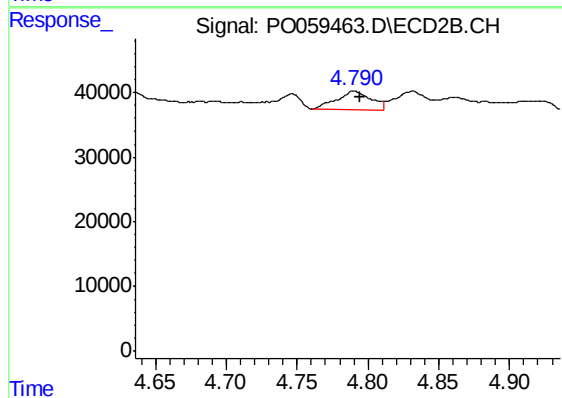

#22 AR-1248-2


R.T.: 4.790 min
Delta R.T.: -0.004 min
Response: 47445
Conc: 41.14 ng/ml

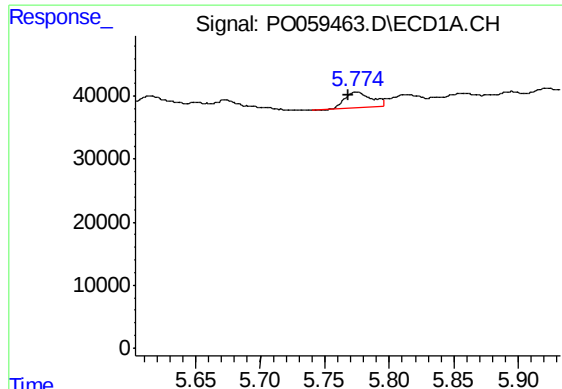

#23 AR-1248-3


R.T.: 5.774 min
Delta R.T.: 0.006 min
Response: 35698
Conc: 21.48 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

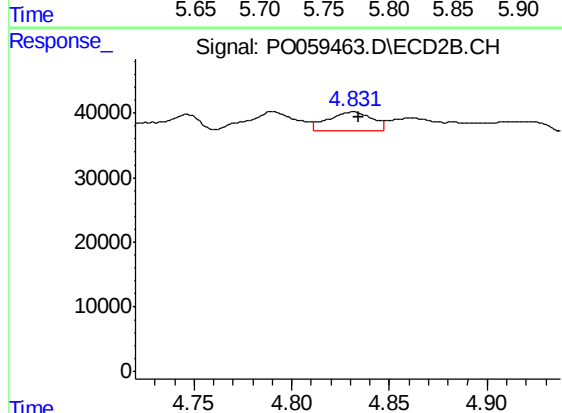


#23 AR-1248-3

R.T.: 4.831 min
Delta R.T.: -0.003 min
Response: 45421
Conc: 38.24 ng/ml

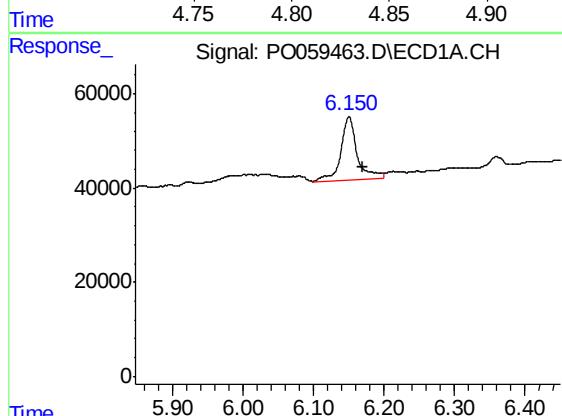


#24 AR-1248-4

R.T.: 6.150 min
Delta R.T.: -0.019 min
Response: 221624
Conc: 108.42 ng/ml

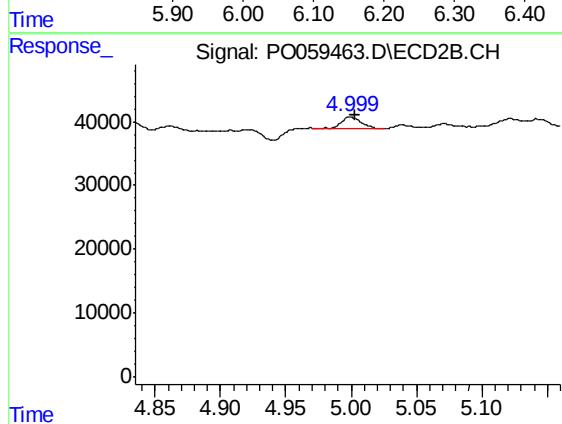

#24 AR-1248-4


R.T.: 5.000 min
Delta R.T.: -0.003 min
Response: 18777
Conc: 12.92 ng/ml

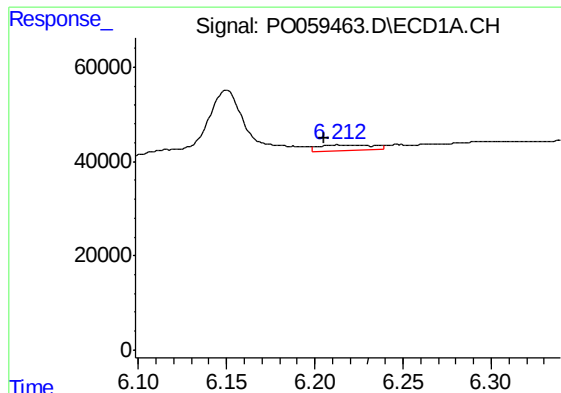

#25 AR-1248-5


R.T.: 6.214 min
Delta R.T.: 0.009 min
Response: 26730
Conc: 13.48 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

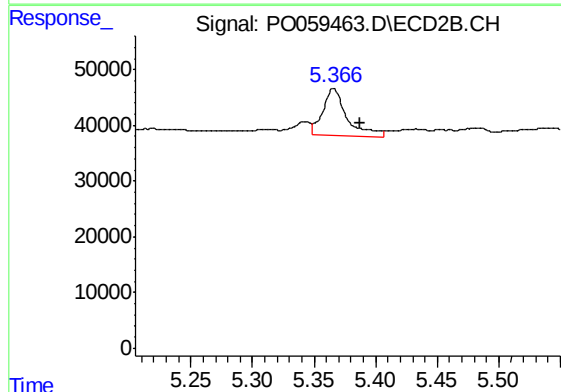


#25 AR-1248-5

R.T.: 5.366 min
Delta R.T.: -0.021 min
Response: 114482
Conc: 79.99 ng/ml

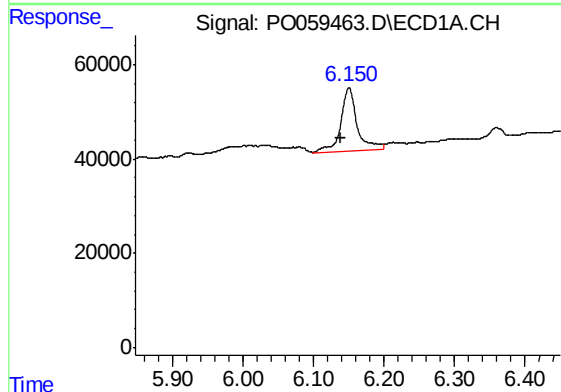


#26 AR-1254-1

R.T.: 6.150 min
Delta R.T.: 0.011 min
Response: 221624
Conc: 106.22 ng/ml

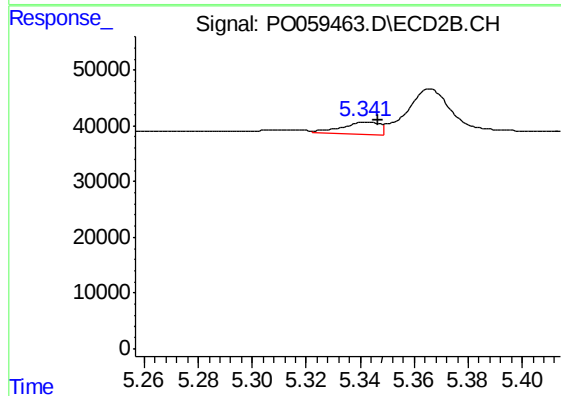

#26 AR-1254-1


R.T.: 5.342 min
Delta R.T.: -0.004 min
Response: 21347
Conc: 9.00 ng/ml



#27 AR-1254-2


R.T.: 6.360 min
Delta R.T.: 0.005 min
Response: 56597
Conc: 16.96 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

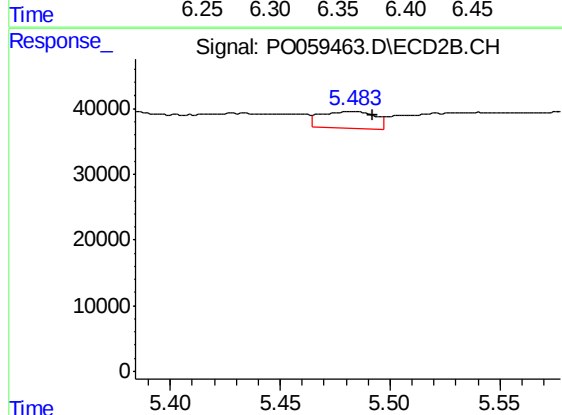


#27 AR-1254-2

R.T.: 5.483 min
Delta R.T.: -0.009 min
Response: 42910
Conc: 20.45 ng/ml

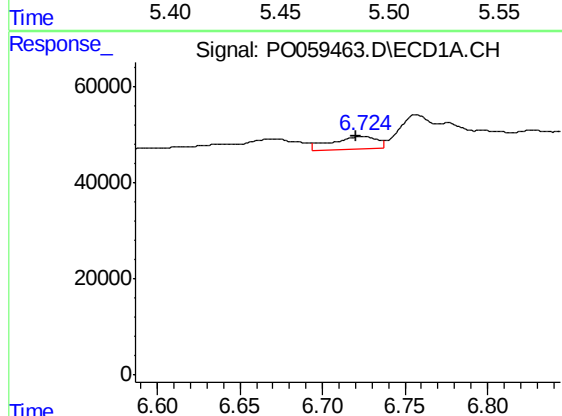


#28 AR-1254-3

R.T.: 6.724 min
Delta R.T.: 0.004 min
Response: 49860
Conc: 14.05 ng/ml

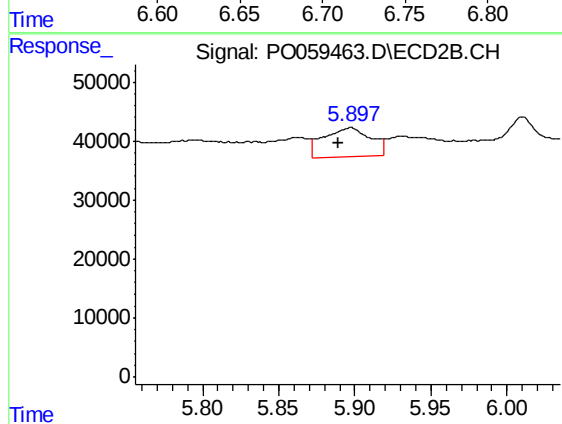

#28 AR-1254-3


R.T.: 5.898 min
Delta R.T.: 0.009 min
Response: 105475
Conc: 31.37 ng/ml



#29 AR-1254-4


R.T.: 7.008 min
Delta R.T.: 0.003 min
Response: 102317
Conc: 34.74 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019




#29 AR-1254-4

R.T.: 6.114 min
Delta R.T.: -0.001 min
Response: 96994
Conc: 47.04 ng/ml




#30 AR-1254-5

R.T.: 7.422 min
Delta R.T.: 0.003 min
Response: 208848
Conc: 67.54 ng/ml

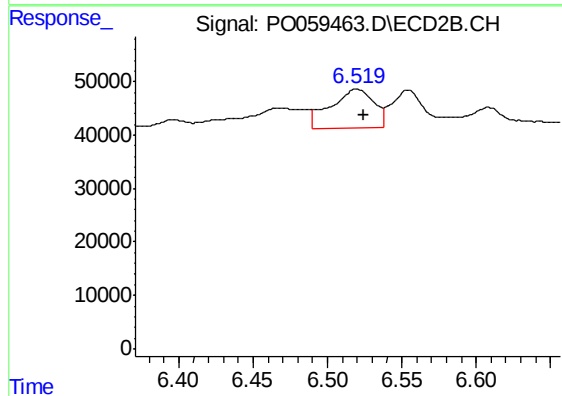

#30 AR-1254-5


R.T.: 6.520 min
Delta R.T.: -0.004 min
Response: 145823
Conc: 46.96 ng/ml



#31 AR-1260-1


R.T.: 6.886 min
Delta R.T.: 0.006 min
Response: 96519
Conc: 35.80 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019




#31 AR-1260-1

R.T.: 6.010 min
Delta R.T.: -0.004 min
Response: 156002
Conc: 68.45 ng/ml




#32 AR-1260-2

R.T.: 7.139 min
Delta R.T.: 0.003 min
Response: 145962
Conc: 39.34 ng/ml

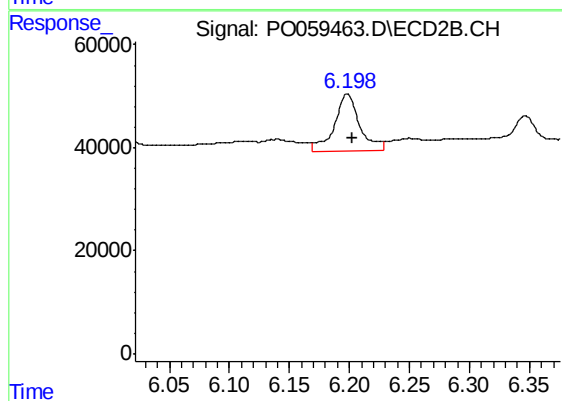

#32 AR-1260-2


R.T.: 6.198 min
Delta R.T.: -0.004 min
Response: 163093
Conc: 55.67 ng/ml



#33 AR-1260-3


R.T.: 7.492 min
Delta R.T.: 0.002 min
Response: 120637
Conc: 36.82 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019




#33 AR-1260-3

R.T.: 6.347 min
Delta R.T.: -0.004 min
Response: 110827
Conc: 41.84 ng/ml




#34 AR-1260-4

R.T.: 7.717 min
Delta R.T.: 0.000 min
Response: 201662
Conc: 65.66 ng/ml

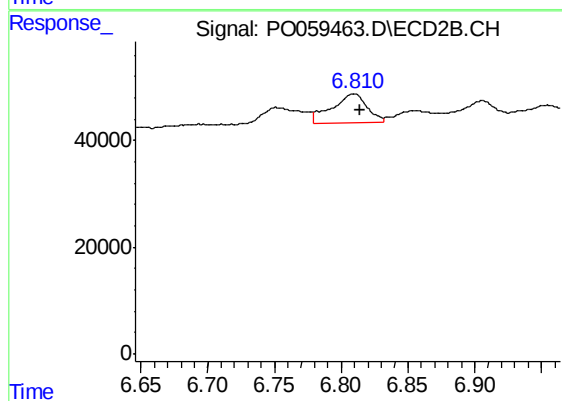

#34 AR-1260-4


R.T.: 6.810 min
Delta R.T.: -0.004 min
Response: 97794
Conc: 43.22 ng/ml

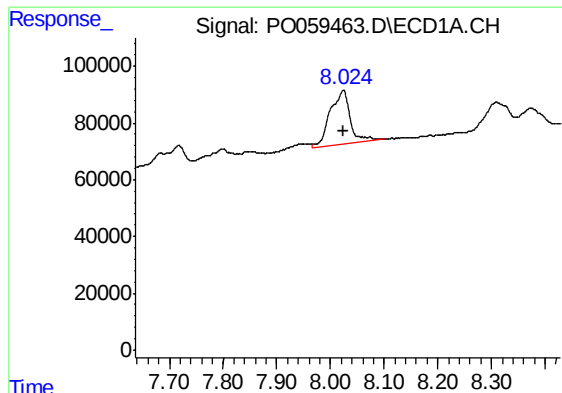

#35 AR-1260-5


R.T.: 8.024 min
Delta R.T.: 0.000 min
Response: 493482
Conc: 69.69 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019




#35 AR-1260-5

R.T.: 7.052 min
Delta R.T.: -0.005 min
Response: 277091
Conc: 50.35 ng/ml




#36 AR-1262-1

R.T.: 7.492 min
Delta R.T.: 0.004 min
Response: 120637
Conc: 24.86 ng/ml

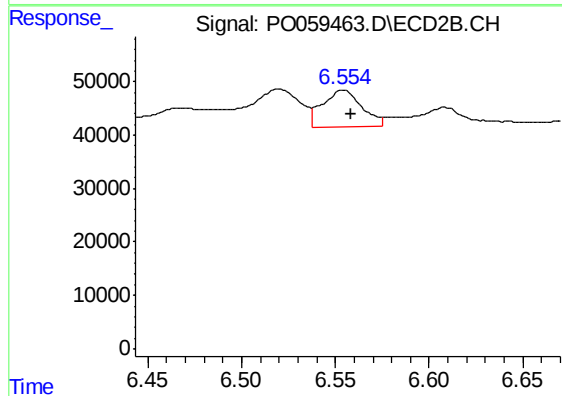

#36 AR-1262-1


R.T.: 6.554 min
Delta R.T.: -0.004 min
Response: 98983
Conc: 26.55 ng/ml



#37 AR-1262-2


R.T.: 8.024 min
Delta R.T.: 0.000 min
Response: 493482
Conc: 63.96 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019




#37 AR-1262-2

R.T.: 7.052 min
Delta R.T.: -0.005 min
Response: 277091
Conc: 47.13 ng/ml




#38 AR-1262-3

R.T.: 8.309 min
Delta R.T.: 0.006 min
Response: 279475
Conc: 54.77 ng/ml

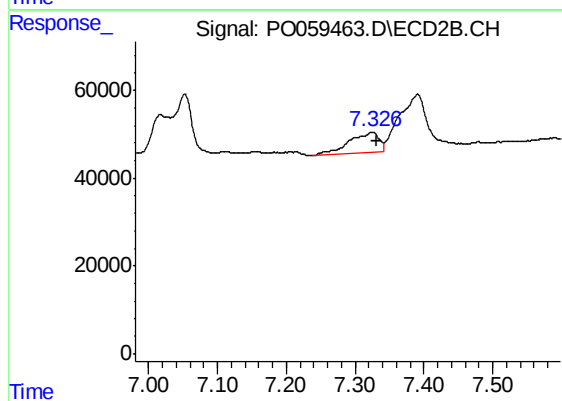

#38 AR-1262-3


R.T.: 7.327 min
Delta R.T.: -0.006 min
Response: 135263
Conc: 53.23 ng/ml



#39 AR-1262-4


R.T.: 8.374 min
Delta R.T.: -0.013 min
Response: 173440
Conc: 44.99 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

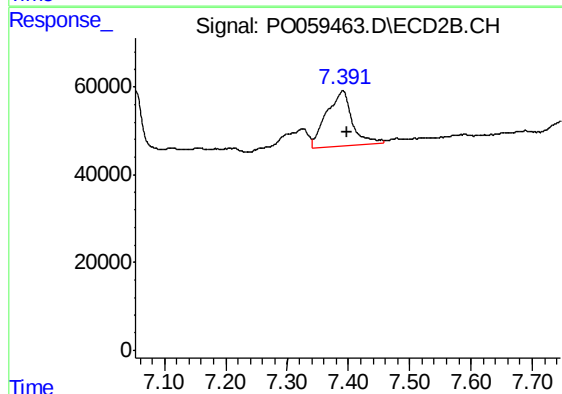


#39 AR-1262-4

R.T.: 7.391 min
Delta R.T.: -0.007 min
Response: 361647
Conc: 81.84 ng/ml




#40 AR-1262-5

R.T.: 8.985 min
Delta R.T.: -0.001 min
Response: 301560
Conc: 117.50 ng/ml

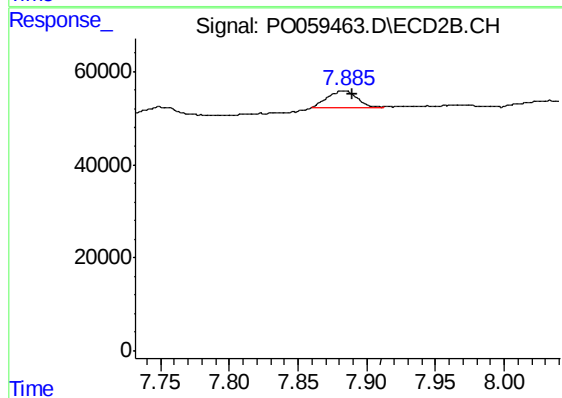

#40 AR-1262-5


R.T.: 7.884 min
Delta R.T.: -0.005 min
Response: 52200
Conc: 28.91 ng/ml



#41 AR-1268-1


R.T.: 8.309 min
Delta R.T.: 0.007 min
Response: 279475
Conc: 29.70 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019




#41 AR-1268-1

R.T.: 7.327 min
Delta R.T.: -0.004 min
Response: 135263
Conc: 19.00 ng/ml




#42 AR-1268-2

R.T.: 8.374 min
Delta R.T.: -0.016 min
Response: 173440
Conc: 22.00 ng/ml

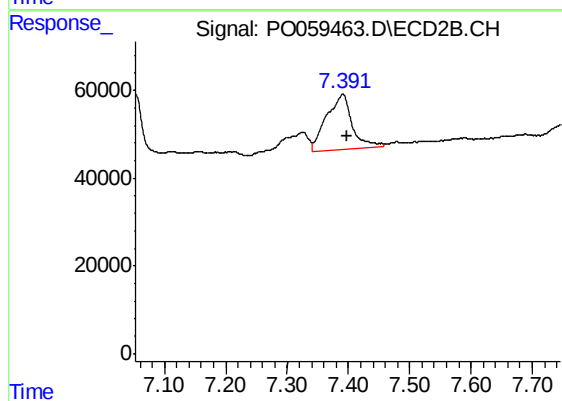

#42 AR-1268-2


R.T.: 7.391 min
Delta R.T.: -0.006 min
Response: 361647
Conc: 56.09 ng/ml



#43 AR-1268-3


R.T.: 8.596 min
Delta R.T.: 0.007 min
Response: 49707
Conc: 7.05 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019




#43 AR-1268-3

R.T.: 7.591 min
Delta R.T.: -0.002 min
Response: 19822
Conc: 3.62 ng/ml




#44 AR-1268-4

R.T.: 8.985 min
Delta R.T.: 0.000 min
Response: 301560
Conc: 108.47 ng/ml

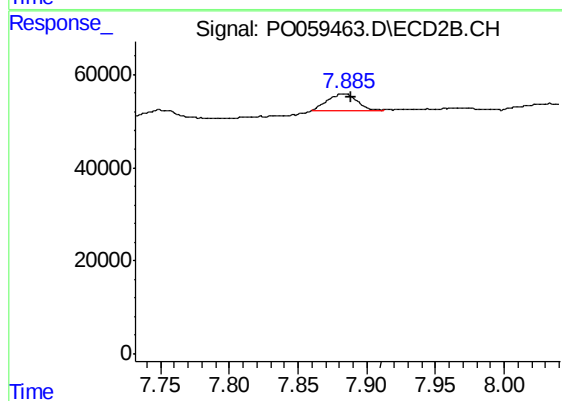

#44 AR-1268-4


R.T.: 7.884 min
Delta R.T.: -0.004 min
Response: 52200
Conc: 25.57 ng/ml

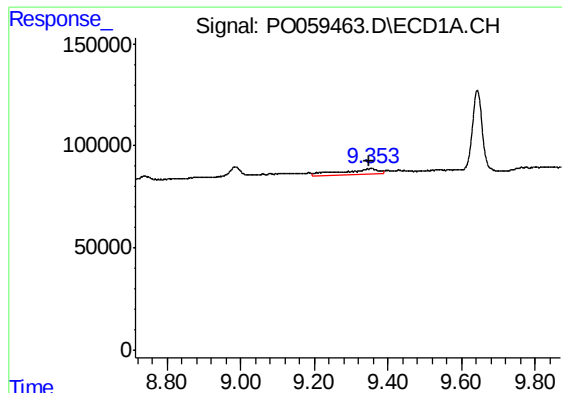

#45 AR-1268-5

R.T.: 9.353 min
Delta R.T.: 0.004 min
Response: 176798
Conc: 9.59 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

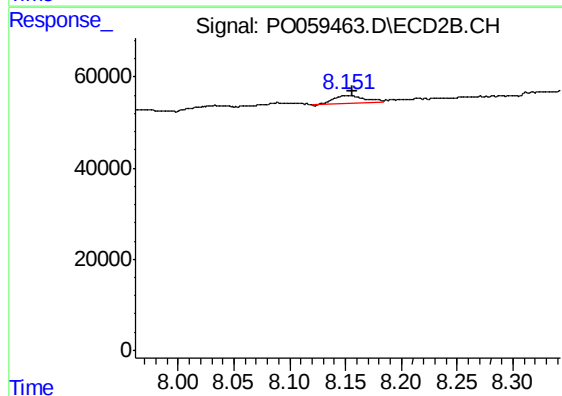

#45 AR-1268-5

R.T.: 8.150 min
Delta R.T.: -0.006 min
Response: 34067
Conc: 2.34 ng/ml