

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081919\
 Data File : P0059464.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Aug 2019 18:35
 Operator : SM/AJ
 Sample : K3591-09
 Misc : AR1221 MDL 25PPB
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-MDL-WATER-03-QT3-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 20 01:06:20 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 17 03:09:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.138	3.505	546667	507536	15.613	14.100
2)	SA Decachlor...	9.627	8.375	891211	625694	16.752	15.518
Target Compounds							
3)	L1 AR-1016-1	5.292	4.572	6558	9752	4.089	7.213 #
4)	L1 AR-1016-2	5.316	4.572	8380	9752	3.503	4.869 #
5)	L1 AR-1016-3	5.372	4.786	8711	6464	5.848	5.975
6)	L1 AR-1016-4	0.000	4.803	0	772	N.D.	0.855 #
8)	L2 AR-1221-1	4.350	3.710	12001	9169	28.339	22.843
9)	L2 AR-1221-2	4.438	3.797	15022	13957	46.250	45.818
10)	L2 AR-1221-3	4.512	3.868	26288	21494	24.992	21.967
11)	L3 AR-1232-1	4.512	3.868	26288	21494	21.091	18.852
12)	L3 AR-1232-2	5.026	4.572	5178	9752	7.331	7.657
13)	L3 AR-1232-3	5.316	4.786	8380	6464	5.472	9.493 #
14)	L3 AR-1232-4	0.000	4.803	0	772	N.D.	1.266 #
15)	L3 AR-1232-5	5.557	0.000	9848	0	16.382	N.D. #
16)	L4 AR-1242-1	5.292	4.572	6558	9752	5.166	9.480 #
17)	L4 AR-1242-2	5.316	4.572	8380	9752	4.516	6.403 #
18)	L4 AR-1242-3	5.372	4.786	8711	6464	7.452	7.737
19)	L4 AR-1242-4	0.000	4.803	0	772	N.D.	0.925 #
20)	L4 AR-1242-5	6.271	5.362	22018	24668	17.522	22.052 #
21)	L5 AR-1248-1	5.292	4.572	6558	9752	6.541	11.777 #
22)	L5 AR-1248-2	5.557	4.786	9848	6464	6.787	5.606
23)	L5 AR-1248-3	0.000	4.803	0	772	N.D.	0.650 #
24)	L5 AR-1248-4	6.137	0.000	102654	0	50.219	N.D. #
25)	L5 AR-1248-5	6.271	5.362	22018	24668	11.103	17.235 #
26)	L6 AR-1254-1	6.137	5.334	102654	9539	49.201	4.022 #
27)	L6 AR-1254-2	6.394	5.465	9396	9928	2.816	4.731 #
28)	L6 AR-1254-3	6.710	5.888	19162	25292	5.400	7.522 #
29)	L6 AR-1254-4	7.065	6.131	38598	6085	13.104	2.951 #
30)	L6 AR-1254-5	7.409	6.515	14595	21290	4.720	6.857 #
31)	L7 AR-1260-1	6.902	5.999	20935	31257	7.766	13.716 #
32)	L7 AR-1260-2	7.128	6.194	14914	34067	4.019	11.627 #
33)	L7 AR-1260-3	7.483	6.341	13549	19847	4.135	7.492 #
34)	L7 AR-1260-4	7.705	6.802	31751	20826	10.338	9.205
35)	L7 AR-1260-5	8.012	7.047	155186	71172	21.916	12.933 #
36)	L8 AR-1262-1	7.483	6.541	13549	16813	2.792	4.511 #
37)	L8 AR-1262-2	8.012	7.047	155186	71172	20.113	12.106 #
38)	L8 AR-1262-3	8.315	7.321	44665	15872	8.754	6.247 #
39)	L8 AR-1262-4	8.393	7.387	6248	49269	1.621	11.150 #
40)	L8 AR-1262-5	8.975	7.881	104365	11324	40.664	6.272 #
41)	L9 AR-1268-1	8.315	7.321	44665	15872	4.746	2.229 #
42)	L9 AR-1268-2	8.393	7.387	6248	49269	0.793	7.641 #
43)	L9 AR-1268-3	8.583	7.586	26107	9813	3.704	1.793 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081919\
 Data File : P0059464.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Aug 2019 18:35
 Operator : SM/AJ
 Sample : K3591-09
 Misc : AR1221 MDL 25PPB
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-MDL-WATER-03-QT3-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 20 01:06:20 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 17 03:09:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
44) L9	AR-1268-4	8.975	7.881	104365	11324	37.541	5.547 #
45) L9	AR-1268-5	9.341	8.152	77214	10621	4.187	0.731 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081919\
Data File : PO059464.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Aug 2019 18:35
Operator : SM/AJ
Sample : K3591-09
Misc : AR1221 MDL 25PPB
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 20 01:06:20 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Aug 17 03:09:44 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

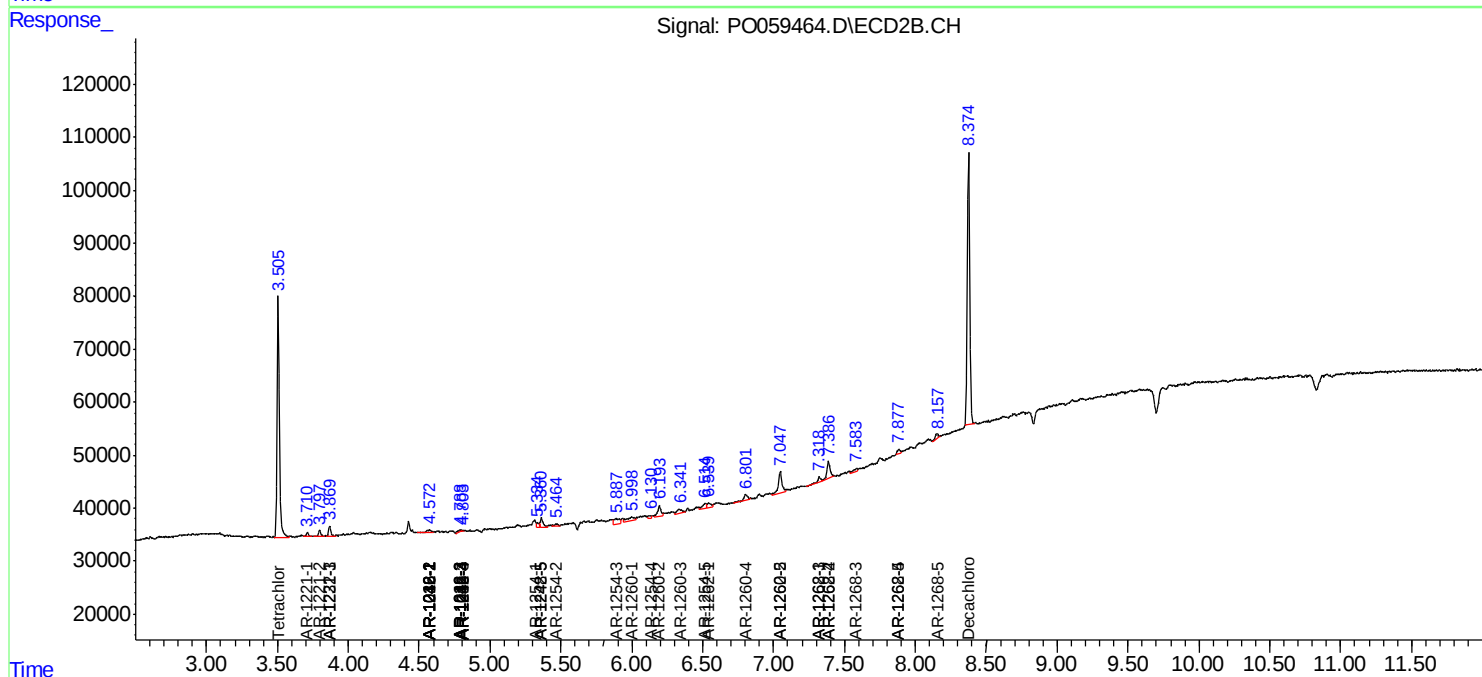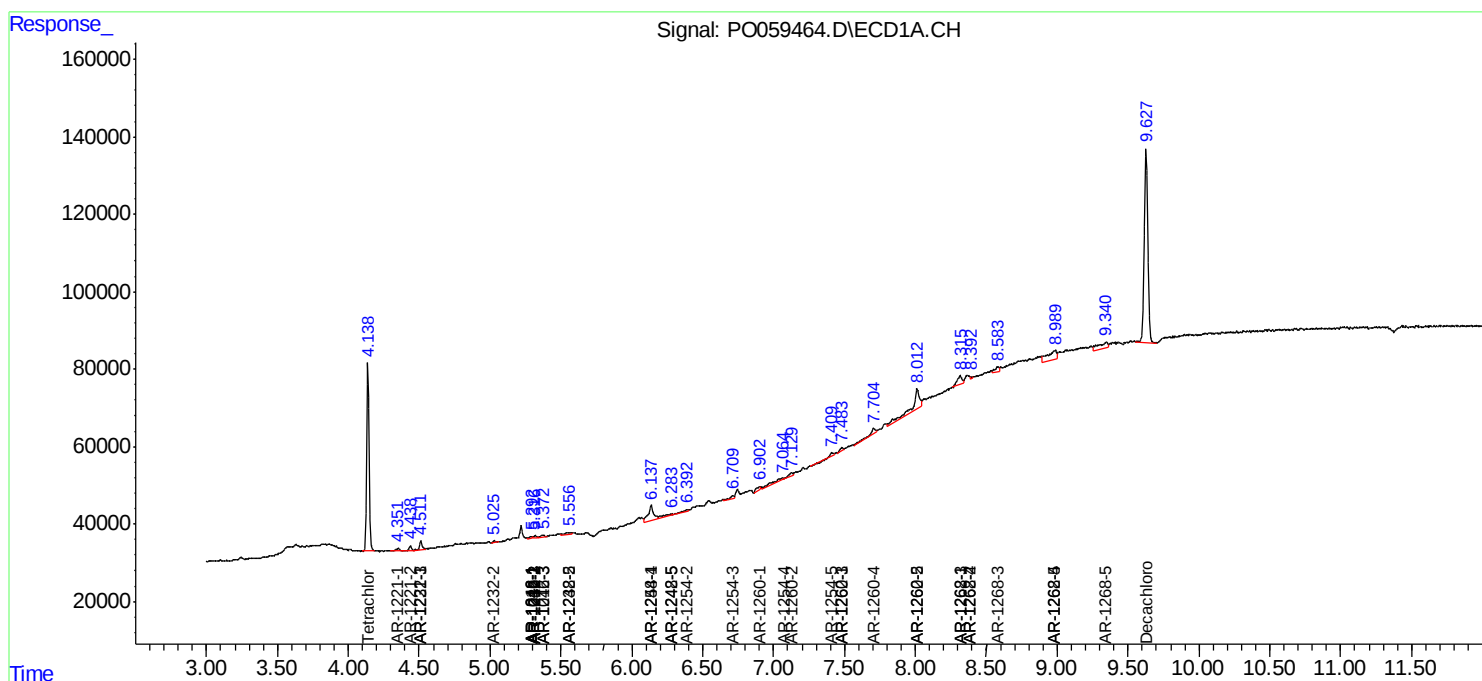


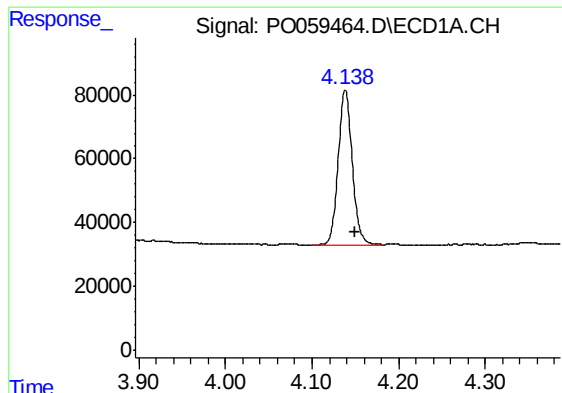

#1 Tetrachloro-m-xylene


R.T.: 4.138 min
Delta R.T.: -0.011 min
Response: 546667
Conc: 15.61 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019




#1 Tetrachloro-m-xylene

R.T.: 3.505 min
Delta R.T.: -0.005 min
Response: 507536
Conc: 14.10 ng/ml

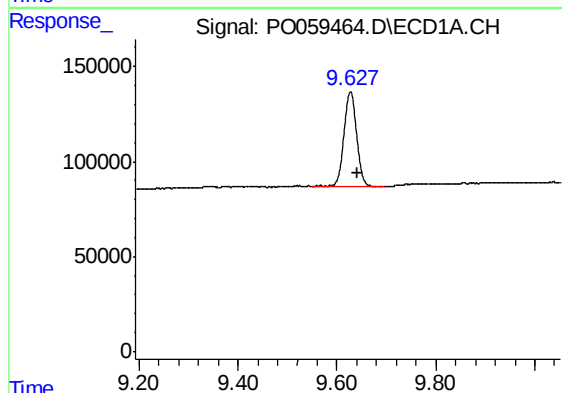


#2 Decachlorobiphenyl

R.T.: 9.627 min
Delta R.T.: -0.013 min
Response: 891211
Conc: 16.75 ng/ml

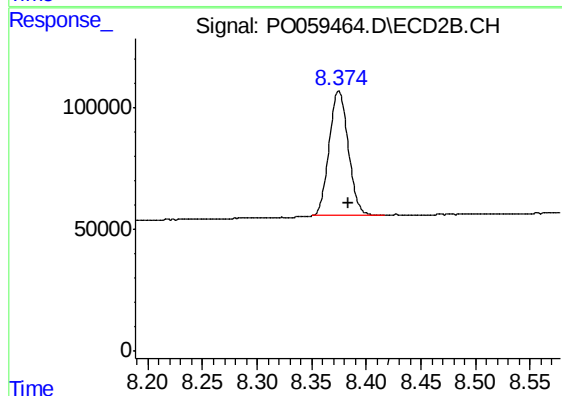

#2 Decachlorobiphenyl


R.T.: 8.375 min
Delta R.T.: -0.008 min
Response: 625694
Conc: 15.52 ng/ml

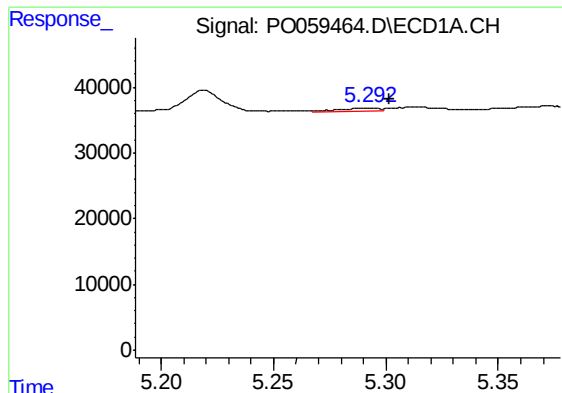

#3 AR-1016-1


R.T.: 5.292 min
Delta R.T.: -0.010 min
Response: 6558
Conc: 4.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

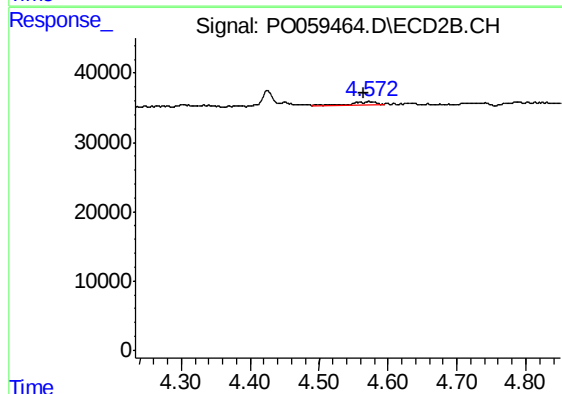


#3 AR-1016-1

R.T.: 4.572 min
Delta R.T.: 0.008 min
Response: 9752
Conc: 7.21 ng/ml

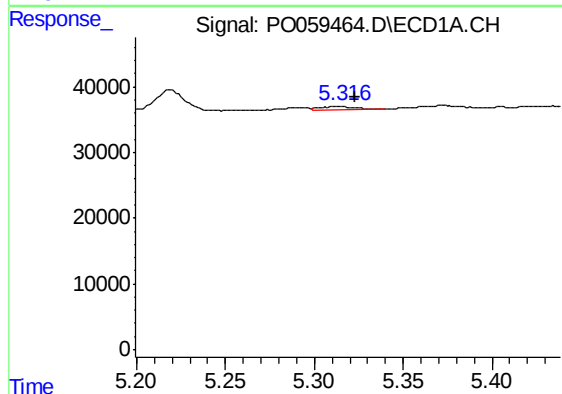


#4 AR-1016-2

R.T.: 5.316 min
Delta R.T.: -0.007 min
Response: 8380
Conc: 3.50 ng/ml

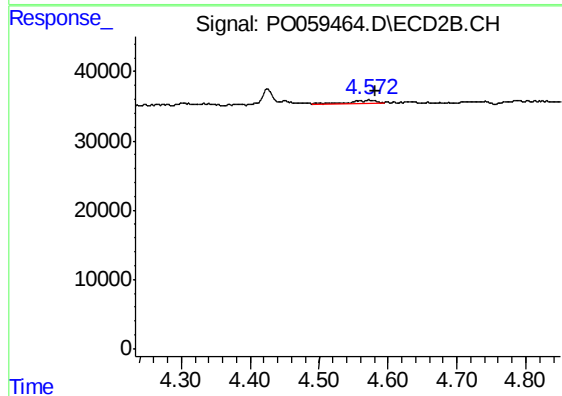

#4 AR-1016-2


R.T.: 4.572 min
Delta R.T.: -0.009 min
Response: 9752
Conc: 4.87 ng/ml

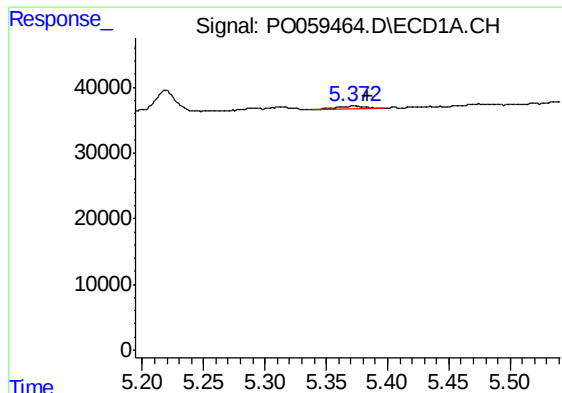

#5 AR-1016-3


R.T.: 5.372 min
Delta R.T.: -0.011 min
Response: 8711
Conc: 5.85 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

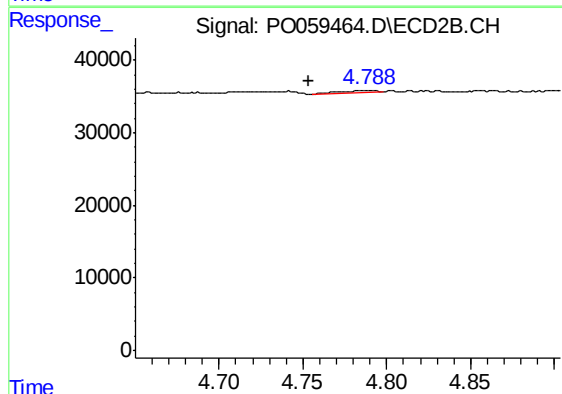


#5 AR-1016-3

R.T.: 4.786 min
Delta R.T.: 0.032 min
Response: 6464
Conc: 5.98 ng/ml

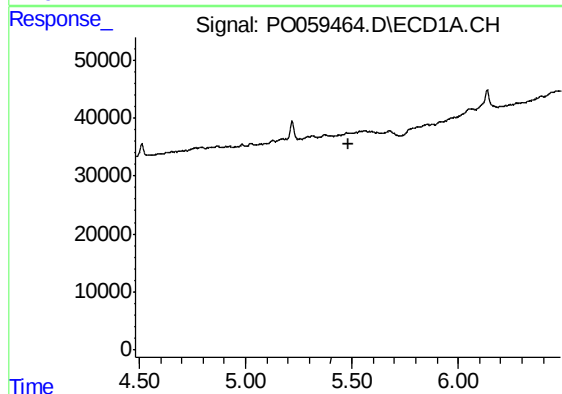


#6 AR-1016-4

R.T.: 0.000 min
Exp R.T. : 5.481 min
Response: 0
Conc: N.D.

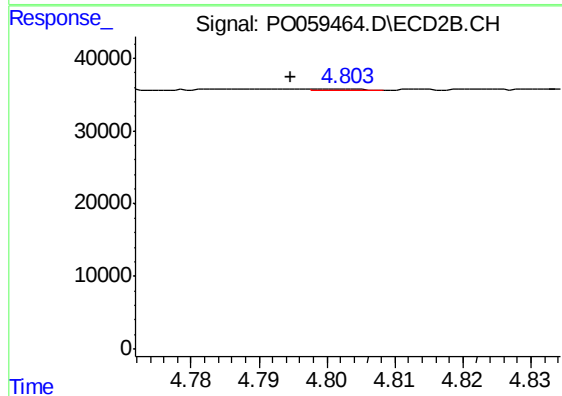

#6 AR-1016-4


R.T.: 4.803 min
Delta R.T.: 0.008 min
Response: 772
Conc: 0.86 ng/ml

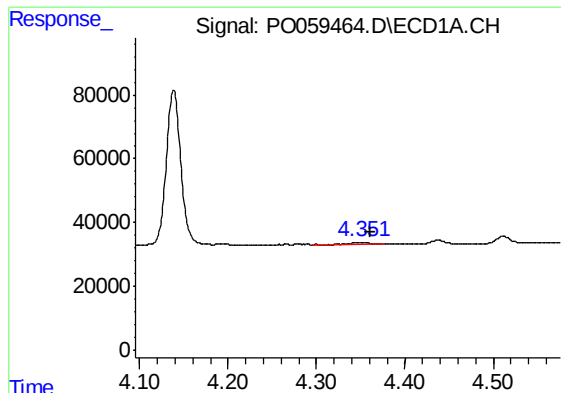

#8 AR-1221-1


R.T.: 4.350 min
Delta R.T.: -0.010 min
Response: 12001
Conc: 28.34 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

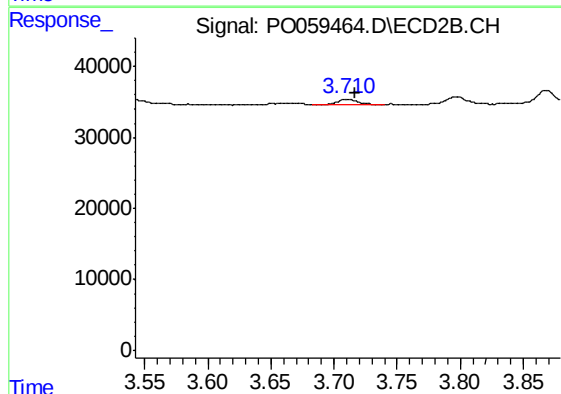


#8 AR-1221-1

R.T.: 3.710 min
Delta R.T.: -0.007 min
Response: 9169
Conc: 22.84 ng/ml

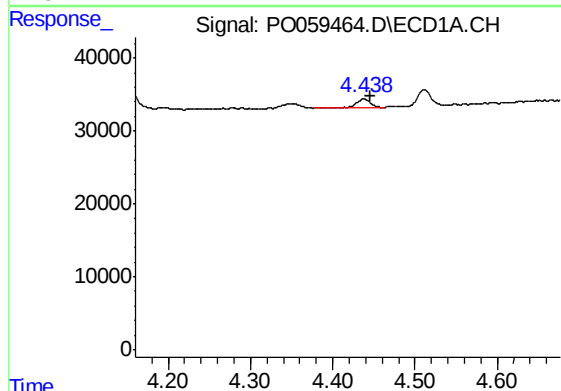


#9 AR-1221-2

R.T.: 4.438 min
Delta R.T.: -0.009 min
Response: 15022
Conc: 46.25 ng/ml

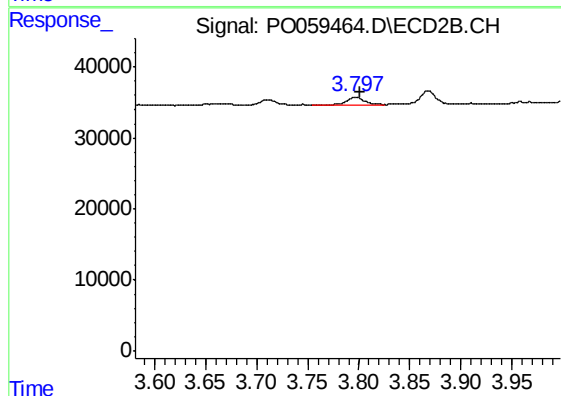

#9 AR-1221-2


R.T.: 3.797 min
Delta R.T.: -0.004 min
Response: 13957
Conc: 45.82 ng/ml

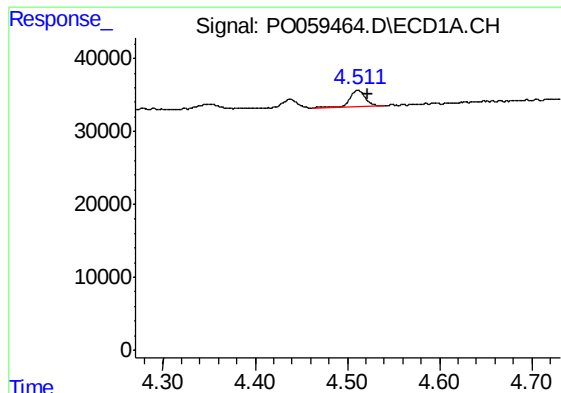

#10 AR-1221-3


R.T.: 4.512 min
Delta R.T.: -0.010 min
Response: 26288
Conc: 24.99 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

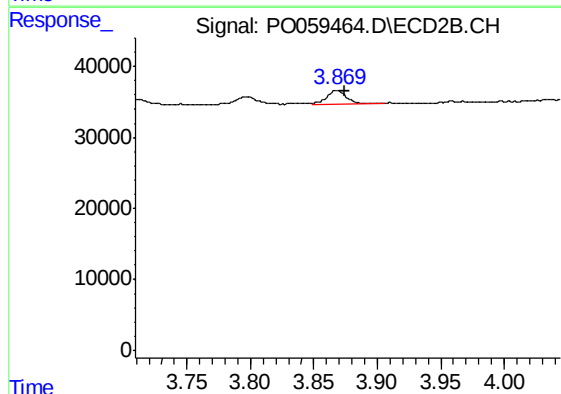


#10 AR-1221-3

R.T.: 3.868 min
Delta R.T.: -0.006 min
Response: 21494
Conc: 21.97 ng/ml

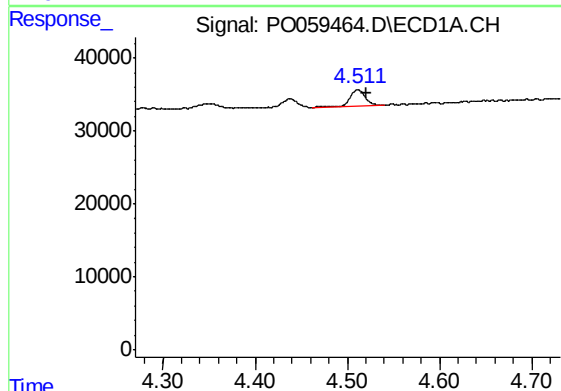


#11 AR-1232-1

R.T.: 4.512 min
Delta R.T.: -0.010 min
Response: 26288
Conc: 21.09 ng/ml

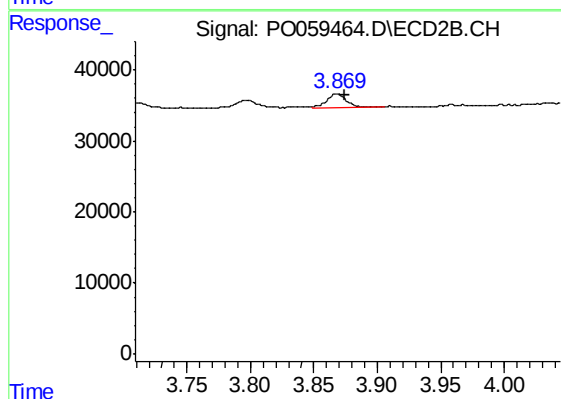

#11 AR-1232-1


R.T.: 3.868 min
Delta R.T.: -0.006 min
Response: 21494
Conc: 18.85 ng/ml

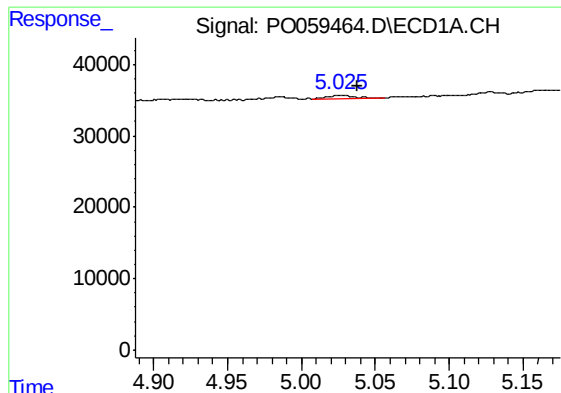

#12 AR-1232-2


R.T.: 5.026 min
Delta R.T.: -0.012 min
Response: 5178
Conc: 7.33 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

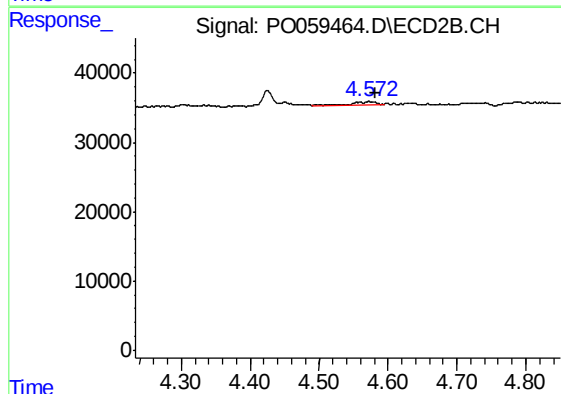


#12 AR-1232-2

R.T.: 4.572 min
Delta R.T.: -0.009 min
Response: 9752
Conc: 7.66 ng/ml

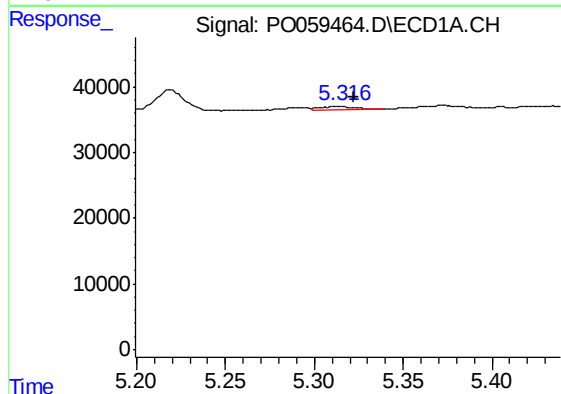


#13 AR-1232-3

R.T.: 5.316 min
Delta R.T.: -0.006 min
Response: 8380
Conc: 5.47 ng/ml

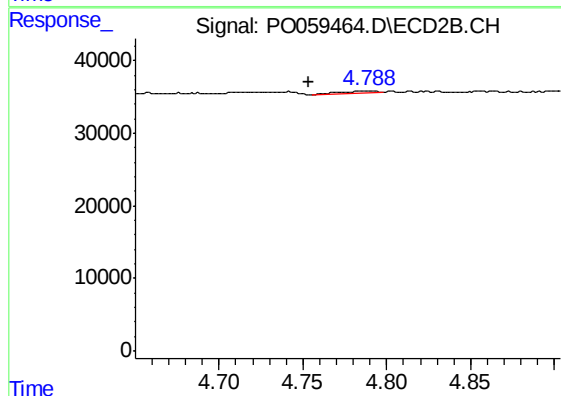

#13 AR-1232-3


R.T.: 4.786 min
Delta R.T.: 0.033 min
Response: 6464
Conc: 9.49 ng/ml

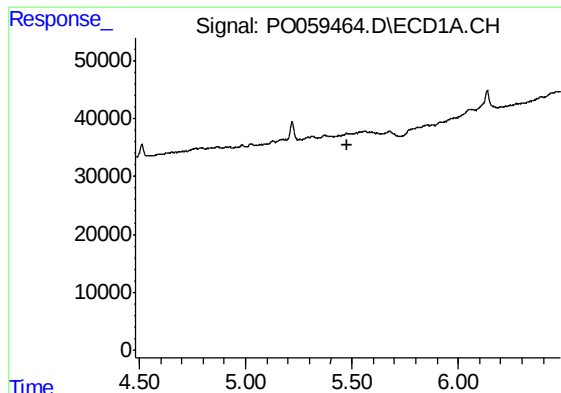

#14 AR-1232-4


R.T.: 0.000 min
Exp R.T. : 5.481 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

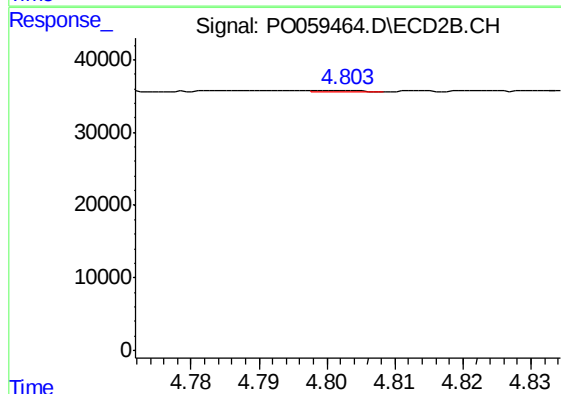


#14 AR-1232-4

R.T.: 4.803 min
Delta R.T.: -0.032 min
Response: 772
Conc: 1.27 ng/ml

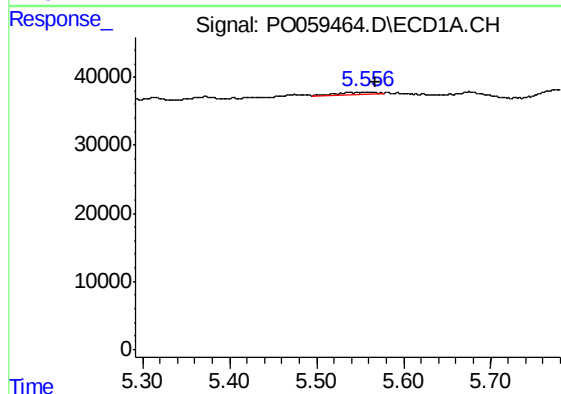


#15 AR-1232-5

R.T.: 5.557 min
Delta R.T.: -0.011 min
Response: 9848
Conc: 16.38 ng/ml

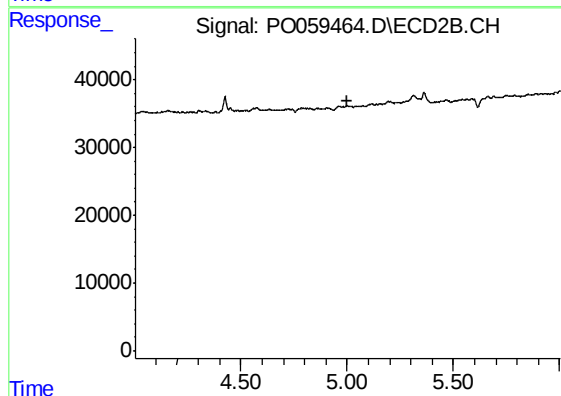

#15 AR-1232-5


R.T.: 0.000 min
Exp R.T. : 5.004 min
Response: 0
Conc: N.D.

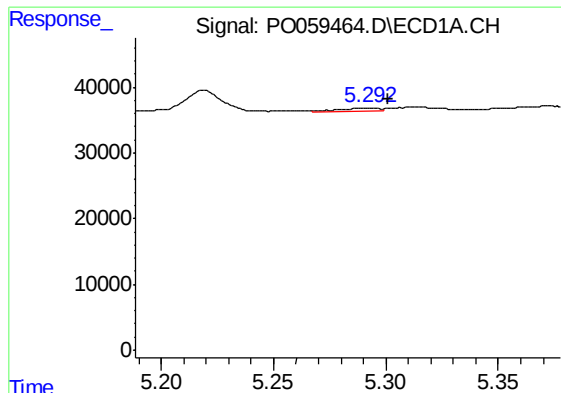

#16 AR-1242-1


R.T.: 5.292 min
Delta R.T.: -0.009 min
Response: 6558
Conc: 5.17 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

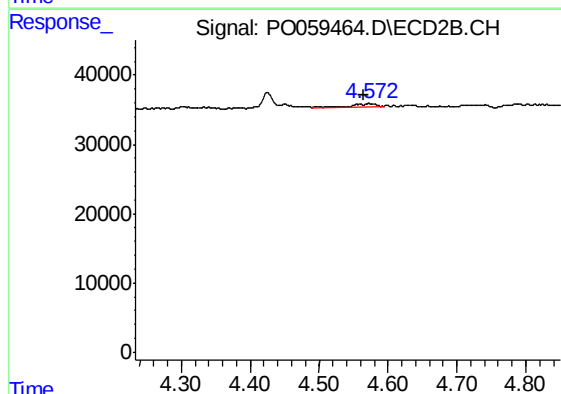


#16 AR-1242-1

R.T.: 4.572 min
Delta R.T.: 0.008 min
Response: 9752
Conc: 9.48 ng/ml

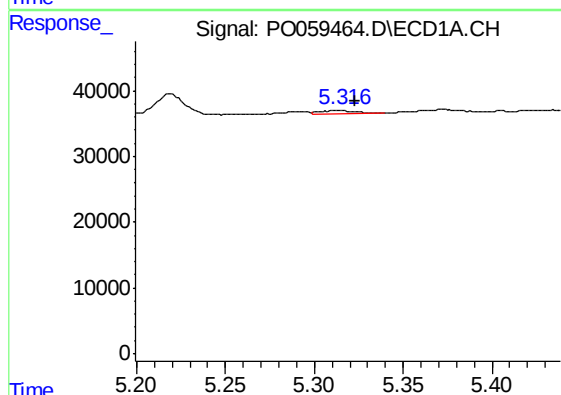


#17 AR-1242-2

R.T.: 5.316 min
Delta R.T.: -0.007 min
Response: 8380
Conc: 4.52 ng/ml

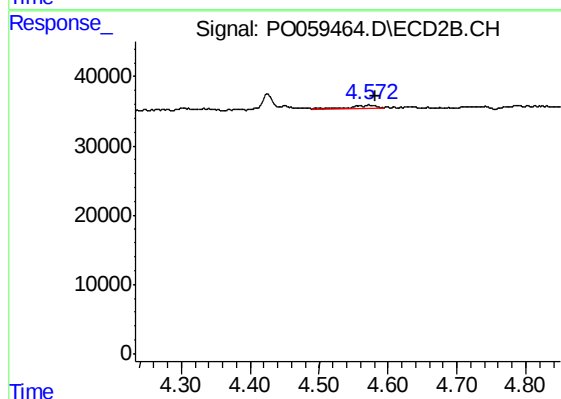

#17 AR-1242-2


R.T.: 4.572 min
Delta R.T.: -0.009 min
Response: 9752
Conc: 6.40 ng/ml



#18 AR-1242-3


R.T.: 5.372 min
Delta R.T.: -0.011 min
Response: 8711
Conc: 7.45 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019




#18 AR-1242-3

R.T.: 4.786 min
Delta R.T.: 0.033 min
Response: 6464
Conc: 7.74 ng/ml




#19 AR-1242-4

R.T.: 0.000 min
Exp R.T. : 5.482 min
Response: 0
Conc: N.D.



#19 AR-1242-4


R.T.: 4.803 min
Delta R.T.: -0.031 min
Response: 772
Conc: 0.93 ng/ml

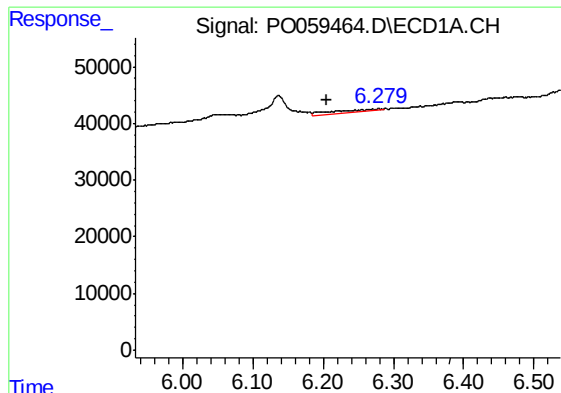

#20 AR-1242-5


R.T.: 6.271 min
Delta R.T.: 0.065 min
Response: 22018
Conc: 17.52 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

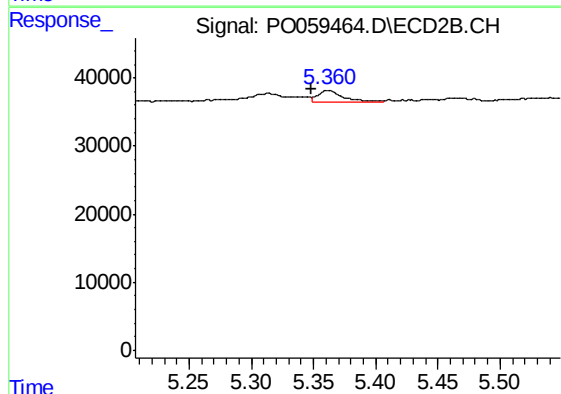


#20 AR-1242-5

R.T.: 5.362 min
Delta R.T.: 0.014 min
Response: 24668
Conc: 22.05 ng/ml

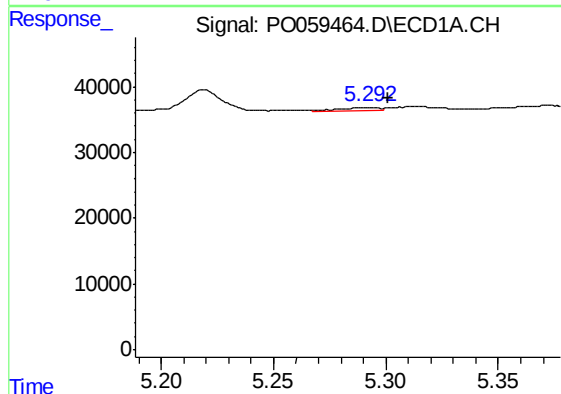


#21 AR-1248-1

R.T.: 5.292 min
Delta R.T.: -0.009 min
Response: 6558
Conc: 6.54 ng/ml

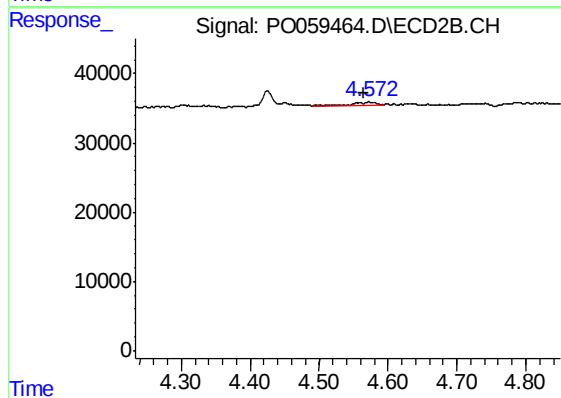

#21 AR-1248-1


R.T.: 4.572 min
Delta R.T.: 0.008 min
Response: 9752
Conc: 11.78 ng/ml

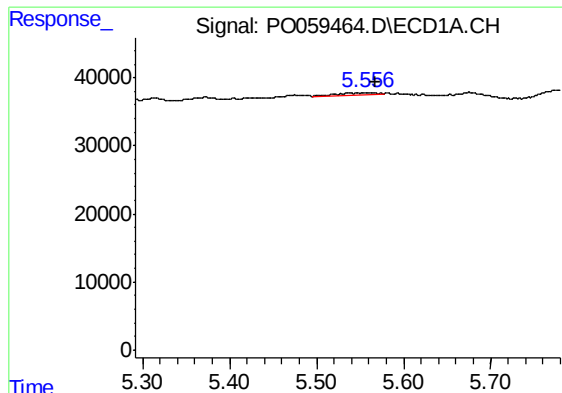

#22 AR-1248-2


R.T.: 5.557 min
Delta R.T.: -0.010 min
Response: 9848
Conc: 6.79 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019




#22 AR-1248-2

R.T.: 4.786 min
Delta R.T.: -0.008 min
Response: 6464
Conc: 5.61 ng/ml




#23 AR-1248-3

R.T.: 0.000 min
Exp R.T. : 5.768 min
Response: 0
Conc: N.D.

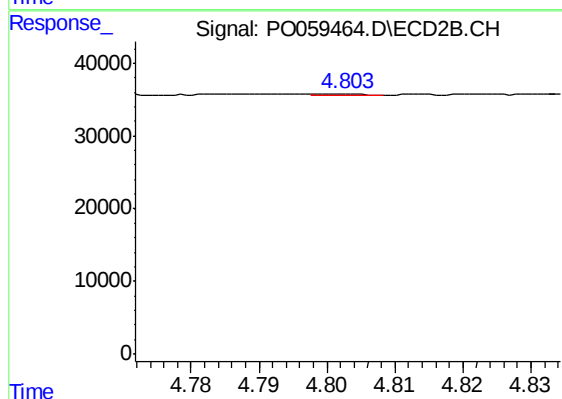

#23 AR-1248-3


R.T.: 4.803 min
Delta R.T.: -0.032 min
Response: 772
Conc: 0.65 ng/ml



#24 AR-1248-4


R.T.: 6.137 min
Delta R.T.: -0.032 min
Response: 102654
Conc: 50.22 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019




#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 5.003 min
Response: 0
Conc: N.D.




#25 AR-1248-5

R.T.: 6.271 min
Delta R.T.: 0.066 min
Response: 22018
Conc: 11.10 ng/ml

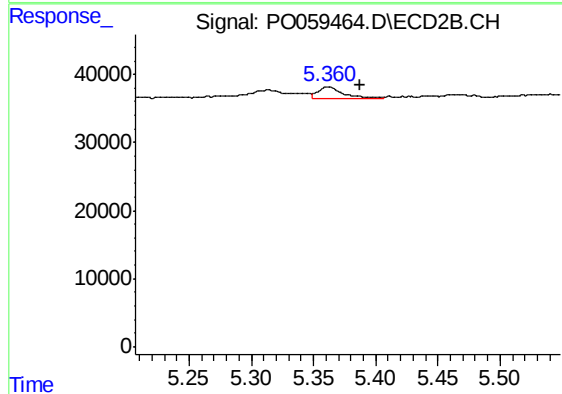

#25 AR-1248-5


R.T.: 5.362 min
Delta R.T.: -0.025 min
Response: 24668
Conc: 17.23 ng/ml

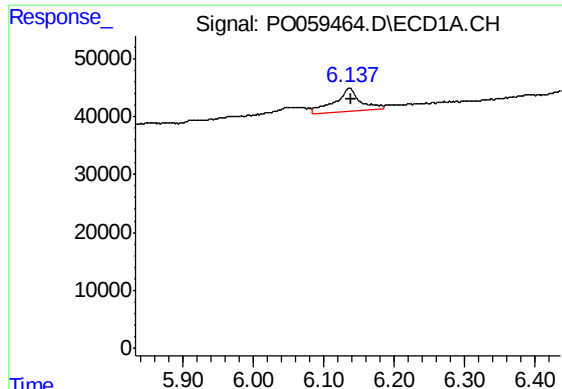

#26 AR-1254-1


R.T.: 6.137 min
Delta R.T.: -0.003 min
Response: 102654
Conc: 49.20 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019




#26 AR-1254-1

R.T.: 5.334 min
Delta R.T.: -0.013 min
Response: 9539
Conc: 4.02 ng/ml




#27 AR-1254-2

R.T.: 6.394 min
Delta R.T.: 0.039 min
Response: 9396
Conc: 2.82 ng/ml

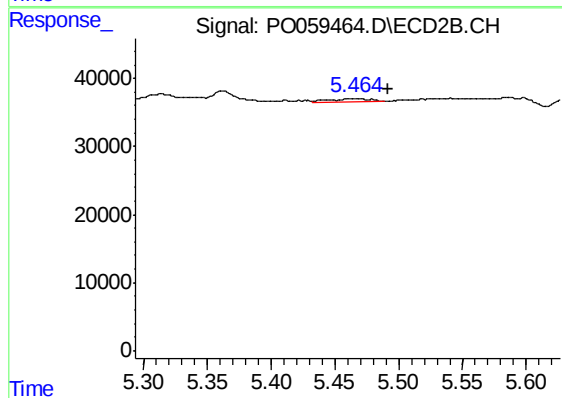

#27 AR-1254-2


R.T.: 5.465 min
Delta R.T.: -0.027 min
Response: 9928
Conc: 4.73 ng/ml

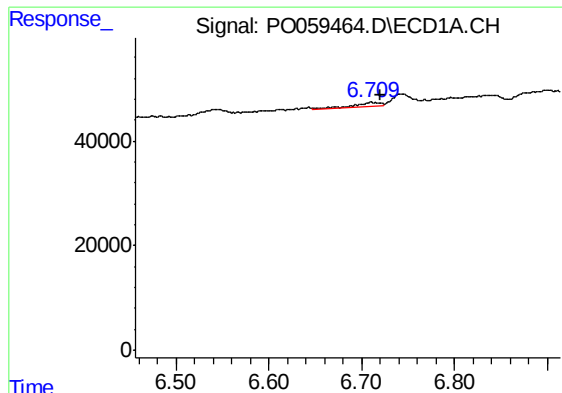

#28 AR-1254-3


R.T.: 6.710 min
Delta R.T.: -0.010 min
Response: 19162
Conc: 5.40 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

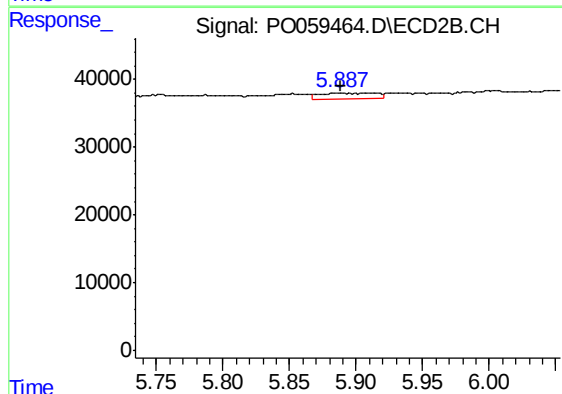


#28 AR-1254-3

R.T.: 5.888 min
Delta R.T.: -0.001 min
Response: 25292
Conc: 7.52 ng/ml




#29 AR-1254-4

R.T.: 7.065 min
Delta R.T.: 0.060 min
Response: 38598
Conc: 13.10 ng/ml

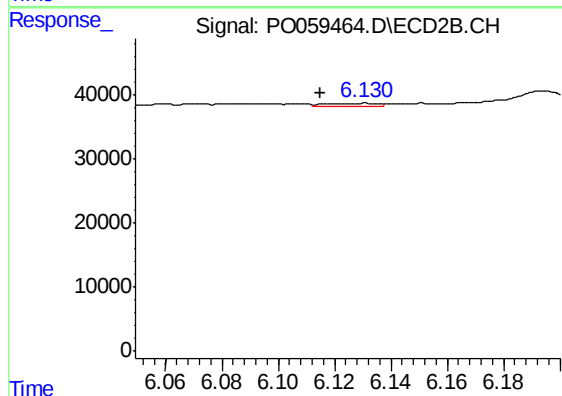

#29 AR-1254-4


R.T.: 6.131 min
Delta R.T.: 0.016 min
Response: 6085
Conc: 2.95 ng/ml



#30 AR-1254-5


R.T.: 7.409 min
Delta R.T.: -0.010 min
Response: 14595
Conc: 4.72 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019




#30 AR-1254-5

R.T.: 6.515 min
Delta R.T.: -0.009 min
Response: 21290
Conc: 6.86 ng/ml




#31 AR-1260-1

R.T.: 6.902 min
Delta R.T.: 0.022 min
Response: 20935
Conc: 7.77 ng/ml

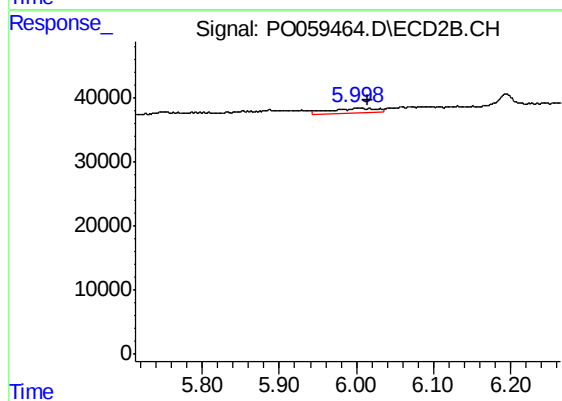

#31 AR-1260-1


R.T.: 5.999 min
Delta R.T.: -0.015 min
Response: 31257
Conc: 13.72 ng/ml



#32 AR-1260-2


R.T.: 7.128 min
Delta R.T.: -0.007 min
Response: 14914
Conc: 4.02 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019




#32 AR-1260-2

R.T.: 6.194 min
Delta R.T.: -0.008 min
Response: 34067
Conc: 11.63 ng/ml




#33 AR-1260-3

R.T.: 7.483 min
Delta R.T.: -0.007 min
Response: 13549
Conc: 4.14 ng/ml

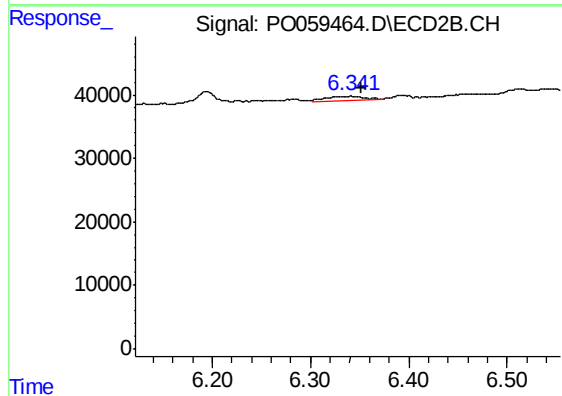

#33 AR-1260-3


R.T.: 6.341 min
Delta R.T.: -0.010 min
Response: 19847
Conc: 7.49 ng/ml

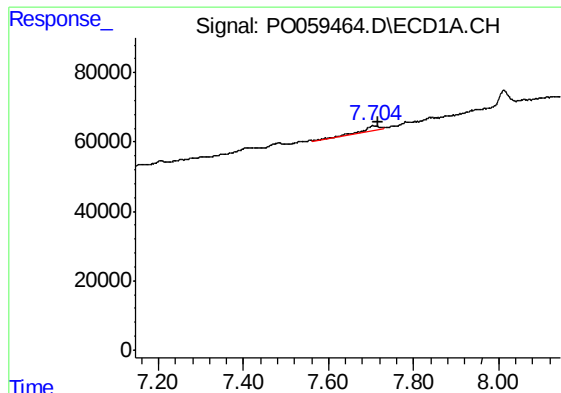

#34 AR-1260-4


R.T.: 7.705 min
Delta R.T.: -0.012 min
Response: 31751
Conc: 10.34 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

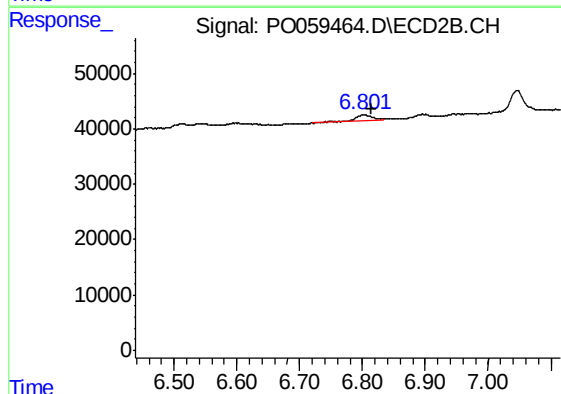


#34 AR-1260-4

R.T.: 6.802 min
Delta R.T.: -0.012 min
Response: 20826
Conc: 9.20 ng/ml

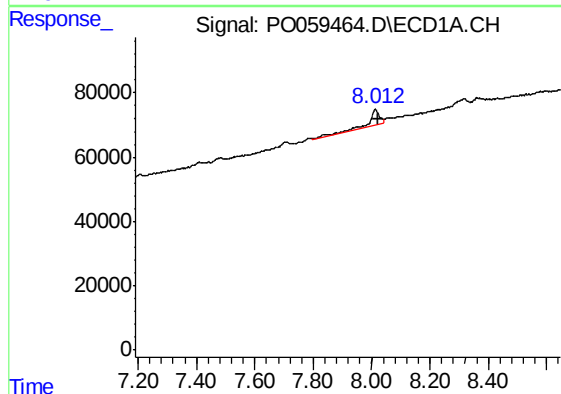


#35 AR-1260-5

R.T.: 8.012 min
Delta R.T.: -0.012 min
Response: 155186
Conc: 21.92 ng/ml

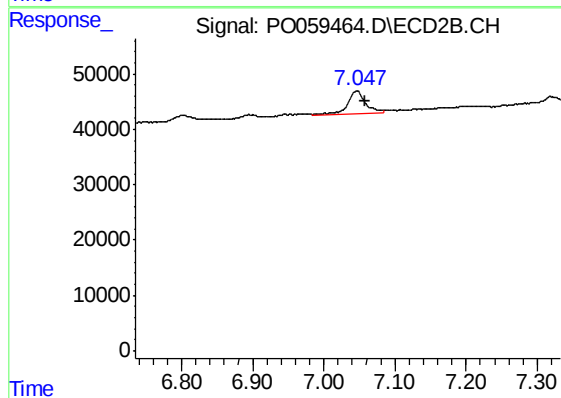

#35 AR-1260-5


R.T.: 7.047 min
Delta R.T.: -0.011 min
Response: 71172
Conc: 12.93 ng/ml

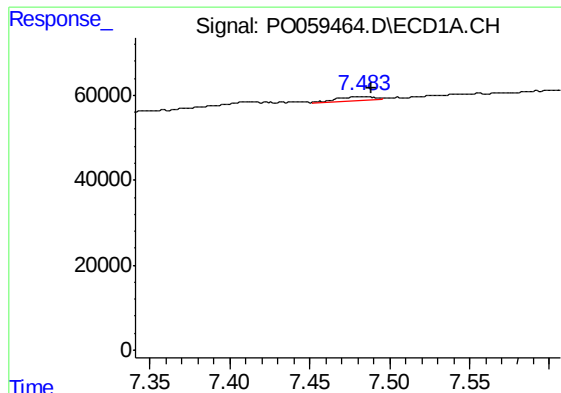

#36 AR-1262-1


R.T.: 7.483 min
Delta R.T.: -0.006 min
Response: 13549
Conc: 2.79 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

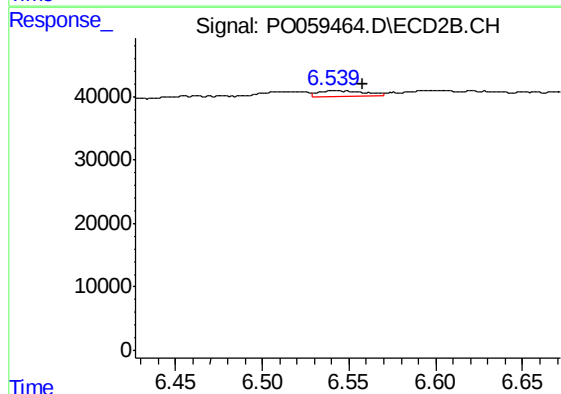


#36 AR-1262-1

R.T.: 6.541 min
Delta R.T.: -0.017 min
Response: 16813
Conc: 4.51 ng/ml

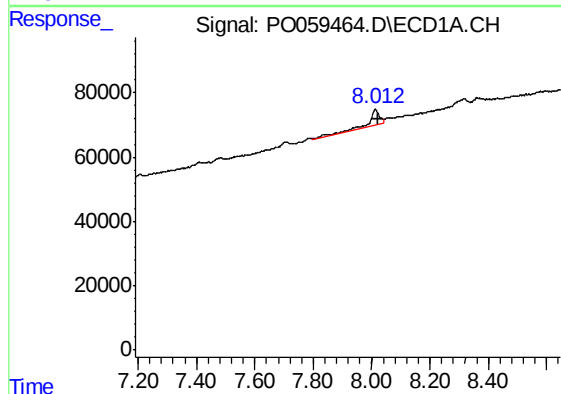


#37 AR-1262-2

R.T.: 8.012 min
Delta R.T.: -0.011 min
Response: 155186
Conc: 20.11 ng/ml

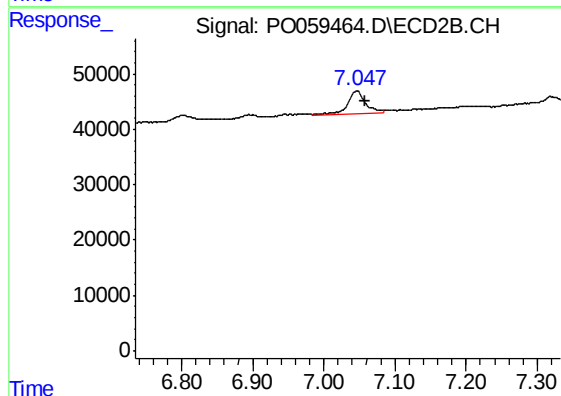

#37 AR-1262-2


R.T.: 7.047 min
Delta R.T.: -0.011 min
Response: 71172
Conc: 12.11 ng/ml



#38 AR-1262-3


R.T.: 8.315 min
Delta R.T.: 0.012 min
Response: 44665
Conc: 8.75 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019




#38 AR-1262-3

R.T.: 7.321 min
Delta R.T.: -0.011 min
Response: 15872
Conc: 6.25 ng/ml




#39 AR-1262-4

R.T.: 8.393 min
Delta R.T.: 0.006 min
Response: 6248
Conc: 1.62 ng/ml

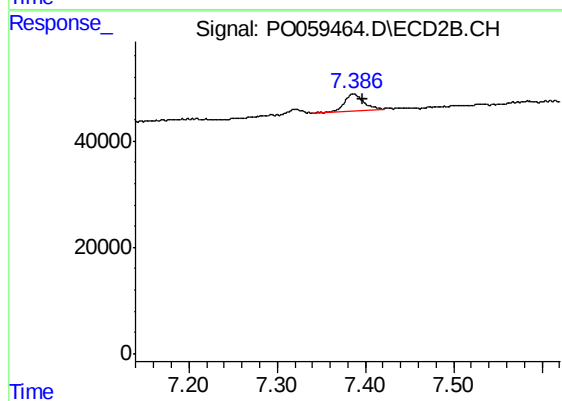

#39 AR-1262-4


R.T.: 7.387 min
Delta R.T.: -0.011 min
Response: 49269
Conc: 11.15 ng/ml

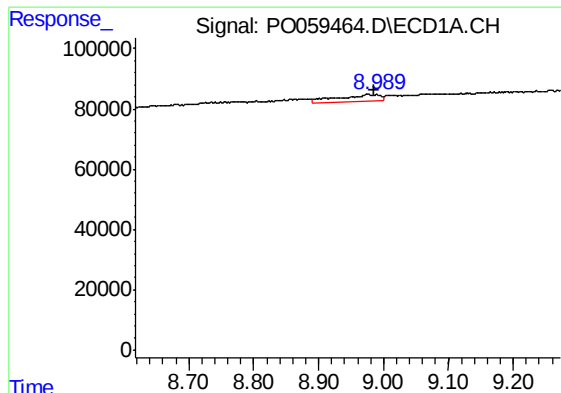

#40 AR-1262-5


R.T.: 8.975 min
Delta R.T.: -0.011 min
Response: 104365
Conc: 40.66 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

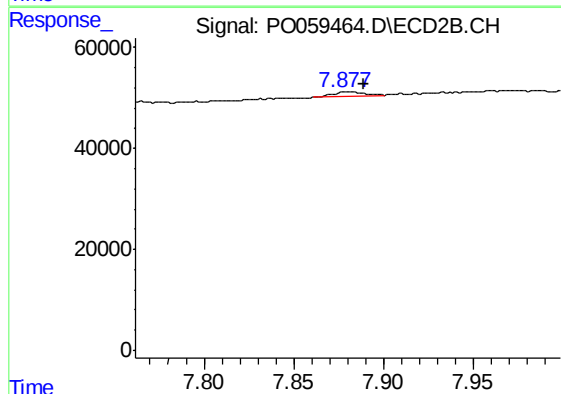


#40 AR-1262-5

R.T.: 7.881 min
Delta R.T.: -0.009 min
Response: 11324
Conc: 6.27 ng/ml

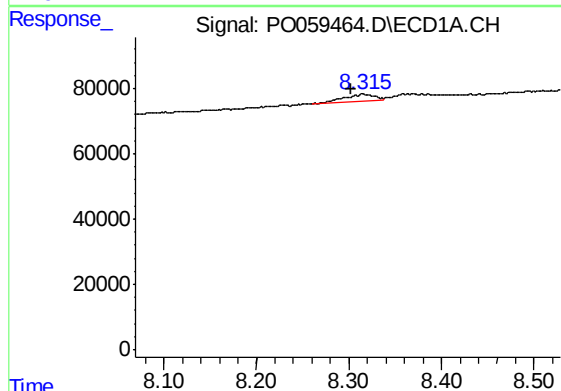


#41 AR-1268-1

R.T.: 8.315 min
Delta R.T.: 0.013 min
Response: 44665
Conc: 4.75 ng/ml

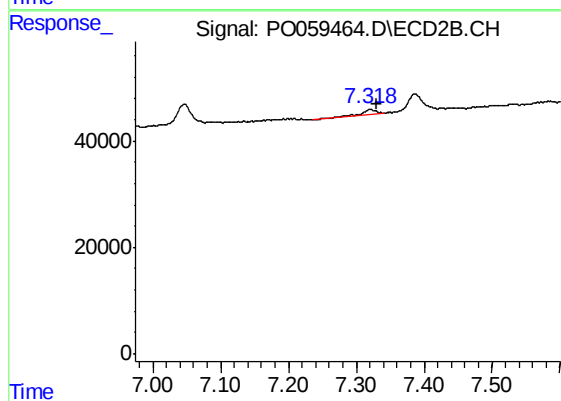

#41 AR-1268-1


R.T.: 7.321 min
Delta R.T.: -0.009 min
Response: 15872
Conc: 2.23 ng/ml

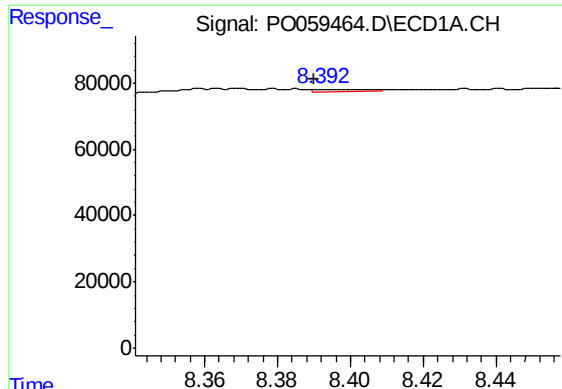

#42 AR-1268-2


R.T.: 8.393 min
Delta R.T.: 0.003 min
Response: 6248
Conc: 0.79 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019




#42 AR-1268-2

R.T.: 7.387 min
Delta R.T.: -0.011 min
Response: 49269
Conc: 7.64 ng/ml




#43 AR-1268-3

R.T.: 8.583 min
Delta R.T.: -0.005 min
Response: 26107
Conc: 3.70 ng/ml

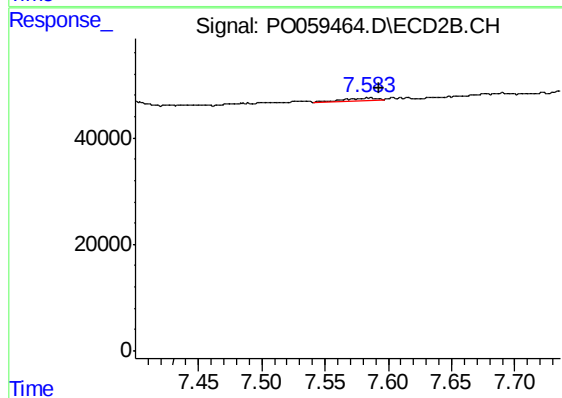

#43 AR-1268-3


R.T.: 7.586 min
Delta R.T.: -0.006 min
Response: 9813
Conc: 1.79 ng/ml

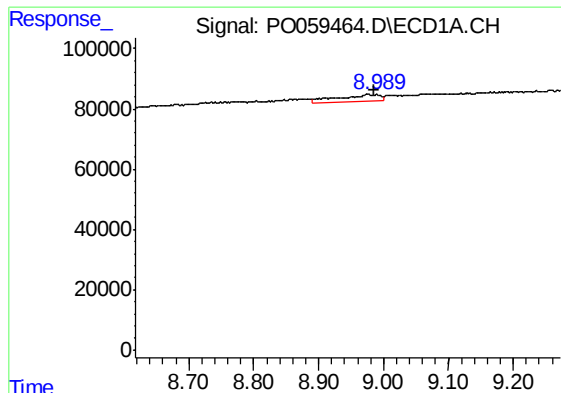

#44 AR-1268-4


R.T.: 8.975 min
Delta R.T.: -0.011 min
Response: 104365
Conc: 37.54 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

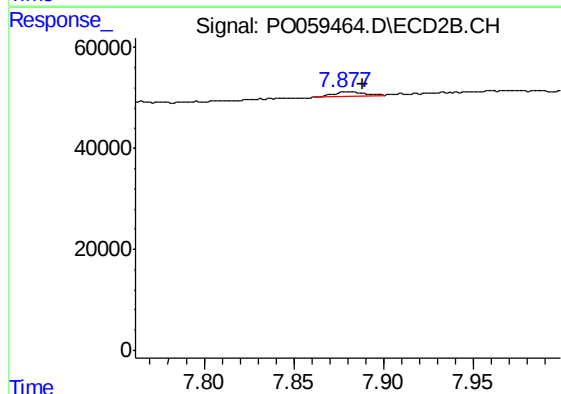


#44 AR-1268-4

R.T.: 7.881 min
Delta R.T.: -0.008 min
Response: 11324
Conc: 5.55 ng/ml

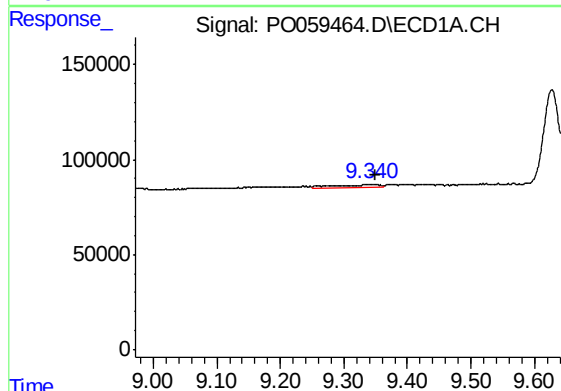

#45 AR-1268-5

R.T.: 9.341 min
Delta R.T.: -0.009 min
Response: 77214
Conc: 4.19 ng/ml

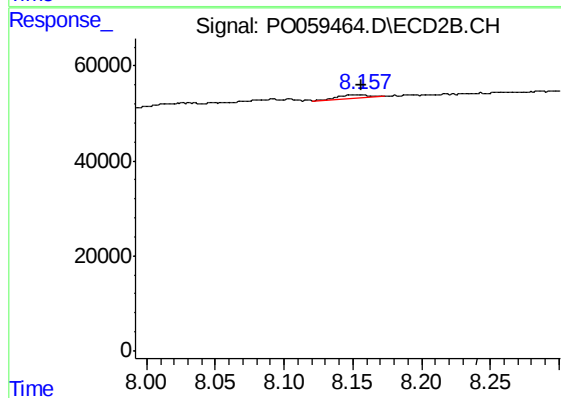

#45 AR-1268-5

R.T.: 8.152 min
Delta R.T.: -0.005 min
Response: 10621
Conc: 0.73 ng/ml