

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081919\
 Data File : P0059465.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Aug 2019 18:52
 Operator : SM/AJ
 Sample : K3591-09
 Misc : AR1232 MDL 25PPB
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-MDL-WATER-03-QT3-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 20 01:07:05 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 17 03:09:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.141	3.505	595433	558393	17.006	15.513
2)	SA Decachlor...	9.627	8.375	937358	685935	17.619	17.012
Target Compounds							
3)	L1 AR-1016-1	5.293	4.557	31547	46043	19.669	34.057 #
4)	L1 AR-1016-2	5.314	4.574	41651	50351	17.409	25.138 #
5)	L1 AR-1016-3	5.374	4.742	29153	31047	19.572	28.698 #
6)	L1 AR-1016-4	5.474	4.787	19750	44671	16.326	49.470 #
7)	L1 AR-1016-5	5.762	4.997	27702	16646	21.572	14.451 #
8)	L2 AR-1221-1	4.351	3.711	9510	9022	22.458	22.478
9)	L2 AR-1221-2	4.439	3.797	16051	16050	49.419	52.688
10)	L2 AR-1221-3	4.514	3.868	35302	31272	33.561	31.960
11)	L3 AR-1232-1	4.514	3.868	35302	31272	28.322	27.428
12)	L3 AR-1232-2	5.028	4.574	21191	50351	29.998	39.535 #
13)	L3 AR-1232-3	5.314	4.742	41651	31047	27.199	45.596 #
14)	L3 AR-1232-4	5.474	4.828	19750	44123	25.260	72.326 #
15)	L3 AR-1232-5	5.560	4.997	19561	16646	32.540	24.453
16)	L4 AR-1242-1	5.293	4.557	31547	46043	24.849	44.761 #
17)	L4 AR-1242-2	5.314	4.574	41651	50351	22.446	33.058 #
18)	L4 AR-1242-3	5.374	4.742	29153	31047	24.942	37.159 #
19)	L4 AR-1242-4	5.474	4.828	19750	44123	20.405	52.881 #
20)	L4 AR-1242-5	6.198	5.340	50476	31820	40.168	28.446 #
21)	L5 AR-1248-1	5.293	4.557	31547	46043	31.466	55.606 #
22)	L5 AR-1248-2	5.560	4.787	19561	44671	13.482	38.739 #
23)	L5 AR-1248-3	5.762	4.828	27702	44123	16.667	37.148 #
24)	L5 AR-1248-4	6.198	4.997	50476	16646	24.693	11.456 #
25)	L5 AR-1248-5	6.198	5.363	50476	140500	25.453	98.163 #
26)	L6 AR-1254-1	6.138	5.340	255945	31820	122.672	13.416 #
27)	L6 AR-1254-2	6.354	5.552	71238	135450	21.353	64.552 #
28)	L6 AR-1254-3	6.710	5.881	72298	78934	20.374	23.475
29)	L6 AR-1254-4	6.994	6.106	144936	32837	49.205	15.926 #
30)	L6 AR-1254-5	7.411	6.520	35631	19951	11.522	6.426 #
31)	L7 AR-1260-1	6.895	6.021	90037	27359	33.399	12.005 #
32)	L7 AR-1260-2	7.121	6.194	161760	115291	43.595	39.350
33)	L7 AR-1260-3	7.479	6.339	20452	4746	6.242	1.792 #
34)	L7 AR-1260-4	7.708	6.801	13478	17493	4.388	7.731 #
35)	L7 AR-1260-5	8.013	7.044	70564	69017	9.965	12.541 #
36)	L8 AR-1262-1	7.479	6.539	20452	10116	4.214	2.714 #
37)	L8 AR-1262-2	8.013	7.044	70564	69017	9.145	11.739 #
38)	L8 AR-1262-3	8.318	7.320	45263	31688	8.871	12.471 #
39)	L8 AR-1262-4	8.397	7.386	2080	63242	0.540	14.312 #
40)	L8 AR-1262-5	8.977	7.879	66709	10006	25.992	5.542 #
41)	L9 AR-1268-1	8.318	7.320	45263	31688	4.810	4.450
42)	L9 AR-1268-2	8.397	7.386	2080	63242	0.264	9.808 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081919\
 Data File : P0059465.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Aug 2019 18:52
 Operator : SM/AJ
 Sample : K3591-09
 Misc : AR1232 MDL 25PPB
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-MDL-WATER-03-QT3-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 20 01:07:05 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 17 03:09:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
43) L9	AR-1268-3	8.594	7.594	15332	1816	2.175	0.332 #
44) L9	AR-1268-4	8.977	7.879	66709	10006	23.996	4.902 #
45) L9	AR-1268-5	9.336	8.152	33956	13747	1.841	0.946 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081919\
Data File : PO059465.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Aug 2019 18:52
Operator : SM/AJ
Sample : K3591-09
Misc : AR1232 MDL 25PPB
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 20 01:07:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Aug 17 03:09:44 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

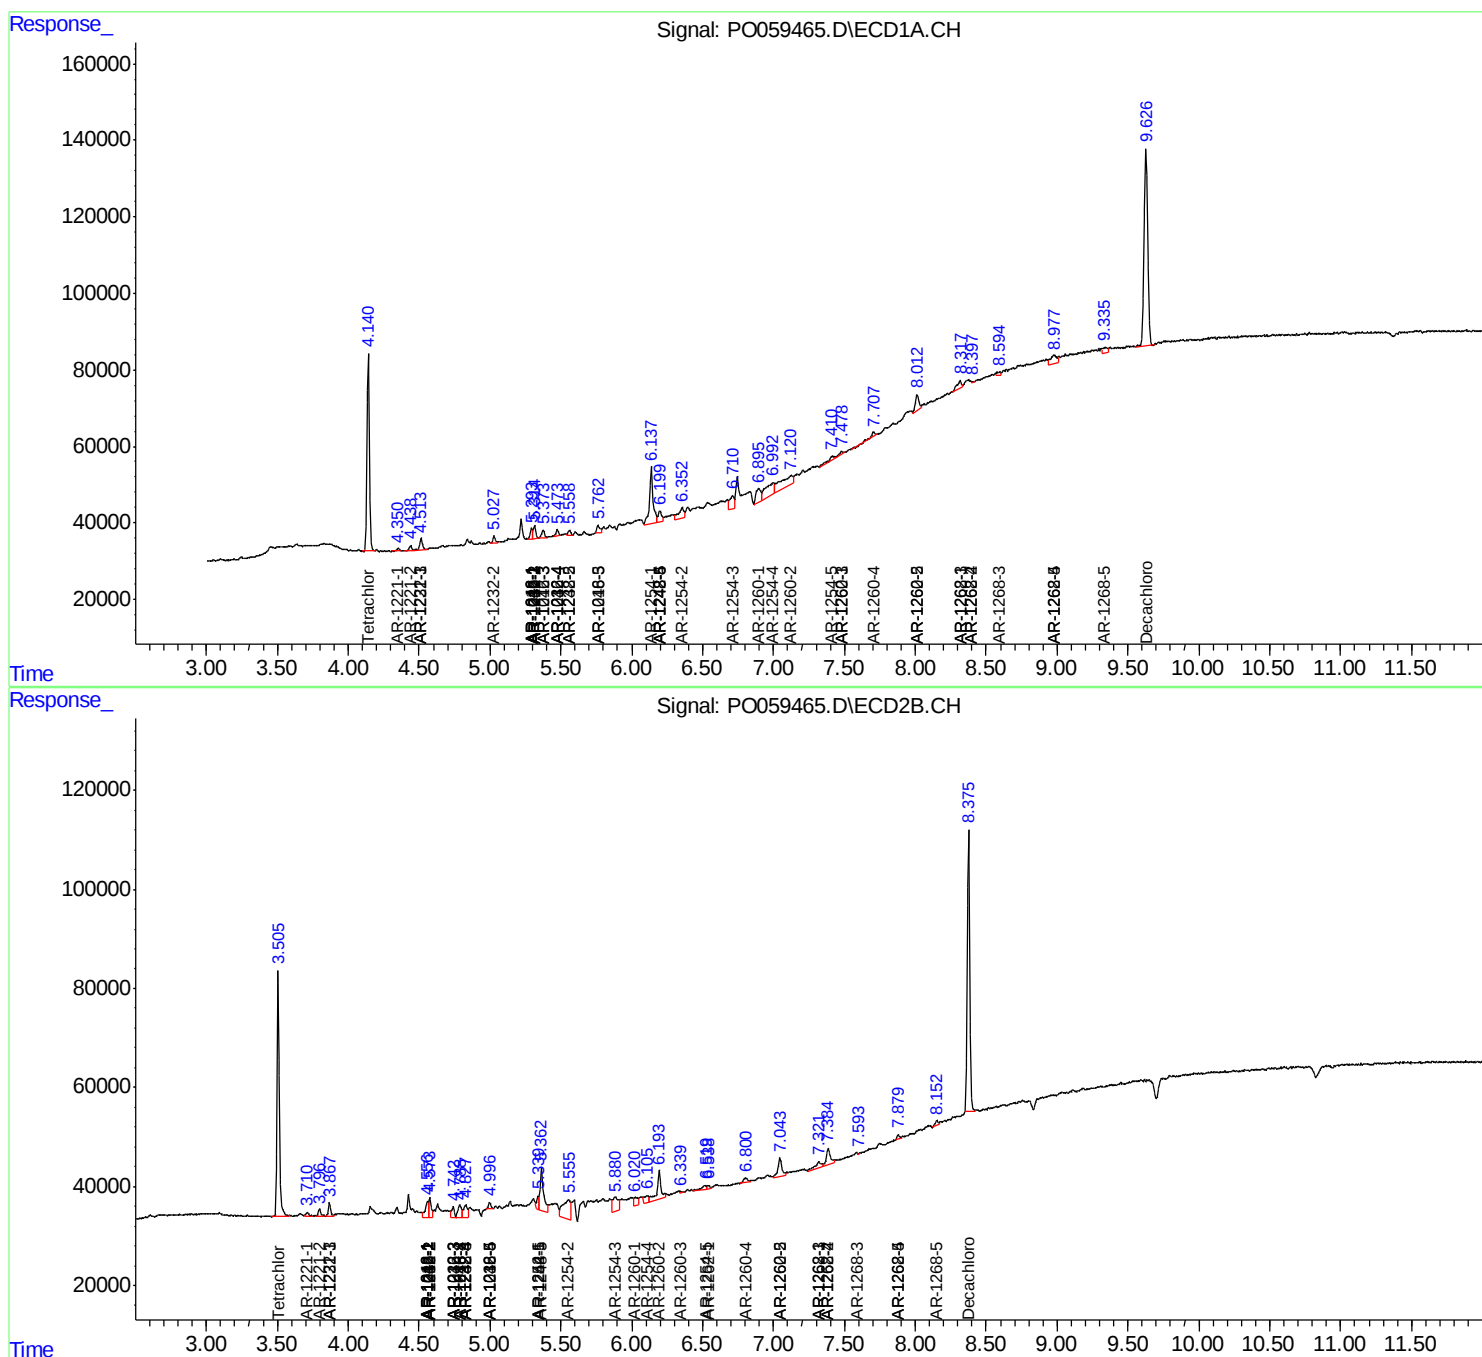


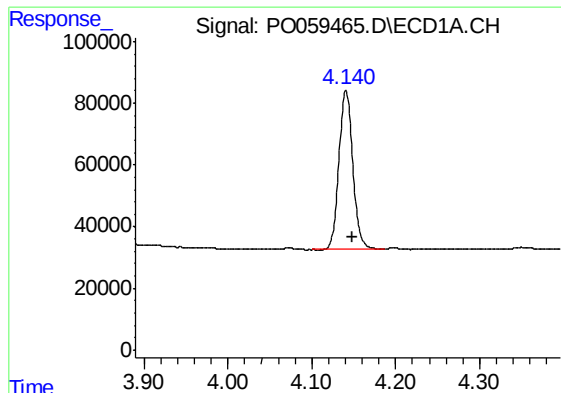

#1 Tetrachloro-m-xylene


R.T.: 4.141 min
Delta R.T.: -0.008 min
Response: 595433
Conc: 17.01 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

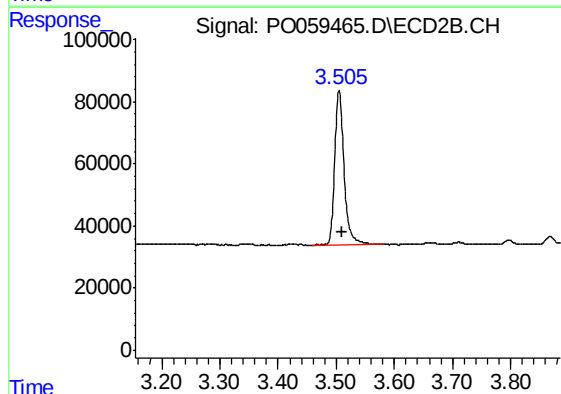


#1 Tetrachloro-m-xylene

R.T.: 3.505 min
Delta R.T.: -0.005 min
Response: 558393
Conc: 15.51 ng/ml

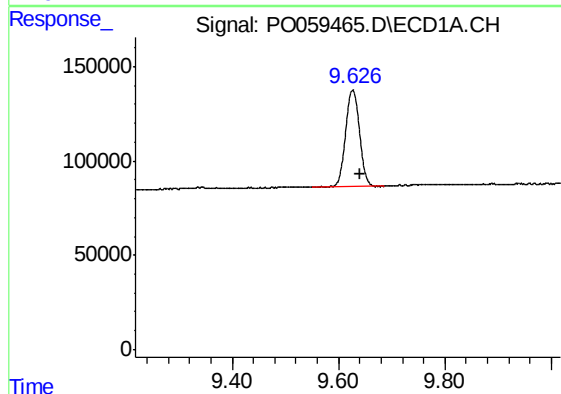


#2 Decachlorobiphenyl

R.T.: 9.627 min
Delta R.T.: -0.014 min
Response: 937358
Conc: 17.62 ng/ml

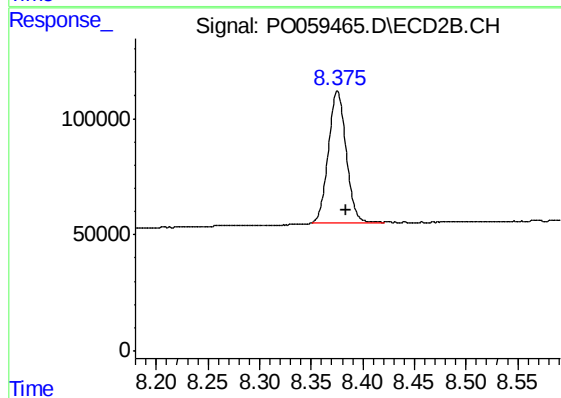

#2 Decachlorobiphenyl


R.T.: 8.375 min
Delta R.T.: -0.008 min
Response: 685935
Conc: 17.01 ng/ml

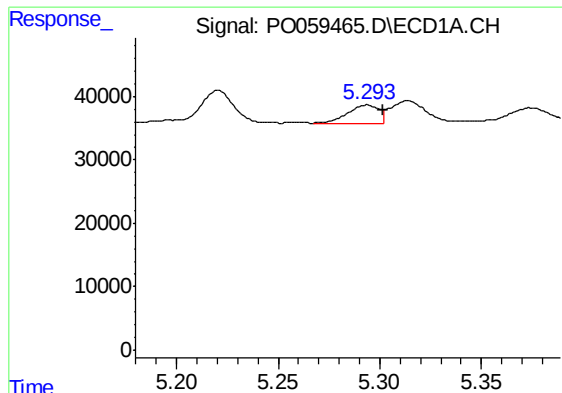

#3 AR-1016-1


R.T.: 5.293 min
Delta R.T.: -0.008 min
Response: 31547
Conc: 19.67 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

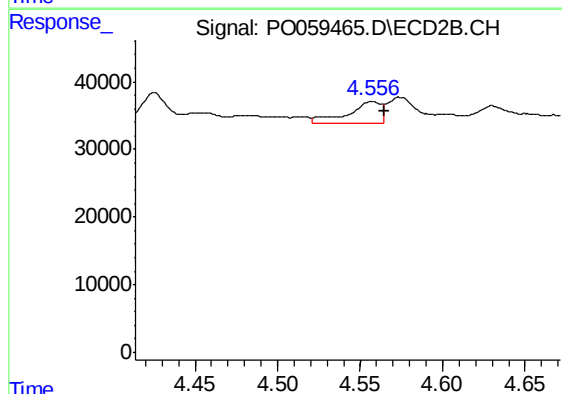


#3 AR-1016-1

R.T.: 4.557 min
Delta R.T.: -0.007 min
Response: 46043
Conc: 34.06 ng/ml

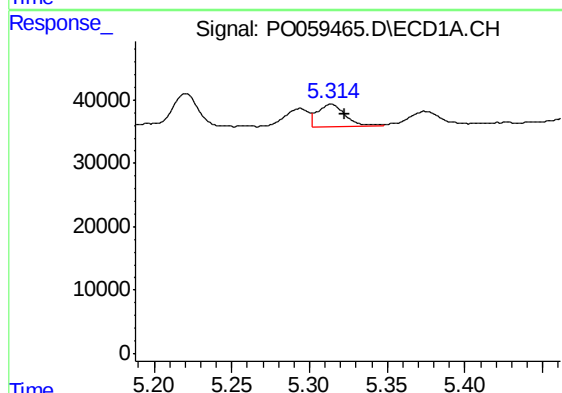


#4 AR-1016-2

R.T.: 5.314 min
Delta R.T.: -0.009 min
Response: 41651
Conc: 17.41 ng/ml

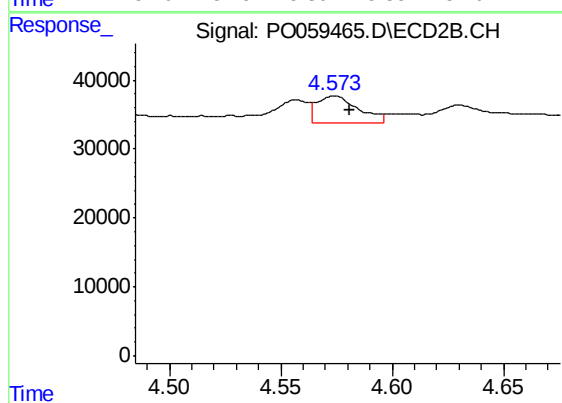

#4 AR-1016-2


R.T.: 4.574 min
Delta R.T.: -0.007 min
Response: 50351
Conc: 25.14 ng/ml

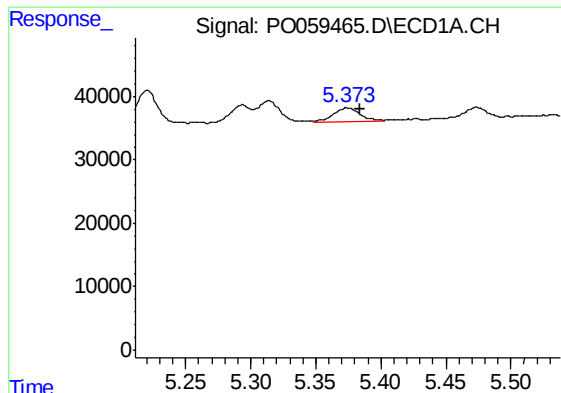

#5 AR-1016-3


R.T.: 5.374 min
Delta R.T.: -0.010 min
Response: 29153
Conc: 19.57 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

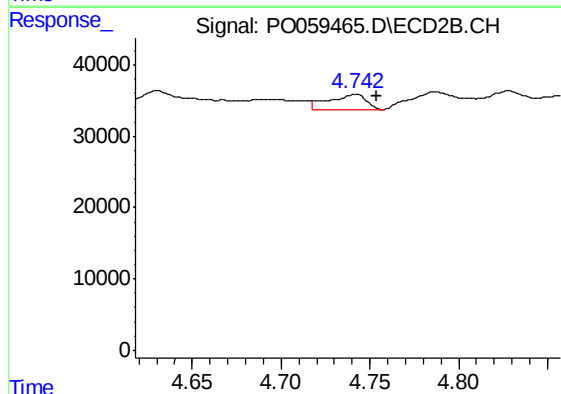


#5 AR-1016-3

R.T.: 4.742 min
Delta R.T.: -0.012 min
Response: 31047
Conc: 28.70 ng/ml

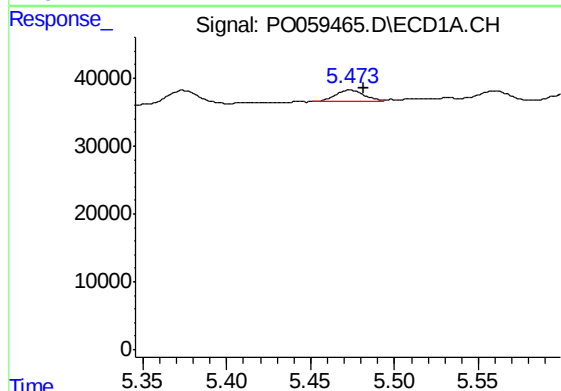


#6 AR-1016-4

R.T.: 5.474 min
Delta R.T.: -0.008 min
Response: 19750
Conc: 16.33 ng/ml

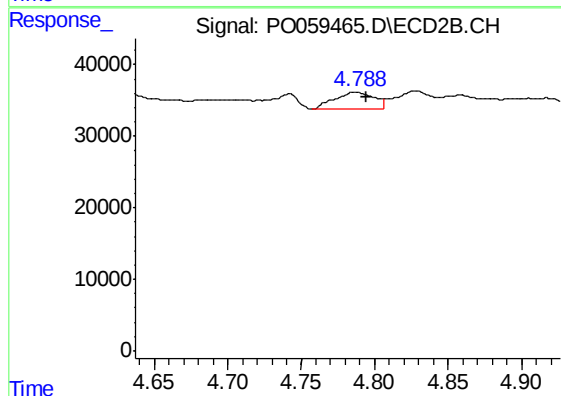

#6 AR-1016-4


R.T.: 4.787 min
Delta R.T.: -0.008 min
Response: 44671
Conc: 49.47 ng/ml



#7 AR-1016-5


R.T.: 5.762 min
Delta R.T.: -0.008 min
Response: 27702
Conc: 21.57 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019




#7 AR-1016-5

R.T.: 4.997 min
Delta R.T.: -0.007 min
Response: 16646
Conc: 14.45 ng/ml




#8 AR-1221-1

R.T.: 4.351 min
Delta R.T.: -0.010 min
Response: 9510
Conc: 22.46 ng/ml

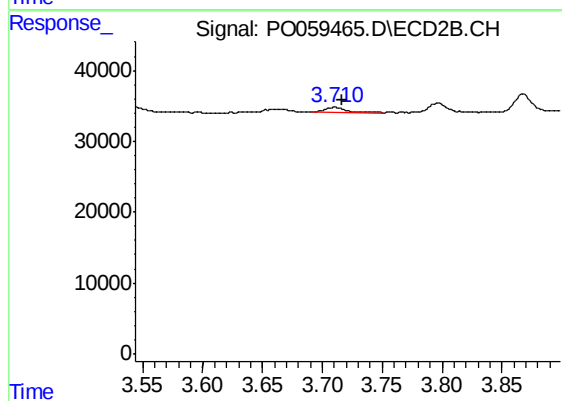

#8 AR-1221-1


R.T.: 3.711 min
Delta R.T.: -0.006 min
Response: 9022
Conc: 22.48 ng/ml



#9 AR-1221-2


R.T.: 4.439 min
Delta R.T.: -0.007 min
Response: 16051
Conc: 49.42 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019




#9 AR-1221-2

R.T.: 3.797 min
Delta R.T.: -0.004 min
Response: 16050
Conc: 52.69 ng/ml

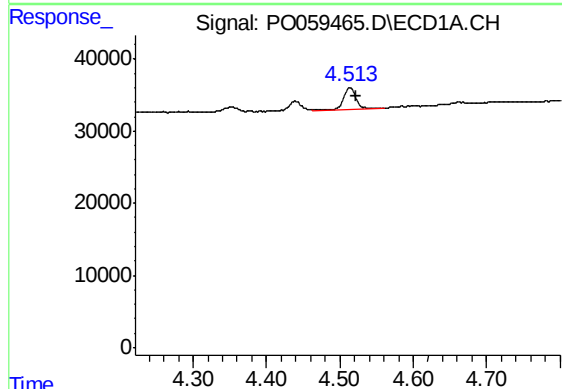


#10 AR-1221-3

R.T.: 4.514 min
Delta R.T.: -0.008 min
Response: 35302
Conc: 33.56 ng/ml

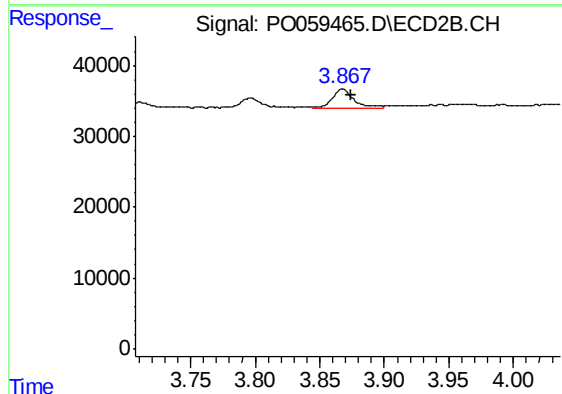

#10 AR-1221-3


R.T.: 3.868 min
Delta R.T.: -0.007 min
Response: 31272
Conc: 31.96 ng/ml



#11 AR-1232-1


R.T.: 4.514 min
Delta R.T.: -0.008 min
Response: 35302
Conc: 28.32 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019




#11 AR-1232-1

R.T.: 3.868 min
Delta R.T.: -0.006 min
Response: 31272
Conc: 27.43 ng/ml




#12 AR-1232-2

R.T.: 5.028 min
Delta R.T.: -0.009 min
Response: 21191
Conc: 30.00 ng/ml

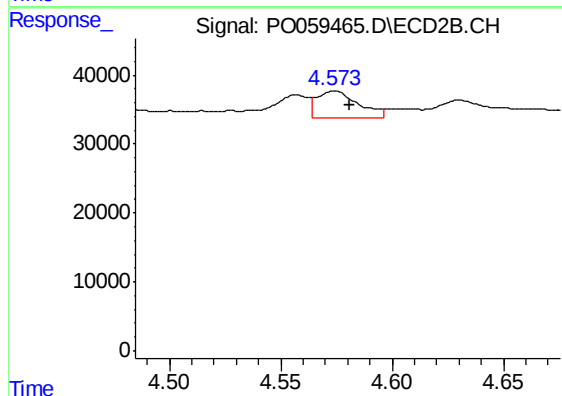

#12 AR-1232-2


R.T.: 4.574 min
Delta R.T.: -0.007 min
Response: 50351
Conc: 39.54 ng/ml



#13 AR-1232-3


R.T.: 5.314 min
Delta R.T.: -0.008 min
Response: 41651
Conc: 27.20 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019




#13 AR-1232-3

R.T.: 4.742 min
Delta R.T.: -0.011 min
Response: 31047
Conc: 45.60 ng/ml




#14 AR-1232-4

R.T.: 5.474 min
Delta R.T.: -0.008 min
Response: 19750
Conc: 25.26 ng/ml

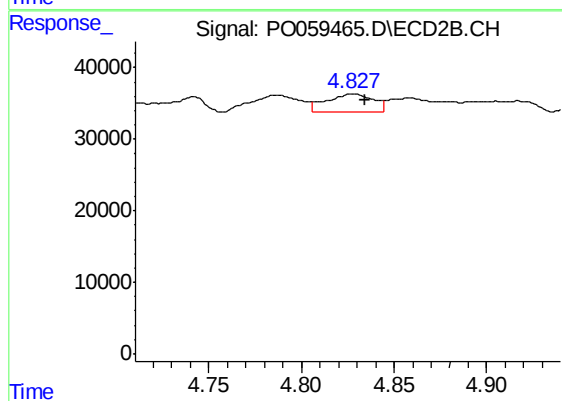

#14 AR-1232-4


R.T.: 4.828 min
Delta R.T.: -0.006 min
Response: 44123
Conc: 72.33 ng/ml

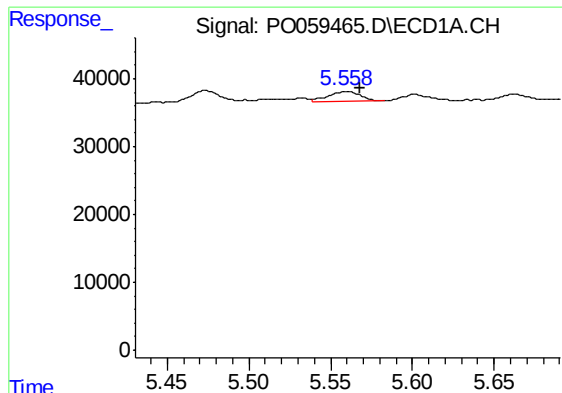

#15 AR-1232-5


R.T.: 5.560 min
Delta R.T.: -0.008 min
Response: 19561
Conc: 32.54 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

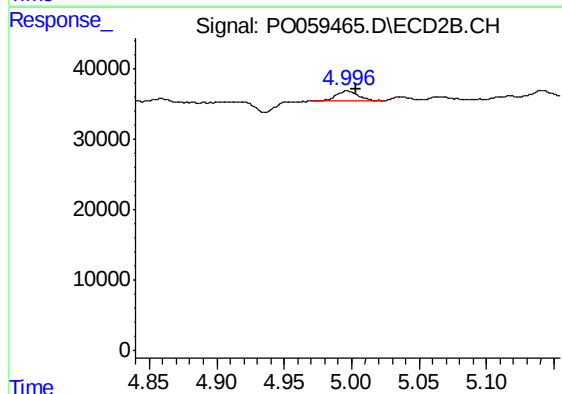


#15 AR-1232-5

R.T.: 4.997 min
Delta R.T.: -0.007 min
Response: 16646
Conc: 24.45 ng/ml

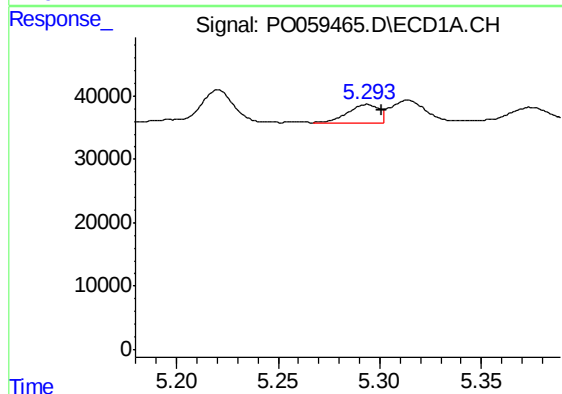


#16 AR-1242-1

R.T.: 5.293 min
Delta R.T.: -0.008 min
Response: 31547
Conc: 24.85 ng/ml

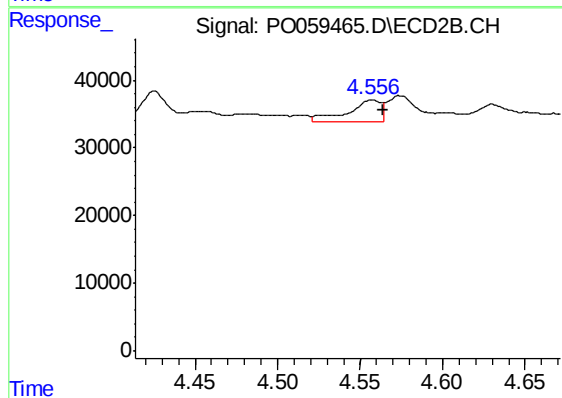

#16 AR-1242-1


R.T.: 4.557 min
Delta R.T.: -0.007 min
Response: 46043
Conc: 44.76 ng/ml

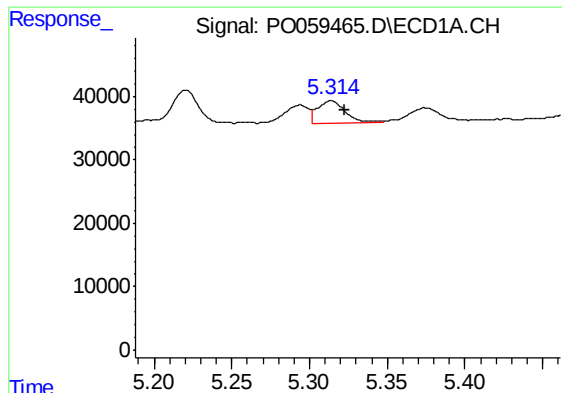

#17 AR-1242-2


R.T.: 5.314 min
Delta R.T.: -0.009 min
Response: 41651
Conc: 22.45 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

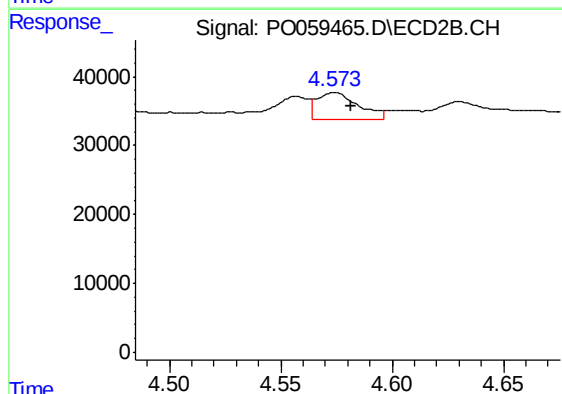


#17 AR-1242-2

R.T.: 4.574 min
Delta R.T.: -0.007 min
Response: 50351
Conc: 33.06 ng/ml

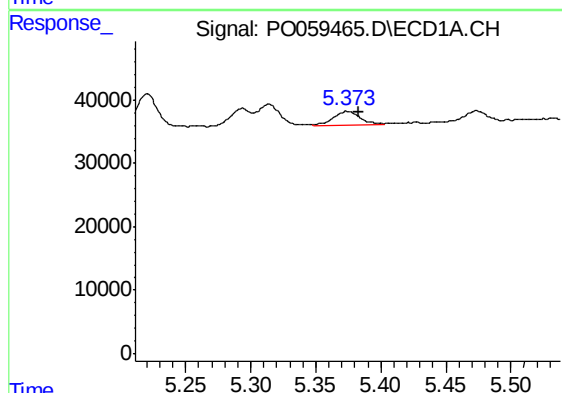


#18 AR-1242-3

R.T.: 5.374 min
Delta R.T.: -0.009 min
Response: 29153
Conc: 24.94 ng/ml

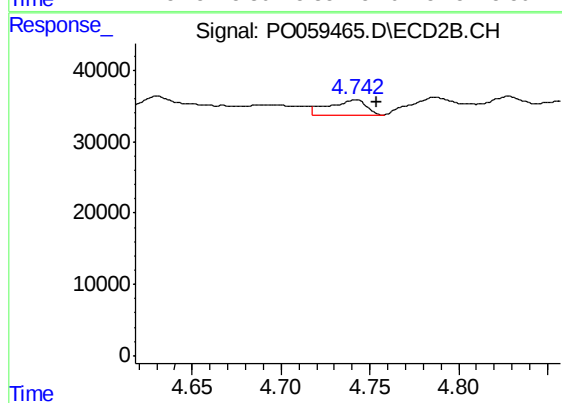

#18 AR-1242-3


R.T.: 4.742 min
Delta R.T.: -0.012 min
Response: 31047
Conc: 37.16 ng/ml

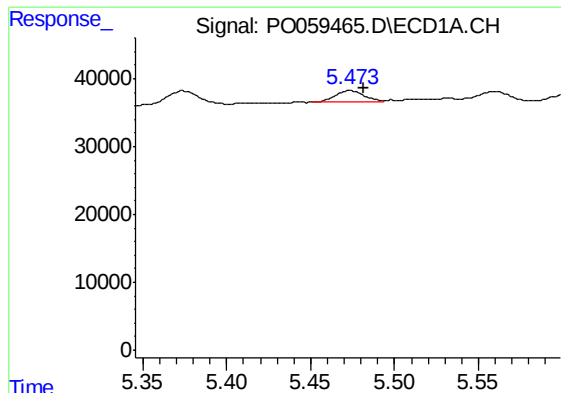

#19 AR-1242-4


R.T.: 5.474 min
Delta R.T.: -0.008 min
Response: 19750
Conc: 20.41 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

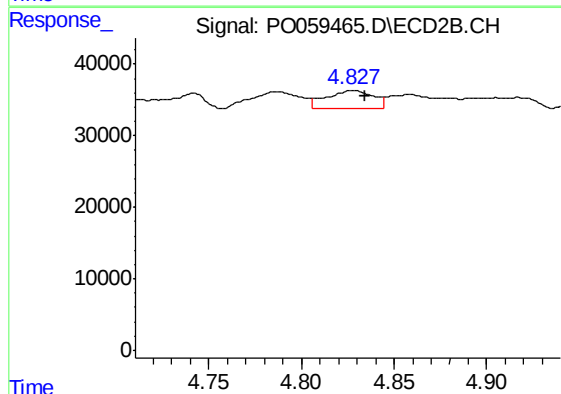


#19 AR-1242-4

R.T.: 4.828 min
Delta R.T.: -0.006 min
Response: 44123
Conc: 52.88 ng/ml

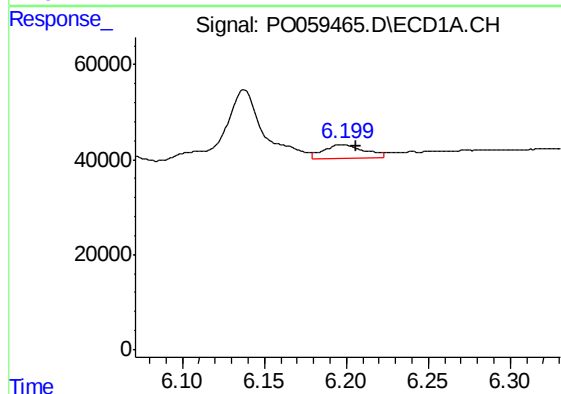


#20 AR-1242-5

R.T.: 6.198 min
Delta R.T.: -0.008 min
Response: 50476
Conc: 40.17 ng/ml

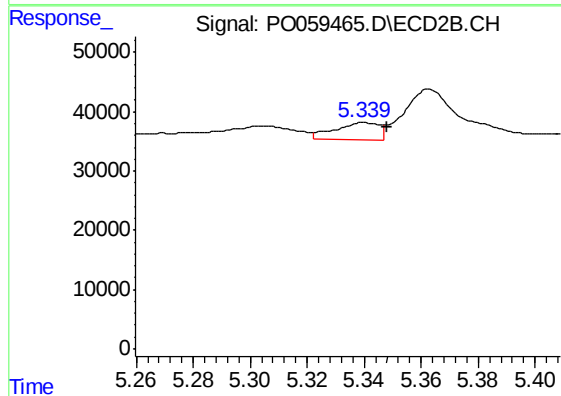

#20 AR-1242-5


R.T.: 5.340 min
Delta R.T.: -0.008 min
Response: 31820
Conc: 28.45 ng/ml

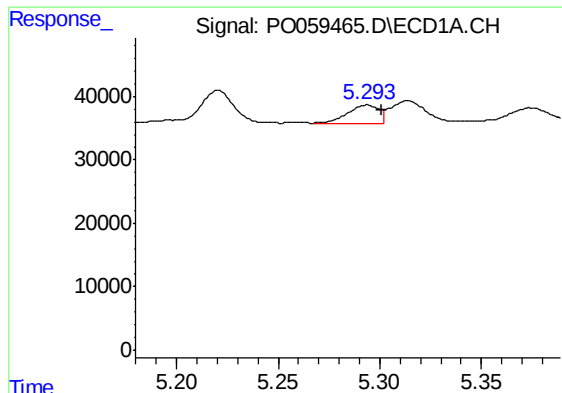

#21 AR-1248-1


R.T.: 5.293 min
Delta R.T.: -0.008 min
Response: 31547
Conc: 31.47 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

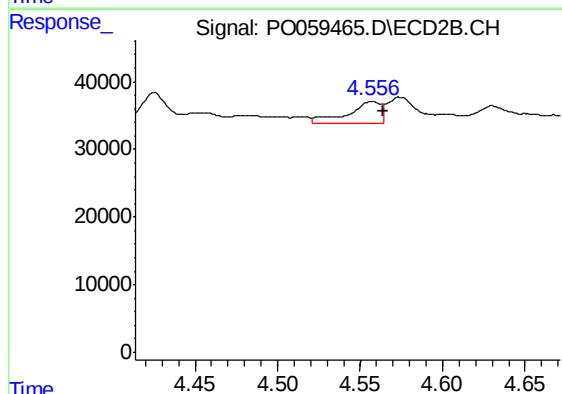


#21 AR-1248-1

R.T.: 4.557 min
Delta R.T.: -0.007 min
Response: 46043
Conc: 55.61 ng/ml

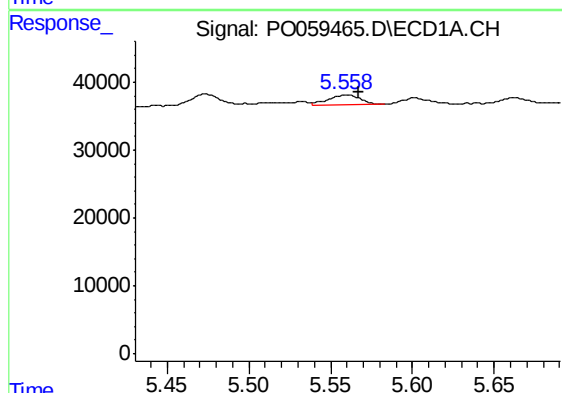


#22 AR-1248-2

R.T.: 5.560 min
Delta R.T.: -0.007 min
Response: 19561
Conc: 13.48 ng/ml

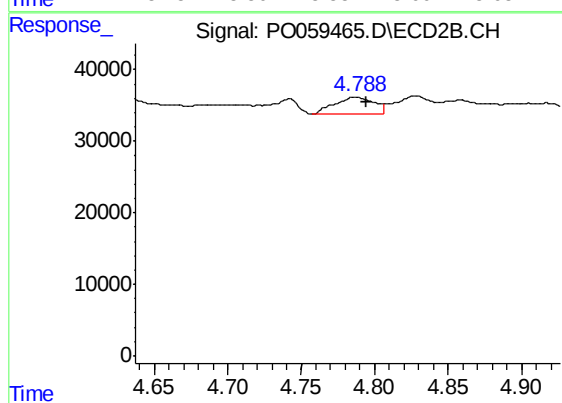

#22 AR-1248-2


R.T.: 4.787 min
Delta R.T.: -0.007 min
Response: 44671
Conc: 38.74 ng/ml



#23 AR-1248-3


R.T.: 5.762 min
Delta R.T.: -0.006 min
Response: 27702
Conc: 16.67 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019




#23 AR-1248-3

R.T.: 4.828 min
Delta R.T.: -0.007 min
Response: 44123
Conc: 37.15 ng/ml




#24 AR-1248-4

R.T.: 6.198 min
Delta R.T.: 0.029 min
Response: 50476
Conc: 24.69 ng/ml

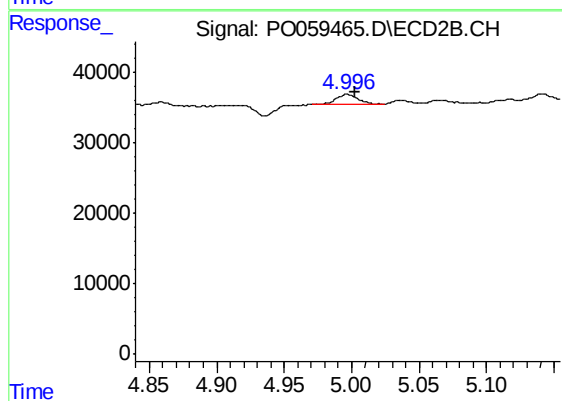

#24 AR-1248-4


R.T.: 4.997 min
Delta R.T.: -0.006 min
Response: 16646
Conc: 11.46 ng/ml

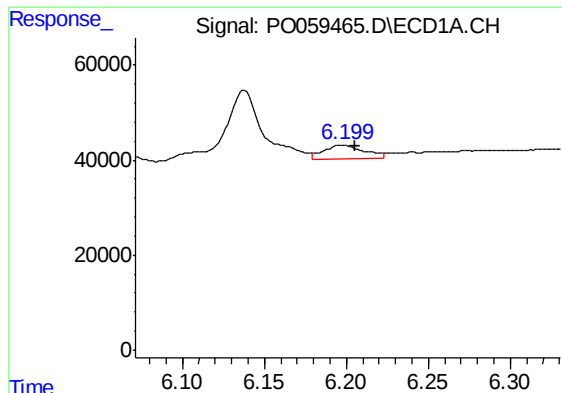

#25 AR-1248-5


R.T.: 6.198 min
Delta R.T.: -0.007 min
Response: 50476
Conc: 25.45 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019




#25 AR-1248-5

R.T.: 5.363 min
Delta R.T.: -0.024 min
Response: 140500
Conc: 98.16 ng/ml

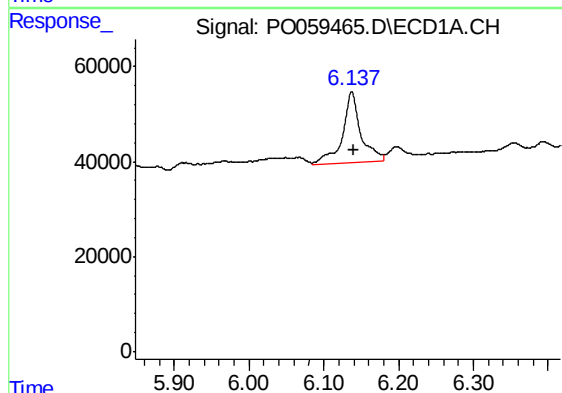


#26 AR-1254-1

R.T.: 6.138 min
Delta R.T.: -0.002 min
Response: 255945
Conc: 122.67 ng/ml

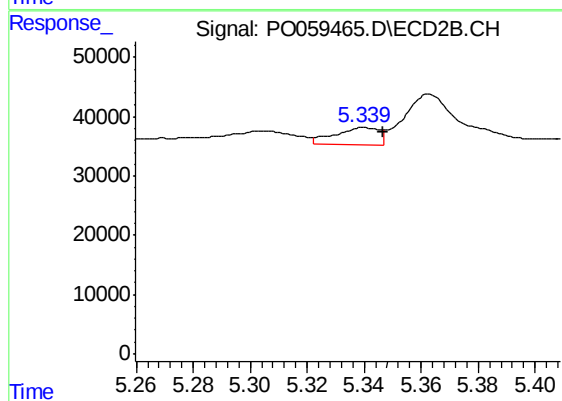

#26 AR-1254-1


R.T.: 5.340 min
Delta R.T.: -0.007 min
Response: 31820
Conc: 13.42 ng/ml



#27 AR-1254-2


R.T.: 6.354 min
Delta R.T.: 0.000 min
Response: 71238
Conc: 21.35 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

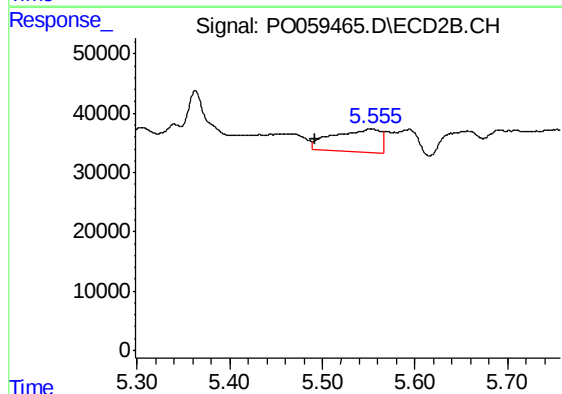


#27 AR-1254-2

R.T.: 5.552 min
Delta R.T.: 0.060 min
Response: 135450
Conc: 64.55 ng/ml

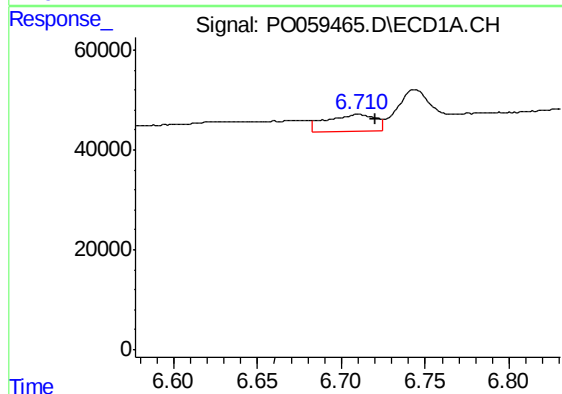


#28 AR-1254-3

R.T.: 6.710 min
Delta R.T.: -0.010 min
Response: 72298
Conc: 20.37 ng/ml

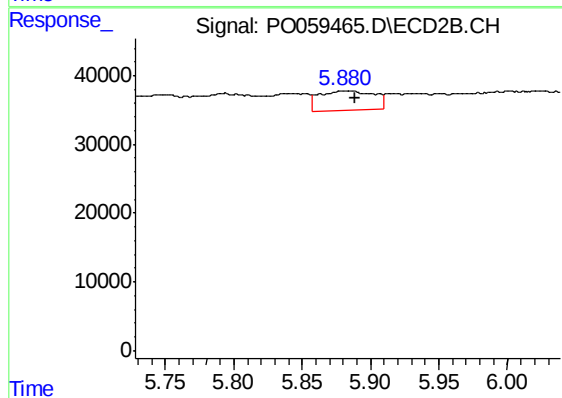

#28 AR-1254-3


R.T.: 5.881 min
Delta R.T.: -0.008 min
Response: 78934
Conc: 23.47 ng/ml

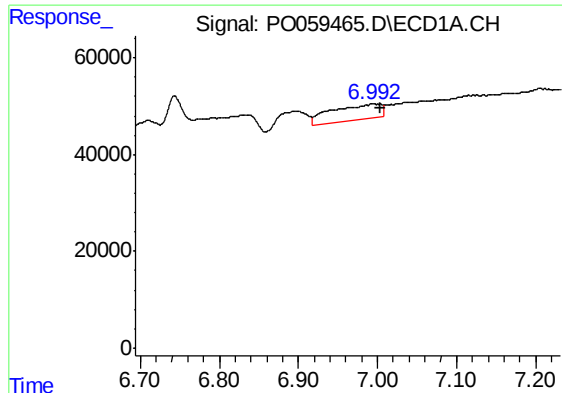

#29 AR-1254-4


R.T.: 6.994 min
Delta R.T.: -0.010 min
Response: 144936
Conc: 49.21 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

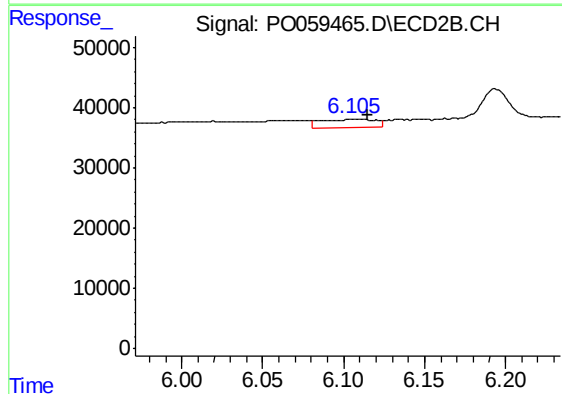


#29 AR-1254-4

R.T.: 6.106 min
Delta R.T.: -0.009 min
Response: 32837
Conc: 15.93 ng/ml

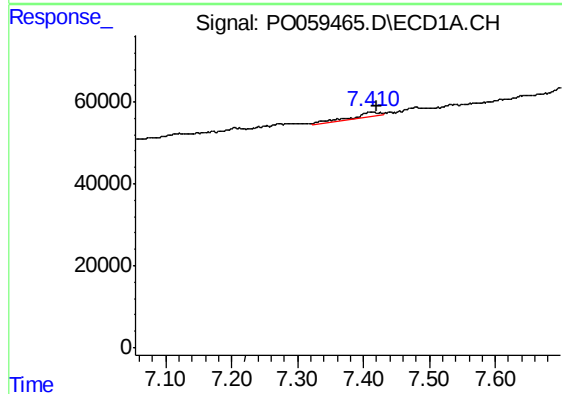


#30 AR-1254-5

R.T.: 7.411 min
Delta R.T.: -0.008 min
Response: 35631
Conc: 11.52 ng/ml

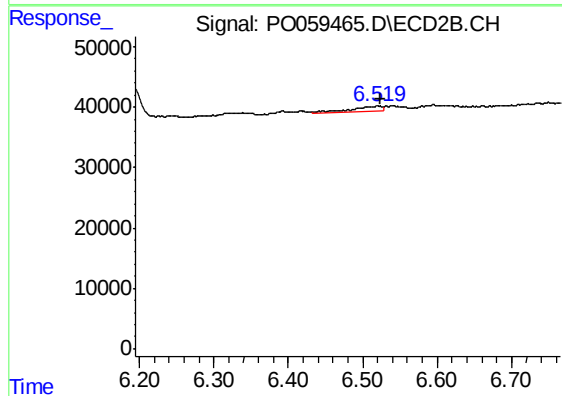

#30 AR-1254-5


R.T.: 6.520 min
Delta R.T.: -0.005 min
Response: 19951
Conc: 6.43 ng/ml

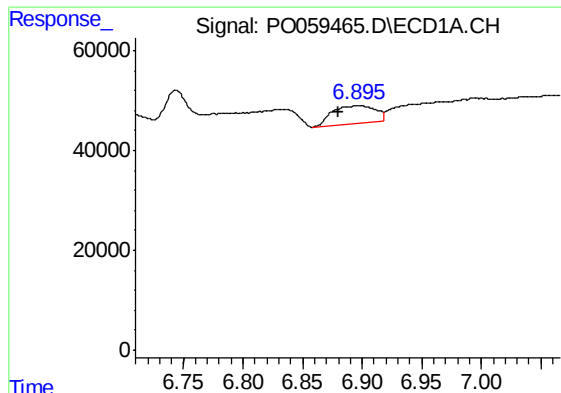

#31 AR-1260-1


R.T.: 6.895 min
Delta R.T.: 0.015 min
Response: 90037
Conc: 33.40 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

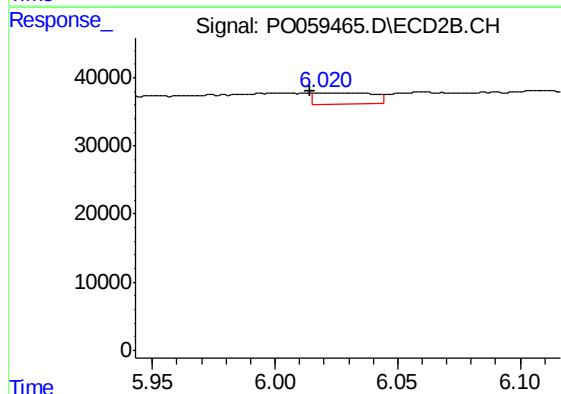


#31 AR-1260-1

R.T.: 6.021 min
Delta R.T.: 0.006 min
Response: 27359
Conc: 12.01 ng/ml

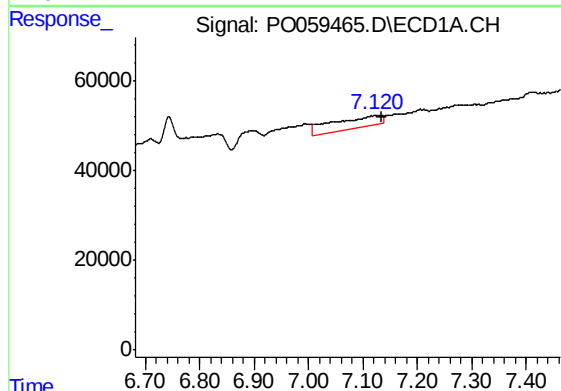


#32 AR-1260-2

R.T.: 7.121 min
Delta R.T.: -0.014 min
Response: 161760
Conc: 43.60 ng/ml

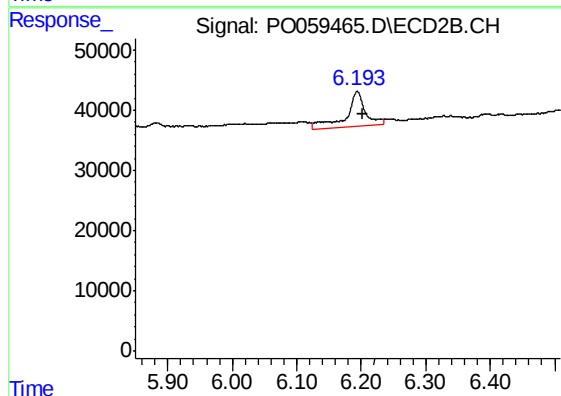

#32 AR-1260-2


R.T.: 6.194 min
Delta R.T.: -0.009 min
Response: 115291
Conc: 39.35 ng/ml



#33 AR-1260-3


R.T.: 7.479 min
Delta R.T.: -0.011 min
Response: 20452
Conc: 6.24 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019




#33 AR-1260-3

R.T.: 6.339 min
Delta R.T.: -0.012 min
Response: 4746
Conc: 1.79 ng/ml




#34 AR-1260-4

R.T.: 7.708 min
Delta R.T.: -0.010 min
Response: 13478
Conc: 4.39 ng/ml

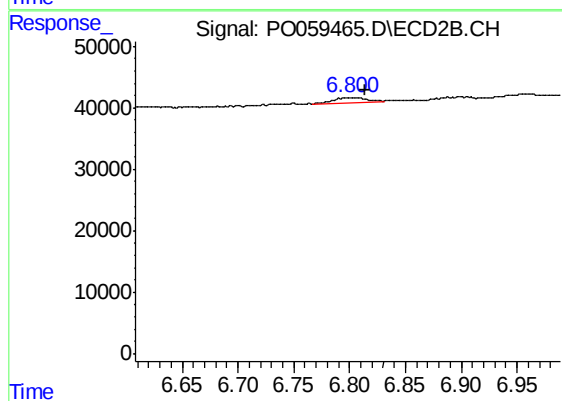

#34 AR-1260-4


R.T.: 6.801 min
Delta R.T.: -0.013 min
Response: 17493
Conc: 7.73 ng/ml



#35 AR-1260-5


R.T.: 8.013 min
Delta R.T.: -0.011 min
Response: 70564
Conc: 9.97 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019




#35 AR-1260-5

R.T.: 7.044 min
Delta R.T.: -0.013 min
Response: 69017
Conc: 12.54 ng/ml




#36 AR-1262-1

R.T.: 7.479 min
Delta R.T.: -0.010 min
Response: 20452
Conc: 4.21 ng/ml

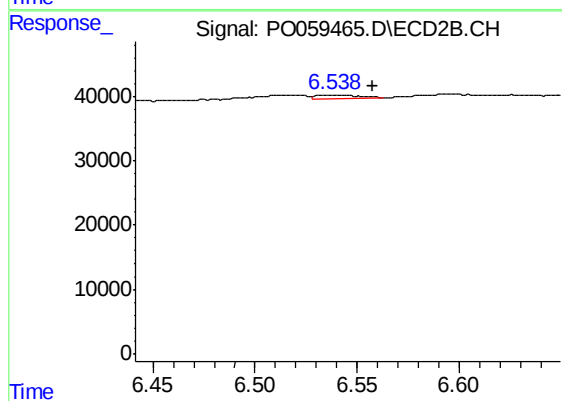

#36 AR-1262-1


R.T.: 6.539 min
Delta R.T.: -0.019 min
Response: 10116
Conc: 2.71 ng/ml



#37 AR-1262-2


R.T.: 8.013 min
Delta R.T.: -0.010 min
Response: 70564
Conc: 9.15 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019




#37 AR-1262-2

R.T.: 7.044 min
Delta R.T.: -0.013 min
Response: 69017
Conc: 11.74 ng/ml




#38 AR-1262-3

R.T.: 8.318 min
Delta R.T.: 0.014 min
Response: 45263
Conc: 8.87 ng/ml

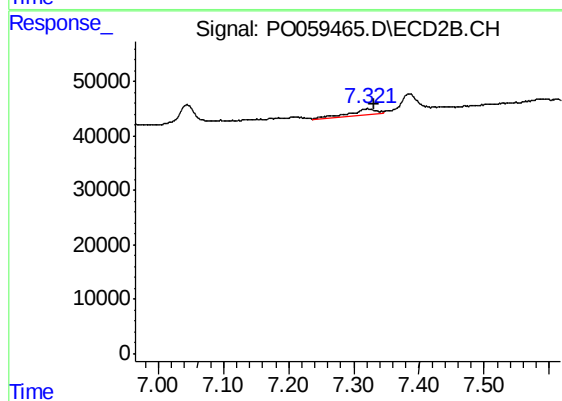

#38 AR-1262-3


R.T.: 7.320 min
Delta R.T.: -0.012 min
Response: 31688
Conc: 12.47 ng/ml

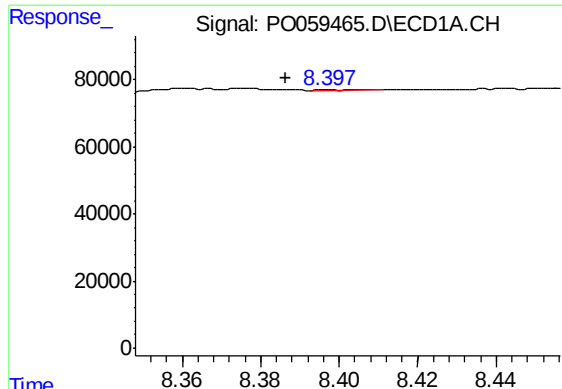

#39 AR-1262-4


R.T.: 8.397 min
Delta R.T.: 0.011 min
Response: 2080
Conc: 0.54 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019




#39 AR-1262-4

R.T.: 7.386 min
Delta R.T.: -0.012 min
Response: 63242
Conc: 14.31 ng/ml




#40 AR-1262-5

R.T.: 8.977 min
Delta R.T.: -0.008 min
Response: 66709
Conc: 25.99 ng/ml

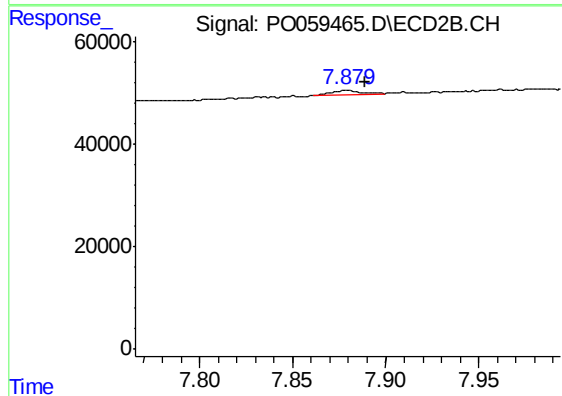

#40 AR-1262-5


R.T.: 7.879 min
Delta R.T.: -0.010 min
Response: 10006
Conc: 5.54 ng/ml



#41 AR-1268-1


R.T.: 8.318 min
Delta R.T.: 0.015 min
Response: 45263
Conc: 4.81 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

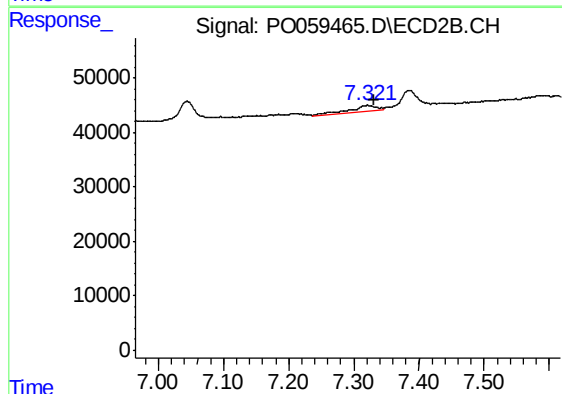


#41 AR-1268-1

R.T.: 7.320 min
Delta R.T.: -0.010 min
Response: 31688
Conc: 4.45 ng/ml




#42 AR-1268-2

R.T.: 8.397 min
Delta R.T.: 0.007 min
Response: 2080
Conc: 0.26 ng/ml

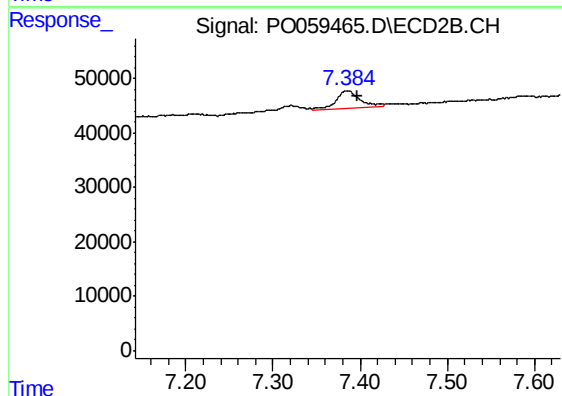

#42 AR-1268-2


R.T.: 7.386 min
Delta R.T.: -0.012 min
Response: 63242
Conc: 9.81 ng/ml

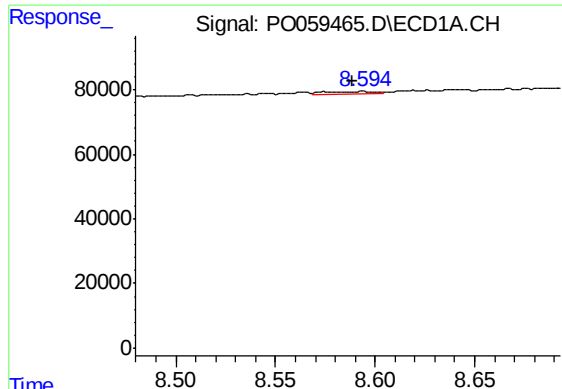

#43 AR-1268-3


R.T.: 8.594 min
Delta R.T.: 0.005 min
Response: 15332
Conc: 2.18 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

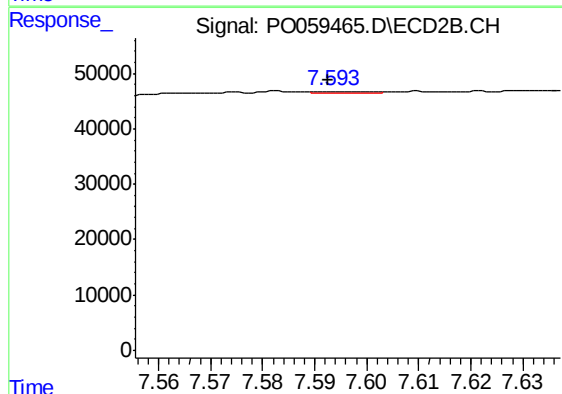


#43 AR-1268-3

R.T.: 7.594 min
Delta R.T.: 0.001 min
Response: 1816
Conc: 0.33 ng/ml




#44 AR-1268-4

R.T.: 8.977 min
Delta R.T.: -0.008 min
Response: 66709
Conc: 24.00 ng/ml

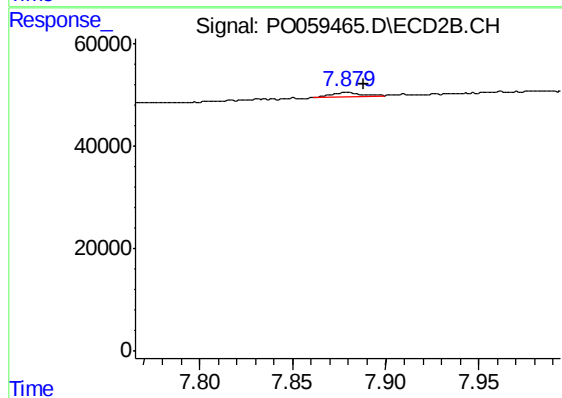

#44 AR-1268-4


R.T.: 7.879 min
Delta R.T.: -0.009 min
Response: 10006
Conc: 4.90 ng/ml

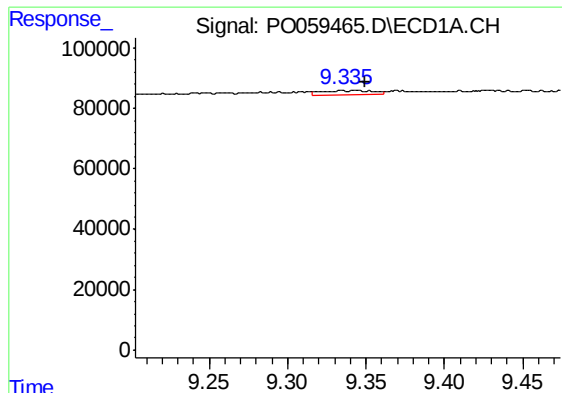

#45 AR-1268-5

R.T.: 9.336 min
Delta R.T.: -0.014 min
Response: 33956
Conc: 1.84 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

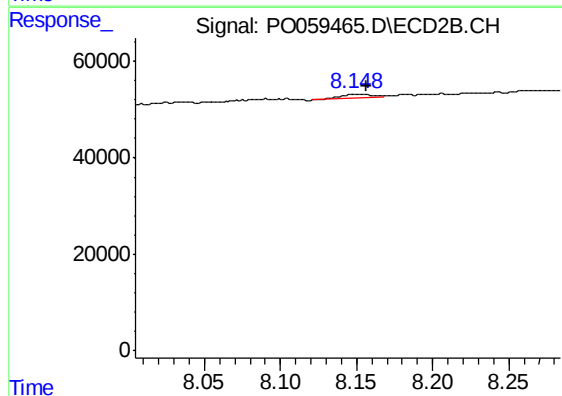

#45 AR-1268-5

R.T.: 8.152 min
Delta R.T.: -0.004 min
Response: 13747
Conc: 0.95 ng/ml