

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081919\
 Data File : P0059466.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Aug 2019 19:09
 Operator : SM/AJ
 Sample : K3591-09
 Misc : AR1242 MDL 25PPB
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-MDL-WATER-03-QT3-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 20 01:07:51 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 17 03:09:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.142	3.507	295654	287601	8.444	7.990
2)	SA Decachlor...	9.627	8.375	437882	329725	8.231	8.178
Target Compounds							
3)	L1 AR-1016-1	5.293	4.558	21883	22916	13.644	16.951
4)	L1 AR-1016-2	5.315	4.576	23526	40745	9.833	20.342 #
5)	L1 AR-1016-3	5.375	4.741	17054	32447	11.449	29.992 #
6)	L1 AR-1016-4	5.474	4.790	11614	58434	9.600	64.712 #
7)	L1 AR-1016-5	5.763	4.998	22235	16266	17.315	14.120
8)	L2 AR-1221-1	0.000	3.667	0	10449	N.D.	26.033 #
9)	L2 AR-1221-2	4.442	3.799	8511	6782	26.205	22.264
10)	L2 AR-1221-3	4.514	3.869	9567	8148	9.095	8.328
11)	L3 AR-1232-1	4.514	3.869	9567	8148	7.675	7.147
12)	L3 AR-1232-2	5.029	4.576	13758	40745	19.476	31.993 #
13)	L3 AR-1232-3	5.315	4.741	23526	32447	15.363	47.652 #
14)	L3 AR-1232-4	5.474	4.830	11614	51968	14.854	85.185 #
15)	L3 AR-1232-5	5.560	4.998	24974	16266	41.546	23.894 #
16)	L4 AR-1242-1	5.293	4.558	21883	22916	17.237	22.278 #
17)	L4 AR-1242-2	5.315	4.576	23526	40745	12.678	26.752 #
18)	L4 AR-1242-3	5.375	4.741	17054	32447	14.590	38.835 #
19)	L4 AR-1242-4	5.474	4.830	11614	51968	12.000	62.283 #
20)	L4 AR-1242-5	6.198	5.364	67637	312760	53.825	279.598 #
21)	L5 AR-1248-1	5.293	4.558	21883	22916	21.827	27.676 #
22)	L5 AR-1248-2	5.560	4.790	24974	58434	17.213	50.675 #
23)	L5 AR-1248-3	5.763	4.830	22235	51968	13.378	43.753 #
24)	L5 AR-1248-4	6.198	4.998	67637	16266	33.089	11.194 #
25)	L5 AR-1248-5	6.198	5.364	67637	312760	34.107	218.517 #
26)	L6 AR-1254-1	6.138	5.364	321332	312760	154.011	131.866
27)	L6 AR-1254-2	6.355	5.460	103009	90823	30.876	43.284 #
28)	L6 AR-1254-3	6.711	5.884	139980	140841	39.448	41.886
29)	L6 AR-1254-4	6.996	6.109	191099	35007	64.877	16.979 #
30)	L6 AR-1254-5	7.443	6.515	32839	52412	10.619	16.880 #
31)	L7 AR-1260-1	6.900	6.003	98508	86714	36.541	38.051
32)	L7 AR-1260-2	7.136	6.195	10752	178073	2.898	60.778 #
33)	L7 AR-1260-3	7.482	6.341	20681	27211	6.312	10.272 #
34)	L7 AR-1260-4	7.706	6.803	32626	16192	10.623	7.157 #
35)	L7 AR-1260-5	8.013	7.045	76314	53823	10.777	9.780
36)	L8 AR-1262-1	7.482	6.538	20681	19017	4.262	5.102
37)	L8 AR-1262-2	8.013	7.045	76314	53823	9.891	9.155
38)	L8 AR-1262-3	8.314	7.321	33524	22557	6.570	8.877 #
39)	L8 AR-1262-4	8.379	7.386	26948	51574	6.991	11.671 #
40)	L8 AR-1262-5	8.974	7.881	79376	9700	30.927	5.373 #
41)	L9 AR-1268-1	8.314	7.321	33524	22557	3.562	3.168
42)	L9 AR-1268-2	8.379	7.386	26948	51574	3.419	7.999 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081919\
 Data File : P0059466.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Aug 2019 19:09
 Operator : SM/AJ
 Sample : K3591-09
 Misc : AR1242 MDL 25PPB
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-MDL-WATER-03-QT3-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 20 01:07:51 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 17 03:09:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
43) L9	AR-1268-3	8.620	0.000	41273	0	5.855	N.D. #
44) L9	AR-1268-4	8.974	7.881	79376	9700	28.552	4.752 #
45) L9	AR-1268-5	9.345	8.152	25177	9105	1.365	0.627 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081919\
Data File : PO059466.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Aug 2019 19:09
Operator : SM/AJ
Sample : K3591-09
Misc : AR1242 MDL 25PPB
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 20 01:07:51 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Aug 17 03:09:44 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

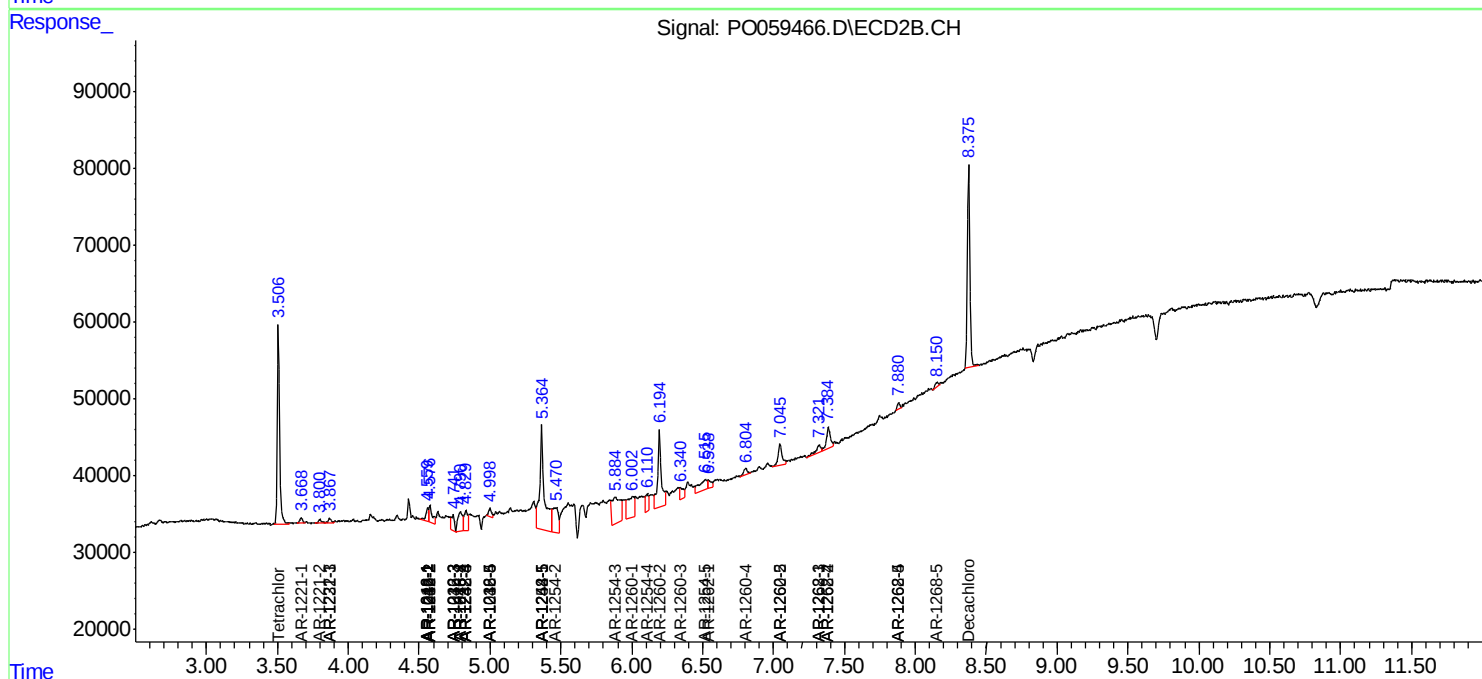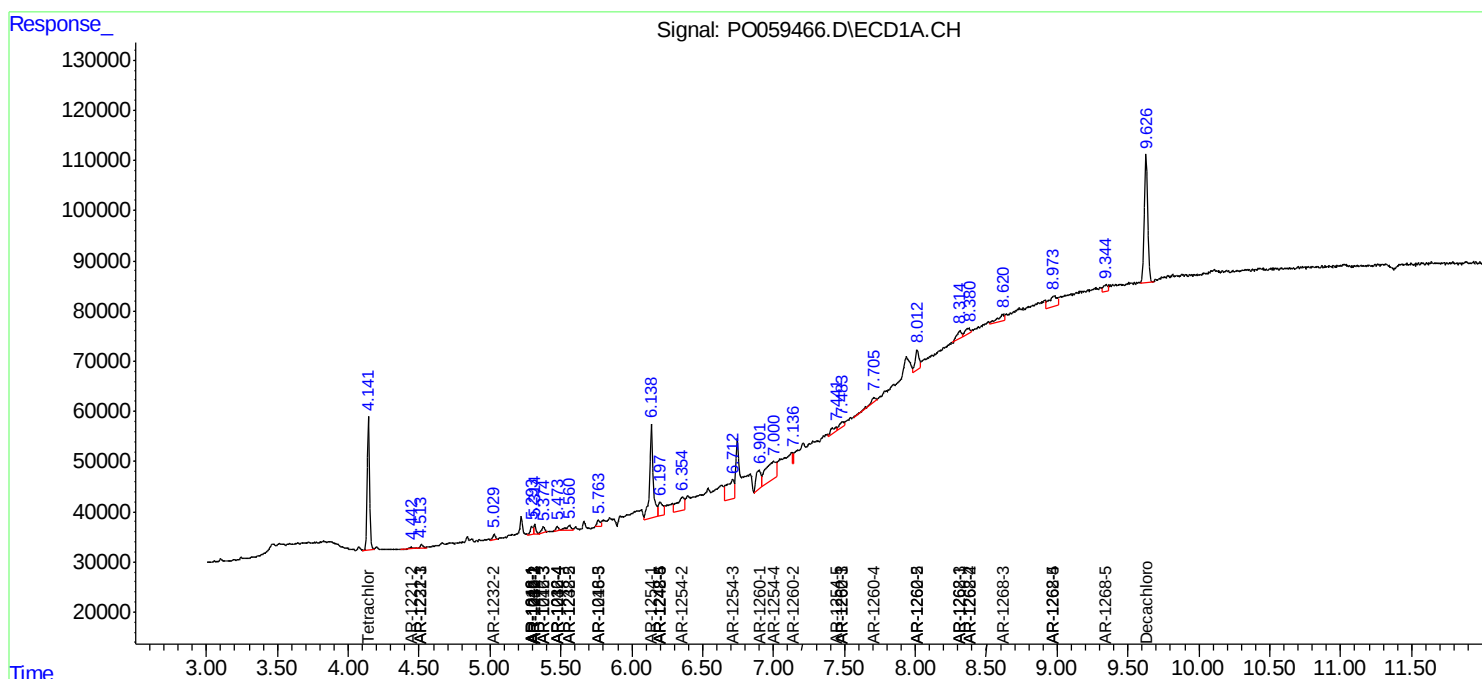


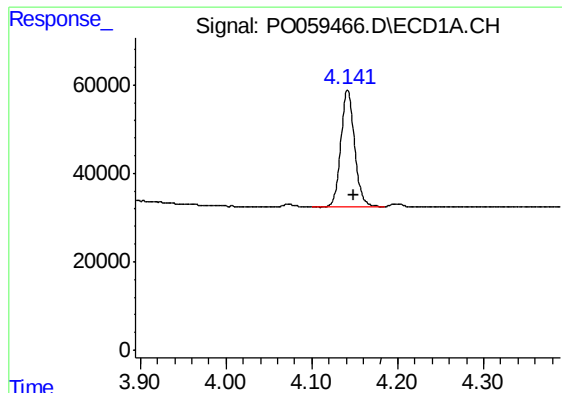

#1 Tetrachloro-m-xylene


R.T.: 4.142 min
Delta R.T.: -0.007 min
Response: 295654
Conc: 8.44 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

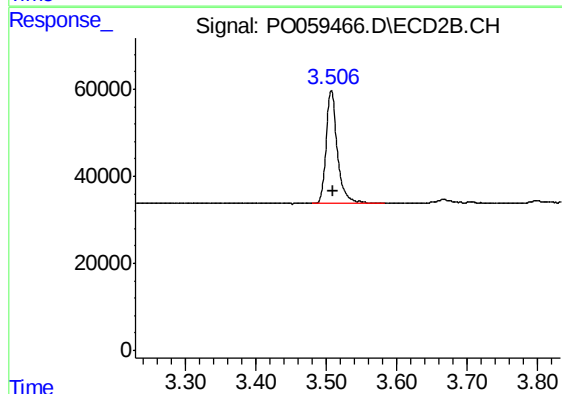


#1 Tetrachloro-m-xylene

R.T.: 3.507 min
Delta R.T.: -0.003 min
Response: 287601
Conc: 7.99 ng/ml




#2 Decachlorobiphenyl

R.T.: 9.627 min
Delta R.T.: -0.014 min
Response: 437882
Conc: 8.23 ng/ml

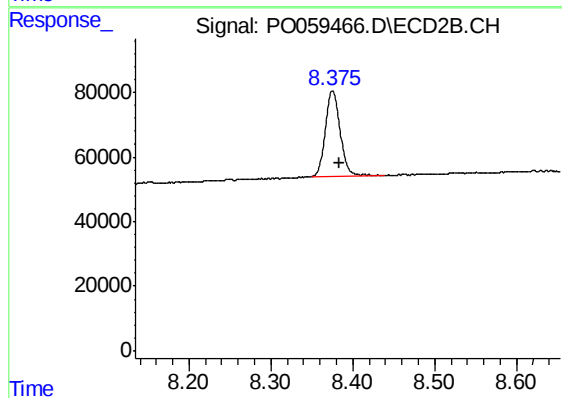

#2 Decachlorobiphenyl


R.T.: 8.375 min
Delta R.T.: -0.008 min
Response: 329725
Conc: 8.18 ng/ml

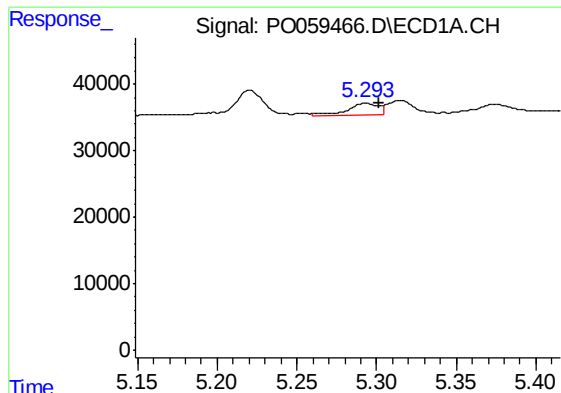

#3 AR-1016-1


R.T.: 5.293 min
Delta R.T.: -0.009 min
Response: 21883
Conc: 13.64 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

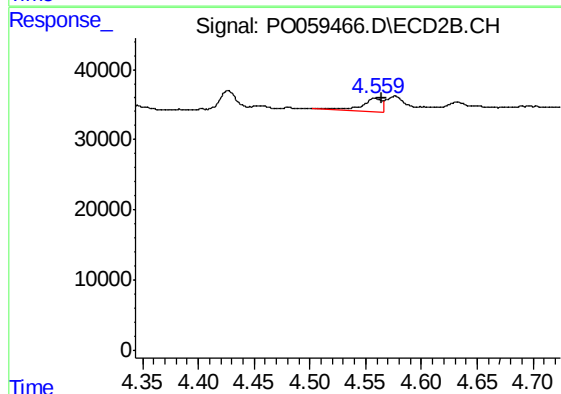


#3 AR-1016-1

R.T.: 4.558 min
Delta R.T.: -0.006 min
Response: 22916
Conc: 16.95 ng/ml

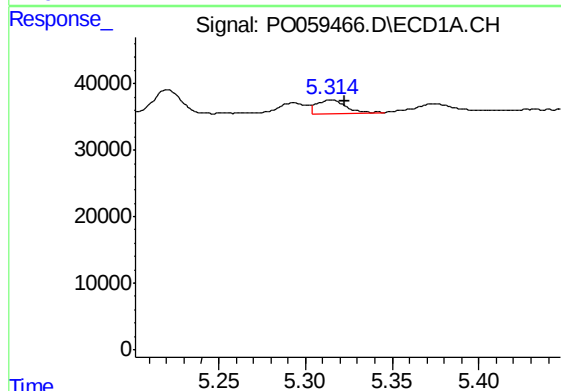


#4 AR-1016-2

R.T.: 5.315 min
Delta R.T.: -0.008 min
Response: 23526
Conc: 9.83 ng/ml

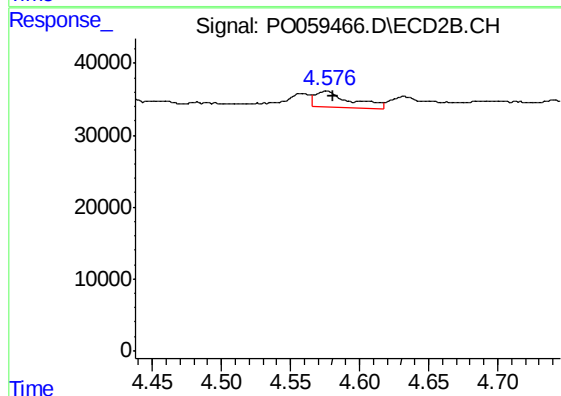

#4 AR-1016-2


R.T.: 4.576 min
Delta R.T.: -0.005 min
Response: 40745
Conc: 20.34 ng/ml

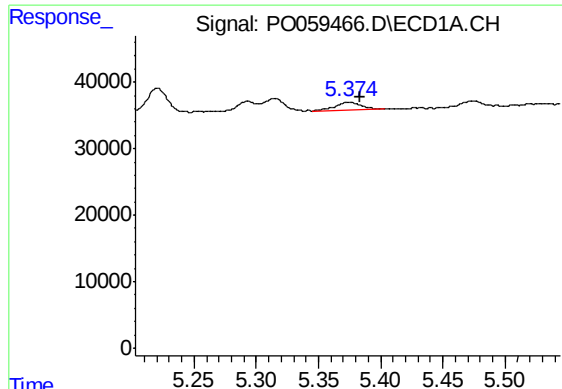

#5 AR-1016-3


R.T.: 5.375 min
Delta R.T.: -0.009 min
Response: 17054
Conc: 11.45 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019




#5 AR-1016-3

R.T.: 4.741 min
Delta R.T.: -0.013 min
Response: 32447
Conc: 29.99 ng/ml




#6 AR-1016-4

R.T.: 5.474 min
Delta R.T.: -0.007 min
Response: 11614
Conc: 9.60 ng/ml

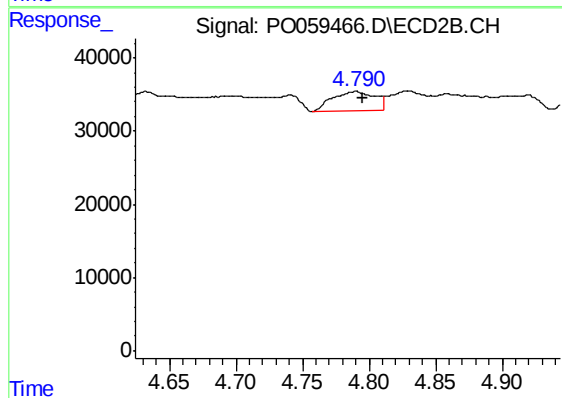

#6 AR-1016-4


R.T.: 4.790 min
Delta R.T.: -0.005 min
Response: 58434
Conc: 64.71 ng/ml



#7 AR-1016-5


R.T.: 5.763 min
Delta R.T.: -0.007 min
Response: 22235
Conc: 17.31 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019




#7 AR-1016-5

R.T.: 4.998 min
Delta R.T.: -0.006 min
Response: 16266
Conc: 14.12 ng/ml

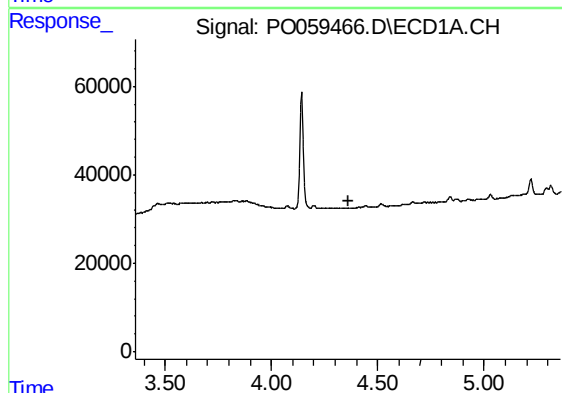


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.360 min
Response: 0
Conc: N.D.

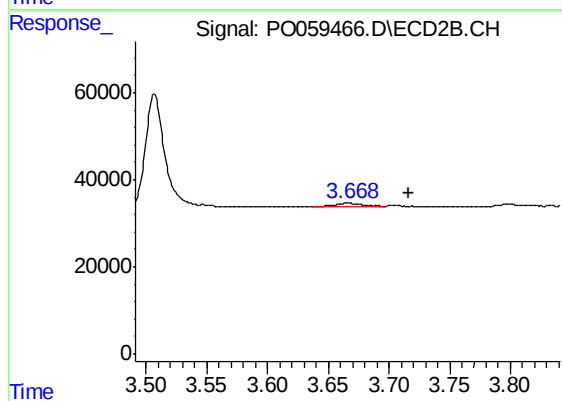

#8 AR-1221-1


R.T.: 3.667 min
Delta R.T.: -0.050 min
Response: 10449
Conc: 26.03 ng/ml



#9 AR-1221-2


R.T.: 4.442 min
Delta R.T.: -0.004 min
Response: 8511
Conc: 26.21 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

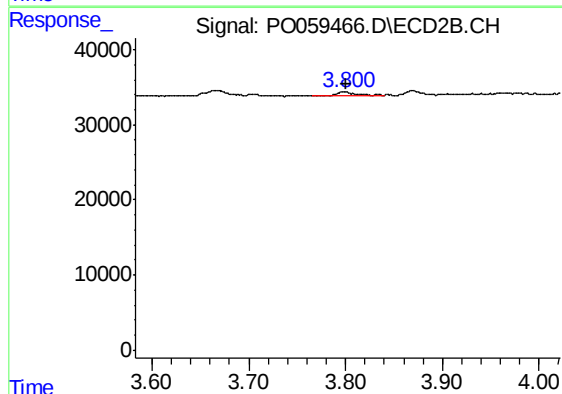


#9 AR-1221-2

R.T.: 3.799 min
Delta R.T.: -0.002 min
Response: 6782
Conc: 22.26 ng/ml




#10 AR-1221-3

R.T.: 4.514 min
Delta R.T.: -0.008 min
Response: 9567
Conc: 9.10 ng/ml

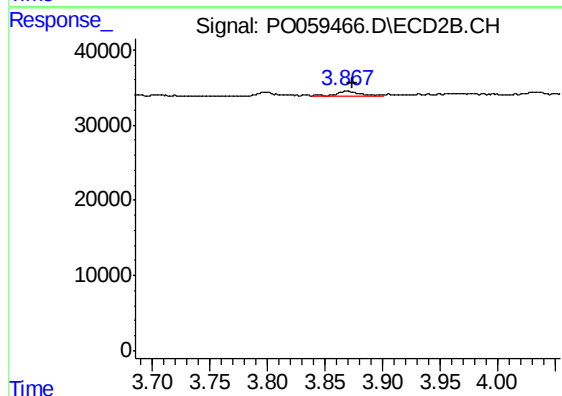

#10 AR-1221-3


R.T.: 3.869 min
Delta R.T.: -0.006 min
Response: 8148
Conc: 8.33 ng/ml

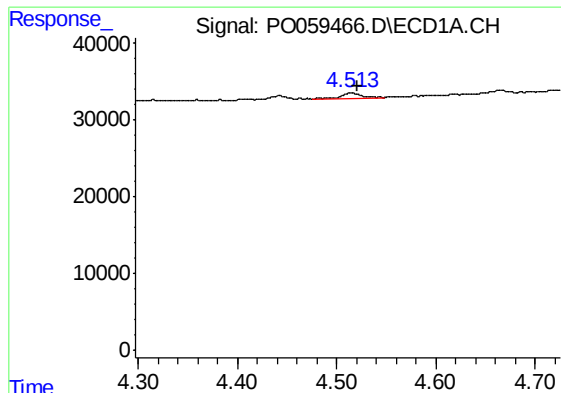

#11 AR-1232-1


R.T.: 4.514 min
Delta R.T.: -0.007 min
Response: 9567
Conc: 7.68 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

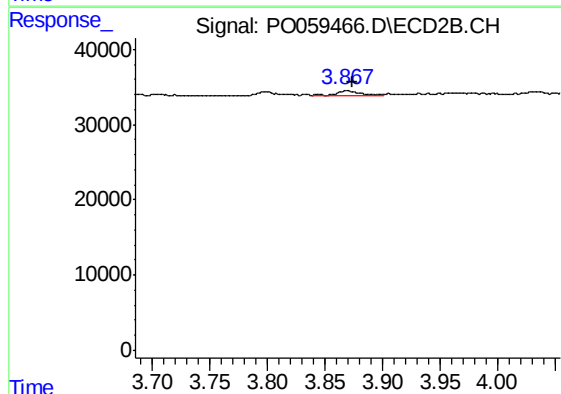


#11 AR-1232-1

R.T.: 3.869 min
Delta R.T.: -0.005 min
Response: 8148
Conc: 7.15 ng/ml

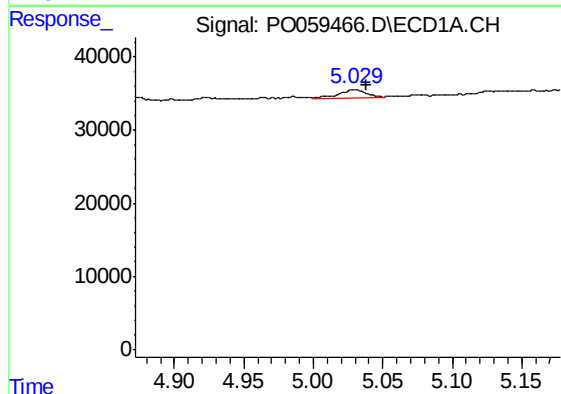


#12 AR-1232-2

R.T.: 5.029 min
Delta R.T.: -0.009 min
Response: 13758
Conc: 19.48 ng/ml

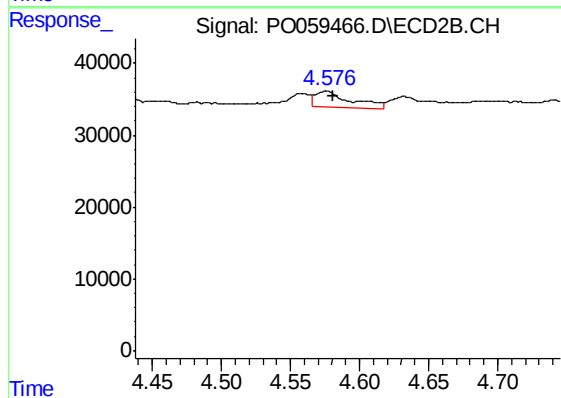

#12 AR-1232-2


R.T.: 4.576 min
Delta R.T.: -0.005 min
Response: 40745
Conc: 31.99 ng/ml



#13 AR-1232-3


R.T.: 5.315 min
Delta R.T.: -0.007 min
Response: 23526
Conc: 15.36 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019




#13 AR-1232-3

R.T.: 4.741 min
Delta R.T.: -0.013 min
Response: 32447
Conc: 47.65 ng/ml




#14 AR-1232-4

R.T.: 5.474 min
Delta R.T.: -0.007 min
Response: 11614
Conc: 14.85 ng/ml

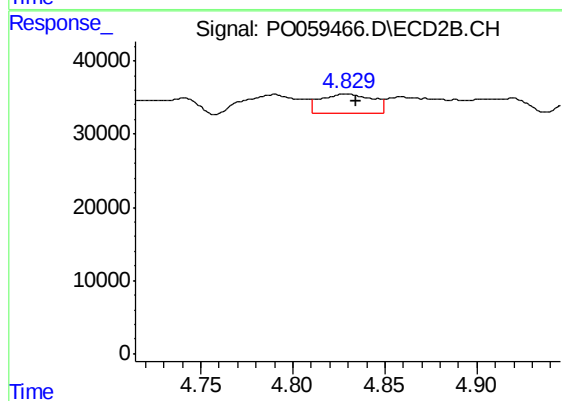

#14 AR-1232-4


R.T.: 4.830 min
Delta R.T.: -0.005 min
Response: 51968
Conc: 85.19 ng/ml



#15 AR-1232-5


R.T.: 5.560 min
Delta R.T.: -0.008 min
Response: 24974
Conc: 41.55 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019




#15 AR-1232-5

R.T.: 4.998 min
Delta R.T.: -0.006 min
Response: 16266
Conc: 23.89 ng/ml




#16 AR-1242-1

R.T.: 5.293 min
Delta R.T.: -0.008 min
Response: 21883
Conc: 17.24 ng/ml

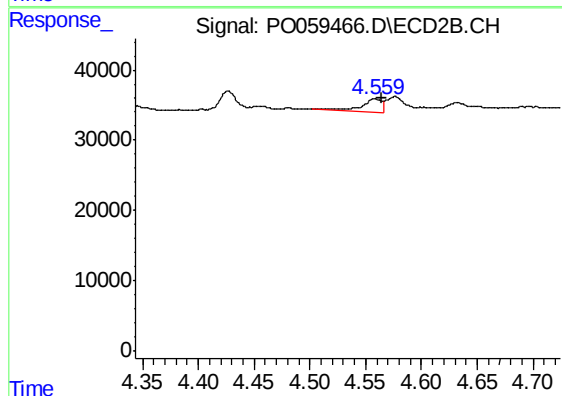

#16 AR-1242-1


R.T.: 4.558 min
Delta R.T.: -0.006 min
Response: 22916
Conc: 22.28 ng/ml



#17 AR-1242-2


R.T.: 5.315 min
Delta R.T.: -0.008 min
Response: 23526
Conc: 12.68 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019




#17 AR-1242-2

R.T.: 4.576 min
Delta R.T.: -0.005 min
Response: 40745
Conc: 26.75 ng/ml




#18 AR-1242-3

R.T.: 5.375 min
Delta R.T.: -0.009 min
Response: 17054
Conc: 14.59 ng/ml

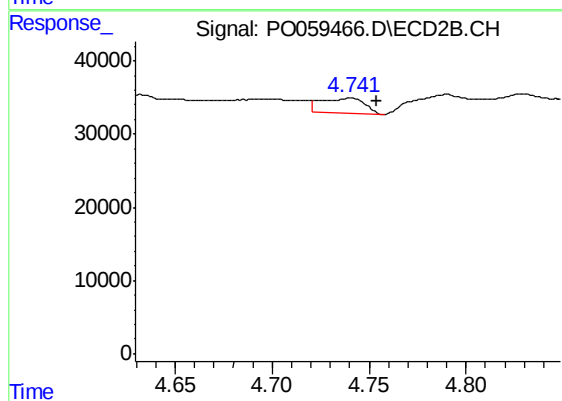

#18 AR-1242-3


R.T.: 4.741 min
Delta R.T.: -0.013 min
Response: 32447
Conc: 38.84 ng/ml

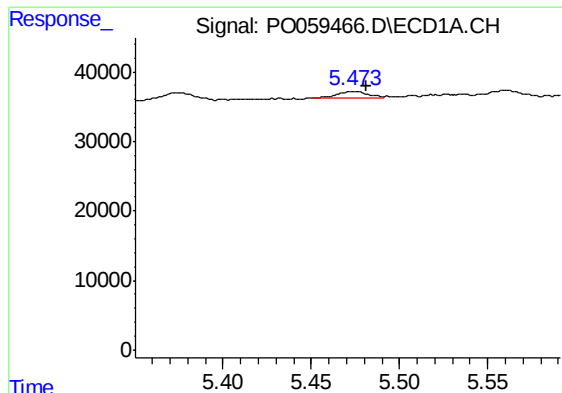

#19 AR-1242-4


R.T.: 5.474 min
Delta R.T.: -0.008 min
Response: 11614
Conc: 12.00 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

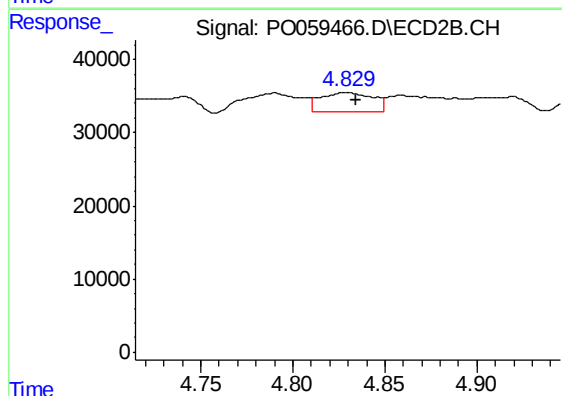


#19 AR-1242-4

R.T.: 4.830 min
Delta R.T.: -0.005 min
Response: 51968
Conc: 62.28 ng/ml

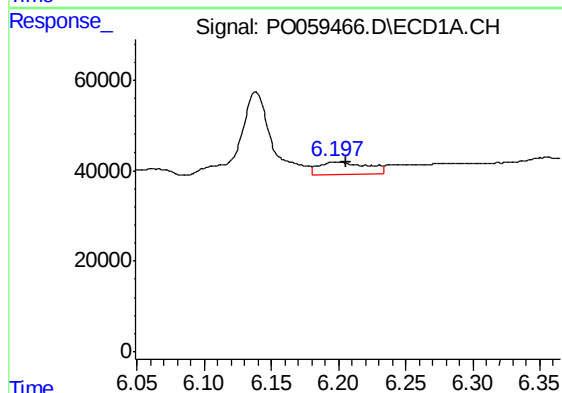


#20 AR-1242-5

R.T.: 6.198 min
Delta R.T.: -0.008 min
Response: 67637
Conc: 53.83 ng/ml

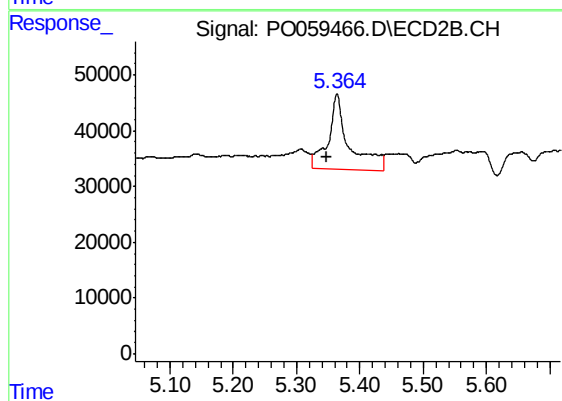

#20 AR-1242-5


R.T.: 5.364 min
Delta R.T.: 0.016 min
Response: 312760
Conc: 279.60 ng/ml



#21 AR-1248-1


R.T.: 5.293 min
Delta R.T.: -0.008 min
Response: 21883
Conc: 21.83 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019




#21 AR-1248-1

R.T.: 4.558 min
Delta R.T.: -0.006 min
Response: 22916
Conc: 27.68 ng/ml




#22 AR-1248-2

R.T.: 5.560 min
Delta R.T.: -0.007 min
Response: 24974
Conc: 17.21 ng/ml

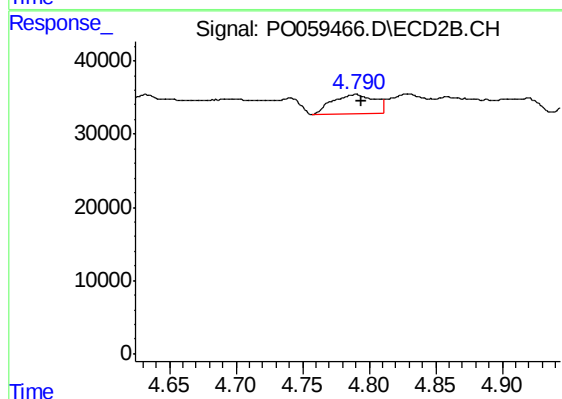

#22 AR-1248-2


R.T.: 4.790 min
Delta R.T.: -0.004 min
Response: 58434
Conc: 50.67 ng/ml



#23 AR-1248-3


R.T.: 5.763 min
Delta R.T.: -0.005 min
Response: 22235
Conc: 13.38 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019




#23 AR-1248-3

R.T.: 4.830 min
Delta R.T.: -0.005 min
Response: 51968
Conc: 43.75 ng/ml




#24 AR-1248-4

R.T.: 6.198 min
Delta R.T.: 0.030 min
Response: 67637
Conc: 33.09 ng/ml

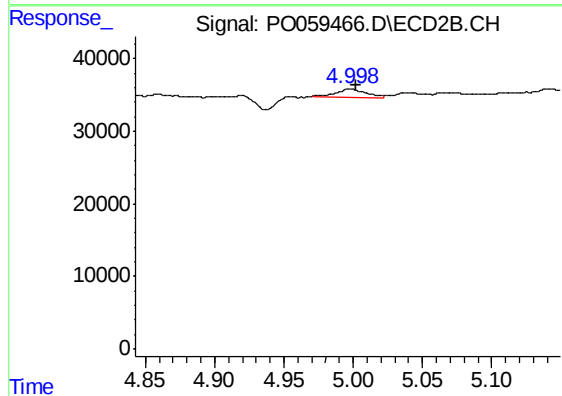

#24 AR-1248-4


R.T.: 4.998 min
Delta R.T.: -0.005 min
Response: 16266
Conc: 11.19 ng/ml

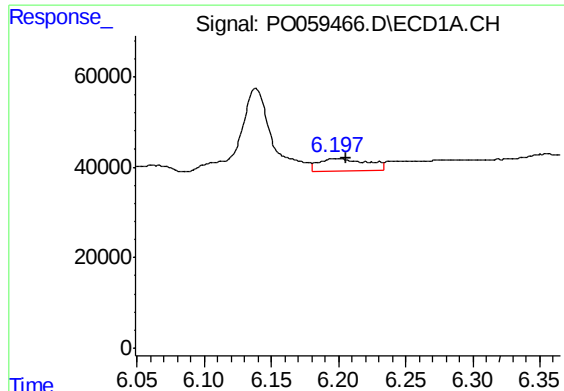

#25 AR-1248-5


R.T.: 6.198 min
Delta R.T.: -0.007 min
Response: 67637
Conc: 34.11 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

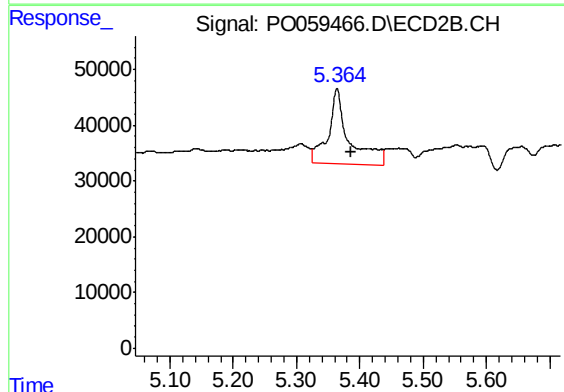


#25 AR-1248-5

R.T.: 5.364 min
Delta R.T.: -0.023 min
Response: 312760
Conc: 218.52 ng/ml

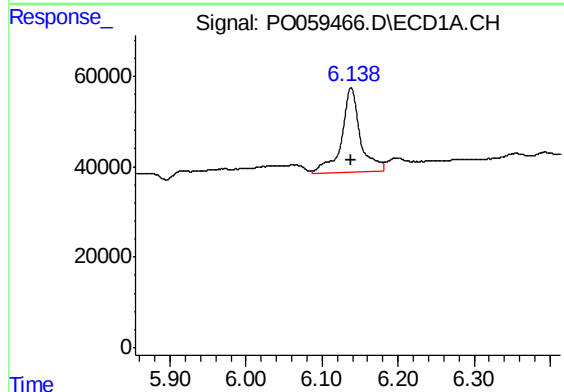


#26 AR-1254-1

R.T.: 6.138 min
Delta R.T.: 0.000 min
Response: 321332
Conc: 154.01 ng/ml

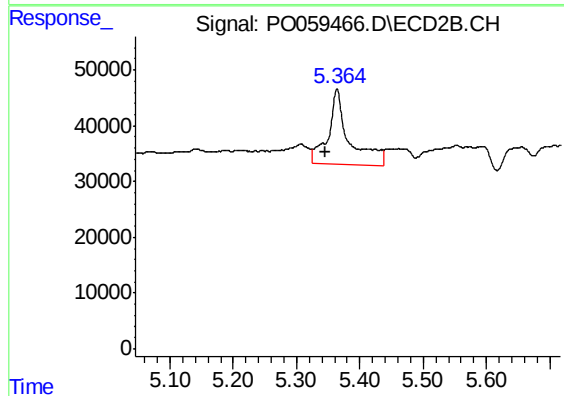

#26 AR-1254-1


R.T.: 5.364 min
Delta R.T.: 0.017 min
Response: 312760
Conc: 131.87 ng/ml

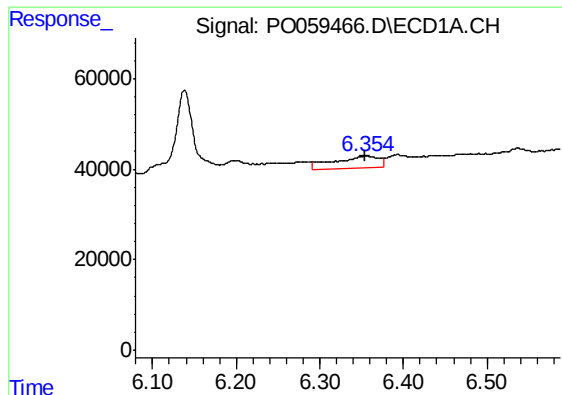

#27 AR-1254-2


R.T.: 6.355 min
Delta R.T.: 0.000 min
Response: 103009
Conc: 30.88 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

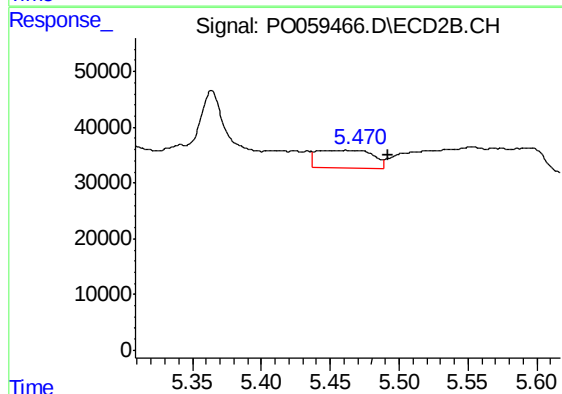


#27 AR-1254-2

R.T.: 5.460 min
Delta R.T.: -0.032 min
Response: 90823
Conc: 43.28 ng/ml

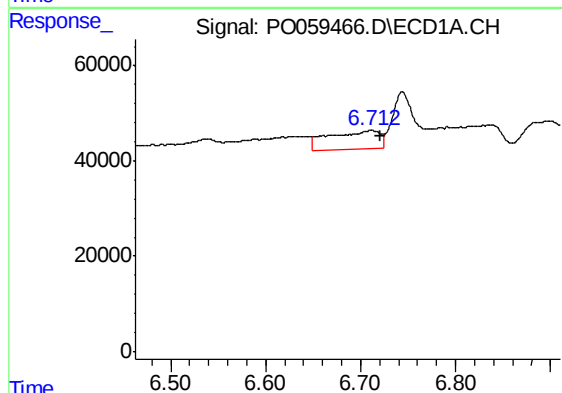


#28 AR-1254-3

R.T.: 6.711 min
Delta R.T.: -0.009 min
Response: 139980
Conc: 39.45 ng/ml

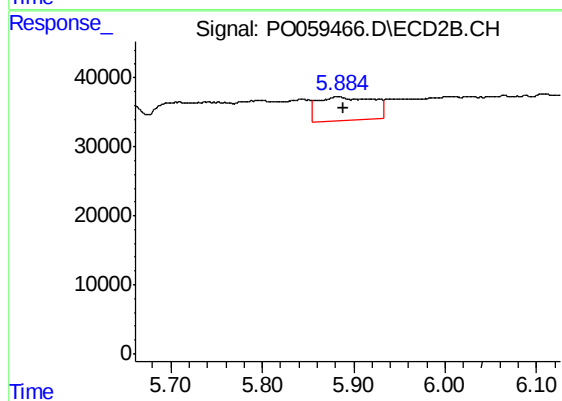

#28 AR-1254-3


R.T.: 5.884 min
Delta R.T.: -0.005 min
Response: 140841
Conc: 41.89 ng/ml



#29 AR-1254-4


R.T.: 6.996 min
Delta R.T.: -0.009 min
Response: 191099
Conc: 64.88 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019




#29 AR-1254-4

R.T.: 6.109 min
Delta R.T.: -0.006 min
Response: 35007
Conc: 16.98 ng/ml




#30 AR-1254-5

R.T.: 7.443 min
Delta R.T.: 0.024 min
Response: 32839
Conc: 10.62 ng/ml

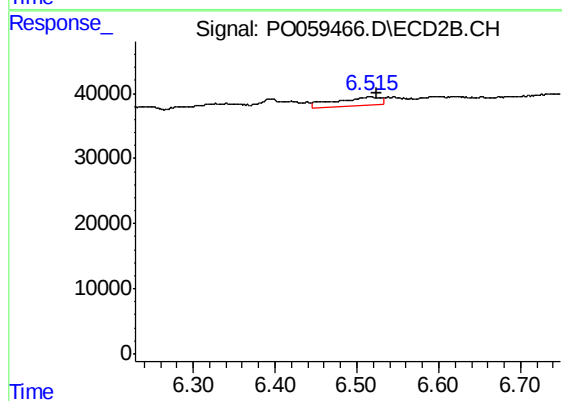

#30 AR-1254-5


R.T.: 6.515 min
Delta R.T.: -0.009 min
Response: 52412
Conc: 16.88 ng/ml

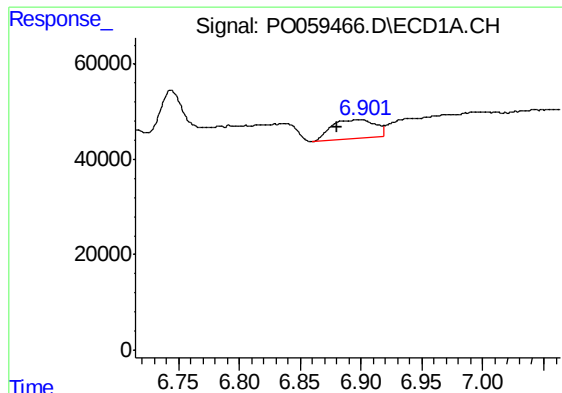

#31 AR-1260-1


R.T.: 6.900 min
Delta R.T.: 0.021 min
Response: 98508
Conc: 36.54 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

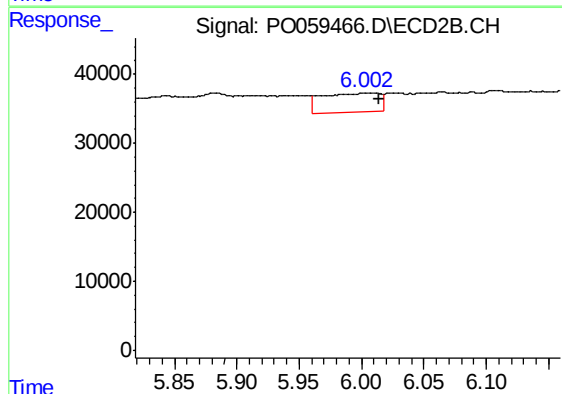


#31 AR-1260-1

R.T.: 6.003 min
Delta R.T.: -0.011 min
Response: 86714
Conc: 38.05 ng/ml




#32 AR-1260-2

R.T.: 7.136 min
Delta R.T.: 0.000 min
Response: 10752
Conc: 2.90 ng/ml

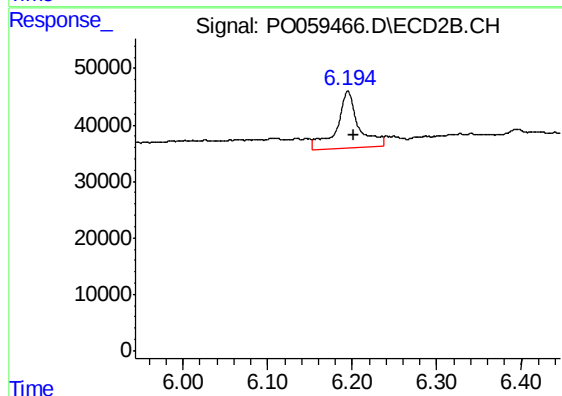

#32 AR-1260-2


R.T.: 6.195 min
Delta R.T.: -0.007 min
Response: 178073
Conc: 60.78 ng/ml



#33 AR-1260-3


R.T.: 7.482 min
Delta R.T.: -0.008 min
Response: 20681
Conc: 6.31 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019




#33 AR-1260-3

R.T.: 6.341 min
Delta R.T.: -0.011 min
Response: 27211
Conc: 10.27 ng/ml




#34 AR-1260-4

R.T.: 7.706 min
Delta R.T.: -0.011 min
Response: 32626
Conc: 10.62 ng/ml

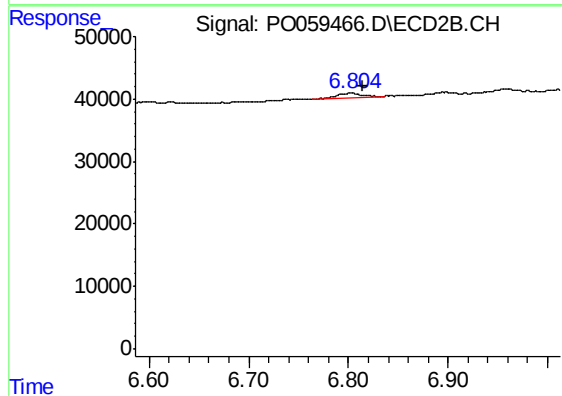

#34 AR-1260-4


R.T.: 6.803 min
Delta R.T.: -0.011 min
Response: 16192
Conc: 7.16 ng/ml

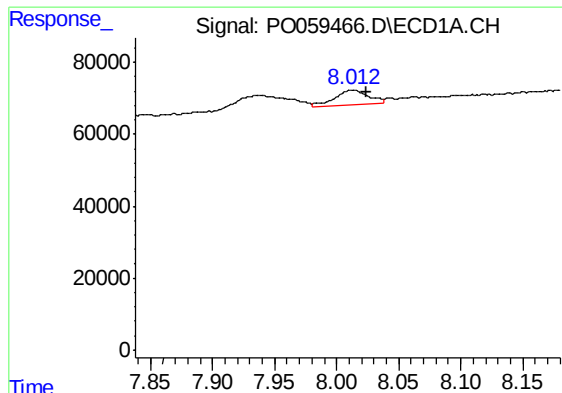

#35 AR-1260-5


R.T.: 8.013 min
Delta R.T.: -0.011 min
Response: 76314
Conc: 10.78 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019




#35 AR-1260-5

R.T.: 7.045 min
Delta R.T.: -0.012 min
Response: 53823
Conc: 9.78 ng/ml




#36 AR-1262-1

R.T.: 7.482 min
Delta R.T.: -0.006 min
Response: 20681
Conc: 4.26 ng/ml

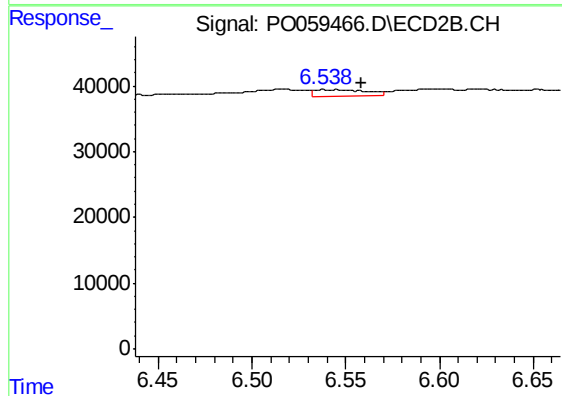

#36 AR-1262-1


R.T.: 6.538 min
Delta R.T.: -0.020 min
Response: 19017
Conc: 5.10 ng/ml



#37 AR-1262-2


R.T.: 8.013 min
Delta R.T.: -0.010 min
Response: 76314
Conc: 9.89 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019




#37 AR-1262-2

R.T.: 7.045 min
Delta R.T.: -0.013 min
Response: 53823
Conc: 9.15 ng/ml




#38 AR-1262-3

R.T.: 8.314 min
Delta R.T.: 0.011 min
Response: 33524
Conc: 6.57 ng/ml

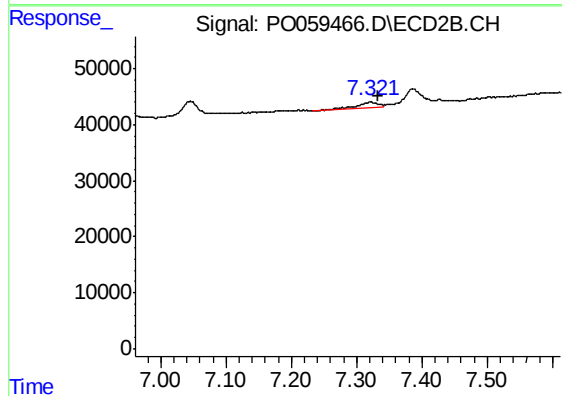

#38 AR-1262-3


R.T.: 7.321 min
Delta R.T.: -0.011 min
Response: 22557
Conc: 8.88 ng/ml

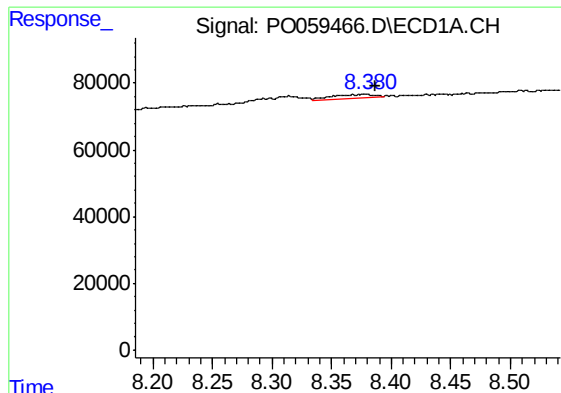

#39 AR-1262-4


R.T.: 8.379 min
Delta R.T.: -0.007 min
Response: 26948
Conc: 6.99 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

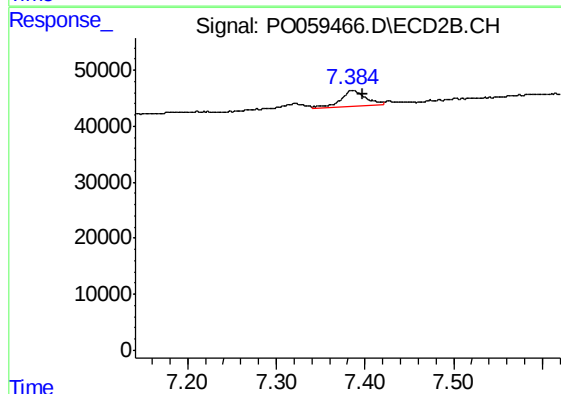


#39 AR-1262-4

R.T.: 7.386 min
Delta R.T.: -0.012 min
Response: 51574
Conc: 11.67 ng/ml

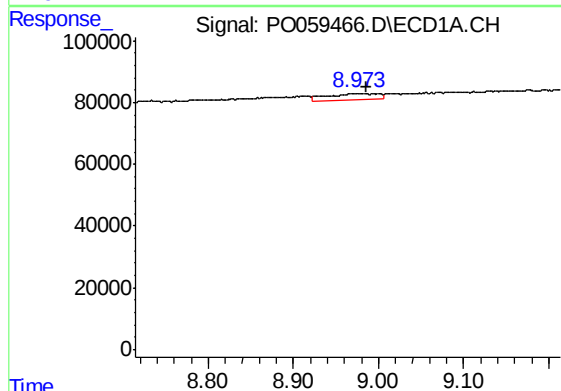


#40 AR-1262-5

R.T.: 8.974 min
Delta R.T.: -0.011 min
Response: 79376
Conc: 30.93 ng/ml

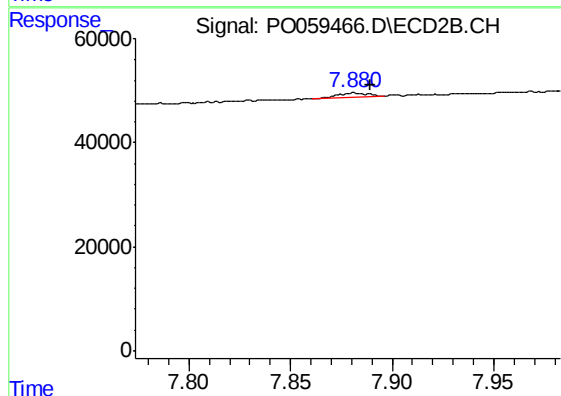

#40 AR-1262-5


R.T.: 7.881 min
Delta R.T.: -0.009 min
Response: 9700
Conc: 5.37 ng/ml



#41 AR-1268-1


R.T.: 8.314 min
Delta R.T.: 0.012 min
Response: 33524
Conc: 3.56 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

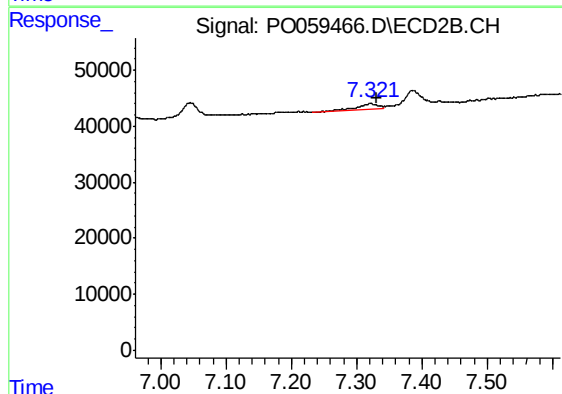


#41 AR-1268-1

R.T.: 7.321 min
Delta R.T.: -0.009 min
Response: 22557
Conc: 3.17 ng/ml

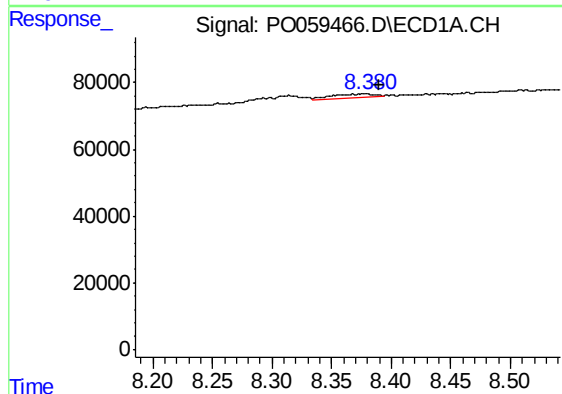


#42 AR-1268-2

R.T.: 8.379 min
Delta R.T.: -0.011 min
Response: 26948
Conc: 3.42 ng/ml

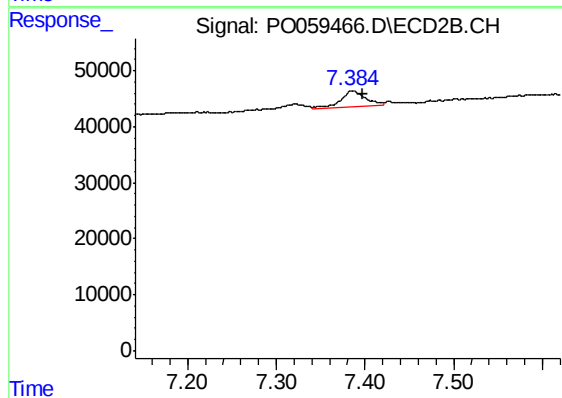

#42 AR-1268-2


R.T.: 7.386 min
Delta R.T.: -0.012 min
Response: 51574
Conc: 8.00 ng/ml



#43 AR-1268-3


R.T.: 8.620 min
Delta R.T.: 0.032 min
Response: 41273
Conc: 5.86 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019




#43 AR-1268-3

R.T.: 0.000 min
Exp R.T. : 7.592 min
Response: 0
Conc: N.D.




#44 AR-1268-4

R.T.: 8.974 min
Delta R.T.: -0.011 min
Response: 79376
Conc: 28.55 ng/ml

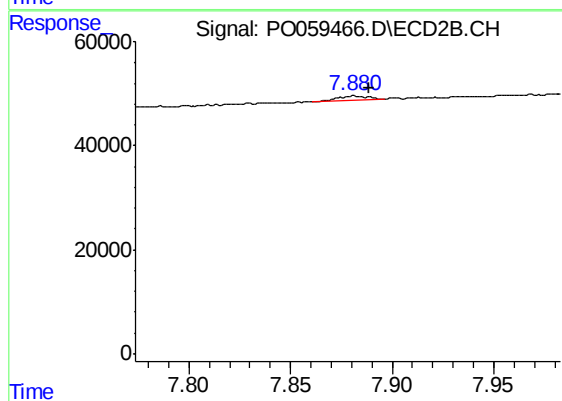

#44 AR-1268-4


R.T.: 7.881 min
Delta R.T.: -0.008 min
Response: 9700
Conc: 4.75 ng/ml

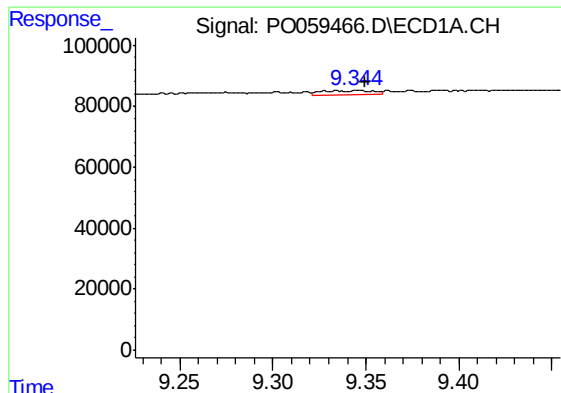

#45 AR-1268-5

R.T.: 9.345 min
Delta R.T.: -0.005 min
Response: 25177
Conc: 1.37 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

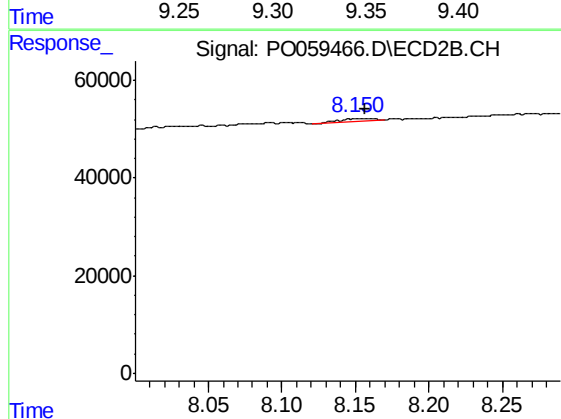

#45 AR-1268-5

R.T.: 8.152 min
Delta R.T.: -0.005 min
Response: 9105
Conc: 0.63 ng/ml