

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081919\
 Data File : P0059467.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Aug 2019 19:26
 Operator : SM/AJ
 Sample : K3591-09
 Misc : AR1248 MDL 25PPB
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-MDL-WATER-03-QT3-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 20 01:08:36 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 17 03:09:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.141	3.506	578057	536284	16.510	14.899
2)	SA Decachlor...	9.628	8.377	977011	736201	18.365	18.258
Target Compounds							
3)	L1 AR-1016-1	5.294	4.559	27263	21969	16.998	16.250
4)	L1 AR-1016-2	5.315	4.575	30213	22194	12.628	11.080
5)	L1 AR-1016-3	5.375	4.748	18213	13219	12.227	12.219
6)	L1 AR-1016-4	5.473	4.789	17473	28767	14.444	31.857 #
7)	L1 AR-1016-5	5.761	4.997	46044	33385	35.856	28.982
9)	L2 AR-1221-2	4.442	3.798	12772	10923	39.323	35.857
10)	L2 AR-1221-3	4.513	0.000	6780	0	6.446	N.D. #
11)	L3 AR-1232-1	4.513	0.000	6780	0	5.440	N.D. #
12)	L3 AR-1232-2	5.029	4.575	13287	22194	18.810	17.427
13)	L3 AR-1232-3	5.315	4.748	30213	13219	19.729	19.413
14)	L3 AR-1232-4	5.473	4.829	17473	27309	22.348	44.764 #
15)	L3 AR-1232-5	5.560	4.997	42983	33385	71.503	49.042 #
16)	L4 AR-1242-1	5.294	4.559	27263	21969	21.475	21.356
17)	L4 AR-1242-2	5.315	4.575	30213	22194	16.281	14.572
18)	L4 AR-1242-3	5.375	4.748	18213	13219	15.582	15.821
19)	L4 AR-1242-4	5.473	4.829	17473	27309	18.053	32.729 #
20)	L4 AR-1242-5	6.197	5.342	57294	59873	45.594	53.525
21)	L5 AR-1248-1	5.294	4.559	27263	21969	27.194	26.531
22)	L5 AR-1248-2	5.560	4.789	42983	28767	29.625	24.947
23)	L5 AR-1248-3	5.761	4.829	46044	27309	27.703	22.992
24)	L5 AR-1248-4	6.161	4.997	61476	33385	30.075	22.975
25)	L5 AR-1248-5	6.197	5.381	57294	40981	28.891	28.632
26)	L6 AR-1254-1	6.131	5.342	92636	59873	44.399	25.244 #
27)	L6 AR-1254-2	6.354	5.486	60037	23757	17.995	11.322 #
28)	L6 AR-1254-3	6.713	5.882	32343	29906	9.115	8.894
29)	L6 AR-1254-4	6.997	6.109	29517	19017	10.021	9.223
30)	L6 AR-1254-5	7.416	6.519	14562	26247	4.709	8.453 #
31)	L7 AR-1260-1	6.881	6.024	5881	16495	2.182	7.238 #
32)	L7 AR-1260-2	7.123	6.196	17614	22403	4.747	7.646 #
33)	L7 AR-1260-3	7.484	6.344	12649	17653	3.861	6.664 #
34)	L7 AR-1260-4	7.702	6.804	23579	18649	7.677	8.242
35)	L7 AR-1260-5	8.012	7.046	87369	73524	12.339	13.360
36)	L8 AR-1262-1	7.484	6.519	12649	26247	2.607	7.041 #
37)	L8 AR-1262-2	8.012	7.046	87369	73524	11.323	12.506
38)	L8 AR-1262-3	8.315	7.323	48164	27258	9.440	10.728
39)	L8 AR-1262-4	8.401	7.388	6468	57128	1.678	12.928 #
40)	L8 AR-1262-5	8.976	7.882	62282	15414	24.267	8.537 #
41)	L9 AR-1268-1	8.315	7.323	48164	27258	5.118	3.828 #
42)	L9 AR-1268-2	8.401	7.388	6468	57128	0.821	8.860 #
43)	L9 AR-1268-3	8.588	7.590	21484	11127	3.048	2.034 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081919\
 Data File : P0059467.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Aug 2019 19:26
 Operator : SM/AJ
 Sample : K3591-09
 Misc : AR1248 MDL 25PPB
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-MDL-WATER-03-QT3-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 20 01:08:36 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 17 03:09:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
44) L9	AR-1268-4	8.976	7.882	62282	15414	22.403	7.551 #
45) L9	AR-1268-5	9.333	8.152	66126	8279	3.586	0.570 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081919\
Data File : PO059467.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Aug 2019 19:26
Operator : SM/AJ
Sample : K3591-09
Misc : AR1248 MDL 25PPB
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 20 01:08:36 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Aug 17 03:09:44 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

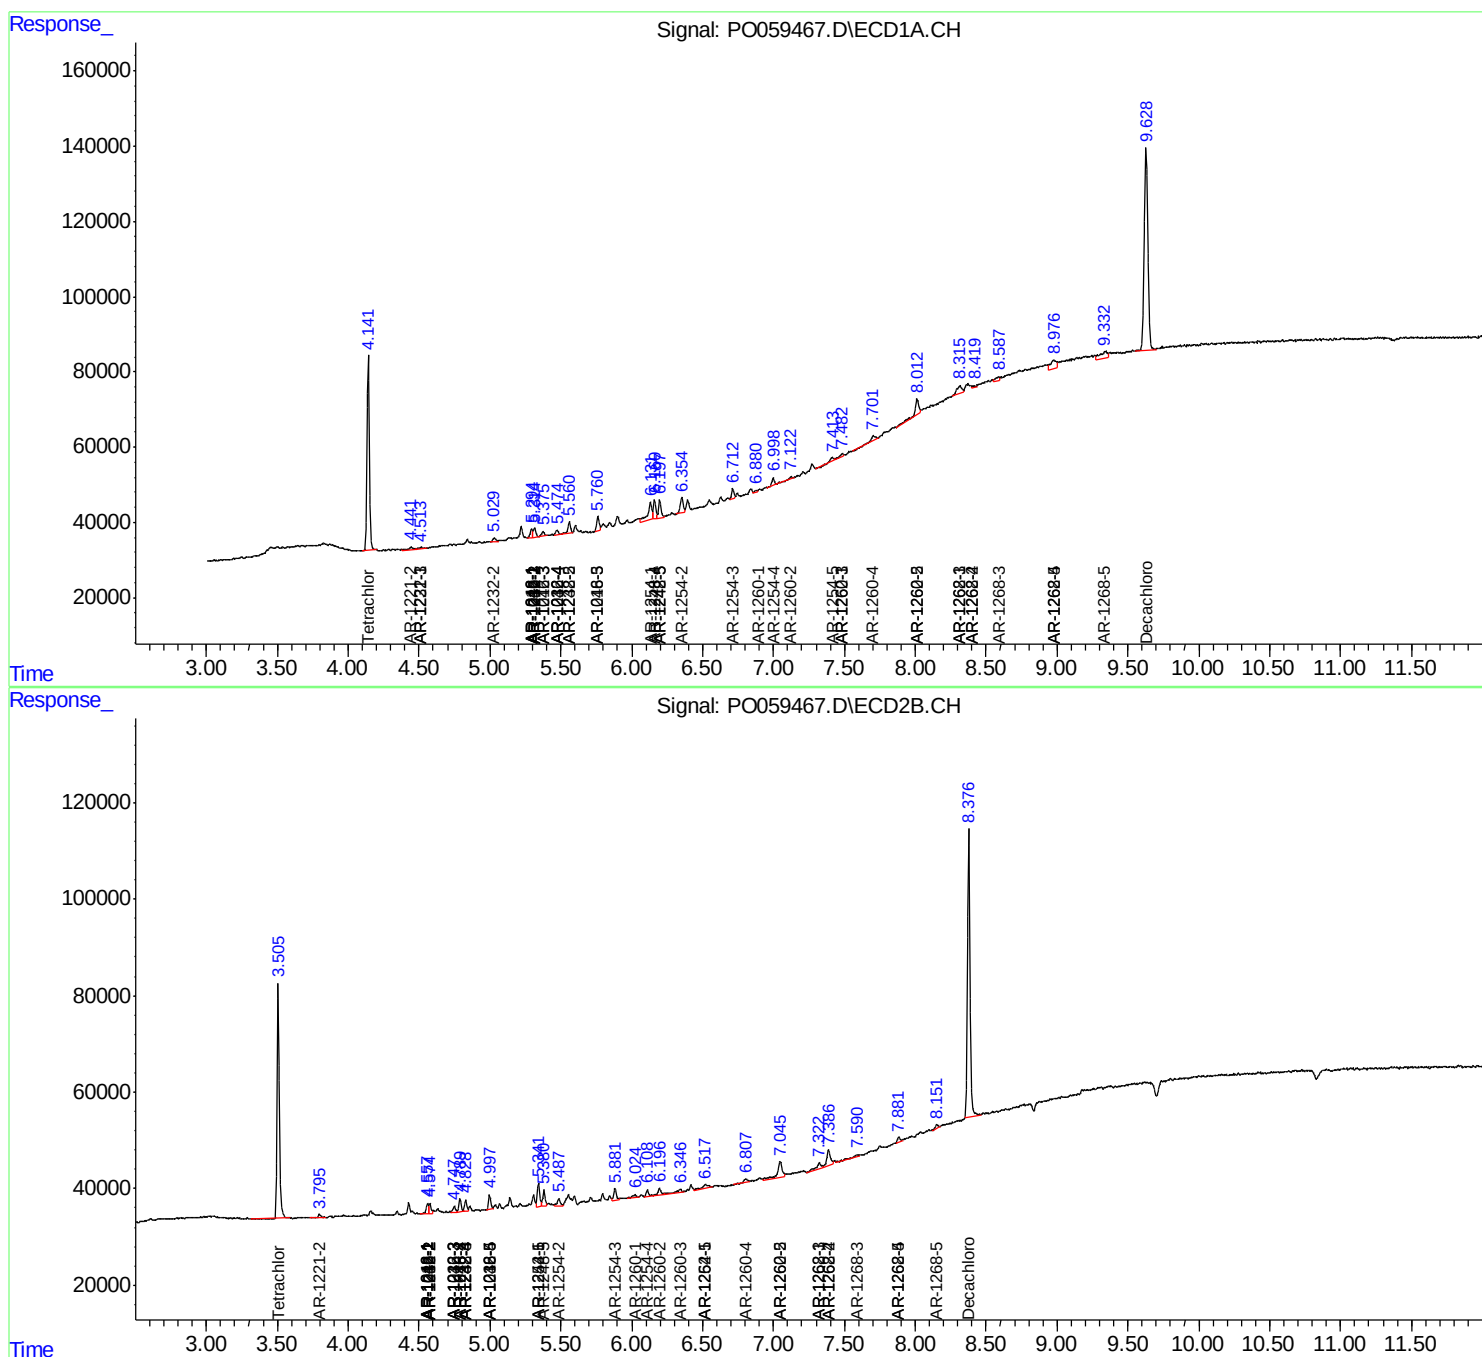




#1 Tetrachloro-m-xylene


R.T.: 4.141 min
Delta R.T.: -0.008 min
Response: 578057
Conc: 16.51 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019




#1 Tetrachloro-m-xylene

R.T.: 3.506 min
Delta R.T.: -0.004 min
Response: 536284
Conc: 14.90 ng/ml

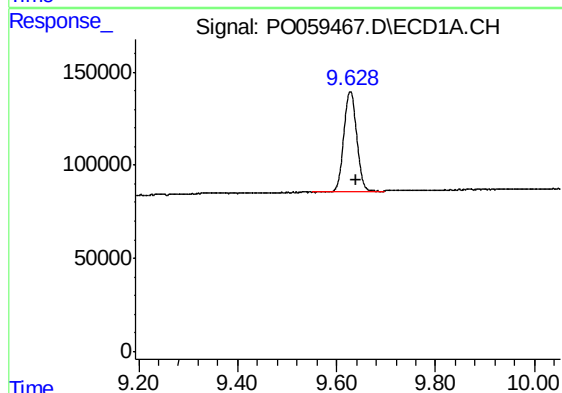


#2 Decachlorobiphenyl

R.T.: 9.628 min
Delta R.T.: -0.013 min
Response: 977011
Conc: 18.36 ng/ml

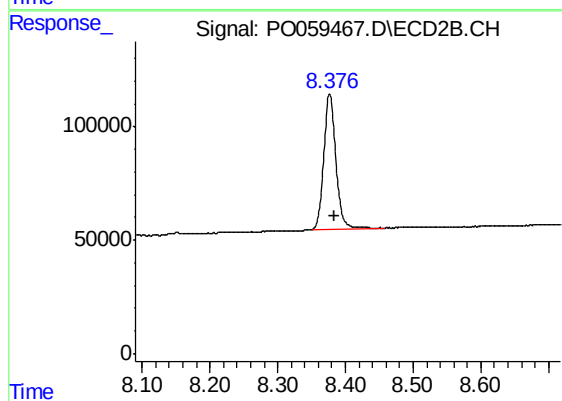

#2 Decachlorobiphenyl


R.T.: 8.377 min
Delta R.T.: -0.006 min
Response: 736201
Conc: 18.26 ng/ml

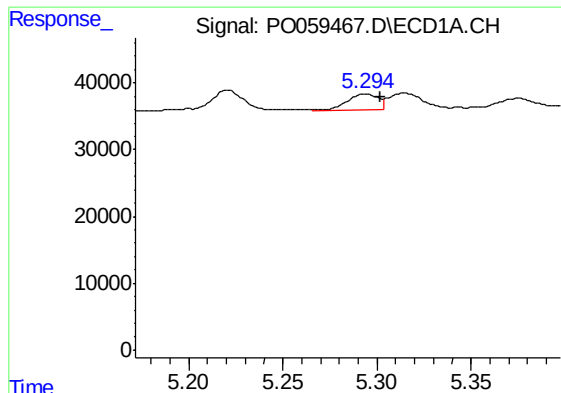

#3 AR-1016-1


R.T.: 5.294 min
Delta R.T.: -0.008 min
Response: 27263
Conc: 17.00 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

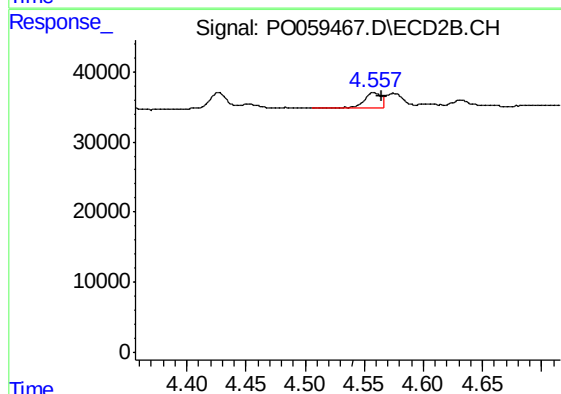


#3 AR-1016-1

R.T.: 4.559 min
Delta R.T.: -0.006 min
Response: 21969
Conc: 16.25 ng/ml

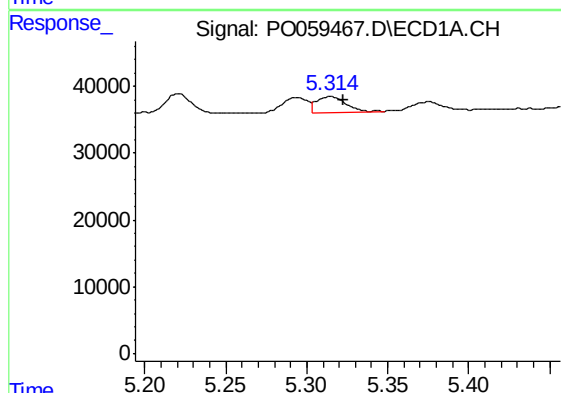


#4 AR-1016-2

R.T.: 5.315 min
Delta R.T.: -0.008 min
Response: 30213
Conc: 12.63 ng/ml

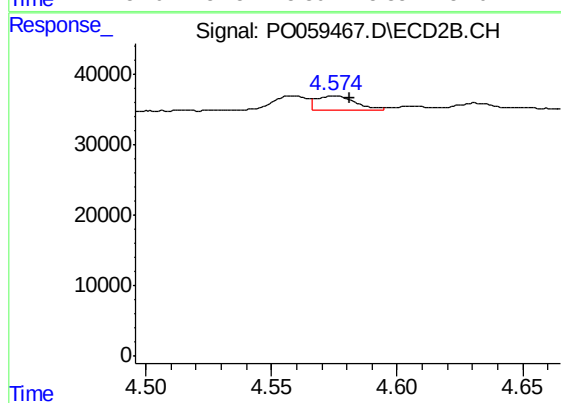

#4 AR-1016-2


R.T.: 4.575 min
Delta R.T.: -0.006 min
Response: 22194
Conc: 11.08 ng/ml

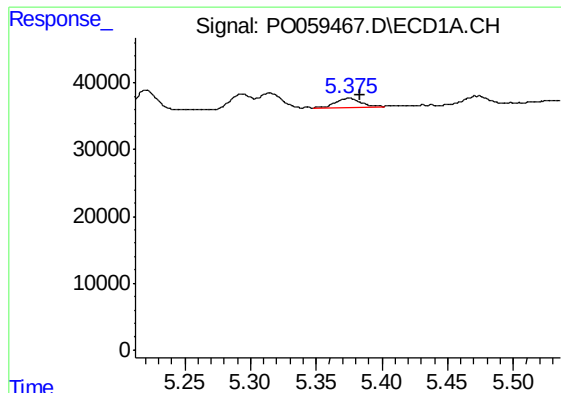

#5 AR-1016-3


R.T.: 5.375 min
Delta R.T.: -0.008 min
Response: 18213
Conc: 12.23 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

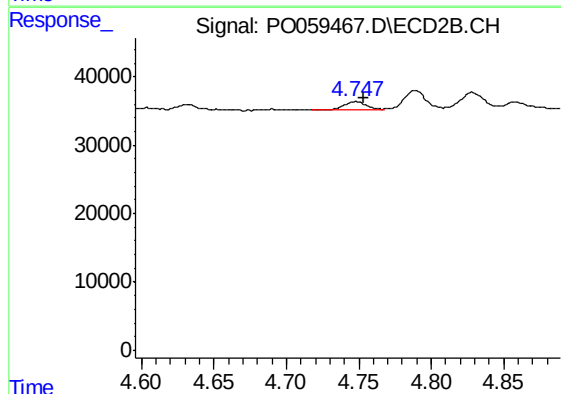


#5 AR-1016-3

R.T.: 4.748 min
Delta R.T.: -0.006 min
Response: 13219
Conc: 12.22 ng/ml

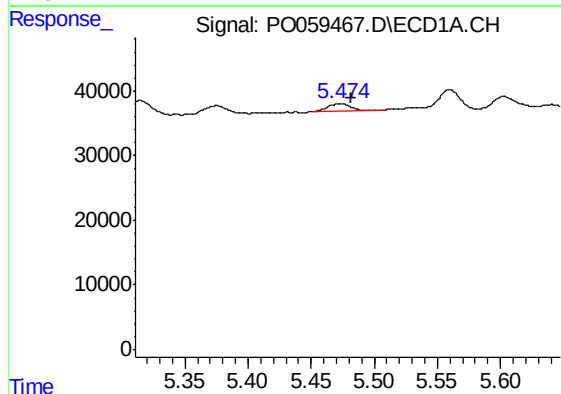


#6 AR-1016-4

R.T.: 5.473 min
Delta R.T.: -0.008 min
Response: 17473
Conc: 14.44 ng/ml

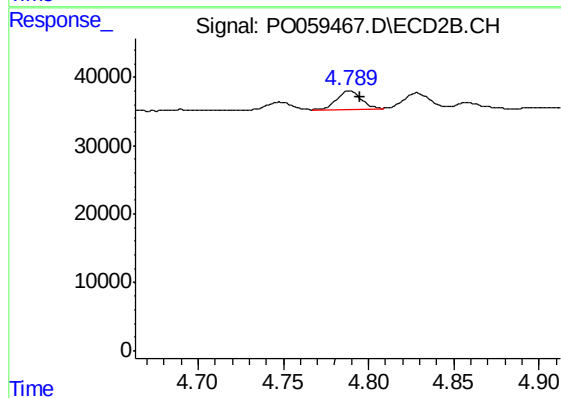

#6 AR-1016-4


R.T.: 4.789 min
Delta R.T.: -0.006 min
Response: 28767
Conc: 31.86 ng/ml

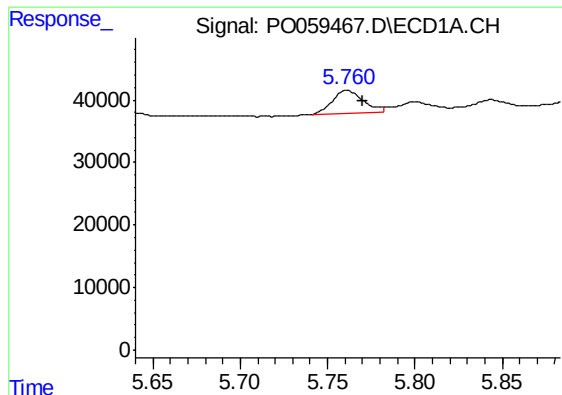

#7 AR-1016-5


R.T.: 5.761 min
Delta R.T.: -0.009 min
Response: 46044
Conc: 35.86 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

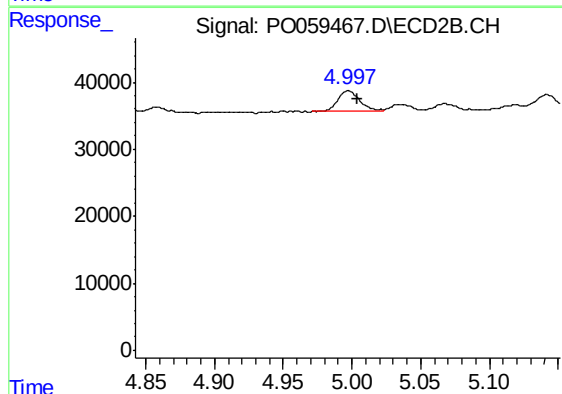


#7 AR-1016-5

R.T.: 4.997 min
Delta R.T.: -0.006 min
Response: 33385
Conc: 28.98 ng/ml

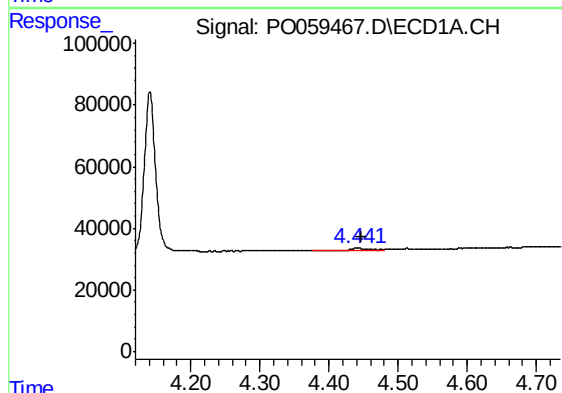


#9 AR-1221-2

R.T.: 4.442 min
Delta R.T.: -0.005 min
Response: 12772
Conc: 39.32 ng/ml

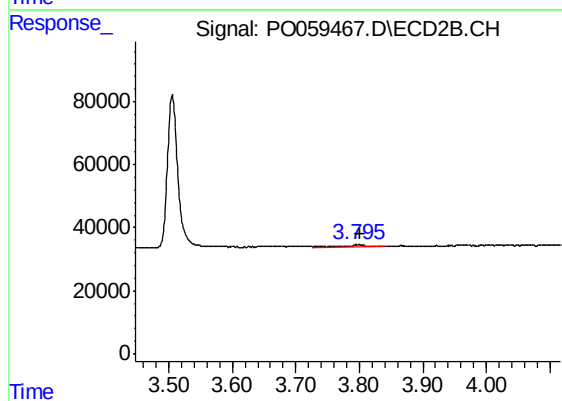

#9 AR-1221-2


R.T.: 3.798 min
Delta R.T.: -0.003 min
Response: 10923
Conc: 35.86 ng/ml

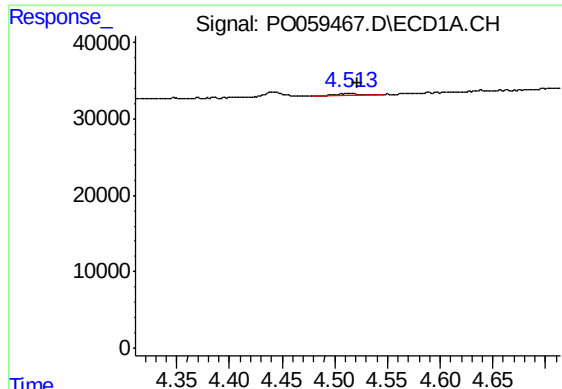

#10 AR-1221-3


R.T.: 4.513 min
Delta R.T.: -0.009 min
Response: 6780
Conc: 6.45 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019




#10 AR-1221-3

R.T.: 0.000 min
Exp R.T. : 3.874 min
Response: 0
Conc: N.D.




#11 AR-1232-1

R.T.: 4.513 min
Delta R.T.: -0.008 min
Response: 6780
Conc: 5.44 ng/ml

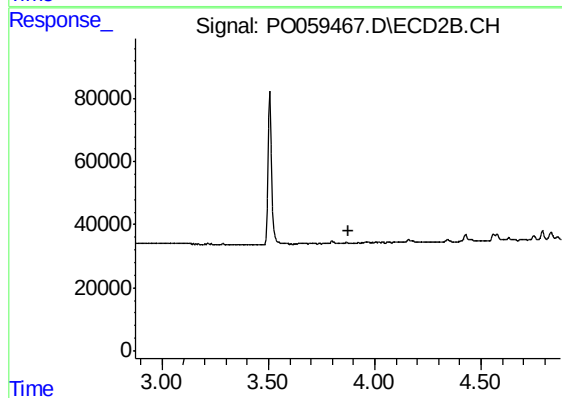

#11 AR-1232-1


R.T.: 0.000 min
Exp R.T. : 3.874 min
Response: 0
Conc: N.D.

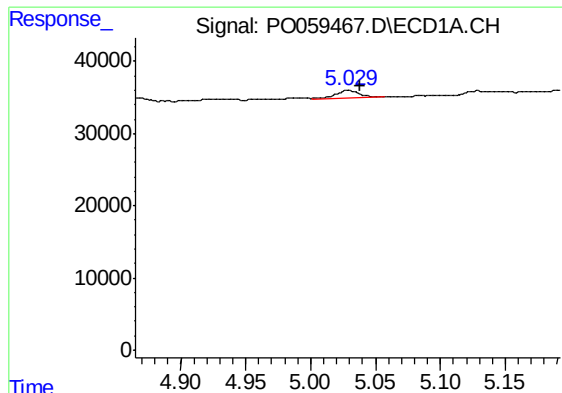

#12 AR-1232-2


R.T.: 5.029 min
Delta R.T.: -0.009 min
Response: 13287
Conc: 18.81 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

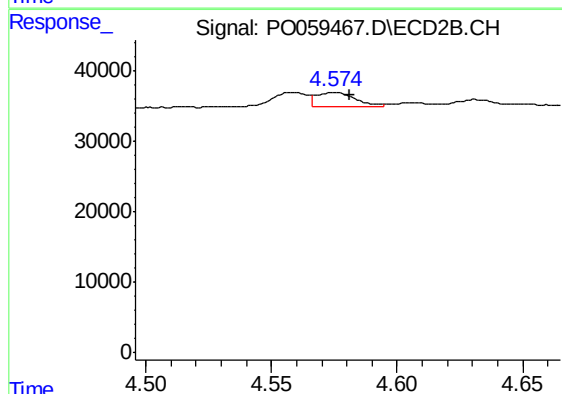


#12 AR-1232-2

R.T.: 4.575 min
Delta R.T.: -0.006 min
Response: 22194
Conc: 17.43 ng/ml

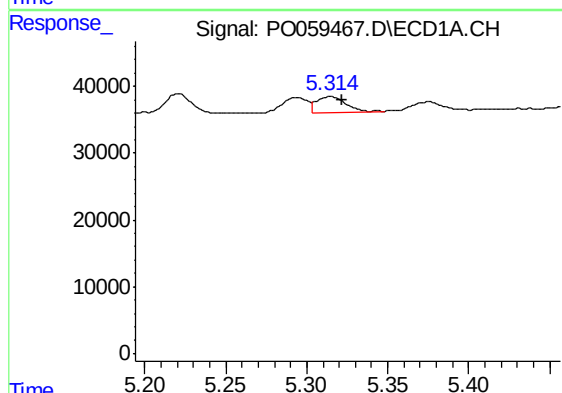


#13 AR-1232-3

R.T.: 5.315 min
Delta R.T.: -0.007 min
Response: 30213
Conc: 19.73 ng/ml

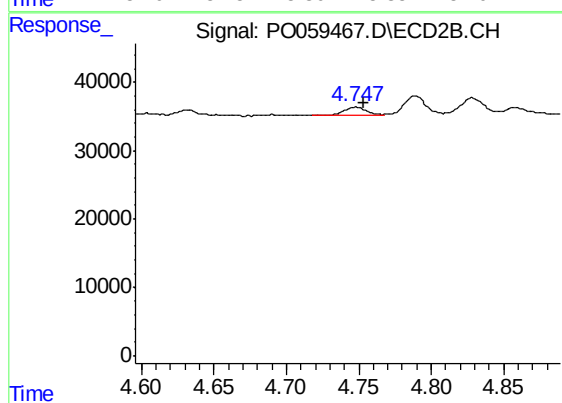

#13 AR-1232-3


R.T.: 4.748 min
Delta R.T.: -0.005 min
Response: 13219
Conc: 19.41 ng/ml

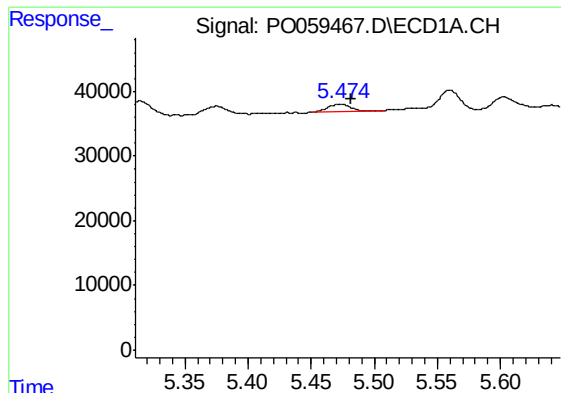

#14 AR-1232-4


R.T.: 5.473 min
Delta R.T.: -0.008 min
Response: 17473
Conc: 22.35 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

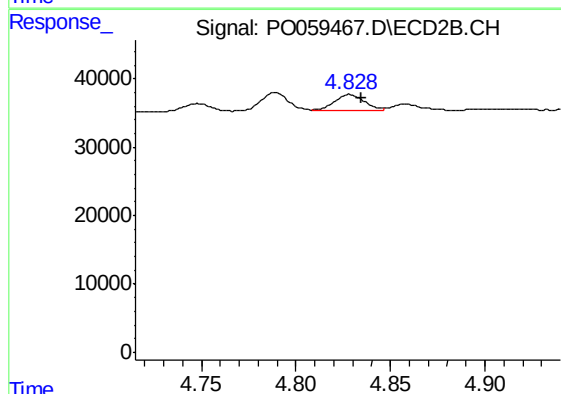


#14 AR-1232-4

R.T.: 4.829 min
Delta R.T.: -0.006 min
Response: 27309
Conc: 44.76 ng/ml

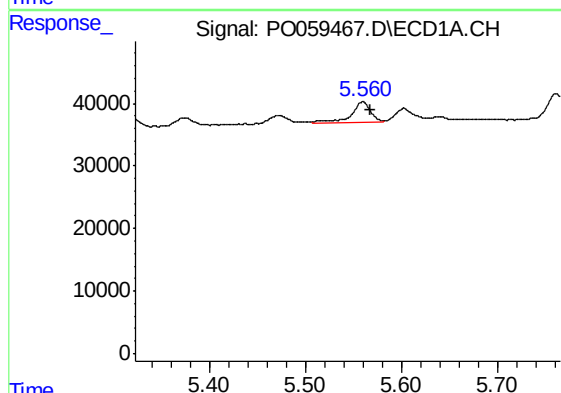


#15 AR-1232-5

R.T.: 5.560 min
Delta R.T.: -0.008 min
Response: 42983
Conc: 71.50 ng/ml

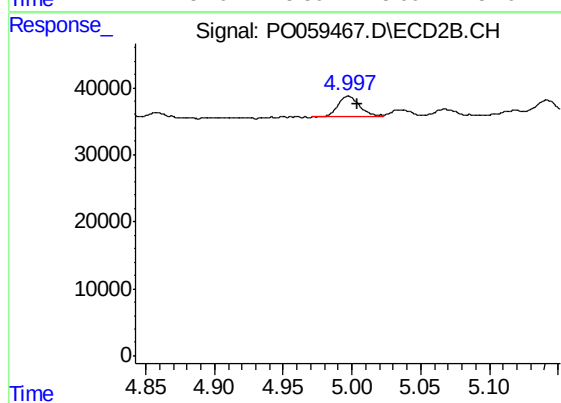

#15 AR-1232-5


R.T.: 4.997 min
Delta R.T.: -0.006 min
Response: 33385
Conc: 49.04 ng/ml



#16 AR-1242-1


R.T.: 5.294 min
Delta R.T.: -0.007 min
Response: 27263
Conc: 21.48 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019




#16 AR-1242-1

R.T.: 4.559 min
Delta R.T.: -0.006 min
Response: 21969
Conc: 21.36 ng/ml




#17 AR-1242-2

R.T.: 5.315 min
Delta R.T.: -0.008 min
Response: 30213
Conc: 16.28 ng/ml

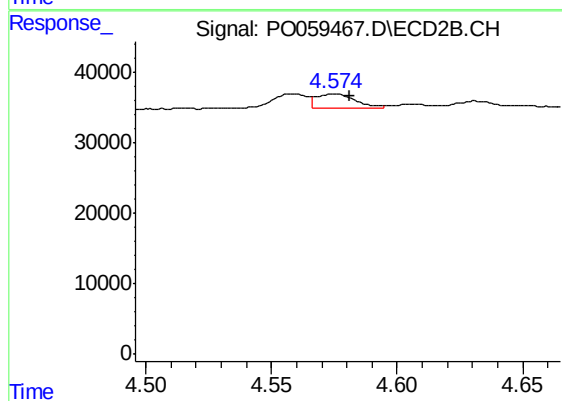

#17 AR-1242-2


R.T.: 4.575 min
Delta R.T.: -0.007 min
Response: 22194
Conc: 14.57 ng/ml

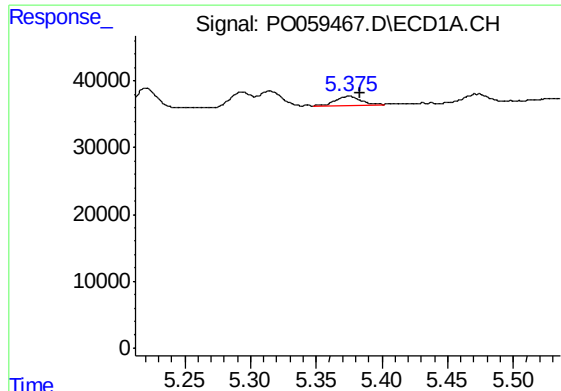

#18 AR-1242-3


R.T.: 5.375 min
Delta R.T.: -0.008 min
Response: 18213
Conc: 15.58 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

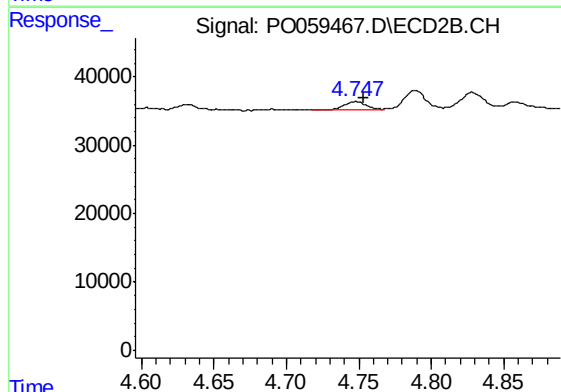


#18 AR-1242-3

R.T.: 4.748 min
Delta R.T.: -0.006 min
Response: 13219
Conc: 15.82 ng/ml

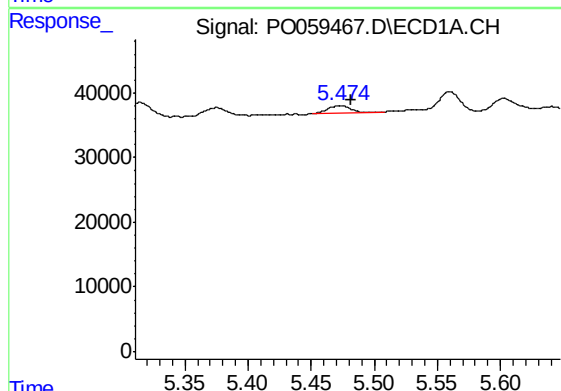


#19 AR-1242-4

R.T.: 5.473 min
Delta R.T.: -0.009 min
Response: 17473
Conc: 18.05 ng/ml

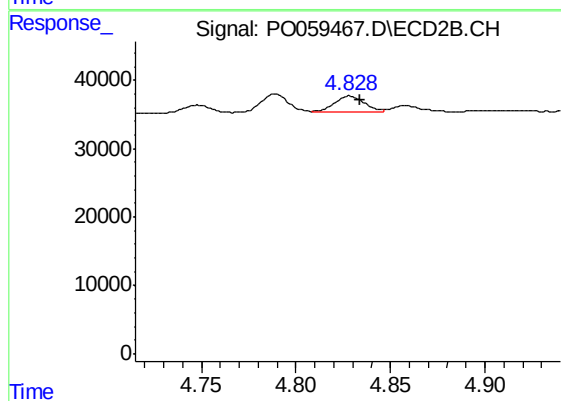

#19 AR-1242-4


R.T.: 4.829 min
Delta R.T.: -0.006 min
Response: 27309
Conc: 32.73 ng/ml



#20 AR-1242-5


R.T.: 6.197 min
Delta R.T.: -0.008 min
Response: 57294
Conc: 45.59 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

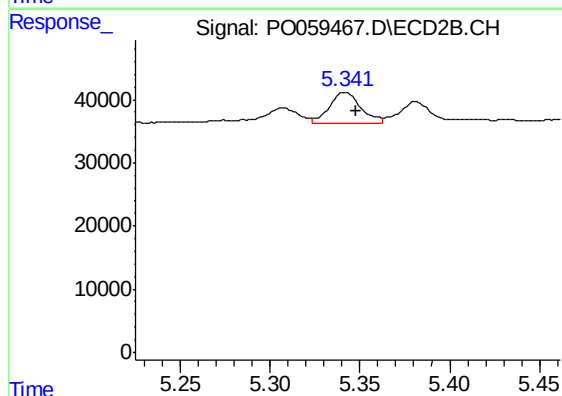


#20 AR-1242-5

R.T.: 5.342 min
Delta R.T.: -0.006 min
Response: 59873
Conc: 53.53 ng/ml

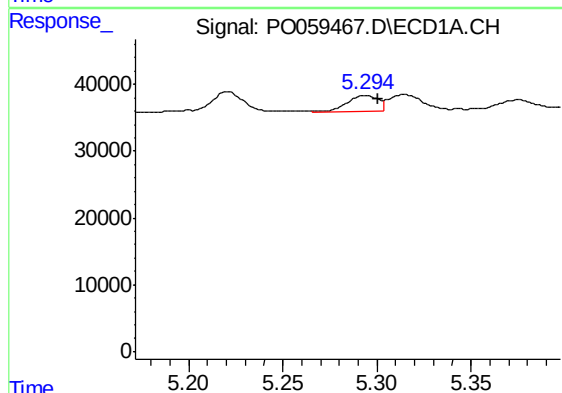


#21 AR-1248-1

R.T.: 5.294 min
Delta R.T.: -0.007 min
Response: 27263
Conc: 27.19 ng/ml

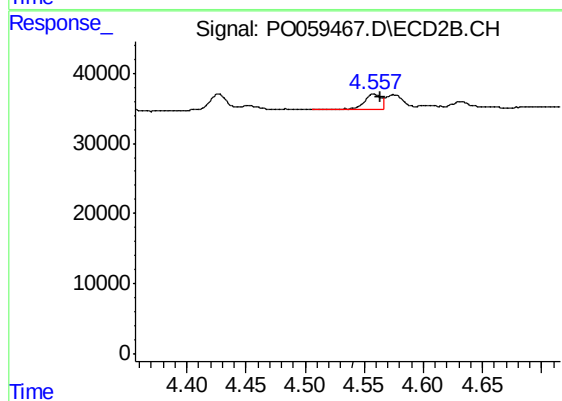

#21 AR-1248-1


R.T.: 4.559 min
Delta R.T.: -0.006 min
Response: 21969
Conc: 26.53 ng/ml

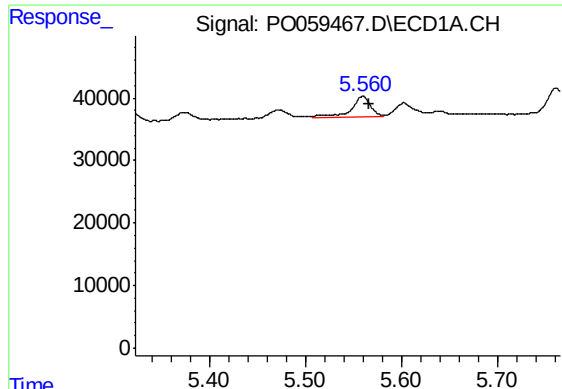

#22 AR-1248-2


R.T.: 5.560 min
Delta R.T.: -0.007 min
Response: 42983
Conc: 29.62 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019




#22 AR-1248-2

R.T.: 4.789 min
Delta R.T.: -0.005 min
Response: 28767
Conc: 24.95 ng/ml




#23 AR-1248-3

R.T.: 5.761 min
Delta R.T.: -0.007 min
Response: 46044
Conc: 27.70 ng/ml

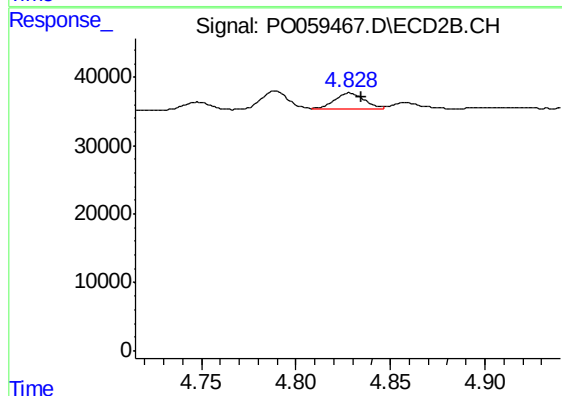

#23 AR-1248-3


R.T.: 4.829 min
Delta R.T.: -0.006 min
Response: 27309
Conc: 22.99 ng/ml



#24 AR-1248-4


R.T.: 6.161 min
Delta R.T.: -0.008 min
Response: 61476
Conc: 30.07 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

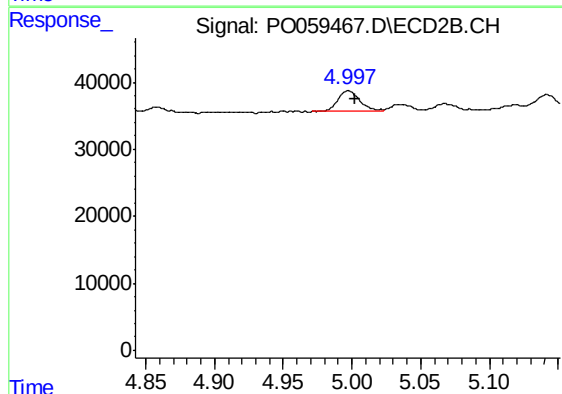


#24 AR-1248-4

R.T.: 4.997 min
Delta R.T.: -0.005 min
Response: 33385
Conc: 22.98 ng/ml




#25 AR-1248-5

R.T.: 6.197 min
Delta R.T.: -0.008 min
Response: 57294
Conc: 28.89 ng/ml

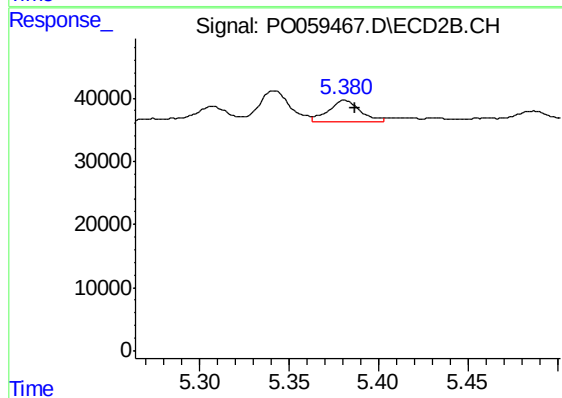

#25 AR-1248-5


R.T.: 5.381 min
Delta R.T.: -0.006 min
Response: 40981
Conc: 28.63 ng/ml



#26 AR-1254-1


R.T.: 6.131 min
Delta R.T.: -0.008 min
Response: 92636
Conc: 44.40 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

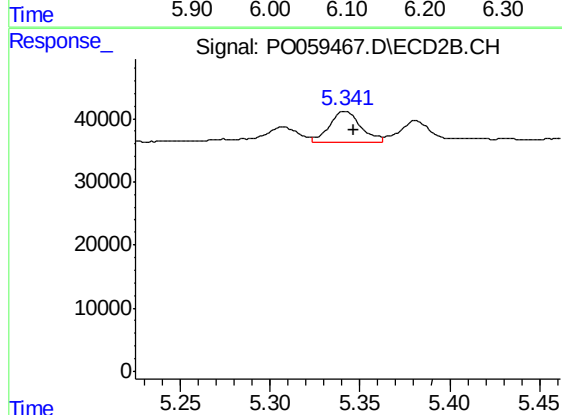


#26 AR-1254-1

R.T.: 5.342 min
Delta R.T.: -0.005 min
Response: 59873
Conc: 25.24 ng/ml

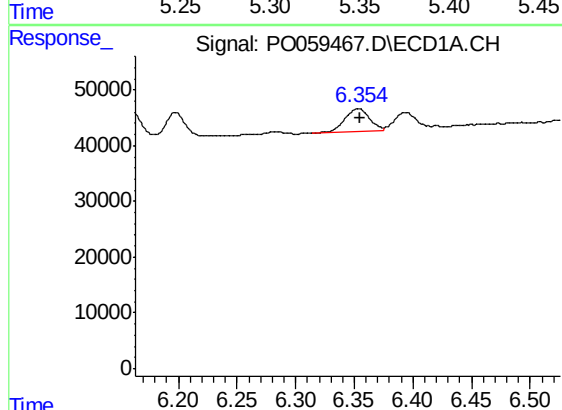


#27 AR-1254-2

R.T.: 6.354 min
Delta R.T.: 0.000 min
Response: 60037
Conc: 18.00 ng/ml

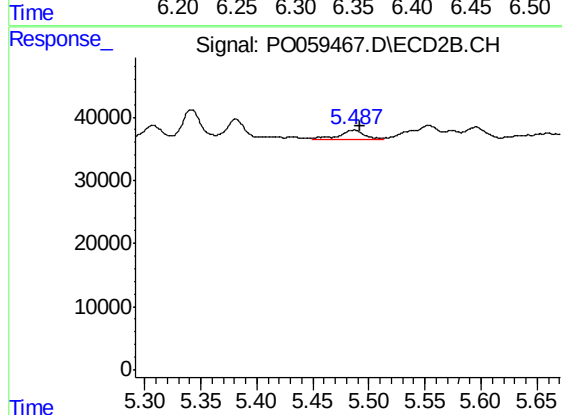

#27 AR-1254-2


R.T.: 5.486 min
Delta R.T.: -0.006 min
Response: 23757
Conc: 11.32 ng/ml

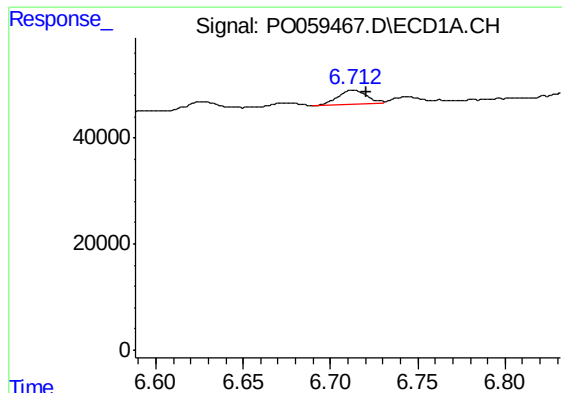

#28 AR-1254-3


R.T.: 6.713 min
Delta R.T.: -0.007 min
Response: 32343
Conc: 9.11 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

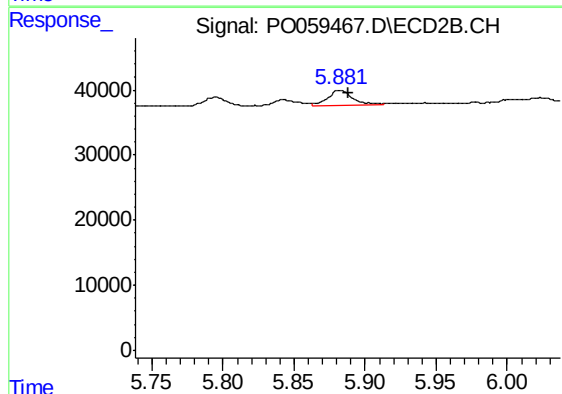


#28 AR-1254-3

R.T.: 5.882 min
Delta R.T.: -0.006 min
Response: 29906
Conc: 8.89 ng/ml




#29 AR-1254-4

R.T.: 6.997 min
Delta R.T.: -0.007 min
Response: 29517
Conc: 10.02 ng/ml

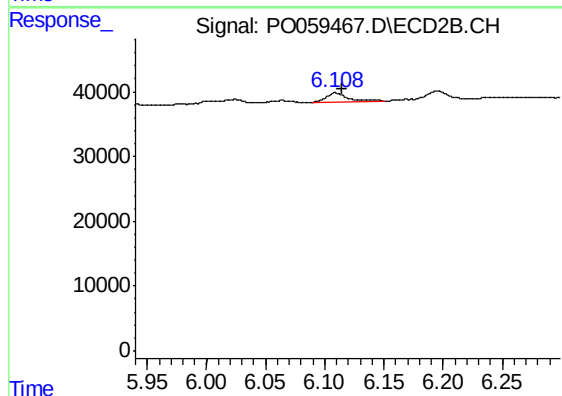

#29 AR-1254-4


R.T.: 6.109 min
Delta R.T.: -0.006 min
Response: 19017
Conc: 9.22 ng/ml



#30 AR-1254-5


R.T.: 7.416 min
Delta R.T.: -0.003 min
Response: 14562
Conc: 4.71 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019




#30 AR-1254-5

R.T.: 6.519 min
Delta R.T.: -0.006 min
Response: 26247
Conc: 8.45 ng/ml




#31 AR-1260-1

R.T.: 6.881 min
Delta R.T.: 0.002 min
Response: 5881
Conc: 2.18 ng/ml

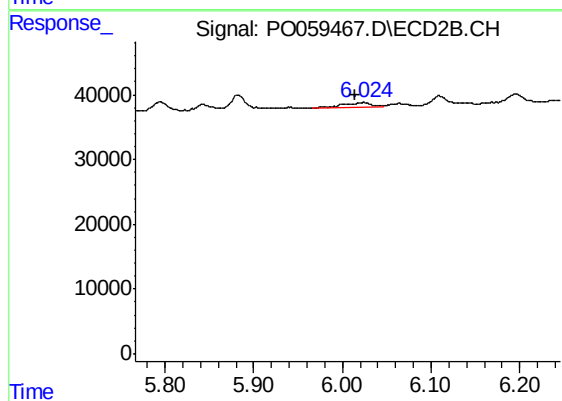

#31 AR-1260-1


R.T.: 6.024 min
Delta R.T.: 0.009 min
Response: 16495
Conc: 7.24 ng/ml



#32 AR-1260-2


R.T.: 7.123 min
Delta R.T.: -0.012 min
Response: 17614
Conc: 4.75 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019




#32 AR-1260-2

R.T.: 6.196 min
Delta R.T.: -0.007 min
Response: 22403
Conc: 7.65 ng/ml




#33 AR-1260-3

R.T.: 7.484 min
Delta R.T.: -0.006 min
Response: 12649
Conc: 3.86 ng/ml

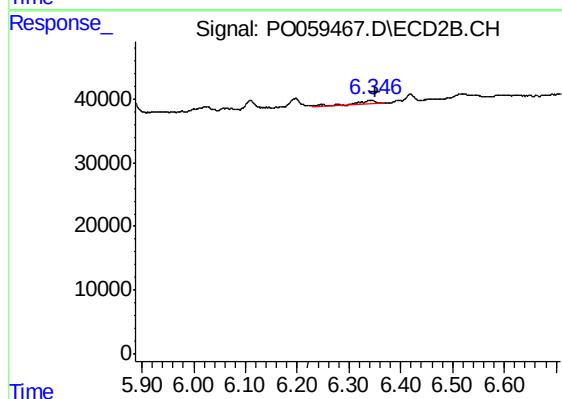

#33 AR-1260-3


R.T.: 6.344 min
Delta R.T.: -0.007 min
Response: 17653
Conc: 6.66 ng/ml



#34 AR-1260-4


R.T.: 7.702 min
Delta R.T.: -0.015 min
Response: 23579
Conc: 7.68 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019




#34 AR-1260-4

R.T.: 6.804 min
Delta R.T.: -0.010 min
Response: 18649
Conc: 8.24 ng/ml




#35 AR-1260-5

R.T.: 8.012 min
Delta R.T.: -0.012 min
Response: 87369
Conc: 12.34 ng/ml

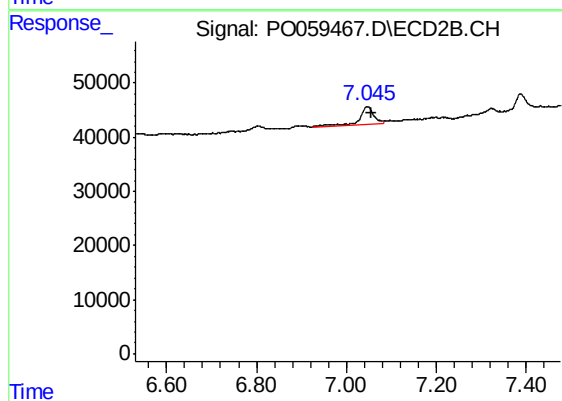

#35 AR-1260-5


R.T.: 7.046 min
Delta R.T.: -0.011 min
Response: 73524
Conc: 13.36 ng/ml



#36 AR-1262-1


R.T.: 7.484 min
Delta R.T.: -0.005 min
Response: 12649
Conc: 2.61 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

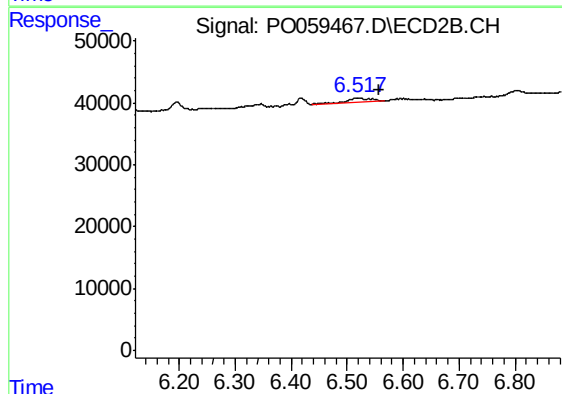


#36 AR-1262-1

R.T.: 6.519 min
Delta R.T.: -0.039 min
Response: 26247
Conc: 7.04 ng/ml




#37 AR-1262-2

R.T.: 8.012 min
Delta R.T.: -0.011 min
Response: 87369
Conc: 11.32 ng/ml

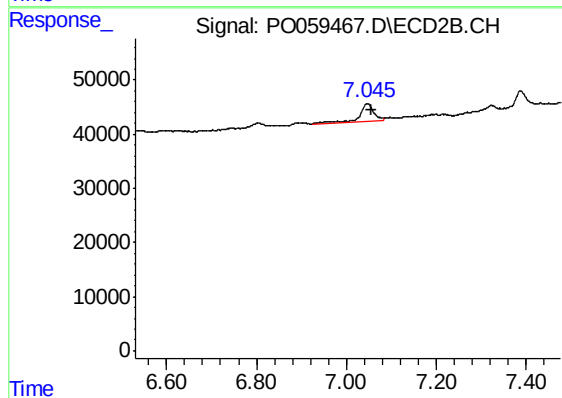

#37 AR-1262-2


R.T.: 7.046 min
Delta R.T.: -0.011 min
Response: 73524
Conc: 12.51 ng/ml



#38 AR-1262-3


R.T.: 8.315 min
Delta R.T.: 0.012 min
Response: 48164
Conc: 9.44 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

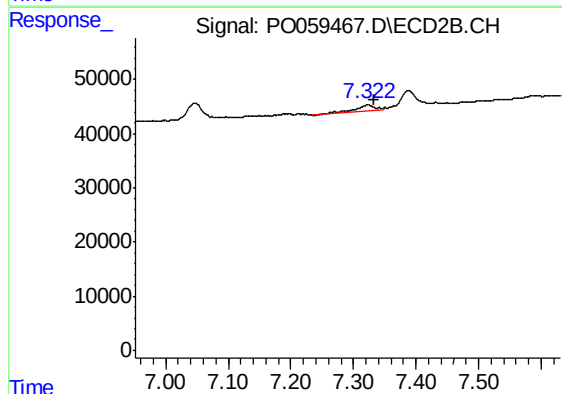


#38 AR-1262-3

R.T.: 7.323 min
Delta R.T.: -0.009 min
Response: 27258
Conc: 10.73 ng/ml




#39 AR-1262-4

R.T.: 8.401 min
Delta R.T.: 0.015 min
Response: 6468
Conc: 1.68 ng/ml

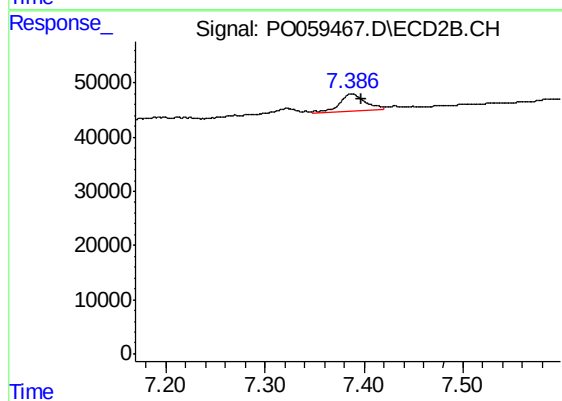

#39 AR-1262-4


R.T.: 7.388 min
Delta R.T.: -0.010 min
Response: 57128
Conc: 12.93 ng/ml



#40 AR-1262-5


R.T.: 8.976 min
Delta R.T.: -0.010 min
Response: 62282
Conc: 24.27 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019




#40 AR-1262-5

R.T.: 7.882 min
Delta R.T.: -0.007 min
Response: 15414
Conc: 8.54 ng/ml




#41 AR-1268-1

R.T.: 8.315 min
Delta R.T.: 0.013 min
Response: 48164
Conc: 5.12 ng/ml

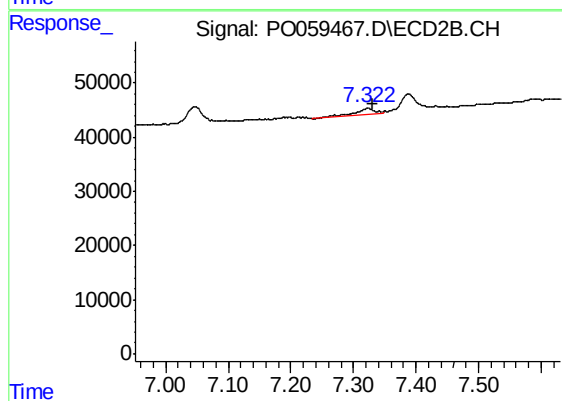

#41 AR-1268-1


R.T.: 7.323 min
Delta R.T.: -0.007 min
Response: 27258
Conc: 3.83 ng/ml

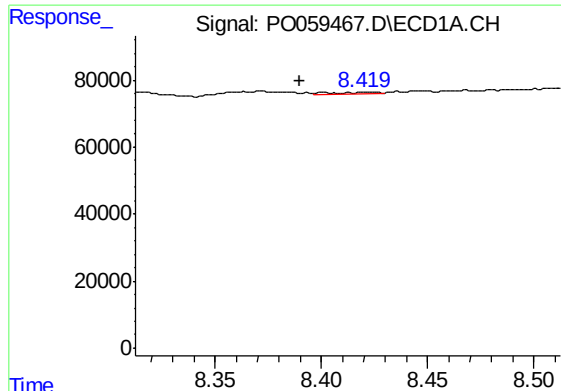

#42 AR-1268-2


R.T.: 8.401 min
Delta R.T.: 0.011 min
Response: 6468
Conc: 0.82 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

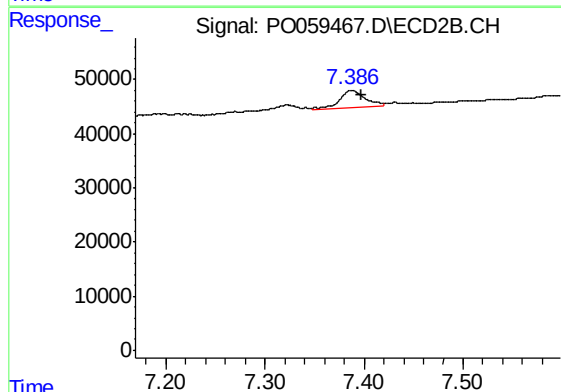


#42 AR-1268-2

R.T.: 7.388 min
Delta R.T.: -0.010 min
Response: 57128
Conc: 8.86 ng/ml

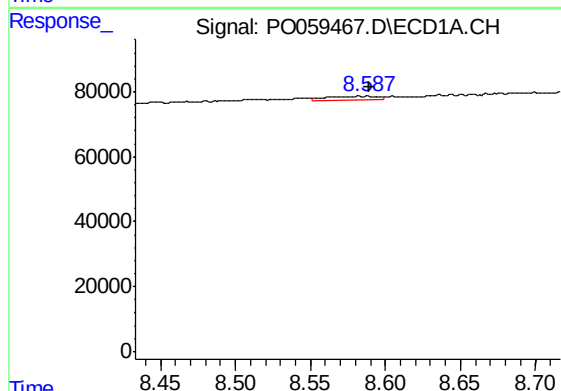


#43 AR-1268-3

R.T.: 8.588 min
Delta R.T.: -0.001 min
Response: 21484
Conc: 3.05 ng/ml

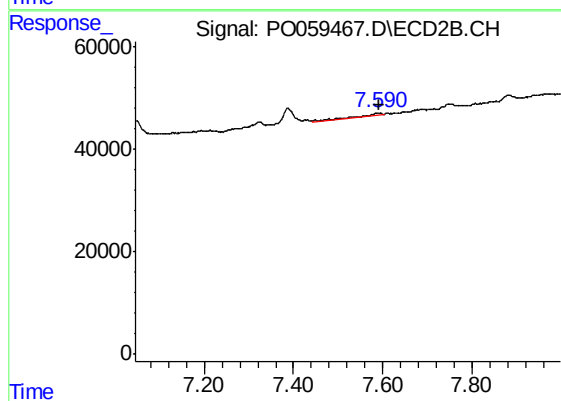

#43 AR-1268-3


R.T.: 7.590 min
Delta R.T.: -0.002 min
Response: 11127
Conc: 2.03 ng/ml



#44 AR-1268-4


R.T.: 8.976 min
Delta R.T.: -0.010 min
Response: 62282
Conc: 22.40 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019




#44 AR-1268-4

R.T.: 7.882 min
Delta R.T.: -0.006 min
Response: 15414
Conc: 7.55 ng/ml



#45 AR-1268-5

R.T.: 9.333 min
Delta R.T.: -0.016 min
Response: 66126
Conc: 3.59 ng/ml

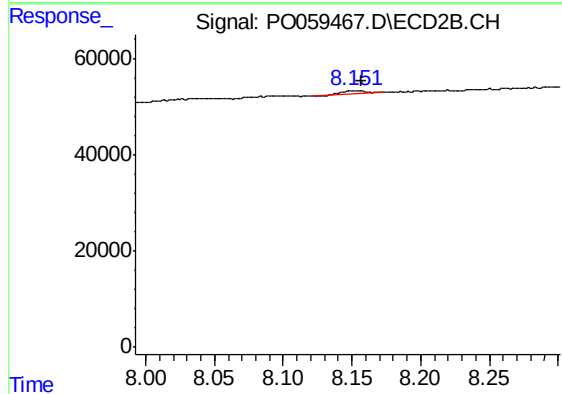

#45 AR-1268-5

R.T.: 8.152 min
Delta R.T.: -0.005 min
Response: 8279
Conc: 0.57 ng/ml