

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081919\
 Data File : P0059468.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Aug 2019 19:42
 Operator : SM/AJ
 Sample : K3591-09
 Misc : AR1254 MDL 25PPB
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-MDL-WATER-03-QT3-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 20 01:09:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 17 03:09:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.137	3.505	453573	431261	12.955	11.981
2)	SA Decachlor...	9.624	8.375	848122	615849	15.942	15.274
Target Compounds							
3)	L1 AR-1016-1	5.315	0.000	8269	0	5.156	N.D. #
4)	L1 AR-1016-2	5.315	0.000	8269	0	3.456	N.D. #
5)	L1 AR-1016-3	5.390	4.788	1616	28068	1.085	25.944 #
6)	L1 AR-1016-4	5.413	4.788	957	28068	0.791	31.083 #
7)	L1 AR-1016-5	5.758	4.997	16618	11195	12.941	9.719
9)	L2 AR-1221-2	4.438	3.798	7532	7006	23.189	22.998
10)	L2 AR-1221-3	4.555	0.000	2556	0	2.430	N.D. #
11)	L3 AR-1232-1	4.555	0.000	2556	0	2.050	N.D. #
12)	L3 AR-1232-2	5.026	0.000	4517	0	6.395	N.D. #
13)	L3 AR-1232-3	5.315	4.788	8269	28068	5.400	41.221 #
14)	L3 AR-1232-4	5.413	4.825	957	11654	1.224	19.103 #
15)	L3 AR-1232-5	5.555	4.997	36382	11195	60.523	16.446 #
16)	L4 AR-1242-1	5.315	0.000	8269	0	6.514	N.D. #
17)	L4 AR-1242-2	5.315	0.000	8269	0	4.456	N.D. #
18)	L4 AR-1242-3	5.390	4.788	1616	28068	1.382	33.594 #
19)	L4 AR-1242-4	5.413	4.825	957	11654	0.989	13.967 #
20)	L4 AR-1242-5	6.197	5.340	18058	92880	14.371	83.032 #
21)	L5 AR-1248-1	5.315	0.000	8269	0	8.248	N.D. #
22)	L5 AR-1248-2	5.555	4.788	36382	28068	25.075	24.341
23)	L5 AR-1248-3	5.758	4.825	16618	11654	9.998	9.812
24)	L5 AR-1248-4	6.156	4.997	27858	11195	13.628	7.705 #
25)	L5 AR-1248-5	6.197	5.410	18058	11206	9.106	7.829
26)	L6 AR-1254-1	6.129	5.340	83586	92880	40.062	39.160
27)	L6 AR-1254-2	6.344	5.485	79960	67819	23.967	32.321 #
28)	L6 AR-1254-3	6.709	5.881	84805	86957	23.899	25.861
29)	L6 AR-1254-4	6.993	6.108	77725	50891	26.388	24.683
30)	L6 AR-1254-5	7.408	6.517	89485	66883	28.937	21.541 #
31)	L7 AR-1260-1	6.869	6.006	37957	55299	14.080	24.266 #
32)	L7 AR-1260-2	7.122	6.194	50224	54255	13.536	18.518 #
33)	L7 AR-1260-3	7.474	6.342	13678	39857	4.175	15.045 #
34)	L7 AR-1260-4	7.699	6.803	48277	13776	15.719	6.089 #
35)	L7 AR-1260-5	8.011	7.047	53674	64099	7.580	11.647 #
36)	L8 AR-1262-1	7.474	6.540	13678	17246	2.818	4.627 #
37)	L8 AR-1262-2	8.011	7.047	53674	64099	6.956	10.903 #
38)	L8 AR-1262-3	8.311	7.321	40552	19551	7.948	7.694
39)	L8 AR-1262-4	8.375	7.386	11650	56824	3.022	12.859 #
40)	L8 AR-1262-5	8.973	7.878	74557	11233	29.049	6.221 #
41)	L9 AR-1268-1	8.311	7.321	40552	19551	4.309	2.746 #
42)	L9 AR-1268-2	8.403	7.386	1727	56824	0.219	8.813 #
43)	L9 AR-1268-3	8.587	7.584	40622	6720	5.763	1.228 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081919\
 Data File : P0059468.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Aug 2019 19:42
 Operator : SM/AJ
 Sample : K3591-09
 Misc : AR1254 MDL 25PPB
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-MDL-WATER-03-QT3-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 20 01:09:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 17 03:09:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
44) L9	AR-1268-4	8.973	7.878	74557	11233	26.819	5.503 #
45) L9	AR-1268-5	9.352	8.150	11003	12657	0.597	0.871 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081919\
Data File : PO059468.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Aug 2019 19:42
Operator : SM/AJ
Sample : K3591-09
Misc : AR1254 MDL 25PPB
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 20 01:09:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Aug 17 03:09:44 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

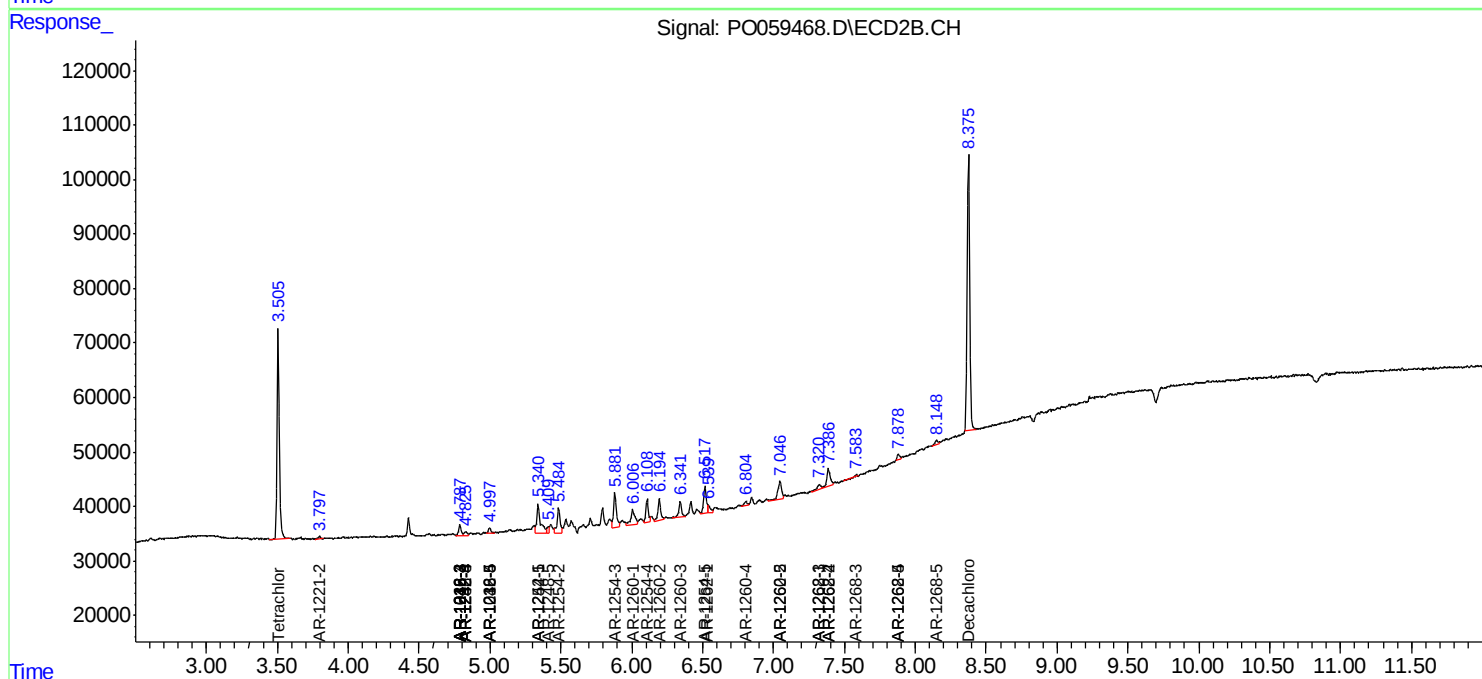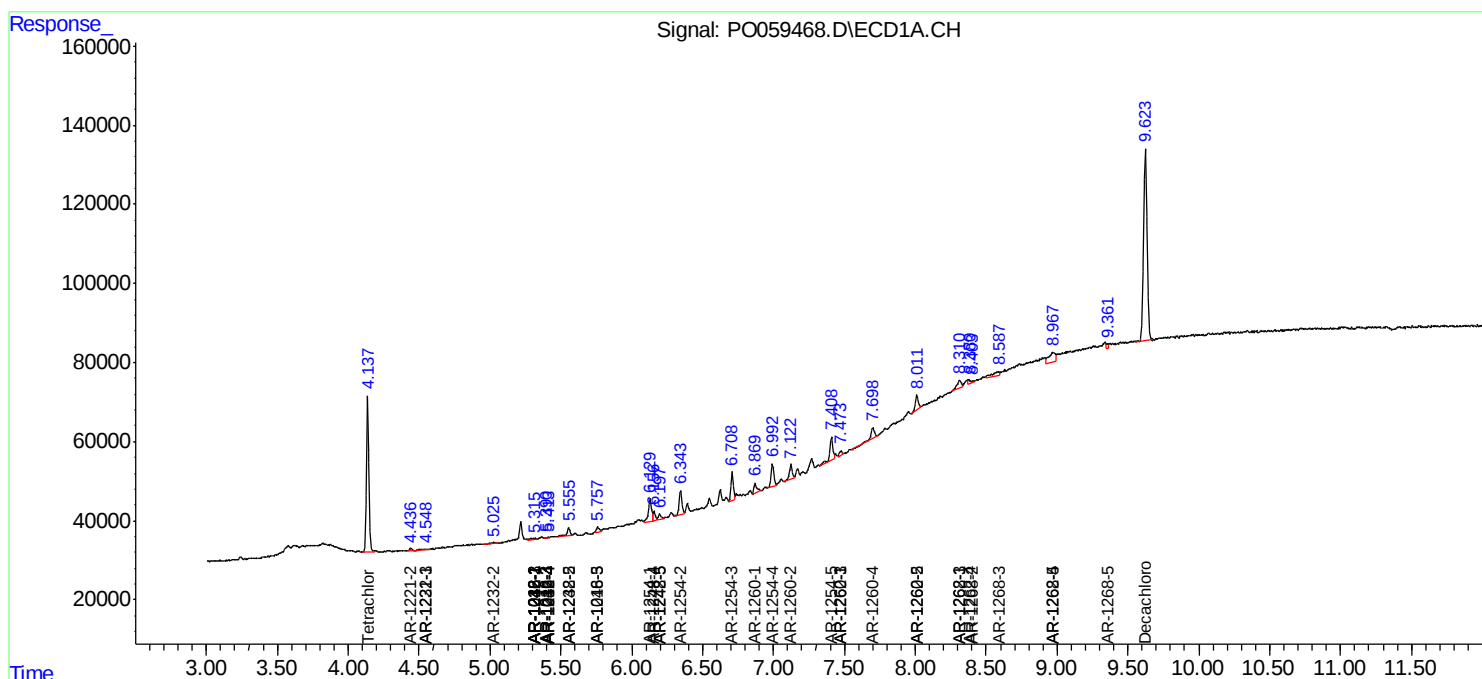




#1 Tetrachloro-m-xylene


R.T.: 4.137 min
Delta R.T.: -0.012 min
Response: 453573
Conc: 12.95 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019




#1 Tetrachloro-m-xylene

R.T.: 3.505 min
Delta R.T.: -0.005 min
Response: 431261
Conc: 11.98 ng/ml




#2 Decachlorobiphenyl

R.T.: 9.624 min
Delta R.T.: -0.017 min
Response: 848122
Conc: 15.94 ng/ml

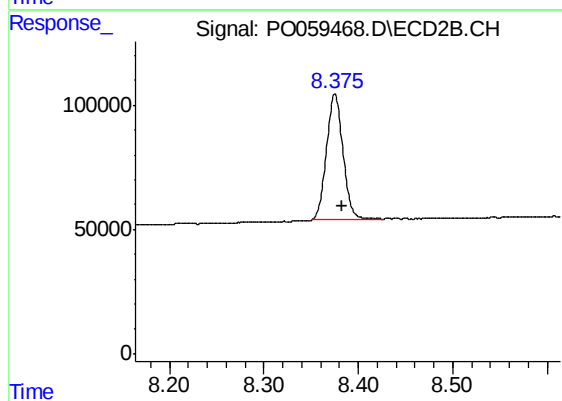

#2 Decachlorobiphenyl


R.T.: 8.375 min
Delta R.T.: -0.008 min
Response: 615849
Conc: 15.27 ng/ml

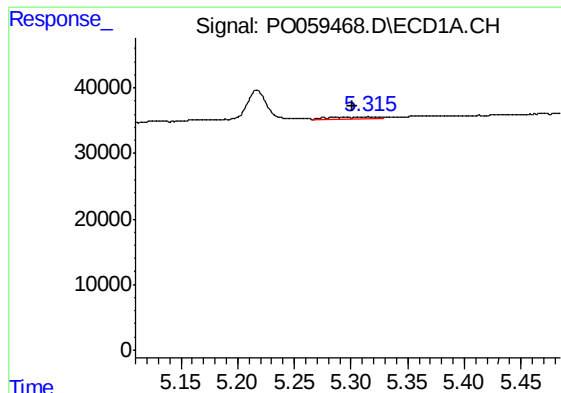

#3 AR-1016-1


R.T.: 5.315 min
Delta R.T.: 0.013 min
Response: 8269
Conc: 5.16 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

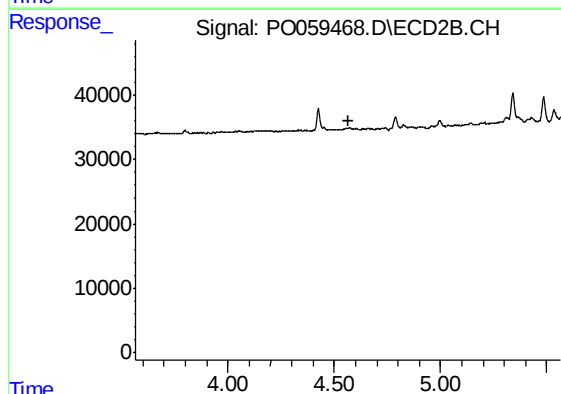


#3 AR-1016-1

R.T.: 0.000 min
Exp R.T. : 4.565 min
Response: 0
Conc: N.D.

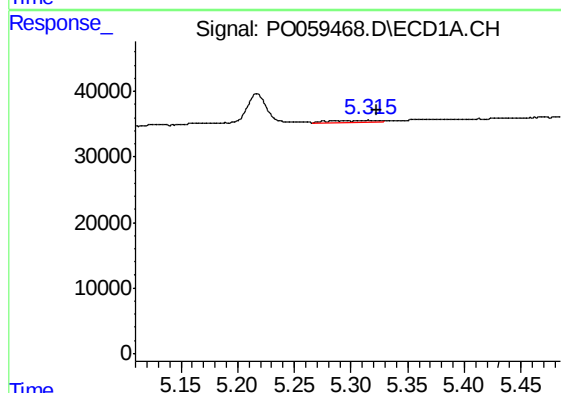


#4 AR-1016-2

R.T.: 5.315 min
Delta R.T.: -0.008 min
Response: 8269
Conc: 3.46 ng/ml

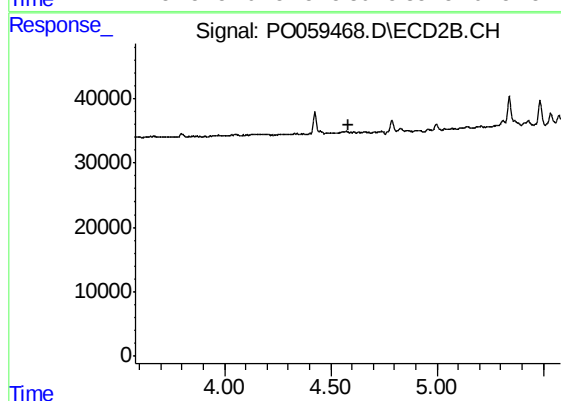

#4 AR-1016-2


R.T.: 0.000 min
Exp R.T. : 4.581 min
Response: 0
Conc: N.D.

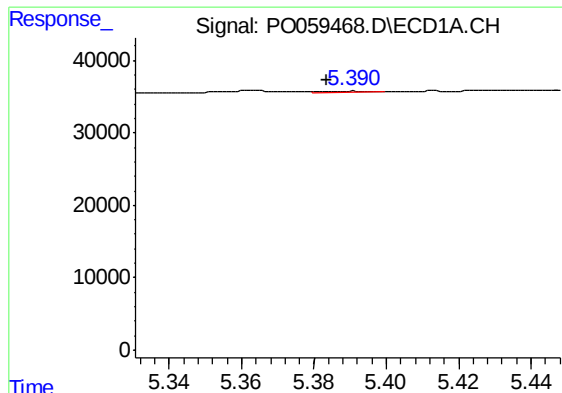

#5 AR-1016-3


R.T.: 5.390 min
Delta R.T.: 0.006 min
Response: 1616
Conc: 1.08 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

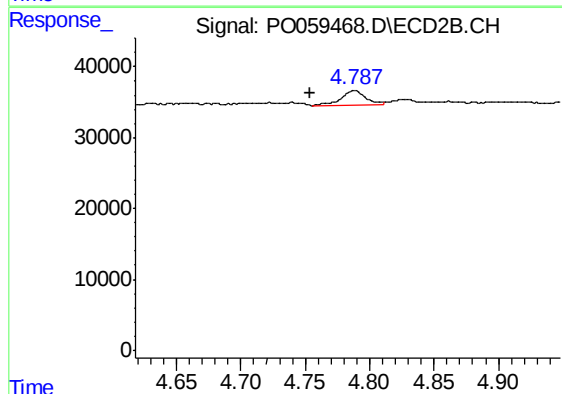


#5 AR-1016-3

R.T.: 4.788 min
Delta R.T.: 0.034 min
Response: 28068
Conc: 25.94 ng/ml

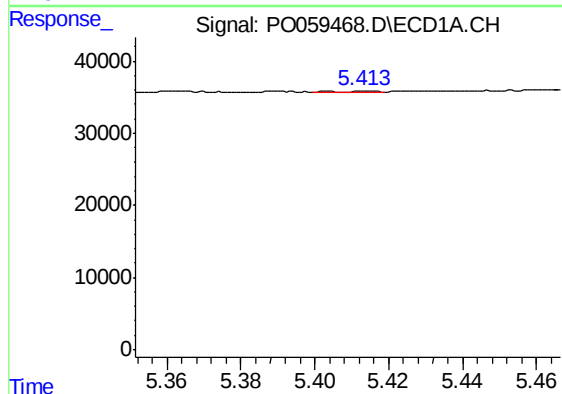


#6 AR-1016-4

R.T.: 5.413 min
Delta R.T.: -0.068 min
Response: 957
Conc: 0.79 ng/ml

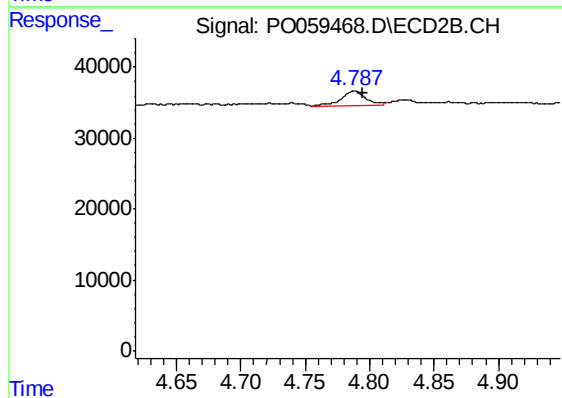

#6 AR-1016-4


R.T.: 4.788 min
Delta R.T.: -0.007 min
Response: 28068
Conc: 31.08 ng/ml



#7 AR-1016-5


R.T.: 5.758 min
Delta R.T.: -0.012 min
Response: 16618
Conc: 12.94 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

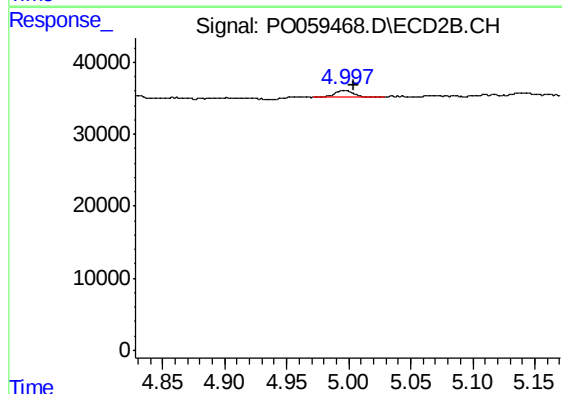


#7 AR-1016-5

R.T.: 4.997 min
Delta R.T.: -0.007 min
Response: 11195
Conc: 9.72 ng/ml

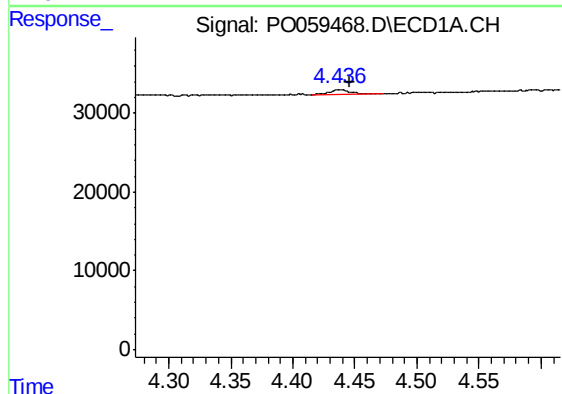


#9 AR-1221-2

R.T.: 4.438 min
Delta R.T.: -0.009 min
Response: 7532
Conc: 23.19 ng/ml

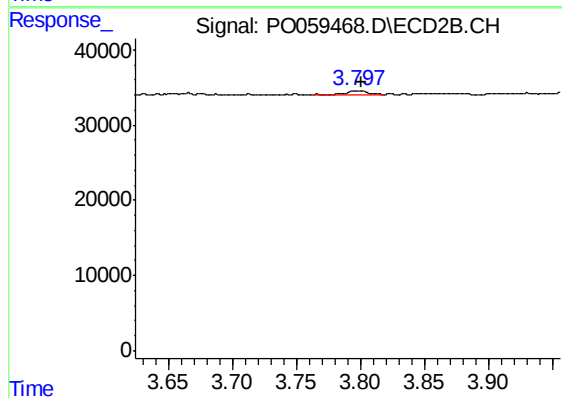

#9 AR-1221-2


R.T.: 3.798 min
Delta R.T.: -0.003 min
Response: 7006
Conc: 23.00 ng/ml



#10 AR-1221-3


R.T.: 4.555 min
Delta R.T.: 0.033 min
Response: 2556
Conc: 2.43 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

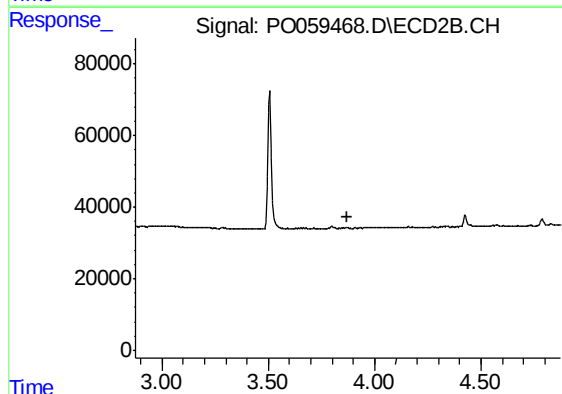


#10 AR-1221-3

R.T.: 0.000 min
Exp R.T. : 3.874 min
Response: 0
Conc: N.D.




#11 AR-1232-1

R.T.: 4.555 min
Delta R.T.: 0.034 min
Response: 2556
Conc: 2.05 ng/ml

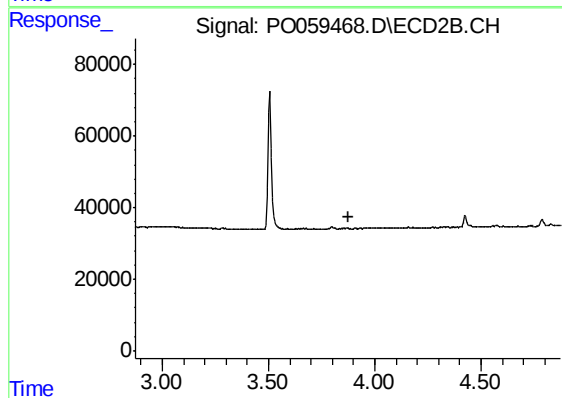

#11 AR-1232-1


R.T.: 0.000 min
Exp R.T. : 3.874 min
Response: 0
Conc: N.D.



#12 AR-1232-2


R.T.: 5.026 min
Delta R.T.: -0.012 min
Response: 4517
Conc: 6.39 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019




#12 AR-1232-2

R.T.: 0.000 min
Exp R.T. : 4.581 min
Response: 0
Conc: N.D.




#13 AR-1232-3

R.T.: 5.315 min
Delta R.T.: -0.007 min
Response: 8269
Conc: 5.40 ng/ml

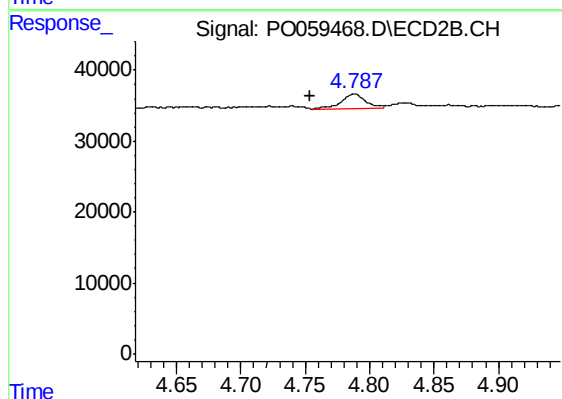

#13 AR-1232-3


R.T.: 4.788 min
Delta R.T.: 0.034 min
Response: 28068
Conc: 41.22 ng/ml

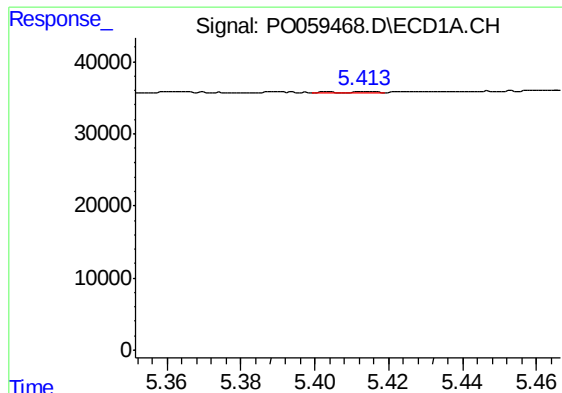

#14 AR-1232-4


R.T.: 5.413 min
Delta R.T.: -0.068 min
Response: 957
Conc: 1.22 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

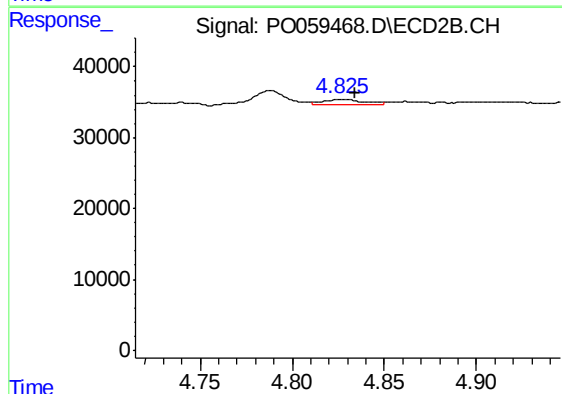


#14 AR-1232-4

R.T.: 4.825 min
Delta R.T.: -0.009 min
Response: 11654
Conc: 19.10 ng/ml

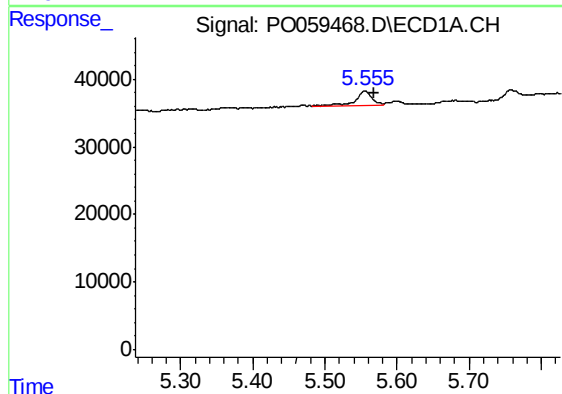


#15 AR-1232-5

R.T.: 5.555 min
Delta R.T.: -0.013 min
Response: 36382
Conc: 60.52 ng/ml

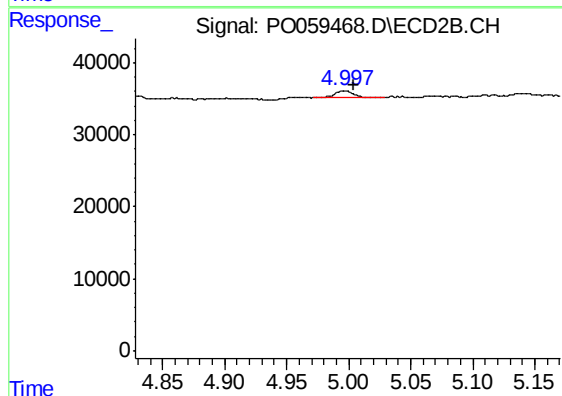

#15 AR-1232-5


R.T.: 4.997 min
Delta R.T.: -0.007 min
Response: 11195
Conc: 16.45 ng/ml



#16 AR-1242-1


R.T.: 5.315 min
Delta R.T.: 0.014 min
Response: 8269
Conc: 6.51 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019




#16 AR-1242-1

R.T.: 0.000 min
Exp R.T. : 4.564 min
Response: 0
Conc: N.D.




#17 AR-1242-2

R.T.: 5.315 min
Delta R.T.: -0.008 min
Response: 8269
Conc: 4.46 ng/ml

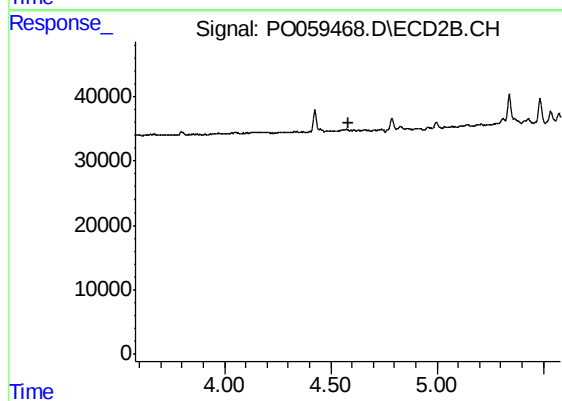

#17 AR-1242-2


R.T.: 0.000 min
Exp R.T. : 4.581 min
Response: 0
Conc: N.D.



#18 AR-1242-3


R.T.: 5.390 min
Delta R.T.: 0.007 min
Response: 1616
Conc: 1.38 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019




#18 AR-1242-3

R.T.: 4.788 min
Delta R.T.: 0.034 min
Response: 28068
Conc: 33.59 ng/ml




#19 AR-1242-4

R.T.: 5.413 min
Delta R.T.: -0.068 min
Response: 957
Conc: 0.99 ng/ml

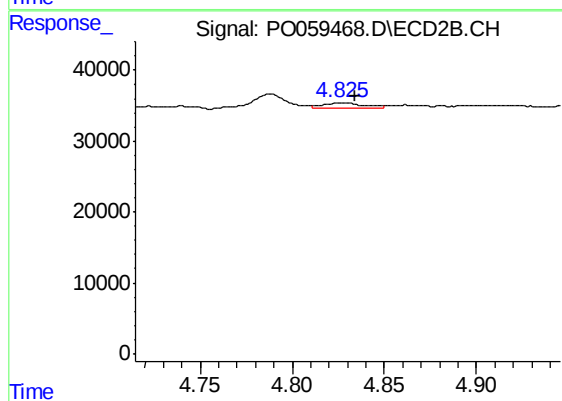

#19 AR-1242-4


R.T.: 4.825 min
Delta R.T.: -0.009 min
Response: 11654
Conc: 13.97 ng/ml

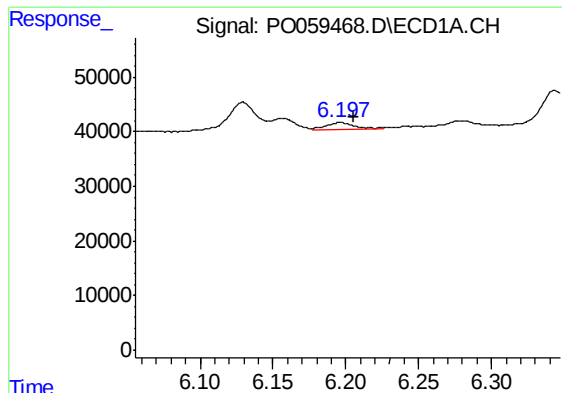

#20 AR-1242-5


R.T.: 6.197 min
Delta R.T.: -0.009 min
Response: 18058
Conc: 14.37 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

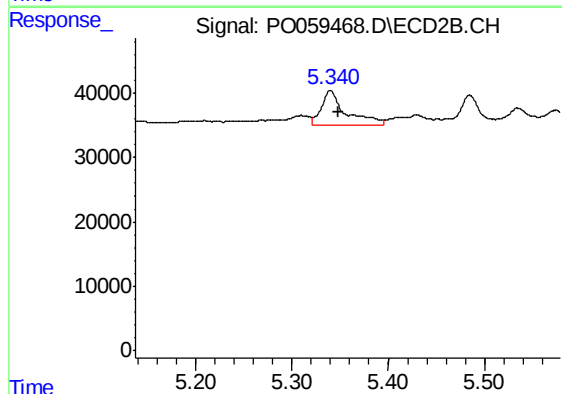


#20 AR-1242-5

R.T.: 5.340 min
Delta R.T.: -0.008 min
Response: 92880
Conc: 83.03 ng/ml




#21 AR-1248-1

R.T.: 5.315 min
Delta R.T.: 0.014 min
Response: 8269
Conc: 8.25 ng/ml

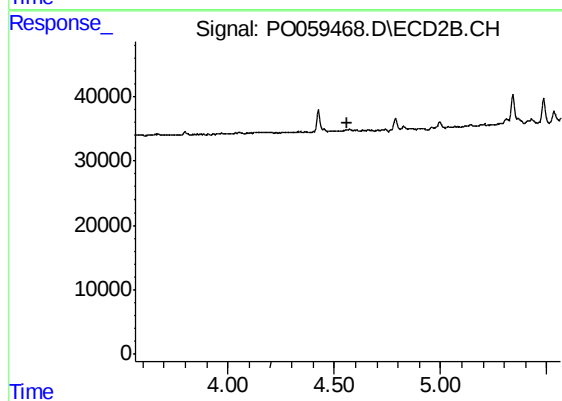

#21 AR-1248-1


R.T.: 0.000 min
Exp R.T. : 4.564 min
Response: 0
Conc: N.D.

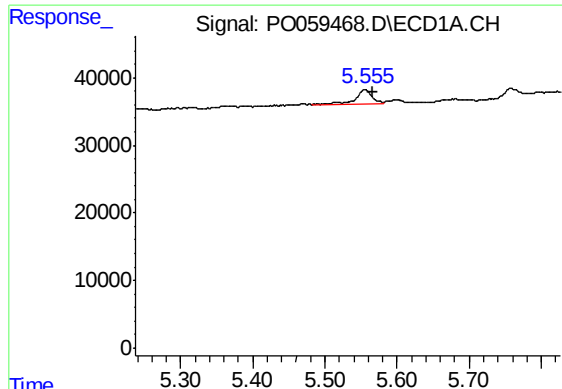

#22 AR-1248-2


R.T.: 5.555 min
Delta R.T.: -0.012 min
Response: 36382
Conc: 25.08 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019




#22 AR-1248-2

R.T.: 4.788 min
Delta R.T.: -0.006 min
Response: 28068
Conc: 24.34 ng/ml




#23 AR-1248-3

R.T.: 5.758 min
Delta R.T.: -0.010 min
Response: 16618
Conc: 10.00 ng/ml

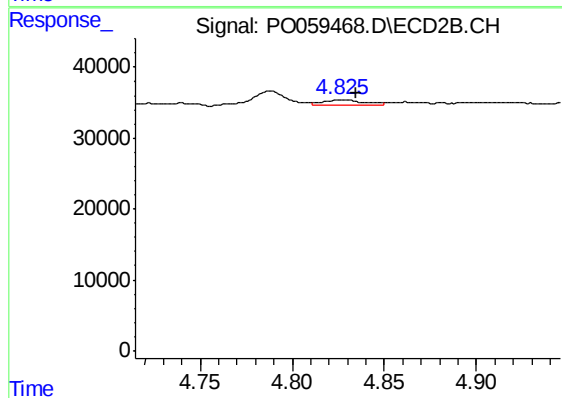

#23 AR-1248-3


R.T.: 4.825 min
Delta R.T.: -0.009 min
Response: 11654
Conc: 9.81 ng/ml



#24 AR-1248-4


R.T.: 6.156 min
Delta R.T.: -0.012 min
Response: 27858
Conc: 13.63 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019




#24 AR-1248-4

R.T.: 4.997 min
Delta R.T.: -0.006 min
Response: 11195
Conc: 7.70 ng/ml




#25 AR-1248-5

R.T.: 6.197 min
Delta R.T.: -0.008 min
Response: 18058
Conc: 9.11 ng/ml

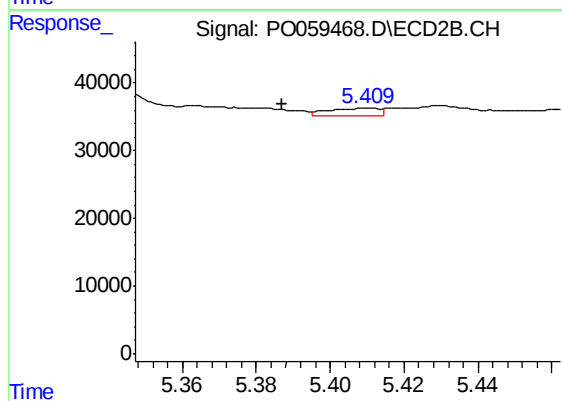

#25 AR-1248-5


R.T.: 5.410 min
Delta R.T.: 0.023 min
Response: 11206
Conc: 7.83 ng/ml



#26 AR-1254-1


R.T.: 6.129 min
Delta R.T.: -0.010 min
Response: 83586
Conc: 40.06 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019




#26 AR-1254-1

R.T.: 5.340 min
Delta R.T.: -0.006 min
Response: 92880
Conc: 39.16 ng/ml




#27 AR-1254-2

R.T.: 6.344 min
Delta R.T.: -0.011 min
Response: 79960
Conc: 23.97 ng/ml

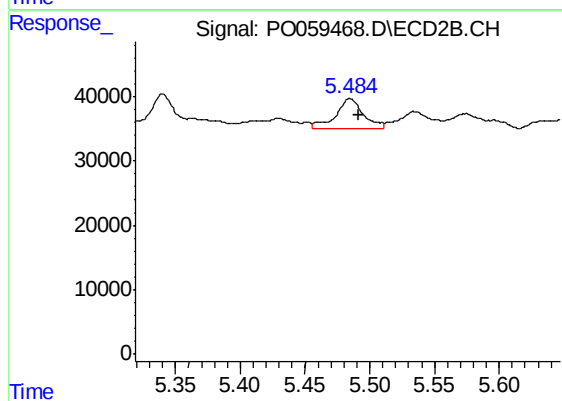

#27 AR-1254-2


R.T.: 5.485 min
Delta R.T.: -0.007 min
Response: 67819
Conc: 32.32 ng/ml



#28 AR-1254-3


R.T.: 6.709 min
Delta R.T.: -0.012 min
Response: 84805
Conc: 23.90 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

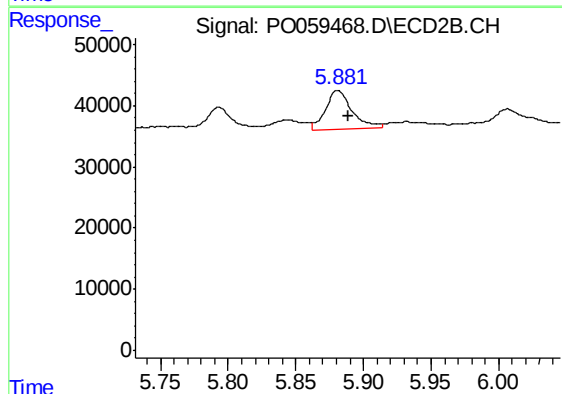


#28 AR-1254-3

R.T.: 5.881 min
Delta R.T.: -0.008 min
Response: 86957
Conc: 25.86 ng/ml




#29 AR-1254-4

R.T.: 6.993 min
Delta R.T.: -0.012 min
Response: 77725
Conc: 26.39 ng/ml

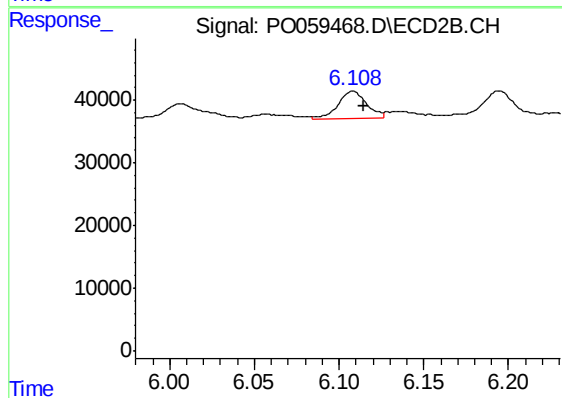

#29 AR-1254-4


R.T.: 6.108 min
Delta R.T.: -0.007 min
Response: 50891
Conc: 24.68 ng/ml



#30 AR-1254-5


R.T.: 7.408 min
Delta R.T.: -0.011 min
Response: 89485
Conc: 28.94 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019




#30 AR-1254-5

R.T.: 6.517 min
Delta R.T.: -0.008 min
Response: 66883
Conc: 21.54 ng/ml




#31 AR-1260-1

R.T.: 6.869 min
Delta R.T.: -0.011 min
Response: 37957
Conc: 14.08 ng/ml

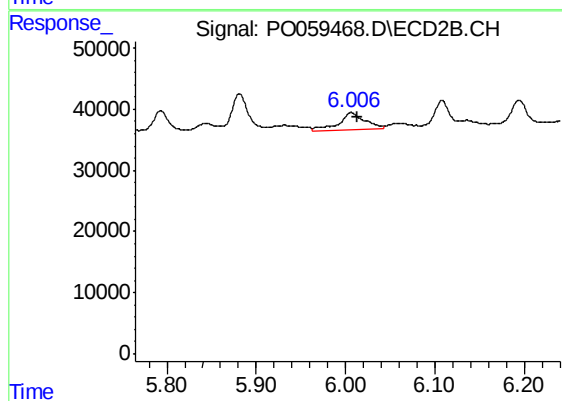

#31 AR-1260-1


R.T.: 6.006 min
Delta R.T.: -0.008 min
Response: 55299
Conc: 24.27 ng/ml



#32 AR-1260-2


R.T.: 7.122 min
Delta R.T.: -0.013 min
Response: 50224
Conc: 13.54 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019




#32 AR-1260-2

R.T.: 6.194 min
Delta R.T.: -0.008 min
Response: 54255
Conc: 18.52 ng/ml




#33 AR-1260-3

R.T.: 7.474 min
Delta R.T.: -0.016 min
Response: 13678
Conc: 4.17 ng/ml

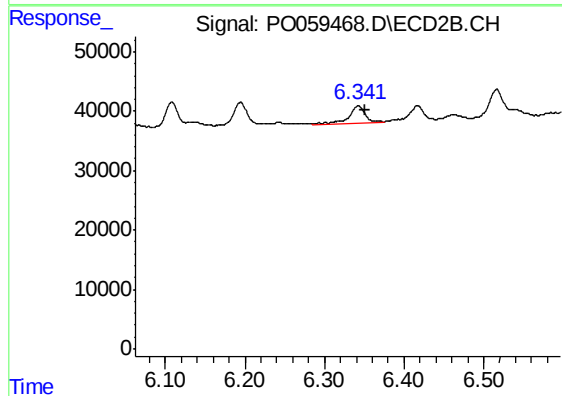

#33 AR-1260-3


R.T.: 6.342 min
Delta R.T.: -0.009 min
Response: 39857
Conc: 15.05 ng/ml



#34 AR-1260-4


R.T.: 7.699 min
Delta R.T.: -0.018 min
Response: 48277
Conc: 15.72 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019




#34 AR-1260-4

R.T.: 6.803 min
Delta R.T.: -0.011 min
Response: 13776
Conc: 6.09 ng/ml




#35 AR-1260-5

R.T.: 8.011 min
Delta R.T.: -0.013 min
Response: 53674
Conc: 7.58 ng/ml

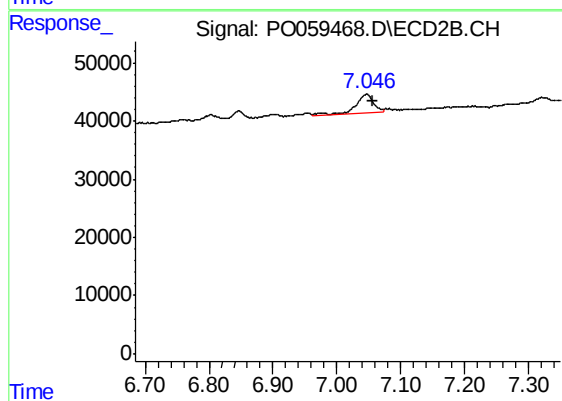

#35 AR-1260-5


R.T.: 7.047 min
Delta R.T.: -0.011 min
Response: 64099
Conc: 11.65 ng/ml

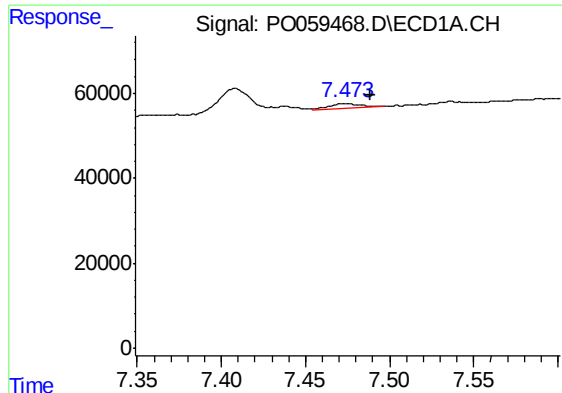

#36 AR-1262-1


R.T.: 7.474 min
Delta R.T.: -0.015 min
Response: 13678
Conc: 2.82 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

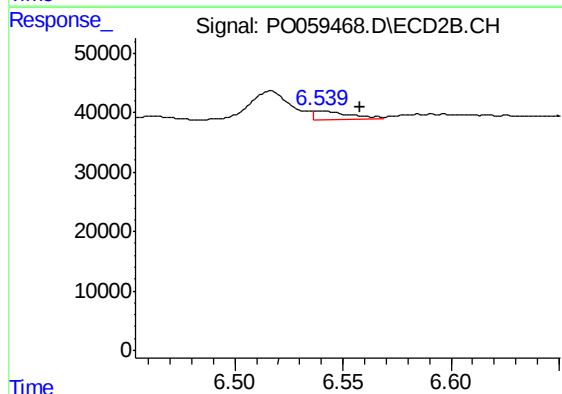


#36 AR-1262-1

R.T.: 6.540 min
Delta R.T.: -0.019 min
Response: 17246
Conc: 4.63 ng/ml

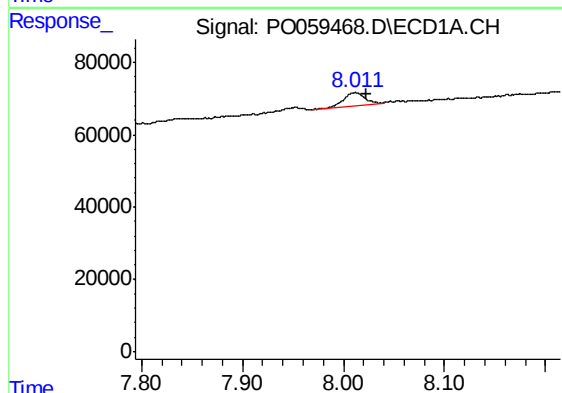


#37 AR-1262-2

R.T.: 8.011 min
Delta R.T.: -0.012 min
Response: 53674
Conc: 6.96 ng/ml

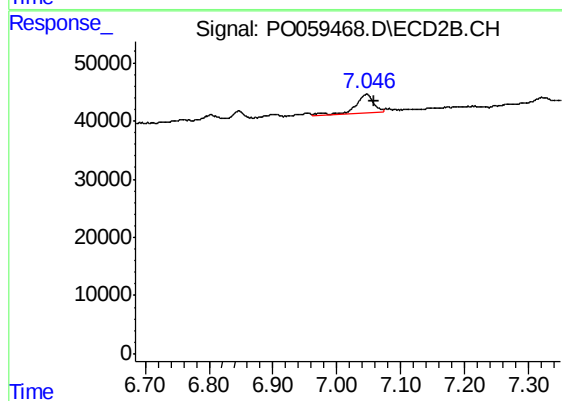

#37 AR-1262-2


R.T.: 7.047 min
Delta R.T.: -0.011 min
Response: 64099
Conc: 10.90 ng/ml

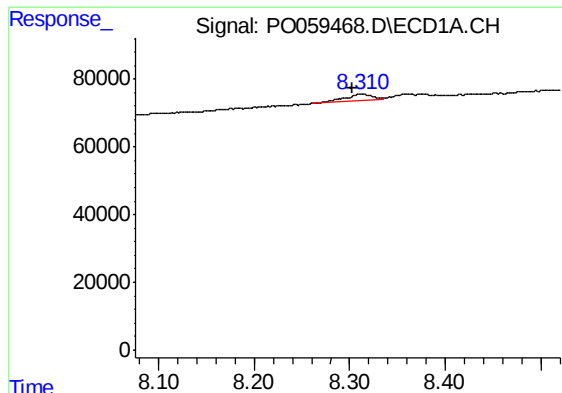

#38 AR-1262-3


R.T.: 8.311 min
Delta R.T.: 0.008 min
Response: 40552
Conc: 7.95 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

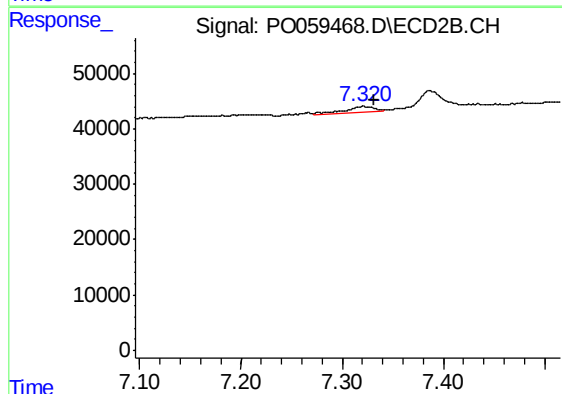


#38 AR-1262-3

R.T.: 7.321 min
Delta R.T.: -0.011 min
Response: 19551
Conc: 7.69 ng/ml

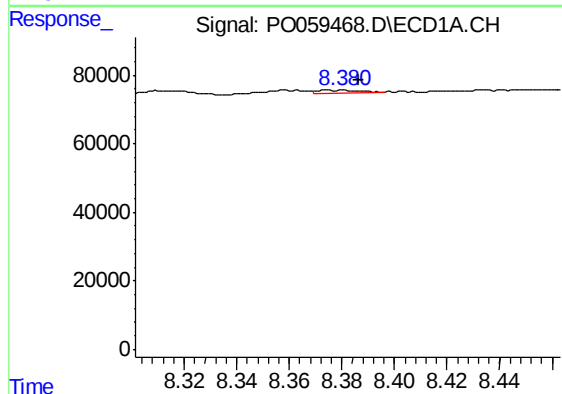


#39 AR-1262-4

R.T.: 8.375 min
Delta R.T.: -0.012 min
Response: 11650
Conc: 3.02 ng/ml

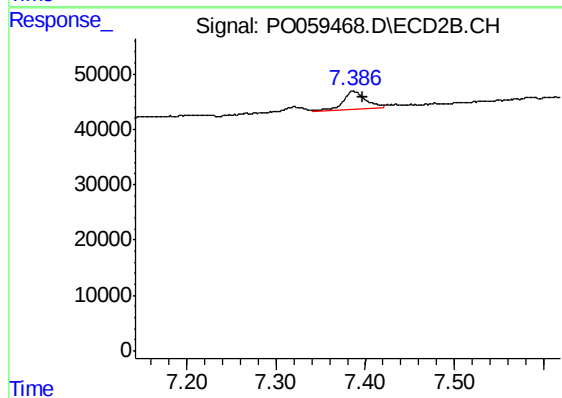

#39 AR-1262-4


R.T.: 7.386 min
Delta R.T.: -0.011 min
Response: 56824
Conc: 12.86 ng/ml



#40 AR-1262-5


R.T.: 8.973 min
Delta R.T.: -0.013 min
Response: 74557
Conc: 29.05 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019




#40 AR-1262-5

R.T.: 7.878 min
Delta R.T.: -0.011 min
Response: 11233
Conc: 6.22 ng/ml




#41 AR-1268-1

R.T.: 8.311 min
Delta R.T.: 0.009 min
Response: 40552
Conc: 4.31 ng/ml

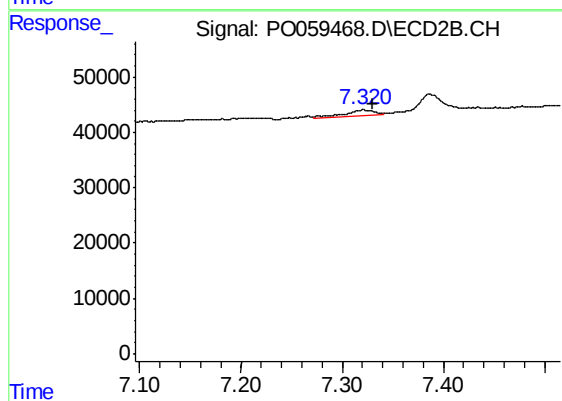

#41 AR-1268-1


R.T.: 7.321 min
Delta R.T.: -0.010 min
Response: 19551
Conc: 2.75 ng/ml

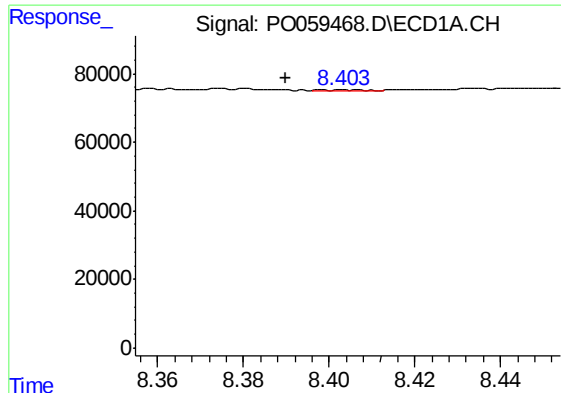

#42 AR-1268-2


R.T.: 8.403 min
Delta R.T.: 0.013 min
Response: 1727
Conc: 0.22 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

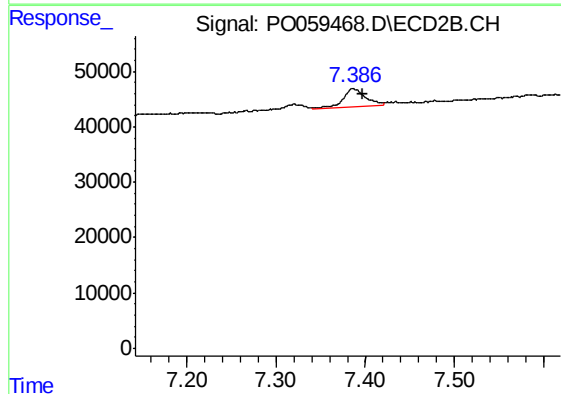


#42 AR-1268-2

R.T.: 7.386 min
Delta R.T.: -0.011 min
Response: 56824
Conc: 8.81 ng/ml

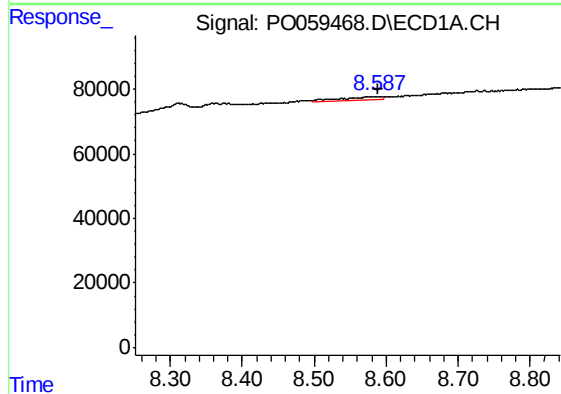


#43 AR-1268-3

R.T.: 8.587 min
Delta R.T.: -0.001 min
Response: 40622
Conc: 5.76 ng/ml

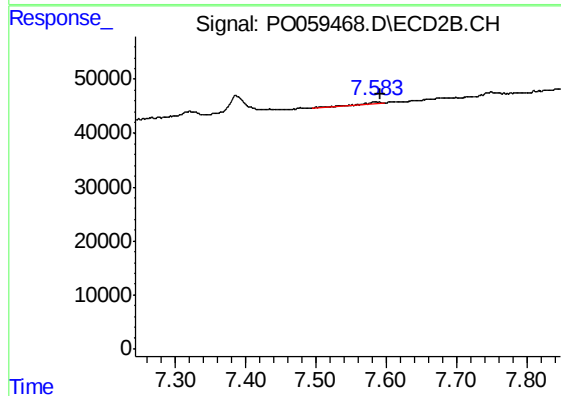

#43 AR-1268-3


R.T.: 7.584 min
Delta R.T.: -0.008 min
Response: 6720
Conc: 1.23 ng/ml

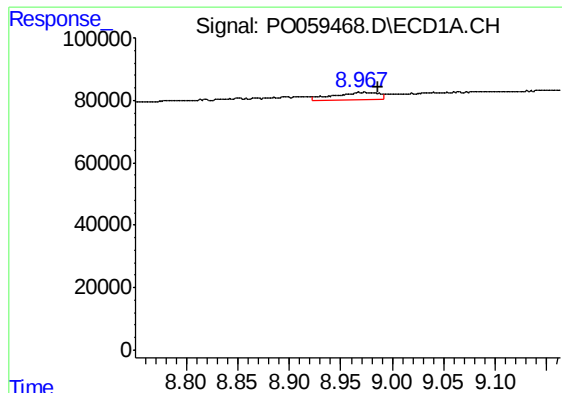

#44 AR-1268-4


R.T.: 8.973 min
Delta R.T.: -0.012 min
Response: 74557
Conc: 26.82 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

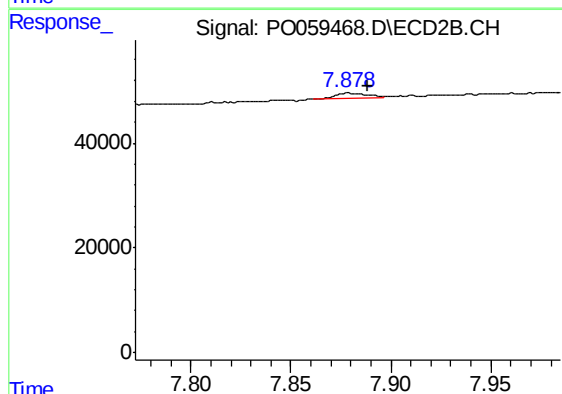


#44 AR-1268-4

R.T.: 7.878 min
Delta R.T.: -0.010 min
Response: 11233
Conc: 5.50 ng/ml

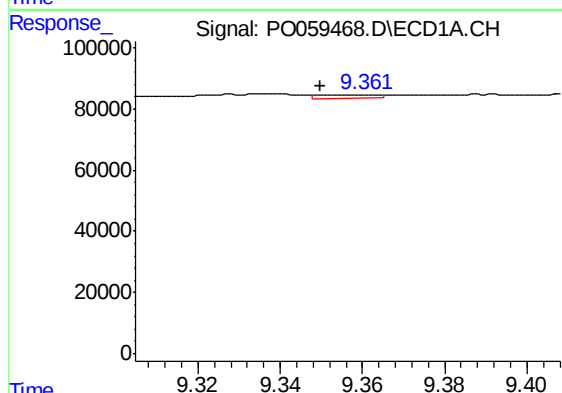

#45 AR-1268-5

R.T.: 9.352 min
Delta R.T.: 0.002 min
Response: 11003
Conc: 0.60 ng/ml

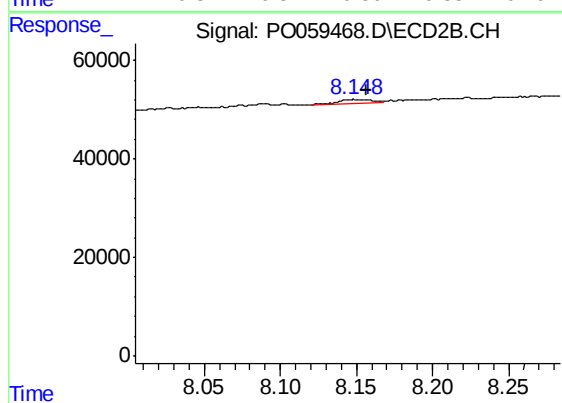

#45 AR-1268-5

R.T.: 8.150 min
Delta R.T.: -0.007 min
Response: 12657
Conc: 0.87 ng/ml