

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081919\
 Data File : P0059469.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Aug 2019 19:58
 Operator : SM/AJ
 Sample : K3591-09
 Misc : AR1262 MDL 25PPB
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-MDL-WATER-03-QT3-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 20 01:10:05 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 17 03:09:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.136	3.505	425164	406879	12.143	11.304
2)	SA Decachlor...	9.624	8.375	792471	566328	14.896	14.045
Target Compounds							
3)	L1 AR-1016-1	5.305	4.572	7363	10561	4.591	7.812 #
4)	L1 AR-1016-2	5.305	4.572	7363	10561	3.078	5.273 #
5)	L1 AR-1016-3	5.361	4.790	4909	8340	3.296	7.709 #
6)	L1 AR-1016-4	5.438	4.790	5391	8340	4.456	9.236 #
7)	L1 AR-1016-5	5.779	0.000	9220	0	7.180	N.D. #
9)	L2 AR-1221-2	4.437	3.796	5928	5831	18.252	19.142
12)	L3 AR-1232-2	5.027	4.572	4275	10561	6.052	8.292 #
13)	L3 AR-1232-3	5.305	4.790	7363	8340	4.808	12.249 #
14)	L3 AR-1232-4	5.438	4.790	5391	8340	6.895	13.672 #
15)	L3 AR-1232-5	5.556	0.000	9227	0	15.350	N.D. #
16)	L4 AR-1242-1	5.305	4.572	7363	10561	5.800	10.267 #
17)	L4 AR-1242-2	5.305	4.572	7363	10561	3.968	6.934 #
18)	L4 AR-1242-3	5.361	4.790	4909	8340	4.200	9.983 #
19)	L4 AR-1242-4	5.438	4.790	5391	8340	5.570	9.996 #
20)	L4 AR-1242-5	6.204	5.340	3823	31512	3.042	28.171 #
21)	L5 AR-1248-1	5.305	4.572	7363	10561	7.345	12.754 #
22)	L5 AR-1248-2	5.556	4.790	9227	8340	6.360	7.233
23)	L5 AR-1248-3	5.779	4.790	9220	8340	5.548	7.022 #
24)	L5 AR-1248-4	6.204	0.000	3823	0	1.870	N.D. #
25)	L5 AR-1248-5	6.204	5.340	3823	31512	1.928	22.017 #
26)	L6 AR-1254-1	6.132	5.340	46988	31512	22.521	13.286 #
27)	L6 AR-1254-2	6.341	5.484	12583	31969	3.772	15.236 #
28)	L6 AR-1254-3	6.708	5.893	5345	30639	1.506	9.112 #
29)	L6 AR-1254-4	6.995	6.135	8896	8572	3.020	4.157 #
30)	L6 AR-1254-5	7.406	6.516	54447	37163	17.607	11.969 #
31)	L7 AR-1260-1	6.867	6.007	50339	39434	18.673	17.304
32)	L7 AR-1260-2	7.122	6.194	70728	59960	19.062	20.465
33)	L7 AR-1260-3	7.477	6.343	102719	51636	31.352	19.492 #
34)	L7 AR-1260-4	7.705	6.806	90707	67358	29.534	29.770
35)	L7 AR-1260-5	8.012	7.049	204972	163883	28.947	29.779
36)	L8 AR-1262-1	7.477	6.551	102719	76896	21.166	20.629
37)	L8 AR-1262-2	8.012	7.049	204972	163883	26.565	27.876
38)	L8 AR-1262-3	8.312	7.323	44339	75000	8.690	29.516 #
39)	L8 AR-1262-4	8.372	7.390	96300	136214	24.982	30.825
40)	L8 AR-1262-5	8.974	7.881	122320	44024	47.659	24.383 #
41)	L9 AR-1268-1	8.312	7.323	44339	75000	4.712	10.532 #
42)	L9 AR-1268-2	8.372	7.390	96300	136214	12.217	21.125 #
43)	L9 AR-1268-3	8.578	7.586	53828	12743	7.637	2.329 #
44)	L9 AR-1268-4	8.974	7.881	122320	44024	43.999	21.567 #
45)	L9 AR-1268-5	9.338	8.150	58823	21069	3.190	1.450 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081919\
Data File : P0059469.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Aug 2019 19:58
Operator : SM/AJ
Sample : K3591-09
Misc : AR1262 MDL 25PPB
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 20 01:10:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Aug 17 03:09:44 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081919\
Data File : PO059469.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Aug 2019 19:58
Operator : SM/AJ
Sample : K3591-09
Misc : AR1262 MDL 25PPB
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 20 01:10:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Aug 17 03:09:44 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

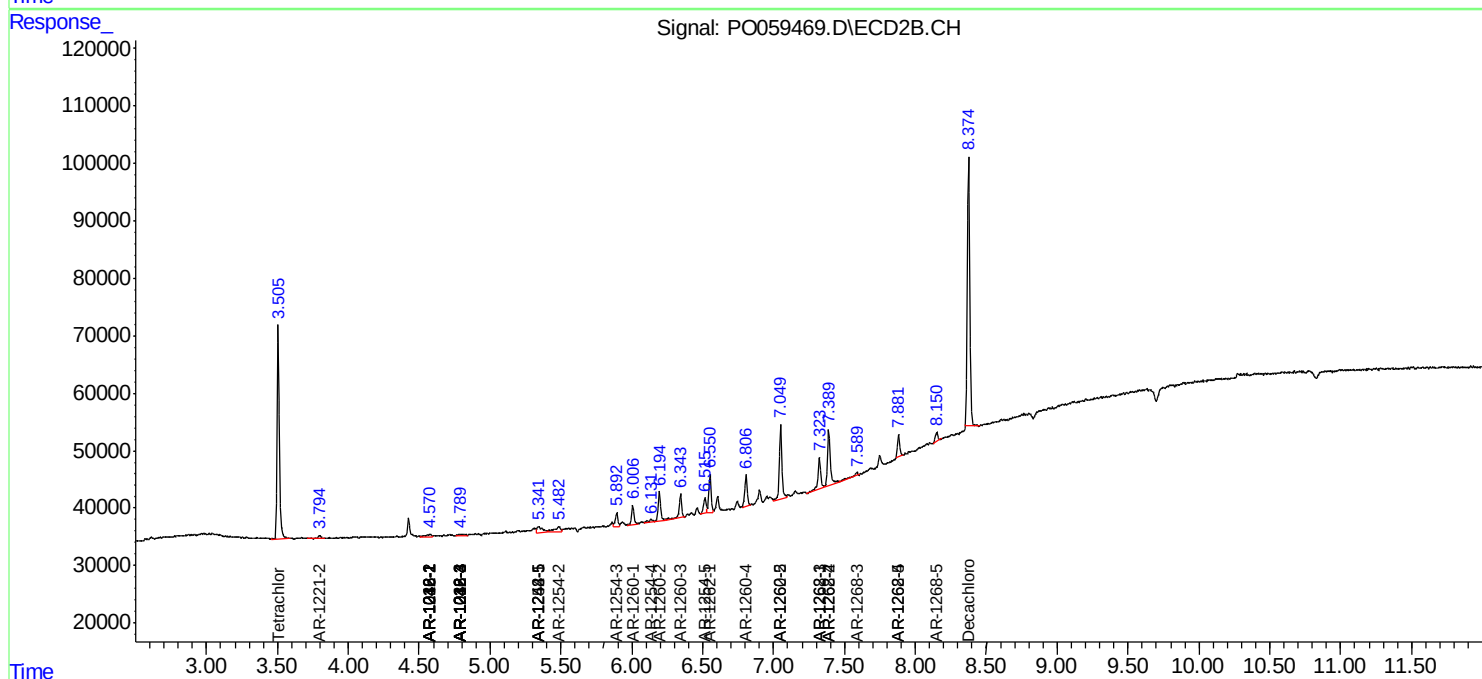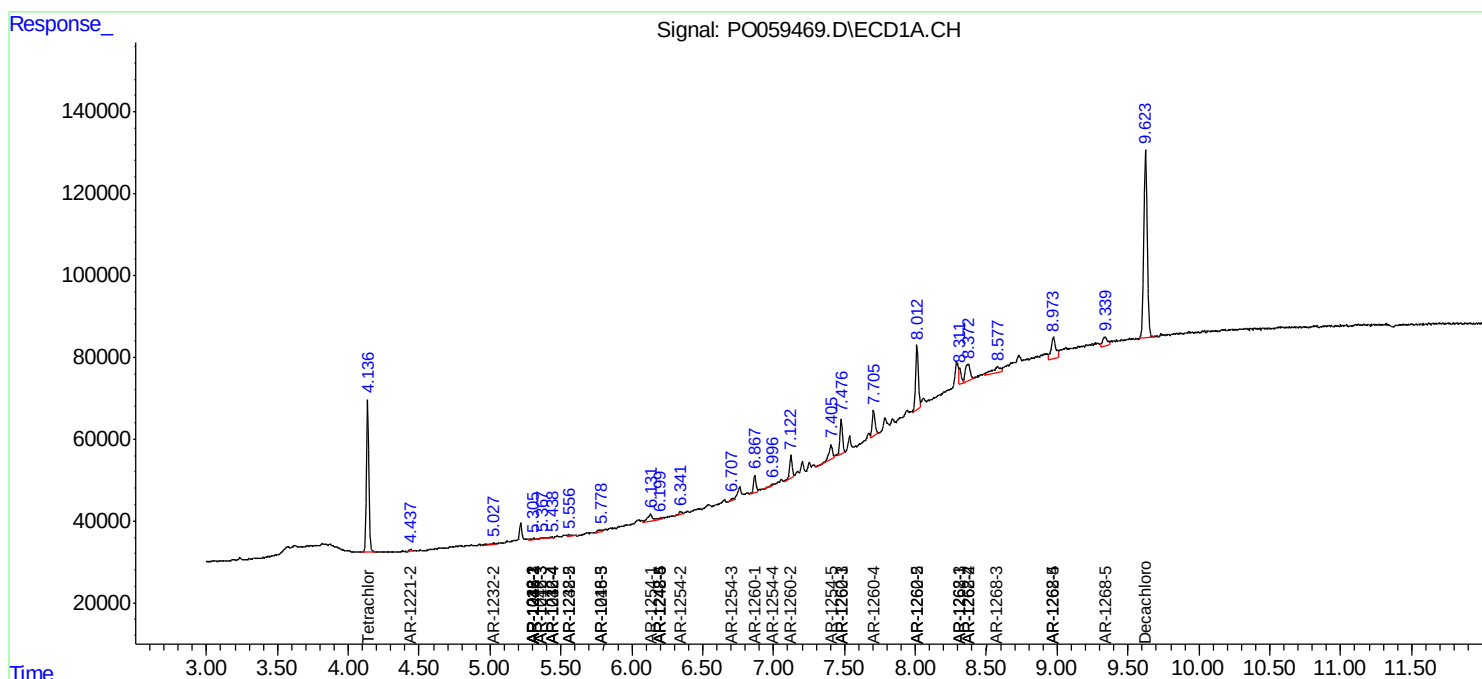


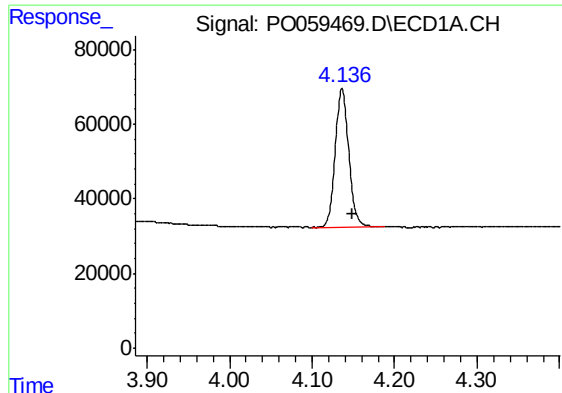

#1 Tetrachloro-m-xylene


R.T.: 4.136 min
Delta R.T.: -0.013 min
Response: 425164
Conc: 12.14 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

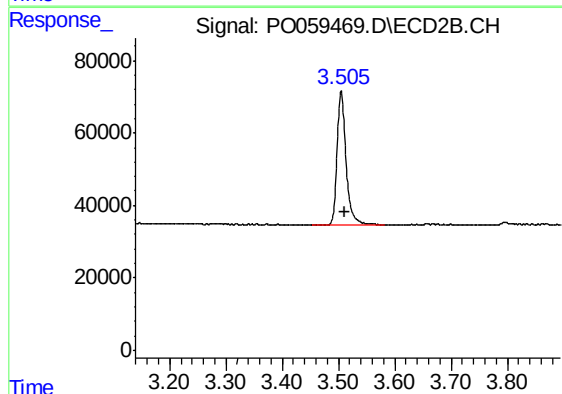


#1 Tetrachloro-m-xylene

R.T.: 3.505 min
Delta R.T.: -0.005 min
Response: 406879
Conc: 11.30 ng/ml

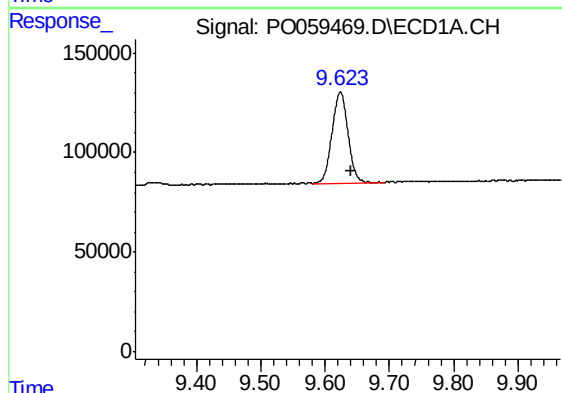


#2 Decachlorobiphenyl

R.T.: 9.624 min
Delta R.T.: -0.017 min
Response: 792471
Conc: 14.90 ng/ml

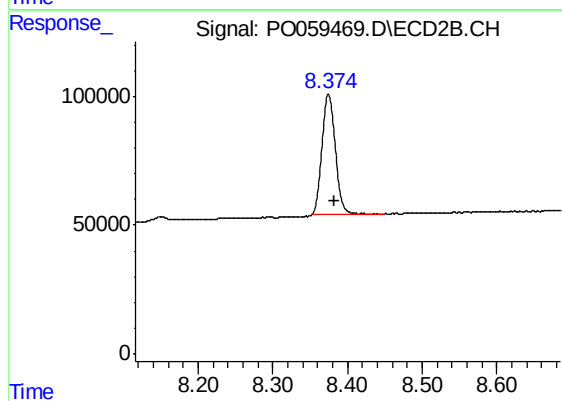

#2 Decachlorobiphenyl


R.T.: 8.375 min
Delta R.T.: -0.009 min
Response: 566328
Conc: 14.05 ng/ml

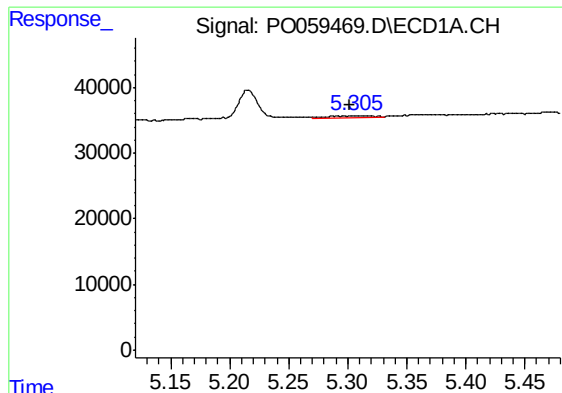

#3 AR-1016-1


R.T.: 5.305 min
Delta R.T.: 0.003 min
Response: 7363
Conc: 4.59 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

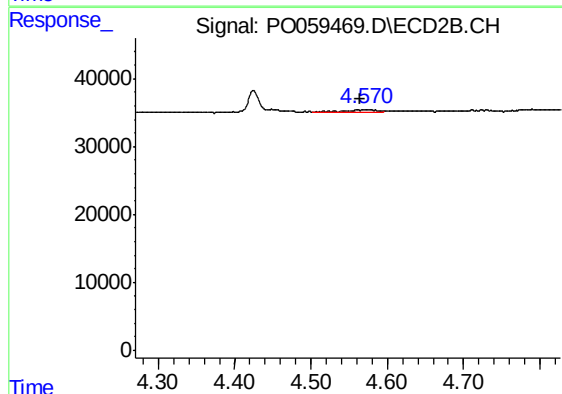


#3 AR-1016-1

R.T.: 4.572 min
Delta R.T.: 0.007 min
Response: 10561
Conc: 7.81 ng/ml

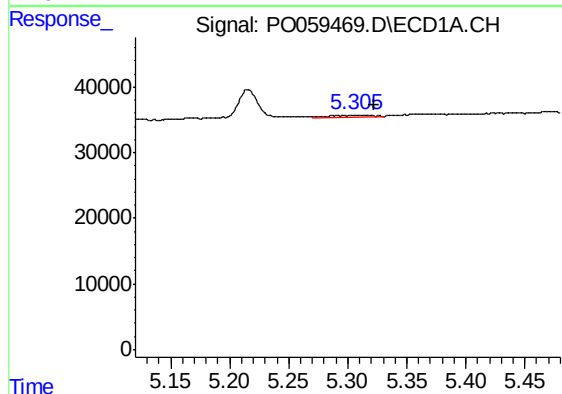


#4 AR-1016-2

R.T.: 5.305 min
Delta R.T.: -0.018 min
Response: 7363
Conc: 3.08 ng/ml

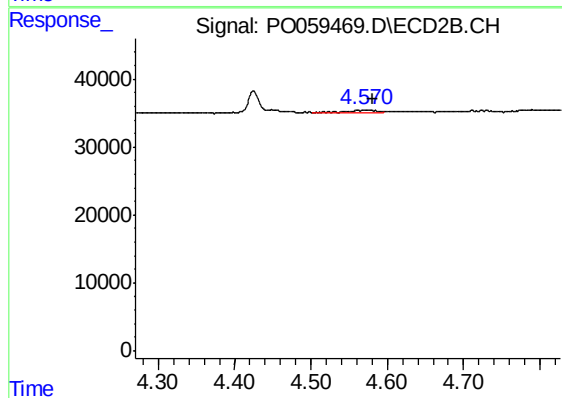

#4 AR-1016-2


R.T.: 4.572 min
Delta R.T.: -0.010 min
Response: 10561
Conc: 5.27 ng/ml

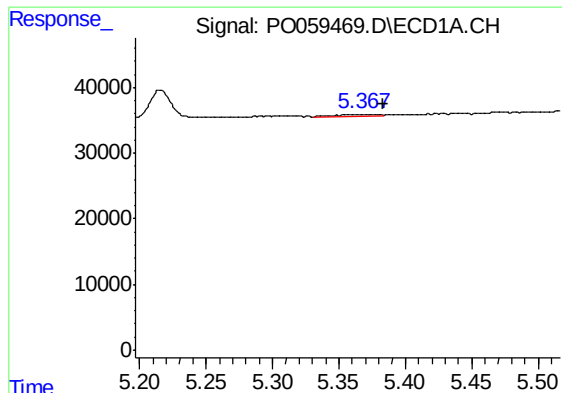

#5 AR-1016-3


R.T.: 5.361 min
Delta R.T.: -0.023 min
Response: 4909
Conc: 3.30 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

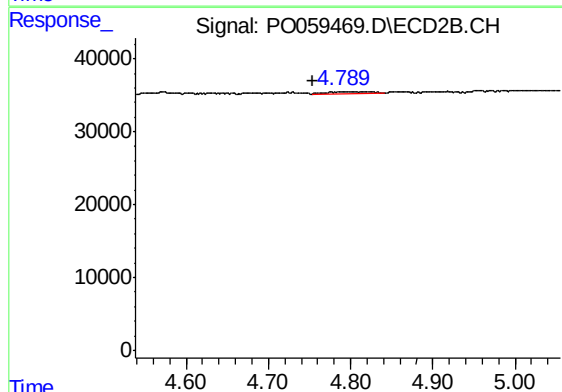


#5 AR-1016-3

R.T.: 4.790 min
Delta R.T.: 0.036 min
Response: 8340
Conc: 7.71 ng/ml

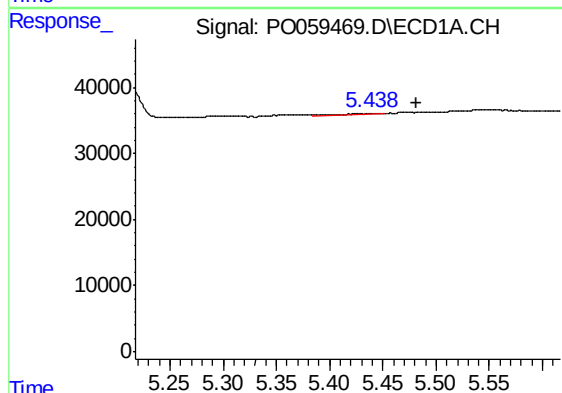


#6 AR-1016-4

R.T.: 5.438 min
Delta R.T.: -0.044 min
Response: 5391
Conc: 4.46 ng/ml

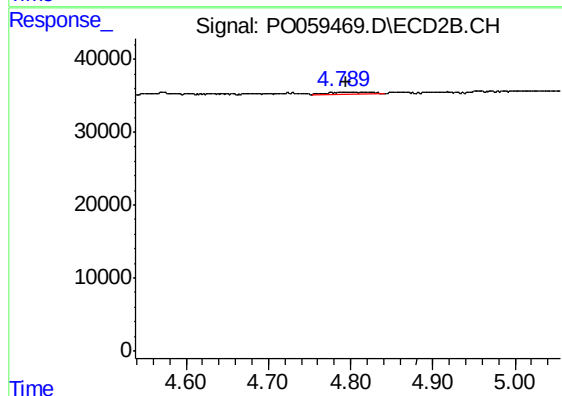

#6 AR-1016-4


R.T.: 4.790 min
Delta R.T.: -0.005 min
Response: 8340
Conc: 9.24 ng/ml

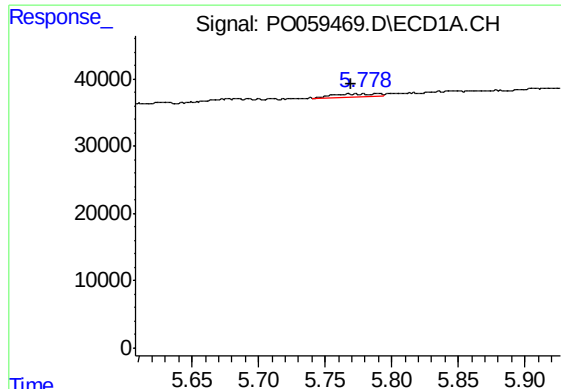

#7 AR-1016-5


R.T.: 5.779 min
Delta R.T.: 0.009 min
Response: 9220
Conc: 7.18 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

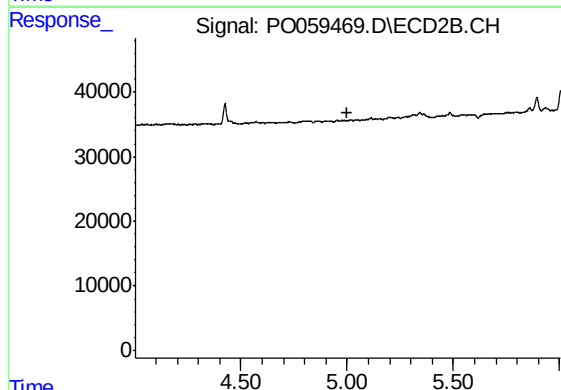


#7 AR-1016-5

R.T.: 0.000 min
Exp R.T. : 5.004 min
Response: 0
Conc: N.D.

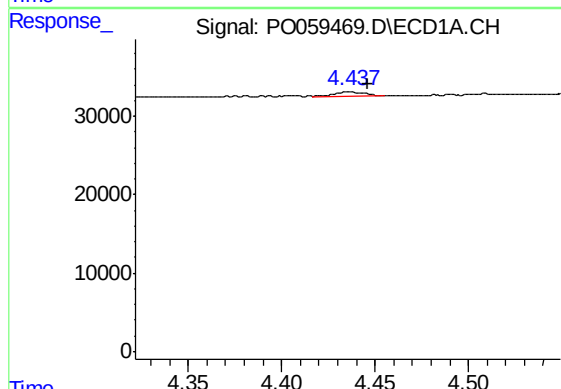


#9 AR-1221-2

R.T.: 4.437 min
Delta R.T.: -0.009 min
Response: 5928
Conc: 18.25 ng/ml

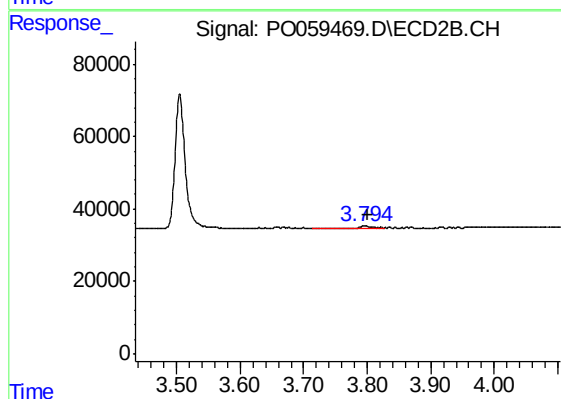

#9 AR-1221-2


R.T.: 3.796 min
Delta R.T.: -0.005 min
Response: 5831
Conc: 19.14 ng/ml

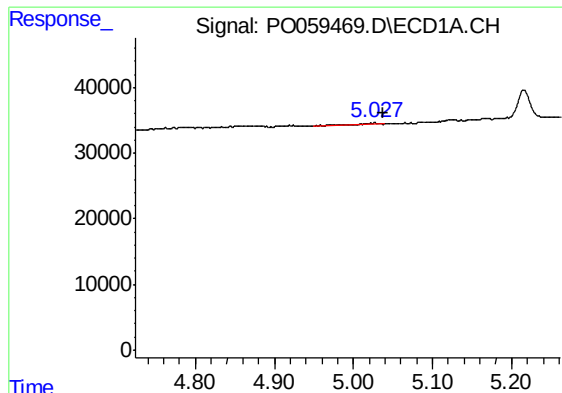

#12 AR-1232-2


R.T.: 5.027 min
Delta R.T.: -0.011 min
Response: 4275
Conc: 6.05 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

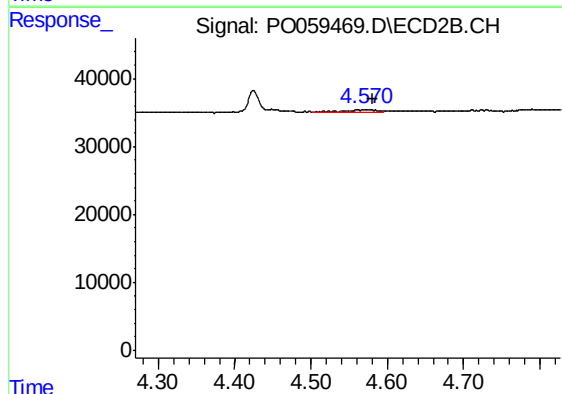


#12 AR-1232-2

R.T.: 4.572 min
Delta R.T.: -0.009 min
Response: 10561
Conc: 8.29 ng/ml

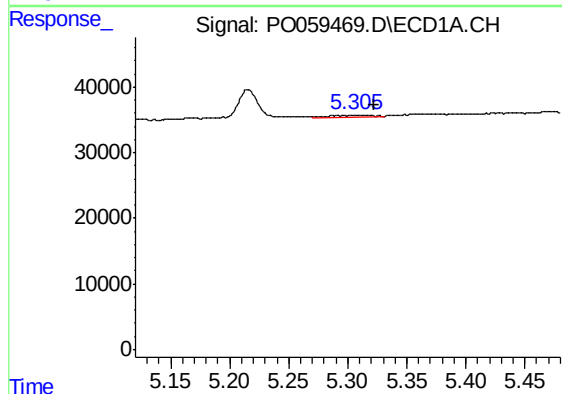


#13 AR-1232-3

R.T.: 5.305 min
Delta R.T.: -0.017 min
Response: 7363
Conc: 4.81 ng/ml

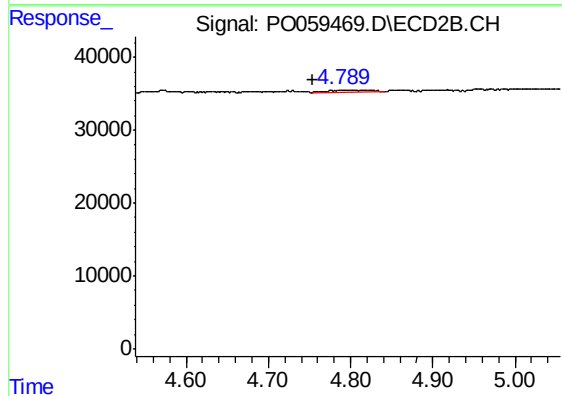

#13 AR-1232-3


R.T.: 4.790 min
Delta R.T.: 0.037 min
Response: 8340
Conc: 12.25 ng/ml



#14 AR-1232-4


R.T.: 5.438 min
Delta R.T.: -0.044 min
Response: 5391
Conc: 6.89 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

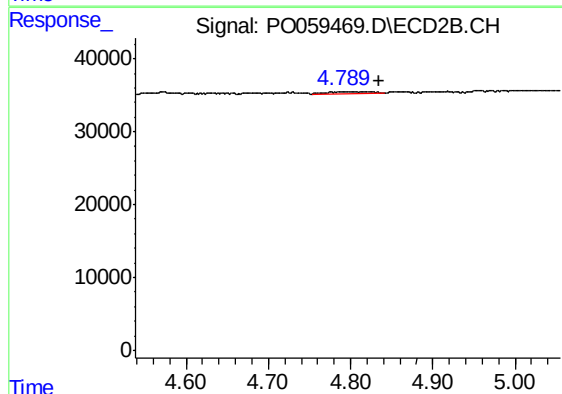


#14 AR-1232-4

R.T.: 4.790 min
Delta R.T.: -0.044 min
Response: 8340
Conc: 13.67 ng/ml




#15 AR-1232-5

R.T.: 5.556 min
Delta R.T.: -0.012 min
Response: 9227
Conc: 15.35 ng/ml

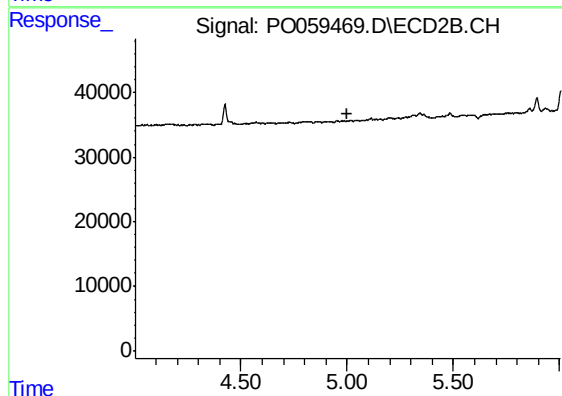

#15 AR-1232-5


R.T.: 0.000 min
Exp R.T. : 5.004 min
Response: 0
Conc: N.D.

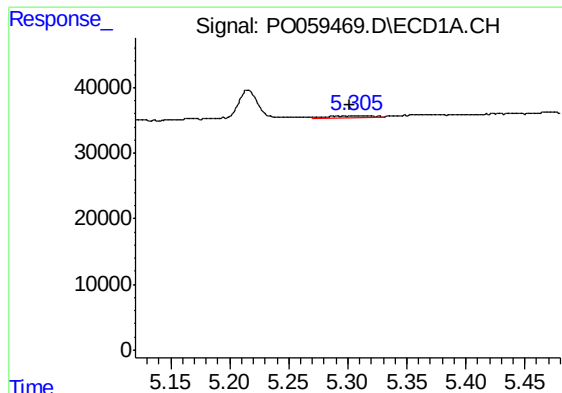

#16 AR-1242-1


R.T.: 5.305 min
Delta R.T.: 0.003 min
Response: 7363
Conc: 5.80 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

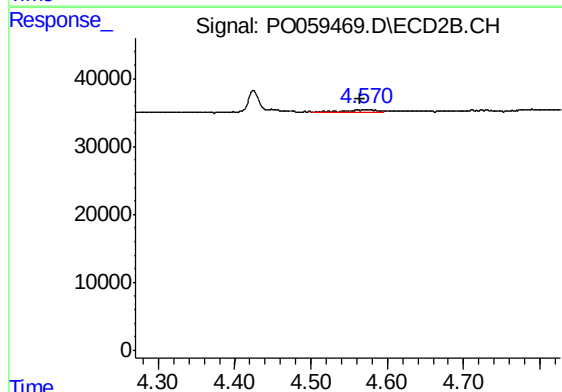


#16 AR-1242-1

R.T.: 4.572 min
Delta R.T.: 0.007 min
Response: 10561
Conc: 10.27 ng/ml




#17 AR-1242-2

R.T.: 5.305 min
Delta R.T.: -0.018 min
Response: 7363
Conc: 3.97 ng/ml

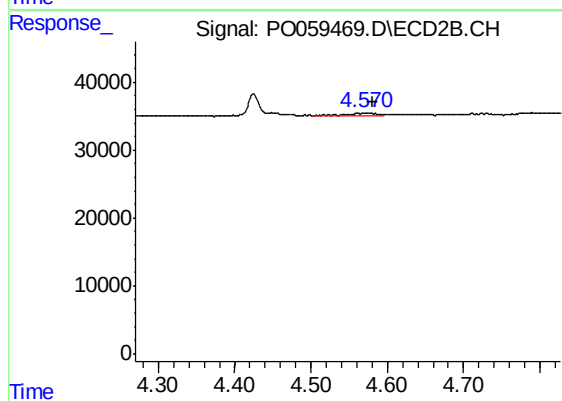

#17 AR-1242-2


R.T.: 4.572 min
Delta R.T.: -0.010 min
Response: 10561
Conc: 6.93 ng/ml

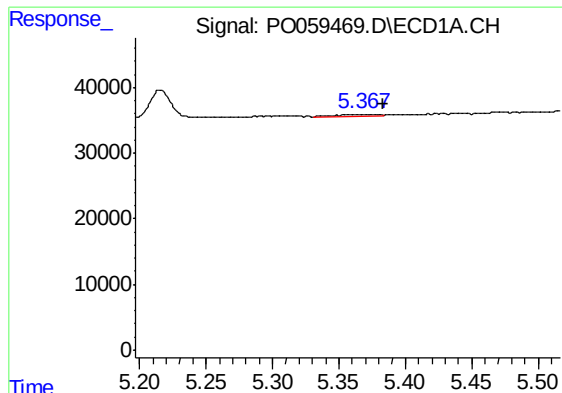

#18 AR-1242-3


R.T.: 5.361 min
Delta R.T.: -0.023 min
Response: 4909
Conc: 4.20 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

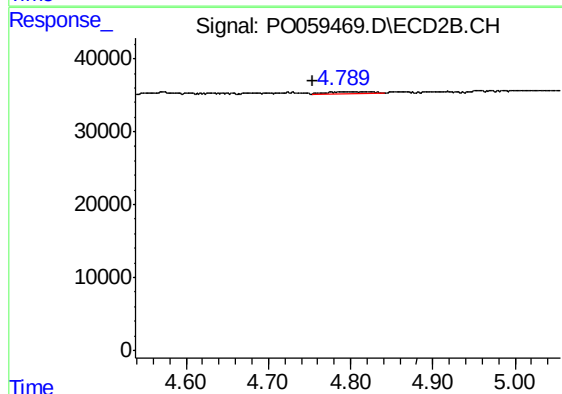


#18 AR-1242-3

R.T.: 4.790 min
Delta R.T.: 0.036 min
Response: 8340
Conc: 9.98 ng/ml




#19 AR-1242-4

R.T.: 5.438 min
Delta R.T.: -0.044 min
Response: 5391
Conc: 5.57 ng/ml

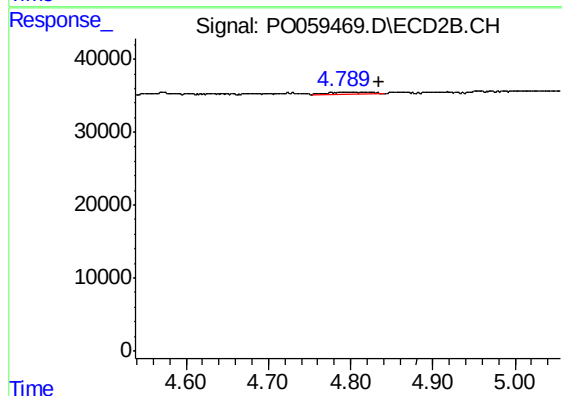

#19 AR-1242-4


R.T.: 4.790 min
Delta R.T.: -0.044 min
Response: 8340
Conc: 10.00 ng/ml



#20 AR-1242-5


R.T.: 6.204 min
Delta R.T.: -0.002 min
Response: 3823
Conc: 3.04 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

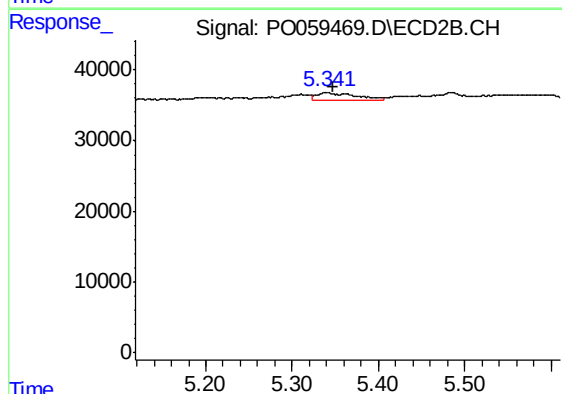


#20 AR-1242-5

R.T.: 5.340 min
Delta R.T.: -0.008 min
Response: 31512
Conc: 28.17 ng/ml

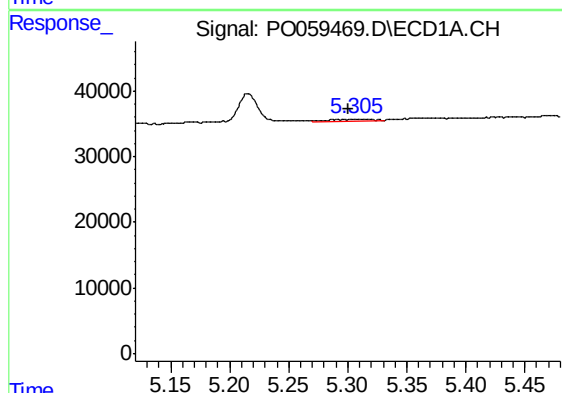


#21 AR-1248-1

R.T.: 5.305 min
Delta R.T.: 0.004 min
Response: 7363
Conc: 7.34 ng/ml

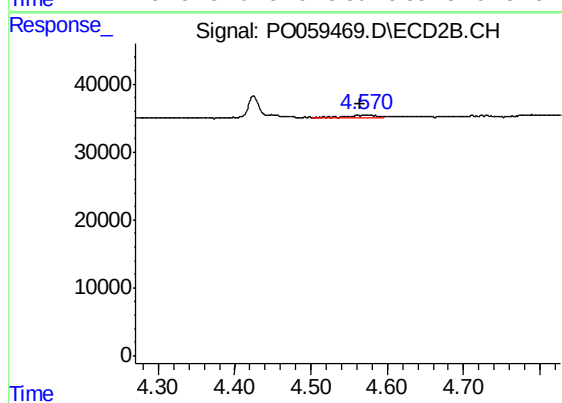

#21 AR-1248-1


R.T.: 4.572 min
Delta R.T.: 0.007 min
Response: 10561
Conc: 12.75 ng/ml

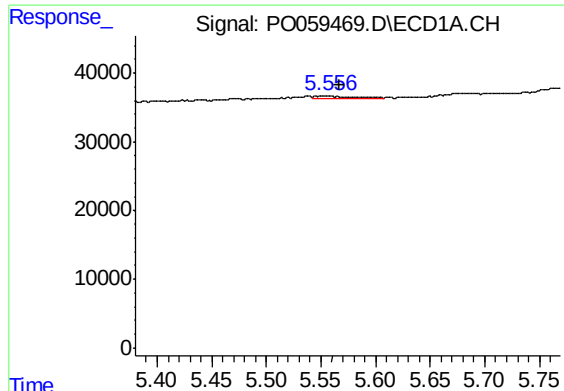

#22 AR-1248-2


R.T.: 5.556 min
Delta R.T.: -0.011 min
Response: 9227
Conc: 6.36 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

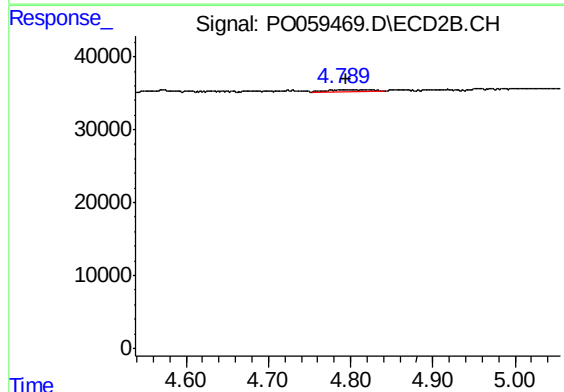


#22 AR-1248-2

R.T.: 4.790 min
Delta R.T.: -0.004 min
Response: 8340
Conc: 7.23 ng/ml

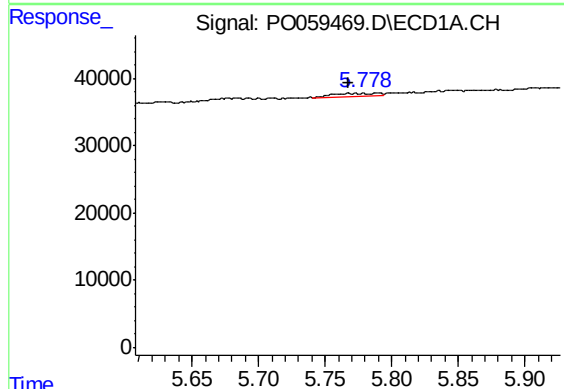


#23 AR-1248-3

R.T.: 5.779 min
Delta R.T.: 0.011 min
Response: 9220
Conc: 5.55 ng/ml

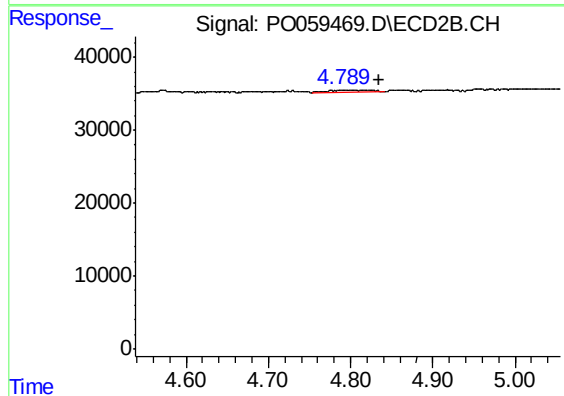

#23 AR-1248-3


R.T.: 4.790 min
Delta R.T.: -0.045 min
Response: 8340
Conc: 7.02 ng/ml



#24 AR-1248-4


R.T.: 6.204 min
Delta R.T.: 0.035 min
Response: 3823
Conc: 1.87 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

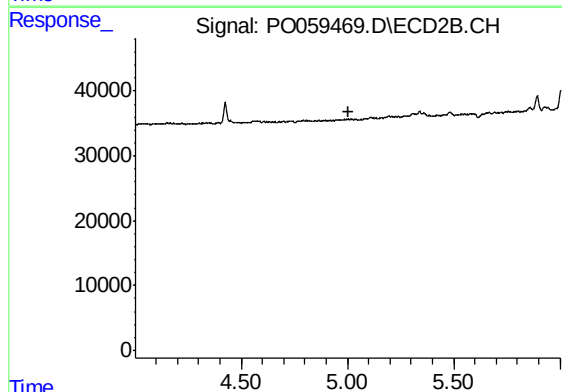


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 5.003 min
Response: 0
Conc: N.D.




#25 AR-1248-5

R.T.: 6.204 min
Delta R.T.: -0.001 min
Response: 3823
Conc: 1.93 ng/ml

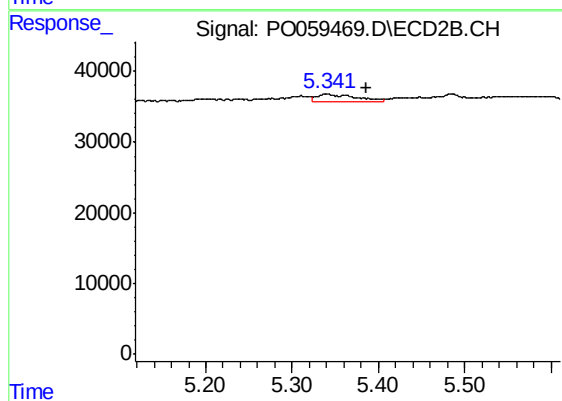

#25 AR-1248-5


R.T.: 5.340 min
Delta R.T.: -0.047 min
Response: 31512
Conc: 22.02 ng/ml

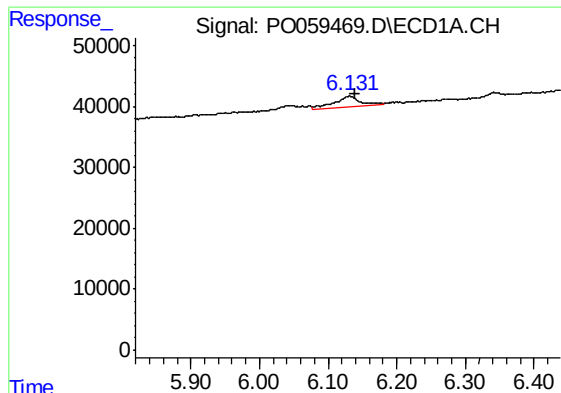

#26 AR-1254-1


R.T.: 6.132 min
Delta R.T.: -0.007 min
Response: 46988
Conc: 22.52 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

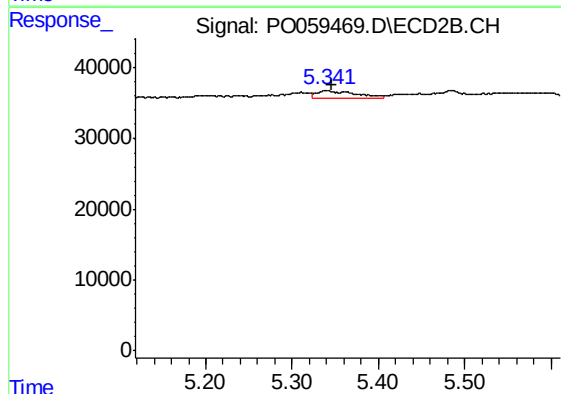


#26 AR-1254-1

R.T.: 5.340 min
Delta R.T.: -0.007 min
Response: 31512
Conc: 13.29 ng/ml

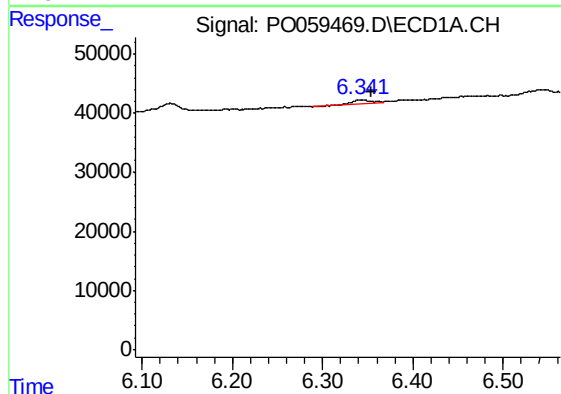


#27 AR-1254-2

R.T.: 6.341 min
Delta R.T.: -0.013 min
Response: 12583
Conc: 3.77 ng/ml

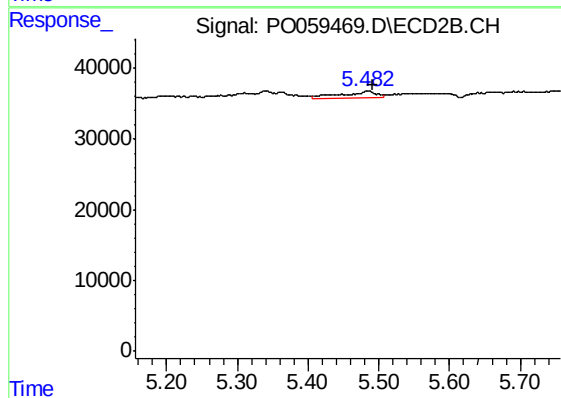

#27 AR-1254-2


R.T.: 5.484 min
Delta R.T.: -0.008 min
Response: 31969
Conc: 15.24 ng/ml



#28 AR-1254-3


R.T.: 6.708 min
Delta R.T.: -0.012 min
Response: 5345
Conc: 1.51 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

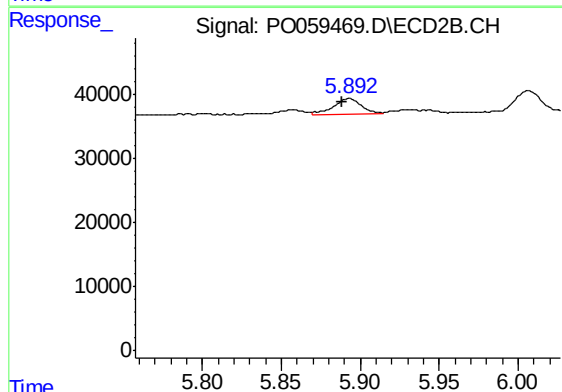


#28 AR-1254-3

R.T.: 5.893 min
Delta R.T.: 0.004 min
Response: 30639
Conc: 9.11 ng/ml




#29 AR-1254-4

R.T.: 6.995 min
Delta R.T.: -0.009 min
Response: 8896
Conc: 3.02 ng/ml

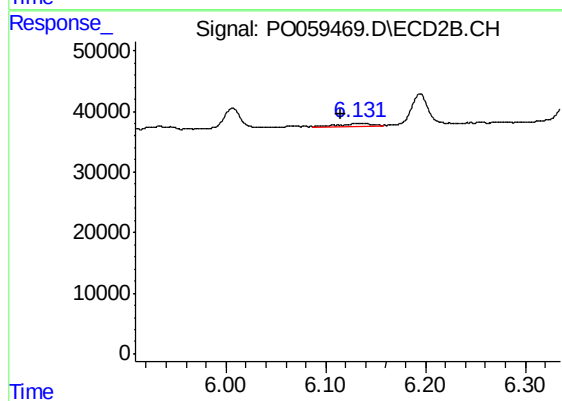

#29 AR-1254-4


R.T.: 6.135 min
Delta R.T.: 0.020 min
Response: 8572
Conc: 4.16 ng/ml



#30 AR-1254-5


R.T.: 7.406 min
Delta R.T.: -0.013 min
Response: 54447
Conc: 17.61 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

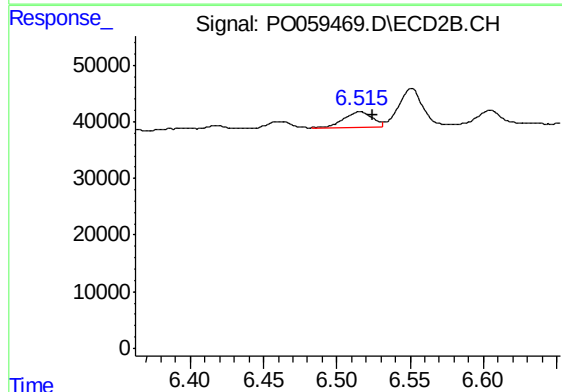


#30 AR-1254-5

R.T.: 6.516 min
Delta R.T.: -0.008 min
Response: 37163
Conc: 11.97 ng/ml

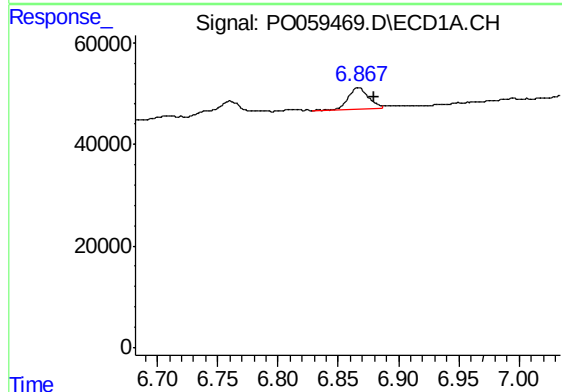


#31 AR-1260-1

R.T.: 6.867 min
Delta R.T.: -0.013 min
Response: 50339
Conc: 18.67 ng/ml

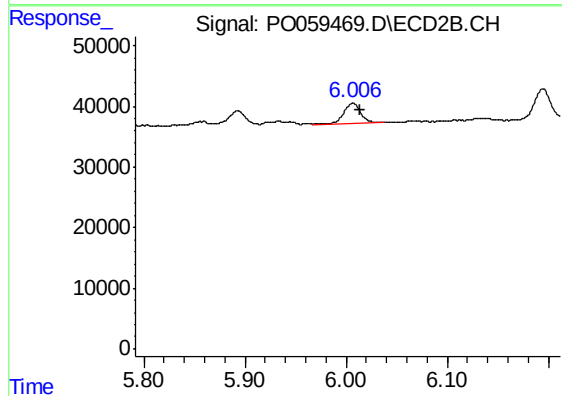

#31 AR-1260-1


R.T.: 6.007 min
Delta R.T.: -0.008 min
Response: 39434
Conc: 17.30 ng/ml



#32 AR-1260-2


R.T.: 7.122 min
Delta R.T.: -0.013 min
Response: 70728
Conc: 19.06 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

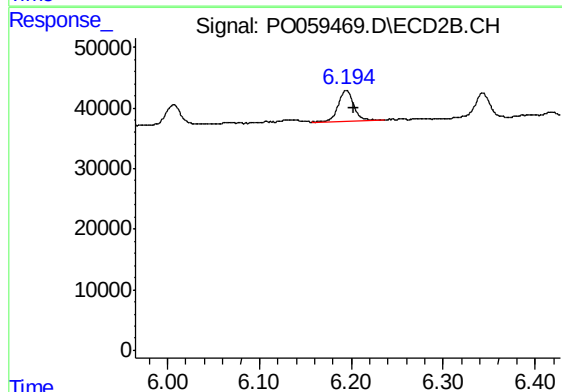


#32 AR-1260-2

R.T.: 6.194 min
Delta R.T.: -0.008 min
Response: 59960
Conc: 20.47 ng/ml

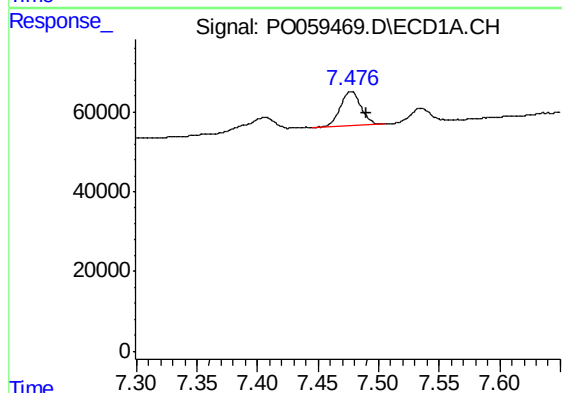


#33 AR-1260-3

R.T.: 7.477 min
Delta R.T.: -0.013 min
Response: 102719
Conc: 31.35 ng/ml

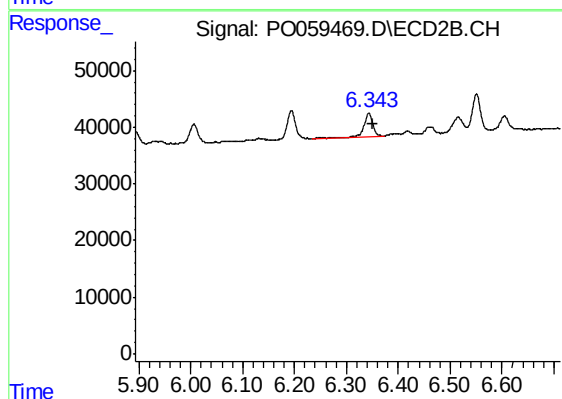

#33 AR-1260-3


R.T.: 6.343 min
Delta R.T.: -0.008 min
Response: 51636
Conc: 19.49 ng/ml



#34 AR-1260-4


R.T.: 7.705 min
Delta R.T.: -0.012 min
Response: 90707
Conc: 29.53 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

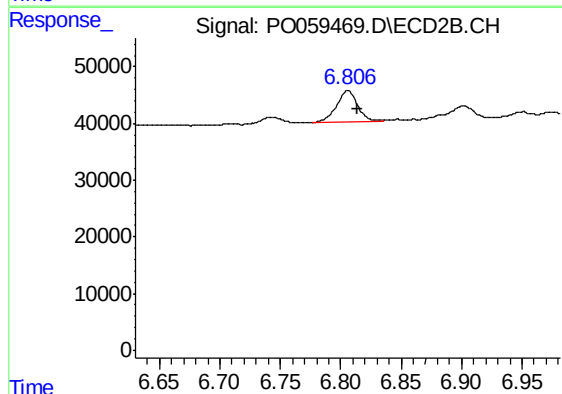


#34 AR-1260-4

R.T.: 6.806 min
Delta R.T.: -0.008 min
Response: 67358
Conc: 29.77 ng/ml

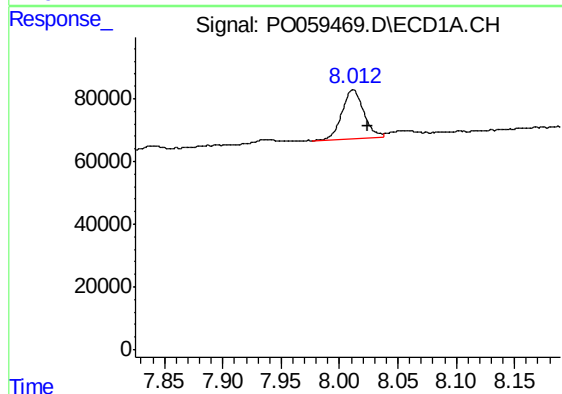


#35 AR-1260-5

R.T.: 8.012 min
Delta R.T.: -0.012 min
Response: 204972
Conc: 28.95 ng/ml

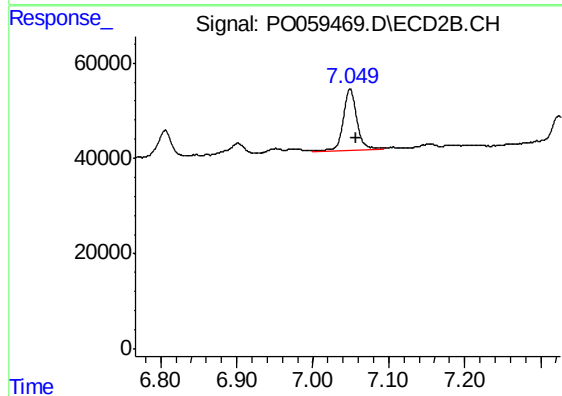

#35 AR-1260-5


R.T.: 7.049 min
Delta R.T.: -0.008 min
Response: 163883
Conc: 29.78 ng/ml

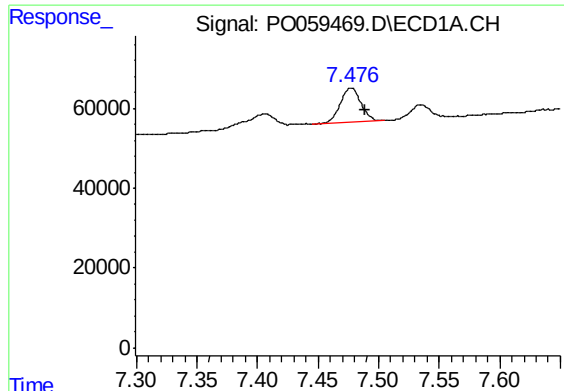

#36 AR-1262-1


R.T.: 7.477 min
Delta R.T.: -0.011 min
Response: 102719
Conc: 21.17 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

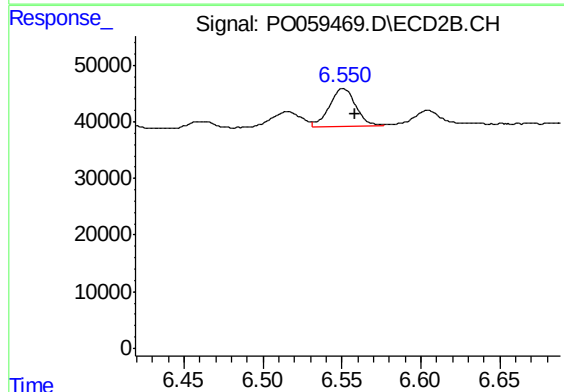


#36 AR-1262-1

R.T.: 6.551 min
Delta R.T.: -0.007 min
Response: 76896
Conc: 20.63 ng/ml

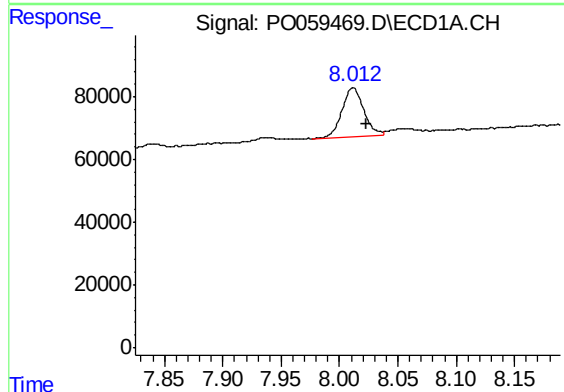


#37 AR-1262-2

R.T.: 8.012 min
Delta R.T.: -0.011 min
Response: 204972
Conc: 26.56 ng/ml

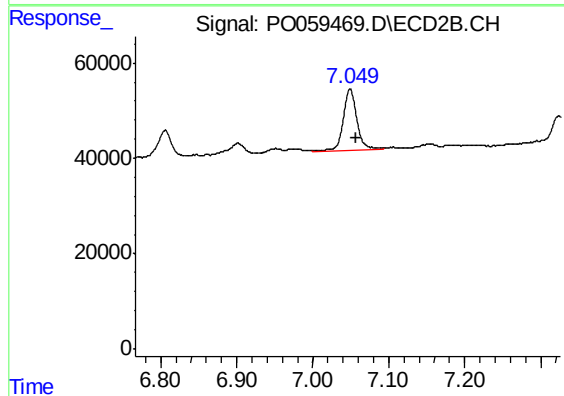

#37 AR-1262-2


R.T.: 7.049 min
Delta R.T.: -0.008 min
Response: 163883
Conc: 27.88 ng/ml

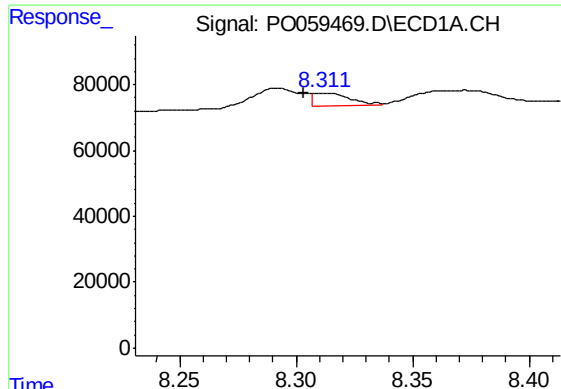

#38 AR-1262-3


R.T.: 8.312 min
Delta R.T.: 0.009 min
Response: 44339
Conc: 8.69 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

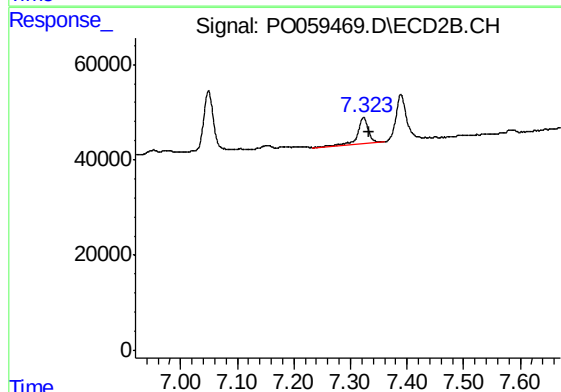


#38 AR-1262-3

R.T.: 7.323 min
Delta R.T.: -0.009 min
Response: 75000
Conc: 29.52 ng/ml

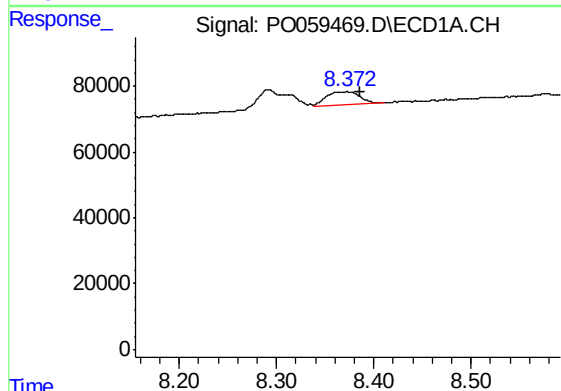


#39 AR-1262-4

R.T.: 8.372 min
Delta R.T.: -0.014 min
Response: 96300
Conc: 24.98 ng/ml

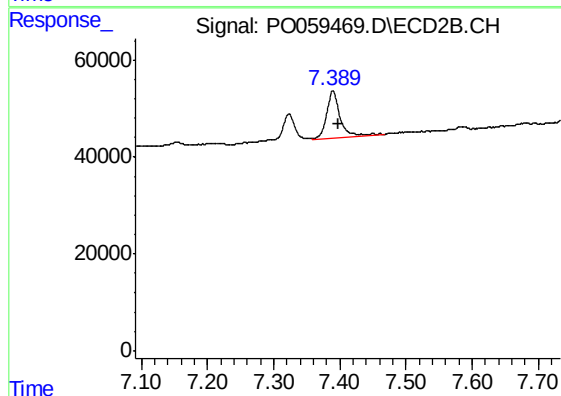

#39 AR-1262-4


R.T.: 7.390 min
Delta R.T.: -0.008 min
Response: 136214
Conc: 30.82 ng/ml

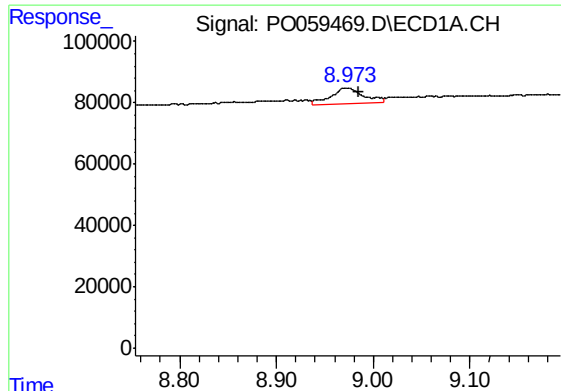

#40 AR-1262-5


R.T.: 8.974 min
Delta R.T.: -0.012 min
Response: 122320
Conc: 47.66 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

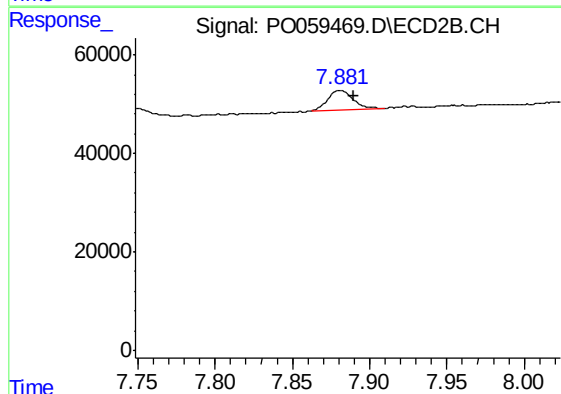


#40 AR-1262-5

R.T.: 7.881 min
Delta R.T.: -0.008 min
Response: 44024
Conc: 24.38 ng/ml

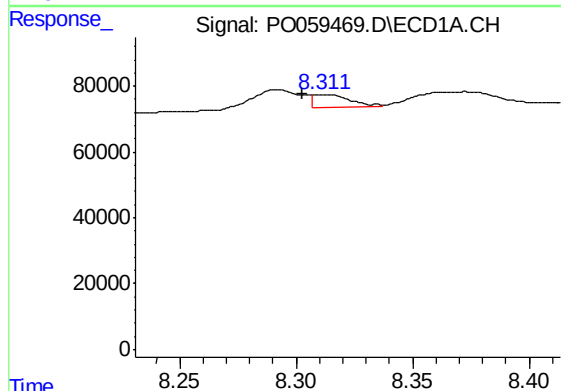


#41 AR-1268-1

R.T.: 8.312 min
Delta R.T.: 0.009 min
Response: 44339
Conc: 4.71 ng/ml

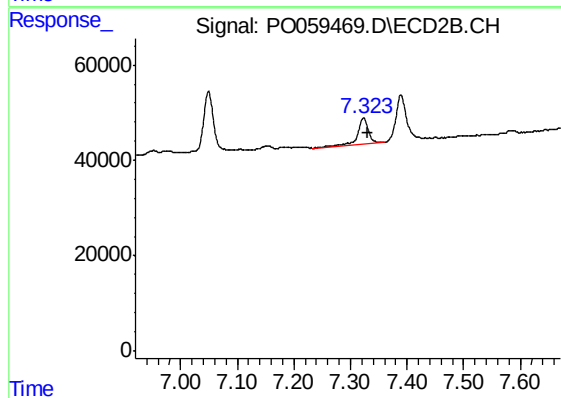

#41 AR-1268-1


R.T.: 7.323 min
Delta R.T.: -0.007 min
Response: 75000
Conc: 10.53 ng/ml



#42 AR-1268-2


R.T.: 8.372 min
Delta R.T.: -0.018 min
Response: 96300
Conc: 12.22 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

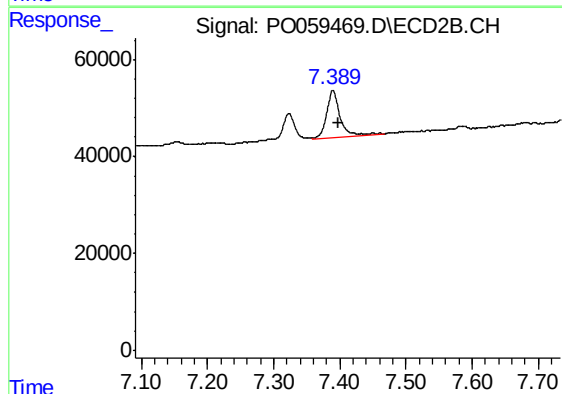


#42 AR-1268-2

R.T.: 7.390 min
Delta R.T.: -0.008 min
Response: 136214
Conc: 21.12 ng/ml

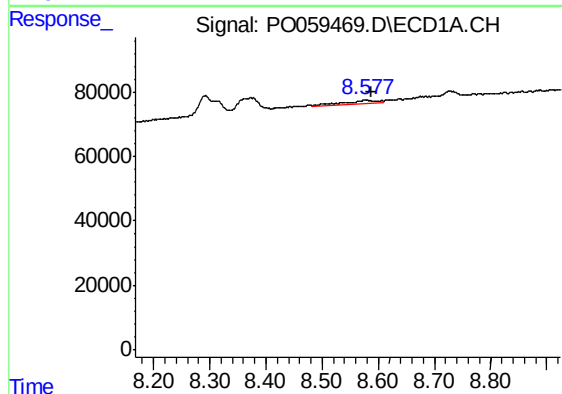


#43 AR-1268-3

R.T.: 8.578 min
Delta R.T.: -0.011 min
Response: 53828
Conc: 7.64 ng/ml

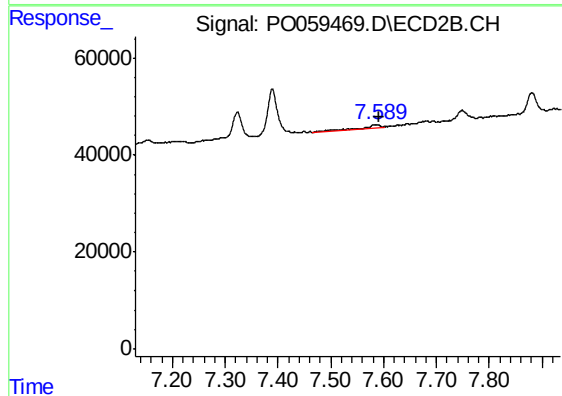

#43 AR-1268-3


R.T.: 7.586 min
Delta R.T.: -0.007 min
Response: 12743
Conc: 2.33 ng/ml

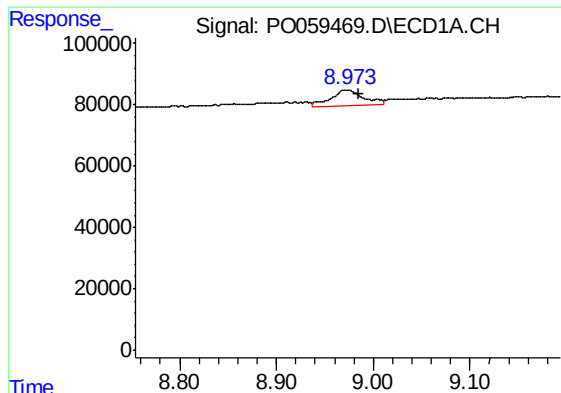

#44 AR-1268-4


R.T.: 8.974 min
Delta R.T.: -0.012 min
Response: 122320
Conc: 44.00 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

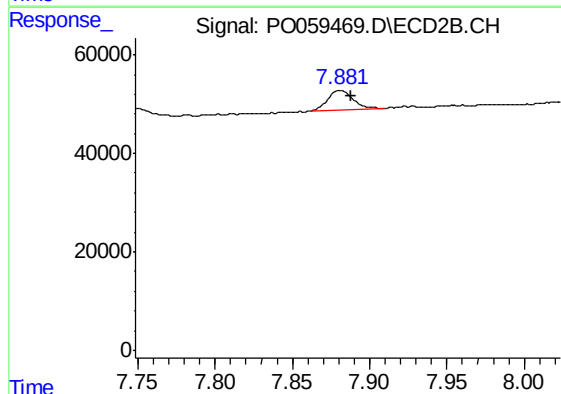


#44 AR-1268-4

R.T.: 7.881 min
Delta R.T.: -0.007 min
Response: 44024
Conc: 21.57 ng/ml

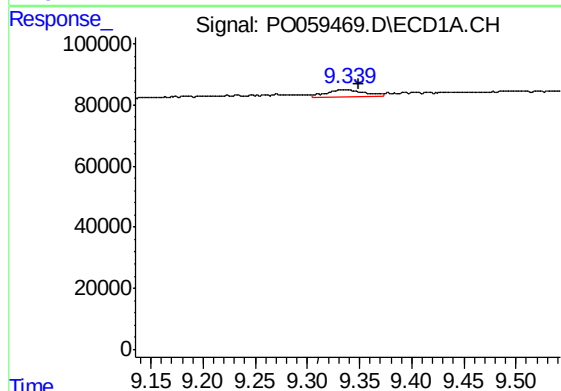

#45 AR-1268-5

R.T.: 9.338 min
Delta R.T.: -0.011 min
Response: 58823
Conc: 3.19 ng/ml

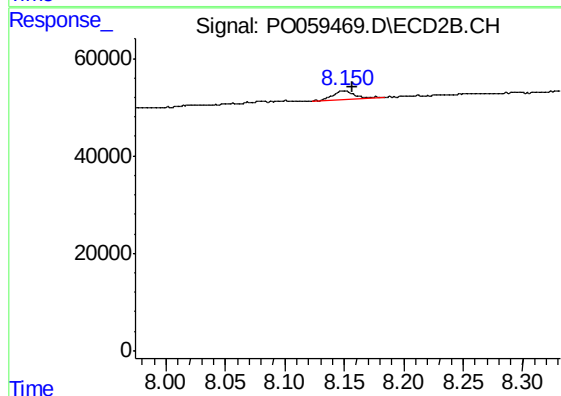

#45 AR-1268-5

R.T.: 8.150 min
Delta R.T.: -0.007 min
Response: 21069
Conc: 1.45 ng/ml