

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0081919\
 Data File : P0059465.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Aug 2019 18:52
 Operator : SM/AJ
 Sample : K3591-09
 Misc : AR1232 MDL 25PPB
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 MDL-MDL-WATER-03-QT3-2019

Manual Integrations
 APPROVED

Ankita
 8/21/2019 12:58:11 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 20 01:07:05 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0081719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 17 03:09:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.141	3.505	595433	558393	17.006	15.513
2)	SA Decachlor...	9.627	8.375	937358	685935	17.619	17.012
Target Compounds							
11)	L3 AR-1232-1	4.514	3.868	35302	31272	28.322	27.428
12)	L3 AR-1232-2	5.028	4.573	21191	31848	29.998	25.007m
13)	L3 AR-1232-3	5.314	4.742	41651	20191	27.199	29.653m
14)	L3 AR-1232-4	5.474	4.827	19750	15128	25.260	24.797m
15)	L3 AR-1232-5	5.558	4.997	15003	16646	24.958m	24.453

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081919\
Data File : PO059465.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Aug 2019 18:52
Operator : SM/AJ
Sample : K3591-09
Misc : AR1232 MDL 25PPB
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019


Manual Integrations
APPROVED

Ankita
8/21/2019 12:58:11 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 20 01:07:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Aug 17 03:09:44 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

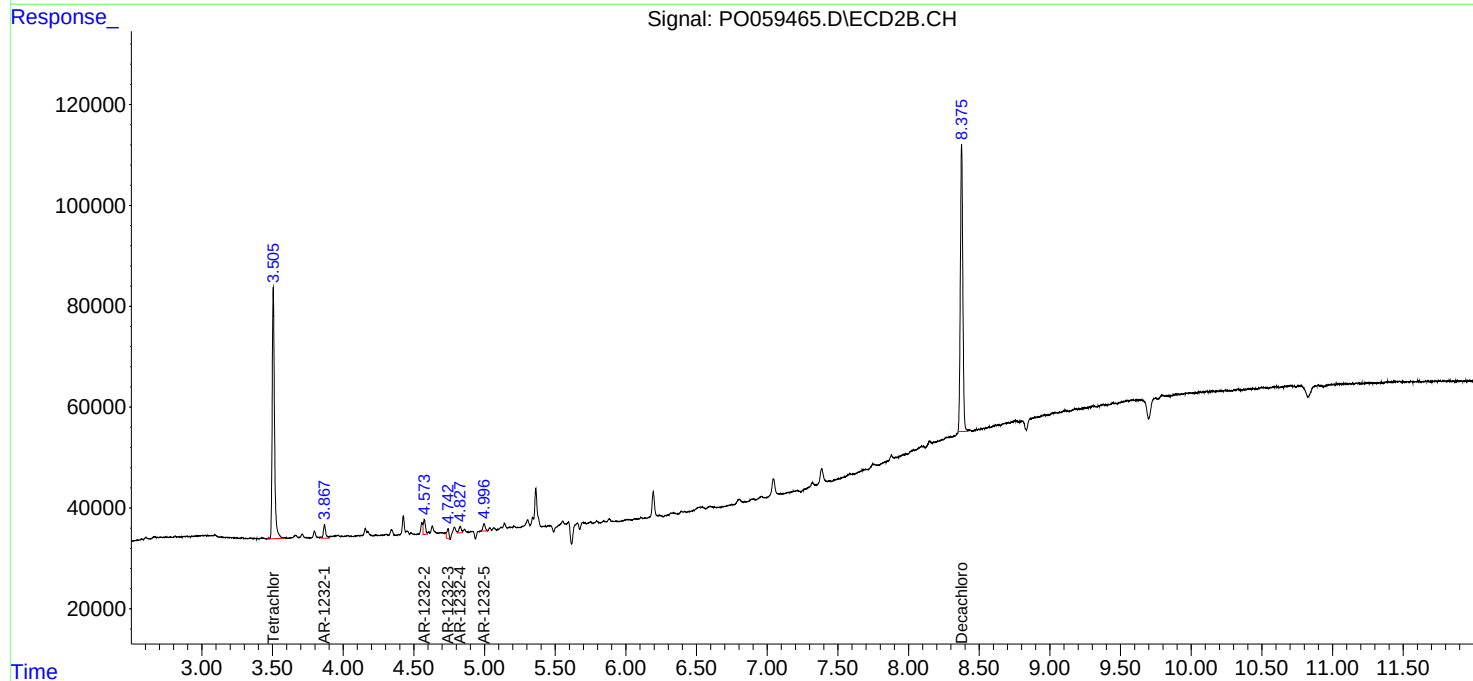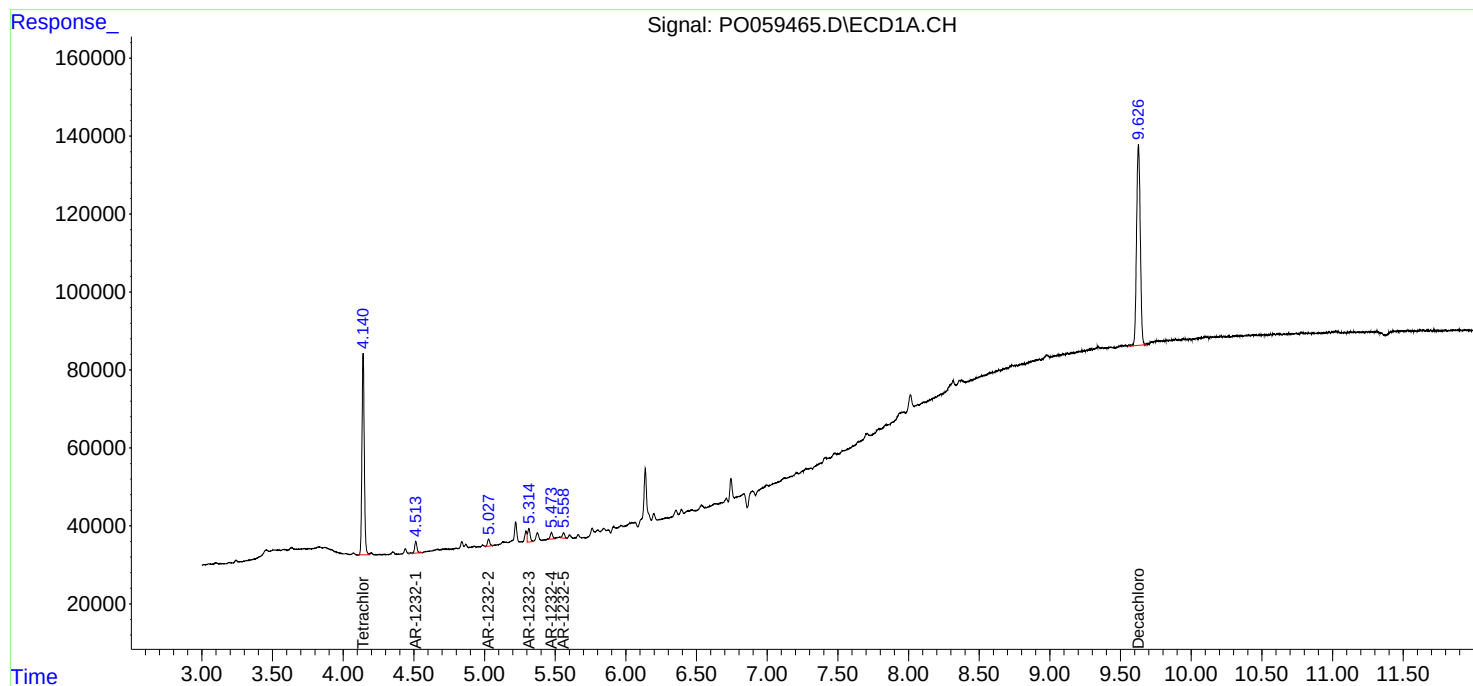

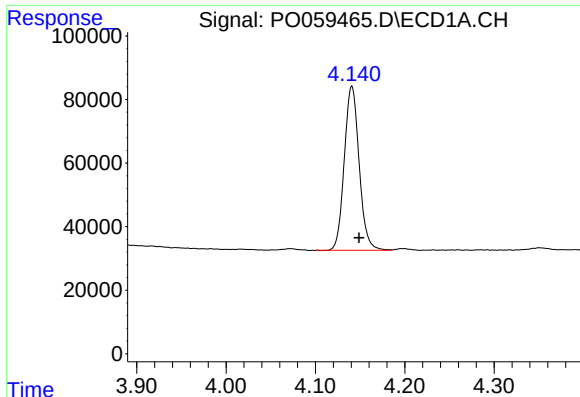


#1 Tetrachloro-m-xylene

R.T.: 4.141 min
Delta R.T.: -0.008 min
Response: 595433
Conc: 17.01 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019


Manual Integrations
APPROVED

Ankita
8/21/2019 12:58:11 PM

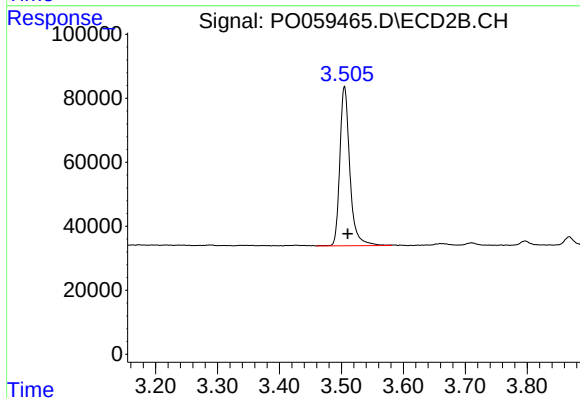


#1 Tetrachloro-m-xylene

R.T.: 3.505 min
Delta R.T.: -0.005 min
Response: 558393
Conc: 15.51 ng/ml

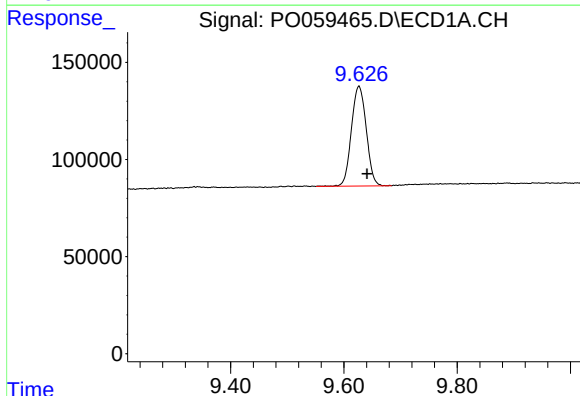


#2 Decachlorobiphenyl

R.T.: 9.627 min
Delta R.T.: -0.014 min
Response: 937358
Conc: 17.62 ng/ml

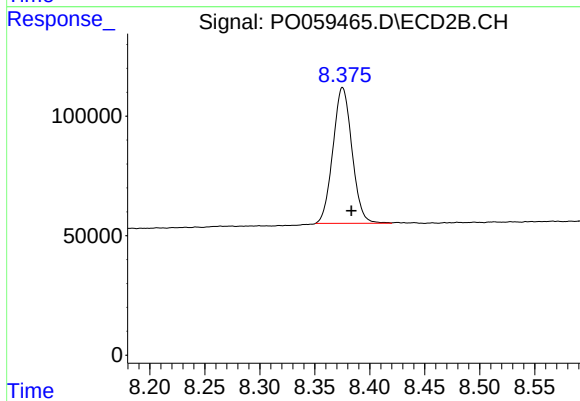

#2 Decachlorobiphenyl

R.T.: 8.375 min
Delta R.T.: -0.008 min
Response: 685935
Conc: 17.01 ng/ml

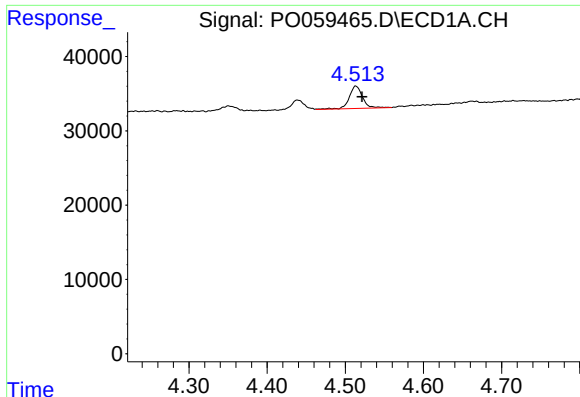


#11 AR-1232-1

R.T.: 4.514 min
Delta R.T.: -0.008 min
Response: 35302
Conc: 28.32 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019


Manual Integrations
APPROVED

Ankita
8/21/2019 12:58:11 PM

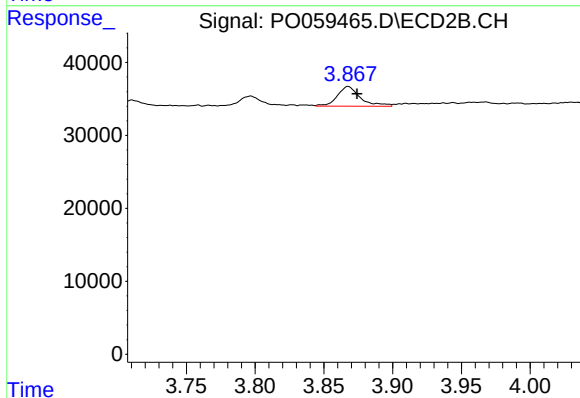


#11 AR-1232-1

R.T.: 3.868 min
Delta R.T.: -0.006 min
Response: 31272
Conc: 27.43 ng/ml

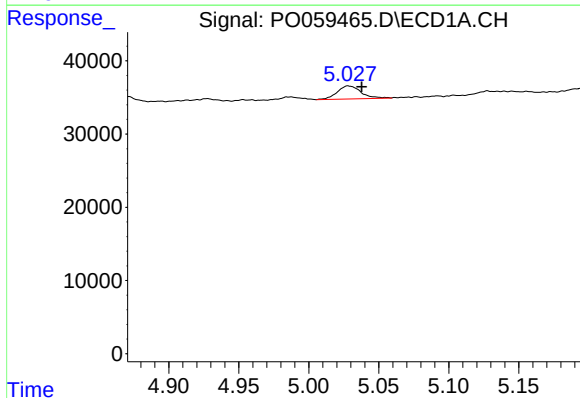


#12 AR-1232-2

R.T.: 5.028 min
Delta R.T.: -0.009 min
Response: 21191
Conc: 30.00 ng/ml

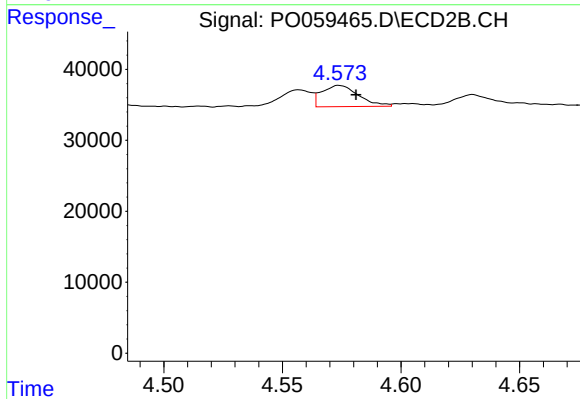

#12 AR-1232-2

R.T.: 4.573 min
Delta R.T.: -0.008 min
Response: 31848
Conc: 25.01 ng/ml m

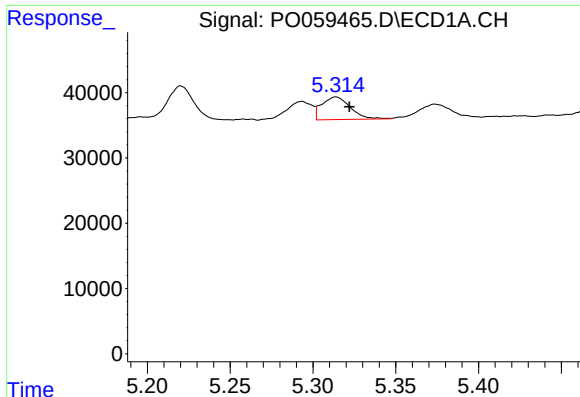


#13 AR-1232-3

R.T.: 5.314 min
Delta R.T.: -0.008 min
Response: 41651
Conc: 27.20 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019


Manual Integrations
APPROVED

Ankita
8/21/2019 12:58:11 PM

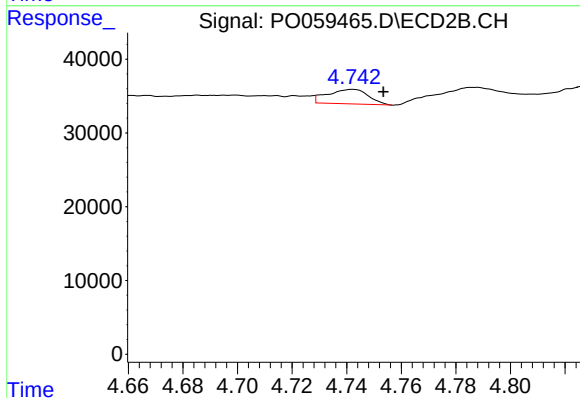


#13 AR-1232-3

R.T.: 4.742 min
Delta R.T.: -0.012 min
Response: 20191
Conc: 29.65 ng/ml m

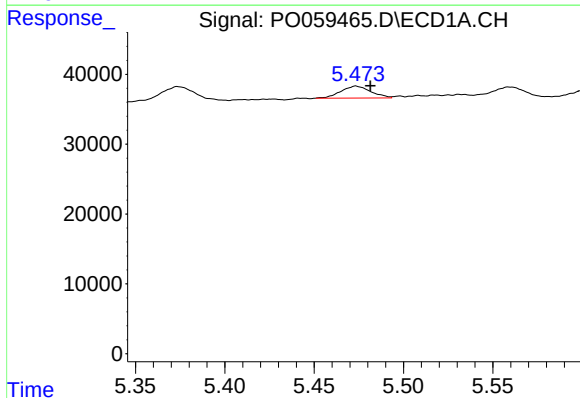


#14 AR-1232-4

R.T.: 5.474 min
Delta R.T.: -0.008 min
Response: 19750
Conc: 25.26 ng/ml

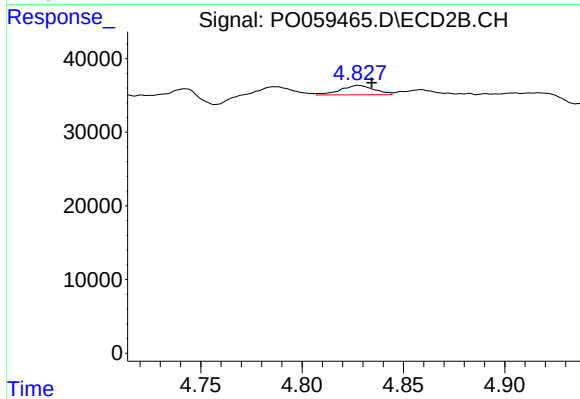

#14 AR-1232-4

R.T.: 4.827 min
Delta R.T.: -0.007 min
Response: 15128
Conc: 24.80 ng/ml m

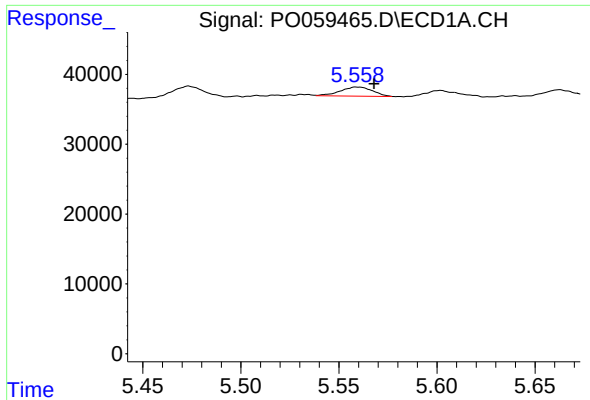


#15 AR-1232-5

R.T.: 5.558 min
Delta R.T.: -0.010 min
Response: 15003
Conc: 24.96 ng/ml m

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

Manual Integrations
APPROVED

Ankita
8/21/2019 12:58:11 PM

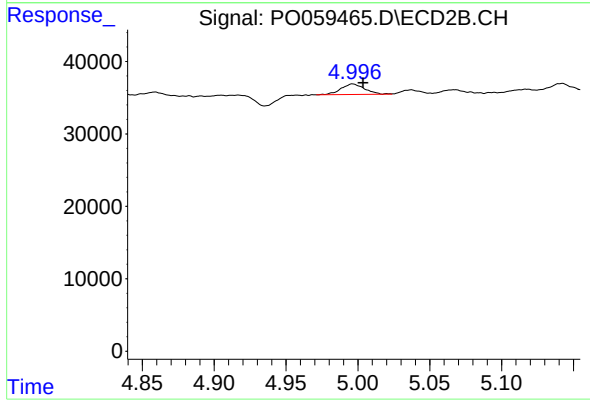

#15 AR-1232-5

R.T.: 4.997 min
Delta R.T.: -0.007 min
Response: 16646
Conc: 24.45 ng/ml