

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081919\
 Data File : P0059468.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Aug 2019 19:42
 Operator : SM/AJ
 Sample : K3591-09
 Misc : AR1254 MDL 25PPB
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-MDL-WATER-03-QT3-2019

Manual Integrations
 APPROVED

Ankita
 8/21/2019 12:58:17 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 20 01:09:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 17 03:09:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.137	3.505	453573	431261	12.955	11.981
2) SA Decachlor...	9.624	8.375	848122	615849	15.942	15.274
Target Compounds						
26) L6 AR-1254-1	6.129	5.340	63881	56709	30.618m	23.910m
27) L6 AR-1254-2	6.344	5.484	79960	45771	23.967	21.813m
28) L6 AR-1254-3	6.709	5.881	84805	69316	23.899	20.614m
29) L6 AR-1254-4	6.993	6.108	77725	50891	26.388	24.683
30) L6 AR-1254-5	7.408	6.517	80461	66883	26.019m	21.541

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081919\
Data File : PO059468.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Aug 2019 19:42
Operator : SM/AJ
Sample : K3591-09
Misc : AR1254 MDL 25PPB
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019


Manual Integrations
APPROVED

Ankita
8/21/2019 12:58:17 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 20 01:09:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Aug 17 03:09:44 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

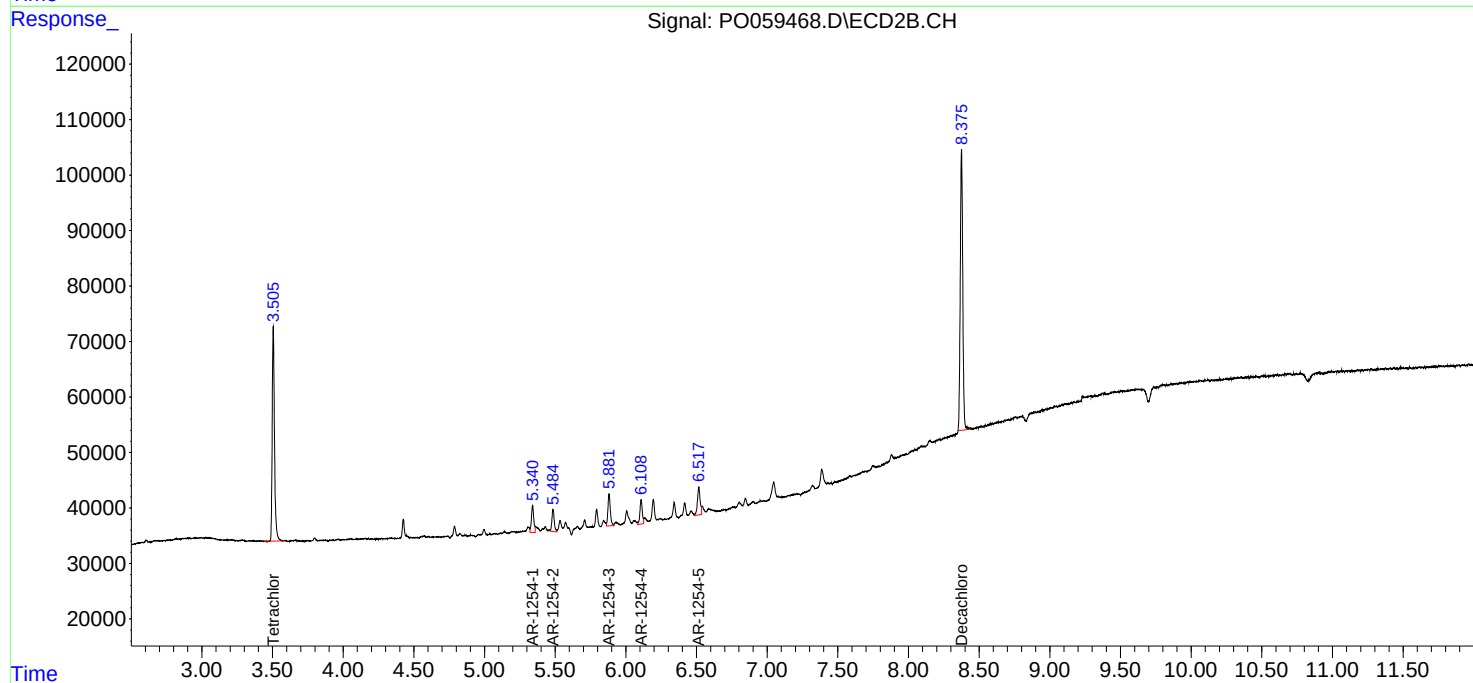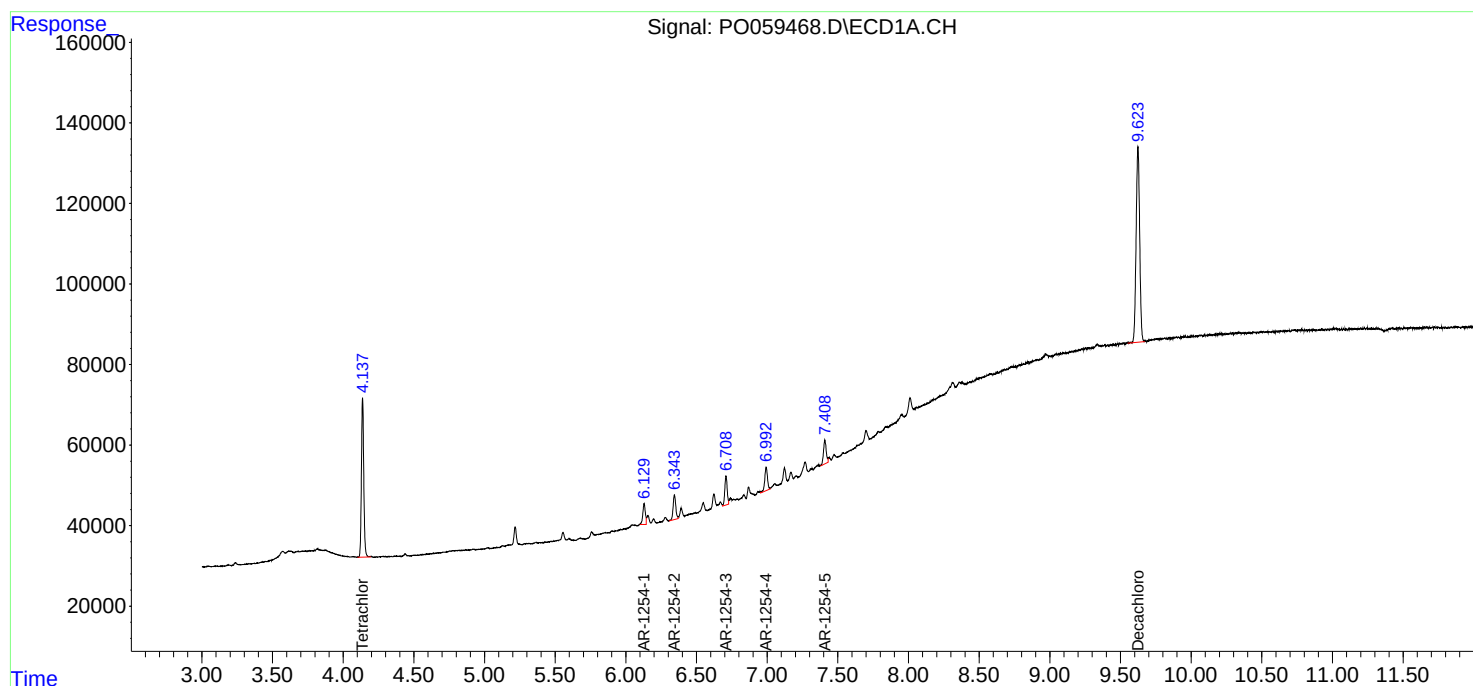

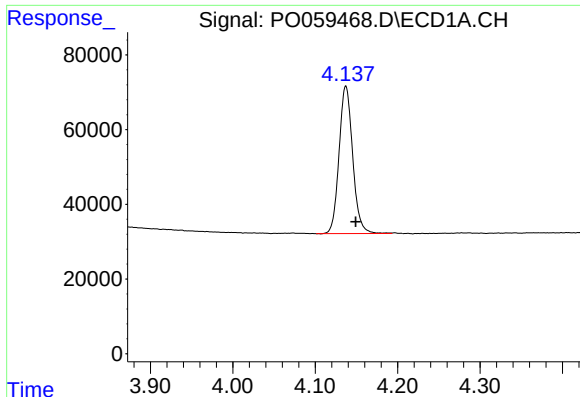


#1 Tetrachloro-m-xylene

R.T.: 4.137 min
Delta R.T.: -0.012 min
Response: 453573
Conc: 12.95 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019


Manual Integrations
APPROVED

Ankita
8/21/2019 12:58:17 PM

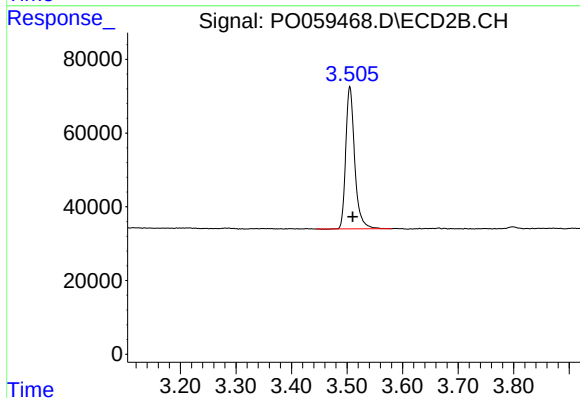


#1 Tetrachloro-m-xylene

R.T.: 3.505 min
Delta R.T.: -0.005 min
Response: 431261
Conc: 11.98 ng/ml

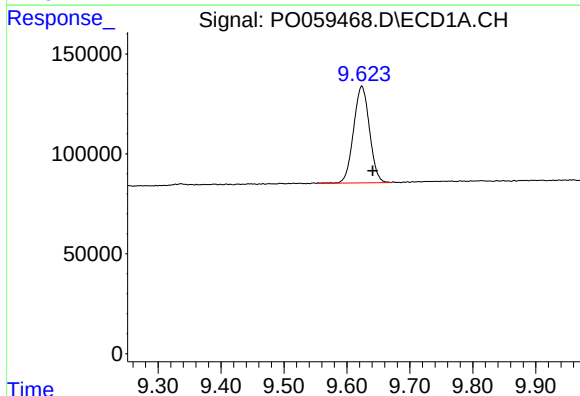


#2 Decachlorobiphenyl

R.T.: 9.624 min
Delta R.T.: -0.017 min
Response: 848122
Conc: 15.94 ng/ml

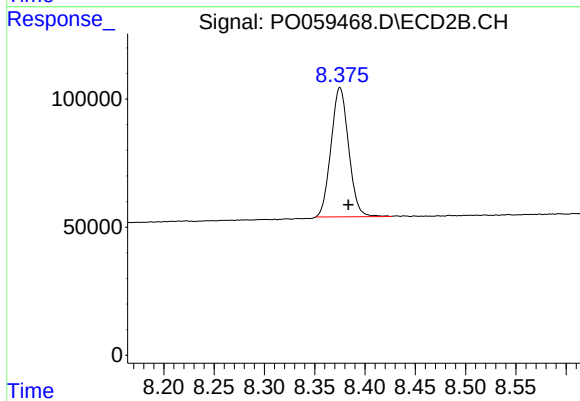

#2 Decachlorobiphenyl

R.T.: 8.375 min
Delta R.T.: -0.008 min
Response: 615849
Conc: 15.27 ng/ml

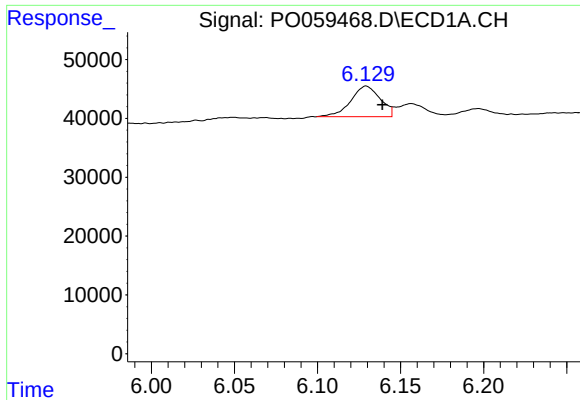


#26 AR-1254-1

R.T.: 6.129 min
Delta R.T.: -0.010 min
Response: 63881
Conc: 30.62 ng/ml m

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019


Manual Integrations
APPROVED

Ankita
8/21/2019 12:58:17 PM

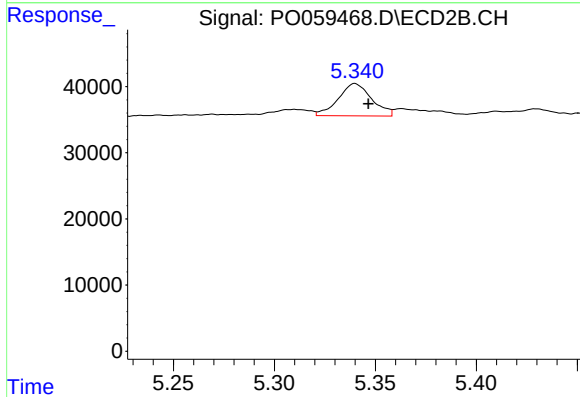


#26 AR-1254-1

R.T.: 5.340 min
Delta R.T.: -0.007 min
Response: 56709
Conc: 23.91 ng/ml m

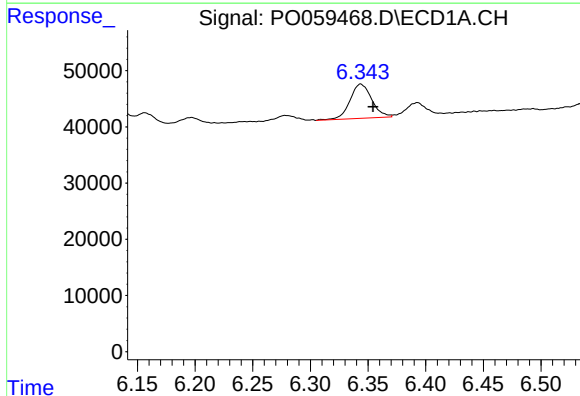


#27 AR-1254-2

R.T.: 6.344 min
Delta R.T.: -0.011 min
Response: 79960
Conc: 23.97 ng/ml

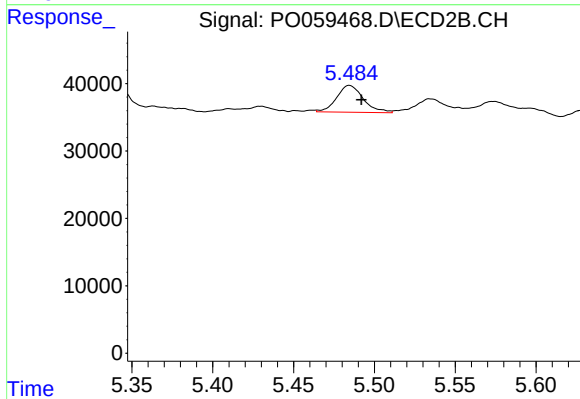

#27 AR-1254-2

R.T.: 5.484 min
Delta R.T.: -0.008 min
Response: 45771
Conc: 21.81 ng/ml m

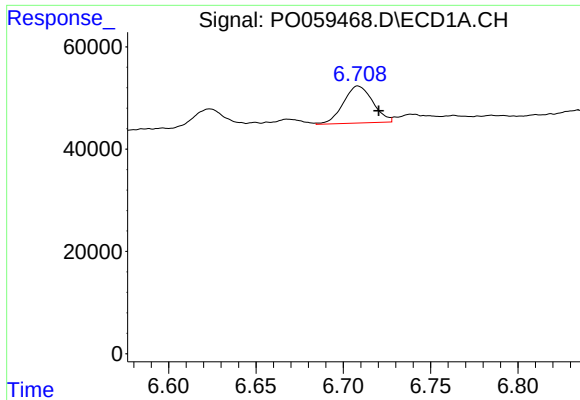


#28 AR-1254-3

R.T.: 6.709 min
Delta R.T.: -0.012 min
Response: 84805
Conc: 23.90 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019


Manual Integrations
APPROVED

Ankita
8/21/2019 12:58:17 PM

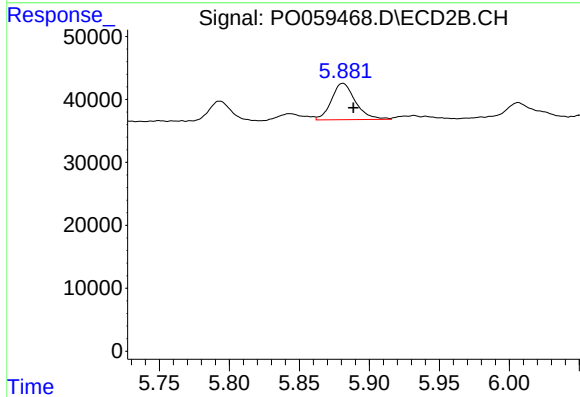


#28 AR-1254-3

R.T.: 5.881 min
Delta R.T.: -0.008 min
Response: 69316
Conc: 20.61 ng/ml m

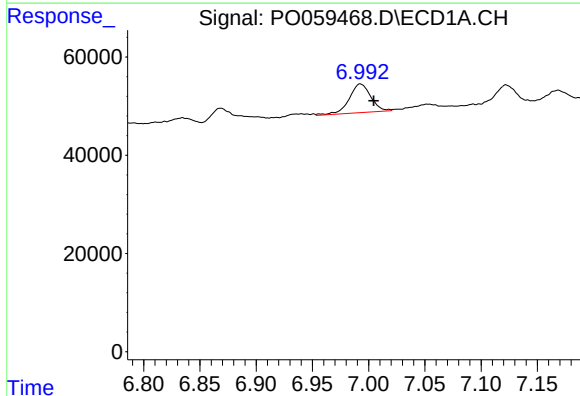


#29 AR-1254-4

R.T.: 6.993 min
Delta R.T.: -0.012 min
Response: 77725
Conc: 26.39 ng/ml

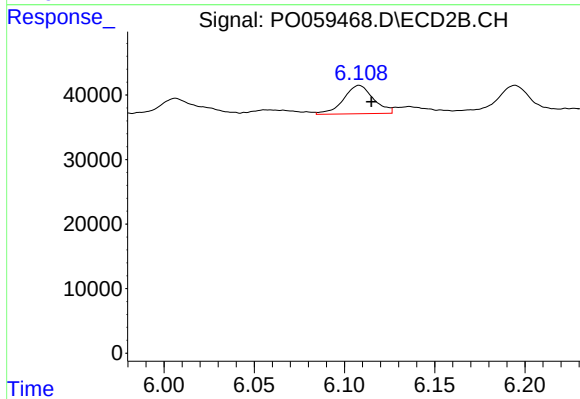

#29 AR-1254-4

R.T.: 6.108 min
Delta R.T.: -0.007 min
Response: 50891
Conc: 24.68 ng/ml

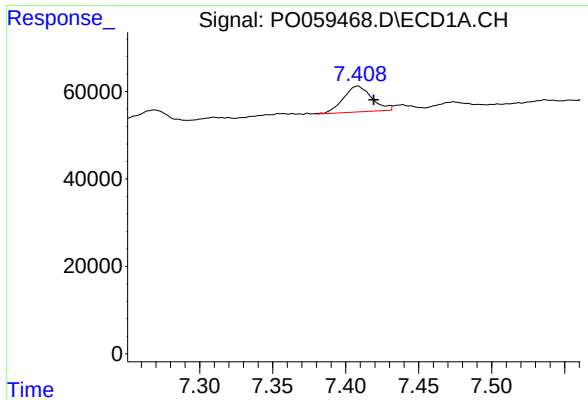


#30 AR-1254-5

R.T.: 7.408 min
Delta R.T.: -0.011 min
Response: 80461
Conc: 26.02 ng/ml m

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

Manual Integrations
APPROVED

Ankita
8/21/2019 12:58:17 PM

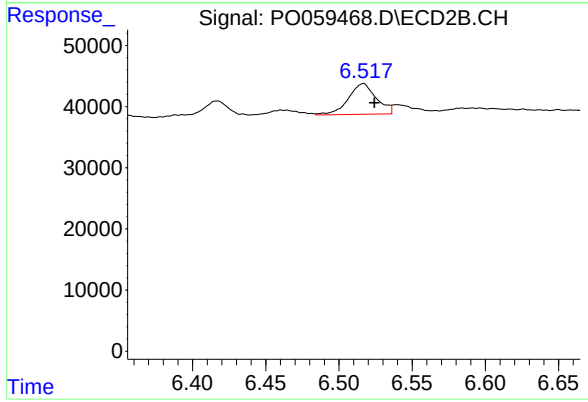

#30 AR-1254-5

R.T.: 6.517 min
Delta R.T.: -0.008 min
Response: 66883
Conc: 21.54 ng/ml