

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0081919\
 Data File : P0059470.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Aug 2019 20:15
 Operator : SM/AJ
 Sample : K3591-09
 Misc : AR1268 MDL 25PPB
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-MDL-WATER-03-QT3-2019

Manual Integrations
 APPROVED

Ankita
 8/21/2019 12:58:20 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 20 01:10:48 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0081719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 17 03:09:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.140	3.505	444657	428146	12.700	11.894
2) SA Decachlor...	9.626	8.376	884532	666804	16.626	16.537
Target Compounds						
41) L9 AR-1268-1	8.293	7.324	228584	162866	24.290	22.871m
42) L9 AR-1268-2	8.380	7.390	181849	174274	23.069	27.028m
43) L9 AR-1268-3	8.579	7.585	171482	126276	24.328	23.078m
44) L9 AR-1268-4	8.973	7.882	65769	53375	23.657m	26.148
45) L9 AR-1268-5	9.337	8.149	383784	306247	20.810m	21.078

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO081919\
Data File : PO059470.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Aug 2019 20:15
Operator : SM/AJ
Sample : K3591-09
Misc : AR1268 MDL 25PPB
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019


Manual Integrations
APPROVED

Ankita
8/21/2019 12:58:20 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 20 01:10:48 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Aug 17 03:09:44 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

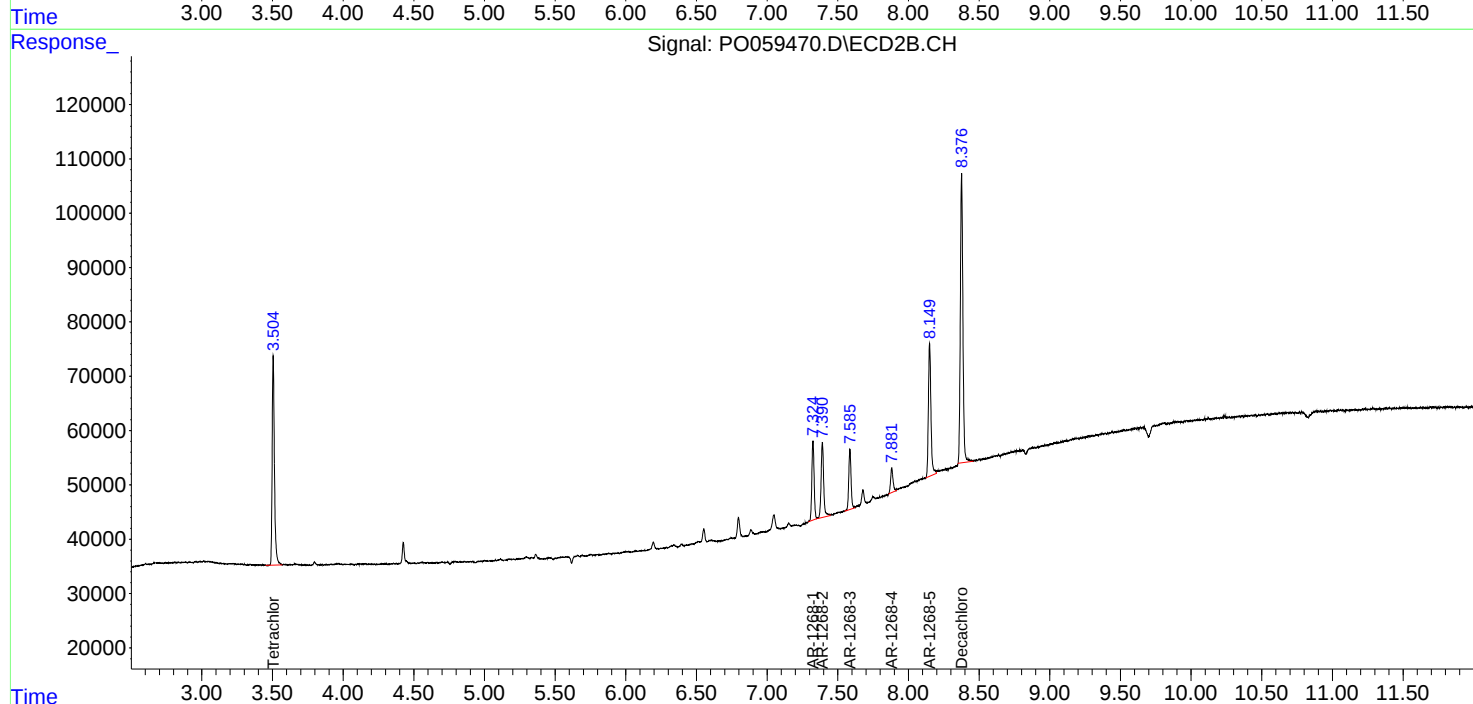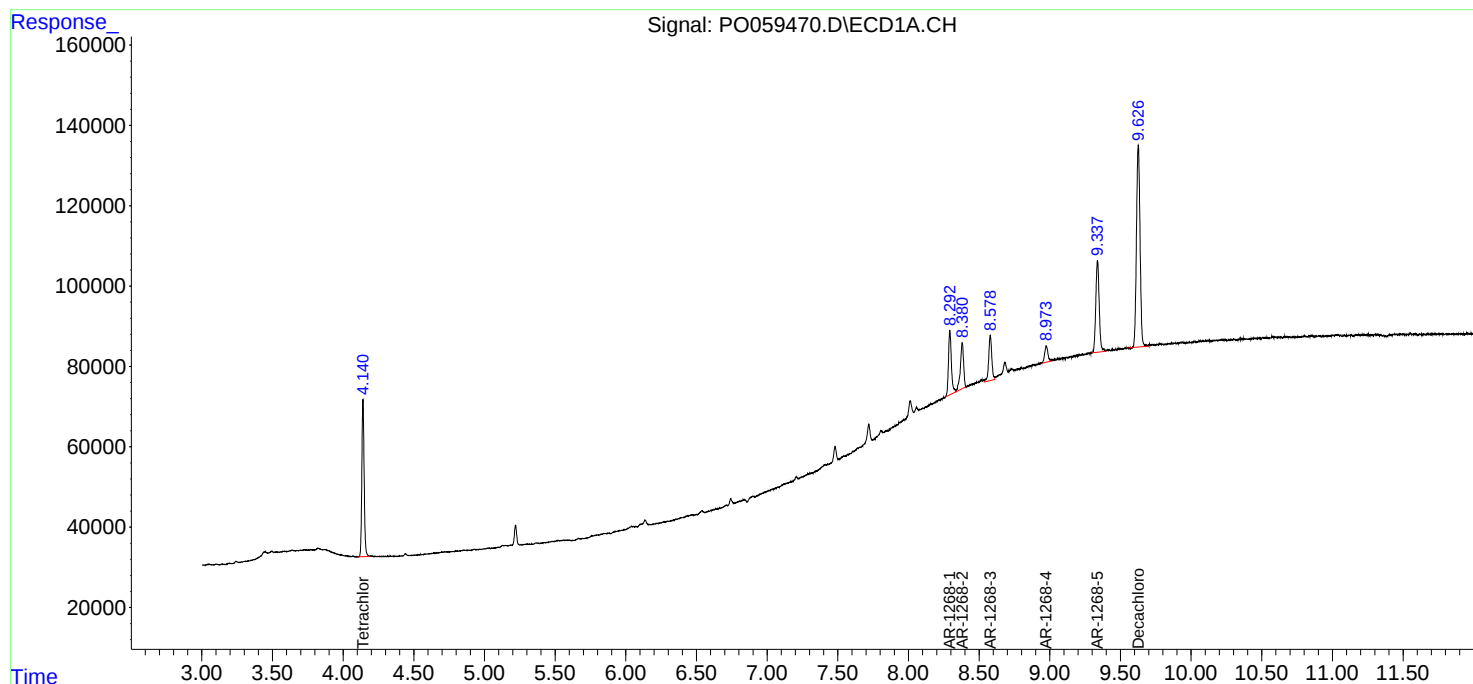

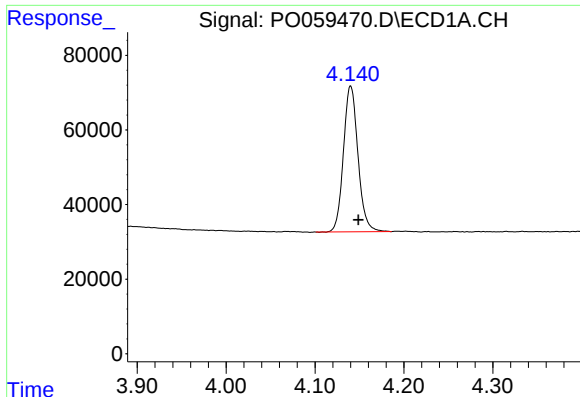


#1 Tetrachloro-m-xylene

R.T.: 4.140 min
Delta R.T.: -0.009 min
Response: 444657
Conc: 12.70 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019


Manual Integrations
APPROVED

Ankita
8/21/2019 12:58:20 PM

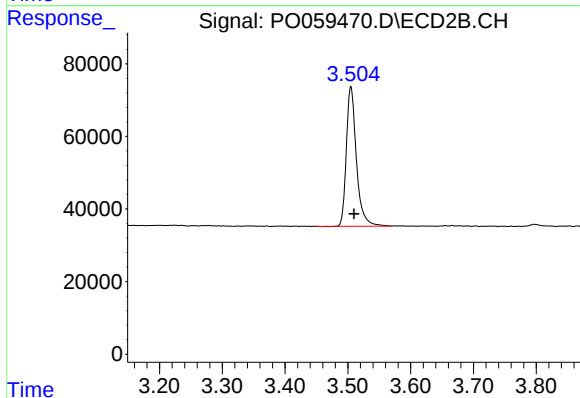


#1 Tetrachloro-m-xylene

R.T.: 3.505 min
Delta R.T.: -0.005 min
Response: 428146
Conc: 11.89 ng/ml

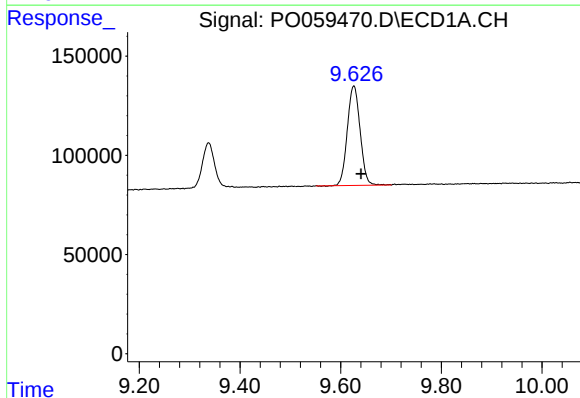


#2 Decachlorobiphenyl

R.T.: 9.626 min
Delta R.T.: -0.015 min
Response: 884532
Conc: 16.63 ng/ml

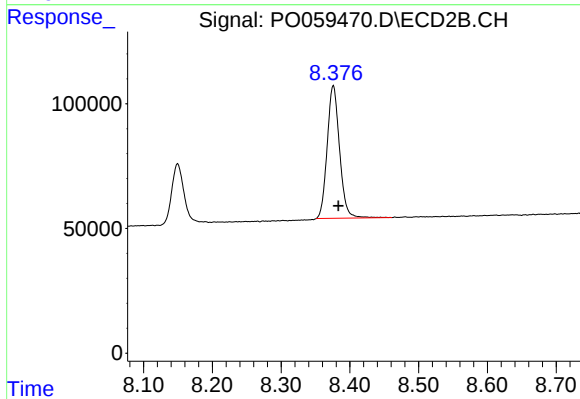

#2 Decachlorobiphenyl

R.T.: 8.376 min
Delta R.T.: -0.007 min
Response: 666804
Conc: 16.54 ng/ml

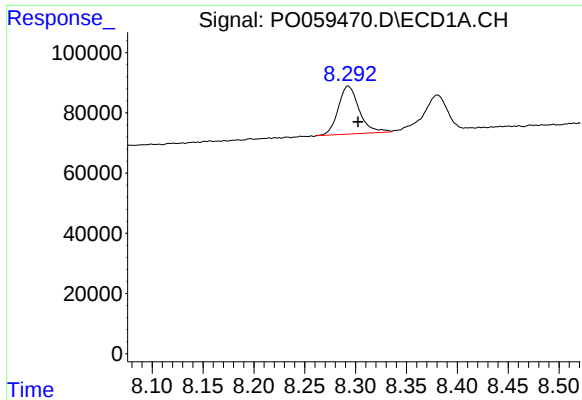


#41 AR-1268-1

R.T.: 8.293 min
Delta R.T.: -0.010 min
Response: 228584
Conc: 24.29 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019


Manual Integrations
APPROVED

Ankita
8/21/2019 12:58:20 PM

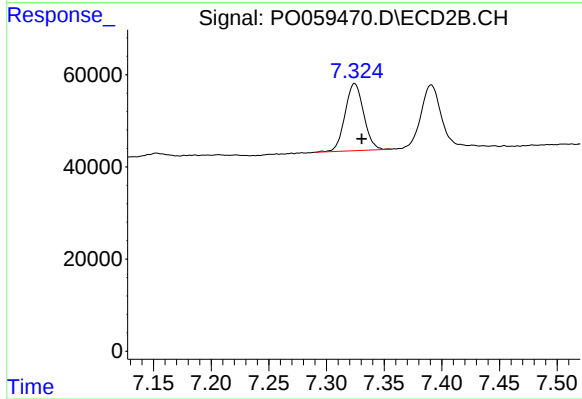


#41 AR-1268-1

R.T.: 7.324 min
Delta R.T.: -0.007 min
Response: 162866
Conc: 22.87 ng/ml m

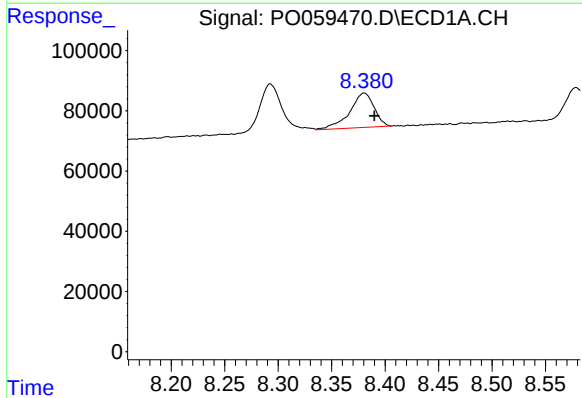


#42 AR-1268-2

R.T.: 8.380 min
Delta R.T.: -0.010 min
Response: 181849
Conc: 23.07 ng/ml

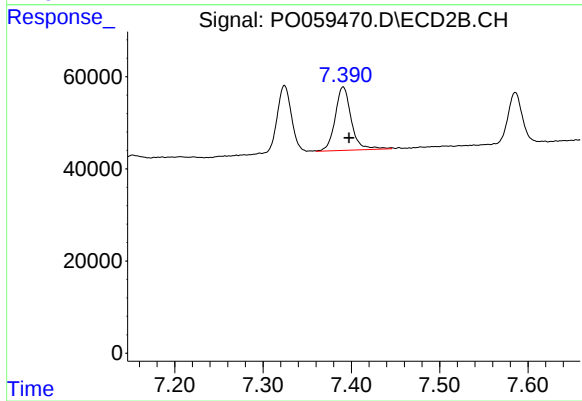

#42 AR-1268-2

R.T.: 7.390 min
Delta R.T.: -0.007 min
Response: 174274
Conc: 27.03 ng/ml m

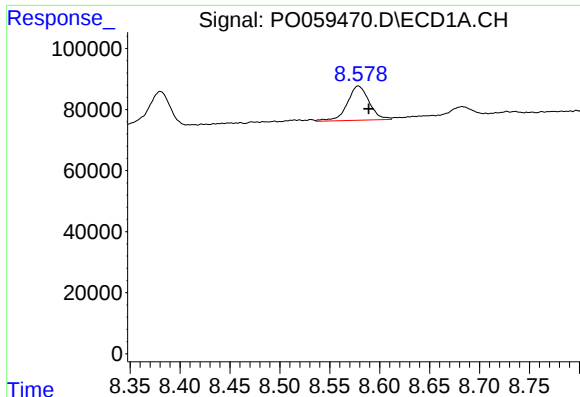


#43 AR-1268-3

R.T.: 8.579 min
Delta R.T.: -0.010 min
Response: 171482
Conc: 24.33 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019


Manual Integrations
APPROVED

Ankita
8/21/2019 12:58:20 PM

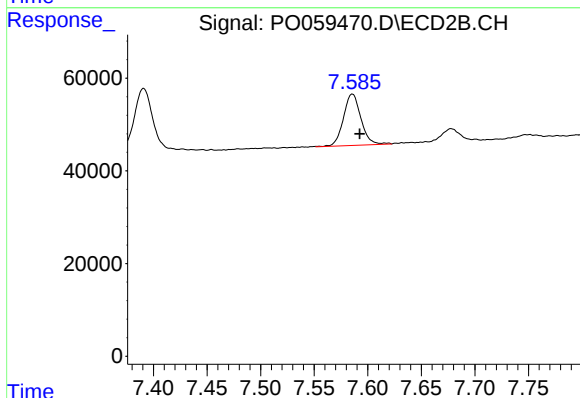


#43 AR-1268-3

R.T.: 7.585 min
Delta R.T.: -0.007 min
Response: 126276
Conc: 23.08 ng/ml m

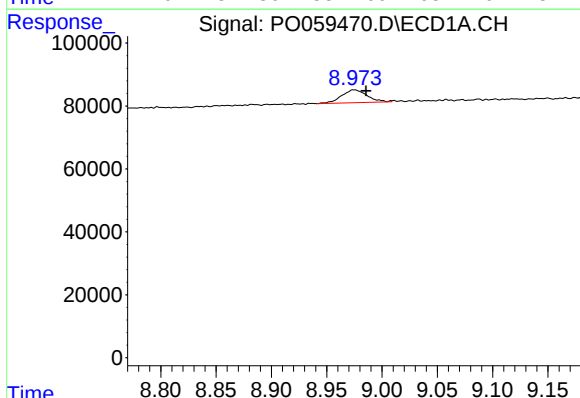


#44 AR-1268-4

R.T.: 8.973 min
Delta R.T.: -0.012 min
Response: 65769
Conc: 23.66 ng/ml m

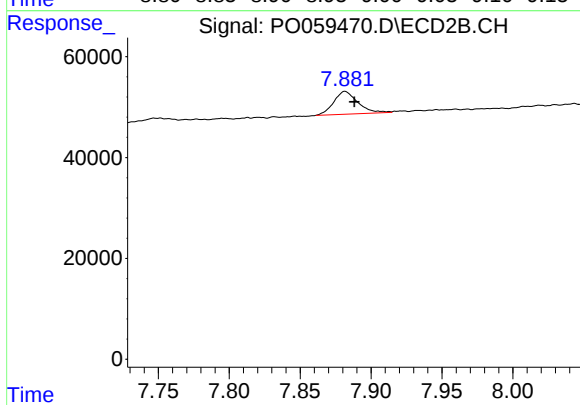

#44 AR-1268-4

R.T.: 7.882 min
Delta R.T.: -0.007 min
Response: 53375
Conc: 26.15 ng/ml

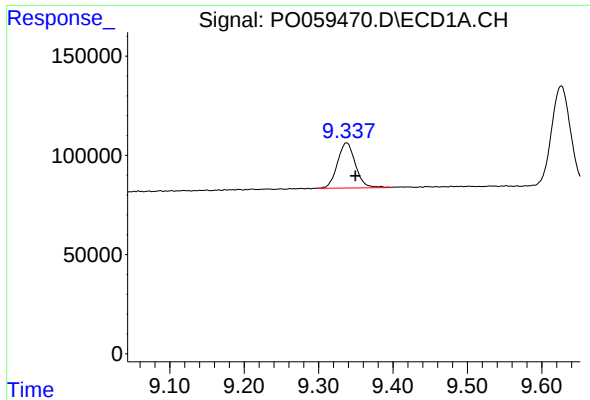


#45 AR-1268-5

R.T.: 9.337 min
Delta R.T.: -0.013 min
Response: 383784
Conc: 20.81 ng/ml m

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

Manual Integrations
APPROVED

Ankita
8/21/2019 12:58:20 PM

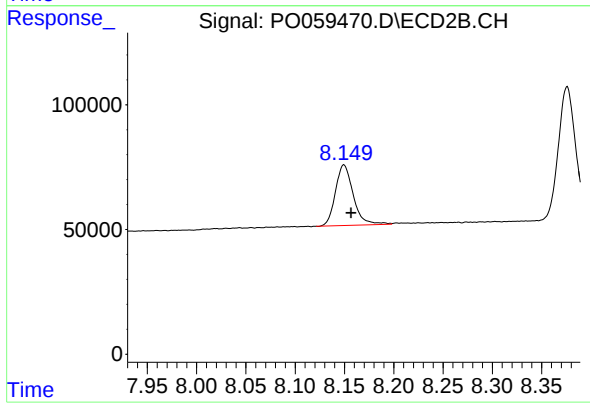

#45 AR-1268-5

R.T.: 8.149 min
Delta R.T.: -0.007 min
Response: 306247
Conc: 21.08 ng/ml