

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081919\
 Data File : P0059483.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Aug 2019 23:50
 Operator : SM/AJ
 Sample : K4400-03 5X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 HA-15

Manual Integrations
 APPROVED

Ankita
 8/21/2019 12:58:36 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 20 01:20:28 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 17 03:09:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.137	3.504	205418	195600	5.867	5.434
2)	SA Decachlor...	9.623	8.375	306025	231561	5.752	5.743
Target Compounds							
26)	L6 AR-1254-1	6.129	5.339	120221	70954	57.621m	29.916m#
27)	L6 AR-1254-2	6.344	5.484	129093	56041	38.694	26.708m#
28)	L6 AR-1254-3	6.709	5.880	137233	113460	38.674m	33.743m
29)	L6 AR-1254-4	6.994	6.107	148576	75036	50.441	36.393m#
30)	L6 AR-1254-5	7.408	6.516	144920	136803	46.863	44.059

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081919\
Data File : PO059483.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Aug 2019 23:50
Operator : SM/AJ
Sample : K4400-03 5X
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
HA-15


Manual Integrations
APPROVED

Ankita
8/21/2019 12:58:36 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 20 01:20:28 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Aug 17 03:09:44 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

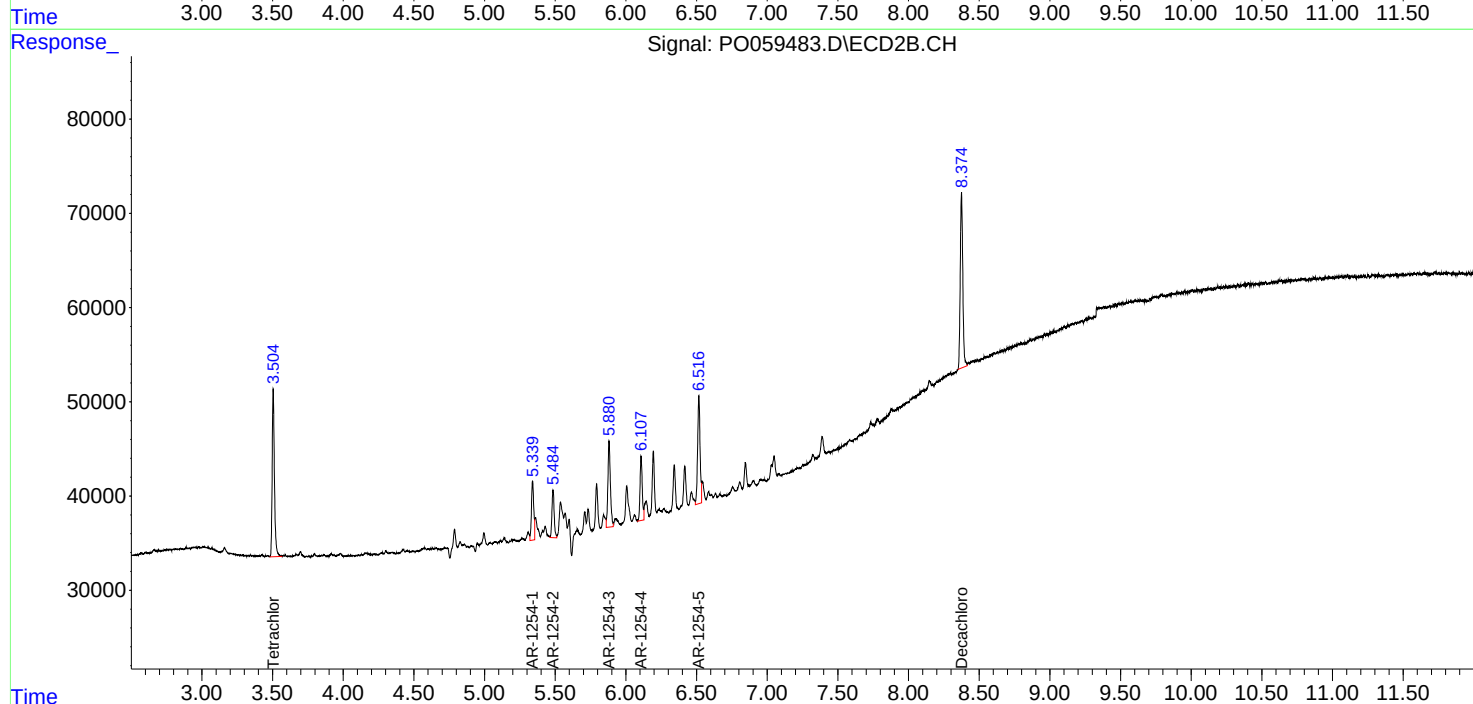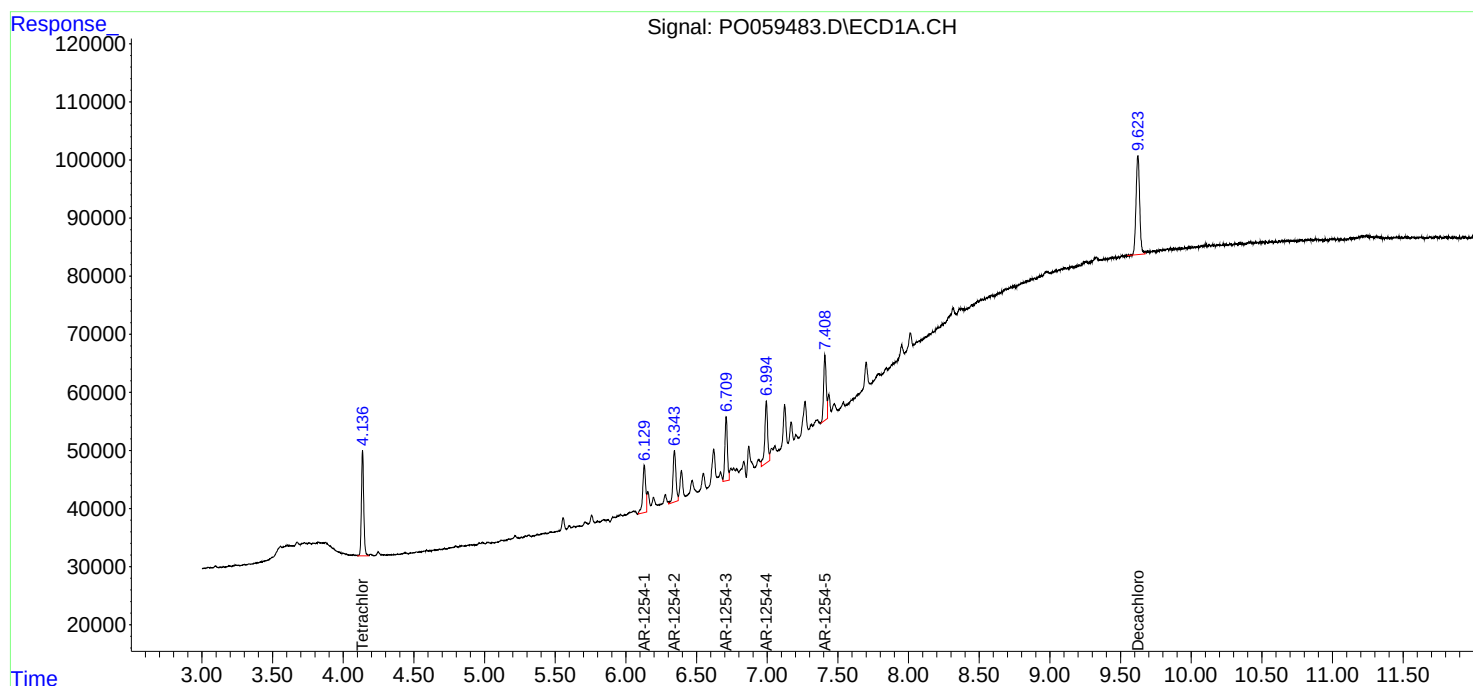

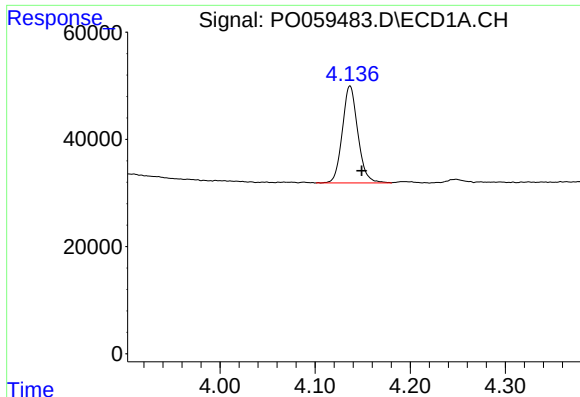


#1 Tetrachloro-m-xylene

R.T.: 4.137 min
Delta R.T.: -0.012 min
Response: 205418
Conc: 5.87 ng/ml

Instrument :
ECD_O
ClientSampleId :
HA-15


Manual Integrations
APPROVED

Ankita
8/21/2019 12:58:36 PM

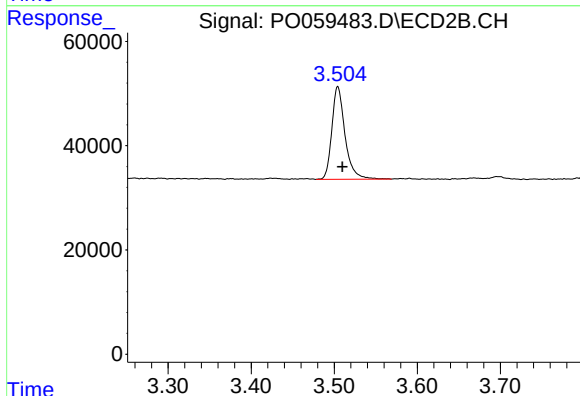


#1 Tetrachloro-m-xylene

R.T.: 3.504 min
Delta R.T.: -0.006 min
Response: 195600
Conc: 5.43 ng/ml

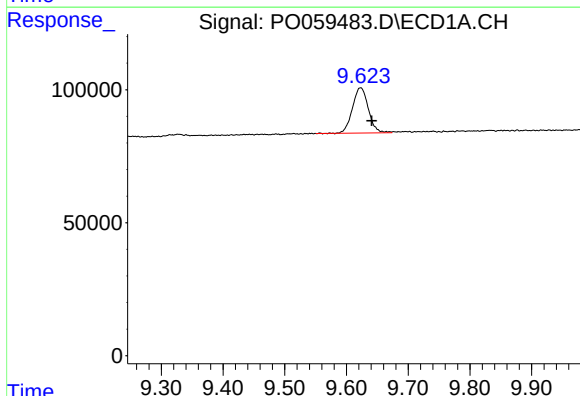


#2 Decachlorobiphenyl

R.T.: 9.623 min
Delta R.T.: -0.018 min
Response: 306025
Conc: 5.75 ng/ml

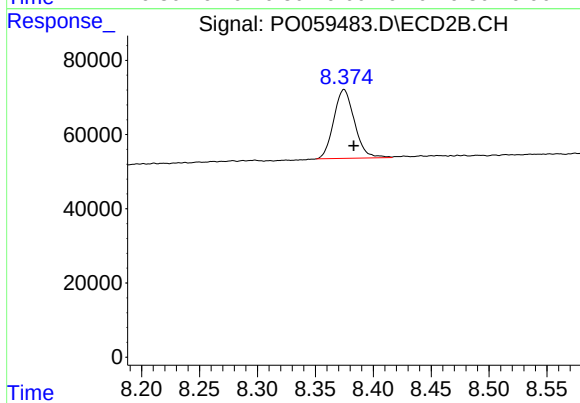

#2 Decachlorobiphenyl

R.T.: 8.375 min
Delta R.T.: -0.009 min
Response: 231561
Conc: 5.74 ng/ml

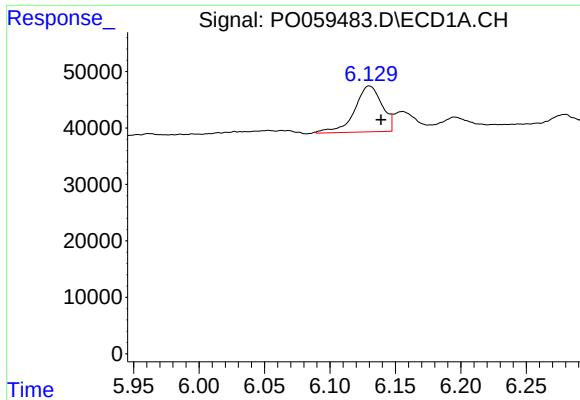


#26 AR-1254-1

R.T.: 6.129 min
Delta R.T.: -0.010 min
Response: 120221
Conc: 57.62 ng/ml m

Instrument :
ECD_O
ClientSampleId :
HA-15


Manual Integrations
APPROVED

Ankita
8/21/2019 12:58:36 PM

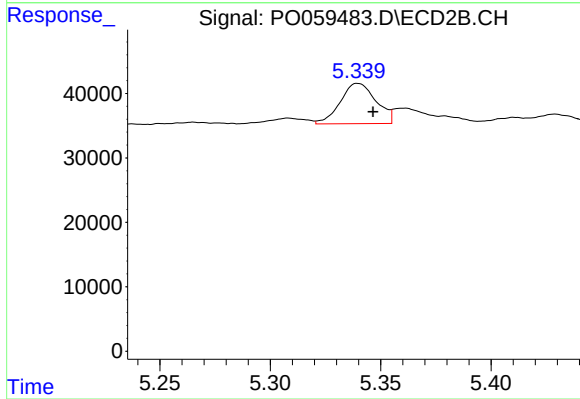


#26 AR-1254-1

R.T.: 5.339 min
Delta R.T.: -0.008 min
Response: 70954
Conc: 29.92 ng/ml m

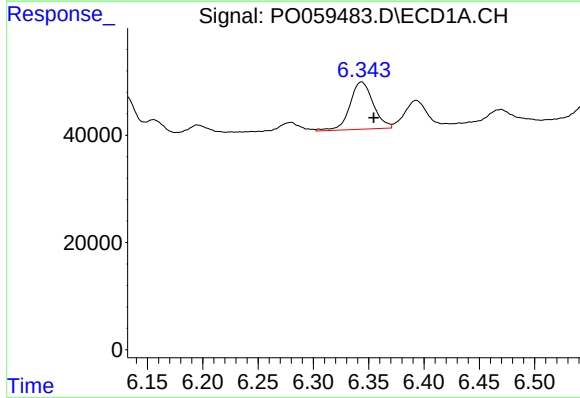


#27 AR-1254-2

R.T.: 6.344 min
Delta R.T.: -0.011 min
Response: 129093
Conc: 38.69 ng/ml

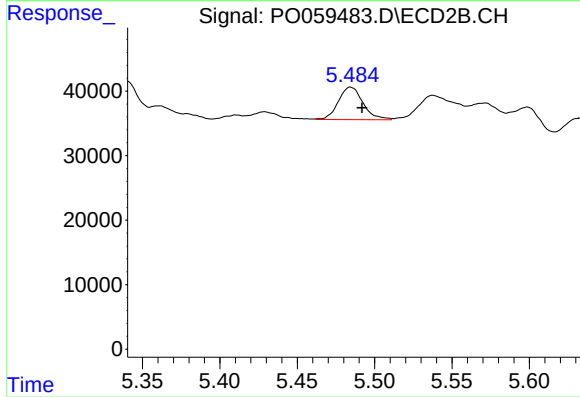

#27 AR-1254-2

R.T.: 5.484 min
Delta R.T.: -0.008 min
Response: 56041
Conc: 26.71 ng/ml m

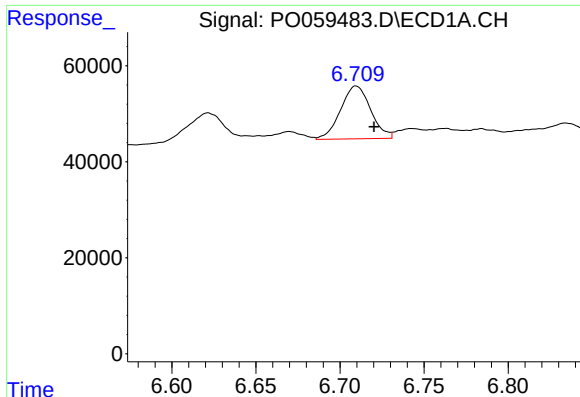


#28 AR-1254-3

R.T.: 6.709 min
Delta R.T.: -0.011 min
Response: 137233
Conc: 38.67 ng/ml m

Instrument :
ECD_O
ClientSampleId :
HA-15


Manual Integrations
APPROVED

Ankita
8/21/2019 12:58:36 PM

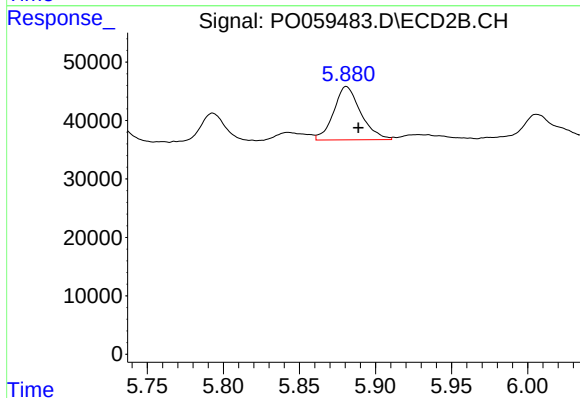


#28 AR-1254-3

R.T.: 5.880 min
Delta R.T.: -0.008 min
Response: 113460
Conc: 33.74 ng/ml m

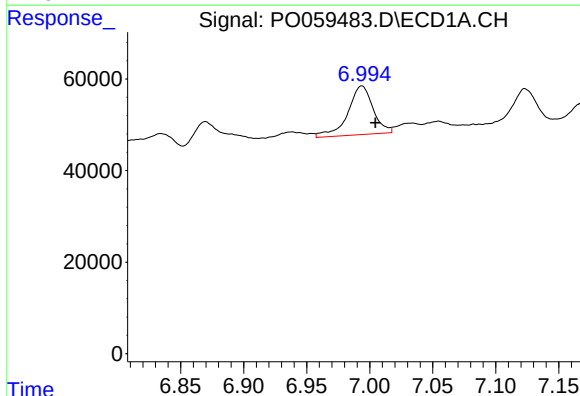


#29 AR-1254-4

R.T.: 6.994 min
Delta R.T.: -0.011 min
Response: 148576
Conc: 50.44 ng/ml

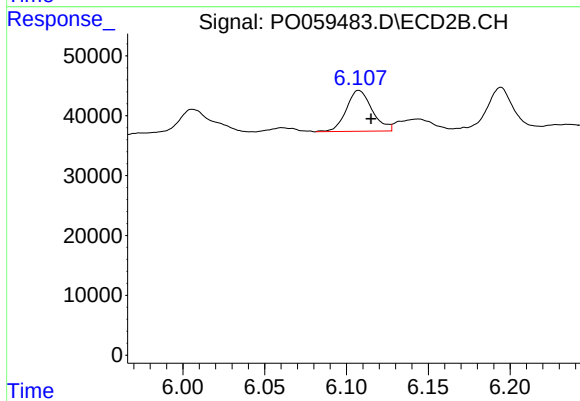

#29 AR-1254-4

R.T.: 6.107 min
Delta R.T.: -0.008 min
Response: 75036
Conc: 36.39 ng/ml m

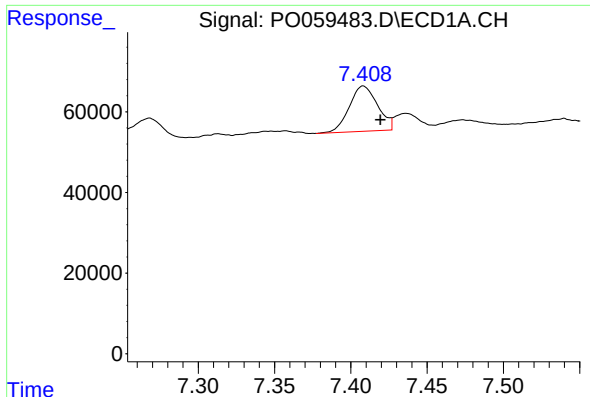


#30 AR-1254-5

R.T.: 7.408 min
Delta R.T.: -0.011 min
Response: 144920
Conc: 46.86 ng/ml

Instrument :
ECD_O
ClientSampleId :
HA-15

Manual Integrations
APPROVED

Ankita
8/21/2019 12:58:36 PM

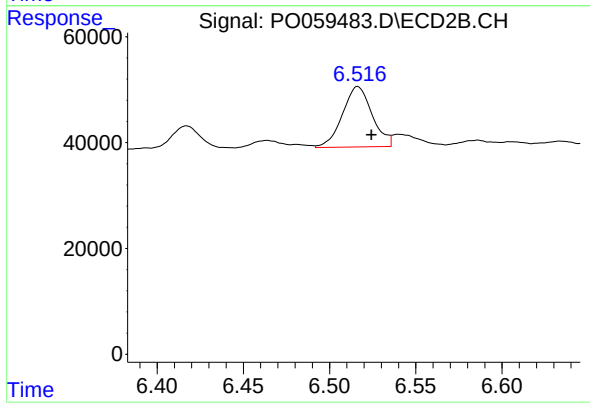

#30 AR-1254-5

R.T.: 6.516 min
Delta R.T.: -0.008 min
Response: 136803
Conc: 44.06 ng/ml