

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081919\
 Data File : P0059488.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Aug 2019 1:11
 Operator : SM/AJ
 Sample : K4380-01
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 STOCKPILE-175-LANDERS-PIT

Manual Integrations
 APPROVED

Ankita
 8/21/2019 12:58:50 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 20 05:25:10 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 17 03:09:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.135	3.504	828091	792129	23.651	22.006
2) SA Decachlor...	9.620	8.373	1252384	955675	23.541	23.702m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081919\
Data File : P0059488.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Aug 2019 1:11
Operator : SM/AJ
Sample : K4380-01
Misc :
ALS Vial : 27 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
STOCKPILE-175-LANDERS-PIT


Manual Integrations
APPROVED

Ankita
8/21/2019 12:58:50 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 20 05:25:10 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Aug 17 03:09:44 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

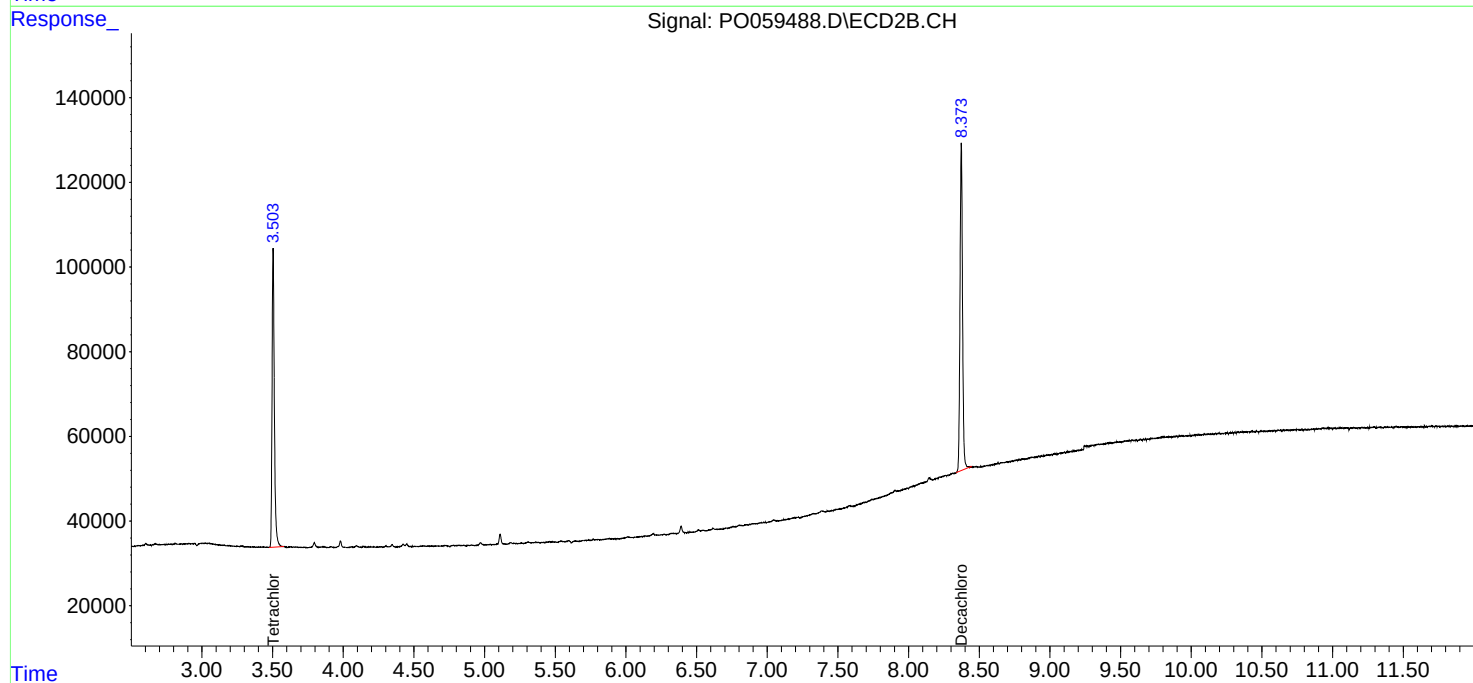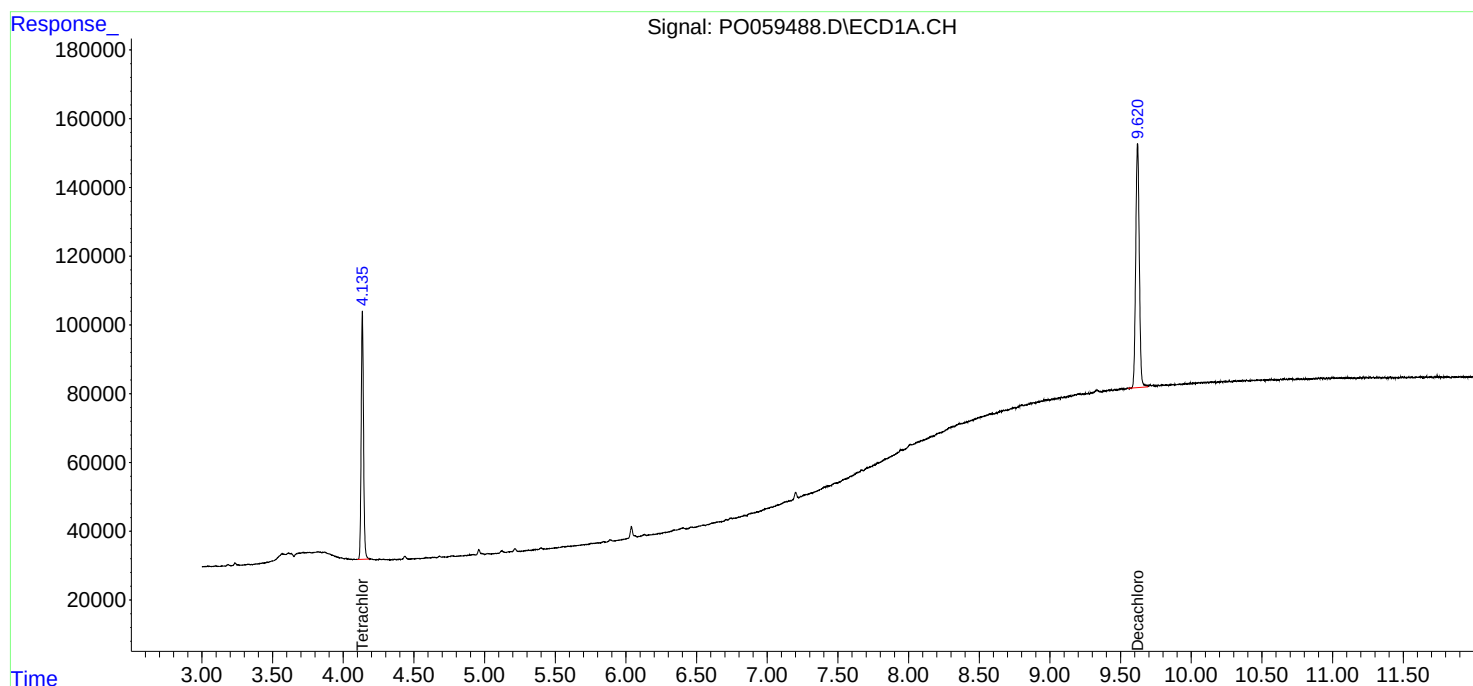

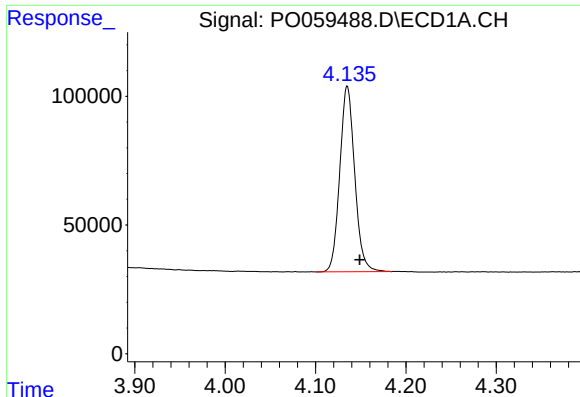


#1 Tetrachloro-m-xylene

R.T.: 4.135 min
Delta R.T.: -0.014 min
Response: 828091
Conc: 23.65 ng/ml

Instrument :
ECD_O
ClientSampleId :
STOCKPILE-175-LANDERS-PIT


Manual Integrations
APPROVED

Ankita
8/21/2019 12:58:50 PM

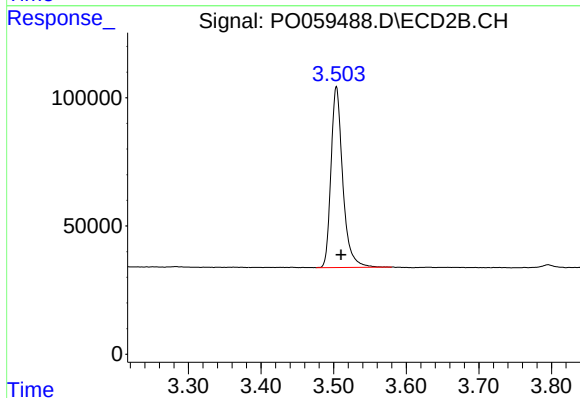


#1 Tetrachloro-m-xylene

R.T.: 3.504 min
Delta R.T.: -0.006 min
Response: 792129
Conc: 22.01 ng/ml

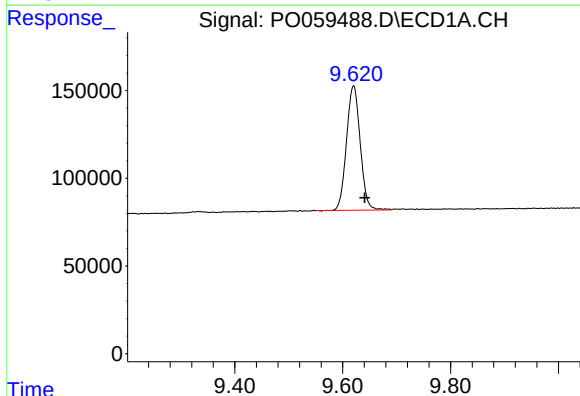

#2 Decachlorobiphenyl

R.T.: 9.620 min
Delta R.T.: -0.020 min
Response: 1252384
Conc: 23.54 ng/ml

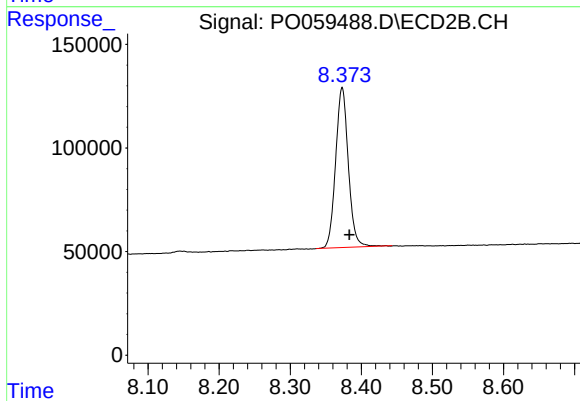

#2 Decachlorobiphenyl

R.T.: 8.373 min
Delta R.T.: -0.011 min
Response: 955675
Conc: 23.70 ng/ml m