

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081924\
 Data File : P0105652.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Aug 2024 17:25
 Operator : YP/AJ
 Sample : P3655-05
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 T-23

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/20/2024
 Supervised By :Ankita Jodhani 08/20/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 20 06:31:29 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Aug 15 11:44:23 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.454	3.725	223.0E6	60481356	23.854m	23.713
2) SA Decachlor...	10.204	8.770	132.2E6	49579056	22.777	25.123

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081924\
Data File : PO105652.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Aug 2024 17:25
Operator : YP/AJ
Sample : P3655-05
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
T-23


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/20/2024
Supervised By :Ankita Jodhani 08/20/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 20 06:31:29 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081524.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Aug 15 11:44:23 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

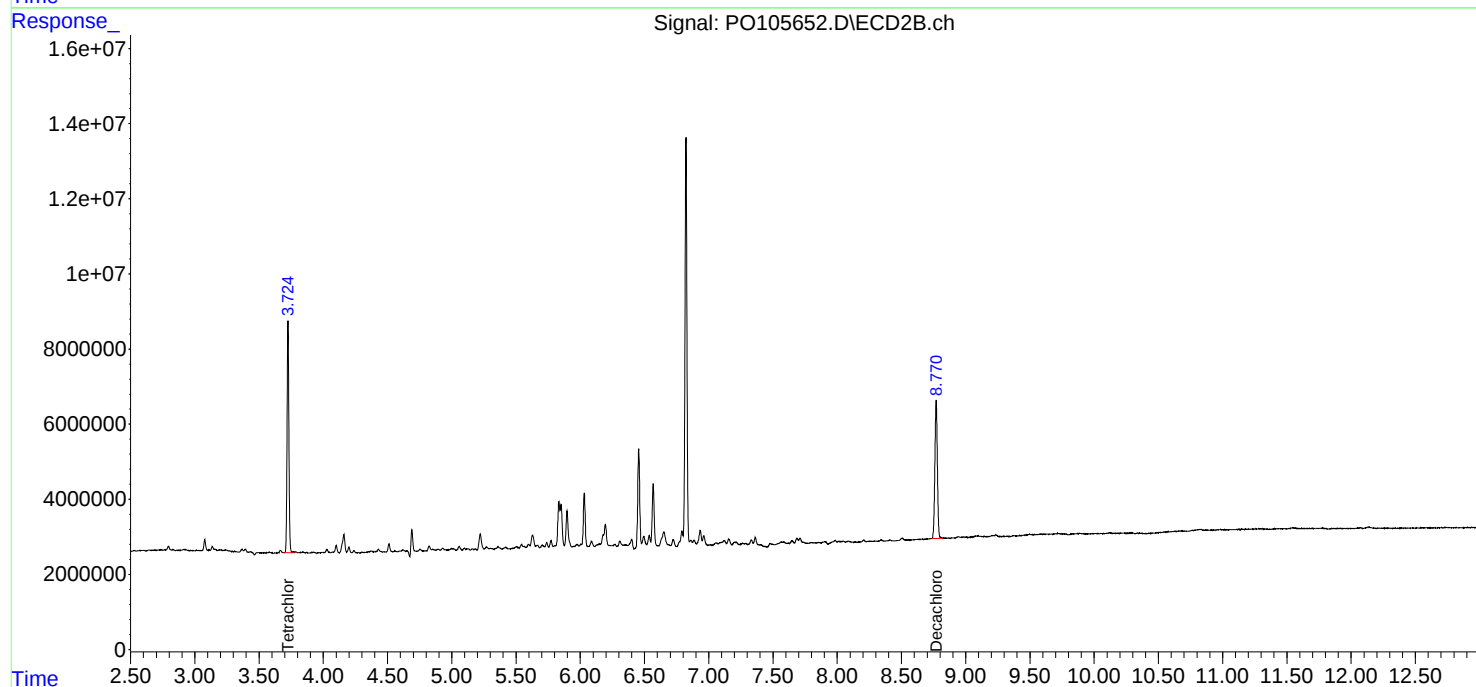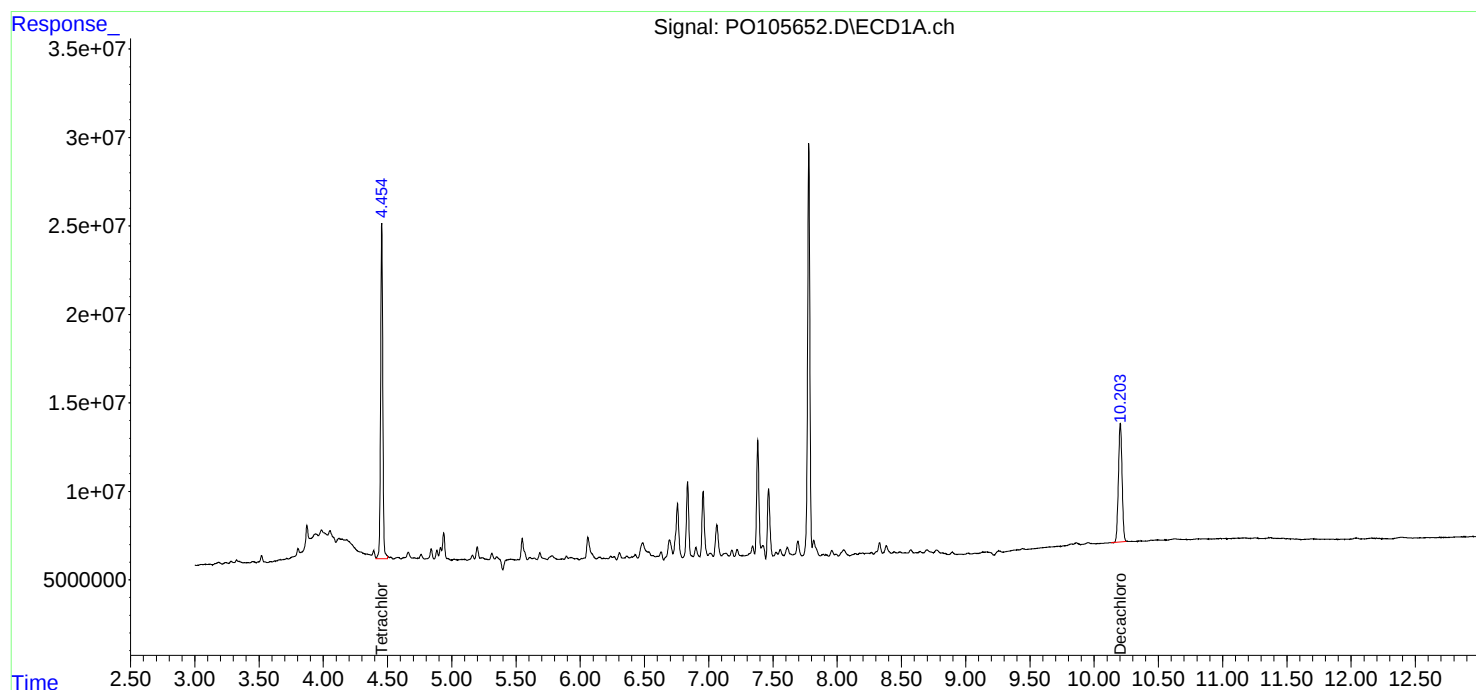

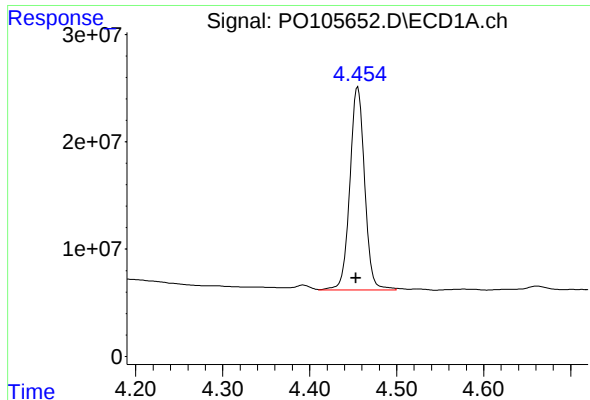


#1 Tetrachloro-m-xylene

R.T.: 4.454 min
Delta R.T.: 0.001 min
Response: 223011308
Conc: 23.85 ng/ml

Instrument :
ECD_O
ClientSampleId :
T-23


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/20/2024
Supervised By :Ankita Jodhani 08/20/2024

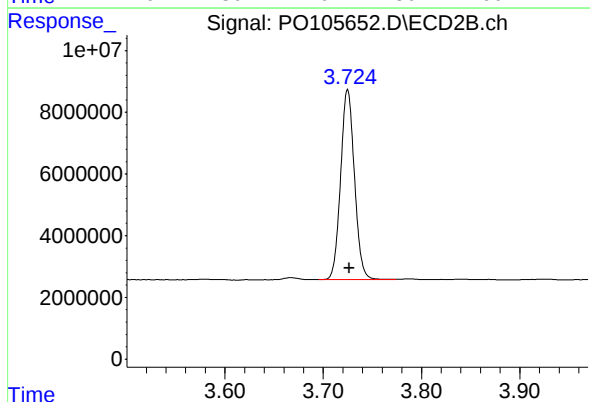


#1 Tetrachloro-m-xylene

R.T.: 3.725 min
Delta R.T.: -0.002 min
Response: 60481356
Conc: 23.71 ng/ml

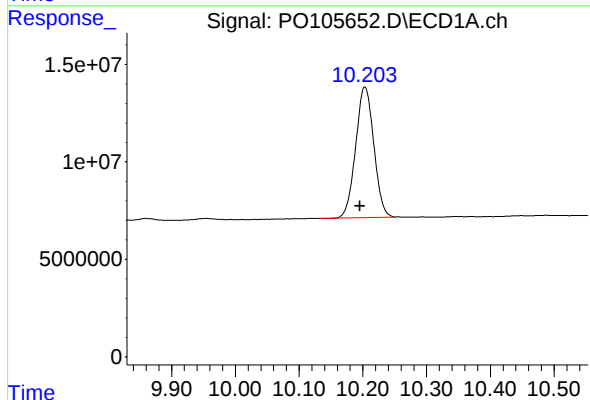

#2 Decachlorobiphenyl

R.T.: 10.204 min
Delta R.T.: 0.008 min
Response: 132214695
Conc: 22.78 ng/ml

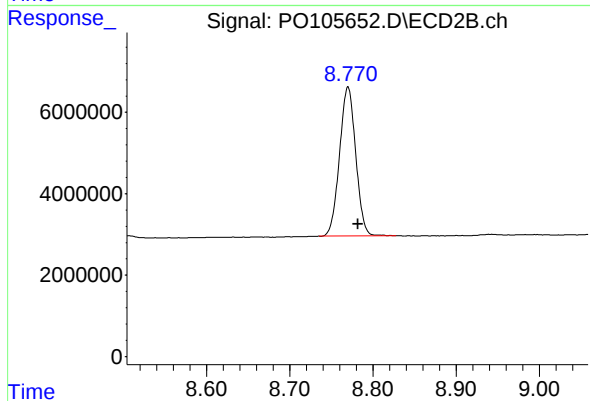

#2 Decachlorobiphenyl

R.T.: 8.770 min
Delta R.T.: -0.012 min
Response: 49579056
Conc: 25.12 ng/ml