

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082019\
 Data File : P0059522.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Aug 2019 11:26
 Operator : SM/AJ
 Sample : K3591-09
 Misc : AR1242 MDL 25 PPB
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-MDL-WATER-03-QT3-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 20 14:45:51 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 17 03:09:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.140	3.505	649274	583535	18.544	16.211
2)	SA Decachlor...	9.622	8.373	789013	593295	14.831	14.714
Target Compounds							
3)	L1 AR-1016-1	5.292	4.557	35257	25835	21.983	19.110
4)	L1 AR-1016-2	5.312	4.574	50985	40503	21.310	20.221
5)	L1 AR-1016-3	5.373	4.746	33174	20072	22.272	18.553
6)	L1 AR-1016-4	5.471	4.788	21297	16048	17.604	17.772
7)	L1 AR-1016-5	5.759	4.995	22733	20468	17.703	17.768
8)	L2 AR-1221-1	4.344	0.000	3800	0	8.974	N.D. #
9)	L2 AR-1221-2	4.438	3.796	13086	10306	40.289	33.831
10)	L2 AR-1221-3	4.512	3.867	17415	12097	16.557	12.363 #
11)	L3 AR-1232-1	4.512	3.867	17415	12097	13.972	10.610
12)	L3 AR-1232-2	5.027	4.574	25070	40503	35.490	31.802
13)	L3 AR-1232-3	5.312	4.746	50985	20072	33.294	29.478
14)	L3 AR-1232-4	5.471	4.826	21297	18753	27.238	30.740
15)	L3 AR-1232-5	5.558	4.995	21680	20468	36.065	30.067
16)	L4 AR-1242-1	5.292	4.557	35257	25835	27.772	25.115
17)	L4 AR-1242-2	5.312	4.574	50985	40503	27.475	26.593
18)	L4 AR-1242-3	5.373	4.746	33174	20072	28.382	24.024
19)	L4 AR-1242-4	5.471	4.826	21297	18753	22.004	22.475
20)	L4 AR-1242-5	6.194	5.340	29737	22089	23.664	19.747
21)	L5 AR-1248-1	5.292	4.557	35257	25835	35.168	31.201
22)	L5 AR-1248-2	5.558	4.788	21680	16048	14.942	13.917
23)	L5 AR-1248-3	5.759	4.826	22733	18753	13.678	15.789
24)	L5 AR-1248-4	6.160	4.995	29344	20468	14.356	14.086
25)	L5 AR-1248-5	6.194	5.380	29737	16522	14.995	11.544
26)	L6 AR-1254-1	6.129	5.340	26944	22089	12.914	9.313 #
27)	L6 AR-1254-2	6.354	5.485	27552	5242	8.258	2.498 #
28)	L6 AR-1254-3	6.710	5.882	9997	10189	2.817	3.030
29)	L6 AR-1254-4	6.994	6.107	8156	5753	2.769	2.790
30)	L6 AR-1254-5	0.000	6.517	0	9059	N.D.	2.918 #
31)	L7 AR-1260-1	6.838	6.006	7720	3511	2.864	1.541 #
32)	L7 AR-1260-2	7.126	6.197	5931	11800	1.598	4.027 #
33)	L7 AR-1260-3	7.490	6.340	61838	1130	18.874	0.426 #
34)	L7 AR-1260-4	0.000	6.815	0	2972	N.D.	1.314 #
35)	L7 AR-1260-5	8.018	7.046	632947	7557	89.388	1.373 #
36)	L8 AR-1262-1	7.490	6.575	61838	3505	12.742	0.940 #
37)	L8 AR-1262-2	8.018	7.046	632947	7557	82.032	1.285 #
38)	L8 AR-1262-3	8.307	7.335	880600	4365	172.589	1.718 #
39)	L8 AR-1262-4	8.390	7.394	91823	6821	23.821	1.544 #
40)	L8 AR-1262-5	8.986	0.000	35302	0	13.755	N.D. #
41)	L9 AR-1268-1	8.307	7.335	880600	4365	93.575	0.613 #
42)	L9 AR-1268-2	8.390	7.394	91823	6821	11.649	1.058 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082019\
 Data File : P0059522.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Aug 2019 11:26
 Operator : SM/AJ
 Sample : K3591-09
 Misc : AR1242 MDL 25 PPB
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-MDL-WATER-03-QT3-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 20 14:45:51 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 17 03:09:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
43) L9	AR-1268-3	8.645	7.588	444085	3874	63.001	0.708 #
44) L9	AR-1268-4	8.986	0.000	35302	0	12.699	N.D. #
45) L9	AR-1268-5	9.344	8.151	31541	7349	1.710	0.506 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO082019\
Data File : PO059522.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Aug 2019 11:26
Operator : SM/AJ
Sample : K3591-09
Misc : AR1242 MDL 25 PPB
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 20 14:45:51 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Aug 17 03:09:44 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

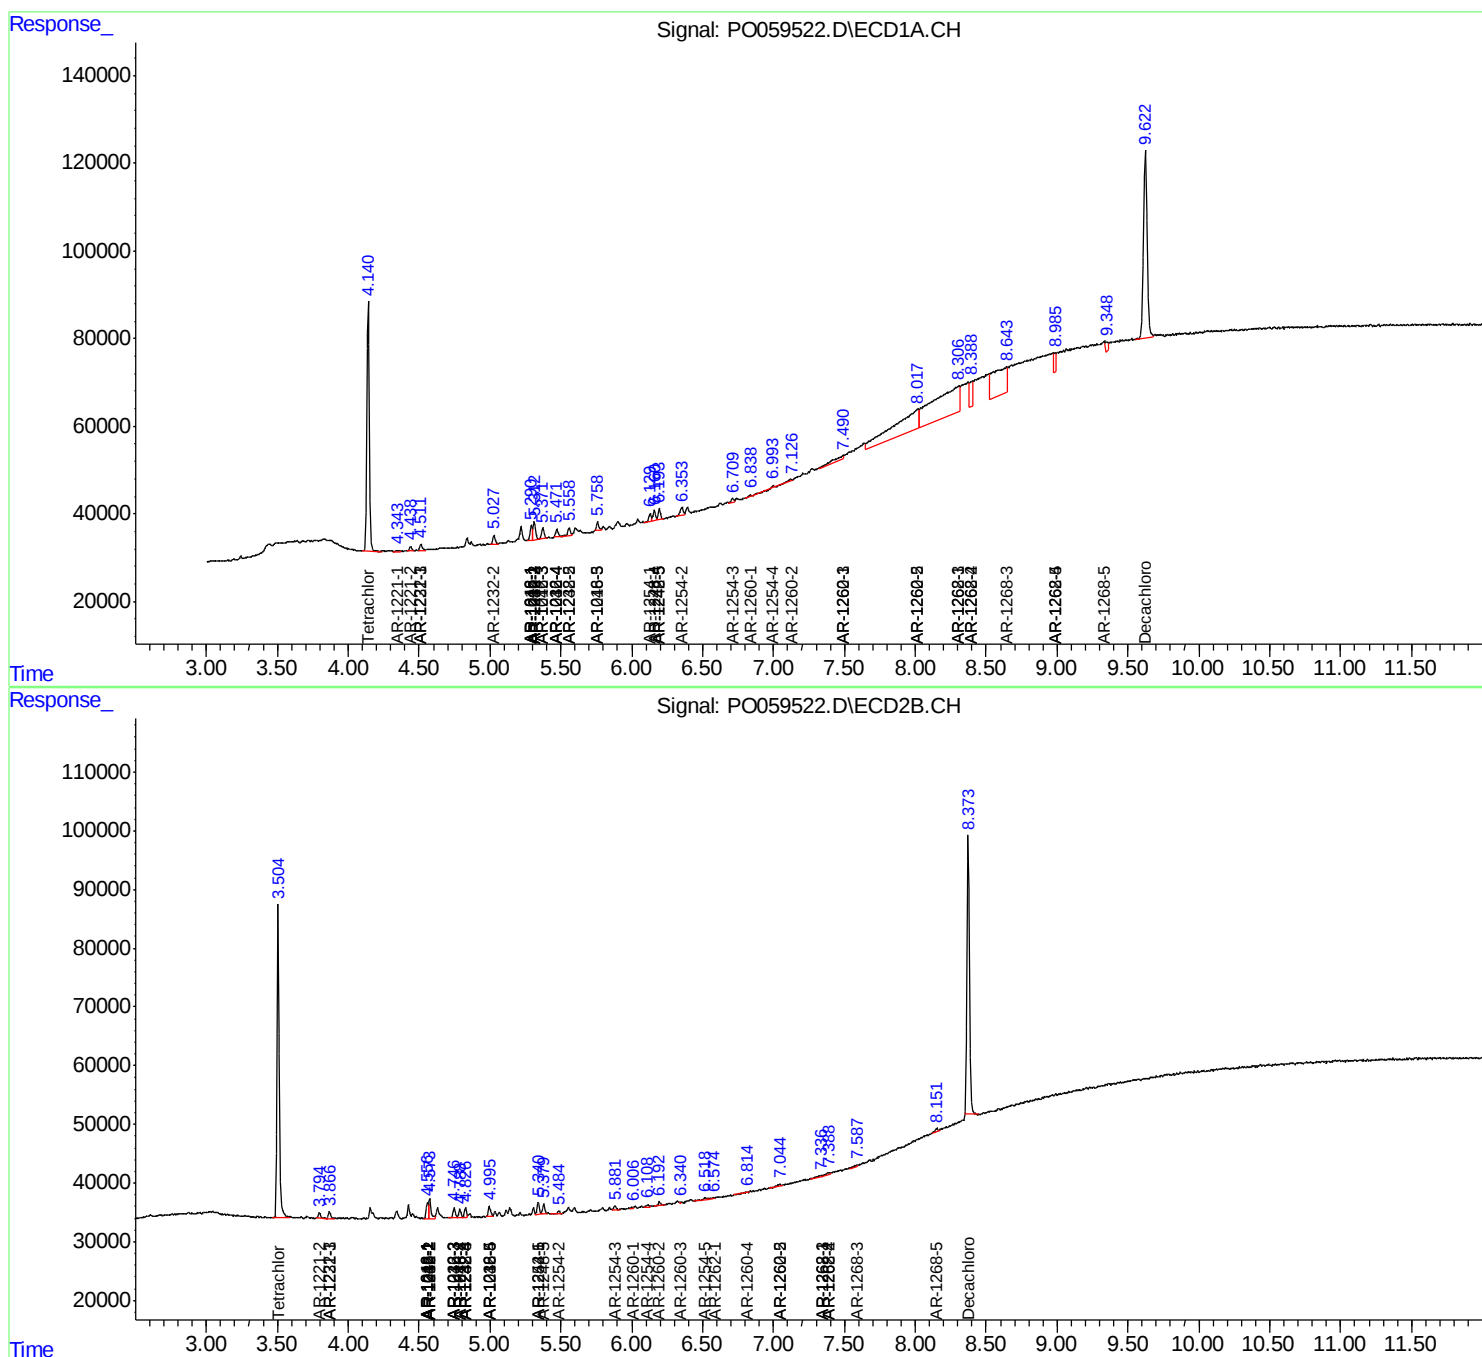




#1 Tetrachloro-m-xylene


R.T.: 4.140 min
Delta R.T.: -0.009 min
Response: 649274
Conc: 18.54 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019




#1 Tetrachloro-m-xylene

R.T.: 3.505 min
Delta R.T.: -0.005 min
Response: 583535
Conc: 16.21 ng/ml




#2 Decachlorobiphenyl

R.T.: 9.622 min
Delta R.T.: -0.018 min
Response: 789013
Conc: 14.83 ng/ml

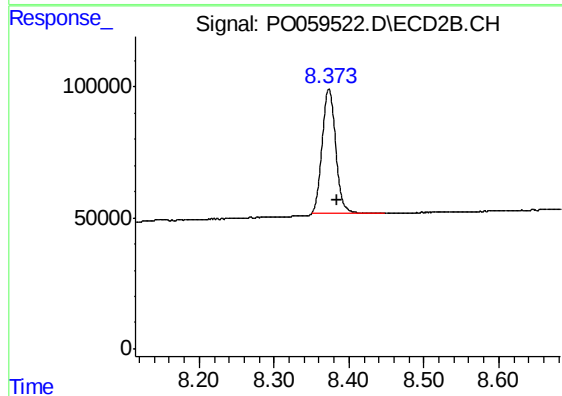

#2 Decachlorobiphenyl


R.T.: 8.373 min
Delta R.T.: -0.010 min
Response: 593295
Conc: 14.71 ng/ml

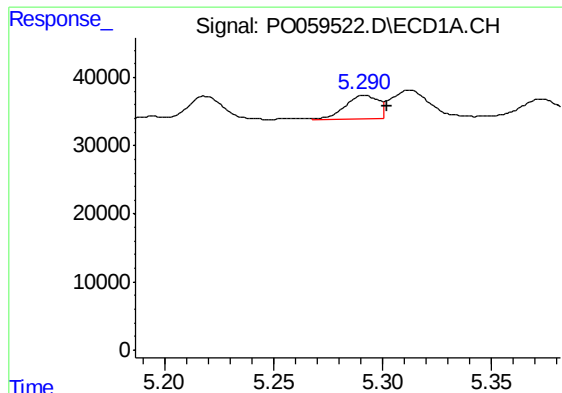

#3 AR-1016-1


R.T.: 5.292 min
Delta R.T.: -0.010 min
Response: 35257
Conc: 21.98 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

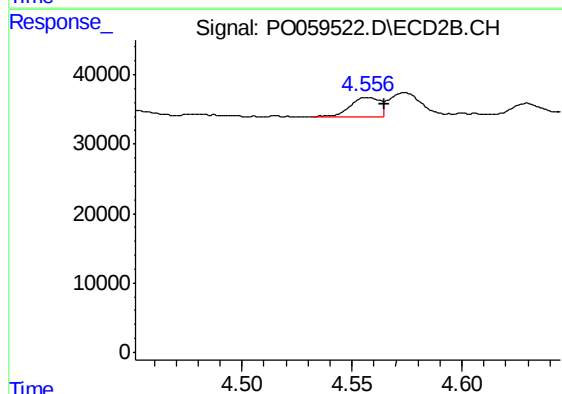


#3 AR-1016-1

R.T.: 4.557 min
Delta R.T.: -0.008 min
Response: 25835
Conc: 19.11 ng/ml

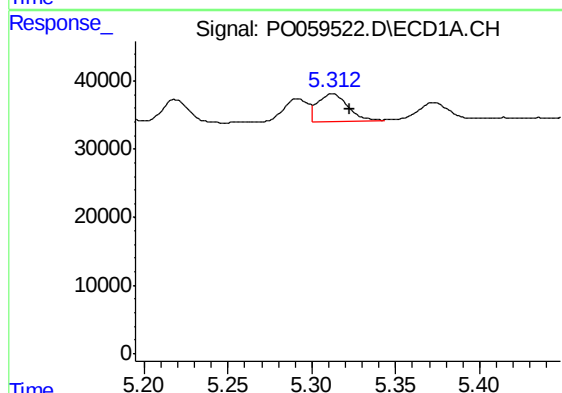


#4 AR-1016-2

R.T.: 5.312 min
Delta R.T.: -0.011 min
Response: 50985
Conc: 21.31 ng/ml

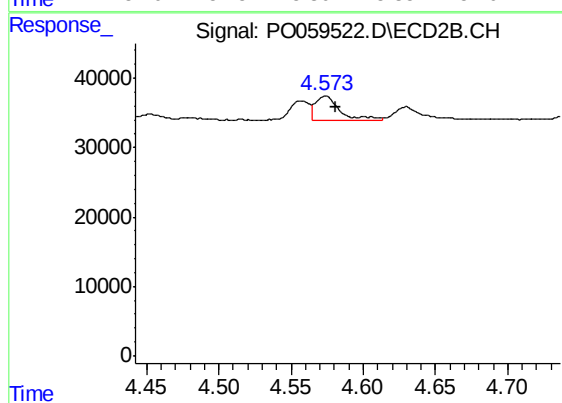

#4 AR-1016-2


R.T.: 4.574 min
Delta R.T.: -0.007 min
Response: 40503
Conc: 20.22 ng/ml



#5 AR-1016-3


R.T.: 5.373 min
Delta R.T.: -0.011 min
Response: 33174
Conc: 22.27 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019




#5 AR-1016-3

R.T.: 4.746 min
Delta R.T.: -0.008 min
Response: 20072
Conc: 18.55 ng/ml




#6 AR-1016-4

R.T.: 5.471 min
Delta R.T.: -0.010 min
Response: 21297
Conc: 17.60 ng/ml

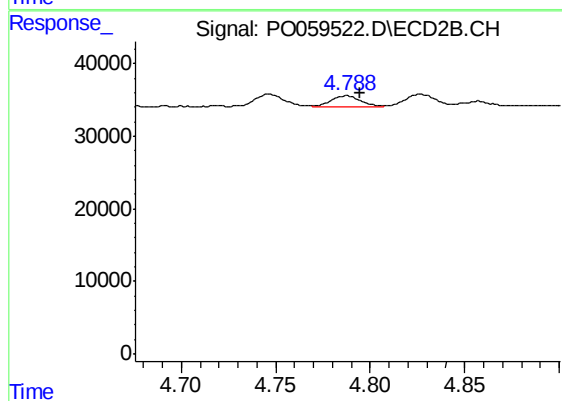

#6 AR-1016-4


R.T.: 4.788 min
Delta R.T.: -0.007 min
Response: 16048
Conc: 17.77 ng/ml

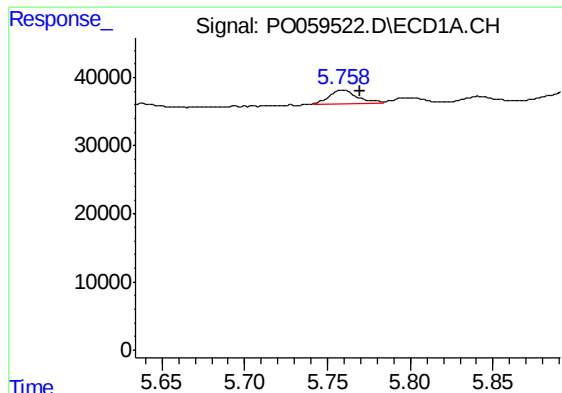

#7 AR-1016-5


R.T.: 5.759 min
Delta R.T.: -0.011 min
Response: 22733
Conc: 17.70 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

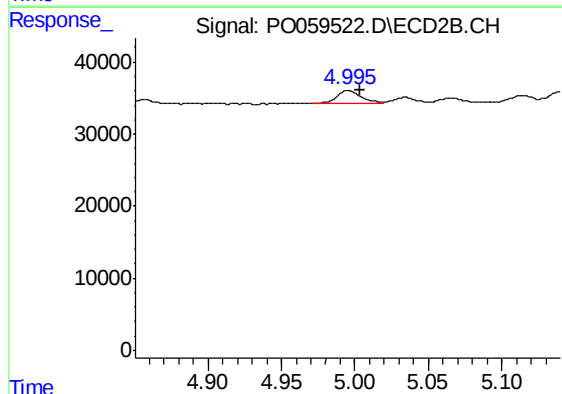


#7 AR-1016-5

R.T.: 4.995 min
Delta R.T.: -0.008 min
Response: 20468
Conc: 17.77 ng/ml

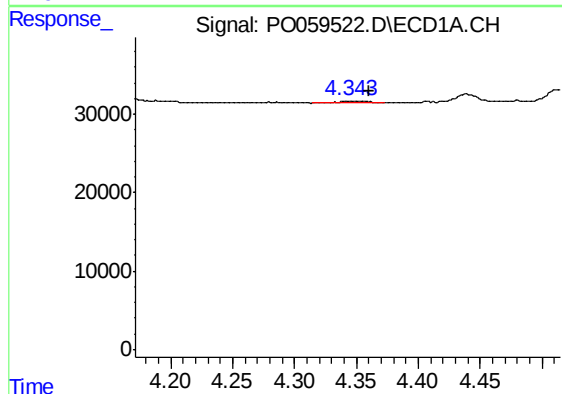


#8 AR-1221-1

R.T.: 4.344 min
Delta R.T.: -0.016 min
Response: 3800
Conc: 8.97 ng/ml

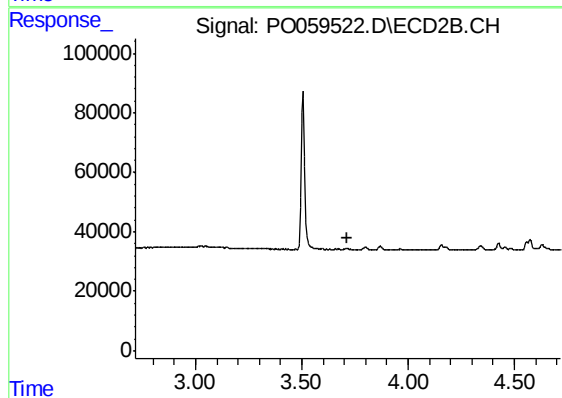

#8 AR-1221-1


R.T.: 0.000 min
Exp R.T. : 3.717 min
Response: 0
Conc: N.D.

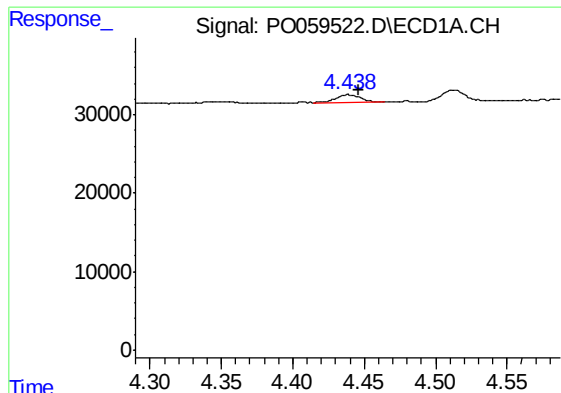

#9 AR-1221-2


R.T.: 4.438 min
Delta R.T.: -0.008 min
Response: 13086
Conc: 40.29 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

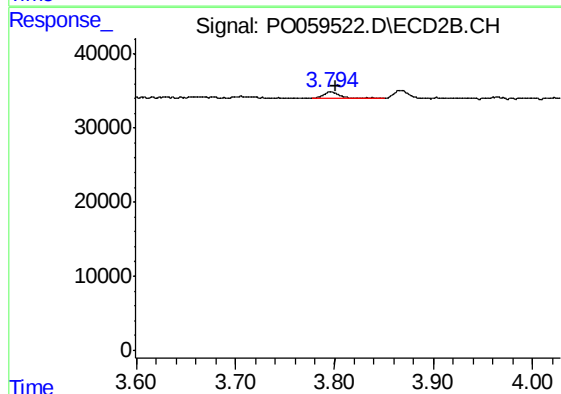


#9 AR-1221-2

R.T.: 3.796 min
Delta R.T.: -0.005 min
Response: 10306
Conc: 33.83 ng/ml

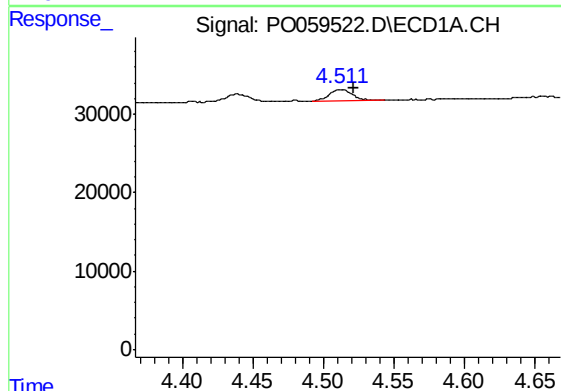


#10 AR-1221-3

R.T.: 4.512 min
Delta R.T.: -0.010 min
Response: 17415
Conc: 16.56 ng/ml

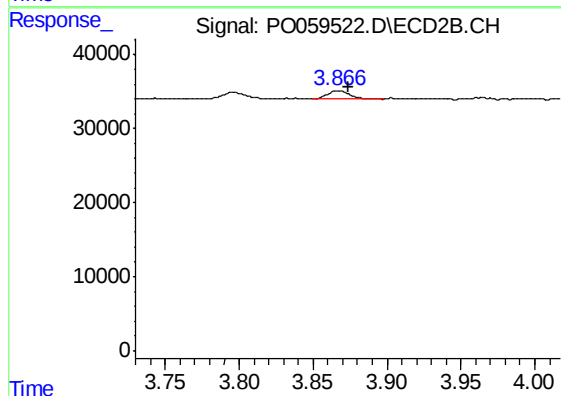

#10 AR-1221-3


R.T.: 3.867 min
Delta R.T.: -0.007 min
Response: 12097
Conc: 12.36 ng/ml

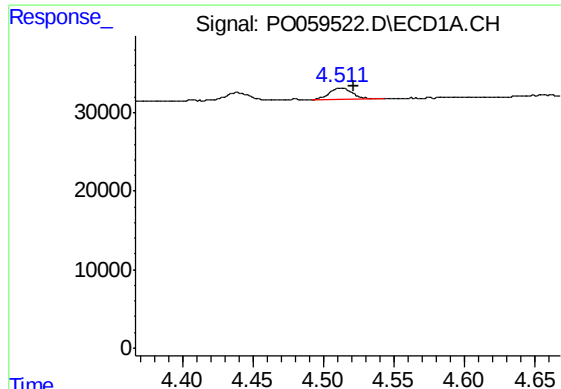

#11 AR-1232-1


R.T.: 4.512 min
Delta R.T.: -0.009 min
Response: 17415
Conc: 13.97 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

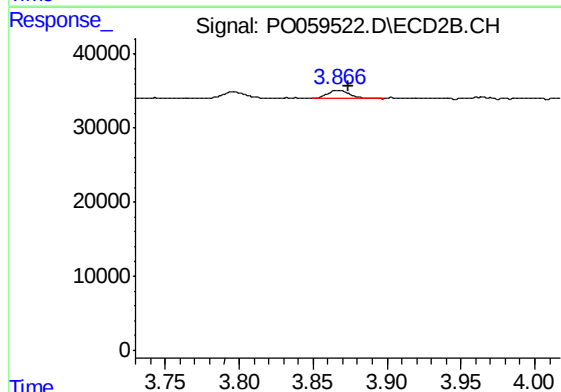


#11 AR-1232-1

R.T.: 3.867 min
Delta R.T.: -0.007 min
Response: 12097
Conc: 10.61 ng/ml

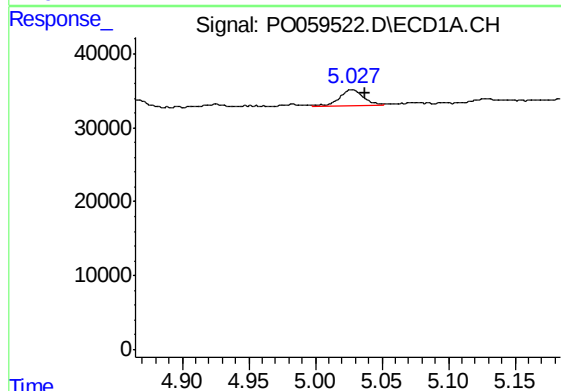


#12 AR-1232-2

R.T.: 5.027 min
Delta R.T.: -0.010 min
Response: 25070
Conc: 35.49 ng/ml

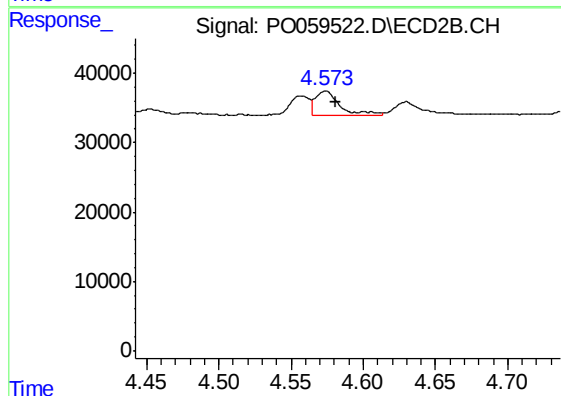

#12 AR-1232-2


R.T.: 4.574 min
Delta R.T.: -0.007 min
Response: 40503
Conc: 31.80 ng/ml

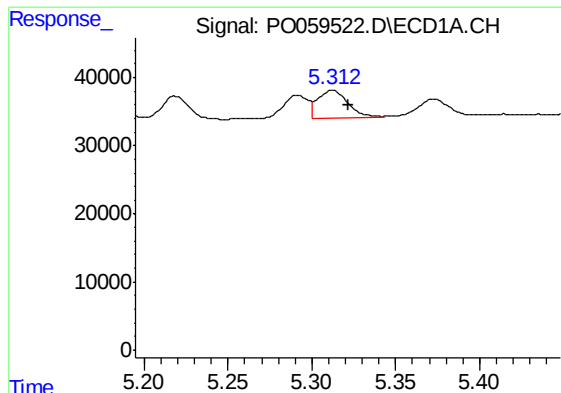

#13 AR-1232-3


R.T.: 5.312 min
Delta R.T.: -0.010 min
Response: 50985
Conc: 33.29 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

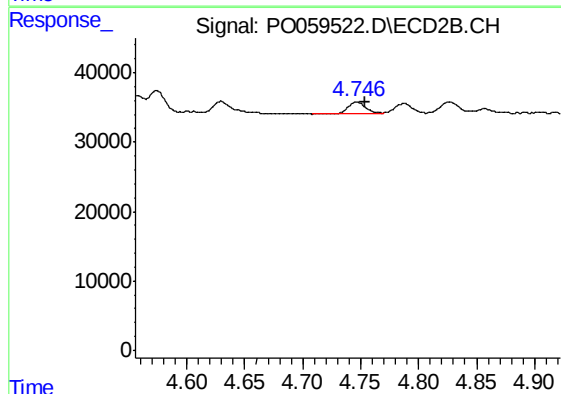


#13 AR-1232-3

R.T.: 4.746 min
Delta R.T.: -0.007 min
Response: 20072
Conc: 29.48 ng/ml

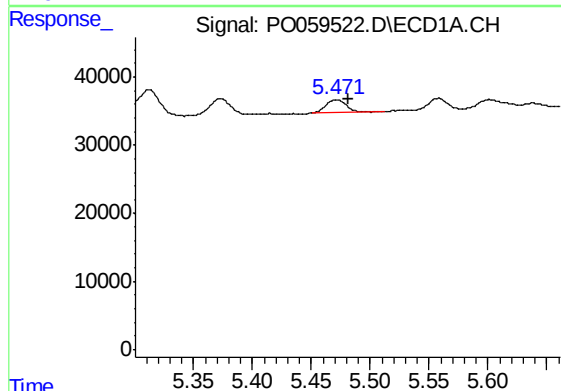


#14 AR-1232-4

R.T.: 5.471 min
Delta R.T.: -0.010 min
Response: 21297
Conc: 27.24 ng/ml

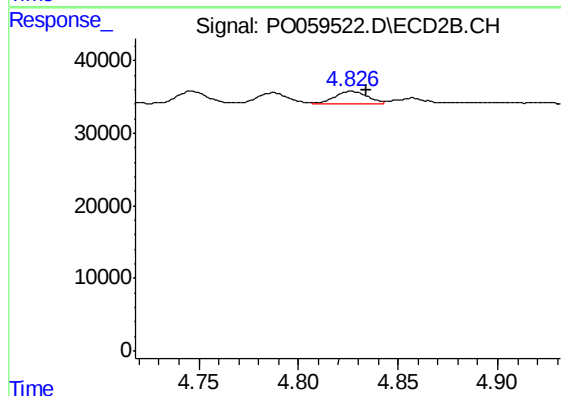

#14 AR-1232-4


R.T.: 4.826 min
Delta R.T.: -0.008 min
Response: 18753
Conc: 30.74 ng/ml

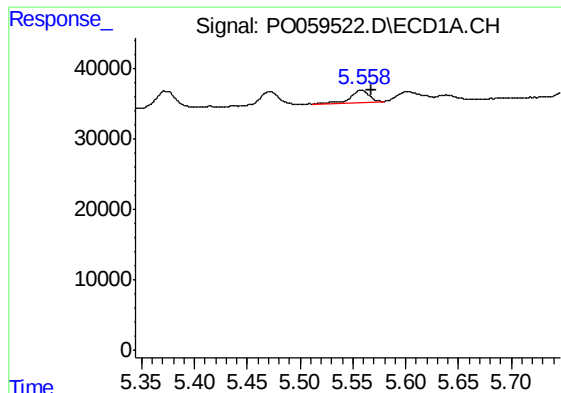

#15 AR-1232-5


R.T.: 5.558 min
Delta R.T.: -0.010 min
Response: 21680
Conc: 36.07 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

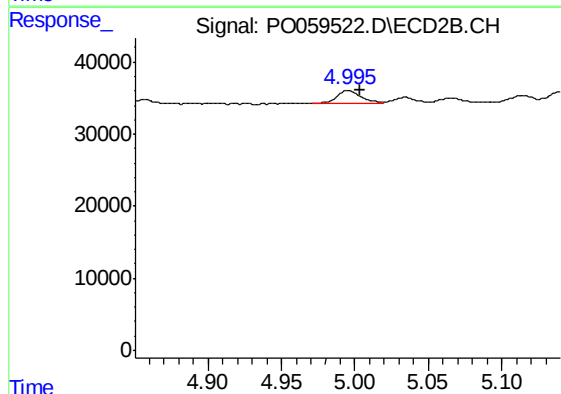


#15 AR-1232-5

R.T.: 4.995 min
Delta R.T.: -0.008 min
Response: 20468
Conc: 30.07 ng/ml

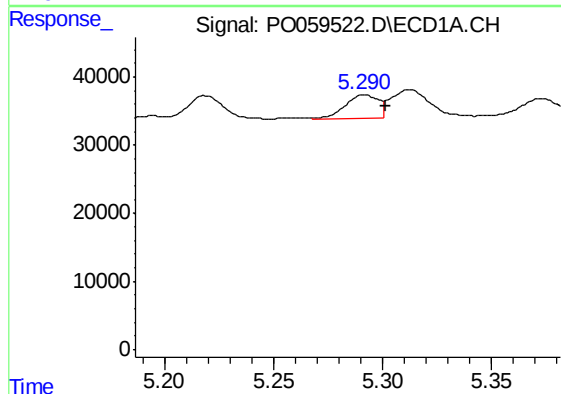


#16 AR-1242-1

R.T.: 5.292 min
Delta R.T.: -0.010 min
Response: 35257
Conc: 27.77 ng/ml

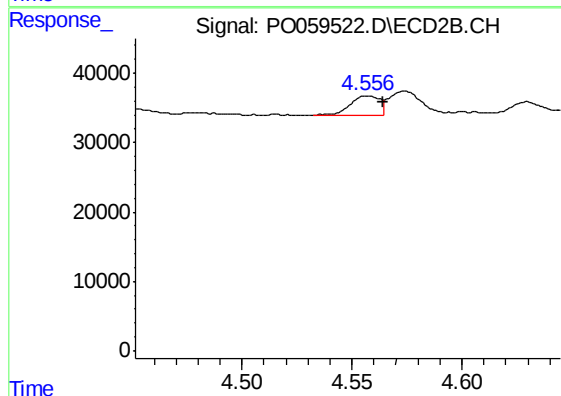

#16 AR-1242-1


R.T.: 4.557 min
Delta R.T.: -0.008 min
Response: 25835
Conc: 25.12 ng/ml

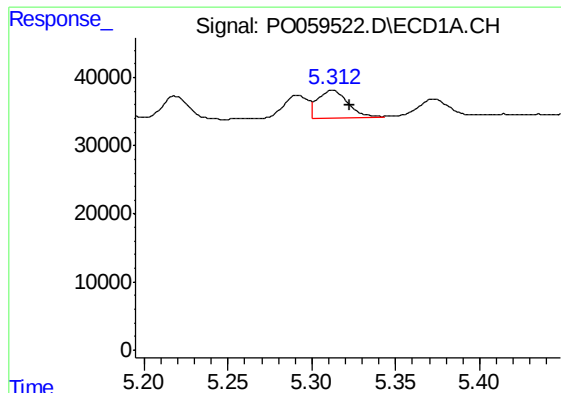

#17 AR-1242-2


R.T.: 5.312 min
Delta R.T.: -0.010 min
Response: 50985
Conc: 27.48 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

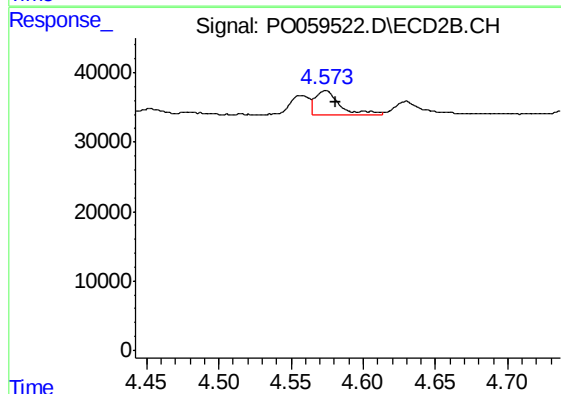


#17 AR-1242-2

R.T.: 4.574 min
Delta R.T.: -0.007 min
Response: 40503
Conc: 26.59 ng/ml

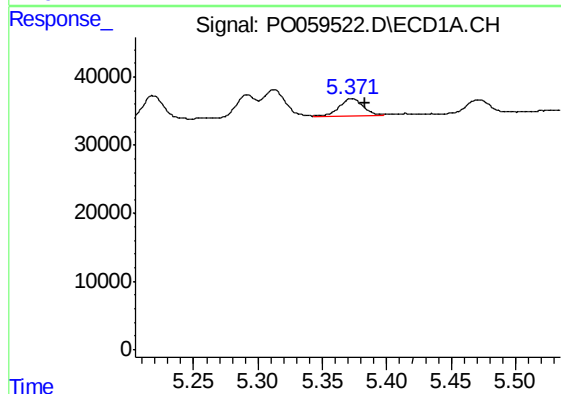


#18 AR-1242-3

R.T.: 5.373 min
Delta R.T.: -0.011 min
Response: 33174
Conc: 28.38 ng/ml

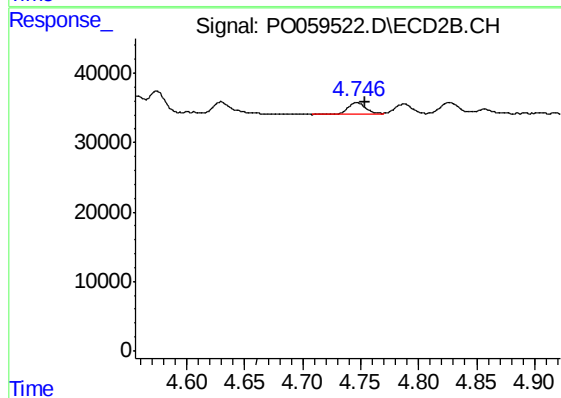

#18 AR-1242-3


R.T.: 4.746 min
Delta R.T.: -0.007 min
Response: 20072
Conc: 24.02 ng/ml

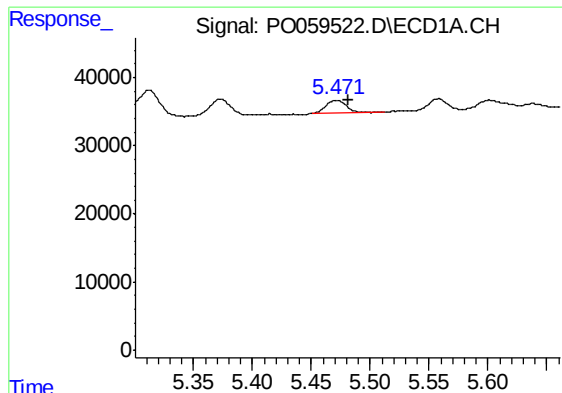

#19 AR-1242-4


R.T.: 5.471 min
Delta R.T.: -0.010 min
Response: 21297
Conc: 22.00 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

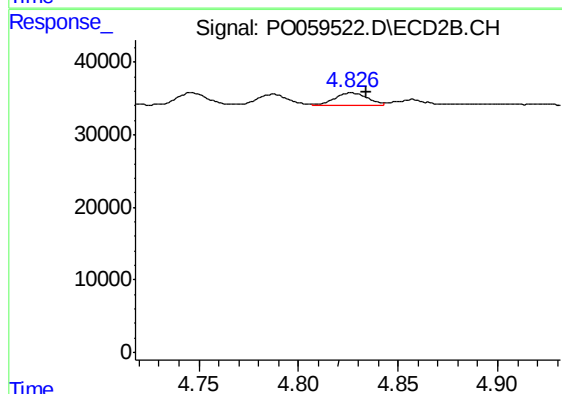


#19 AR-1242-4

R.T.: 4.826 min
Delta R.T.: -0.008 min
Response: 18753
Conc: 22.48 ng/ml

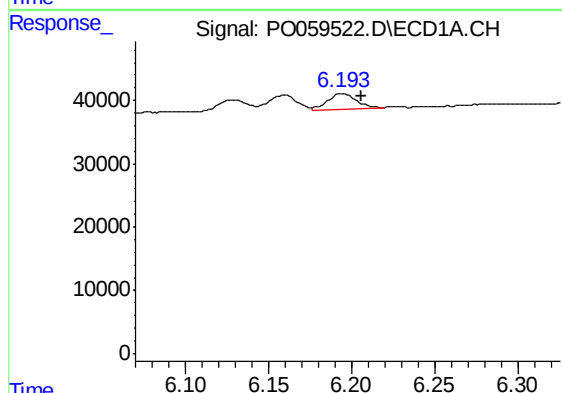


#20 AR-1242-5

R.T.: 6.194 min
Delta R.T.: -0.012 min
Response: 29737
Conc: 23.66 ng/ml

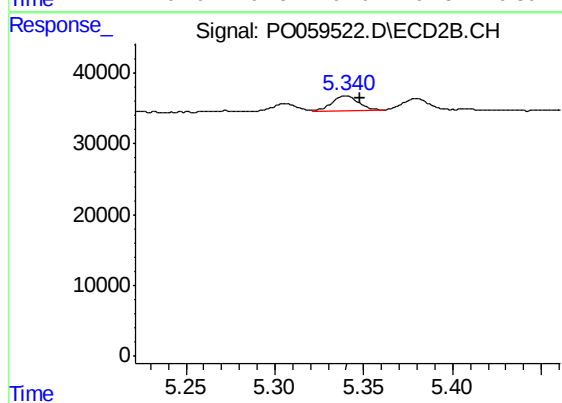

#20 AR-1242-5


R.T.: 5.340 min
Delta R.T.: -0.008 min
Response: 22089
Conc: 19.75 ng/ml



#21 AR-1248-1


R.T.: 5.292 min
Delta R.T.: -0.009 min
Response: 35257
Conc: 35.17 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019




#21 AR-1248-1

R.T.: 4.557 min
Delta R.T.: -0.007 min
Response: 25835
Conc: 31.20 ng/ml

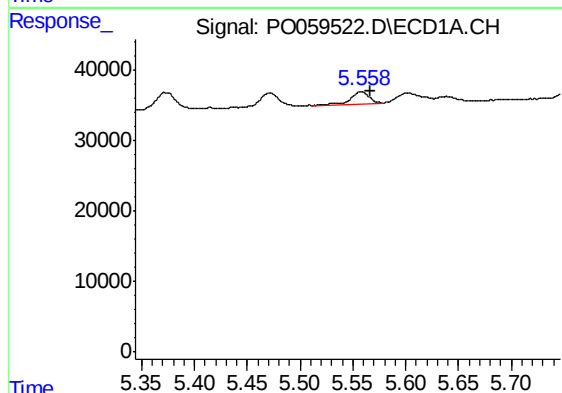


#22 AR-1248-2

R.T.: 5.558 min
Delta R.T.: -0.009 min
Response: 21680
Conc: 14.94 ng/ml

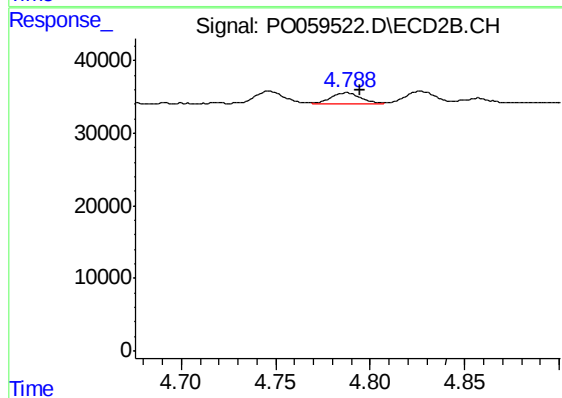

#22 AR-1248-2


R.T.: 4.788 min
Delta R.T.: -0.007 min
Response: 16048
Conc: 13.92 ng/ml

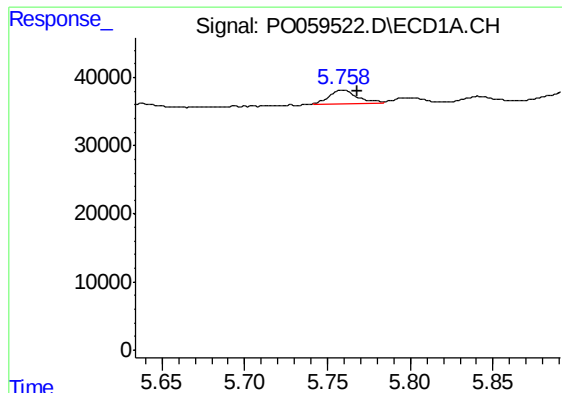

#23 AR-1248-3


R.T.: 5.759 min
Delta R.T.: -0.009 min
Response: 22733
Conc: 13.68 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

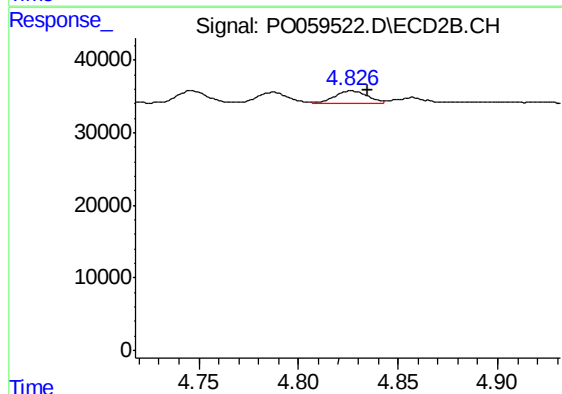


#23 AR-1248-3

R.T.: 4.826 min
Delta R.T.: -0.008 min
Response: 18753
Conc: 15.79 ng/ml




#24 AR-1248-4

R.T.: 6.160 min
Delta R.T.: -0.009 min
Response: 29344
Conc: 14.36 ng/ml

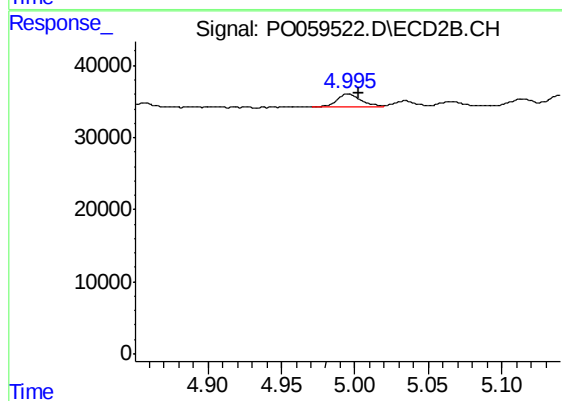

#24 AR-1248-4


R.T.: 4.995 min
Delta R.T.: -0.007 min
Response: 20468
Conc: 14.09 ng/ml

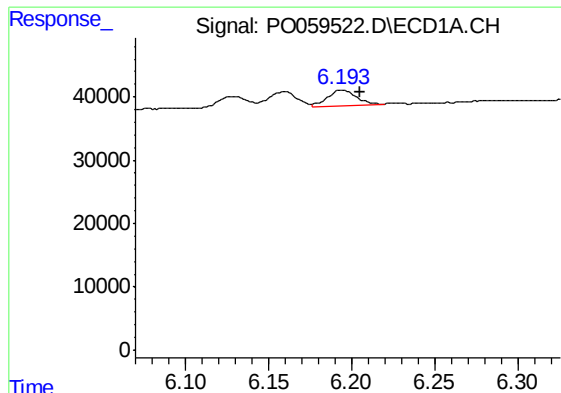

#25 AR-1248-5


R.T.: 6.194 min
Delta R.T.: -0.011 min
Response: 29737
Conc: 15.00 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

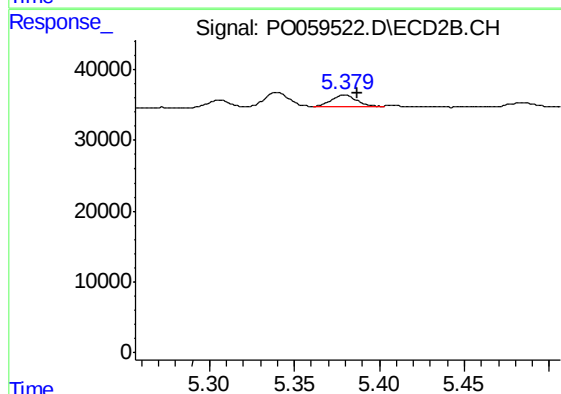


#25 AR-1248-5

R.T.: 5.380 min
Delta R.T.: -0.007 min
Response: 16522
Conc: 11.54 ng/ml

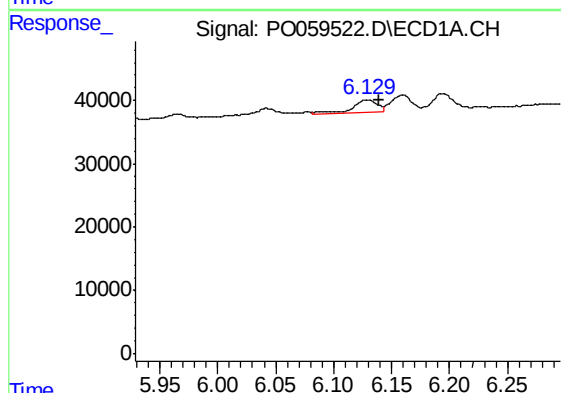


#26 AR-1254-1

R.T.: 6.129 min
Delta R.T.: -0.010 min
Response: 26944
Conc: 12.91 ng/ml

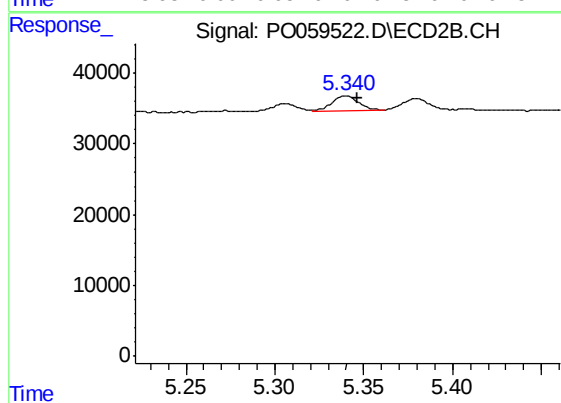

#26 AR-1254-1


R.T.: 5.340 min
Delta R.T.: -0.007 min
Response: 22089
Conc: 9.31 ng/ml



#27 AR-1254-2


R.T.: 6.354 min
Delta R.T.: 0.000 min
Response: 27552
Conc: 8.26 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019




#27 AR-1254-2

R.T.: 5.485 min
Delta R.T.: -0.007 min
Response: 5242
Conc: 2.50 ng/ml




#28 AR-1254-3

R.T.: 6.710 min
Delta R.T.: -0.010 min
Response: 9997
Conc: 2.82 ng/ml

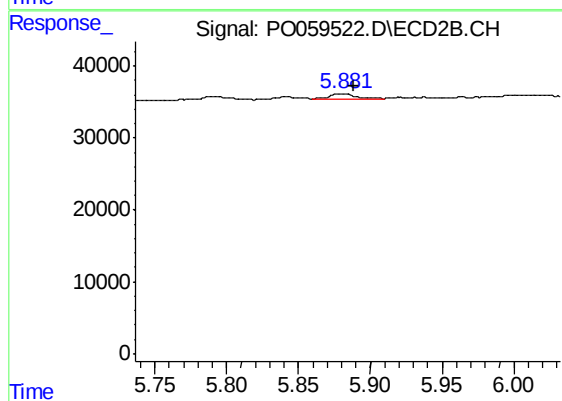

#28 AR-1254-3


R.T.: 5.882 min
Delta R.T.: -0.007 min
Response: 10189
Conc: 3.03 ng/ml

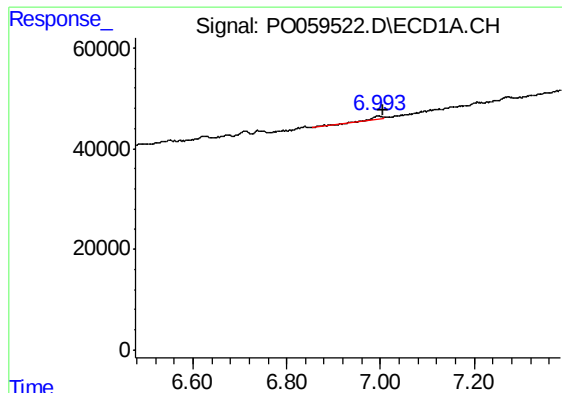

#29 AR-1254-4


R.T.: 6.994 min
Delta R.T.: -0.010 min
Response: 8156
Conc: 2.77 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

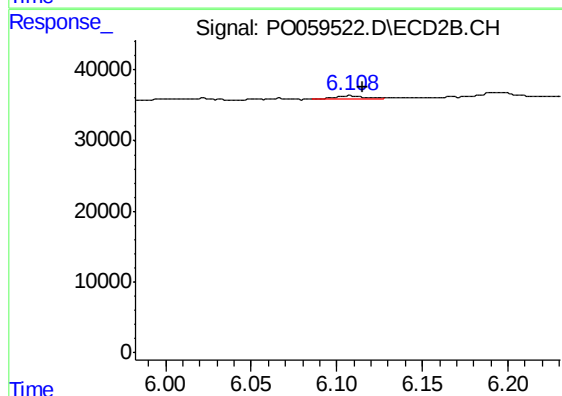


#29 AR-1254-4

R.T.: 6.107 min
Delta R.T.: -0.008 min
Response: 5753
Conc: 2.79 ng/ml

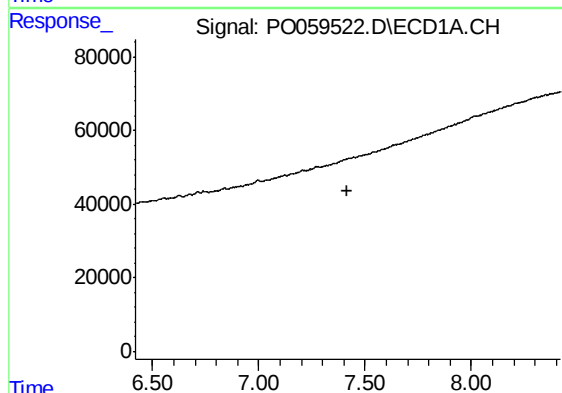


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 7.419 min
Response: 0
Conc: N.D.

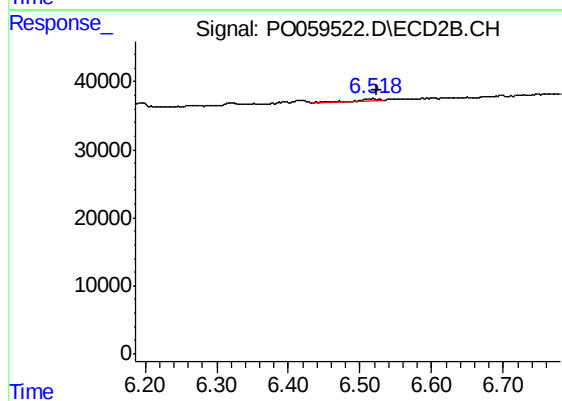

#30 AR-1254-5


R.T.: 6.517 min
Delta R.T.: -0.007 min
Response: 9059
Conc: 2.92 ng/ml



#31 AR-1260-1


R.T.: 6.838 min
Delta R.T.: -0.042 min
Response: 7720
Conc: 2.86 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

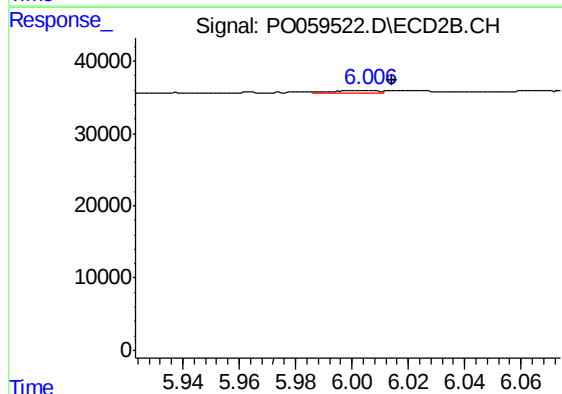


#31 AR-1260-1

R.T.: 6.006 min
Delta R.T.: -0.008 min
Response: 3511
Conc: 1.54 ng/ml




#32 AR-1260-2

R.T.: 7.126 min
Delta R.T.: -0.009 min
Response: 5931
Conc: 1.60 ng/ml

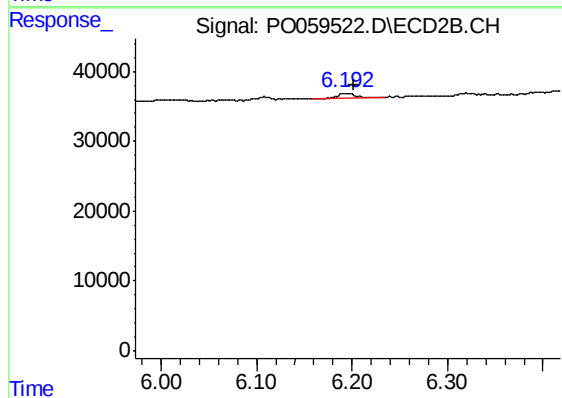

#32 AR-1260-2


R.T.: 6.197 min
Delta R.T.: -0.005 min
Response: 11800
Conc: 4.03 ng/ml



#33 AR-1260-3


R.T.: 7.490 min
Delta R.T.: 0.000 min
Response: 61838
Conc: 18.87 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019




#33 AR-1260-3

R.T.: 6.340 min
Delta R.T.: -0.011 min
Response: 1130
Conc: 0.43 ng/ml




#34 AR-1260-4

R.T.: 0.000 min
Exp R.T. : 7.717 min
Response: 0
Conc: N.D.

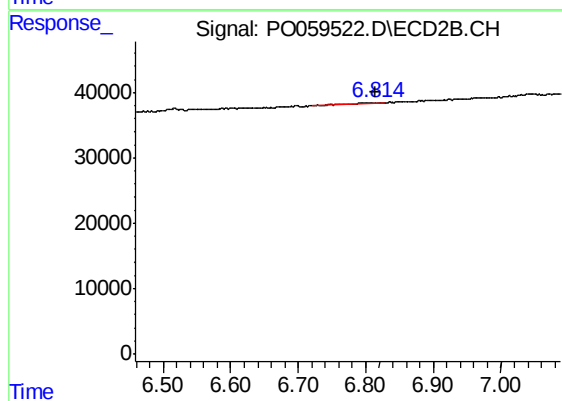

#34 AR-1260-4


R.T.: 6.815 min
Delta R.T.: 0.000 min
Response: 2972
Conc: 1.31 ng/ml

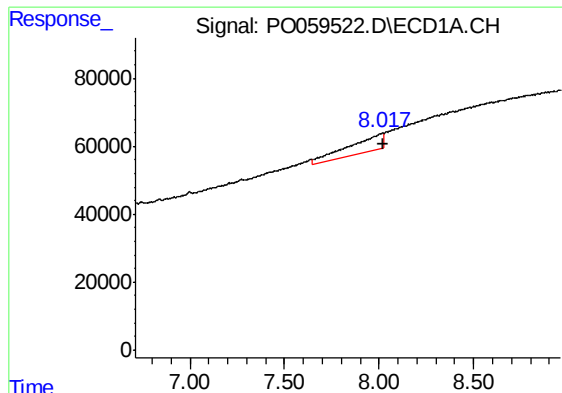

#35 AR-1260-5


R.T.: 8.018 min
Delta R.T.: -0.007 min
Response: 632947
Conc: 89.39 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

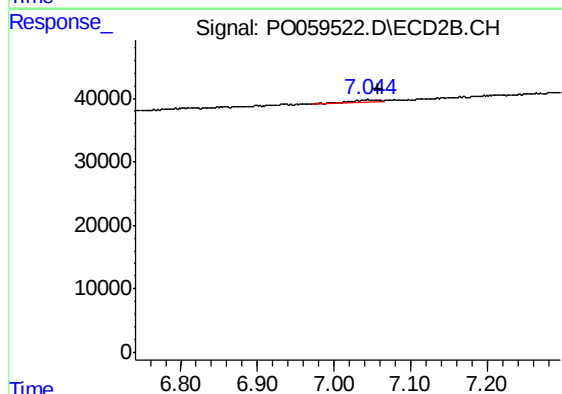


#35 AR-1260-5

R.T.: 7.046 min
Delta R.T.: -0.012 min
Response: 7557
Conc: 1.37 ng/ml

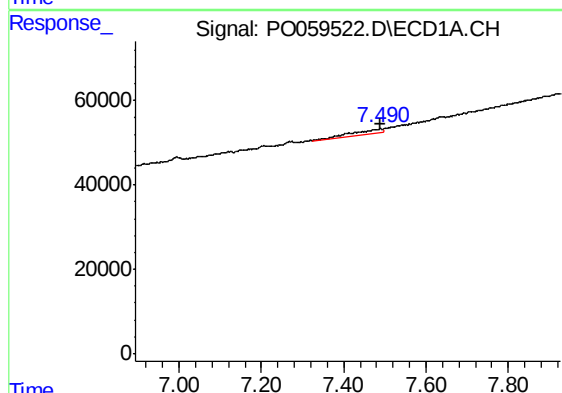


#36 AR-1262-1

R.T.: 7.490 min
Delta R.T.: 0.000 min
Response: 61838
Conc: 12.74 ng/ml

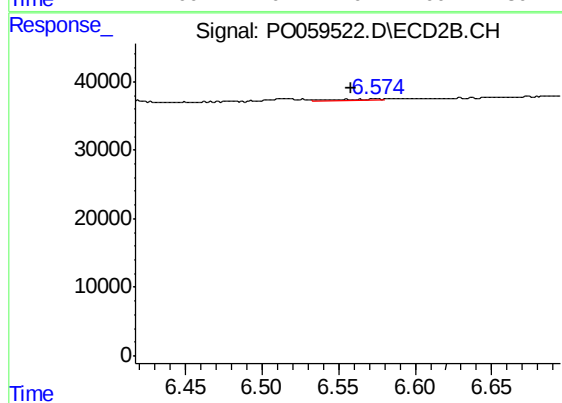

#36 AR-1262-1


R.T.: 6.575 min
Delta R.T.: 0.017 min
Response: 3505
Conc: 0.94 ng/ml



#37 AR-1262-2


R.T.: 8.018 min
Delta R.T.: -0.006 min
Response: 632947
Conc: 82.03 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019




#37 AR-1262-2

R.T.: 7.046 min
Delta R.T.: -0.012 min
Response: 7557
Conc: 1.29 ng/ml




#38 AR-1262-3

R.T.: 8.307 min
Delta R.T.: 0.004 min
Response: 880600
Conc: 172.59 ng/ml

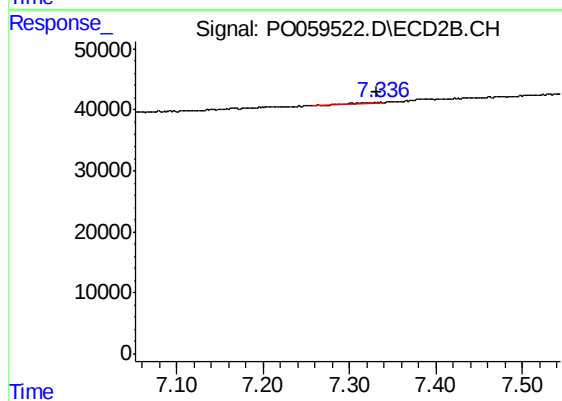

#38 AR-1262-3


R.T.: 7.335 min
Delta R.T.: 0.002 min
Response: 4365
Conc: 1.72 ng/ml

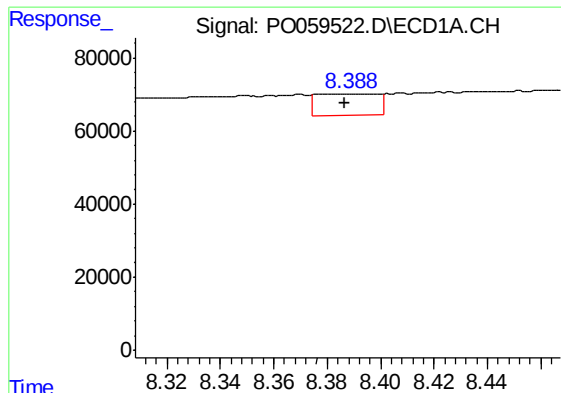

#39 AR-1262-4


R.T.: 8.390 min
Delta R.T.: 0.003 min
Response: 91823
Conc: 23.82 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

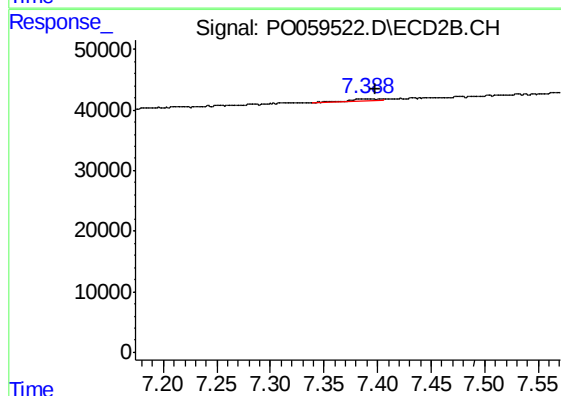


#39 AR-1262-4

R.T.: 7.394 min
Delta R.T.: -0.003 min
Response: 6821
Conc: 1.54 ng/ml

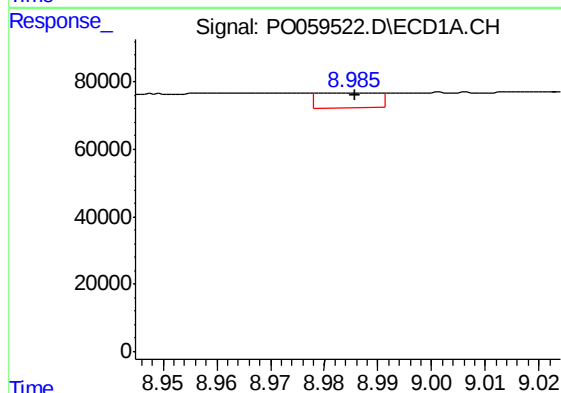


#40 AR-1262-5

R.T.: 8.986 min
Delta R.T.: 0.000 min
Response: 35302
Conc: 13.75 ng/ml

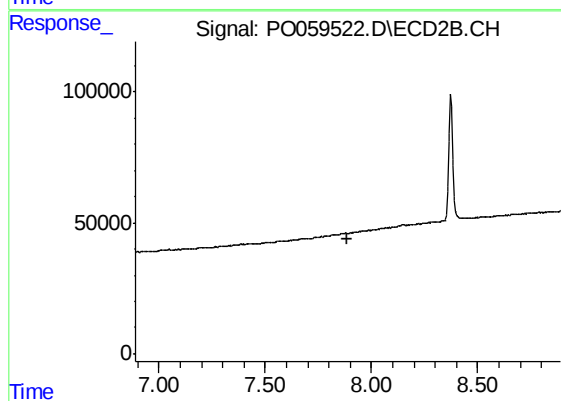

#40 AR-1262-5


R.T.: 0.000 min
Exp R.T. : 7.889 min
Response: 0
Conc: N.D.



#41 AR-1268-1


R.T.: 8.307 min
Delta R.T.: 0.004 min
Response: 880600
Conc: 93.57 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019




#41 AR-1268-1

R.T.: 7.335 min
Delta R.T.: 0.004 min
Response: 4365
Conc: 0.61 ng/ml




#42 AR-1268-2

R.T.: 8.390 min
Delta R.T.: 0.000 min
Response: 91823
Conc: 11.65 ng/ml

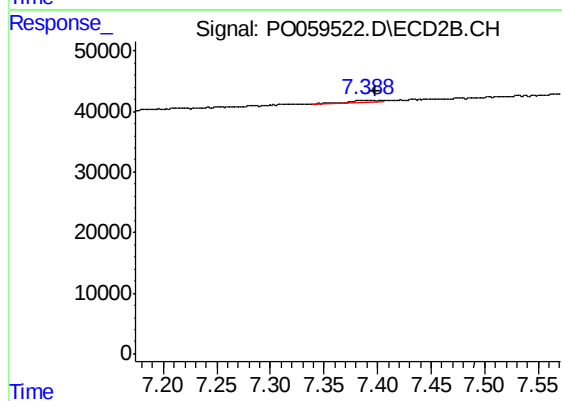

#42 AR-1268-2


R.T.: 7.394 min
Delta R.T.: -0.003 min
Response: 6821
Conc: 1.06 ng/ml



#43 AR-1268-3


R.T.: 8.645 min
Delta R.T.: 0.056 min
Response: 444085
Conc: 63.00 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019




#43 AR-1268-3

R.T.: 7.588 min
Delta R.T.: -0.005 min
Response: 3874
Conc: 0.71 ng/ml




#44 AR-1268-4

R.T.: 8.986 min
Delta R.T.: 0.000 min
Response: 35302
Conc: 12.70 ng/ml

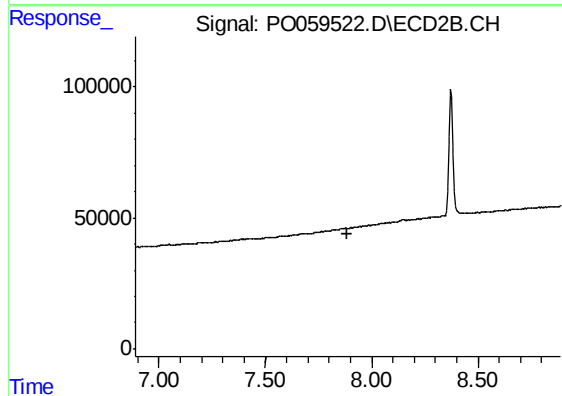

#44 AR-1268-4


R.T.: 0.000 min
Exp R.T. : 7.888 min
Response: 0
Conc: N.D.

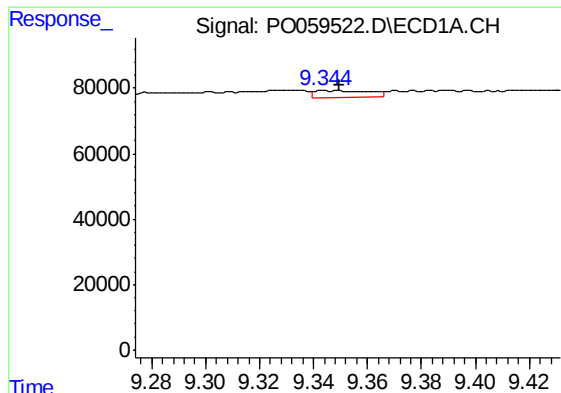

#45 AR-1268-5

R.T.: 9.344 min
Delta R.T.: -0.006 min
Response: 31541
Conc: 1.71 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

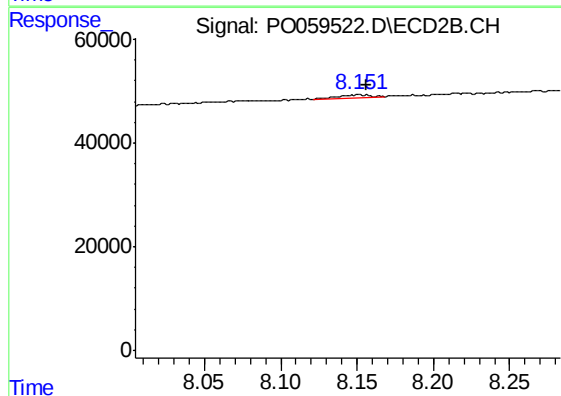

#45 AR-1268-5

R.T.: 8.151 min
Delta R.T.: -0.006 min
Response: 7349
Conc: 0.51 ng/ml