

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082119\
 Data File : P0059599.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Aug 2019 18:36
 Operator : SM/AJ
 Sample : K4444-01 5X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SES-GODWIN-PUMP-082019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 22 03:55:17 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 17 03:09:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.131	3.501	164604	152034	4.701	4.224
2)	SA Decachlor...	9.614	8.368	197926	132649	3.720	3.290
Target Compounds							
3)	L1 AR-1016-1	5.309	0.000	5469	0	3.410	N.D. #
4)	L1 AR-1016-2	5.323	0.000	601	0	0.251	N.D. #
5)	L1 AR-1016-3	5.376	4.787	1035	8959	0.695	8.281 #
6)	L1 AR-1016-4	5.438	4.787	6087	8959	5.032	9.922 #
7)	L1 AR-1016-5	5.765	0.000	480	0	0.374	N.D. #
8)	L2 AR-1221-1	4.362	3.663	2076	25615	4.901	63.816 #
9)	L2 AR-1221-2	4.463	3.833	1383	8060	4.257	26.460 #
10)	L2 AR-1221-3	4.509	3.833	2192	8060	2.084	8.238 #
11)	L3 AR-1232-1	4.509	3.833	2192	8060	1.759	7.070 #
12)	L3 AR-1232-2	5.043	0.000	778	0	1.101	N.D. #
13)	L3 AR-1232-3	5.323	4.787	601	8959	0.392	13.158 #
14)	L3 AR-1232-4	5.438	4.787	6087	8959	7.785	14.686 #
15)	L3 AR-1232-5	5.578	0.000	9845	0	16.378	N.D. #
16)	L4 AR-1242-1	5.309	0.000	5469	0	4.308	N.D. #
17)	L4 AR-1242-2	5.323	0.000	601	0	0.324	N.D. #
18)	L4 AR-1242-3	5.376	4.787	1035	8959	0.886	10.723 #
19)	L4 AR-1242-4	5.438	4.787	6087	8959	6.289	10.738 #
20)	L4 AR-1242-5	6.167	5.316	1407	2999	1.120	2.681 #
21)	L5 AR-1248-1	5.309	0.000	5469	0	5.455	N.D. #
22)	L5 AR-1248-2	5.578	4.787	9845	8959	6.785	7.770
23)	L5 AR-1248-3	5.765	4.787	480	8959	0.289	7.543 #
24)	L5 AR-1248-4	6.167	0.000	1407	0	0.688	N.D. #
25)	L5 AR-1248-5	6.167	0.000	1407	0	0.709	N.D. #
26)	L6 AR-1254-1	6.125	5.316	22767	2999	10.912	1.264 #
27)	L6 AR-1254-2	6.348	0.000	4353	0	1.305	N.D. #
28)	L6 AR-1254-3	6.703	5.885	4887	3114	1.377	0.926 #
29)	L6 AR-1254-4	6.993	6.133	2632	5271	0.893	2.556 #
30)	L6 AR-1254-5	7.414	6.514	36281	4510	11.732	1.452 #
31)	L7 AR-1260-1	6.877	5.997	1464	6742	0.543	2.958 #
32)	L7 AR-1260-2	7.150	6.190	3054	9240	0.823	3.154 #
33)	L7 AR-1260-3	7.481	6.337	39590	7497	12.084	2.830 #
34)	L7 AR-1260-4	0.000	6.820	0	1057	N.D.	0.467 #
35)	L7 AR-1260-5	8.014	7.046	26779	7284	3.782	1.324 #
36)	L8 AR-1262-1	7.481	6.543	39590	2208	8.158	0.592 #
37)	L8 AR-1262-2	8.014	7.046	26779	7284	3.471	1.239 #
38)	L8 AR-1262-3	8.300	7.317	227462	5557	44.580	2.187 #
39)	L8 AR-1262-4	8.374	7.384	267189	7842	69.315	1.775 #
40)	L8 AR-1262-5	8.983	0.000	80463	0	31.350	N.D. #
41)	L9 AR-1268-1	8.300	7.317	227462	5557	24.171	0.780 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082119\
 Data File : P0059599.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Aug 2019 18:36
 Operator : SM/AJ
 Sample : K4444-01 5X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SES-GODWIN-PUMP-082019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 22 03:55:17 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 17 03:09:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.374	7.384	267189	7842	33.896	1.216 #
43) L9	AR-1268-3	8.562	7.576	818933	7142	116.180	1.305 #
44) L9	AR-1268-4	8.983	0.000	80463	0	28.943	N.D. #
45) L9	AR-1268-5	9.344	8.145	13853	4120	0.751	0.284 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO082119\
Data File : PO059599.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Aug 2019 18:36
Operator : SM/AJ
Sample : K4444-01 5X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
SES-GODWIN-PUMP-082019

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 22 03:55:17 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Aug 17 03:09:44 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

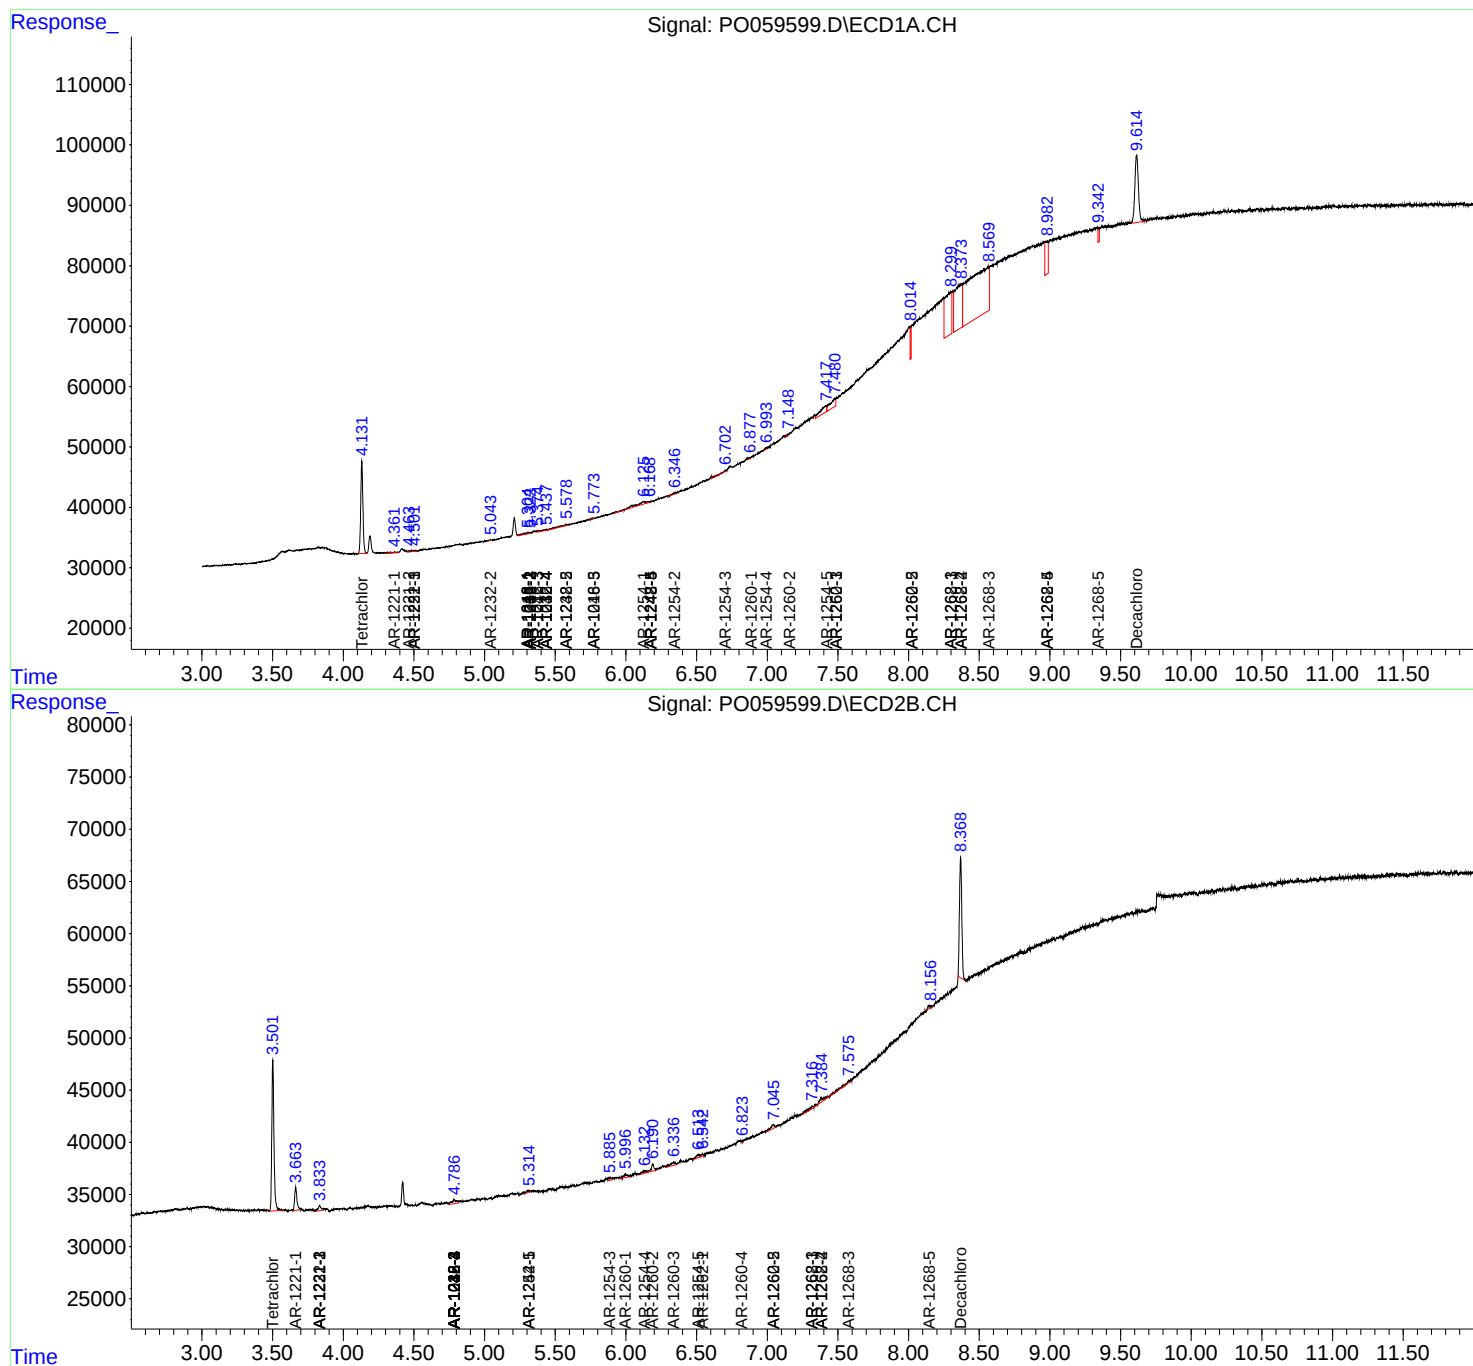


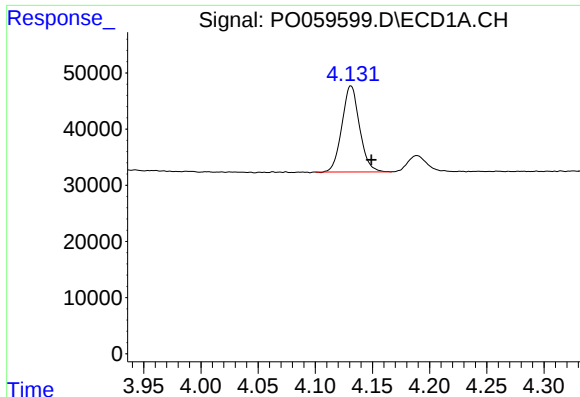

#1 Tetrachloro-m-xylene


R.T.: 4.131 min
Delta R.T.: -0.018 min
Response: 164604
Conc: 4.70 ng/ml

Instrument :
ECD_O
ClientSampleId :
SES-GODWIN-PUMP-082019

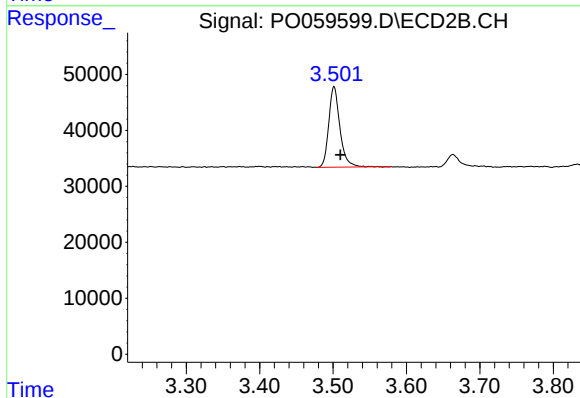


#1 Tetrachloro-m-xylene

R.T.: 3.501 min
Delta R.T.: -0.009 min
Response: 152034
Conc: 4.22 ng/ml

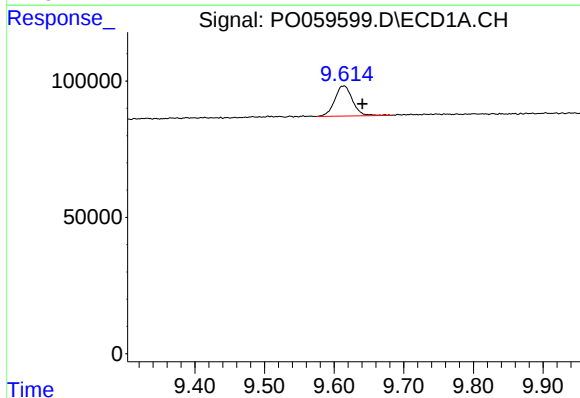


#2 Decachlorobiphenyl

R.T.: 9.614 min
Delta R.T.: -0.027 min
Response: 197926
Conc: 3.72 ng/ml

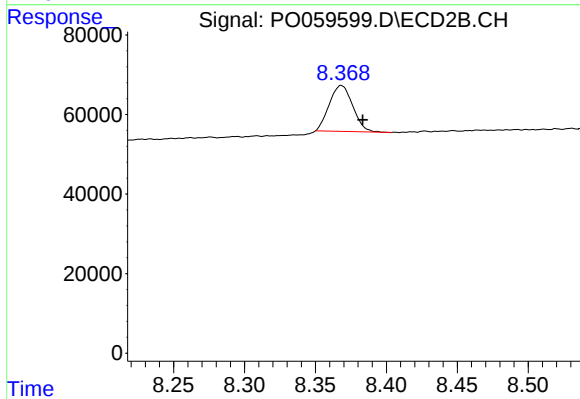

#2 Decachlorobiphenyl


R.T.: 8.368 min
Delta R.T.: -0.015 min
Response: 132649
Conc: 3.29 ng/ml

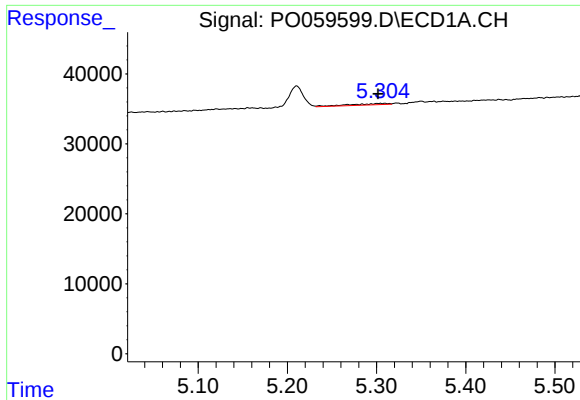

#3 AR-1016-1


R.T.: 5.309 min
Delta R.T.: 0.008 min
Response: 5469
Conc: 3.41 ng/ml

Instrument :
ECD_O
ClientSampleId :
SES-GODWIN-PUMP-082019

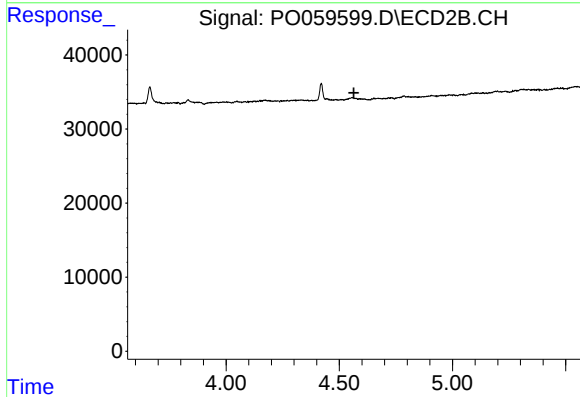


#3 AR-1016-1

R.T.: 0.000 min
Exp R.T. : 4.565 min
Response: 0
Conc: N.D.

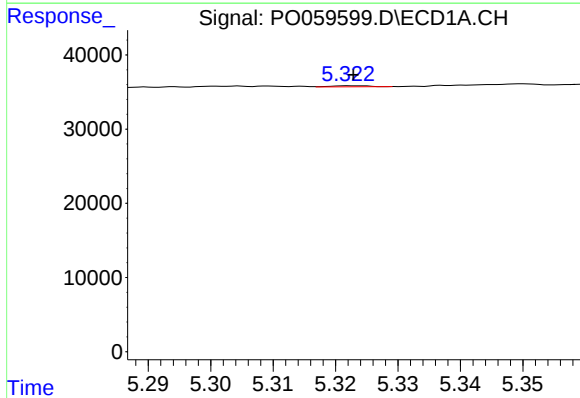


#4 AR-1016-2

R.T.: 5.323 min
Delta R.T.: 0.000 min
Response: 601
Conc: 0.25 ng/ml

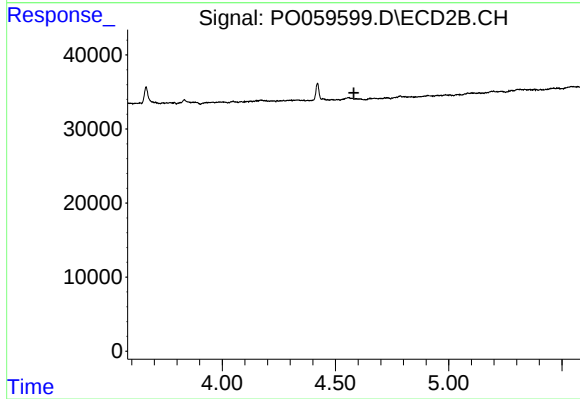

#4 AR-1016-2


R.T.: 0.000 min
Exp R.T. : 4.581 min
Response: 0
Conc: N.D.

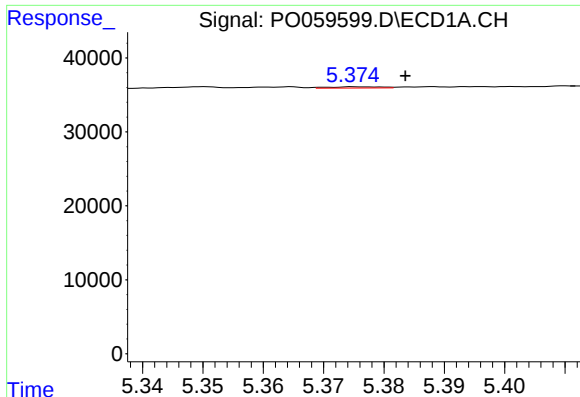

#5 AR-1016-3


R.T.: 5.376 min
Delta R.T.: -0.008 min
Response: 1035
Conc: 0.69 ng/ml

Instrument :
ECD_O
ClientSampleId :
SES-GODWIN-PUMP-082019

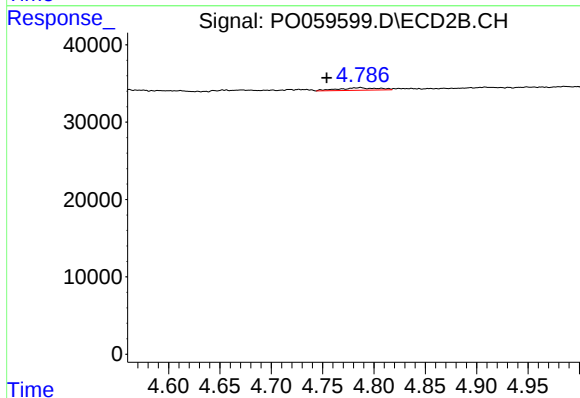


#5 AR-1016-3

R.T.: 4.787 min
Delta R.T.: 0.033 min
Response: 8959
Conc: 8.28 ng/ml

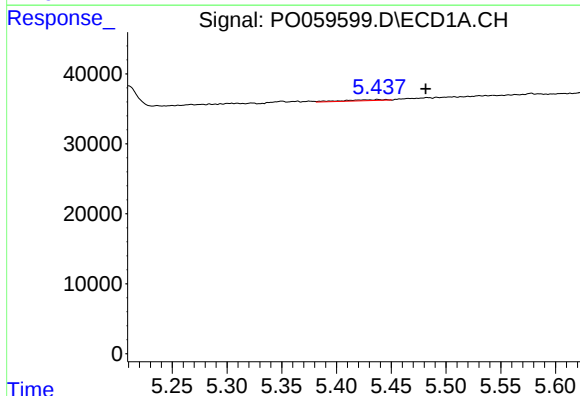


#6 AR-1016-4

R.T.: 5.438 min
Delta R.T.: -0.044 min
Response: 6087
Conc: 5.03 ng/ml

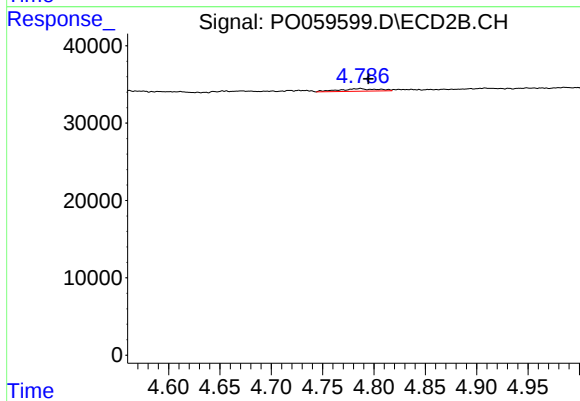

#6 AR-1016-4


R.T.: 4.787 min
Delta R.T.: -0.008 min
Response: 8959
Conc: 9.92 ng/ml

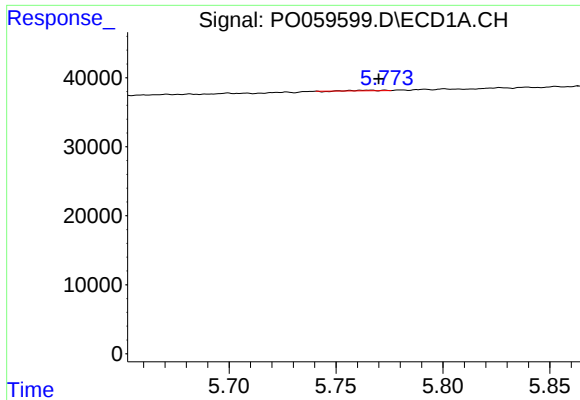

#7 AR-1016-5


R.T.: 5.765 min
Delta R.T.: -0.004 min
Response: 480
Conc: 0.37 ng/ml

Instrument :
ECD_O
ClientSampleId :
SES-GODWIN-PUMP-082019

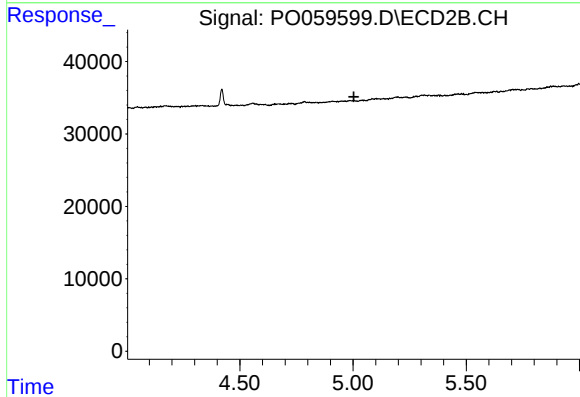


#7 AR-1016-5

R.T.: 0.000 min
Exp R.T. : 5.004 min
Response: 0
Conc: N.D.

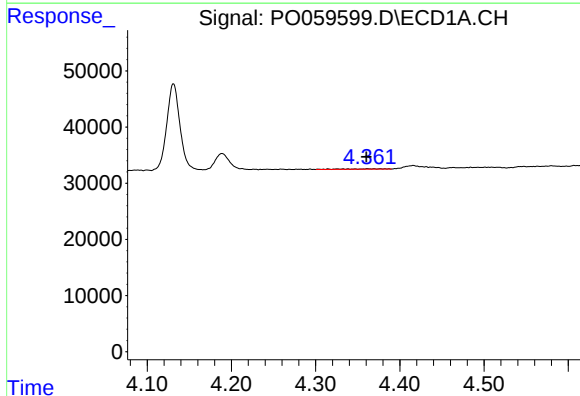


#8 AR-1221-1

R.T.: 4.362 min
Delta R.T.: 0.002 min
Response: 2076
Conc: 4.90 ng/ml

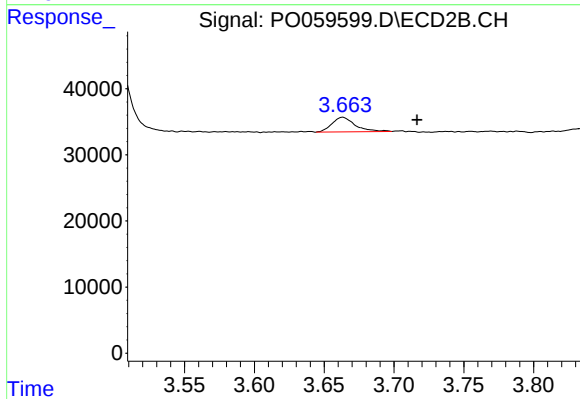

#8 AR-1221-1


R.T.: 3.663 min
Delta R.T.: -0.053 min
Response: 25615
Conc: 63.82 ng/ml

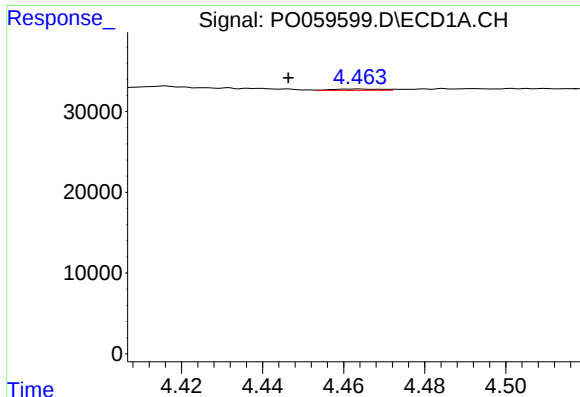

#9 AR-1221-2


R.T.: 4.463 min
Delta R.T.: 0.017 min
Response: 1383
Conc: 4.26 ng/ml

Instrument :
ECD_O
ClientSampleId :
SES-GODWIN-PUMP-082019

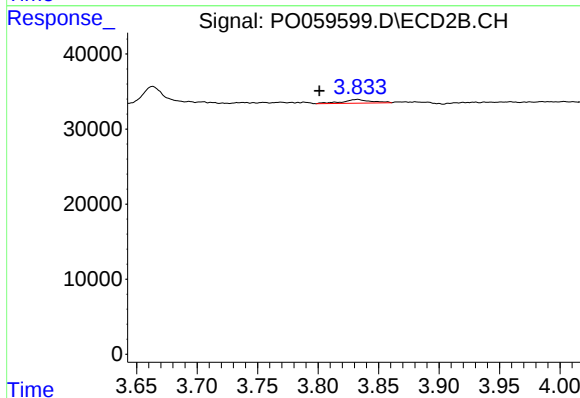


#9 AR-1221-2

R.T.: 3.833 min
Delta R.T.: 0.032 min
Response: 8060
Conc: 26.46 ng/ml

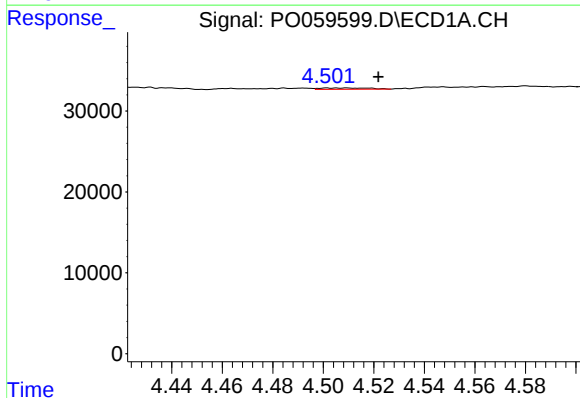


#10 AR-1221-3

R.T.: 4.509 min
Delta R.T.: -0.013 min
Response: 2192
Conc: 2.08 ng/ml

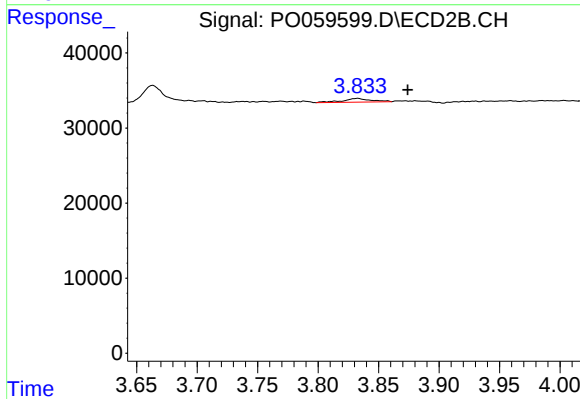

#10 AR-1221-3


R.T.: 3.833 min
Delta R.T.: -0.041 min
Response: 8060
Conc: 8.24 ng/ml

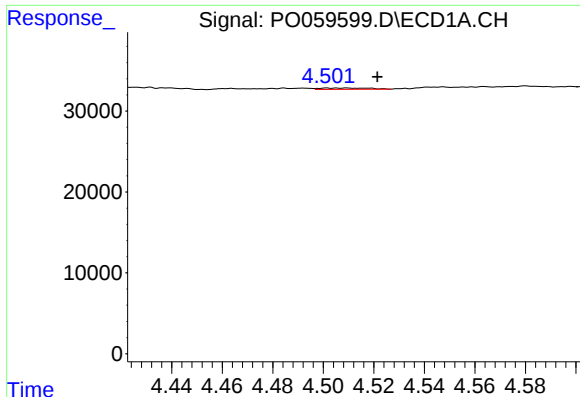

#11 AR-1232-1


R.T.: 4.509 min
Delta R.T.: -0.012 min
Response: 2192
Conc: 1.76 ng/ml

Instrument :
ECD_O
ClientSampleId :
SES-GODWIN-PUMP-082019

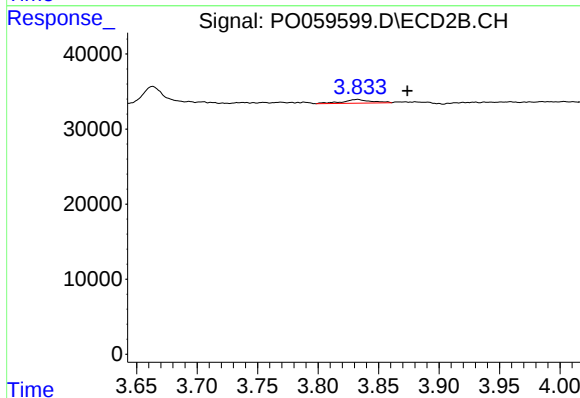


#11 AR-1232-1

R.T.: 3.833 min
Delta R.T.: -0.041 min
Response: 8060
Conc: 7.07 ng/ml

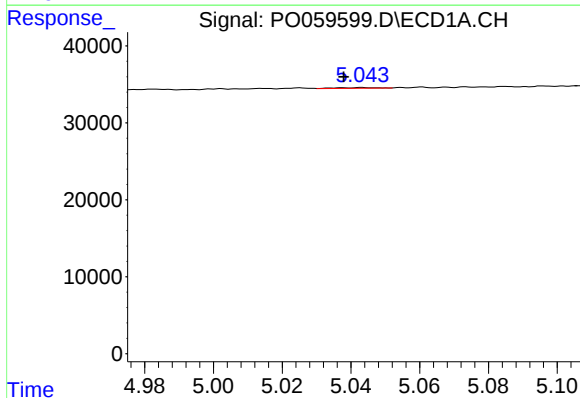


#12 AR-1232-2

R.T.: 5.043 min
Delta R.T.: 0.006 min
Response: 778
Conc: 1.10 ng/ml

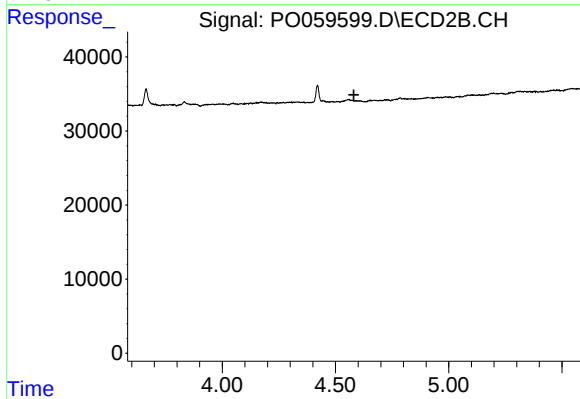

#12 AR-1232-2


R.T.: 0.000 min
Exp R.T.: 4.581 min
Response: 0
Conc: N.D.

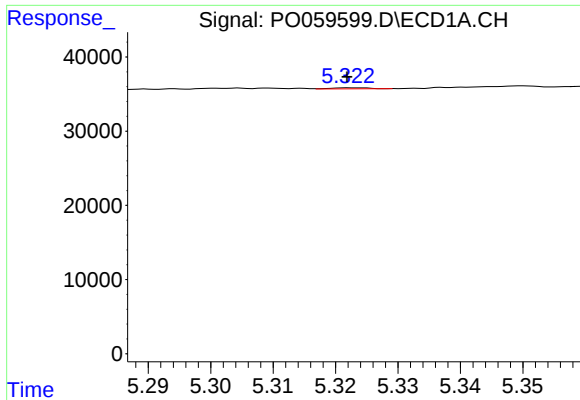

#13 AR-1232-3


R.T.: 5.323 min
Delta R.T.: 0.001 min
Response: 601
Conc: 0.39 ng/ml

Instrument :
ECD_O
ClientSampleId :
SES-GODWIN-PUMP-082019

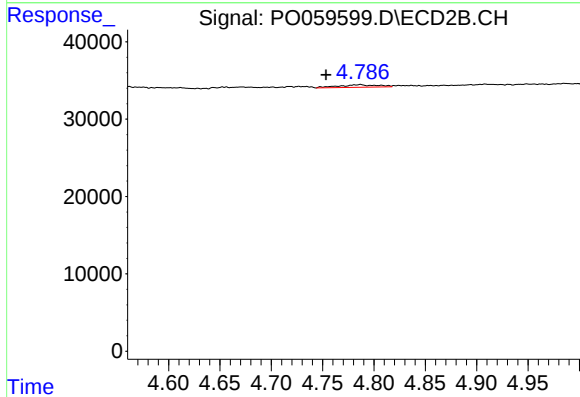


#13 AR-1232-3

R.T.: 4.787 min
Delta R.T.: 0.033 min
Response: 8959
Conc: 13.16 ng/ml

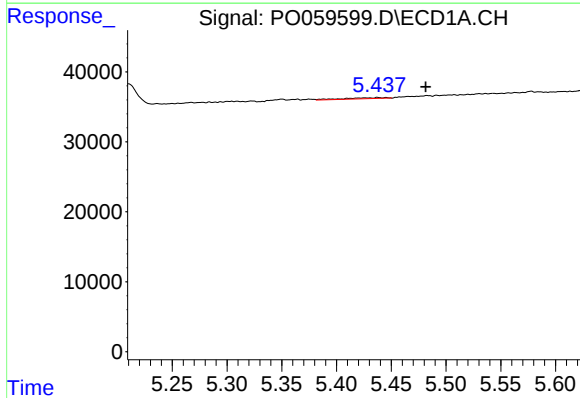


#14 AR-1232-4

R.T.: 5.438 min
Delta R.T.: -0.044 min
Response: 6087
Conc: 7.79 ng/ml

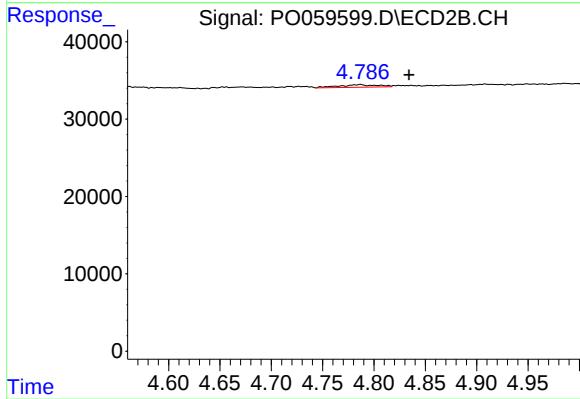

#14 AR-1232-4


R.T.: 4.787 min
Delta R.T.: -0.048 min
Response: 8959
Conc: 14.69 ng/ml

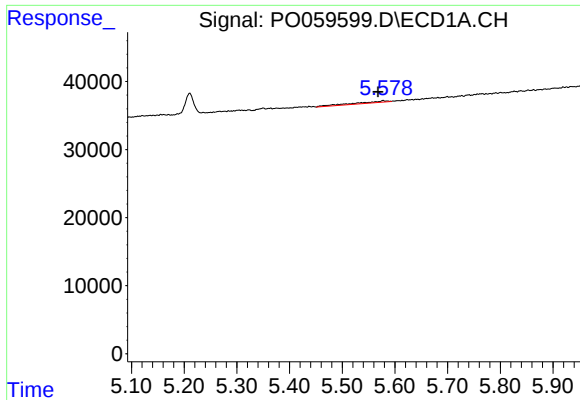

#15 AR-1232-5


R.T.: 5.578 min
Delta R.T.: 0.010 min
Response: 9845
Conc: 16.38 ng/ml

Instrument :
ECD_O
ClientSampleId :
SES-GODWIN-PUMP-082019

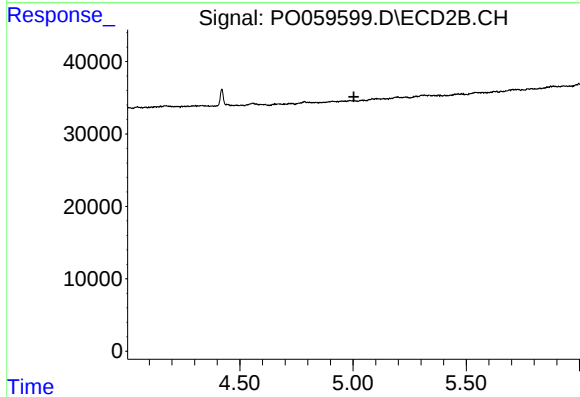


#15 AR-1232-5

R.T.: 0.000 min
Exp R.T. : 5.004 min
Response: 0
Conc: N.D.

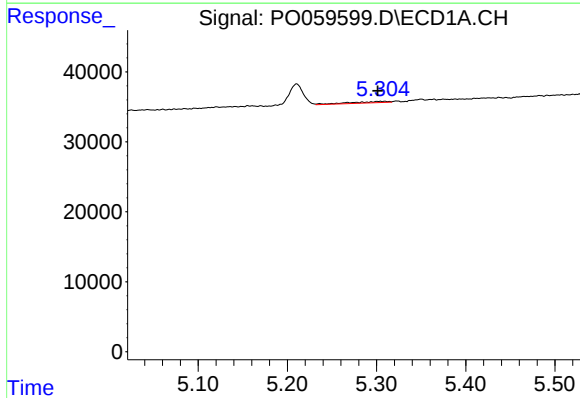


#16 AR-1242-1

R.T.: 5.309 min
Delta R.T.: 0.008 min
Response: 5469
Conc: 4.31 ng/ml

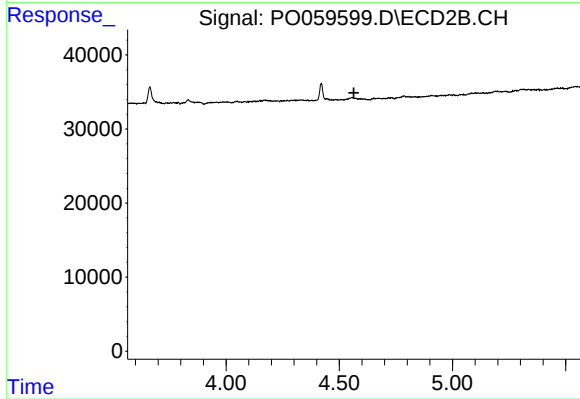

#16 AR-1242-1


R.T.: 0.000 min
Exp R.T. : 4.564 min
Response: 0
Conc: N.D.

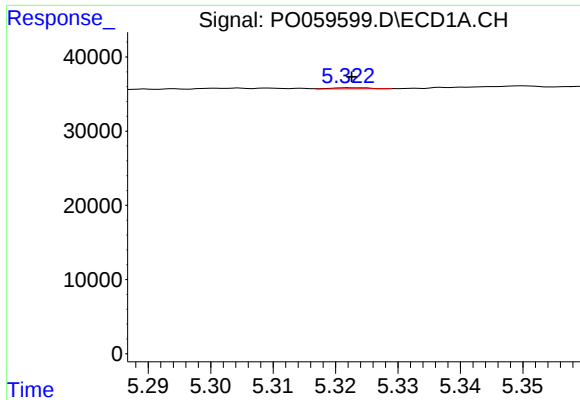

#17 AR-1242-2


R.T.: 5.323 min
Delta R.T.: 0.000 min
Response: 601
Conc: 0.32 ng/ml

Instrument :
ECD_O
ClientSampleId :
SES-GODWIN-PUMP-082019

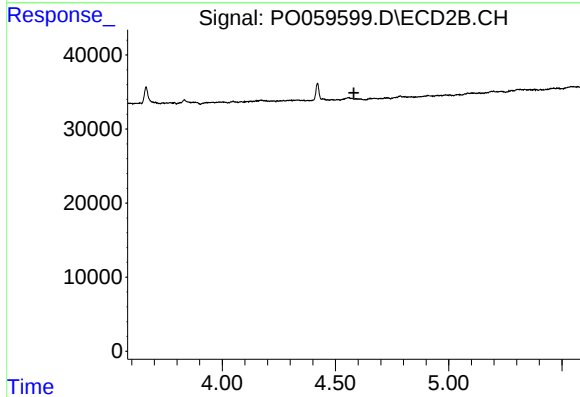


#17 AR-1242-2

R.T.: 0.000 min
Exp R.T. : 4.581 min
Response: 0
Conc: N.D.

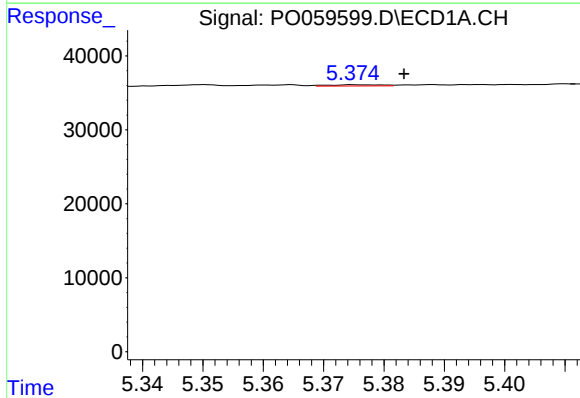


#18 AR-1242-3

R.T.: 5.376 min
Delta R.T.: -0.008 min
Response: 1035
Conc: 0.89 ng/ml

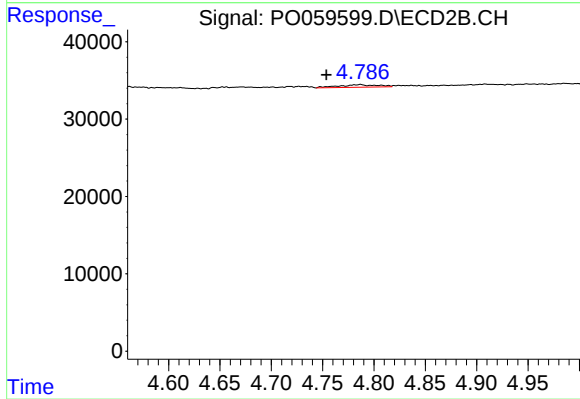

#18 AR-1242-3


R.T.: 4.787 min
Delta R.T.: 0.033 min
Response: 8959
Conc: 10.72 ng/ml

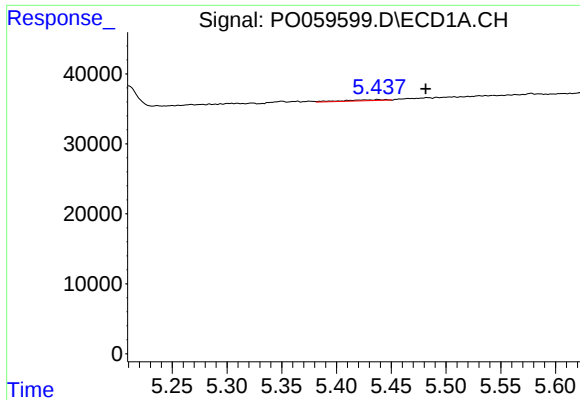

#19 AR-1242-4


R.T.: 5.438 min
Delta R.T.: -0.044 min
Response: 6087
Conc: 6.29 ng/ml

Instrument :
ECD_O
ClientSampleId :
SES-GODWIN-PUMP-082019

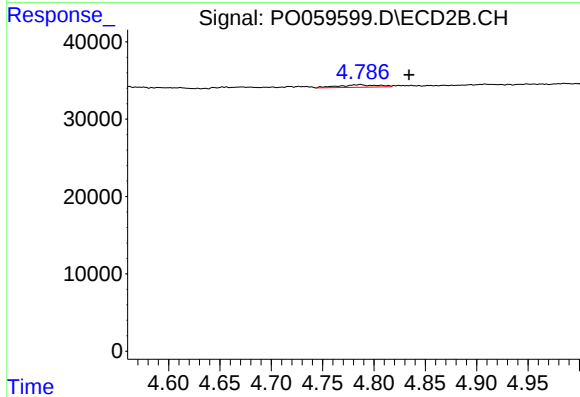


#19 AR-1242-4

R.T.: 4.787 min
Delta R.T.: -0.047 min
Response: 8959
Conc: 10.74 ng/ml

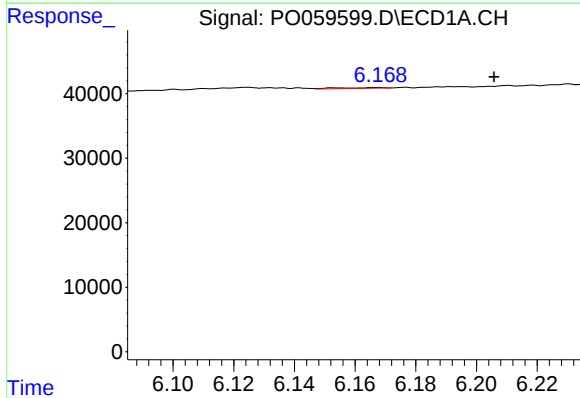


#20 AR-1242-5

R.T.: 6.167 min
Delta R.T.: -0.039 min
Response: 1407
Conc: 1.12 ng/ml

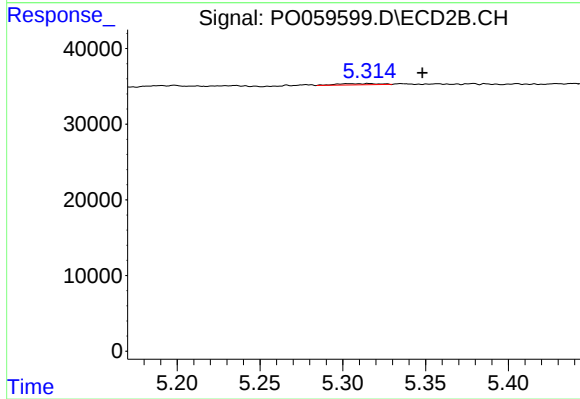

#20 AR-1242-5


R.T.: 5.316 min
Delta R.T.: -0.032 min
Response: 2999
Conc: 2.68 ng/ml

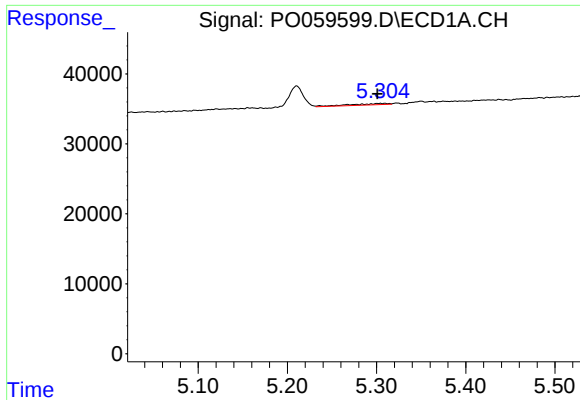

#21 AR-1248-1


R.T.: 5.309 min
Delta R.T.: 0.008 min
Response: 5469
Conc: 5.46 ng/ml

Instrument :
ECD_O
ClientSampleId :
SES-GODWIN-PUMP-082019

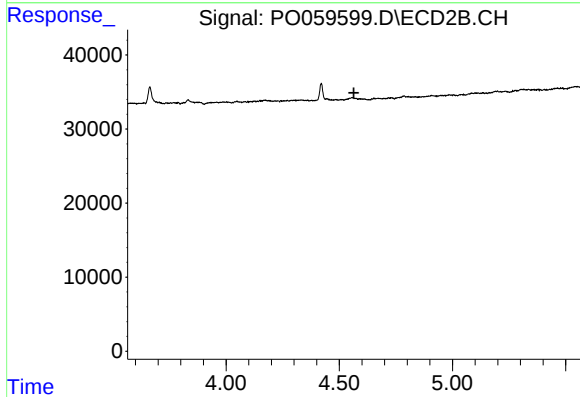


#21 AR-1248-1

R.T.: 0.000 min
Exp R.T. : 4.564 min
Response: 0
Conc: N.D.

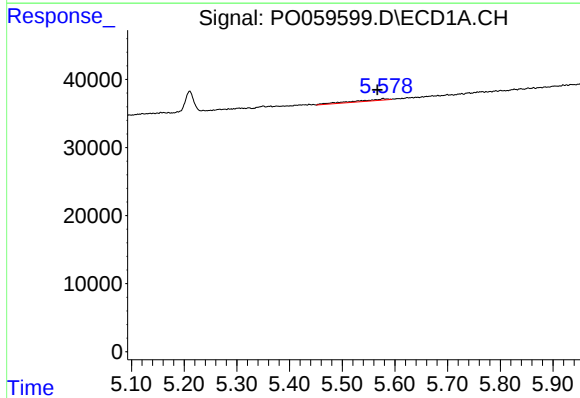


#22 AR-1248-2

R.T.: 5.578 min
Delta R.T.: 0.010 min
Response: 9845
Conc: 6.79 ng/ml

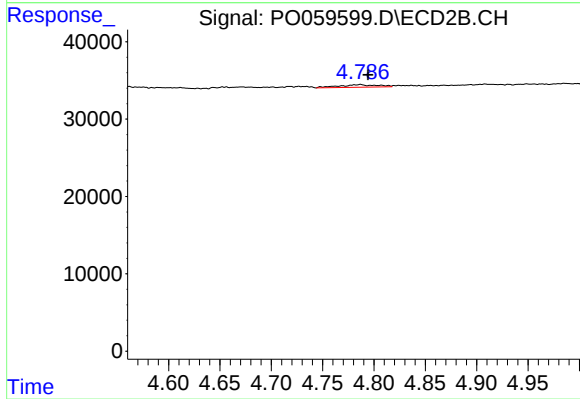

#22 AR-1248-2


R.T.: 4.787 min
Delta R.T.: -0.007 min
Response: 8959
Conc: 7.77 ng/ml

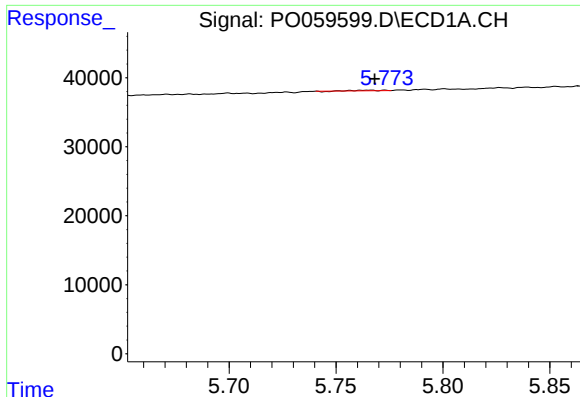

#23 AR-1248-3


R.T.: 5.765 min
Delta R.T.: -0.003 min
Response: 480
Conc: 0.29 ng/ml

Instrument :
ECD_O
ClientSampleId :
SES-GODWIN-PUMP-082019

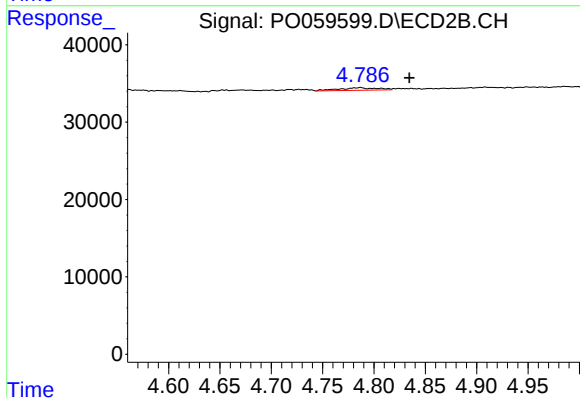


#23 AR-1248-3

R.T.: 4.787 min
Delta R.T.: -0.048 min
Response: 8959
Conc: 7.54 ng/ml

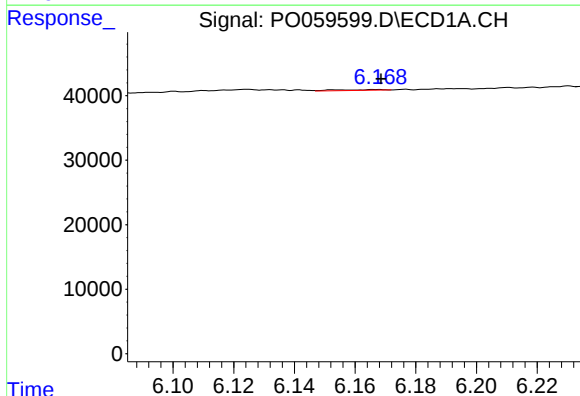


#24 AR-1248-4

R.T.: 6.167 min
Delta R.T.: -0.002 min
Response: 1407
Conc: 0.69 ng/ml

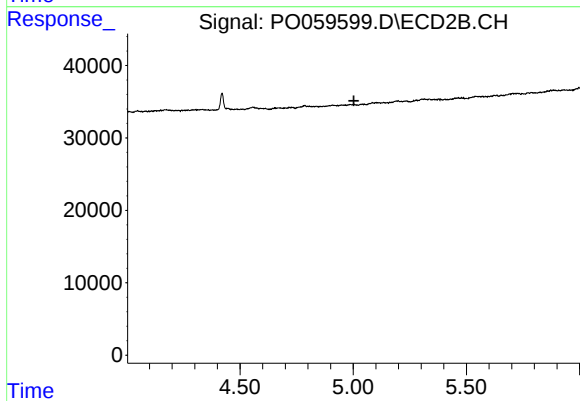

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T.: 5.003 min
Response: 0
Conc: N.D.

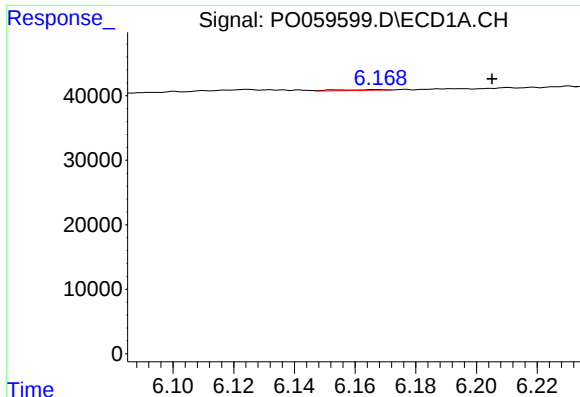

#25 AR-1248-5


R.T.: 6.167 min
Delta R.T.: -0.038 min
Response: 1407
Conc: 0.71 ng/ml

Instrument :
ECD_O
ClientSampleId :
SES-GODWIN-PUMP-082019

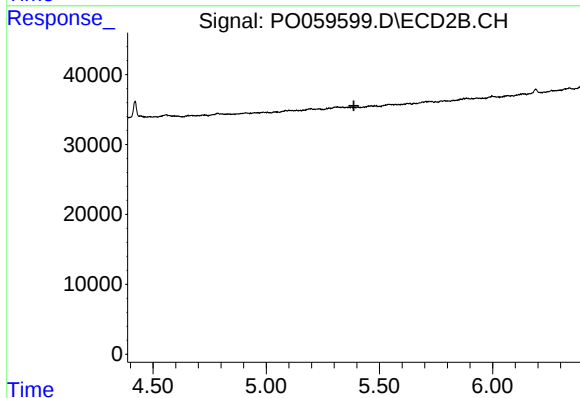


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T. : 5.387 min
Response: 0
Conc: N.D.

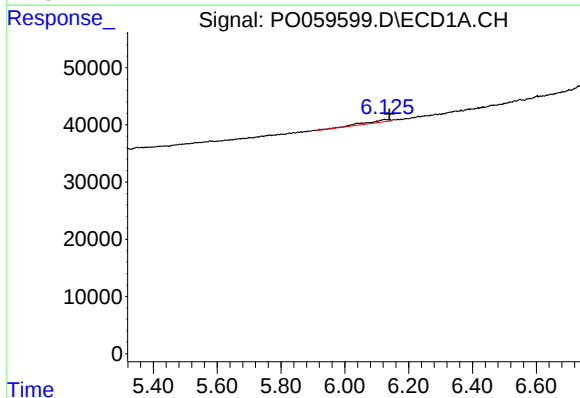


#26 AR-1254-1

R.T.: 6.125 min
Delta R.T.: -0.015 min
Response: 22767
Conc: 10.91 ng/ml

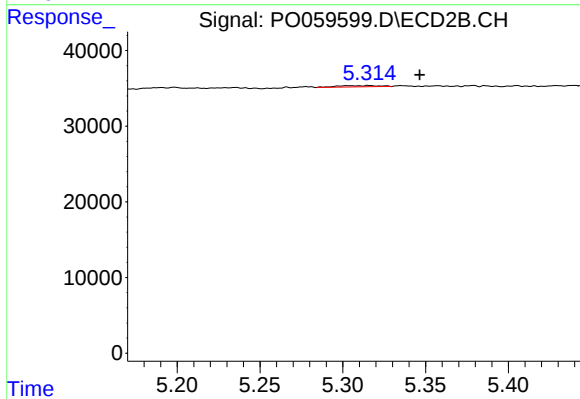

#26 AR-1254-1


R.T.: 5.316 min
Delta R.T.: -0.031 min
Response: 2999
Conc: 1.26 ng/ml

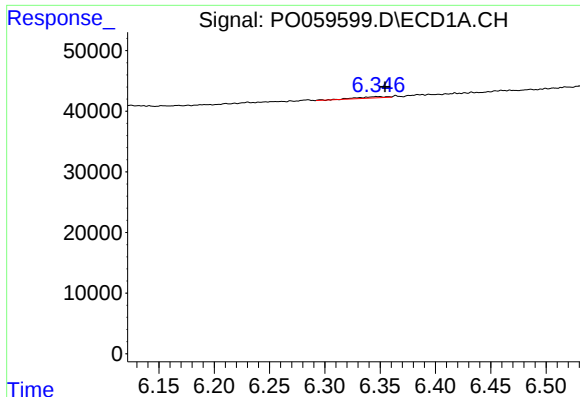

#27 AR-1254-2


R.T.: 6.348 min
Delta R.T.: -0.007 min
Response: 4353
Conc: 1.30 ng/ml

Instrument :
ECD_O
ClientSampleId :
SES-GODWIN-PUMP-082019

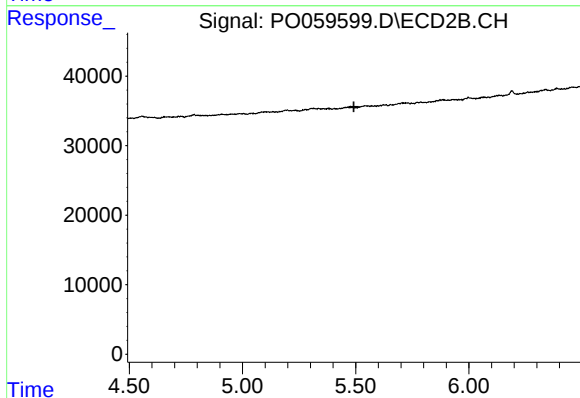


#27 AR-1254-2

R.T.: 0.000 min
Exp R.T. : 5.492 min
Response: 0
Conc: N.D.

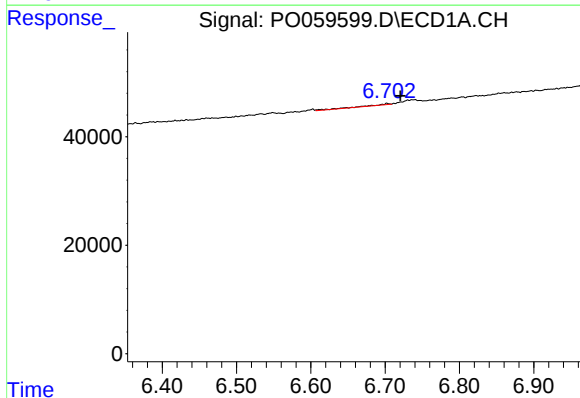


#28 AR-1254-3

R.T.: 6.703 min
Delta R.T.: -0.018 min
Response: 4887
Conc: 1.38 ng/ml

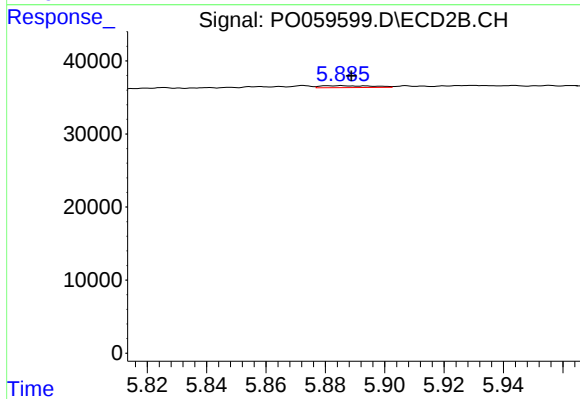

#28 AR-1254-3


R.T.: 5.885 min
Delta R.T.: -0.004 min
Response: 3114
Conc: 0.93 ng/ml

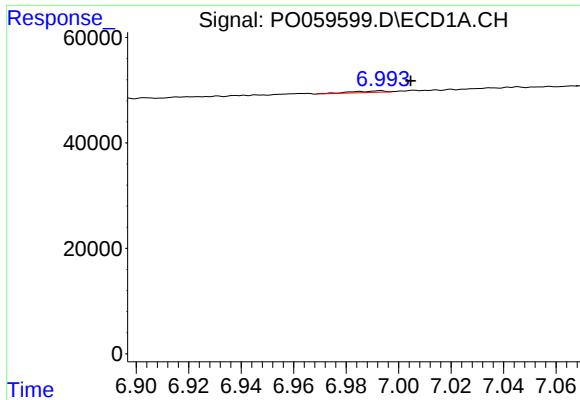

#29 AR-1254-4


R.T.: 6.993 min
Delta R.T.: -0.012 min
Response: 2632
Conc: 0.89 ng/ml

Instrument :
ECD_O
ClientSampleId :
SES-GODWIN-PUMP-082019

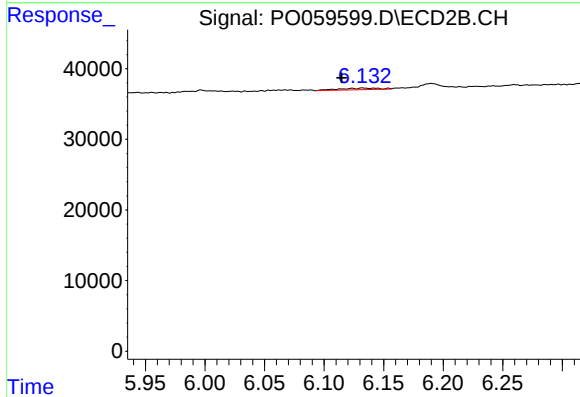


#29 AR-1254-4

R.T.: 6.133 min
Delta R.T.: 0.018 min
Response: 5271
Conc: 2.56 ng/ml

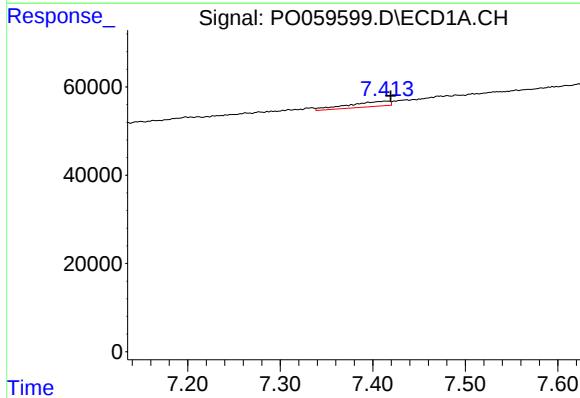


#30 AR-1254-5

R.T.: 7.414 min
Delta R.T.: -0.005 min
Response: 36281
Conc: 11.73 ng/ml

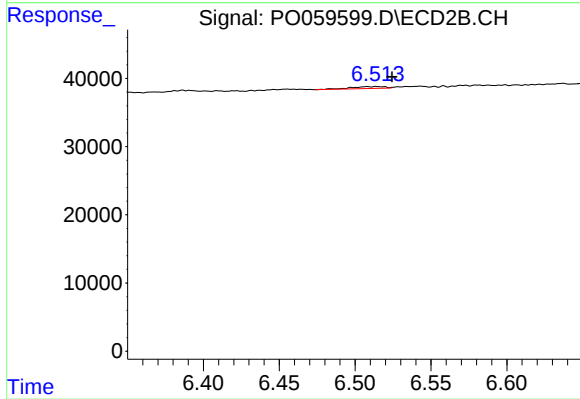

#30 AR-1254-5


R.T.: 6.514 min
Delta R.T.: -0.010 min
Response: 4510
Conc: 1.45 ng/ml

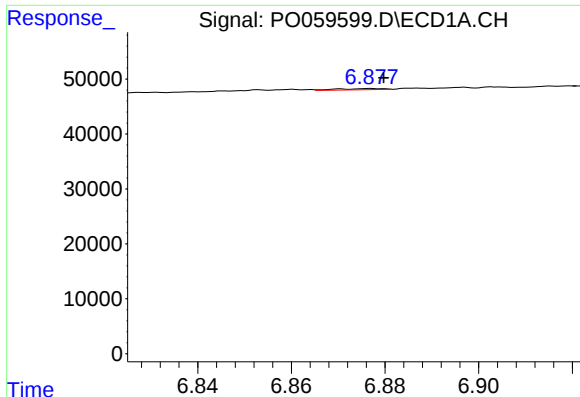

#31 AR-1260-1


R.T.: 6.877 min
Delta R.T.: -0.002 min
Response: 1464
Conc: 0.54 ng/ml

Instrument :
ECD_O
ClientSampleId :
SES-GODWIN-PUMP-082019

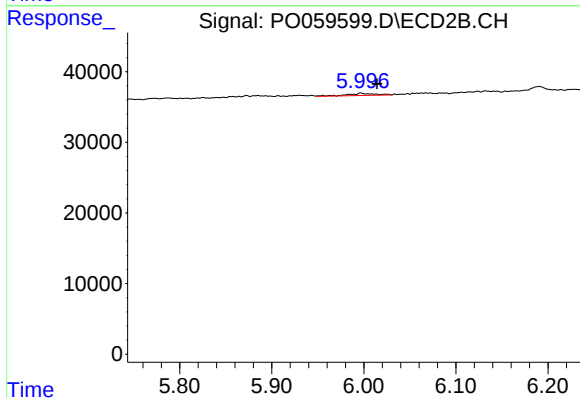


#31 AR-1260-1

R.T.: 5.997 min
Delta R.T.: -0.017 min
Response: 6742
Conc: 2.96 ng/ml

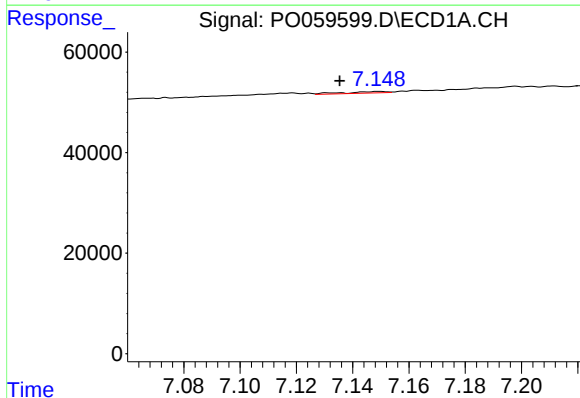


#32 AR-1260-2

R.T.: 7.150 min
Delta R.T.: 0.014 min
Response: 3054
Conc: 0.82 ng/ml

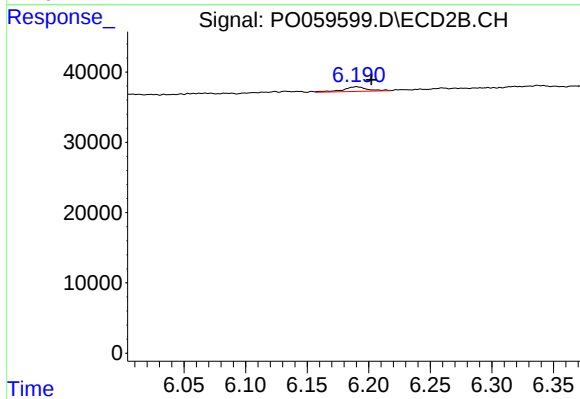

#32 AR-1260-2


R.T.: 6.190 min
Delta R.T.: -0.012 min
Response: 9240
Conc: 3.15 ng/ml

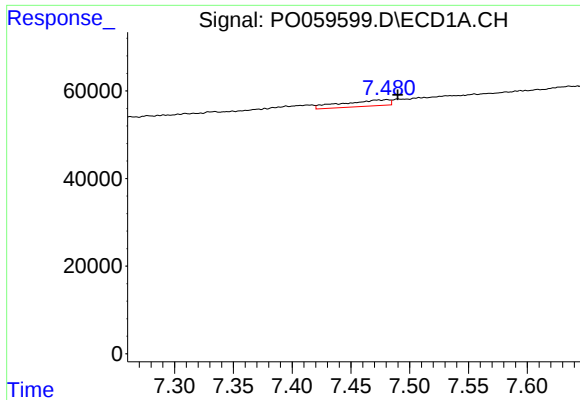

#33 AR-1260-3


R.T.: 7.481 min
Delta R.T.: -0.009 min
Response: 39590
Conc: 12.08 ng/ml

Instrument :
ECD_O
ClientSampleId :
SES-GODWIN-PUMP-082019

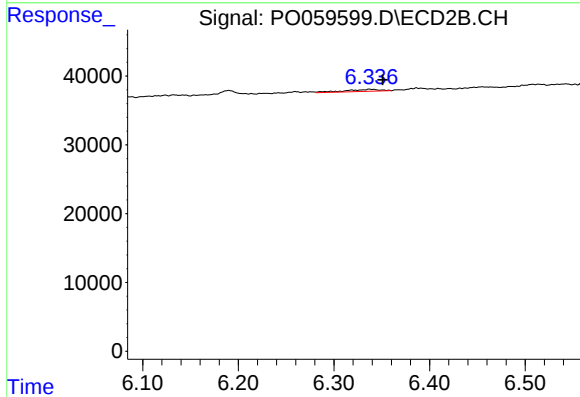


#33 AR-1260-3

R.T.: 6.337 min
Delta R.T.: -0.014 min
Response: 7497
Conc: 2.83 ng/ml

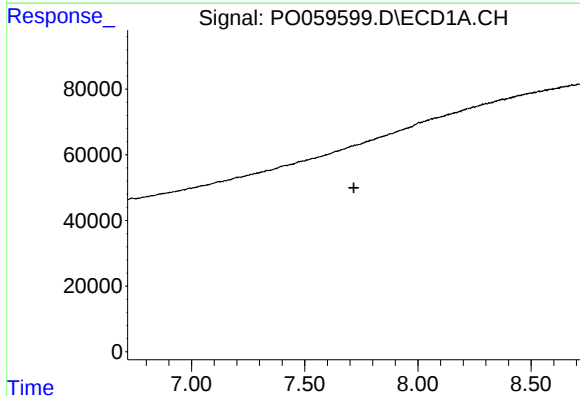


#34 AR-1260-4

R.T.: 0.000 min
Exp R.T. : 7.717 min
Response: 0
Conc: N.D.

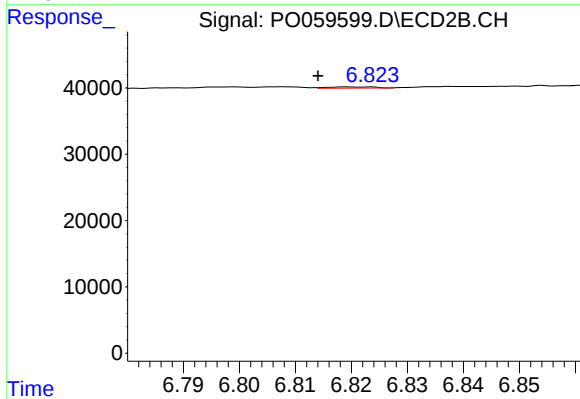

#34 AR-1260-4


R.T.: 6.820 min
Delta R.T.: 0.006 min
Response: 1057
Conc: 0.47 ng/ml

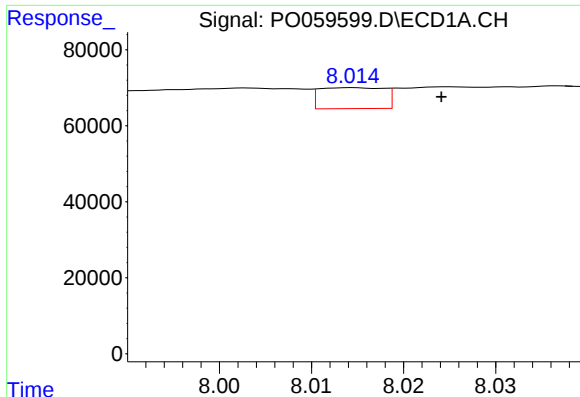

#35 AR-1260-5


R.T.: 8.014 min
Delta R.T.: -0.010 min
Response: 26779
Conc: 3.78 ng/ml

Instrument :
ECD_O
ClientSampleId :
SES-GODWIN-PUMP-082019

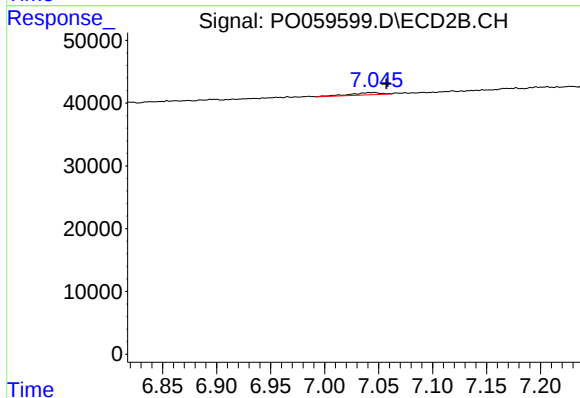


#35 AR-1260-5

R.T.: 7.046 min
Delta R.T.: -0.011 min
Response: 7284
Conc: 1.32 ng/ml

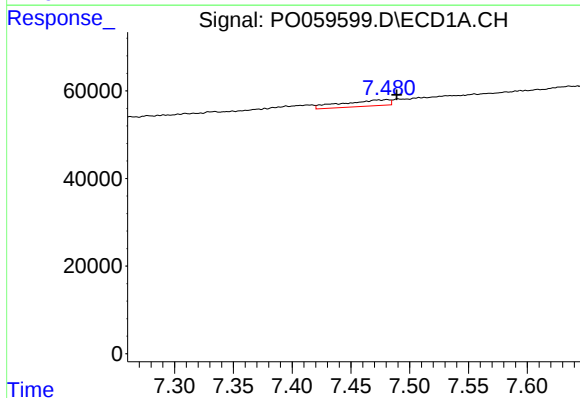


#36 AR-1262-1

R.T.: 7.481 min
Delta R.T.: -0.008 min
Response: 39590
Conc: 8.16 ng/ml

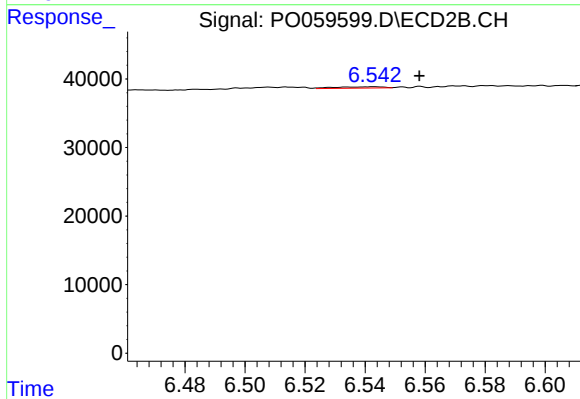

#36 AR-1262-1


R.T.: 6.543 min
Delta R.T.: -0.015 min
Response: 2208
Conc: 0.59 ng/ml

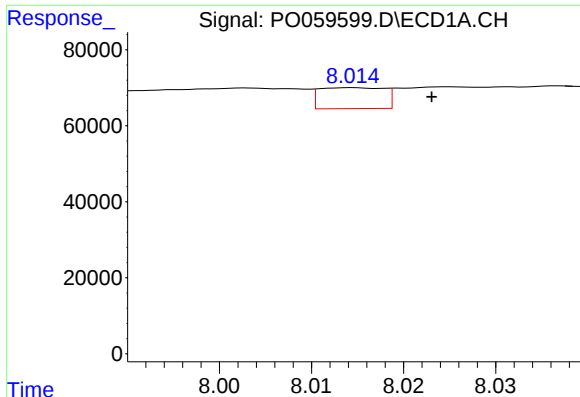

#37 AR-1262-2


R.T.: 8.014 min
Delta R.T.: -0.009 min
Response: 26779
Conc: 3.47 ng/ml

Instrument :
ECD_O
ClientSampleId :
SES-GODWIN-PUMP-082019

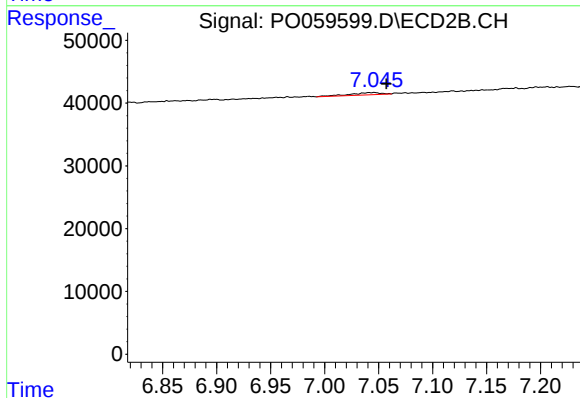


#37 AR-1262-2

R.T.: 7.046 min
Delta R.T.: -0.011 min
Response: 7284
Conc: 1.24 ng/ml

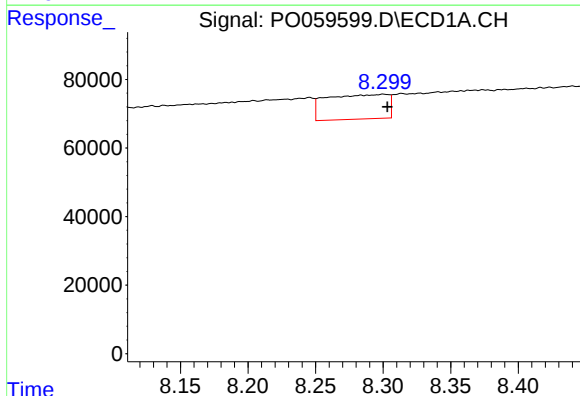


#38 AR-1262-3

R.T.: 8.300 min
Delta R.T.: -0.003 min
Response: 227462
Conc: 44.58 ng/ml

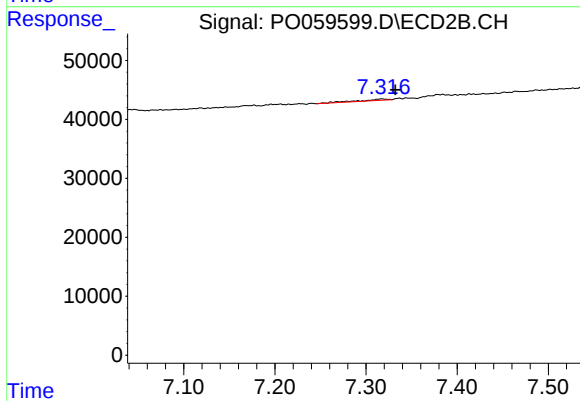

#38 AR-1262-3


R.T.: 7.317 min
Delta R.T.: -0.015 min
Response: 5557
Conc: 2.19 ng/ml

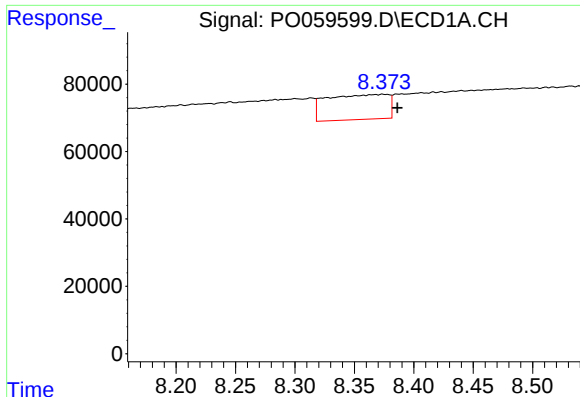

#39 AR-1262-4


R.T.: 8.374 min
Delta R.T.: -0.012 min
Response: 267189
Conc: 69.31 ng/ml

Instrument :
ECD_O
ClientSampleId :
SES-GODWIN-PUMP-082019

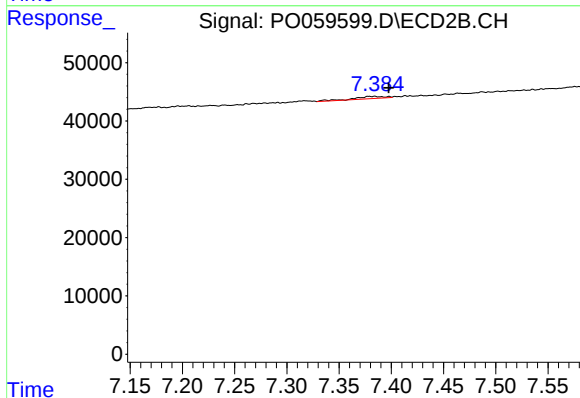


#39 AR-1262-4

R.T.: 7.384 min
Delta R.T.: -0.014 min
Response: 7842
Conc: 1.77 ng/ml

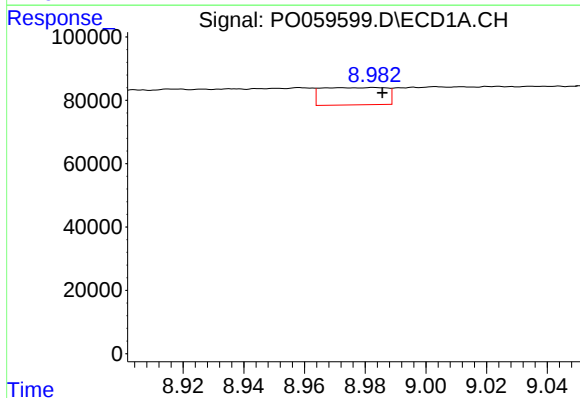


#40 AR-1262-5

R.T.: 8.983 min
Delta R.T.: -0.003 min
Response: 80463
Conc: 31.35 ng/ml

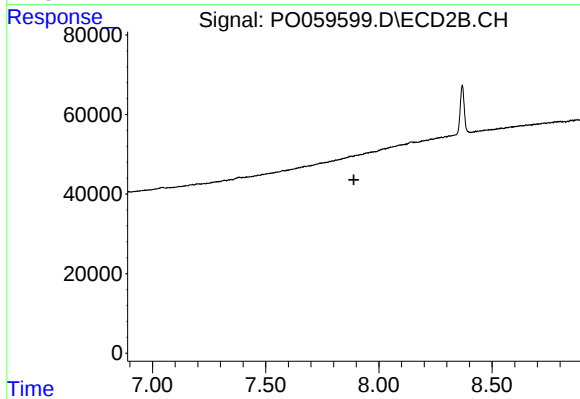

#40 AR-1262-5


R.T.: 0.000 min
Exp R.T.: 7.889 min
Response: 0
Conc: N.D.

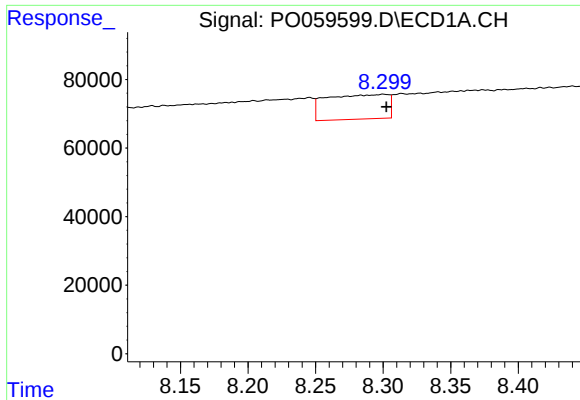

#41 AR-1268-1


R.T.: 8.300 min
Delta R.T.: -0.002 min
Response: 227462
Conc: 24.17 ng/ml

Instrument :
ECD_O
ClientSampleId :
SES-GODWIN-PUMP-082019

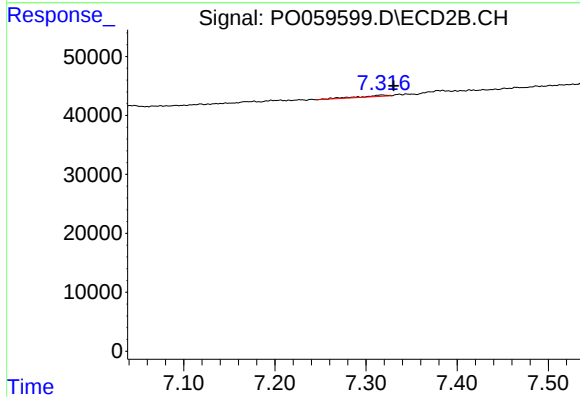


#41 AR-1268-1

R.T.: 7.317 min
Delta R.T.: -0.013 min
Response: 5557
Conc: 0.78 ng/ml

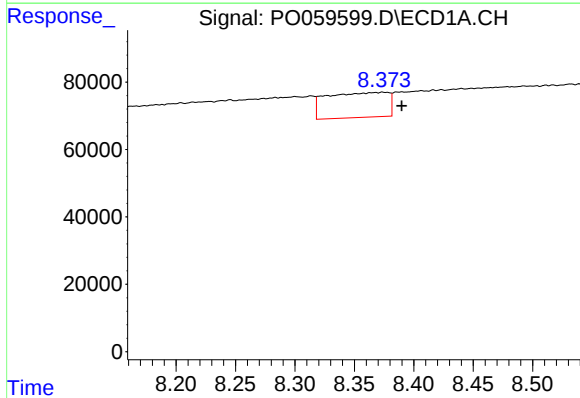


#42 AR-1268-2

R.T.: 8.374 min
Delta R.T.: -0.016 min
Response: 267189
Conc: 33.90 ng/ml

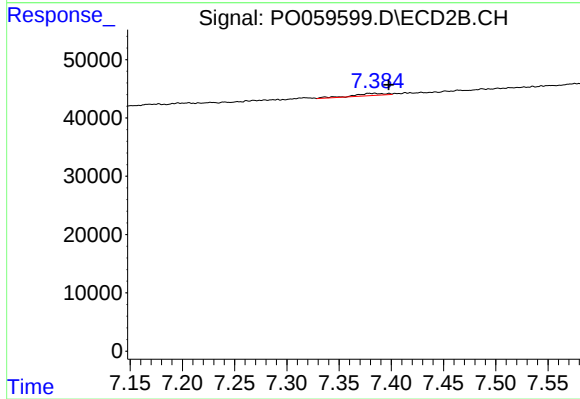

#42 AR-1268-2


R.T.: 7.384 min
Delta R.T.: -0.013 min
Response: 7842
Conc: 1.22 ng/ml

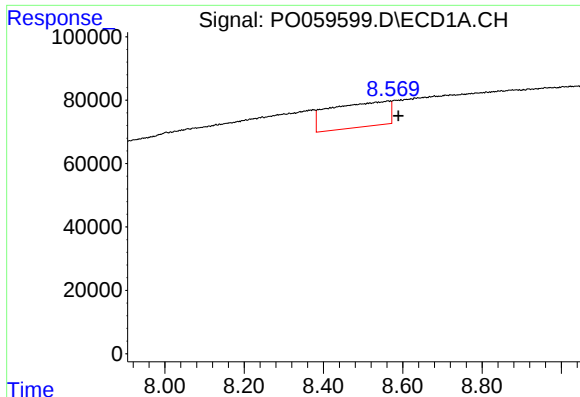

#43 AR-1268-3


R.T.: 8.562 min
Delta R.T.: -0.027 min
Response: 818933
Conc: 116.18 ng/ml

Instrument :
ECD_O
ClientSampleId :
SES-GODWIN-PUMP-082019

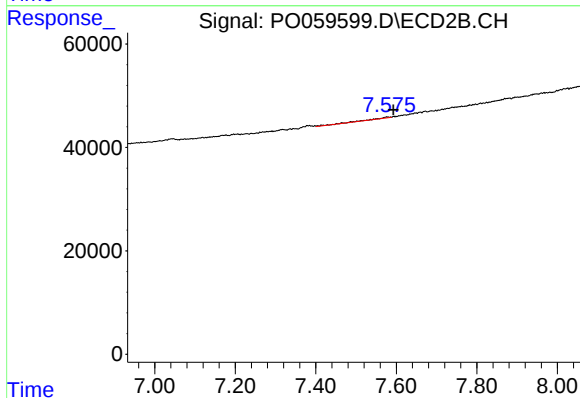


#43 AR-1268-3

R.T.: 7.576 min
Delta R.T.: -0.016 min
Response: 7142
Conc: 1.31 ng/ml

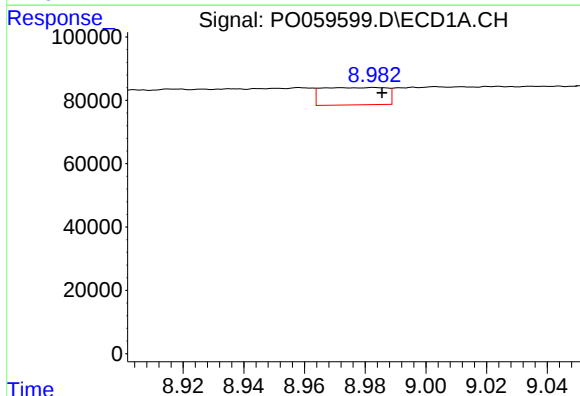


#44 AR-1268-4

R.T.: 8.983 min
Delta R.T.: -0.003 min
Response: 80463
Conc: 28.94 ng/ml

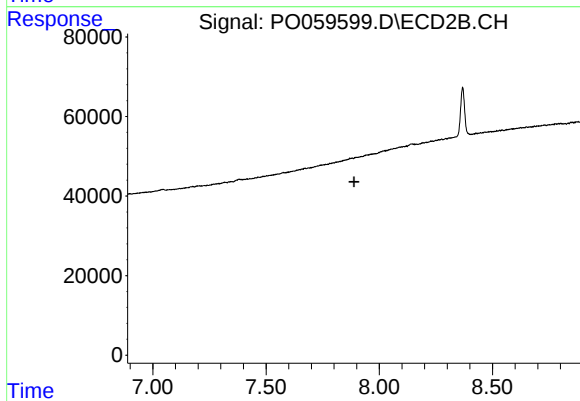

#44 AR-1268-4


R.T.: 0.000 min
Exp R.T.: 7.888 min
Response: 0
Conc: N.D.

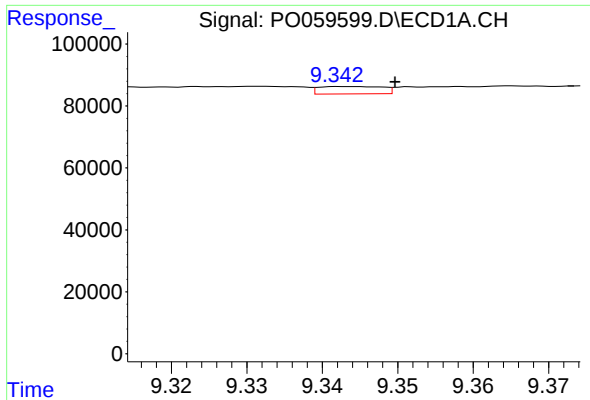

#45 AR-1268-5

R.T.: 9.344 min
Delta R.T.: -0.006 min
Response: 13853
Conc: 0.75 ng/ml

Instrument :
ECD_O
ClientSampleId :
SES-GODWIN-PUMP-082019

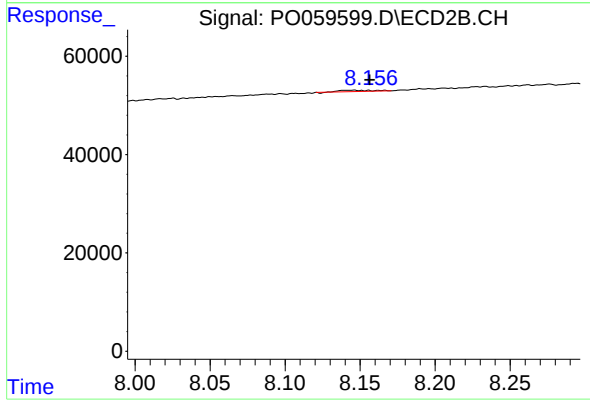

#45 AR-1268-5

R.T.: 8.145 min
Delta R.T.: -0.011 min
Response: 4120
Conc: 0.28 ng/ml