

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082119\
 Data File : P0059576.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Aug 2019 9:50
 Operator : SM/AJ
 Sample : K4400-03
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 HA-15

Manual Integrations
 APPROVED

Ankita
 8/22/2019 3:32:42 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 21 14:42:40 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 17 03:09:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.134	3.501	891876	838820	25.473	23.303
2) SA Decachlor...	9.617	8.368	1355361	998012	25.477	24.752m
Target Compounds						
26) L6 AR-1254-1	6.123	5.335	286437	316181	137.287m	133.308
27) L6 AR-1254-2	6.340	5.480	480720	277518	144.090	132.258
28) L6 AR-1254-3	6.706	5.875	535629	521016	150.947	154.949
29) L6 AR-1254-4	6.989	6.102	472573	341691	160.437	165.722
30) L6 AR-1254-5	7.404	6.511	604610	688950	195.515m	221.886

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO082119\
Data File : PO059576.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Aug 2019 9:50
Operator : SM/AJ
Sample : K4400-03
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
HA-15


Manual Integrations
APPROVED

Ankita
8/22/2019 3:32:42 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 14:42:40 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Aug 17 03:09:44 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

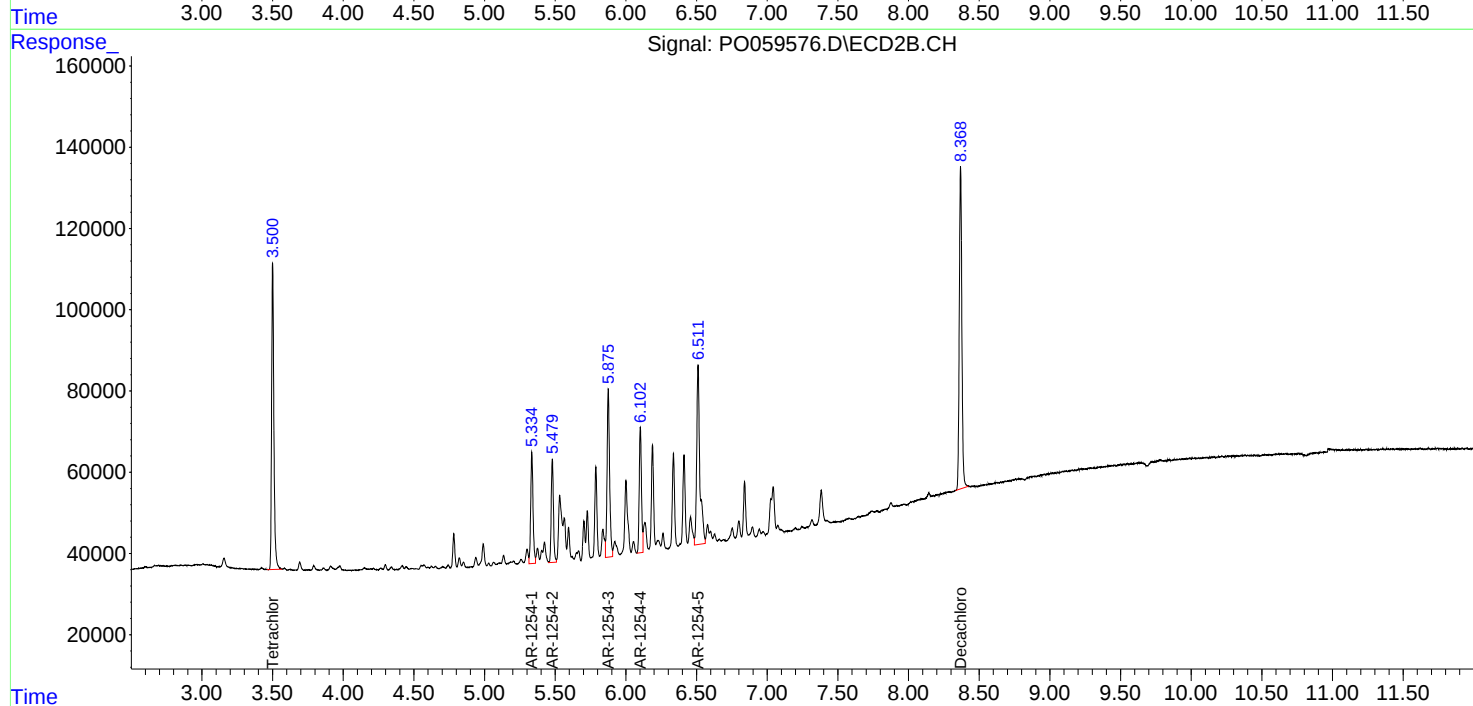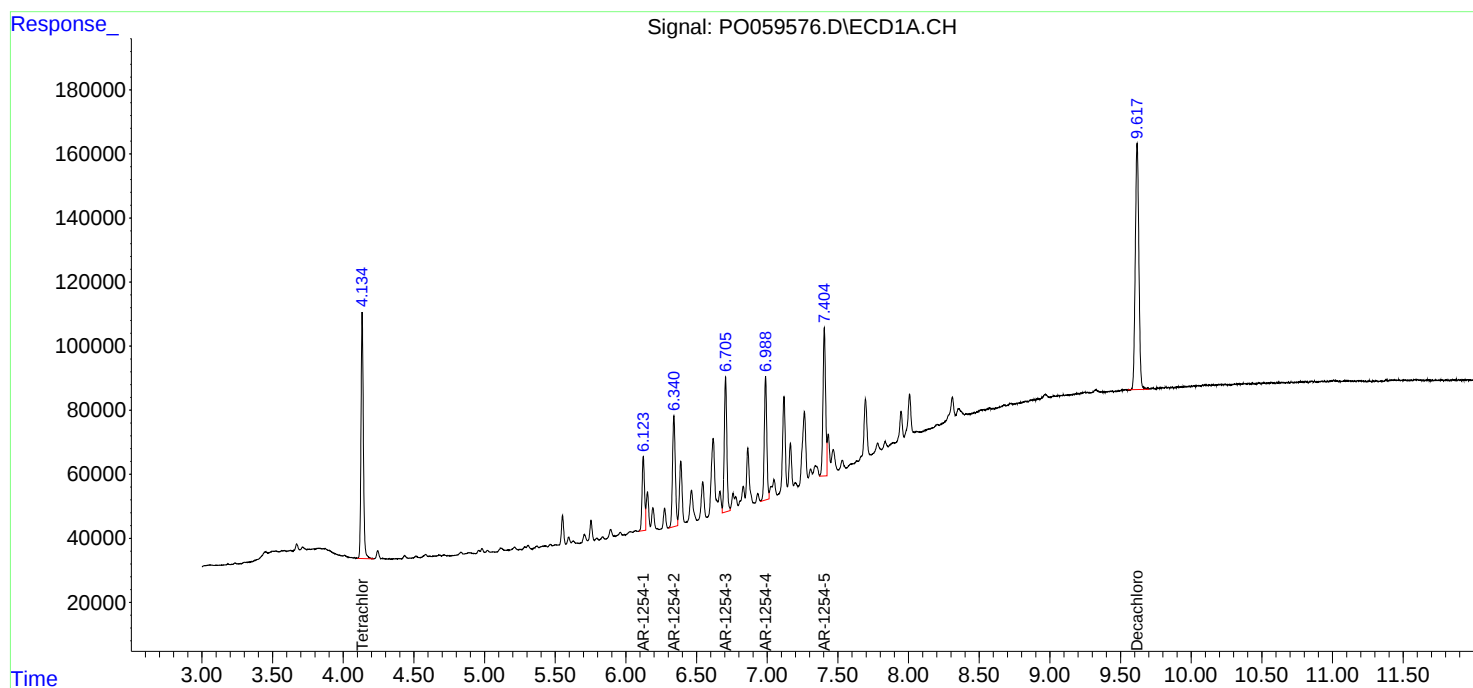

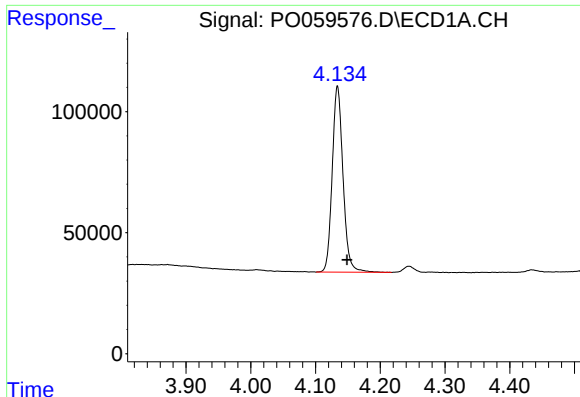


#1 Tetrachloro-m-xylene

R.T.: 4.134 min
Delta R.T.: -0.015 min
Response: 891876
Conc: 25.47 ng/ml

Instrument :
ECD_O
ClientSampleId :
HA-15


Manual Integrations
APPROVED

Ankita
8/22/2019 3:32:42 PM

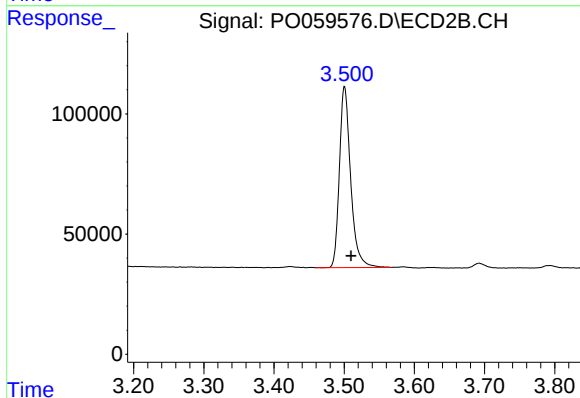


#1 Tetrachloro-m-xylene

R.T.: 3.501 min
Delta R.T.: -0.009 min
Response: 838820
Conc: 23.30 ng/ml

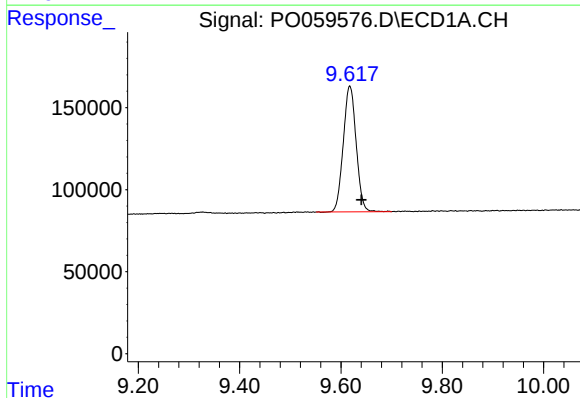


#2 Decachlorobiphenyl

R.T.: 9.617 min
Delta R.T.: -0.023 min
Response: 1355361
Conc: 25.48 ng/ml

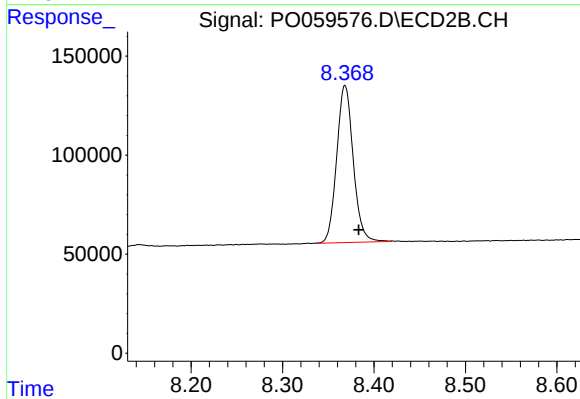

#2 Decachlorobiphenyl

R.T.: 8.368 min
Delta R.T.: -0.016 min
Response: 998012
Conc: 24.75 ng/ml m

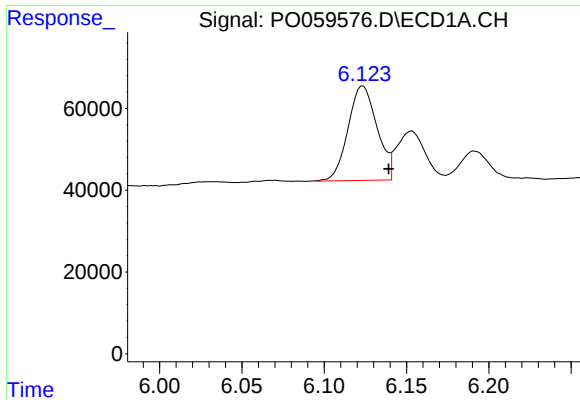


#26 AR-1254-1

R.T.: 6.123 min
Delta R.T.: -0.016 min
Response: 286437
Conc: 137.29 ng/ml m

Instrument :
ECD_O
ClientSampleId :
HA-15


Manual Integrations
APPROVED

Ankita
8/22/2019 3:32:42 PM

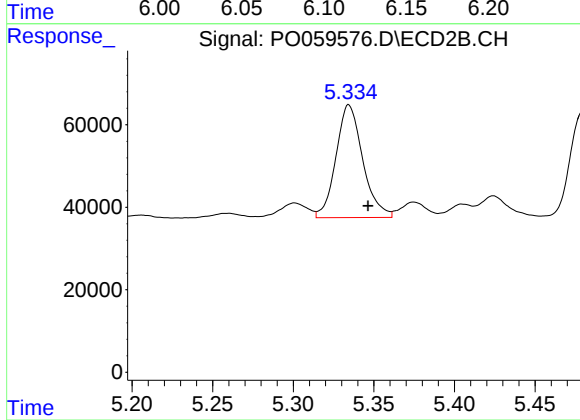


#26 AR-1254-1

R.T.: 5.335 min
Delta R.T.: -0.012 min
Response: 316181
Conc: 133.31 ng/ml

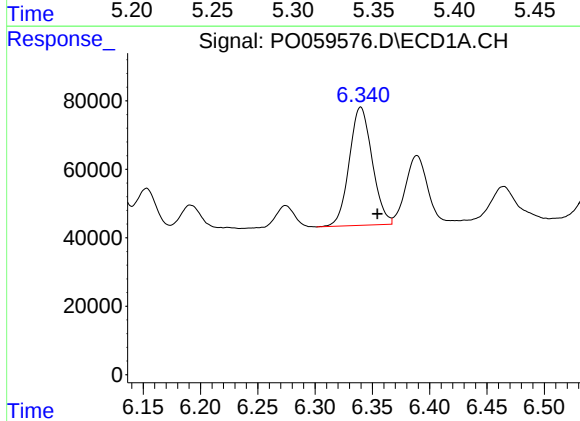


#27 AR-1254-2

R.T.: 6.340 min
Delta R.T.: -0.015 min
Response: 480720
Conc: 144.09 ng/ml

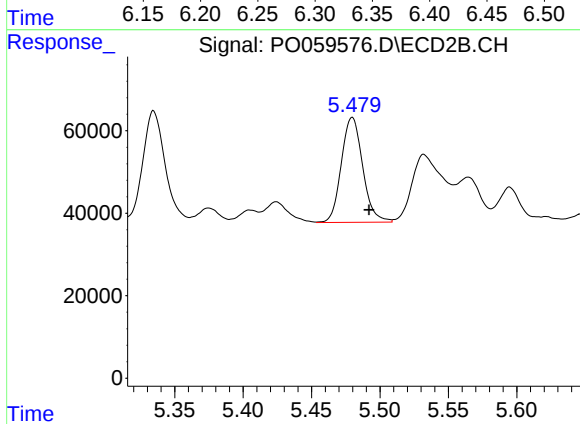

#27 AR-1254-2

R.T.: 5.480 min
Delta R.T.: -0.012 min
Response: 277518
Conc: 132.26 ng/ml

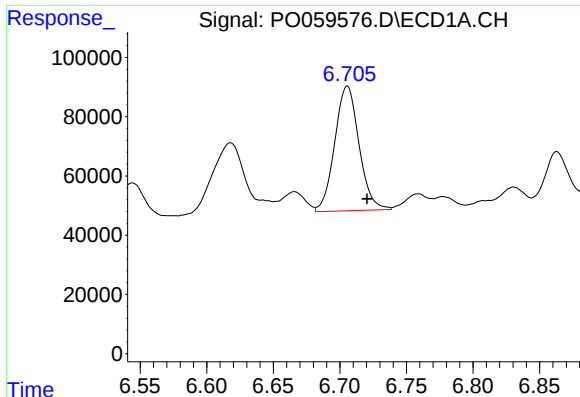


#28 AR-1254-3

R.T.: 6.706 min
Delta R.T.: -0.015 min
Response: 535629
Conc: 150.95 ng/ml

Instrument :
ECD_O
ClientSampleId :
HA-15


Manual Integrations
APPROVED

Ankita
8/22/2019 3:32:42 PM

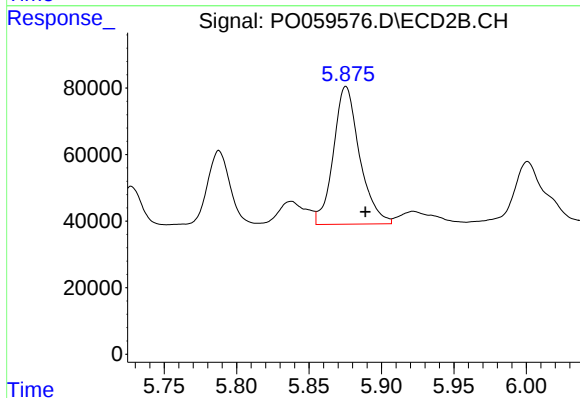


#28 AR-1254-3

R.T.: 5.875 min
Delta R.T.: -0.013 min
Response: 521016
Conc: 154.95 ng/ml

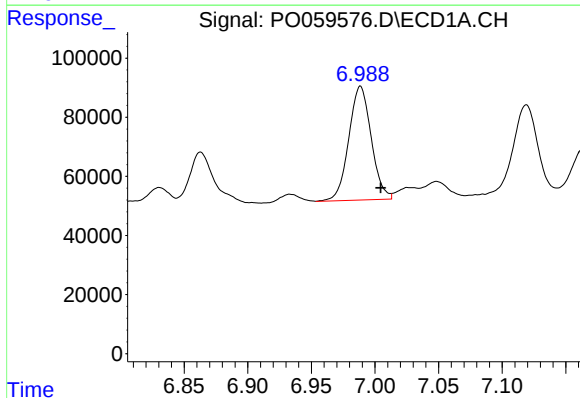


#29 AR-1254-4

R.T.: 6.989 min
Delta R.T.: -0.016 min
Response: 472573
Conc: 160.44 ng/ml

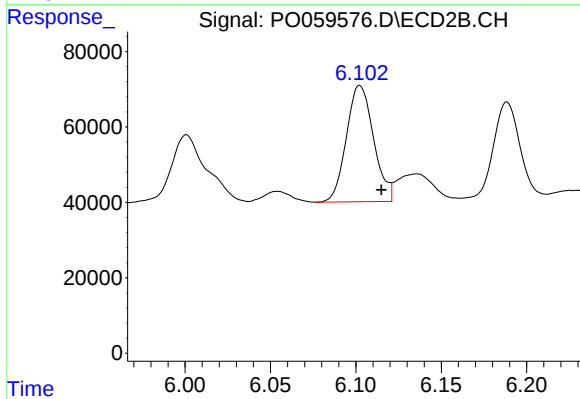

#29 AR-1254-4

R.T.: 6.102 min
Delta R.T.: -0.013 min
Response: 341691
Conc: 165.72 ng/ml

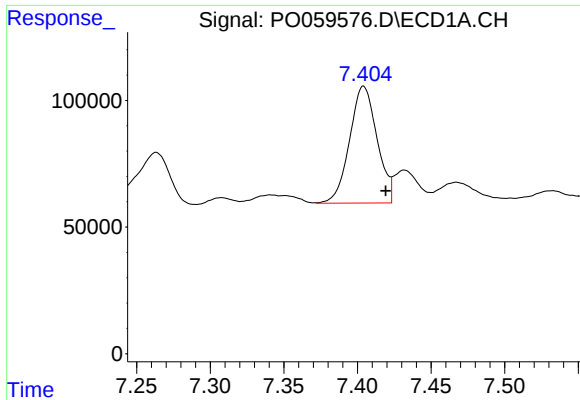


#30 AR-1254-5

R.T.: 7.404 min
Delta R.T.: -0.016 min
Response: 604610
Conc: 195.52 ng/ml m

Instrument :
ECD_O
ClientSampleId :
HA-15

Manual Integrations
APPROVED

Ankita
8/22/2019 3:32:42 PM

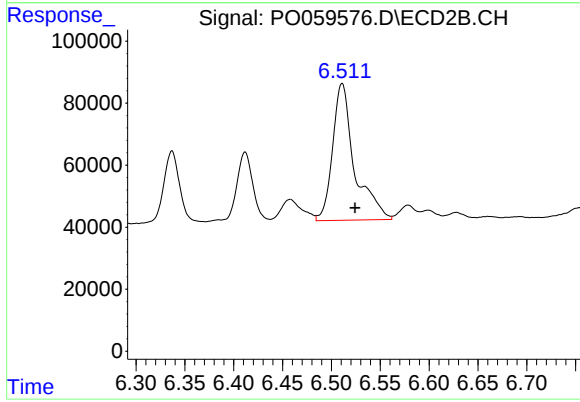

#30 AR-1254-5

R.T.: 6.511 min
Delta R.T.: -0.013 min
Response: 688950
Conc: 221.89 ng/ml