

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082119\
 Data File : P0059599.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Aug 2019 18:36
 Operator : SM/AJ
 Sample : K4444-01 5X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SES-GODWIN-PUMP-082019

Manual Integrations
 APPROVED

Ankita
 8/22/2019 3:33:41 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 22 03:55:17 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 17 03:09:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.131	3.501	164604	152034	4.701	4.224
2) SA Decachlor...	9.614	8.368	197926	150174	3.720	3.724m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO082119\
Data File : PO059599.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Aug 2019 18:36
Operator : SM/AJ
Sample : K4444-01 5X
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SES-GODWIN-PUMP-082019


Manual Integrations
APPROVED

Ankita
8/22/2019 3:33:41 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 22 03:55:17 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Aug 17 03:09:44 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

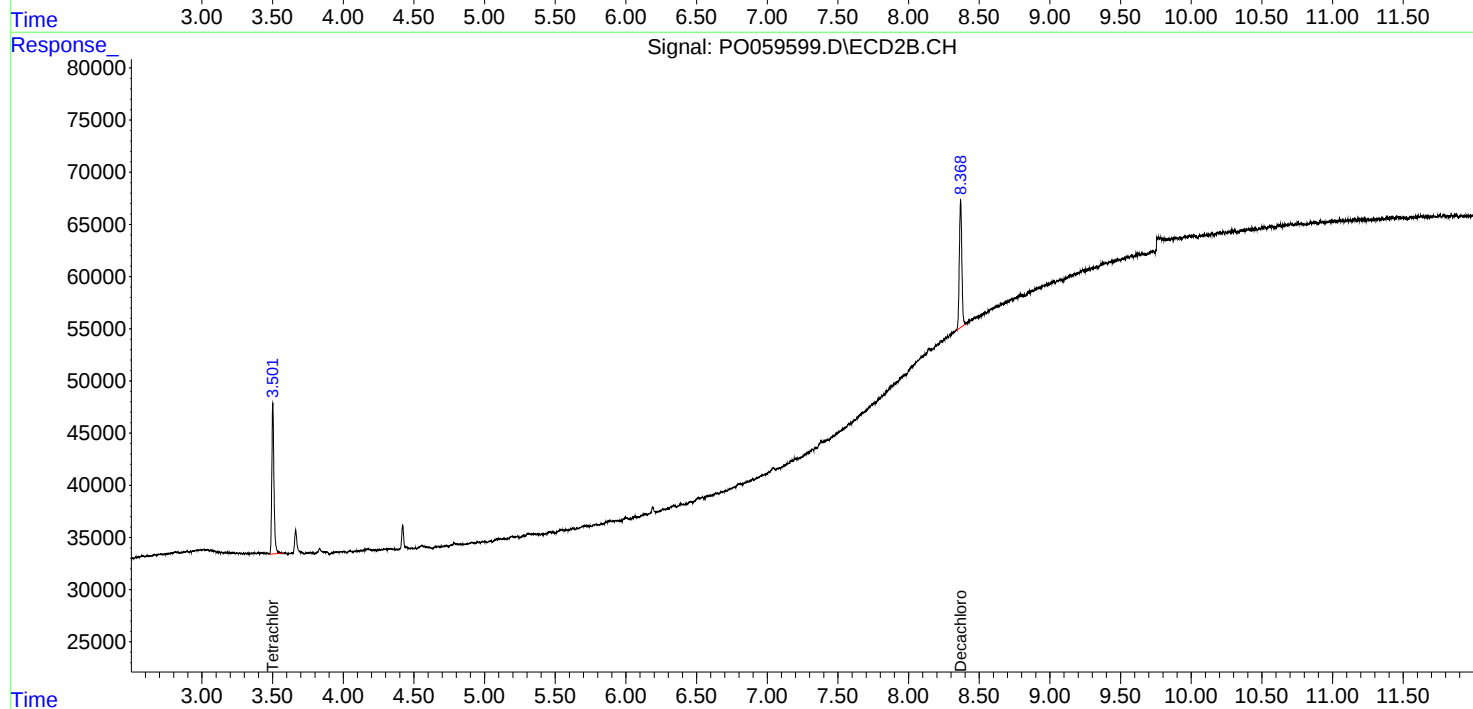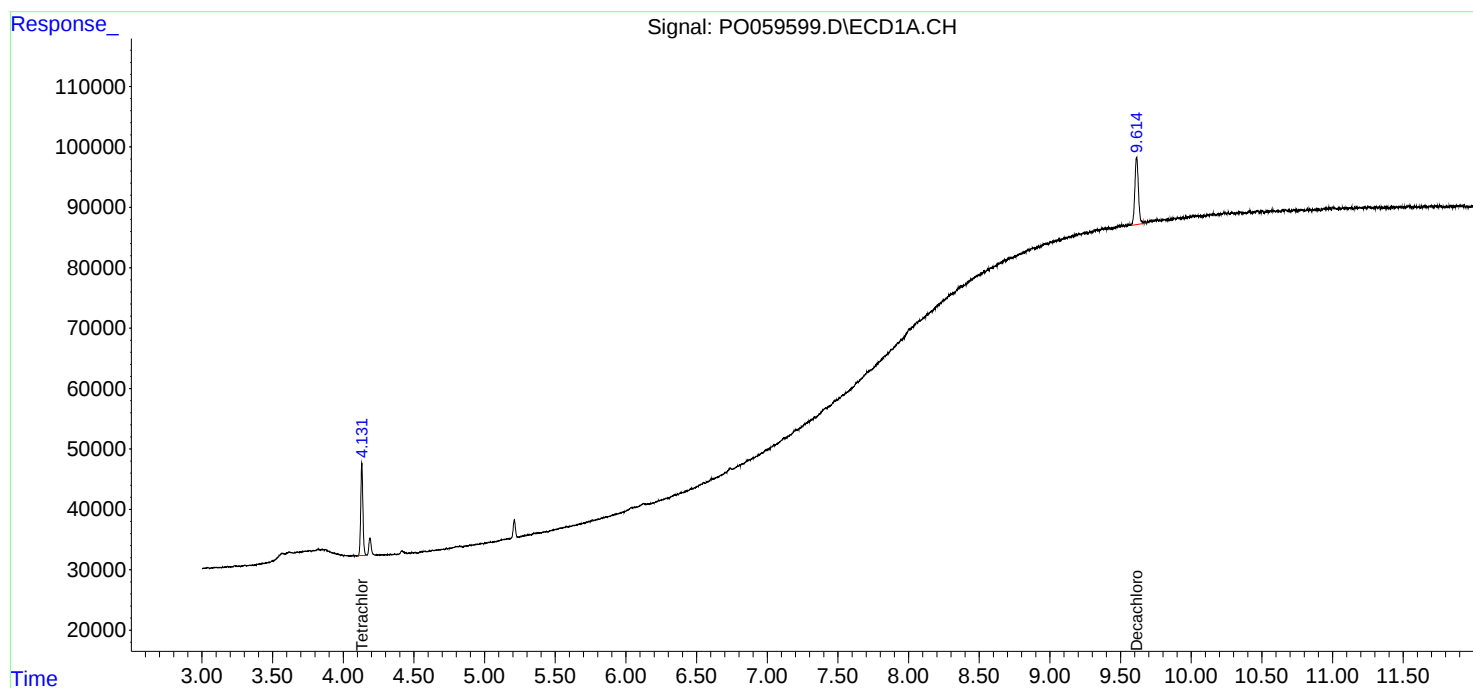

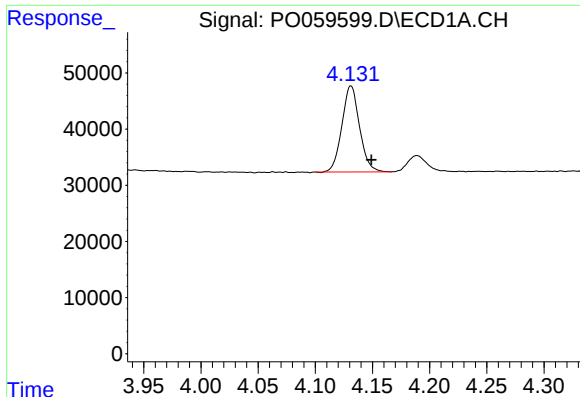


#1 Tetrachloro-m-xylene

R.T.: 4.131 min
Delta R.T.: -0.018 min
Response: 164604
Conc: 4.70 ng/ml

Instrument :
ECD_O
ClientSampleId :
SES-GODWIN-PUMP-082019


Manual Integrations
APPROVED

Ankita
8/22/2019 3:33:41 PM

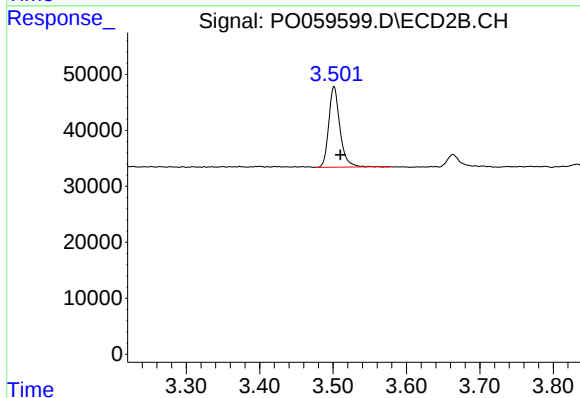


#1 Tetrachloro-m-xylene

R.T.: 3.501 min
Delta R.T.: -0.009 min
Response: 152034
Conc: 4.22 ng/ml

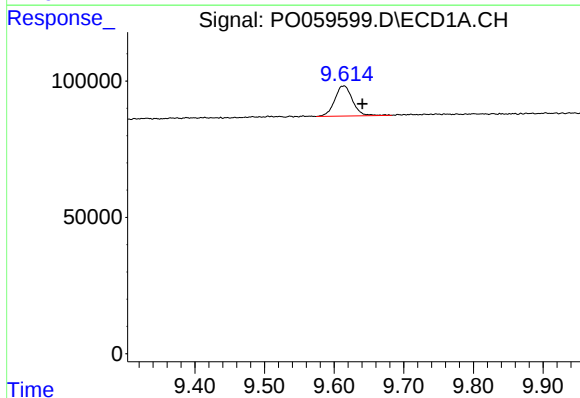

#2 Decachlorobiphenyl

R.T.: 9.614 min
Delta R.T.: -0.027 min
Response: 197926
Conc: 3.72 ng/ml

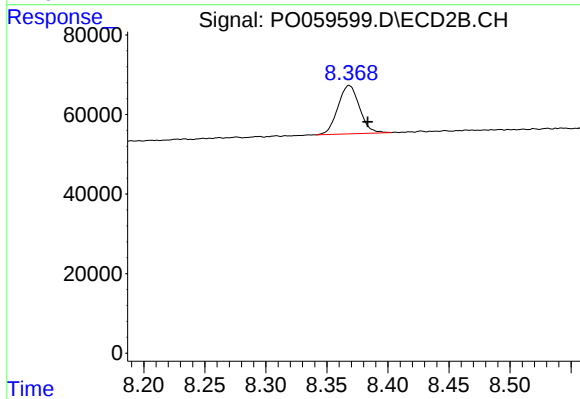

#2 Decachlorobiphenyl

R.T.: 8.368 min
Delta R.T.: -0.016 min
Response: 150174
Conc: 3.72 ng/ml m