

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082119\
 Data File : P0059625.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Aug 2019 2:07
 Operator : SM/AJ
 Sample : K4449-07 5X
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MIXING-BOX-1-082019-83

Manual Integrations
 APPROVED

Ankita
 8/22/2019 3:34:51 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 22 04:06:54 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 17 03:09:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.130	3.500	189200	171844	5.404	4.774m
2) SA Decachlor...	9.612	8.367	217906	172513	4.096m	4.278m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082119\
Data File : P0059625.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Aug 2019 2:07
Operator : SM/AJ
Sample : K4449-07 5X
Misc :
ALS Vial : 30 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
MIXING-BOX-1-082019-83


Manual Integrations
APPROVED

Ankita
8/22/2019 3:34:51 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 22 04:06:54 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Aug 17 03:09:44 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

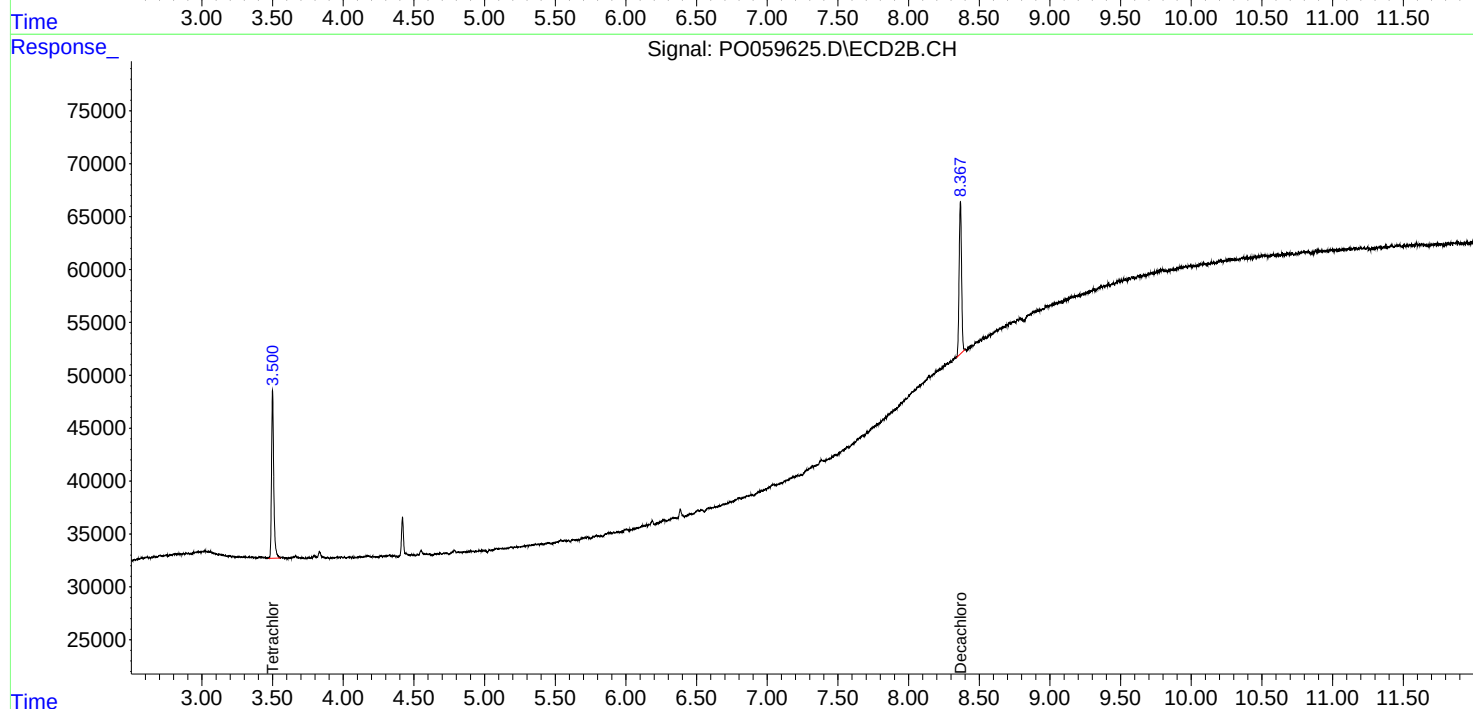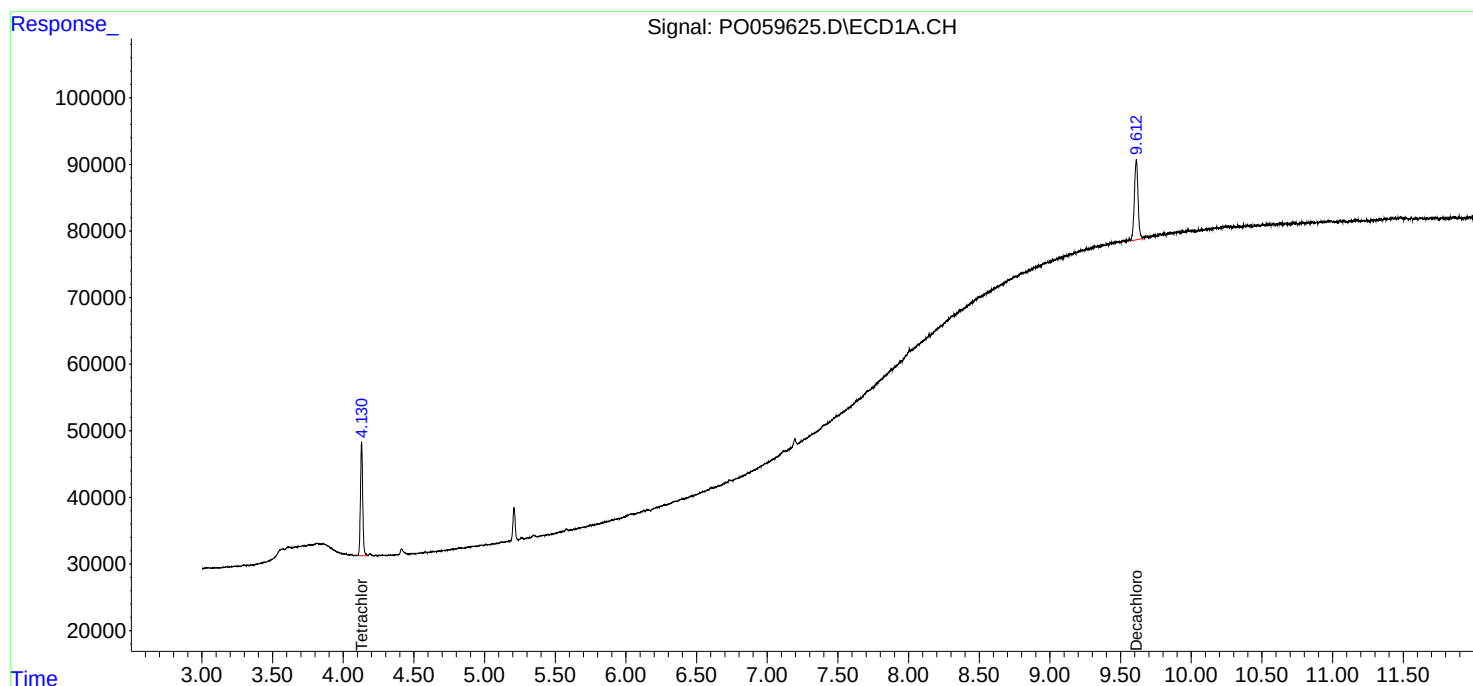

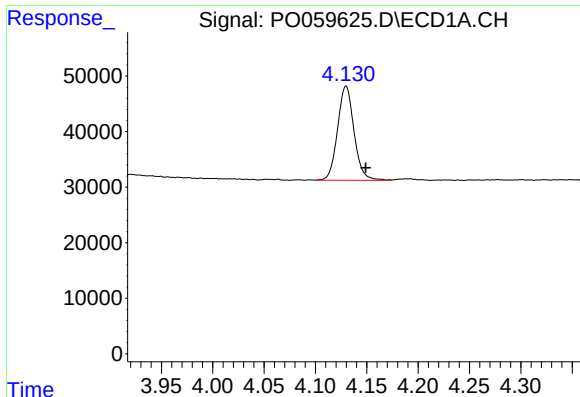


#1 Tetrachloro-m-xylene

R.T.: 4.130 min
Delta R.T.: -0.019 min
Response: 189200
Conc: 5.40 ng/ml

Instrument :
ECD_O
ClientSampleId :
MIXING-BOX-1-082019-83


Manual Integrations
APPROVED

Ankita
8/22/2019 3:34:51 PM

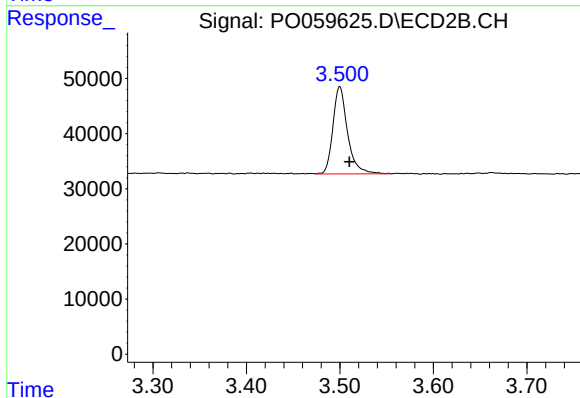


#1 Tetrachloro-m-xylene

R.T.: 3.500 min
Delta R.T.: -0.010 min
Response: 171844
Conc: 4.77 ng/ml m

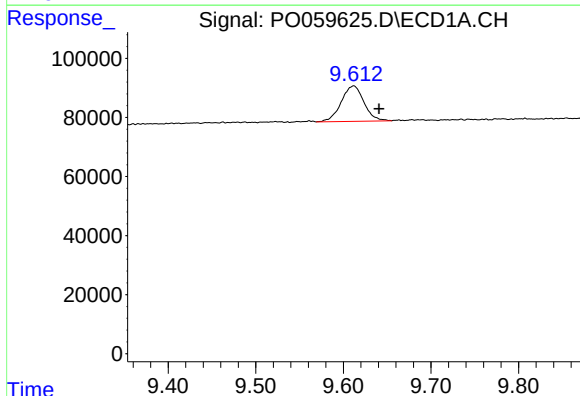

#2 Decachlorobiphenyl

R.T.: 9.612 min
Delta R.T.: -0.029 min
Response: 217906
Conc: 4.10 ng/ml m

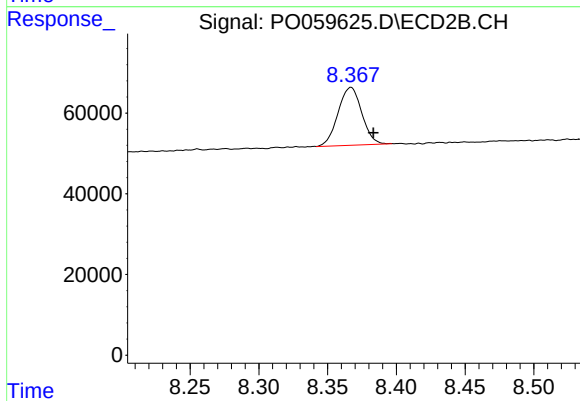

#2 Decachlorobiphenyl

R.T.: 8.367 min
Delta R.T.: -0.017 min
Response: 172513
Conc: 4.28 ng/ml m