

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082119\
 Data File : P0059626.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Aug 2019 2:23
 Operator : SM/AJ
 Sample : K4449-08 5X
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MIXING-BOX-1-082019-97

Manual Integrations
 APPROVED

Ankita
 8/22/2019 3:35:10 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 22 04:07:22 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 17 03:09:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.130	3.500	180326	168812	5.150	4.690
2) SA Decachlor...	9.610	8.365	206062	164290	3.873m	4.075m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082119\
Data File : P0059626.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Aug 2019 2:23
Operator : SM/AJ
Sample : K4449-08 5X
Misc :
ALS Vial : 31 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
MIXING-BOX-1-082019-97


Manual Integrations
APPROVED

Ankita
8/22/2019 3:35:10 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 22 04:07:22 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Aug 17 03:09:44 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

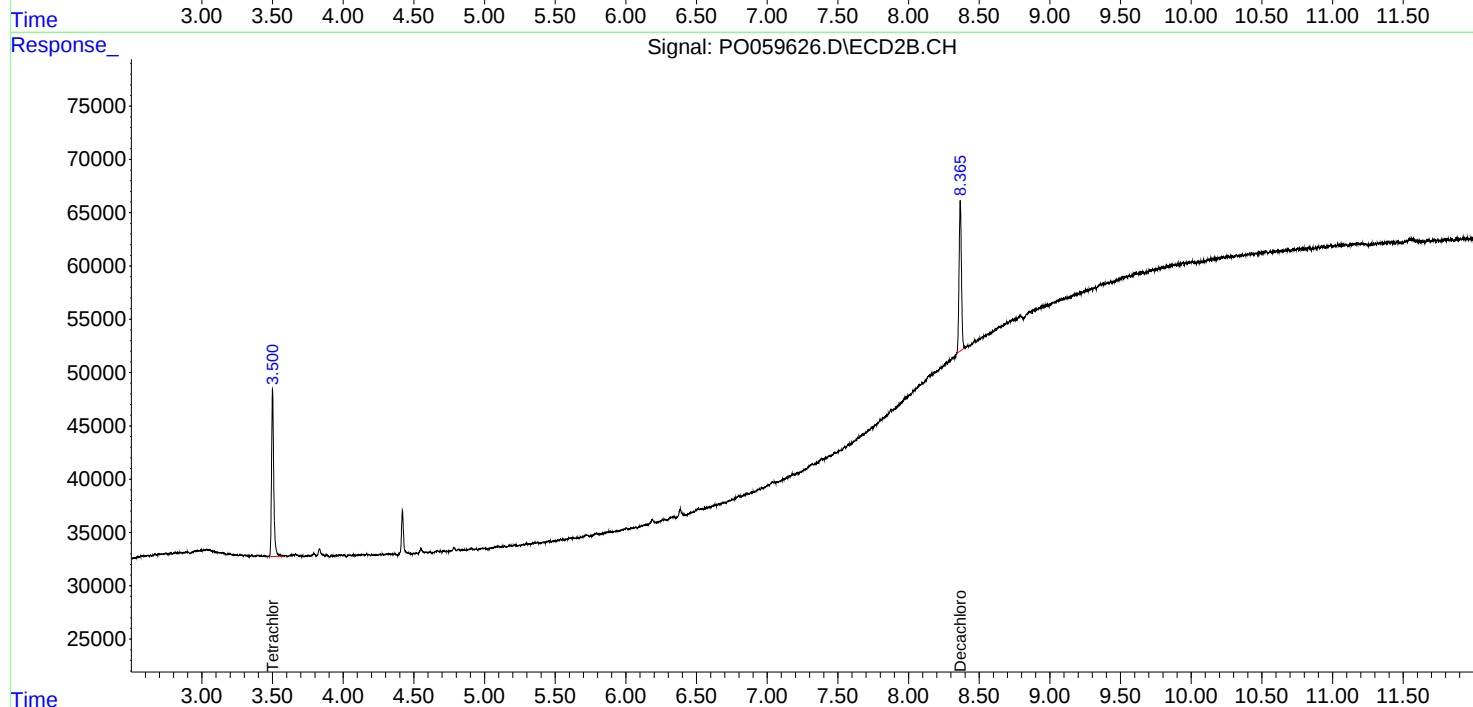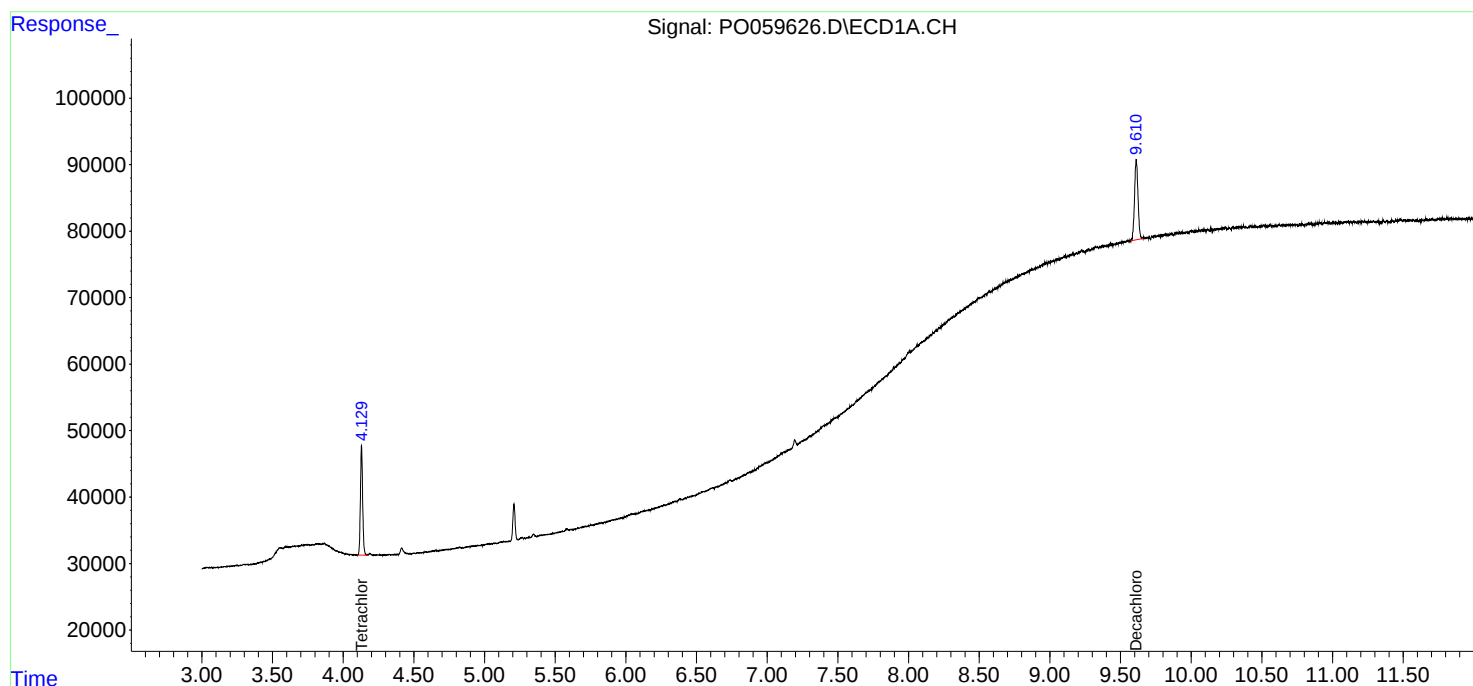

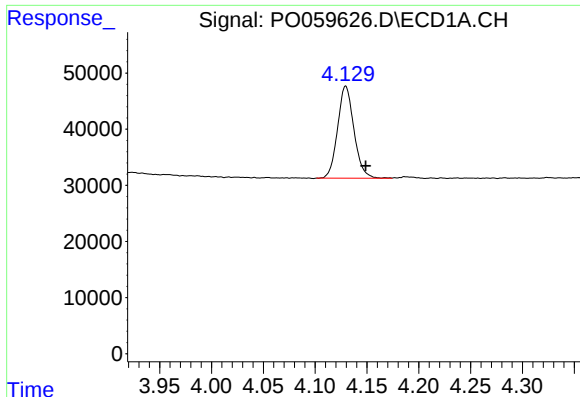


#1 Tetrachloro-m-xylene

R.T.: 4.130 min
Delta R.T.: -0.019 min
Response: 180326
Conc: 5.15 ng/ml

Instrument :
ECD_O
ClientSampleId :
MIXING-BOX-1-082019-97


Manual Integrations
APPROVED

Ankita
8/22/2019 3:35:10 PM

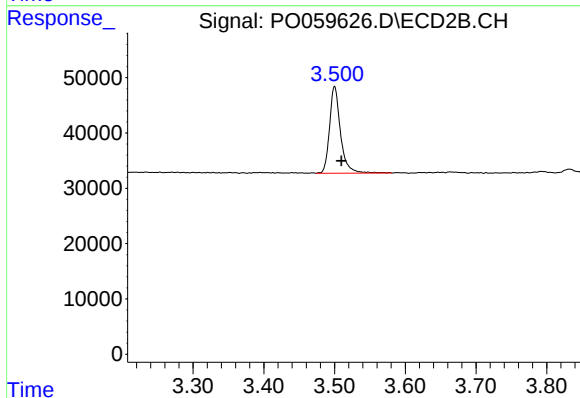


#1 Tetrachloro-m-xylene

R.T.: 3.500 min
Delta R.T.: -0.010 min
Response: 168812
Conc: 4.69 ng/ml

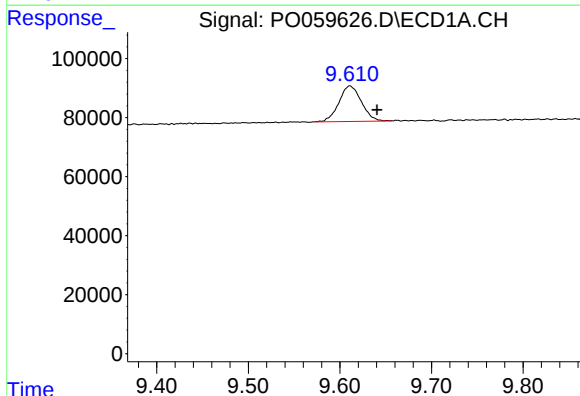

#2 Decachlorobiphenyl

R.T.: 9.610 min
Delta R.T.: -0.030 min
Response: 206062
Conc: 3.87 ng/ml m

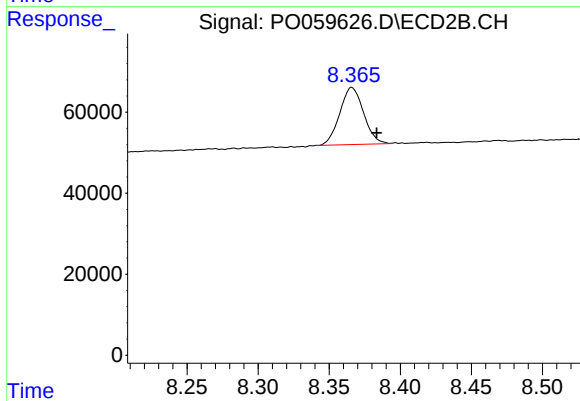

#2 Decachlorobiphenyl

R.T.: 8.365 min
Delta R.T.: -0.018 min
Response: 164290
Conc: 4.07 ng/ml m