

Data Path : Z:\bestpcbsrv\HPCHEM1\ECD 0\Data\P0082218\  
Data File : P0048399.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 22 Aug 2018 12:23  
Operator : SM/SJ  
Sample : J4545-01  
Misc :  
ALS Vial : 14 Sample Multiplier: 1

Instrument :  
ECD\_O  
ClientSampleId :  
RB-BASELINE-WATER

Manual Integrations  
APPROVED

Sohil  
8/23/2018 10:35:00 AM

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Aug 22 12:49:44 2018  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0072718.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Fri Jul 27 02:33:29 2018  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

| Compound                    | RT#1   | RT#2  | Resp#1  | Resp#2  | nq/ml   | nq/ml  |
|-----------------------------|--------|-------|---------|---------|---------|--------|
| -----                       |        |       |         |         |         |        |
| System Monitoring Compounds |        |       |         |         |         |        |
| 1) SA Tetrachlo...          | 4.392  | 3.637 | 2498441 | 2918274 | 12.375m | 11.877 |
| 2) SA Decachlor...          | 10.080 | 8.615 | 2185030 | 1753573 | 13.397  | 11.156 |

Target Compounds

-----

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0082218\  
Data File : P0048399.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 22 Aug 2018 12:23  
Operator : SM/SJ  
Sample : J4545-01  
Misc :  
ALS Vial : 14 Sample Multiplier: 1



Instrument :  
ECD\_O  
ClientSampleId :  
RB-BASELINE-WATER


Manual Integrations  
APPROVED

Sohil  
8/23/2018 10:35:00 AM

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Aug 22 12:49:44 2018  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0072718.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Fri Jul 27 02:33:29 2018  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

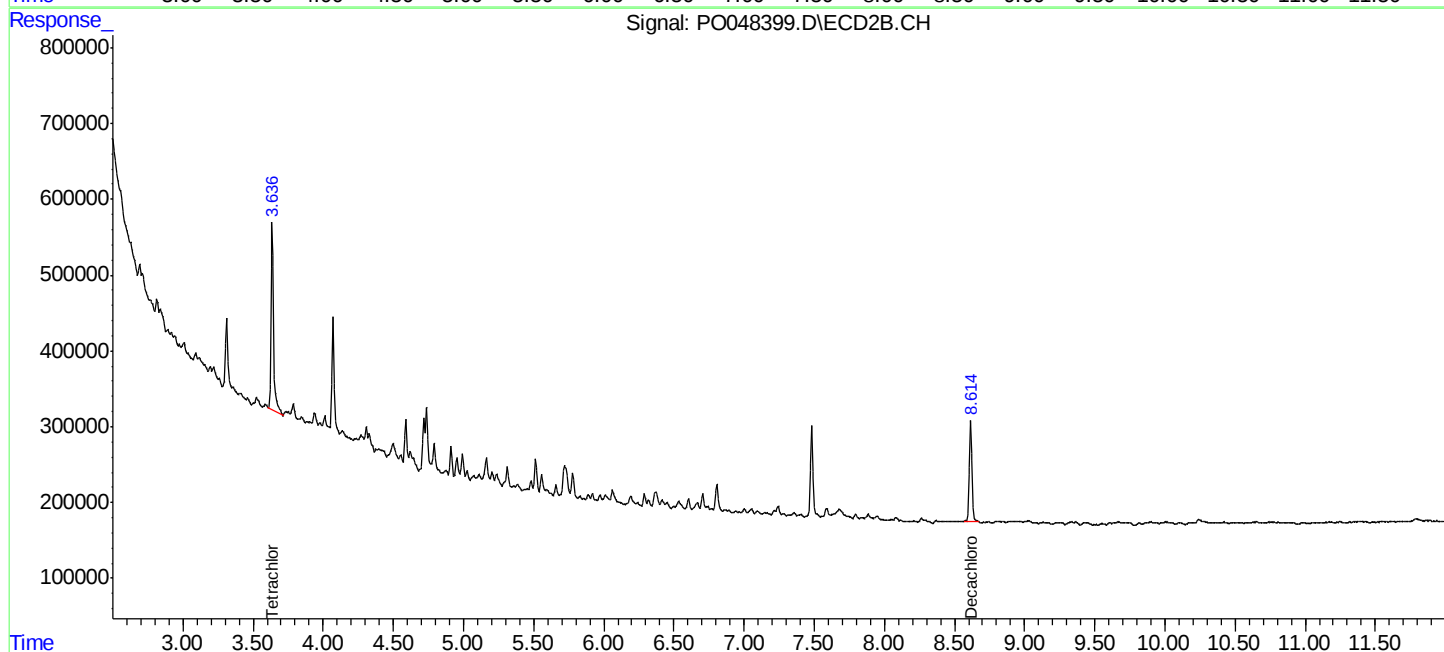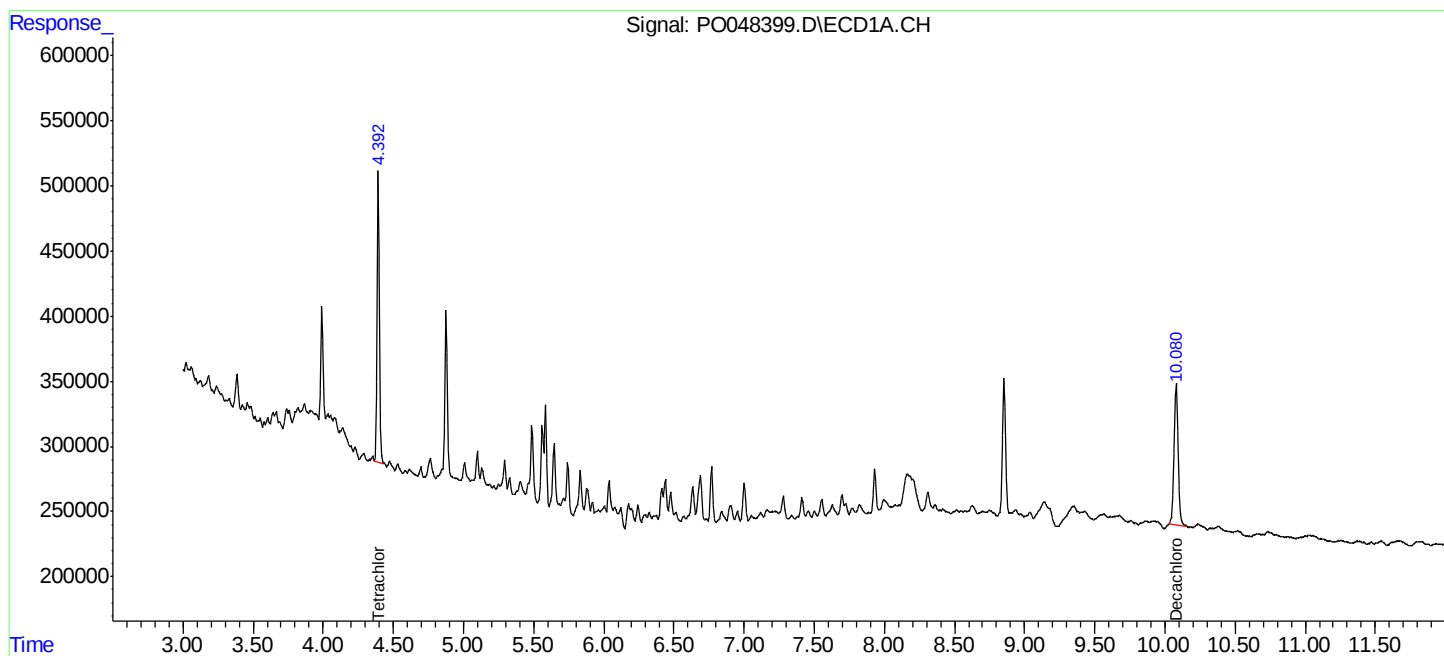

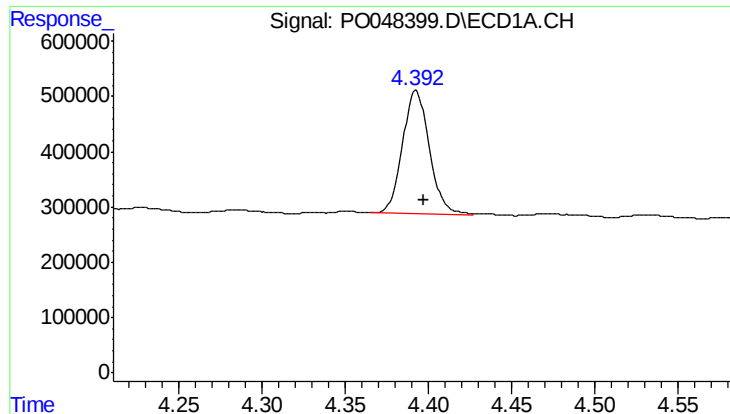


#1 Tetrachloro-m-xylene

R.T.: 4.392 min  
Delta R.T.: -0.005 min  
Response: 2498441  
Conc: 12.37 ng/ml

Instrument :  
ECD\_O  
ClientSampleId :  
RB-BASELINE-WATER


Manual Integrations  
APPROVED

Sohil  
8/23/2018 10:35:00 AM

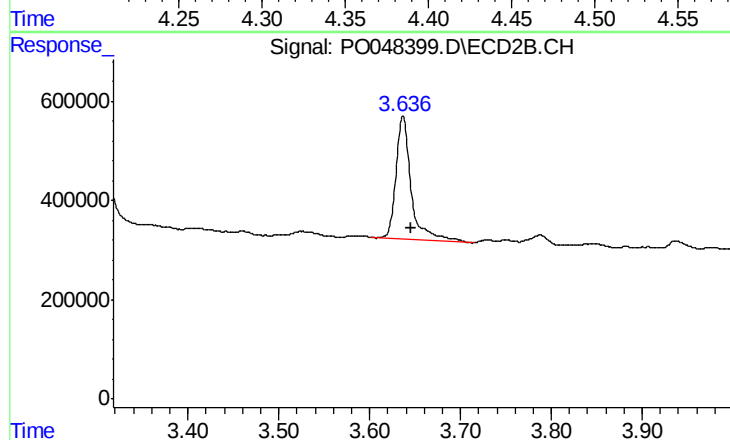


#1 Tetrachloro-m-xylene

R.T.: 3.637 min  
Delta R.T.: -0.009 min  
Response: 2918274  
Conc: 11.88 ng/ml

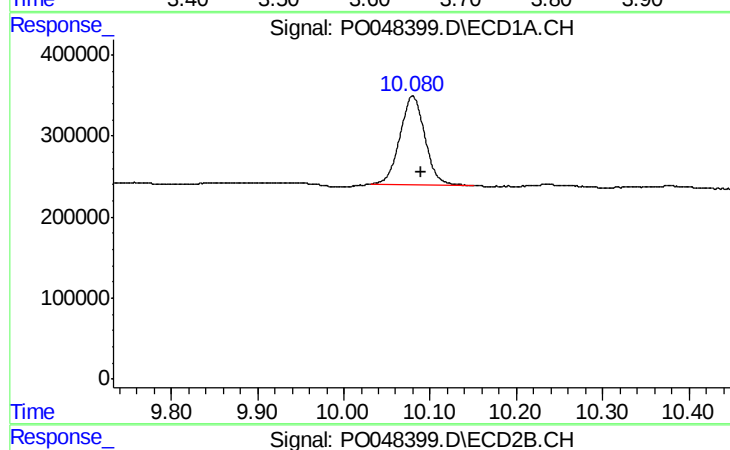

#2 Decachlorobiphenyl

R.T.: 10.080 min  
Delta R.T.: -0.010 min  
Response: 2185030  
Conc: 13.40 ng/ml

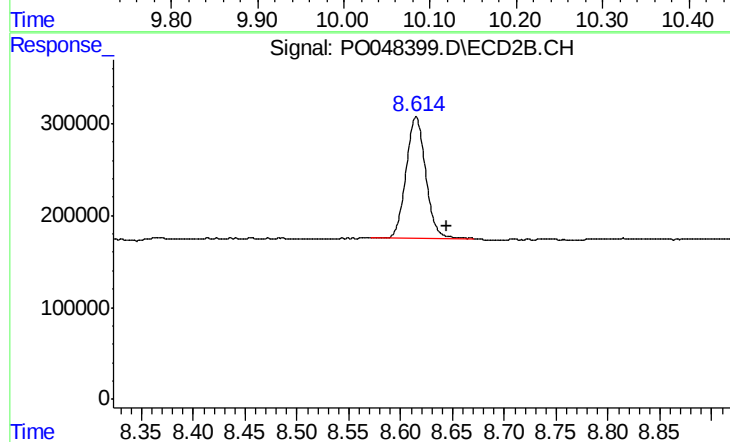

#2 Decachlorobiphenyl

R.T.: 8.615 min  
Delta R.T.: -0.030 min  
Response: 1753573  
Conc: 11.16 ng/ml