

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082419\
 Data File : P0059811.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Aug 2019 22:06
 Operator : SM/AJ
 Sample : K4490-05
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 STUCCO-AND-BRICK

Manual Integrations
 APPROVED

Ankita
 8/26/2019 3:08:27 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 26 03:31:55 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 17 03:09:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.121	3.495	862600	817946	24.637m	22.723
2) SA Decachlor...	9.586	8.354	1381975	1034617	25.977	25.659m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082419\
Data File : P0059811.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Aug 2019 22:06
Operator : SM/AJ
Sample : K4490-05
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
STUCCO-AND-BRICK


Manual Integrations
APPROVED

Ankita
8/26/2019 3:08:27 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 26 03:31:55 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Aug 17 03:09:44 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

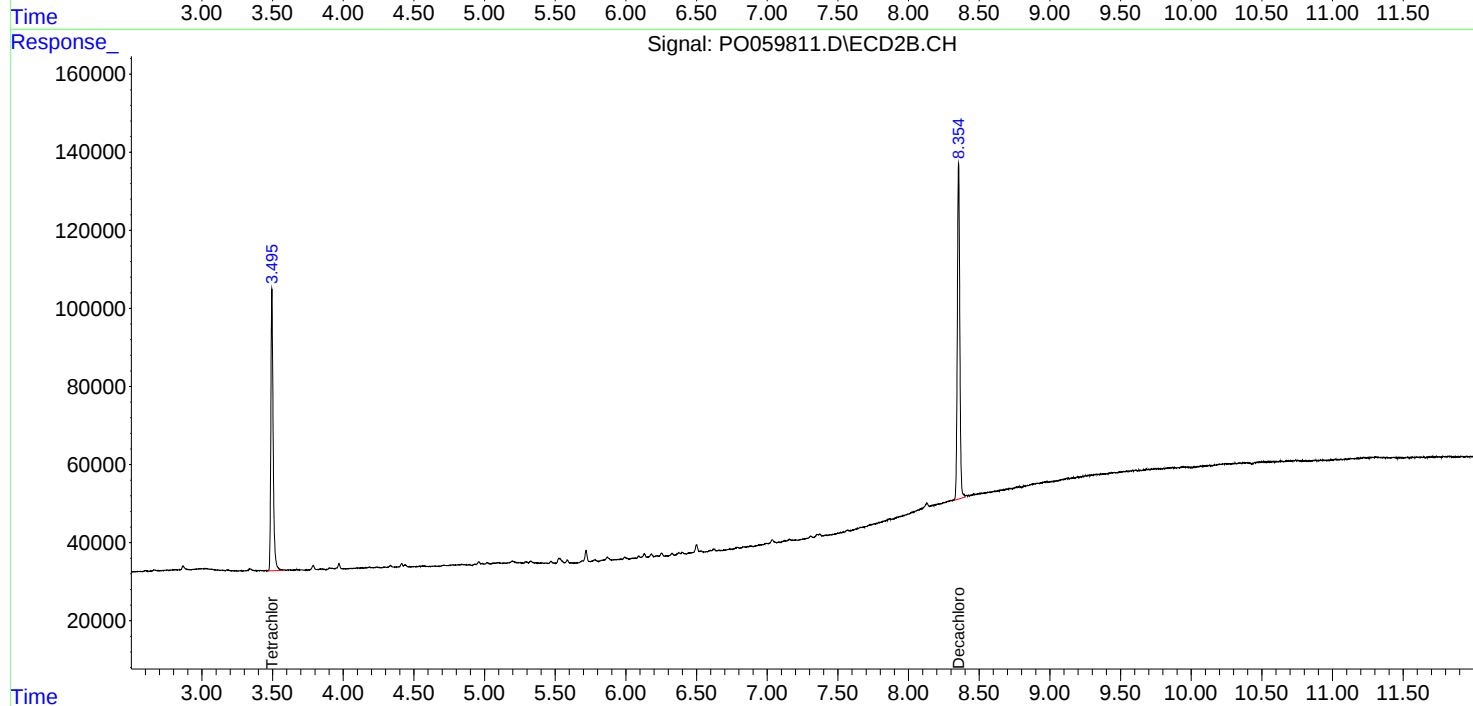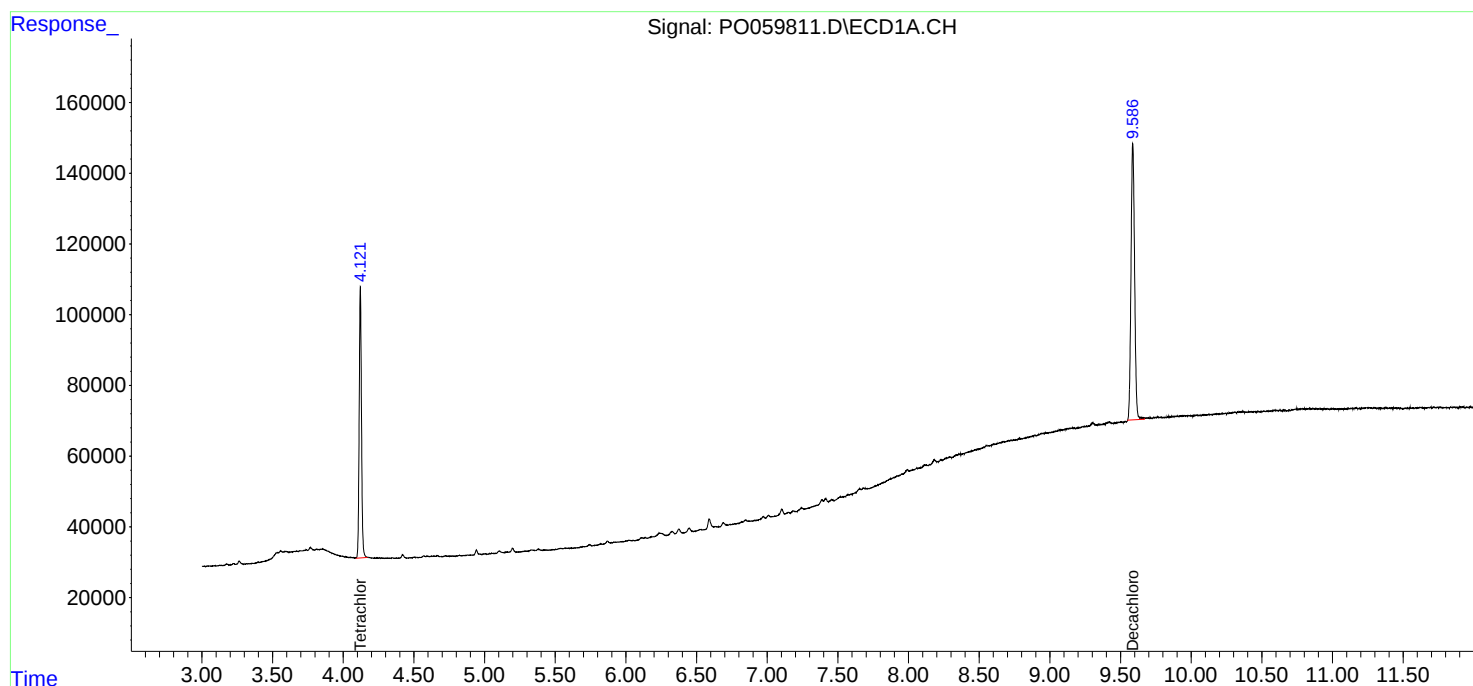

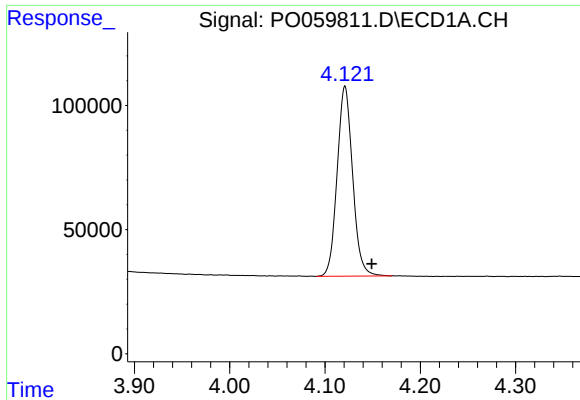


#1 Tetrachloro-m-xylene

R.T.: 4.121 min
Delta R.T.: -0.028 min
Response: 862600
Conc: 24.64 ng/ml m

Instrument :
ECD_O
ClientSampleId :
STUCCO-AND-BRICK


Manual Integrations
APPROVED

Ankita
8/26/2019 3:08:27 PM

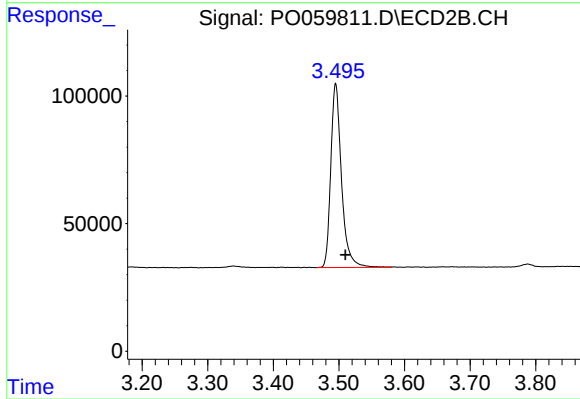


#1 Tetrachloro-m-xylene

R.T.: 3.495 min
Delta R.T.: -0.015 min
Response: 817946
Conc: 22.72 ng/ml

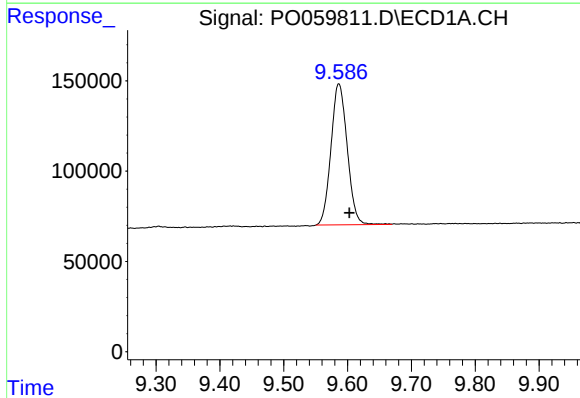

#2 Decachlorobiphenyl

R.T.: 9.586 min
Delta R.T.: -0.017 min
Response: 1381975
Conc: 25.98 ng/ml

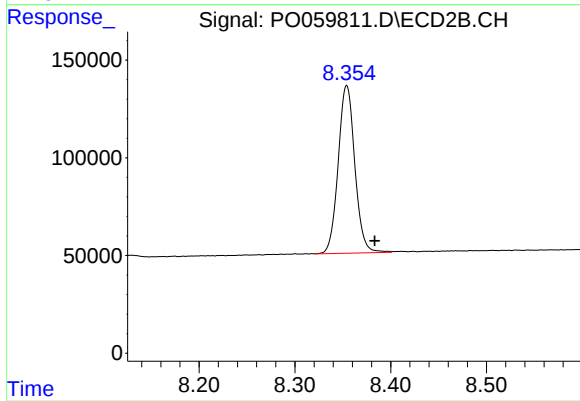

#2 Decachlorobiphenyl

R.T.: 8.354 min
Delta R.T.: -0.030 min
Response: 1034617
Conc: 25.66 ng/ml m