

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082419\
 Data File : P0059812.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Aug 2019 22:22
 Operator : SM/AJ
 Sample : K4490-07
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CONCRETE-SLAB

Manual Integrations
 APPROVED

Ankita
 8/26/2019 3:08:28 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 26 03:32:20 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 17 03:09:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.120	3.496	818536	782303	23.378m	21.733
2) SA Decachlor...	9.589	8.367	1261123	2072481	23.705	51.400 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO082419\
Data File : PO059812.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Aug 2019 22:22
Operator : SM/AJ
Sample : K4490-07
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
CONCRETE-SLAB


Manual Integrations
APPROVED

Ankita
8/26/2019 3:08:28 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 26 03:32:20 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Aug 17 03:09:44 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

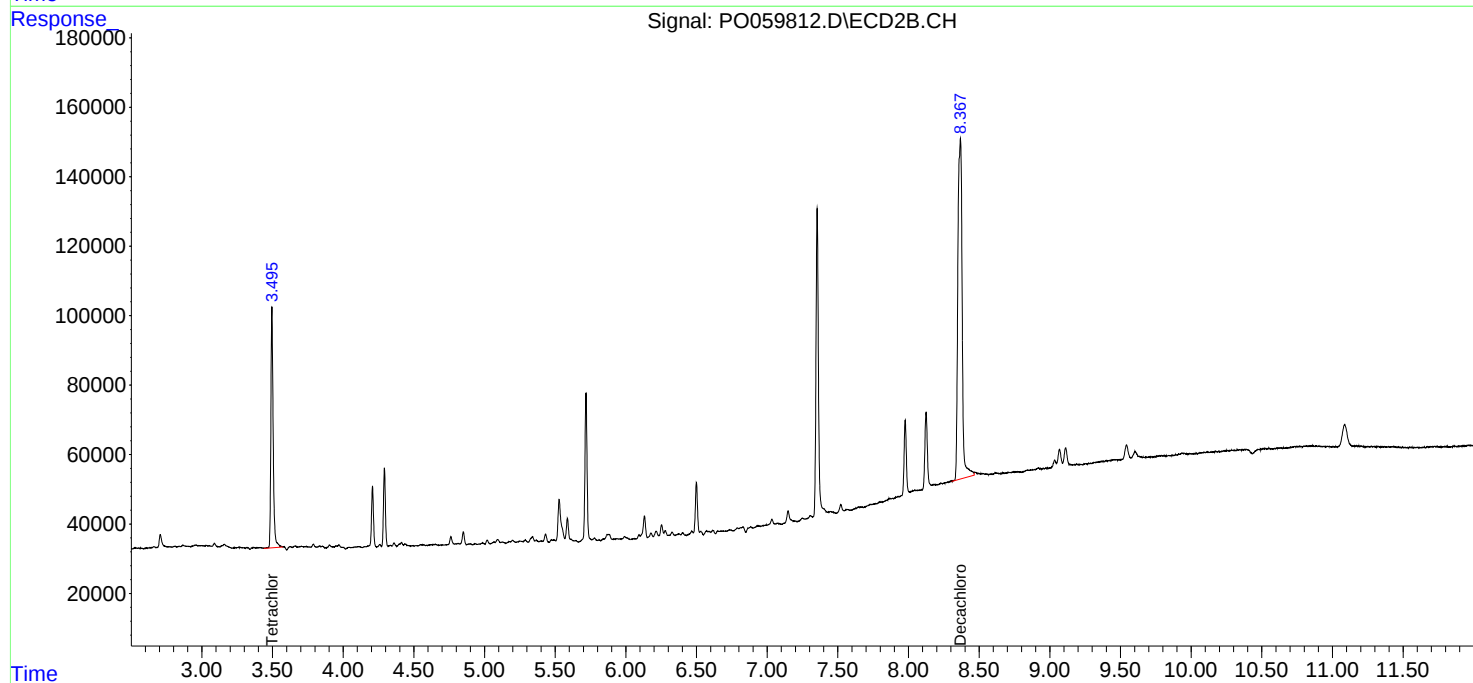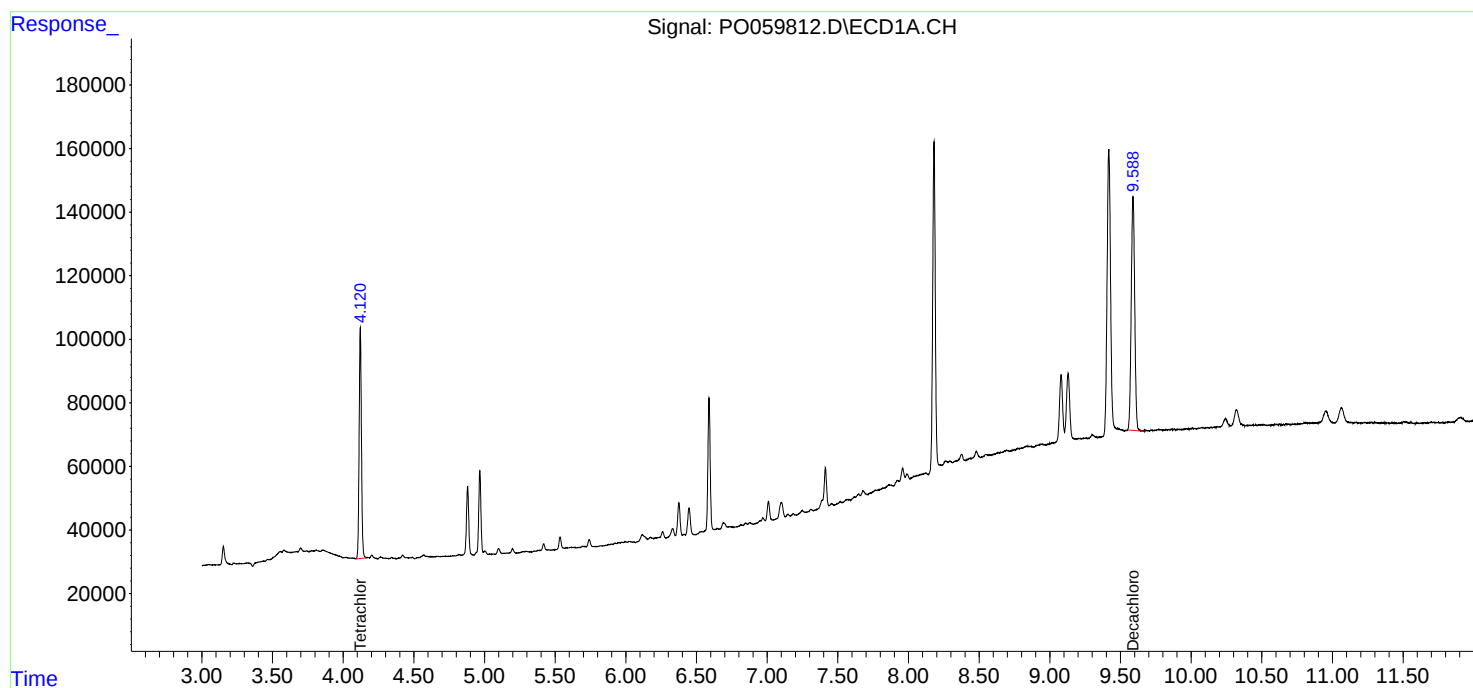

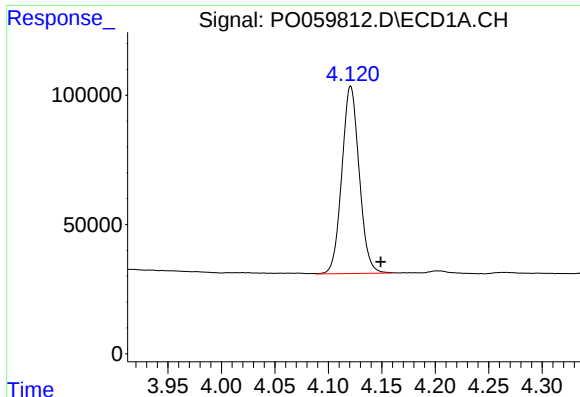


#1 Tetrachloro-m-xylene

R.T.: 4.120 min
Delta R.T.: -0.029 min
Response: 818536
Conc: 23.38 ng/ml m

Instrument :
ECD_O
ClientSampleId :
CONCRETE-SLAB


Manual Integrations
APPROVED

Ankita
8/26/2019 3:08:28 PM

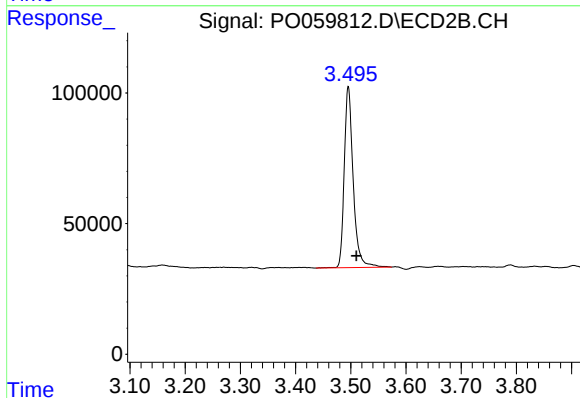


#1 Tetrachloro-m-xylene

R.T.: 3.496 min
Delta R.T.: -0.014 min
Response: 782303
Conc: 21.73 ng/ml

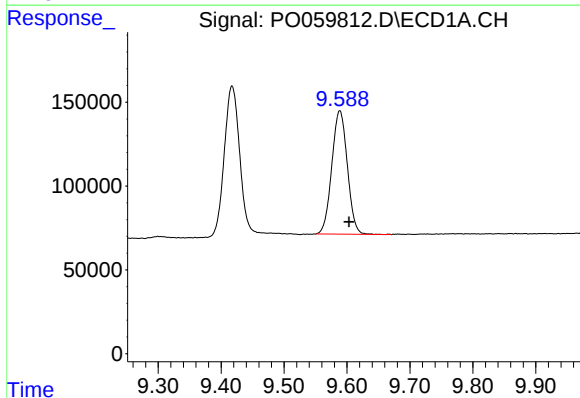

#2 Decachlorobiphenyl

R.T.: 9.589 min
Delta R.T.: -0.014 min
Response: 1261123
Conc: 23.71 ng/ml

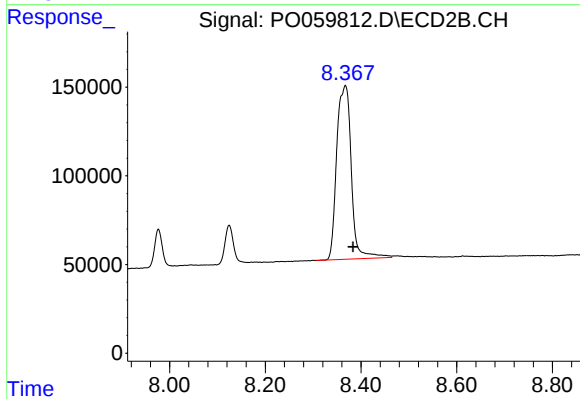

#2 Decachlorobiphenyl

R.T.: 8.367 min
Delta R.T.: -0.016 min
Response: 2072481
Conc: 51.40 ng/ml