

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082419\
 Data File : P0059829.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Aug 2019 2:57
 Operator : SM/AJ
 Sample : K4510-10
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SB-14-COMP

Manual Integrations
 APPROVED

Ankita
 8/26/2019 3:09:19 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 26 03:41:12 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 17 03:09:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.119	3.494	874093	824241	24.965m	22.898
2) SA Decachlor...	9.584	8.352	1189214	902879	22.354m	22.392m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO082419\
Data File : PO059829.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Aug 2019 2:57
Operator : SM/AJ
Sample : K4510-10
Misc :
ALS Vial : 29 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SB-14-COMP


Manual Integrations
APPROVED

Ankita
8/26/2019 3:09:19 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 26 03:41:12 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Aug 17 03:09:44 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

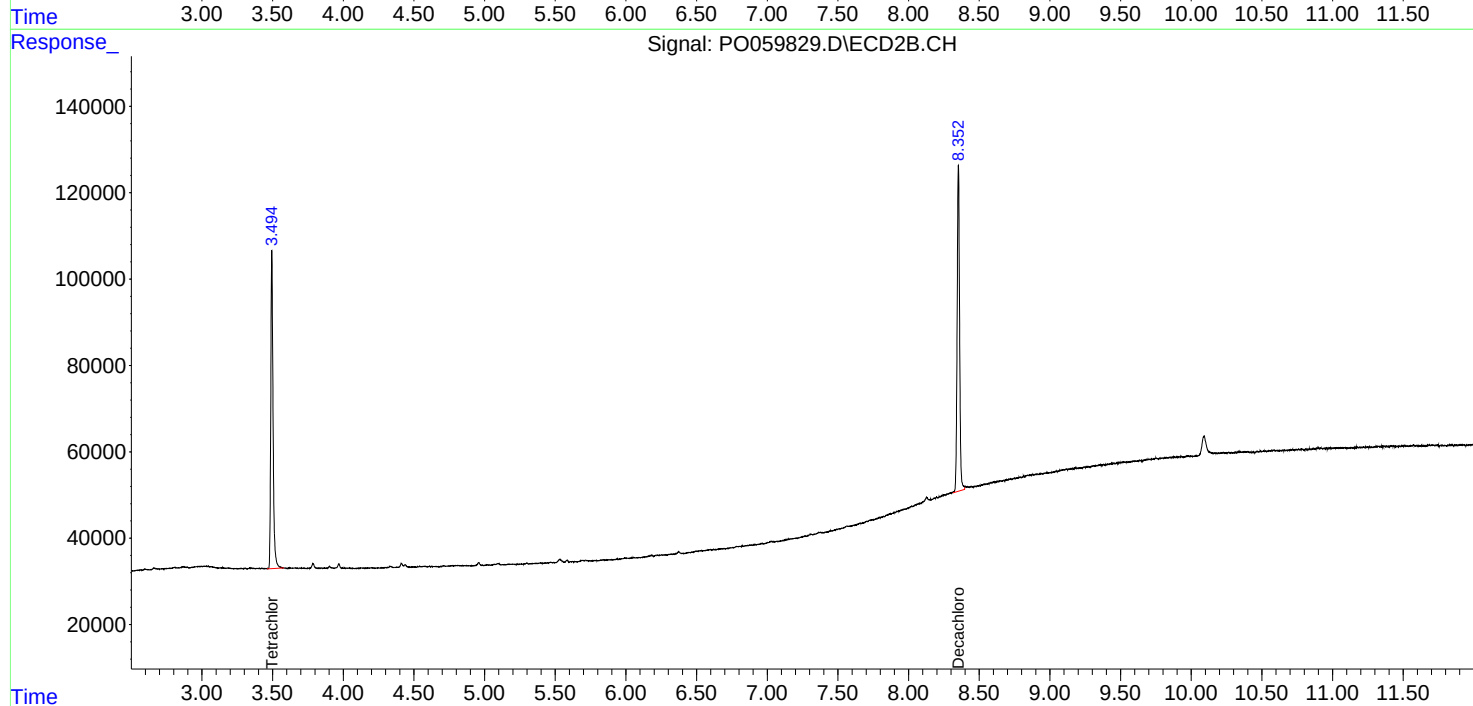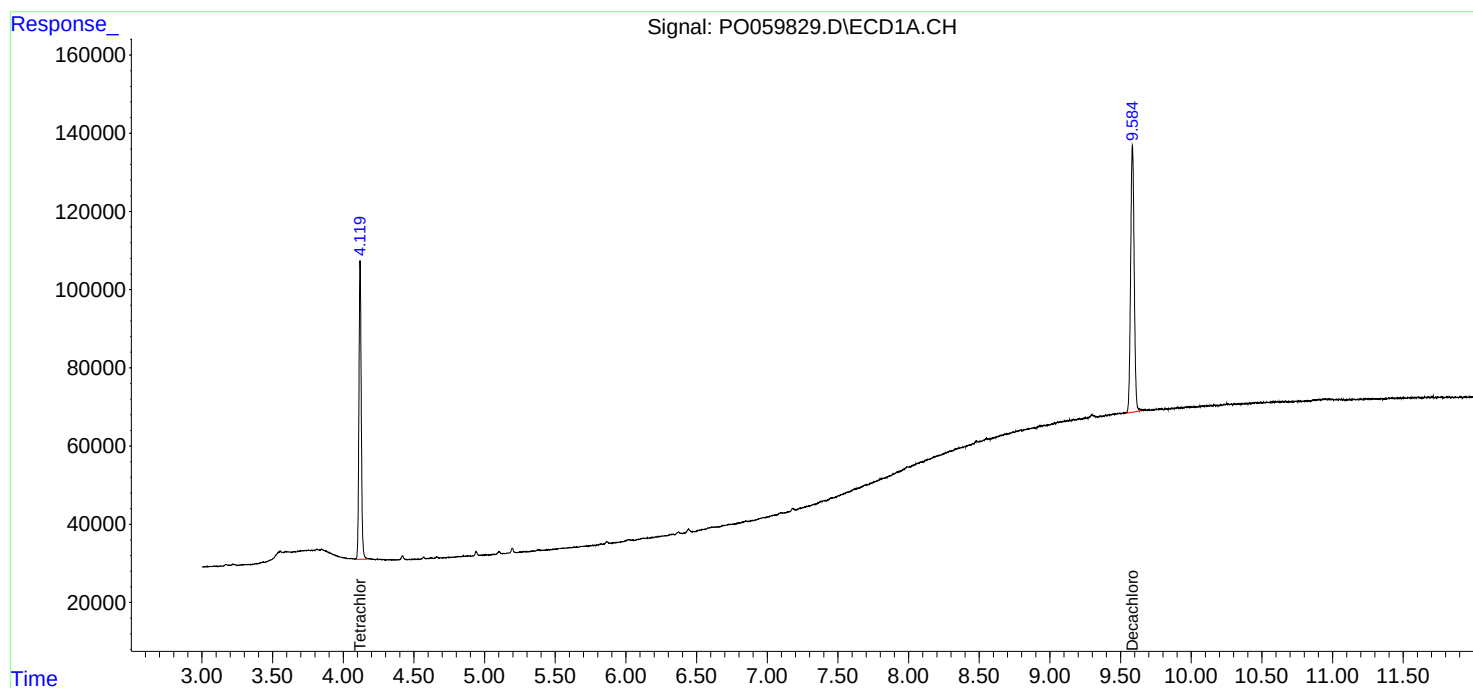

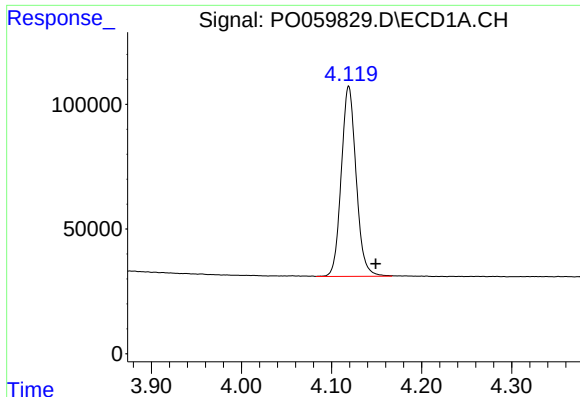


#1 Tetrachloro-m-xylene

R.T.: 4.119 min
Delta R.T.: -0.030 min
Response: 874093
Conc: 24.97 ng/ml m

Instrument :
ECD_O
ClientSampleId :
SB-14-COMP


Manual Integrations
APPROVED

Ankita
8/26/2019 3:09:19 PM

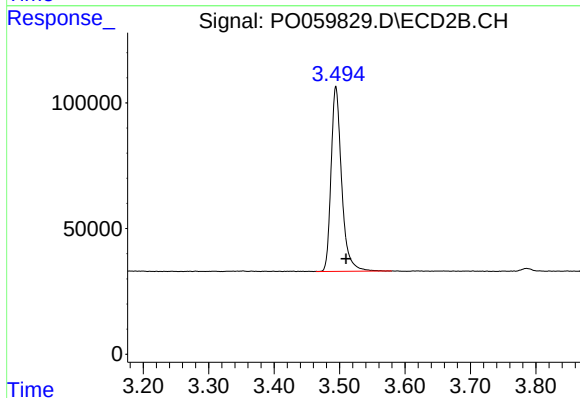


#1 Tetrachloro-m-xylene

R.T.: 3.494 min
Delta R.T.: -0.016 min
Response: 824241
Conc: 22.90 ng/ml

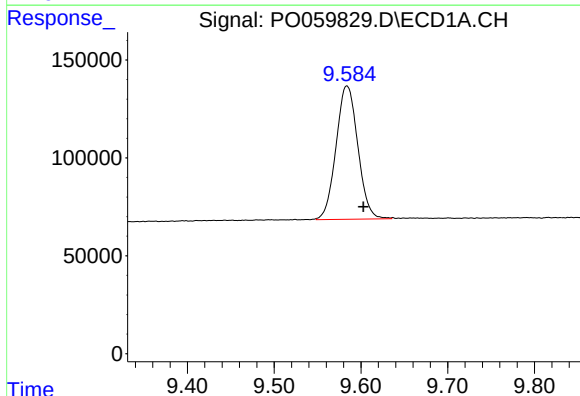

#2 Decachlorobiphenyl

R.T.: 9.584 min
Delta R.T.: -0.019 min
Response: 1189214
Conc: 22.35 ng/ml m

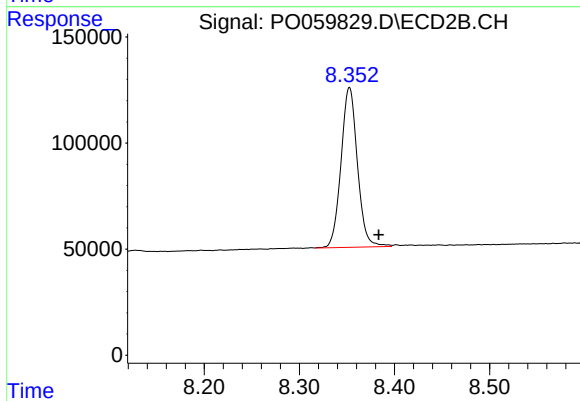

#2 Decachlorobiphenyl

R.T.: 8.352 min
Delta R.T.: -0.031 min
Response: 902879
Conc: 22.39 ng/ml m