

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090123\
 Data File : P0097624.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Sep 2023 11:22
 Operator : YP/AJ
 Sample : 04242-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 DEBRIS-CONCRETE-COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 01 12:45:32 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0082823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 29 10:29:21 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.444	3.625	64162050	13893620	19.224	20.594
2) SA Decachlor...	10.292	8.665	37928418	13282624	20.665	23.139

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO090123\
Data File : PO097624.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Sep 2023 11:22
Operator : YP/AJ
Sample : 04242-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
DEBRIS-CONCRETE-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 01 12:45:32 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO082823.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 29 10:29:21 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

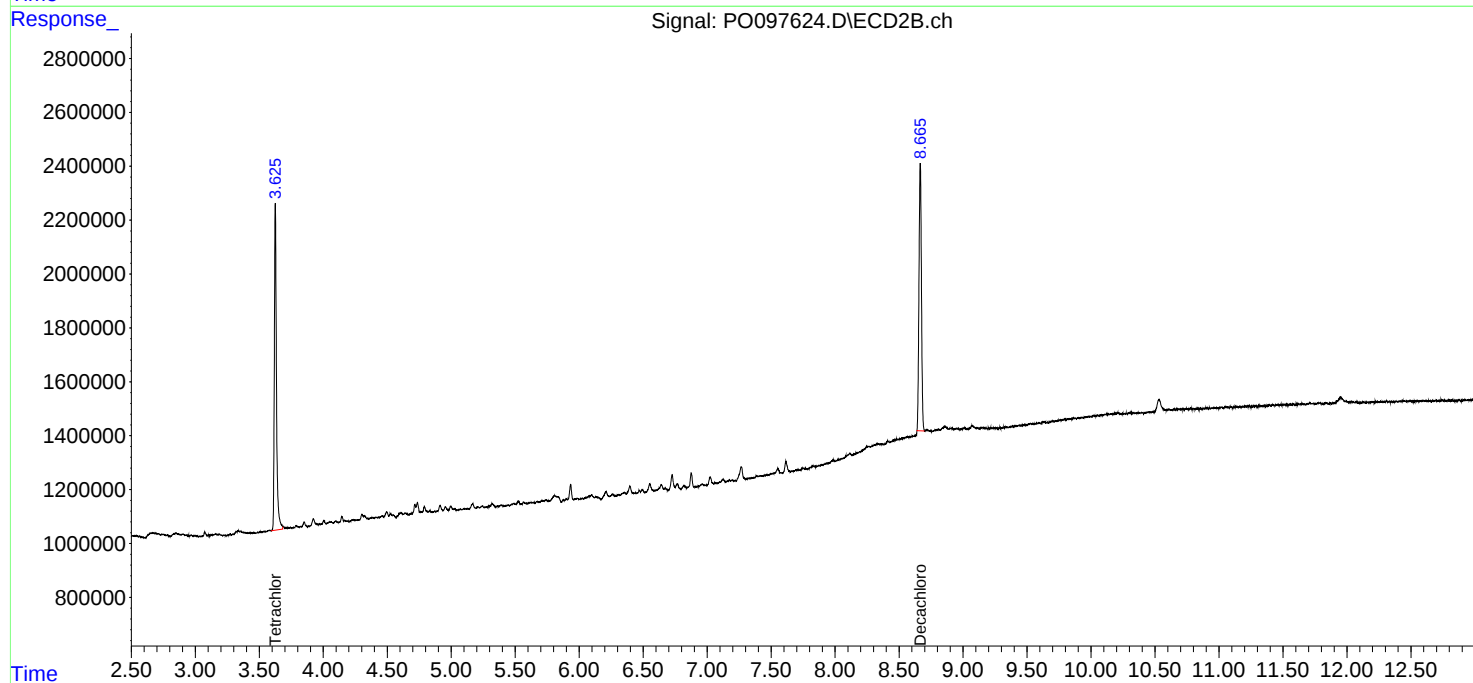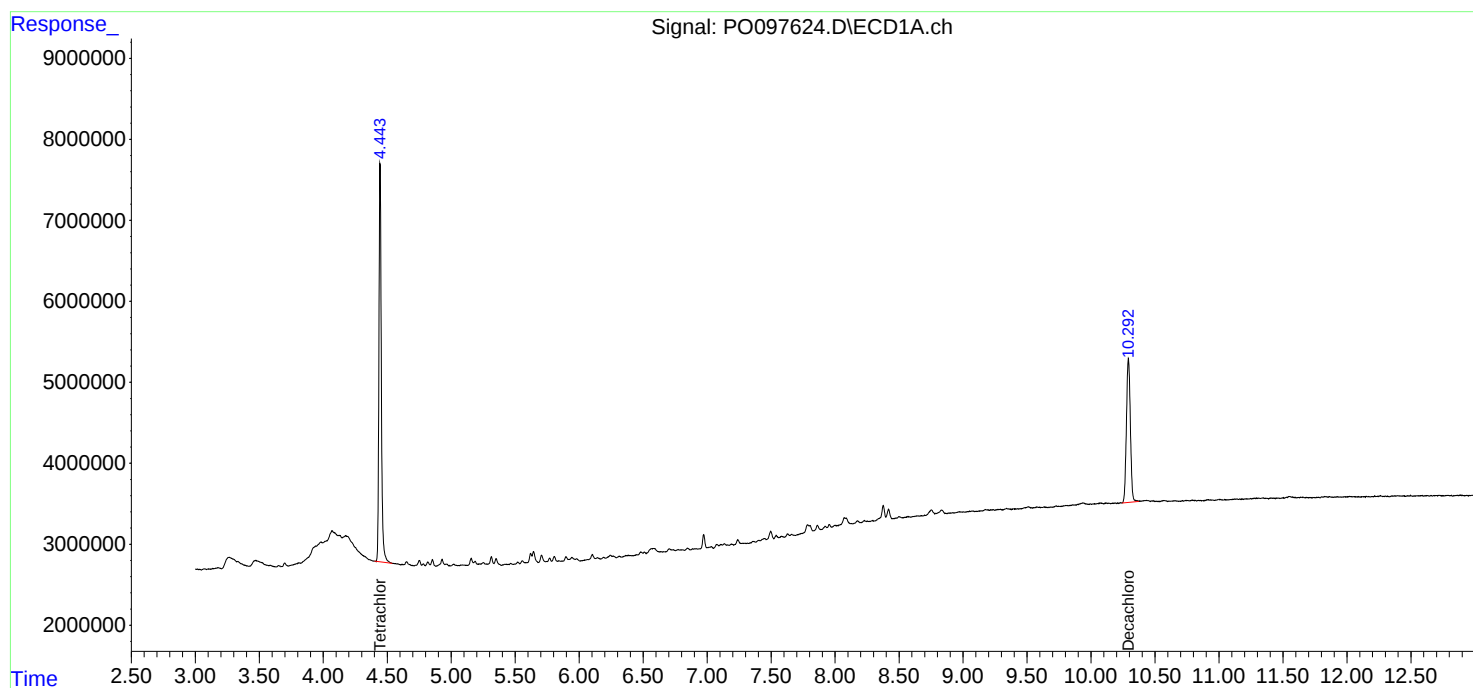


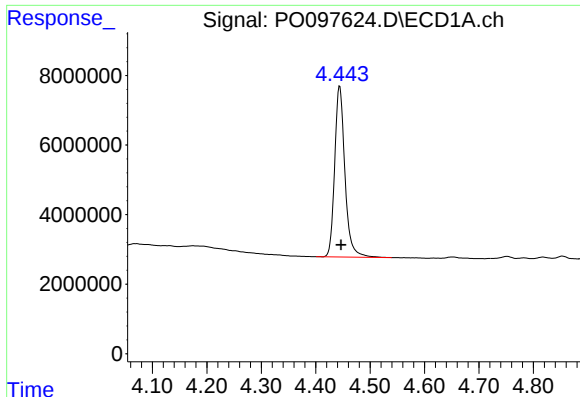

#1 Tetrachloro-m-xylene


R.T.: 4.444 min
Delta R.T.: -0.003 min
Response: 64162050
Conc: 19.22 ng/ml

Instrument :
ECD_O
ClientSampleId :
DEBRIS-CONCRETE-COMP

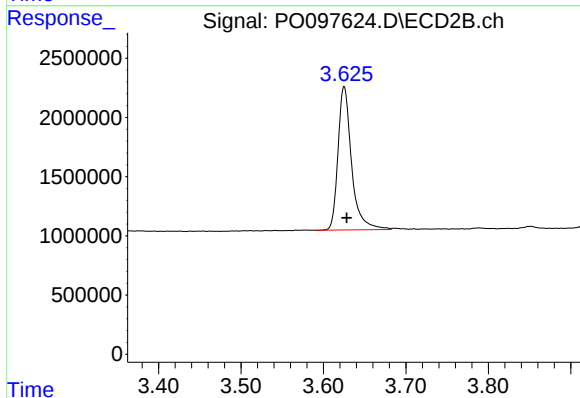


#1 Tetrachloro-m-xylene

R.T.: 3.625 min
Delta R.T.: -0.003 min
Response: 13893620
Conc: 20.59 ng/ml

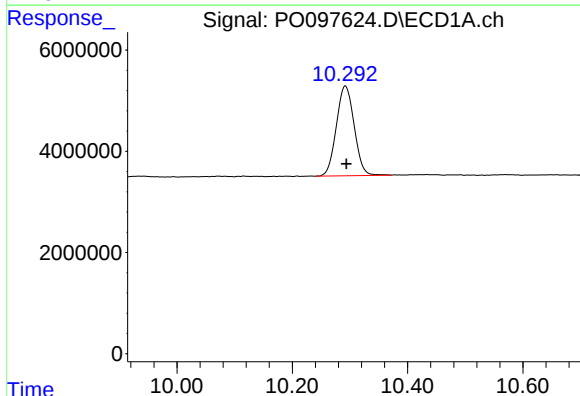

#2 Decachlorobiphenyl

R.T.: 10.292 min
Delta R.T.: -0.001 min
Response: 37928418
Conc: 20.67 ng/ml

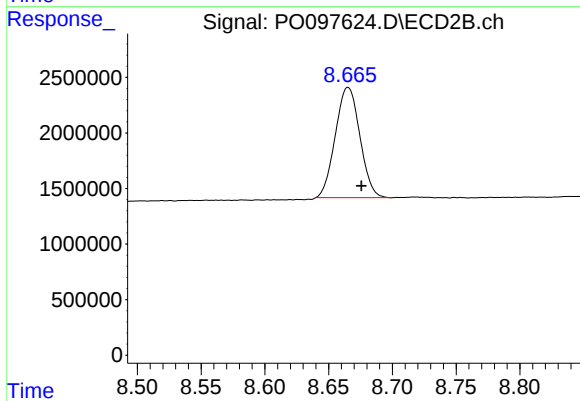

#2 Decachlorobiphenyl

R.T.: 8.665 min
Delta R.T.: -0.011 min
Response: 13282624
Conc: 23.14 ng/ml