

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090123\
 Data File : P0097646.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Sep 2023 18:41
 Operator : YP/AJ
 Sample : 04246-16 10X
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BC704970LOK-END-2-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 02 00:11:12 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0082823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 29 10:29:21 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.444	3.625	4494273	850891	1.347	1.261
2) SA Decachlor...	10.292	8.665	3723082	1292263	2.029m	2.251m

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO090123\
Data File : PO097646.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Sep 2023 18:41
Operator : YP/AJ
Sample : 04246-16 10X
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
BC704970LOK-END-2-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 02 00:11:12 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO082823.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 29 10:29:21 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

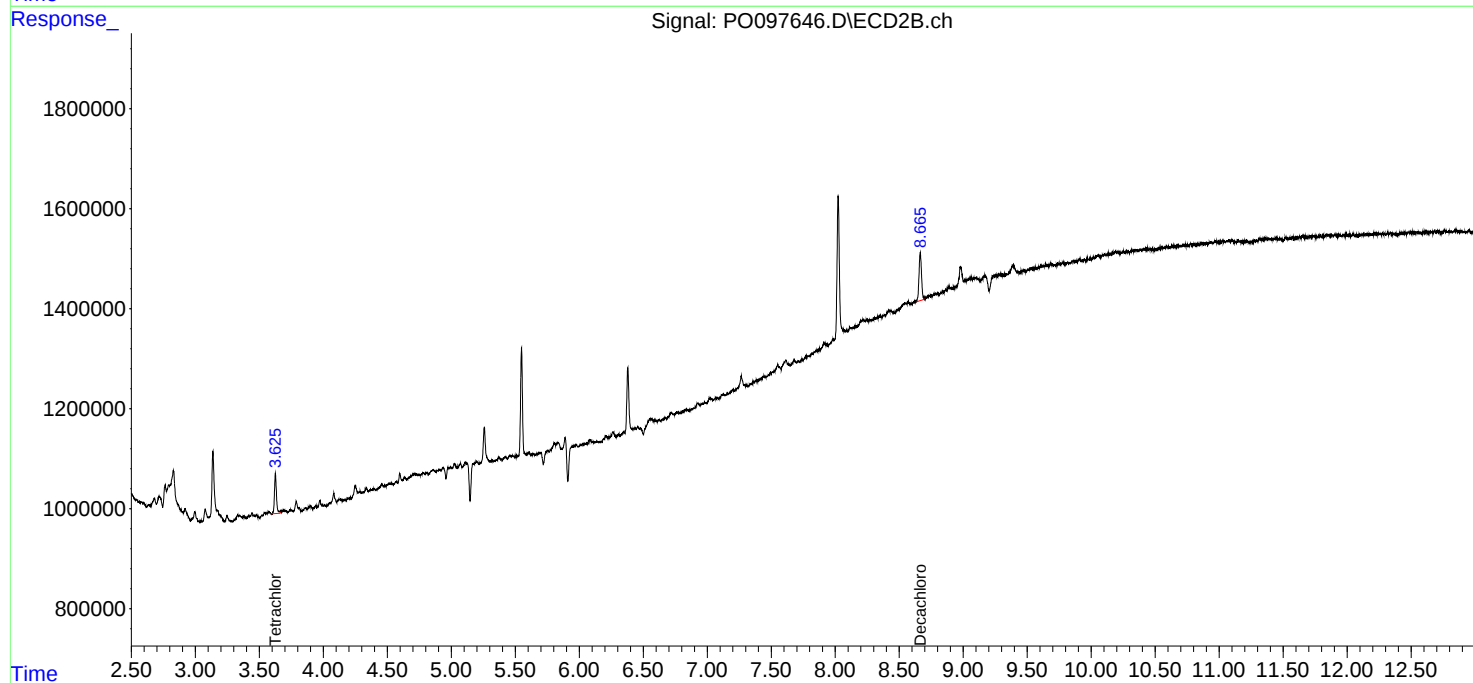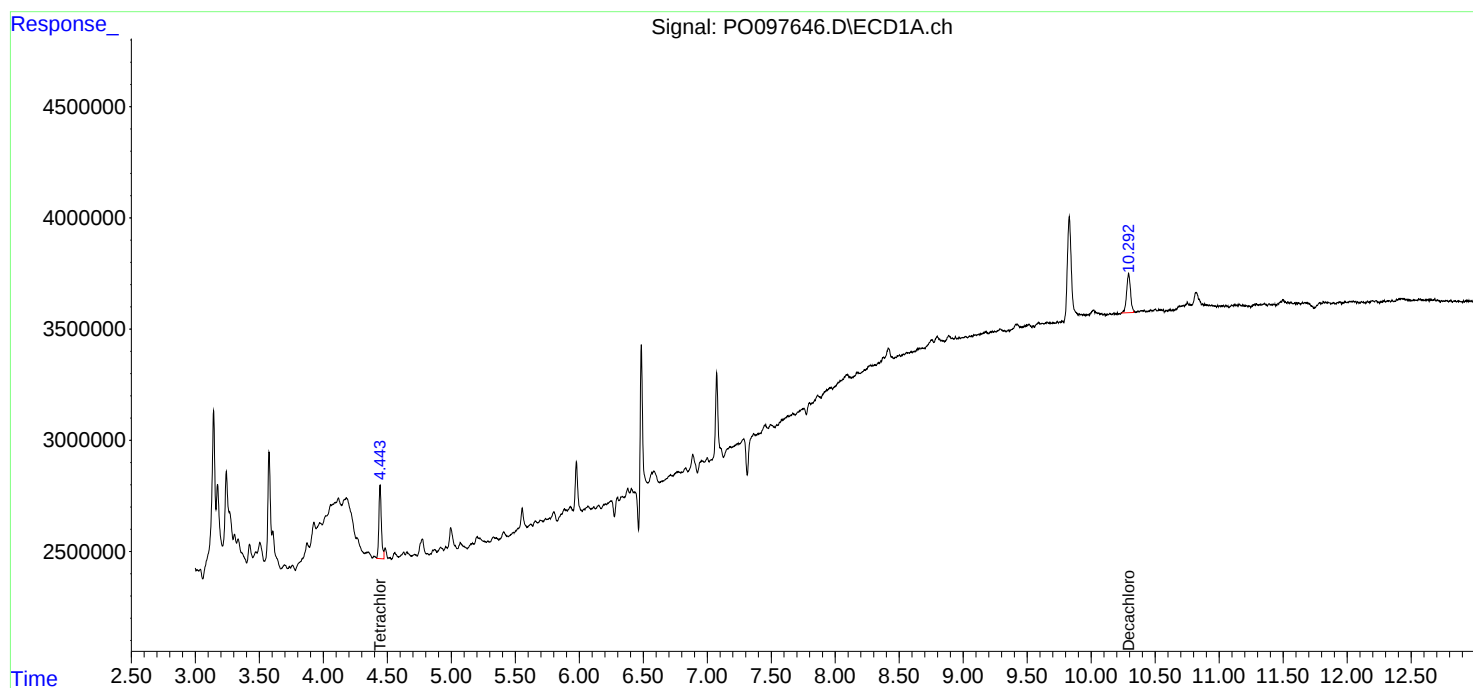


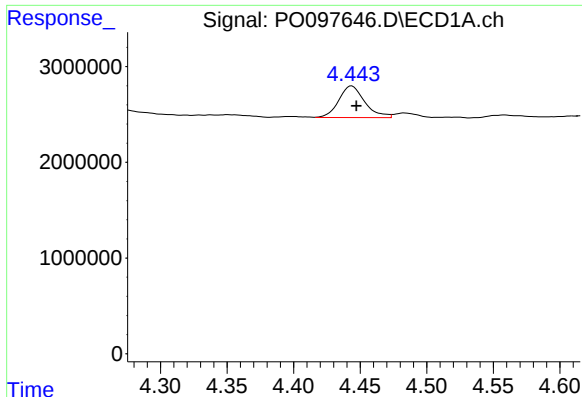

#1 Tetrachloro-m-xylene


R.T.: 4.444 min
Delta R.T.: -0.003 min
Response: 4494273
Conc: 1.35 ng/ml

Instrument :
ECD_O
ClientSampleId :
BC704970LOK-END-2-2

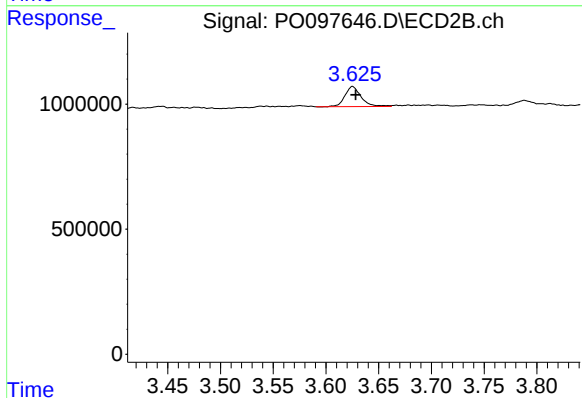


#1 Tetrachloro-m-xylene

R.T.: 3.625 min
Delta R.T.: -0.003 min
Response: 850891
Conc: 1.26 ng/ml

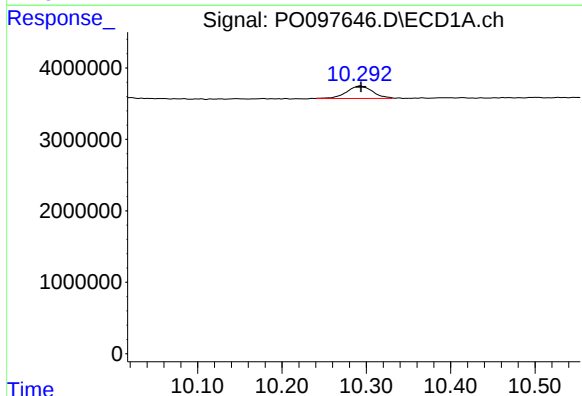

#2 Decachlorobiphenyl

R.T.: 10.292 min
Delta R.T.: -0.001 min
Response: 3723082
Conc: 2.03 ng/ml m

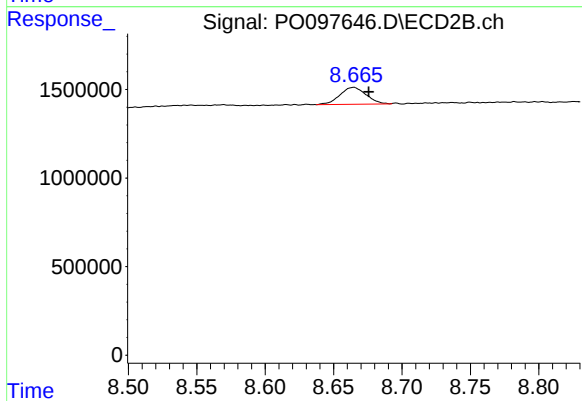

#2 Decachlorobiphenyl

R.T.: 8.665 min
Delta R.T.: -0.011 min
Response: 1292263
Conc: 2.25 ng/ml m