

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090123\
 Data File : P0097652.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Sep 2023 21:27
 Operator : YP/AJ
 Sample : 04246-17 10X
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BC122903LOK-END-1-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/05/2023
 Supervised By :Ankita Jodhani 09/05/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 02 00:18:55 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0082823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 29 10:29:21 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.443	3.623	4772641	1066366	1.430	1.581m
2) SA Decachlor...	10.288	8.662	3644831	1376255	1.986m	2.397m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO090123\
Data File : PO097652.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Sep 2023 21:27
Operator : YP/AJ
Sample : 04246-17 10X
Misc :
ALS Vial : 27 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
BC122903LOK-END-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/05/2023
Supervised By :Ankita Jodhani 09/05/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 02 00:18:55 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO082823.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 29 10:29:21 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

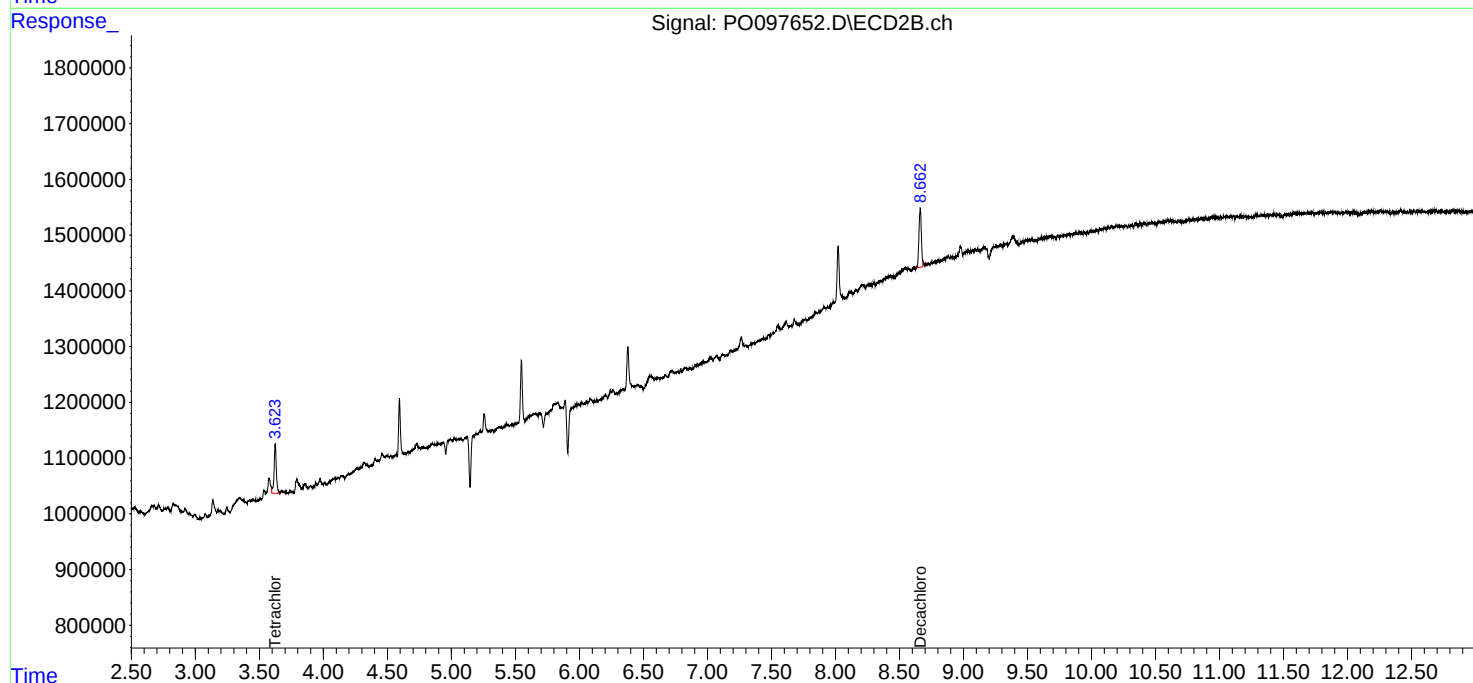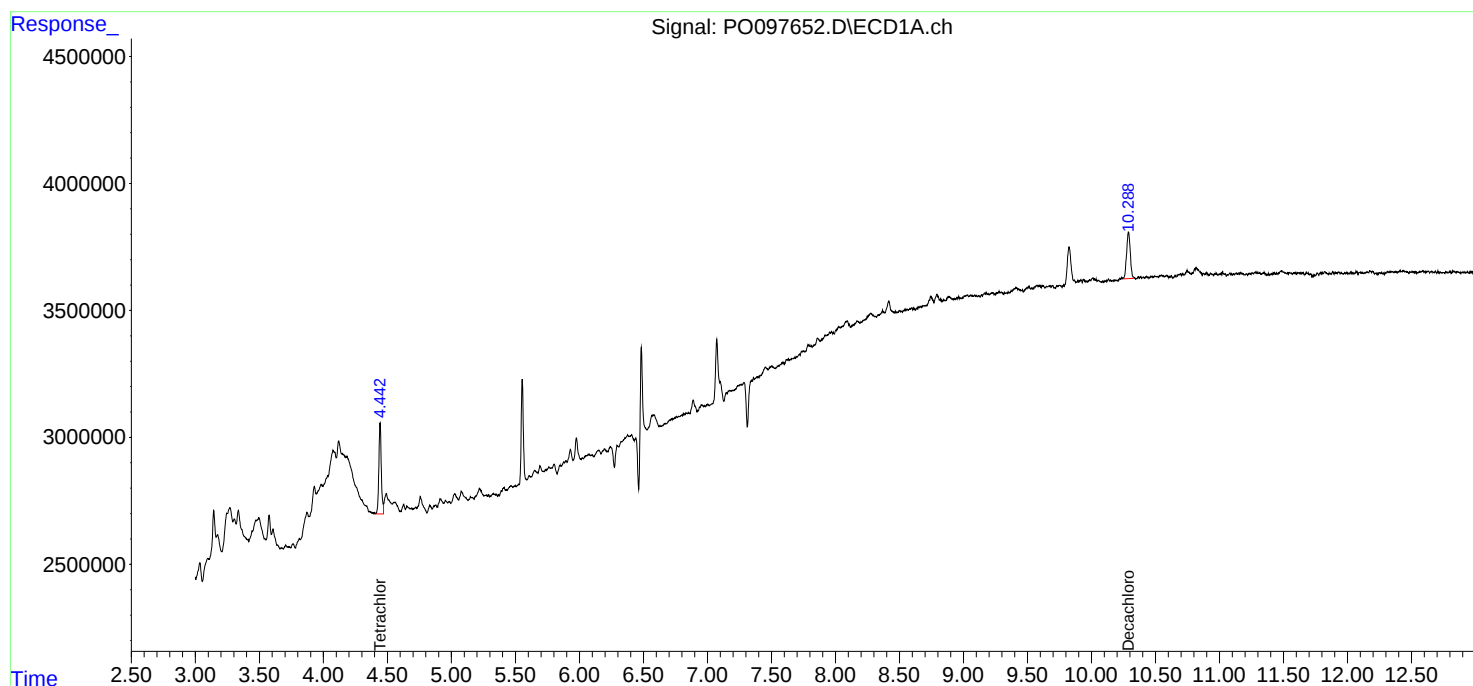

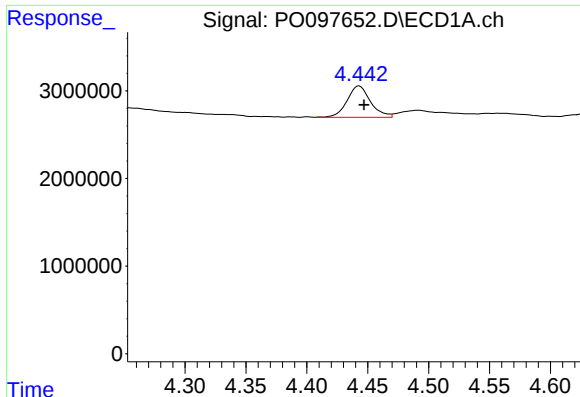


#1 Tetrachloro-m-xylene

R.T.: 4.443 min
Delta R.T.: -0.004 min
Response: 4772641
Conc: 1.43 ng/ml

Instrument :
ECD_O
ClientSampleId :
BC122903LOK-END-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/05/2023
Supervised By :Ankita Jodhani 09/05/2023

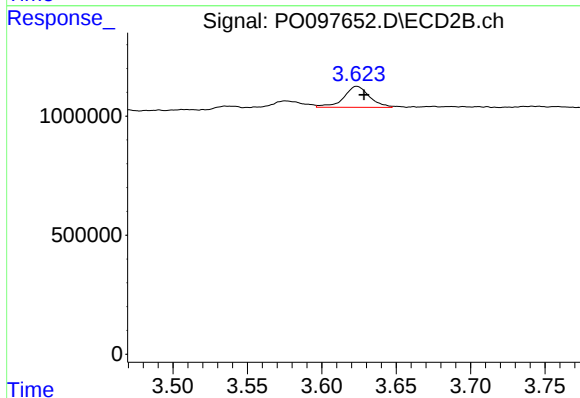


#1 Tetrachloro-m-xylene

R.T.: 3.623 min
Delta R.T.: -0.005 min
Response: 1066366
Conc: 1.58 ng/ml m

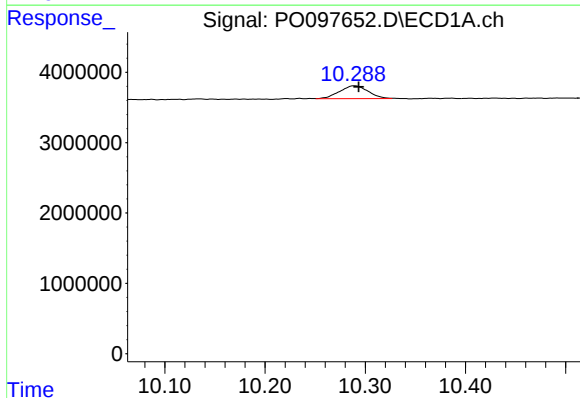

#2 Decachlorobiphenyl

R.T.: 10.288 min
Delta R.T.: -0.005 min
Response: 3644831
Conc: 1.99 ng/ml m

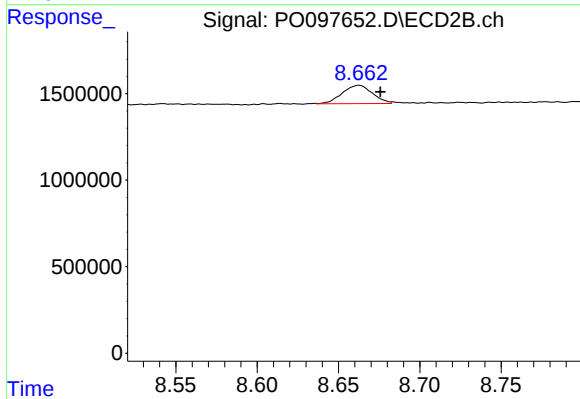

#2 Decachlorobiphenyl

R.T.: 8.662 min
Delta R.T.: -0.014 min
Response: 1376255
Conc: 2.40 ng/ml m