

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0090123\
 Data File : P0097676.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Sep 2023 05:17
 Operator : YP/AJ
 Sample : 04258-01
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 PAINT-CHIPS-COMP

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/05/2023
 Supervised By :Ankita Jodhani 09/05/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 02 05:55:42 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0082823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 29 10:29:21 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.442	3.623	61875325	13248780	18.539	19.639
2) SA Decachlor...	10.288	8.659	44552100	15382254	24.274	26.797m
Target Compounds						
26) L6 AR-1254-1	6.480	5.520	5506839	3765442	50.089m	97.562m#
27) L6 AR-1254-2	6.701	5.669	13605413	2437745	83.489	71.570m
28) L6 AR-1254-3	7.077	6.074	13040151	3323163	80.072m	62.631m
29) L6 AR-1254-4	7.360	6.302	6126099	2133538	62.851m	78.242m
30) L6 AR-1254-5	7.803	6.723	70021007	23119983	620.077m	524.393m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO090123\
Data File : PO097676.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Sep 2023 05:17
Operator : YP/AJ
Sample : 04258-01
Misc :
ALS Vial : 46 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PAINT-CHIPS-COMP


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/05/2023
Supervised By :Ankita Jodhani 09/05/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 02 05:55:42 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO082823.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 29 10:29:21 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

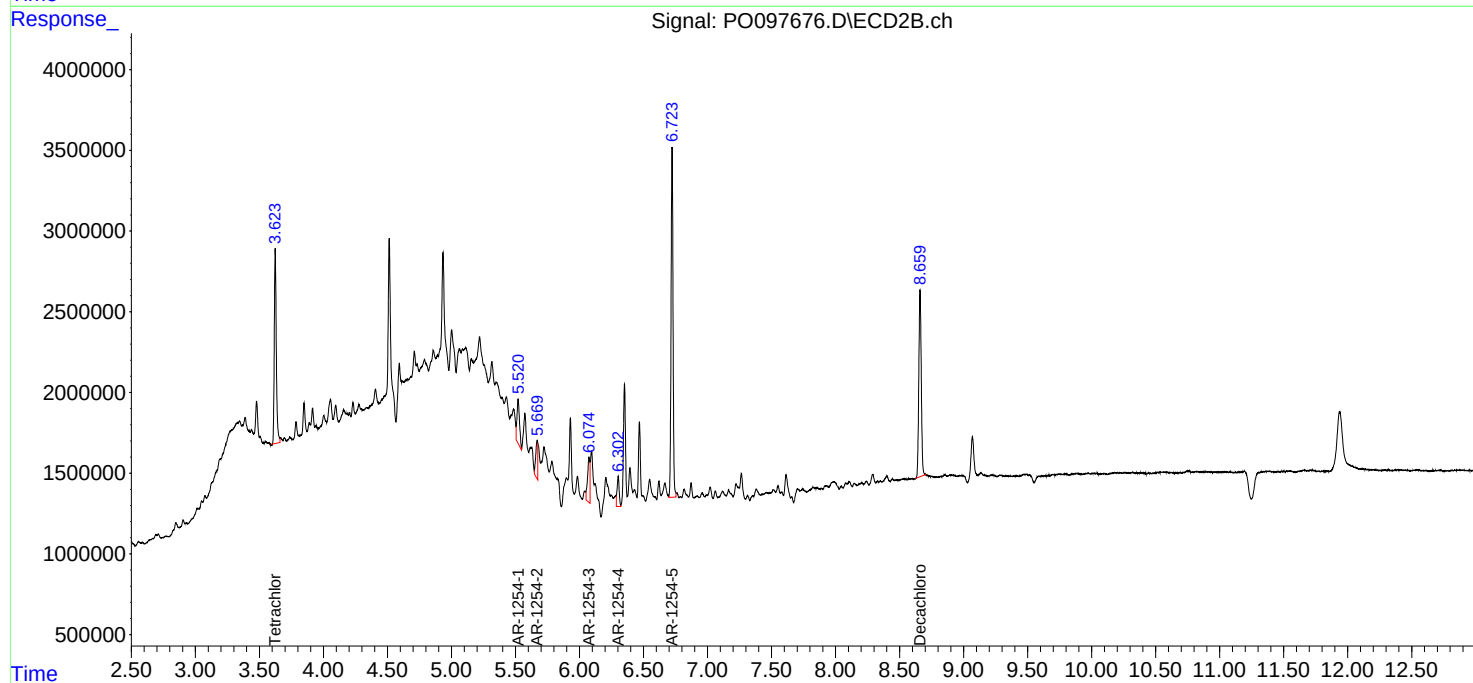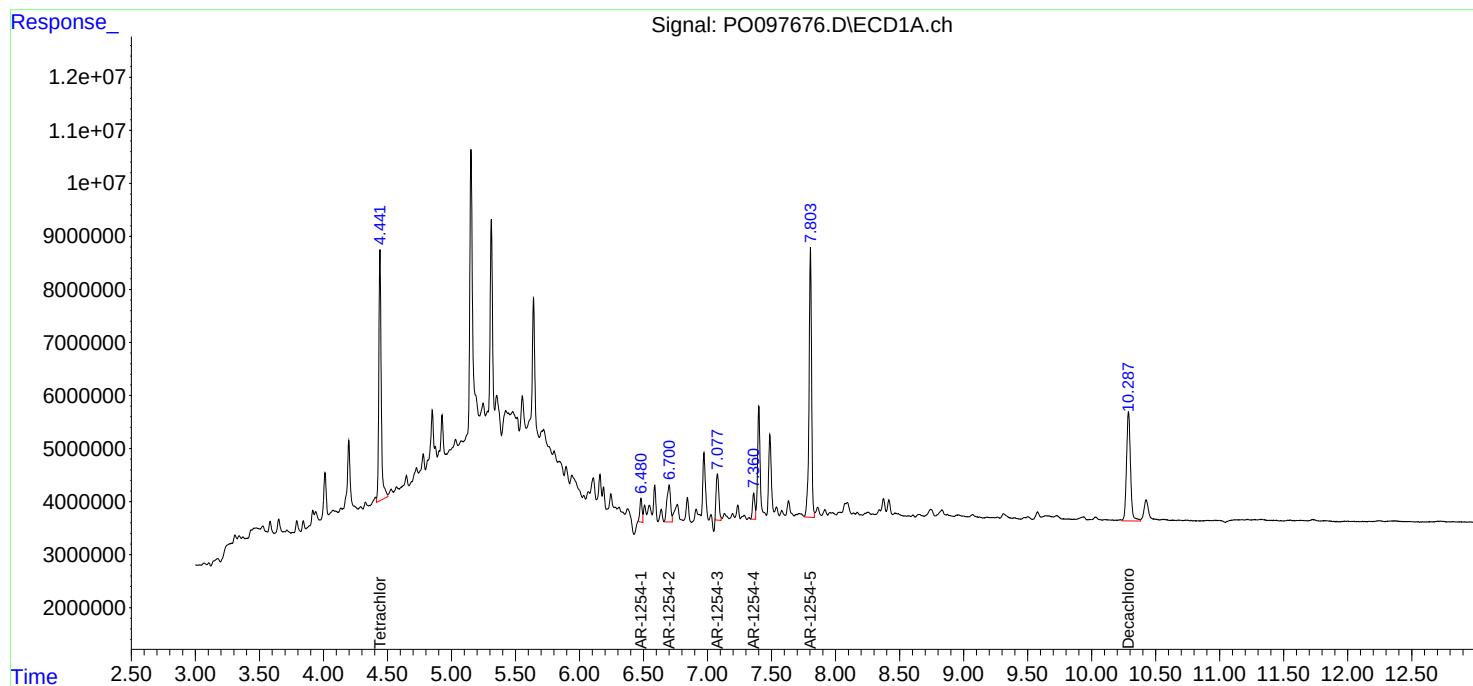

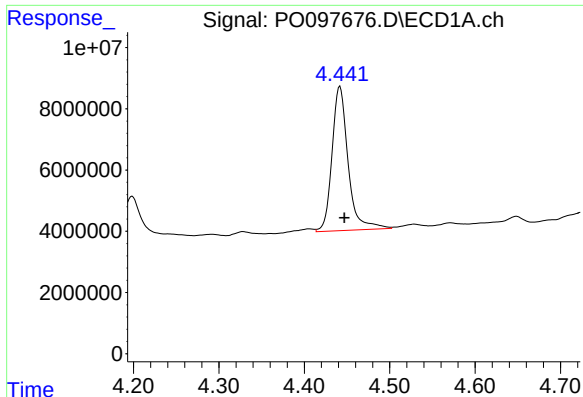


#1 Tetrachloro-m-xylene

R.T.: 4.442 min
Delta R.T.: -0.005 min
Response: 61875325
Conc: 18.54 ng/ml

Instrument :
ECD_O
ClientSampleId :
PAINT-CHIPS-COMP


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/05/2023
Supervised By :Ankita Jodhani 09/05/2023

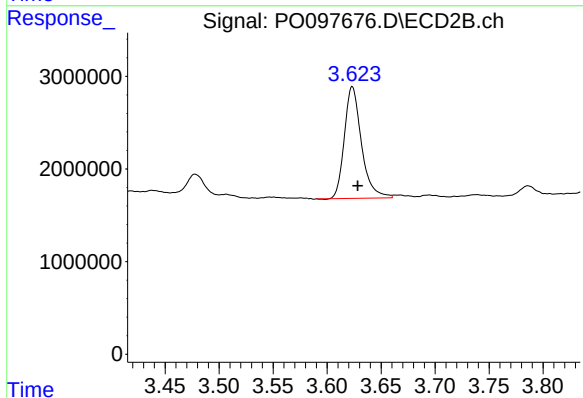


#1 Tetrachloro-m-xylene

R.T.: 3.623 min
Delta R.T.: -0.005 min
Response: 13248780
Conc: 19.64 ng/ml

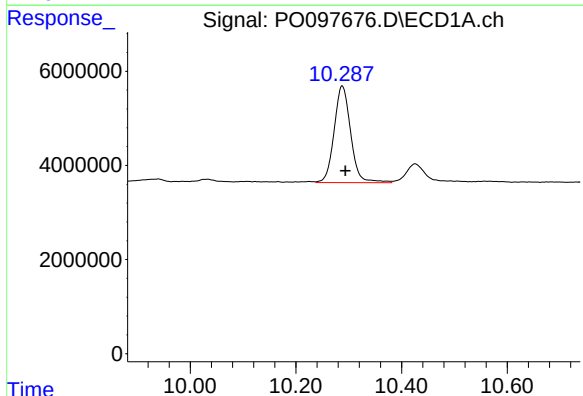


#2 Decachlorobiphenyl

R.T.: 10.288 min
Delta R.T.: -0.006 min
Response: 44552100
Conc: 24.27 ng/ml

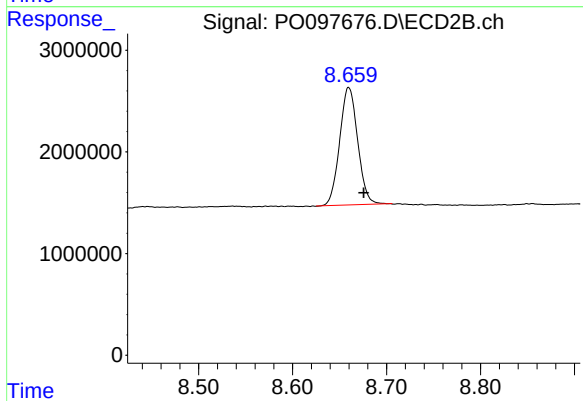

#2 Decachlorobiphenyl

R.T.: 8.659 min
Delta R.T.: -0.017 min
Response: 15382254
Conc: 26.80 ng/ml m

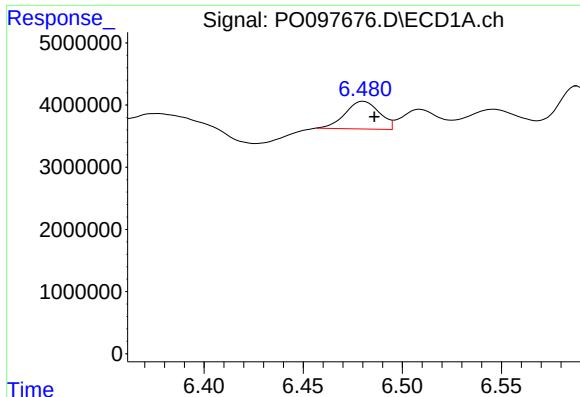


#26 AR-1254-1

R.T.: 6.480 min
Delta R.T.: -0.006 min
Response: 5506839
Conc: 50.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
PAINT-CHIPS-COMP


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/05/2023
Supervised By :Ankita Jodhani 09/05/2023

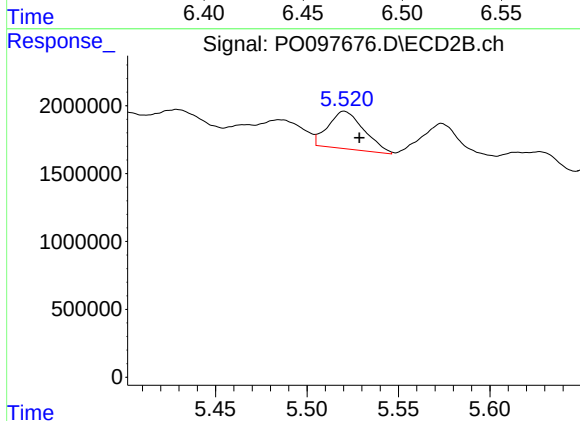


#26 AR-1254-1

R.T.: 5.520 min
Delta R.T.: -0.008 min
Response: 3765442
Conc: 97.56 ng/ml m

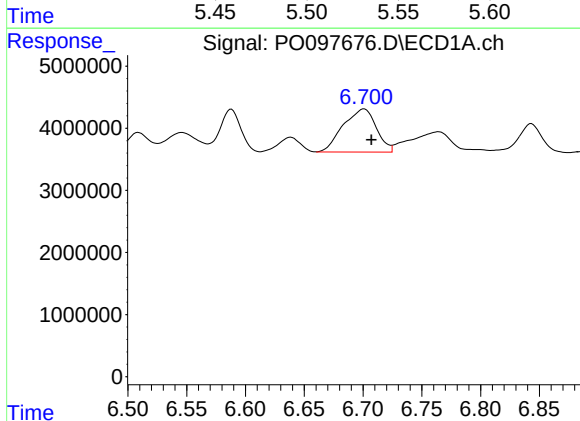


#27 AR-1254-2

R.T.: 6.701 min
Delta R.T.: -0.006 min
Response: 13605413
Conc: 83.49 ng/ml

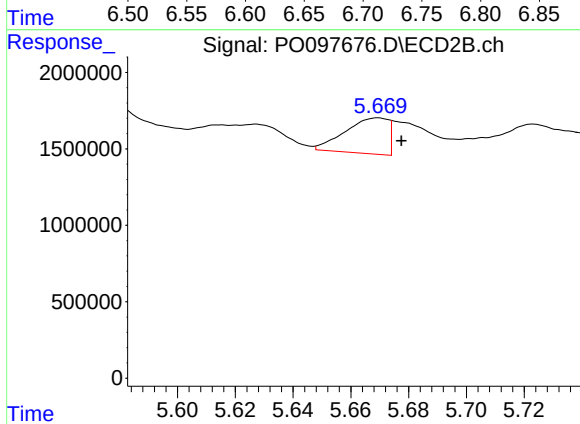

#27 AR-1254-2

R.T.: 5.669 min
Delta R.T.: -0.008 min
Response: 2437745
Conc: 71.57 ng/ml m

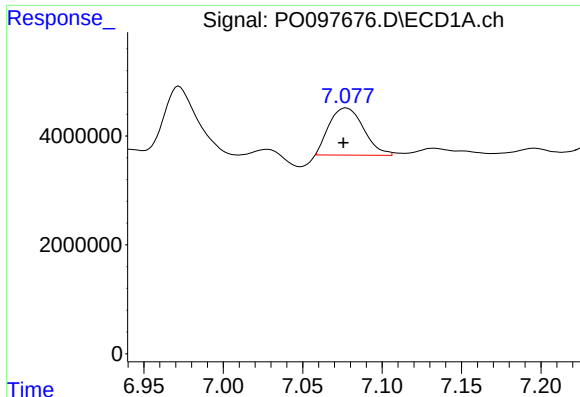


#28 AR-1254-3

R.T.: 7.077 min
Delta R.T.: 0.001 min
Response: 13040151
Conc: 80.07 ng/ml

Instrument :
ECD_O
ClientSampleId :
PAINT-CHIPS-COMP


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/05/2023
Supervised By :Ankita Jodhani 09/05/2023

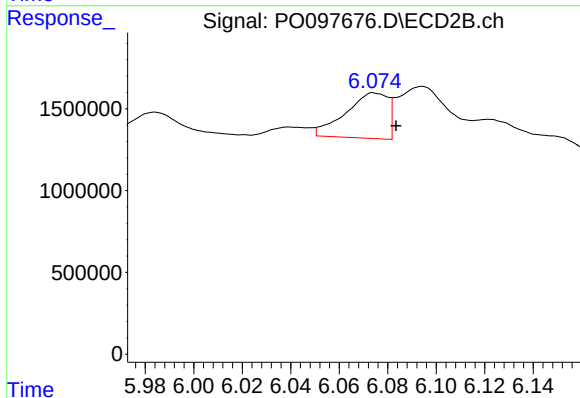


#28 AR-1254-3

R.T.: 6.074 min
Delta R.T.: -0.010 min
Response: 3323163
Conc: 62.63 ng/ml m

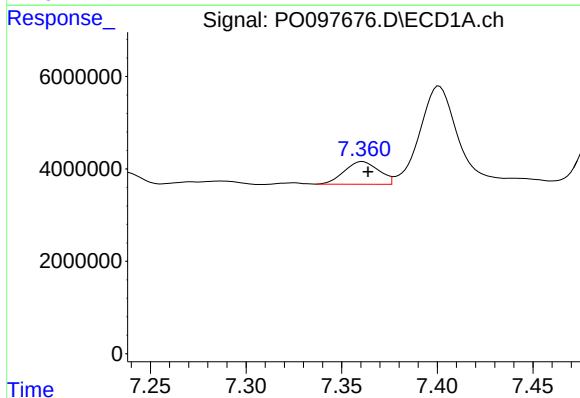


#29 AR-1254-4

R.T.: 7.360 min
Delta R.T.: -0.003 min
Response: 6126099
Conc: 62.85 ng/ml m

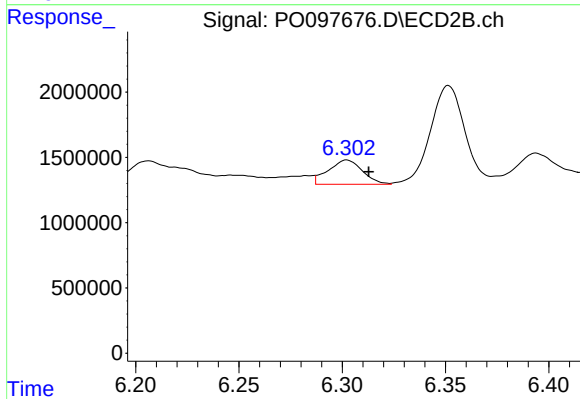

#29 AR-1254-4

R.T.: 6.302 min
Delta R.T.: -0.011 min
Response: 2133538
Conc: 78.24 ng/ml m

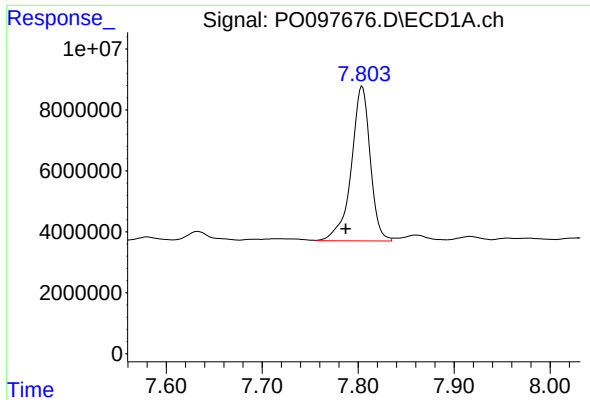


#30 AR-1254-5

R.T.: 7.803 min
Delta R.T.: 0.016 min
Response: 70021007
Conc: 620.08 ng/ml

Instrument :
ECD_O
ClientSampleId :
PAINT-CHIPS-COMP

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/05/2023
Supervised By :Ankita Jodhani 09/05/2023

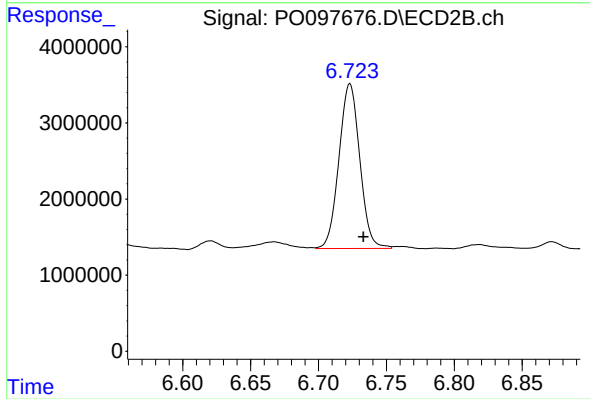

#30 AR-1254-5

R.T.: 6.723 min
Delta R.T.: -0.010 min
Response: 23119983
Conc: 524.39 ng/ml m