

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0090225\
 Data File : P0113385.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Sep 2025 12:25
 Operator : YP/AJ
 Sample : PB169484BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB169484BL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/03/2025
 Supervised By :mohammad ahmed 09/04/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 02 14:12:53 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 19 06:08:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.659	3.650	160.8E6	93954049	19.644	18.566m
2) SA Decachlor...	8.675	8.620	133.0E6	37226417	19.184	19.646

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO090225\
Data File : PO113385.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Sep 2025 12:25
Operator : YP/AJ
Sample : PB169484BL
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PB169484BL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/03/2025
Supervised By :mohammad ahmed 09/04/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 02 14:12:53 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 19 06:08:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

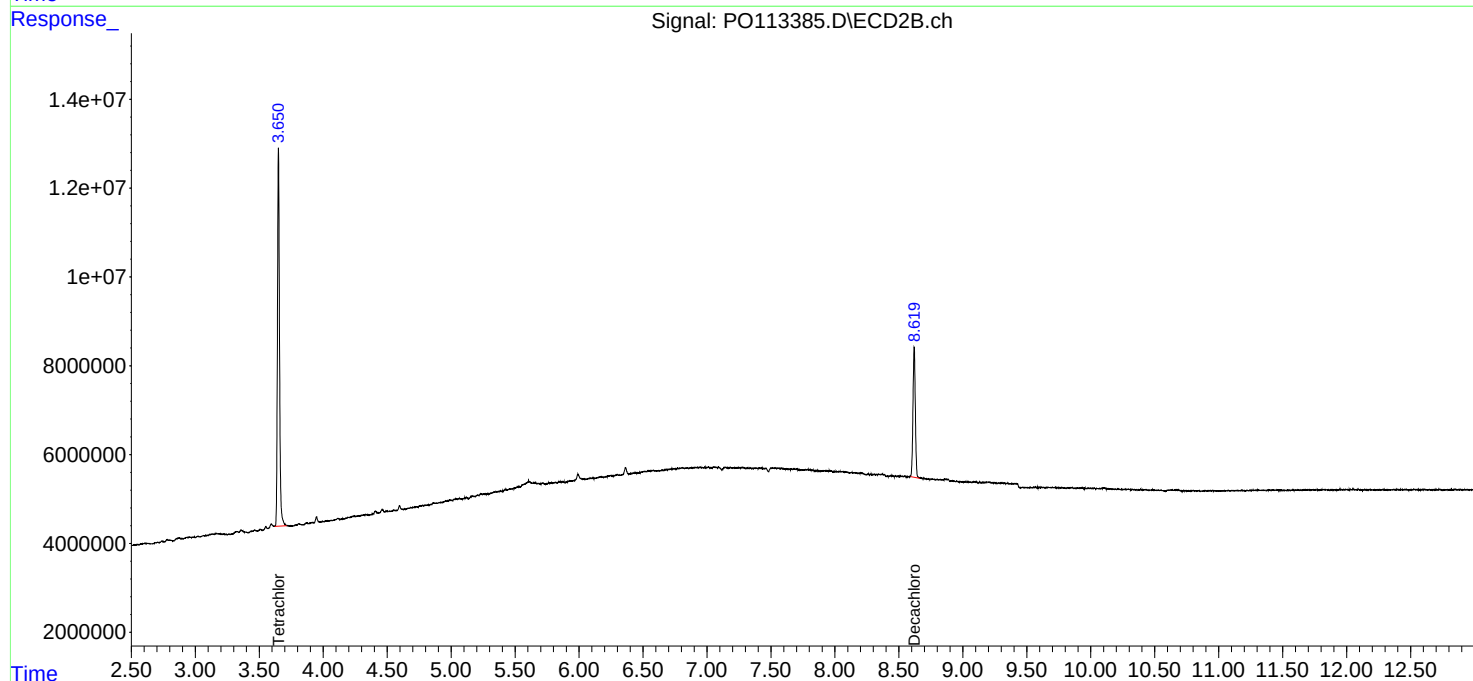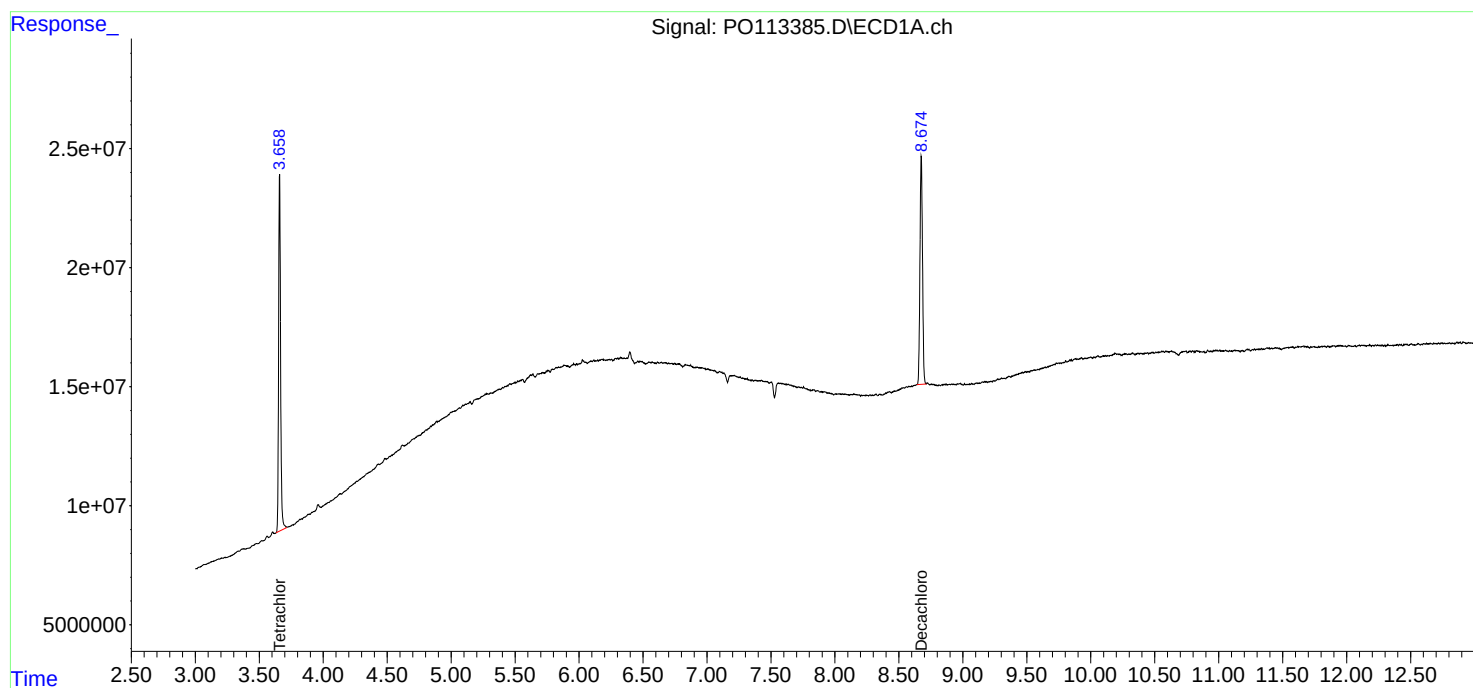

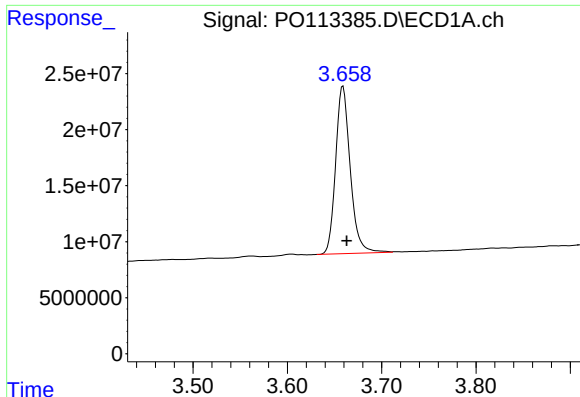


#1 Tetrachloro-m-xylene

R.T.: 3.659 min
Delta R.T.: -0.004 min
Response: 160814027
Conc: 19.64 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB169484BL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/03/2025
Supervised By :mohammad ahmed 09/04/2025

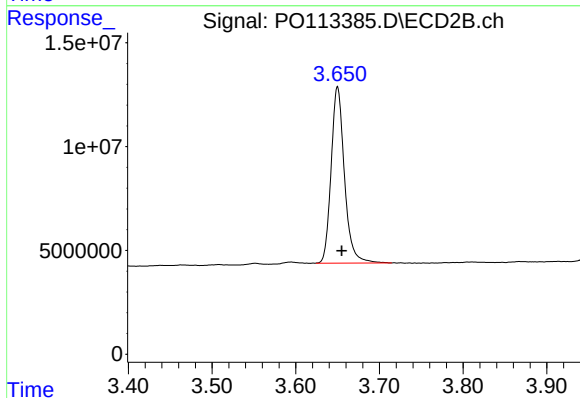


#1 Tetrachloro-m-xylene

R.T.: 3.650 min
Delta R.T.: -0.005 min
Response: 93954049
Conc: 18.57 ng/ml m

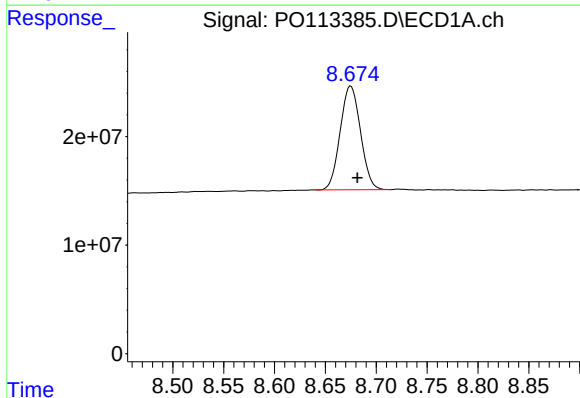

#2 Decachlorobiphenyl

R.T.: 8.675 min
Delta R.T.: -0.007 min
Response: 132969470
Conc: 19.18 ng/ml

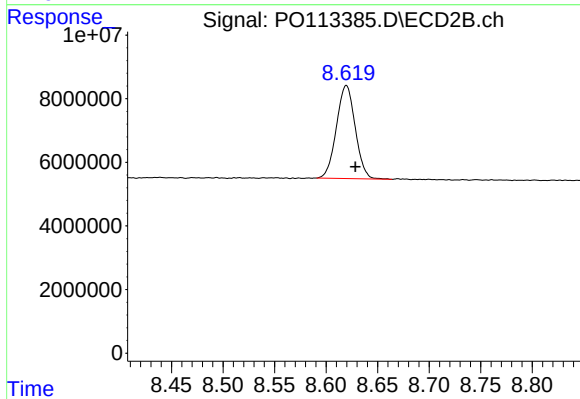

#2 Decachlorobiphenyl

R.T.: 8.620 min
Delta R.T.: -0.009 min
Response: 37226417
Conc: 19.65 ng/ml