

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092518\
 Data File : P0049276.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Sep 2018 13:29
 Operator : SM/SJ
 Sample : J5042-04
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 NYSEG-CLRK-PH4-A9-B1

Manual Integrations
 APPROVED

Sohil
 9/26/2018 11:52:03 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 26 01:00:52 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091918.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Sep 20 02:02:28 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.391	3.523	2965894	3261817	15.973m	15.784m
2) SA Decachlor...	10.102	8.455	2322271	1722504	8.448m	8.414

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO092518\
Data File : PO049276.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Sep 2018 13:29
Operator : SM/SJ
Sample : J5042-04
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
NYSEG-CLRK-PH4-A9-B1


Manual Integrations
APPROVED

Sohil
9/26/2018 11:52:03 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 26 01:00:52 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091918.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Sep 20 02:02:28 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

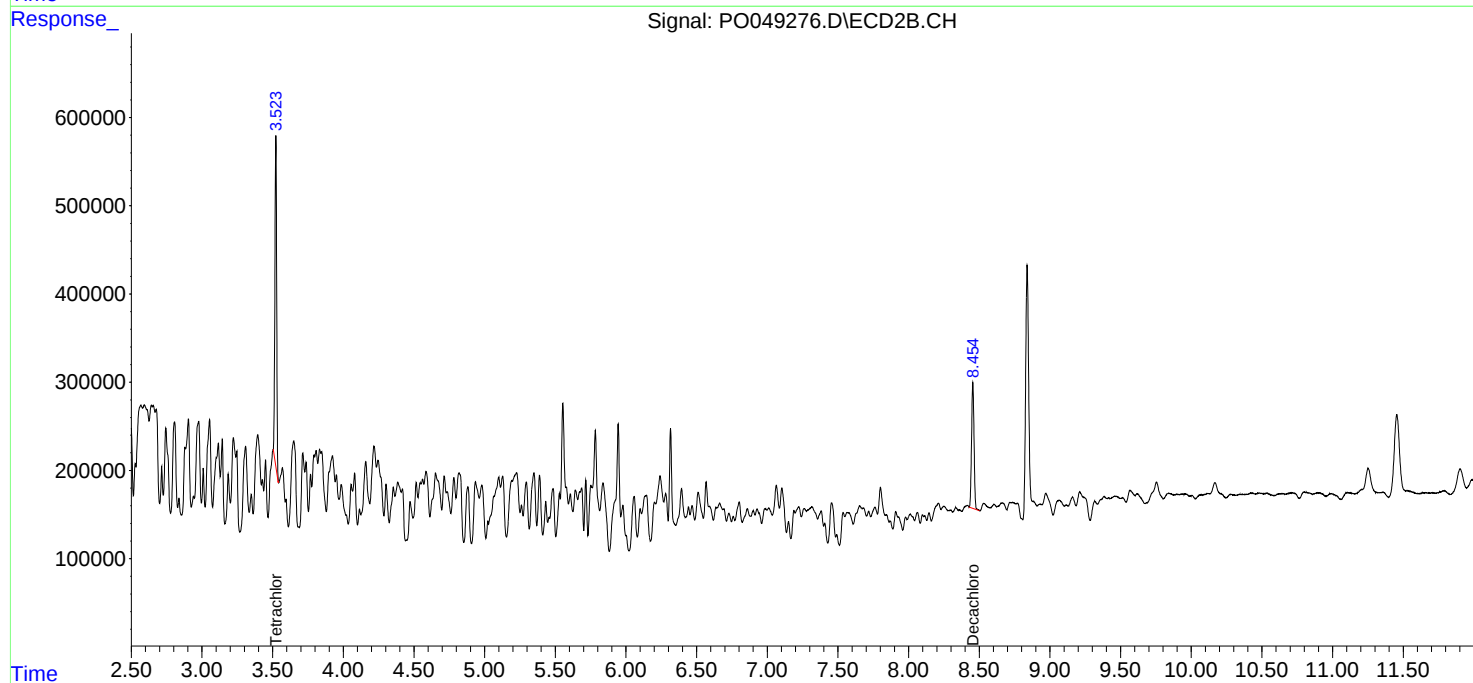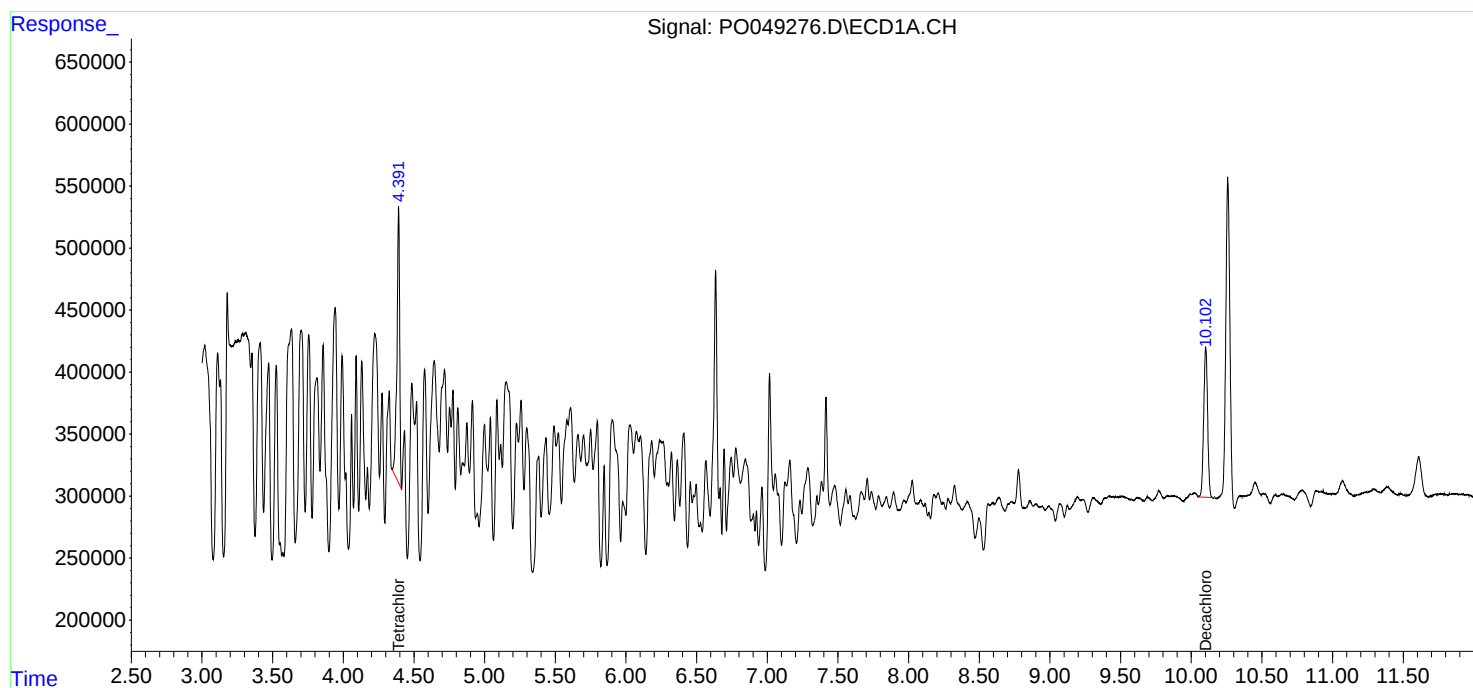

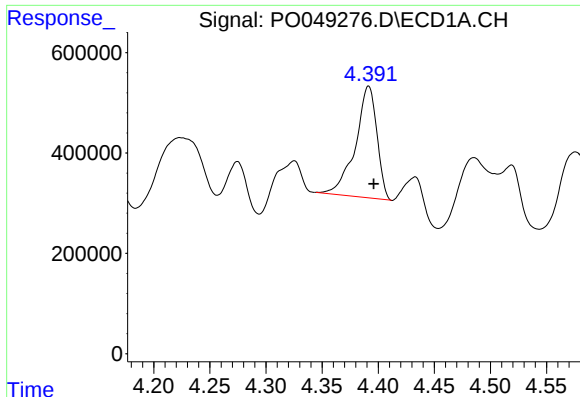


#1 Tetrachloro-m-xylene

R.T.: 4.391 min
Delta R.T.: -0.005 min
Response: 2965894
Conc: 15.97 ng/ml m

Instrument :
ECD_O
ClientSampleId :
NYSEG-CLRK-PH4-A9-B1


Manual Integrations
APPROVED

Sohil
9/26/2018 11:52:03 AM

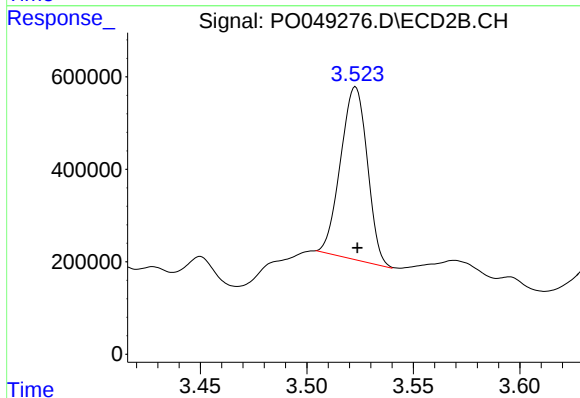


#1 Tetrachloro-m-xylene

R.T.: 3.523 min
Delta R.T.: -0.001 min
Response: 3261817
Conc: 15.78 ng/ml m

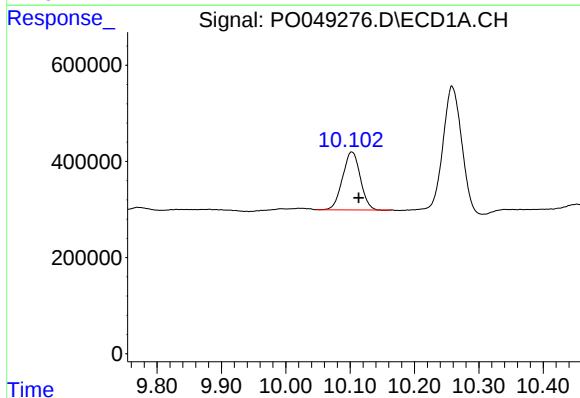

#2 Decachlorobiphenyl

R.T.: 10.102 min
Delta R.T.: -0.012 min
Response: 2322271
Conc: 8.45 ng/ml m

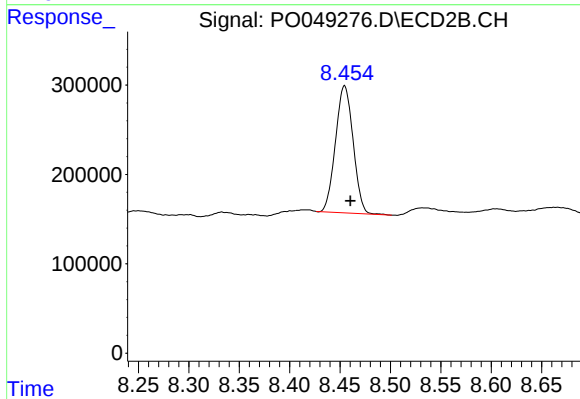

#2 Decachlorobiphenyl

R.T.: 8.455 min
Delta R.T.: -0.006 min
Response: 1722504
Conc: 8.41 ng/ml