

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092518\
 Data File : P0049281.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Sep 2018 15:50
 Operator : SM/SJ
 Sample : J5042-04RE
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 NYSEG-CLRK-PH4-A9-B1RE

Manual Integrations
 APPROVED

Sohil
 9/26/2018 11:52:07 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 26 01:05:03 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091918.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Sep 20 02:02:28 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.399	3.525	3158674	3313478	17.012m	16.034m
2) SA Decachlor...	10.114	8.459	2489105	1850961	9.055	9.042

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO092518\
Data File : PO049281.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Sep 2018 15:50
Operator : SM/SJ
Sample : J5042-04RE
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
NYSEG-CLRK-PH4-A9-B1RE


Manual Integrations
APPROVED

Sohil
9/26/2018 11:52:07 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 26 01:05:03 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091918.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Sep 20 02:02:28 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

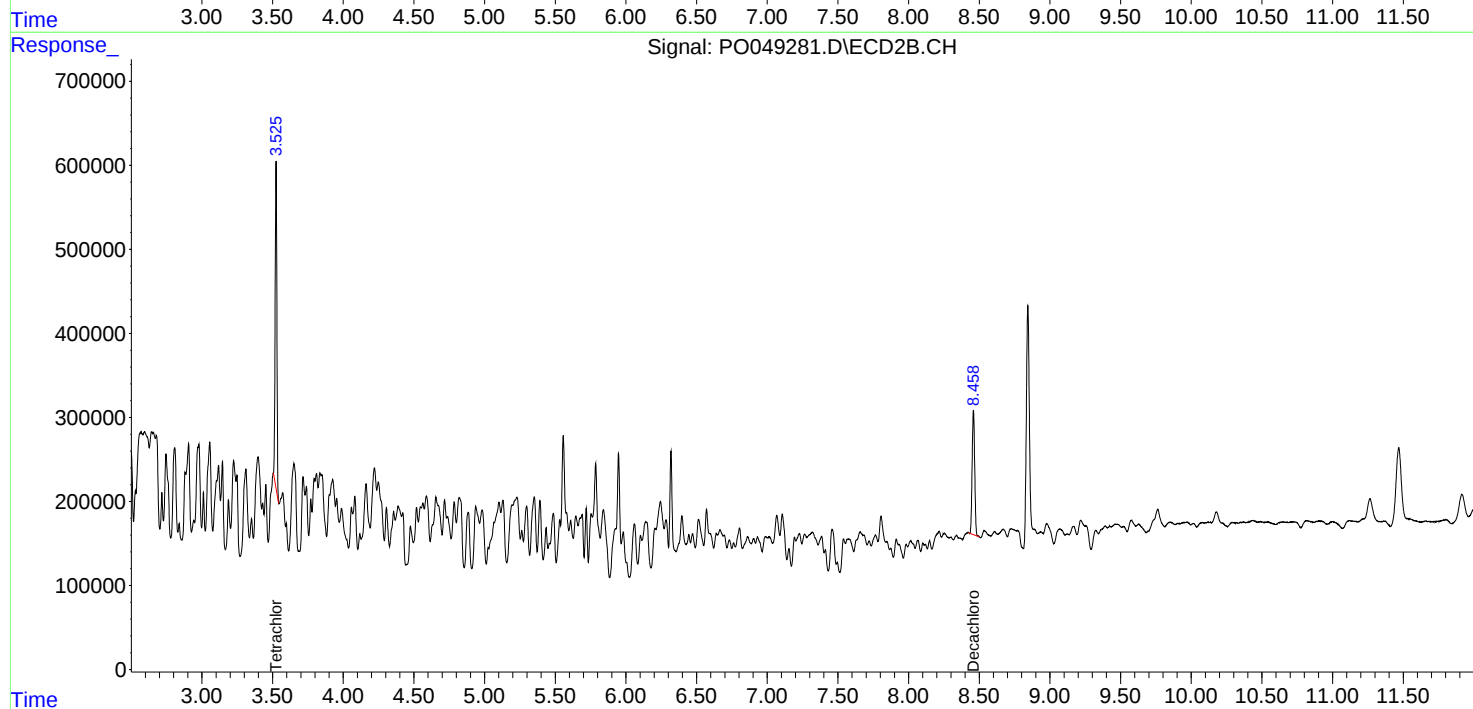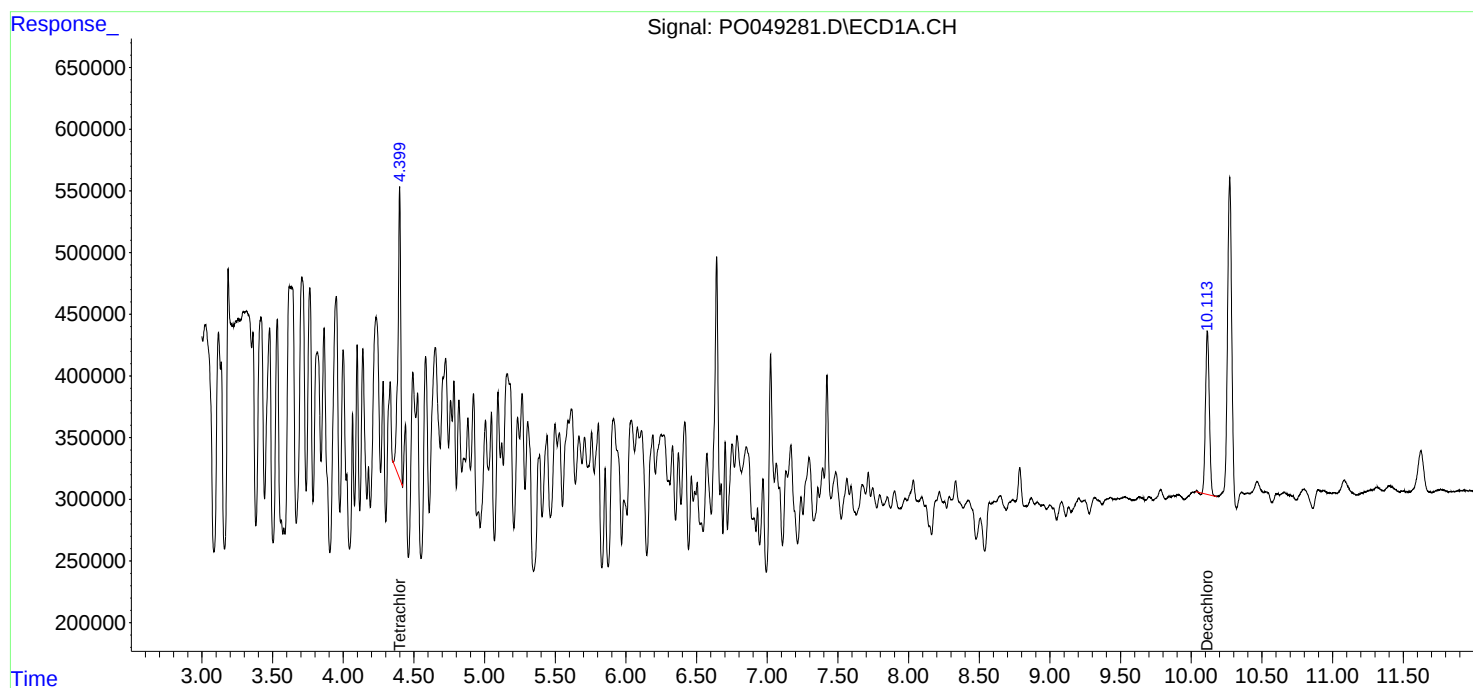

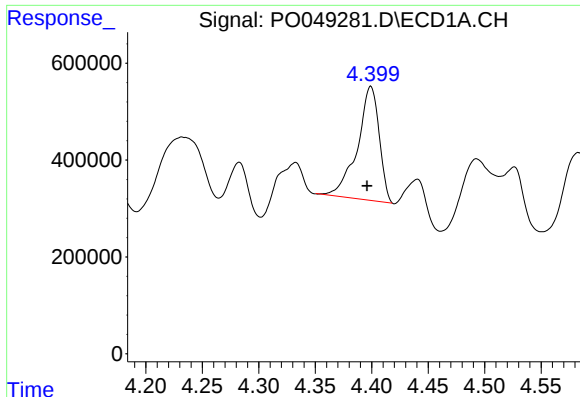


#1 Tetrachloro-m-xylene

R.T.: 4.399 min
Delta R.T.: 0.003 min
Response: 3158674
Conc: 17.01 ng/ml m

Instrument :
ECD_O
ClientSampleId :
NYSEG-CLRK-PH4-A9-B1RE


Manual Integrations
APPROVED

Sohil
9/26/2018 11:52:07 AM

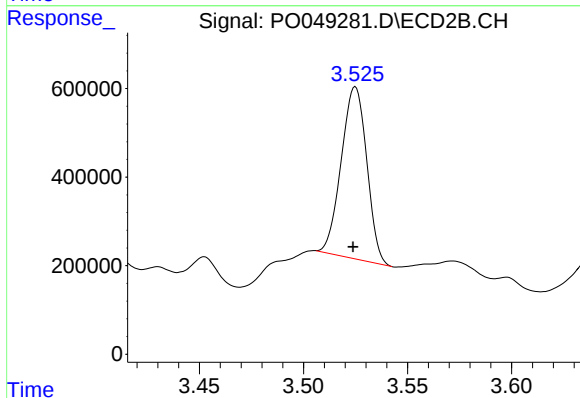


#1 Tetrachloro-m-xylene

R.T.: 3.525 min
Delta R.T.: 0.000 min
Response: 3313478
Conc: 16.03 ng/ml m

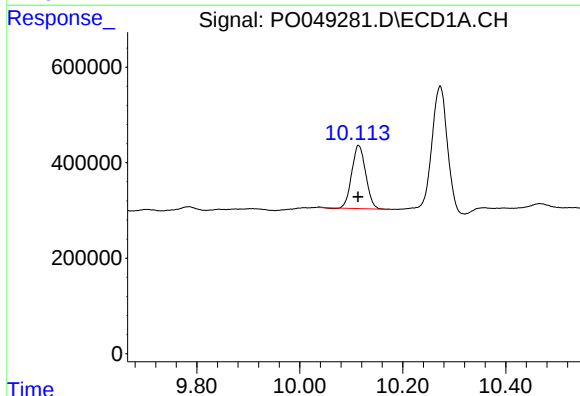

#2 Decachlorobiphenyl

R.T.: 10.114 min
Delta R.T.: 0.000 min
Response: 2489105
Conc: 9.06 ng/ml

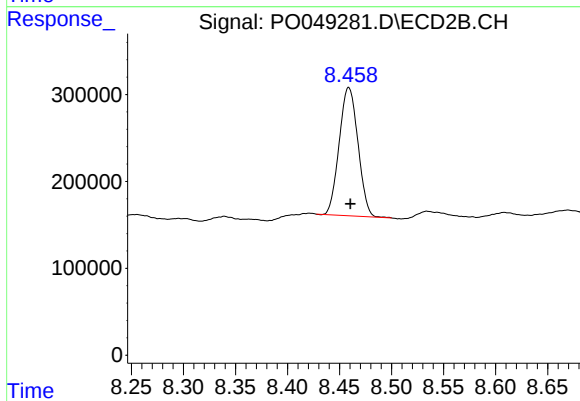

#2 Decachlorobiphenyl

R.T.: 8.459 min
Delta R.T.: -0.002 min
Response: 1850961
Conc: 9.04 ng/ml